

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
 Data File : PS009416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2020 17:27
 Operator : DD\AJ
 Sample : L2012-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 17:56:14 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.932	270.8E6	263.2E6	489.598	479.207
Target Compounds							
1) T	Dalapon	3.006	2.588	16061022	53572094	20.595	68.040 #
2) T	3,5-DICHL...	0.000	6.108	0	40133196	N.D.	49.346
6) T	MCP	7.596	0.000	7945870	0	3.229	N.D. #
7) T	MCPA	7.793	0.000	61471856	0	20.183	N.D. #
8) T	DICHLORPROP	0.000	7.751	0	29753782	N.D.	53.628
12) T	2,4,5-T	9.452	0.000	18215138	0	7.160	N.D. #
14) T	DINOSEB	11.187	10.047	21395804	20314656	10.467	9.249
15) T	Picloram	11.014	11.020	15361153	12222153	5.061	3.001 #
16) T	DCPA	11.551	10.965	10958510	12490918	3.161	3.225



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
Data File : PS009416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2020 17:27
Operator : DD\AJ
Sample : L2012-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 17:56:14 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

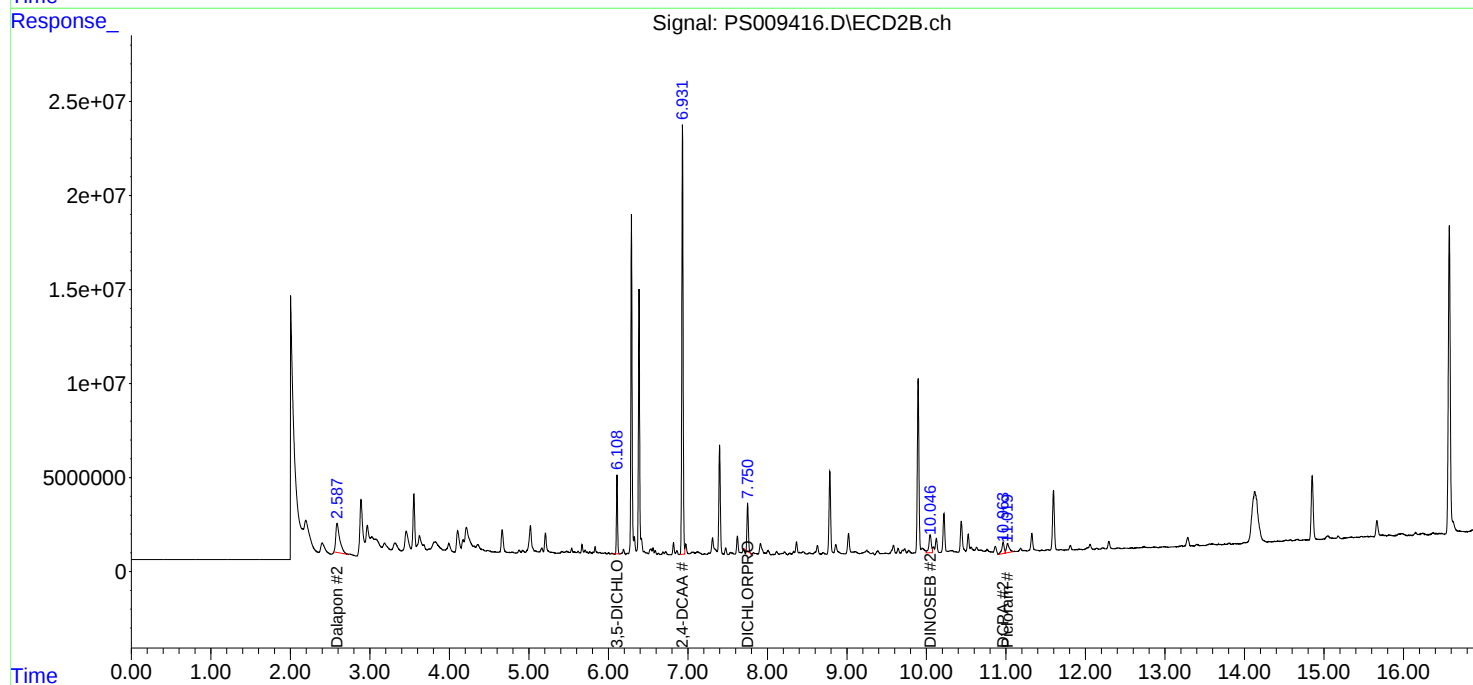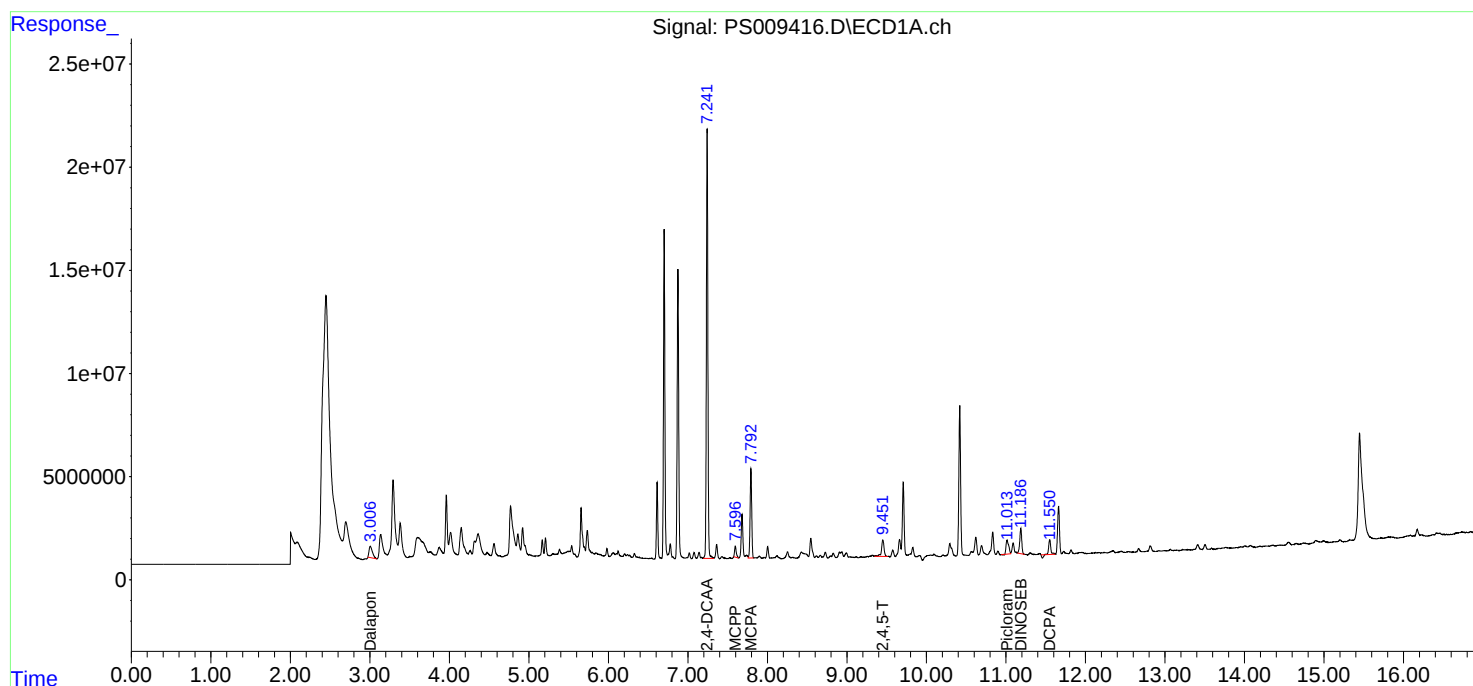


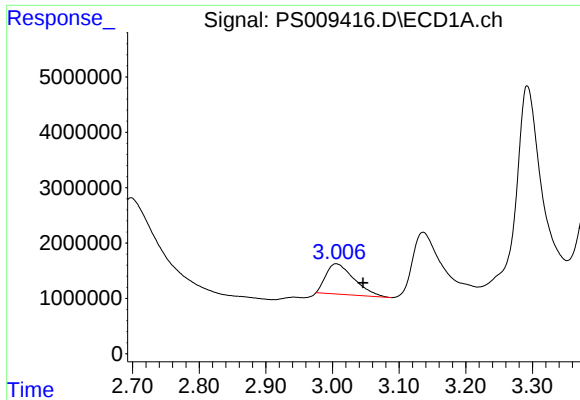

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 16061022
Conc: 20.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

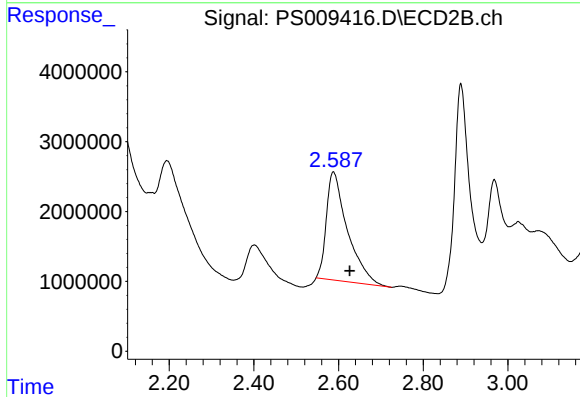


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 53572094
Conc: 68.04 ng/ml

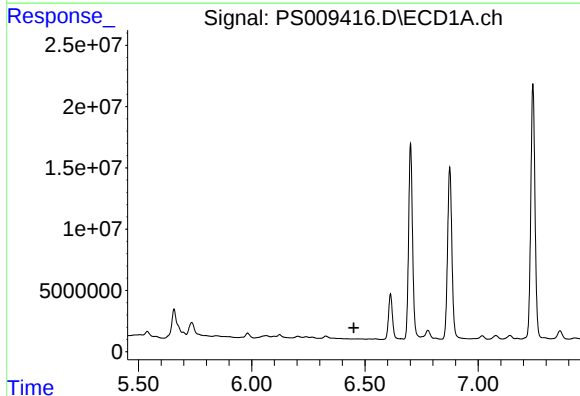


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

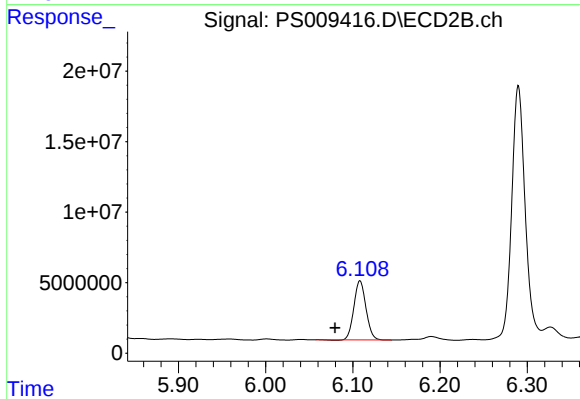

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.108 min
Delta R.T.: 0.029 min
Response: 40133196
Conc: 49.35 ng/ml

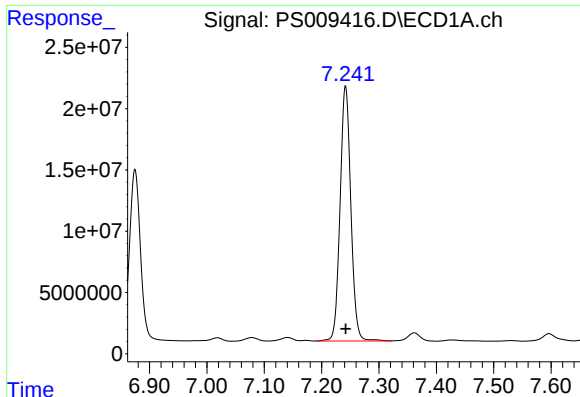

#4 2,4-DCAA


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 270831029
Conc: 489.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

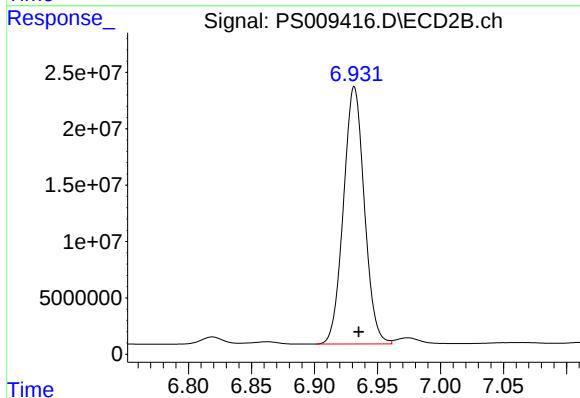


#4 2,4-DCAA

R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 263179173
Conc: 479.21 ng/ml

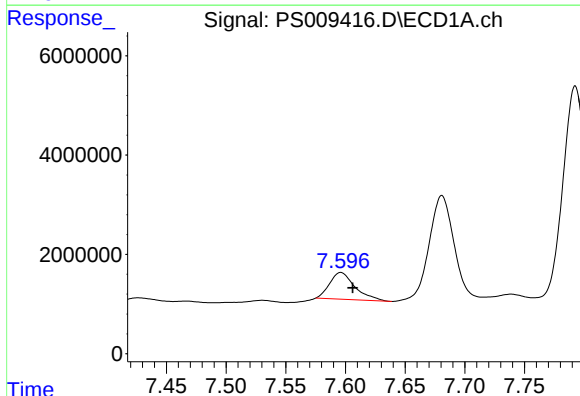


#6 MCP

R.T.: 7.596 min
Delta R.T.: -0.010 min
Response: 7945870
Conc: 3.23 ug/ml

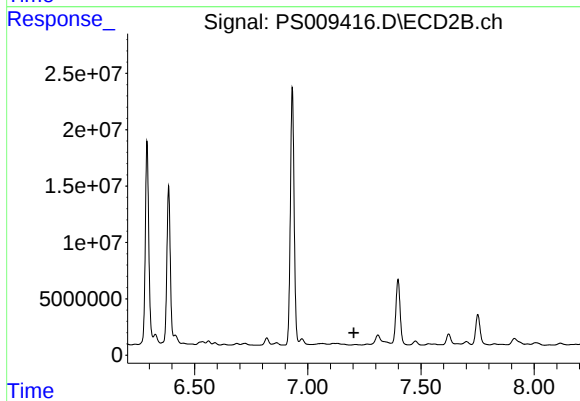

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

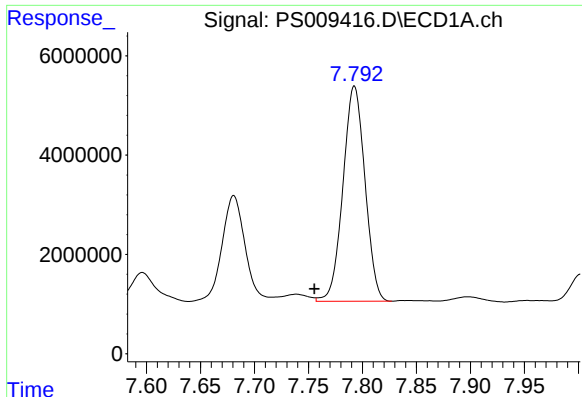

#7 MCPA


R.T.: 7.793 min
Delta R.T.: 0.037 min
Response: 61471856
Conc: 20.18 ug/ml

Instrument :
ECD_S
ClientSampleId :

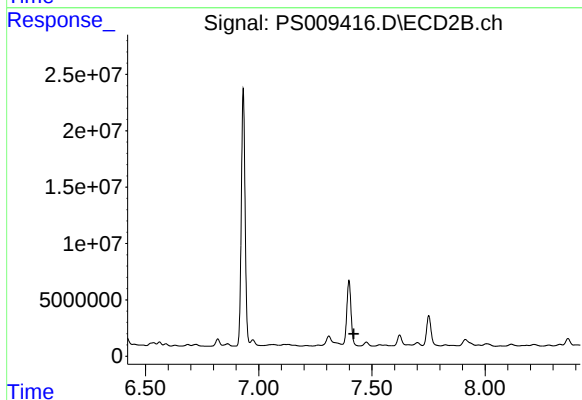


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.420 min
Response: 0
Conc: N.D.

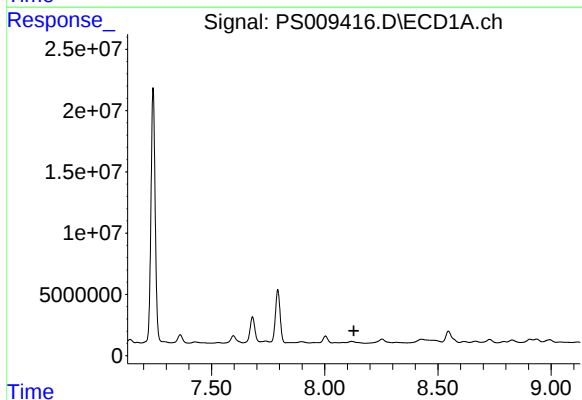


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

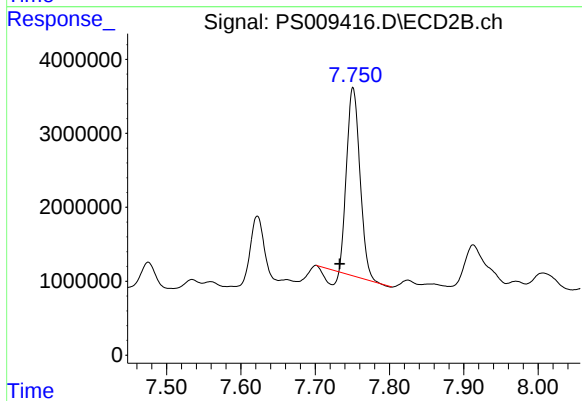

#8 DICHLORPROP


R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 29753782
Conc: 53.63 ng/ml

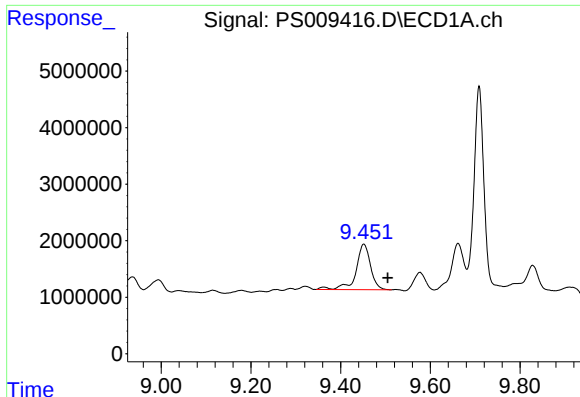

#12 2,4,5-T


R.T.: 9.452 min
Delta R.T.: -0.053 min
Response: 18215138
Conc: 7.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

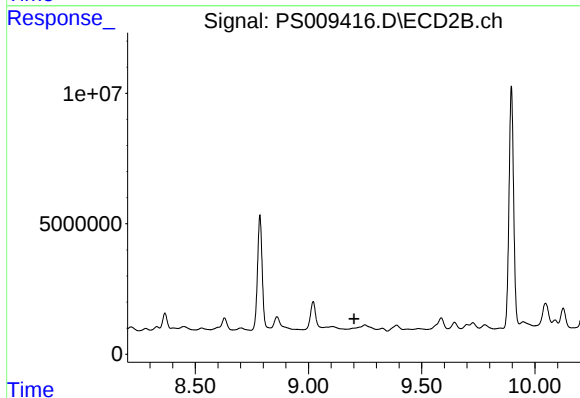


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

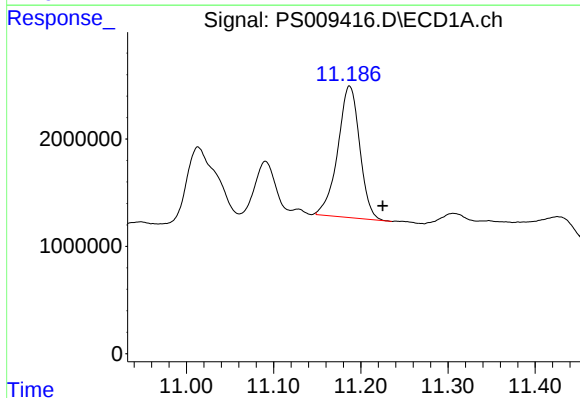


#14 DINOSEB

R.T.: 11.187 min
Delta R.T.: -0.038 min
Response: 21395804
Conc: 10.47 ng/ml

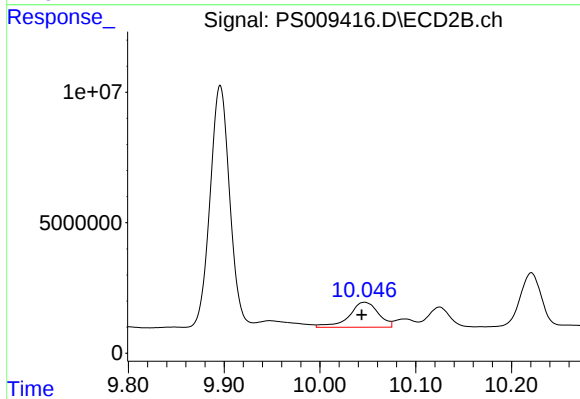

#14 DINOSEB


R.T.: 10.047 min
Delta R.T.: 0.003 min
Response: 20314656
Conc: 9.25 ng/ml

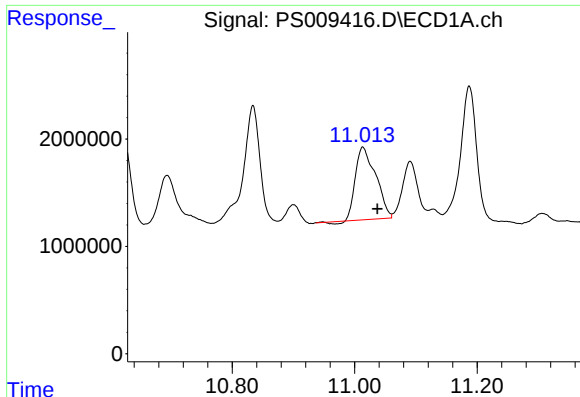

#15 Picloram


R.T.: 11.014 min
Delta R.T.: -0.024 min
Response: 15361153
Conc: 5.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

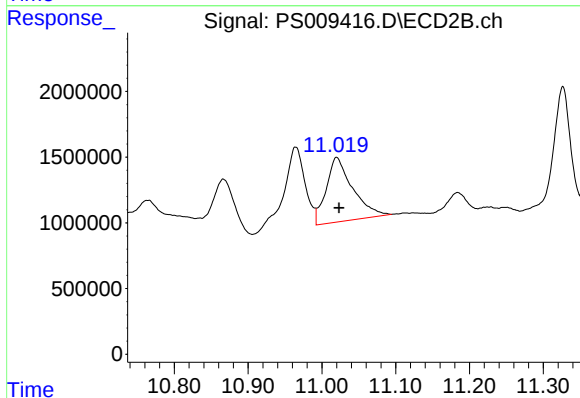


#15 Picloram

R.T.: 11.020 min
Delta R.T.: -0.003 min
Response: 12222153
Conc: 3.00 ng/ml

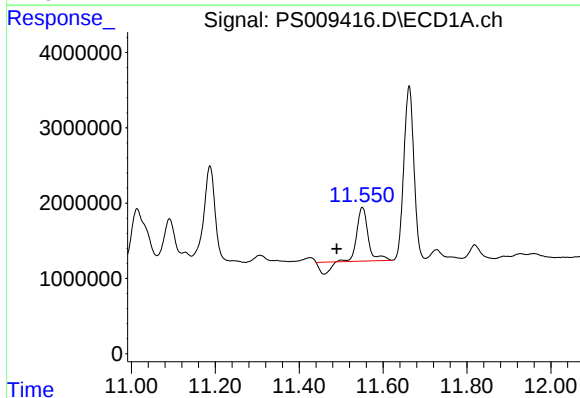

#16 DCPA

R.T.: 11.551 min
Delta R.T.: 0.062 min
Response: 10958510
Conc: 3.16 ng/ml

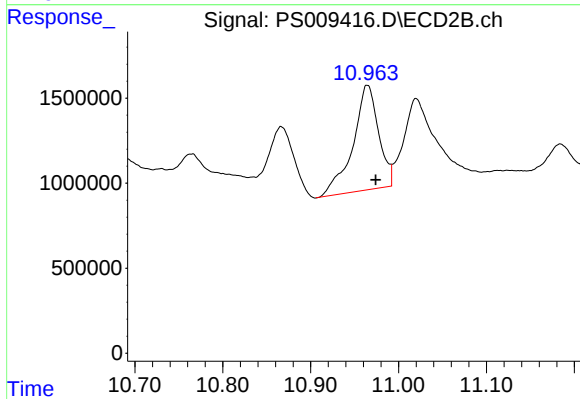

#16 DCPA

R.T.: 10.965 min
Delta R.T.: -0.009 min
Response: 12490918
Conc: 3.23 ng/ml