

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
 Data File : PS009418.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2020 18:13
 Operator : DD\AJ
 Sample : PB127787BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 18:32:00 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.932	324.7E6	318.5E6	587.059	579.969
Target Compounds							
1) T	Dalapon	3.006	2.588	18893380	74296222	24.227	94.361 #
2) T	3,5-DICHL...	0.000	6.109	0	51645458	N.D.	63.501
6) T	MCP	7.597	0.000	8347609	0	3.392	N.D. #
7) T	MCPA	7.793	7.399	71994776	44488027	23.638	16.485 #
8) T	DICHLORPROP	0.000	7.752	0	31935585	N.D.	57.560
11) T	2,4,5-TP ...	0.000	8.785	0	29313113	N.D.	9.833
12) T	2,4,5-T	9.452	0.000	20154074	0	7.923	N.D. #
14) T	DINOSEB	11.188	10.045	32095184	22324868	15.701	10.164 #
15) T	Picloram	11.015	11.020	20204344	21402349	6.657	5.256
16) T	DCPA	0.000	11.020	0	21402349	N.D.	5.526



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
Data File : PS009418.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2020 18:13
Operator : DD\AJ
Sample : PB127787BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 18:32:00 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

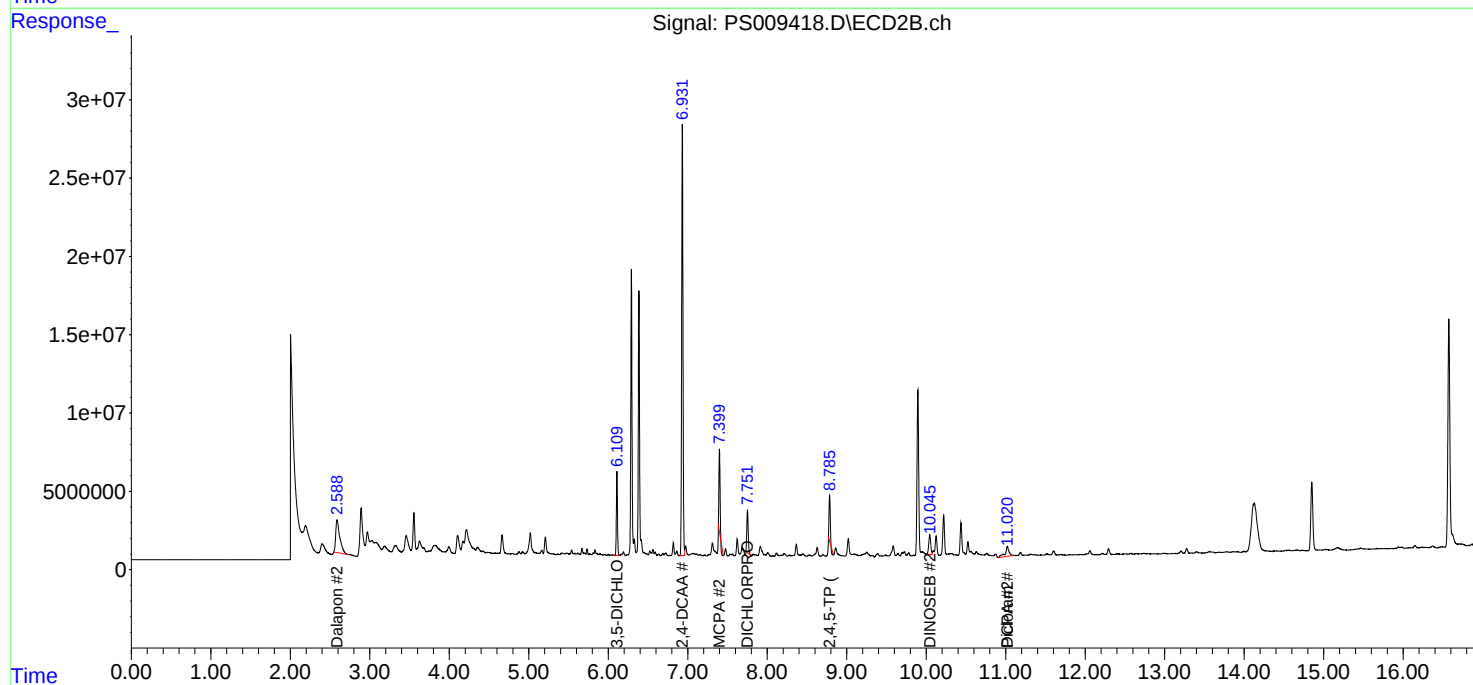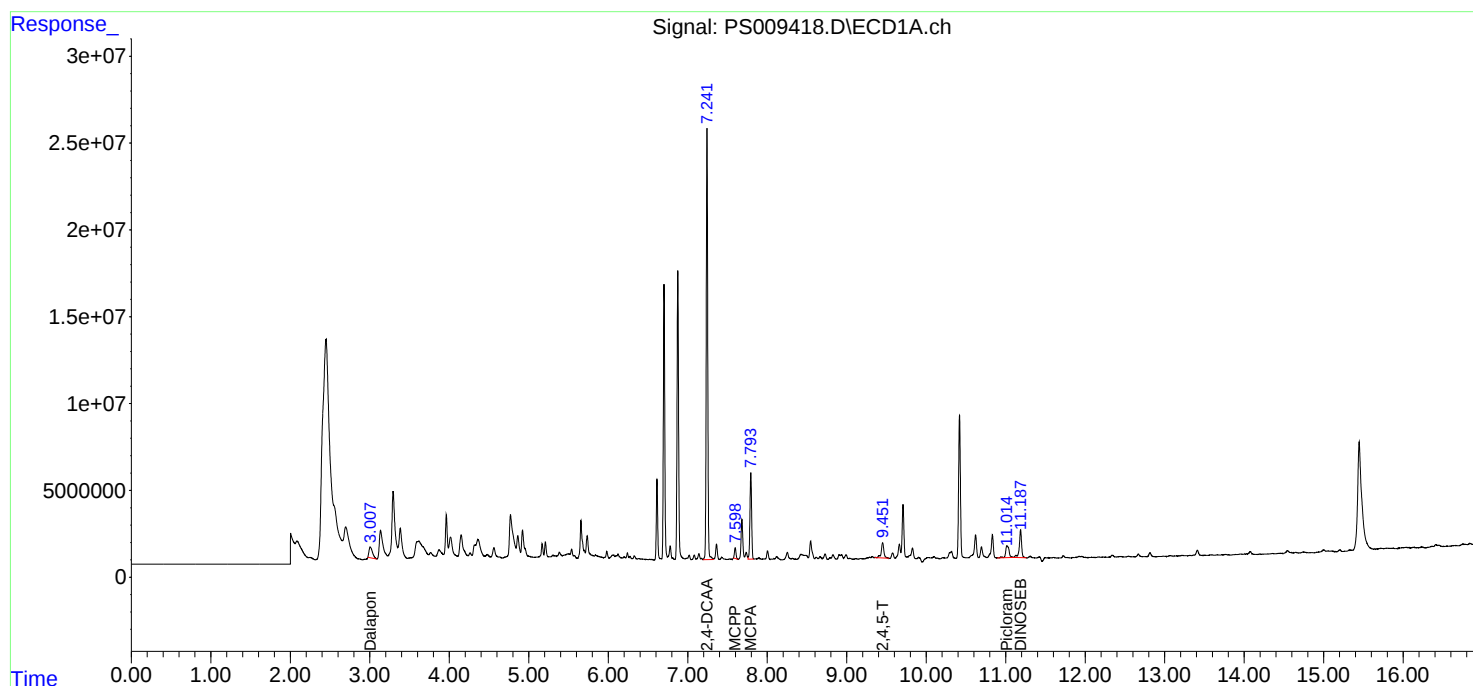


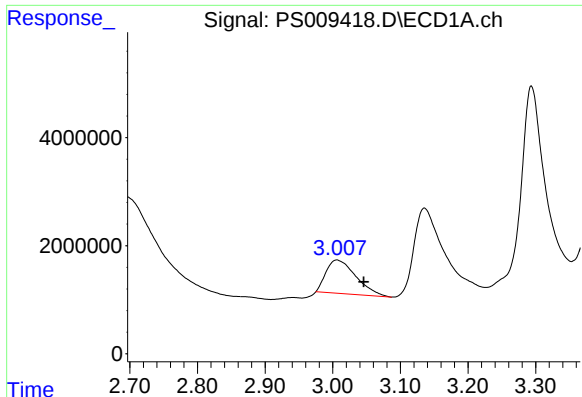

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 18893380
Conc: 24.23 ng/ml

Instrument :
ECD_S
ClientSampleId :

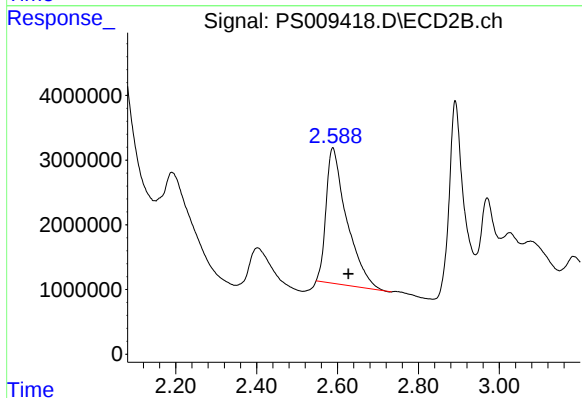


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 74296222
Conc: 94.36 ng/ml

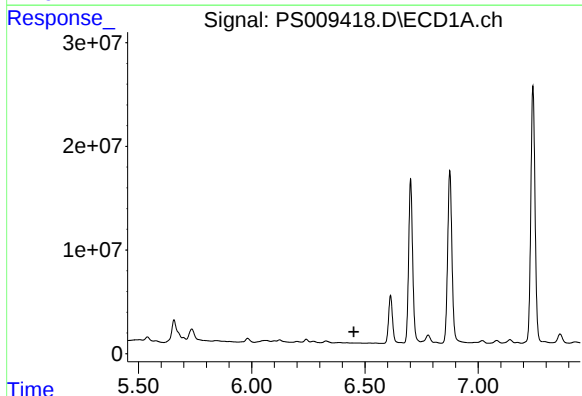


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

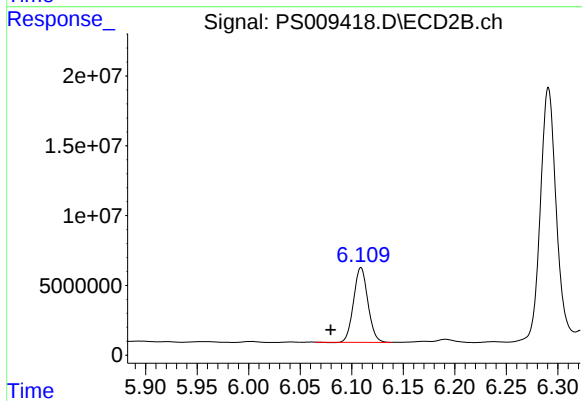

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.109 min
Delta R.T.: 0.029 min
Response: 51645458
Conc: 63.50 ng/ml

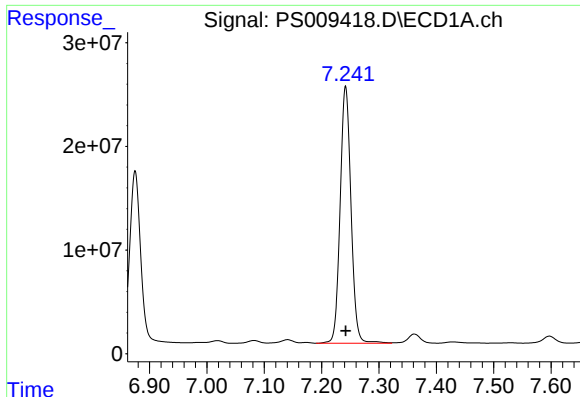

#4 2,4-DCAA


R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 324743326
Conc: 587.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

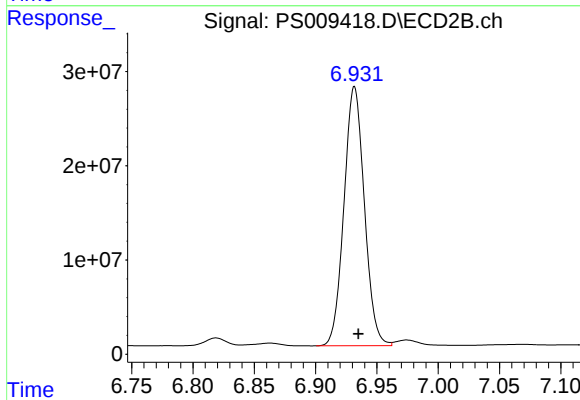


#4 2,4-DCAA

R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 318517693
Conc: 579.97 ng/ml

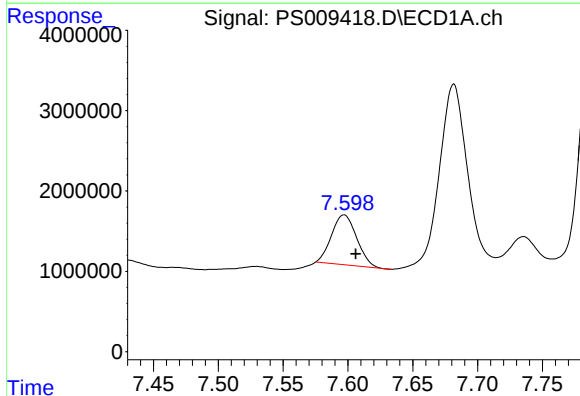


#6 MCP

R.T.: 7.597 min
Delta R.T.: -0.009 min
Response: 8347609
Conc: 3.39 ug/ml

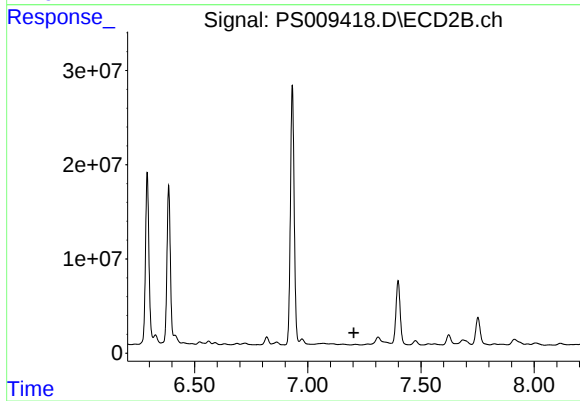

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

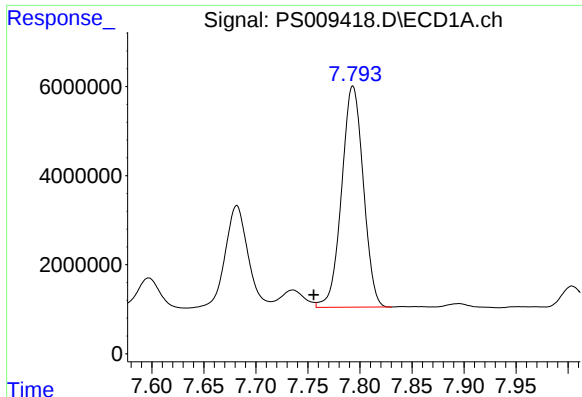

#7 MCPA


R.T.: 7.793 min
Delta R.T.: 0.038 min
Response: 71994776
Conc: 23.64 ug/ml

Instrument :
ECD_S
ClientSampleId :

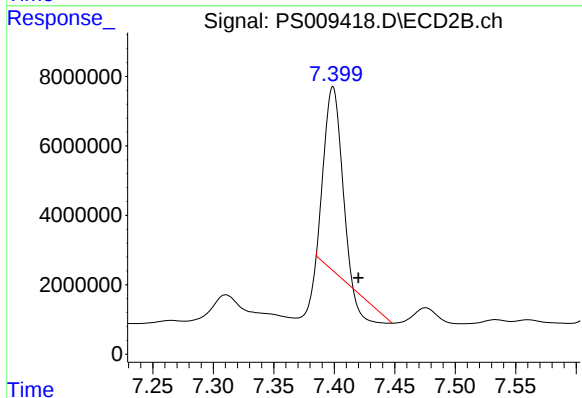


#7 MCPA

R.T.: 7.399 min
Delta R.T.: -0.021 min
Response: 44488027
Conc: 16.49 ug/ml

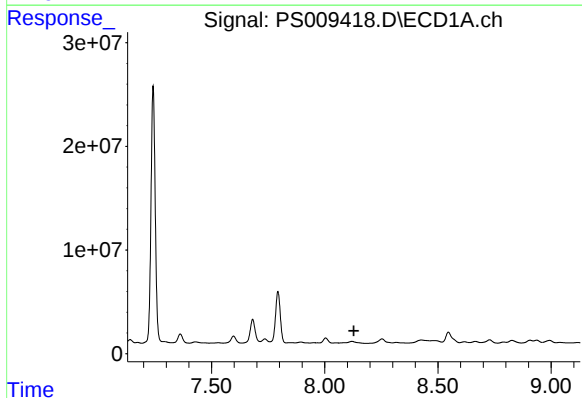


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

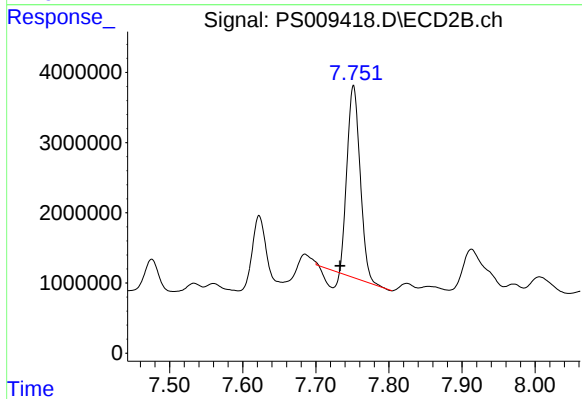

#8 DICHLORPROP


R.T.: 7.752 min
Delta R.T.: 0.019 min
Response: 31935585
Conc: 57.56 ng/ml

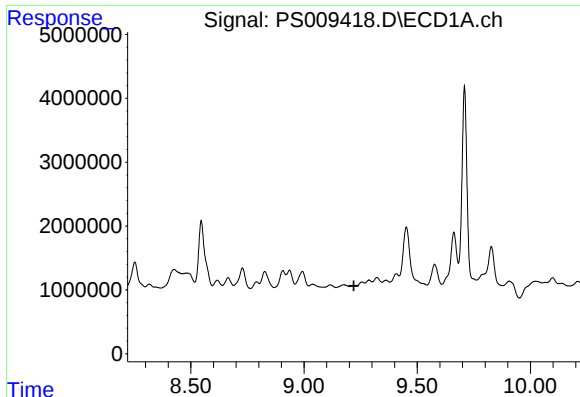

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

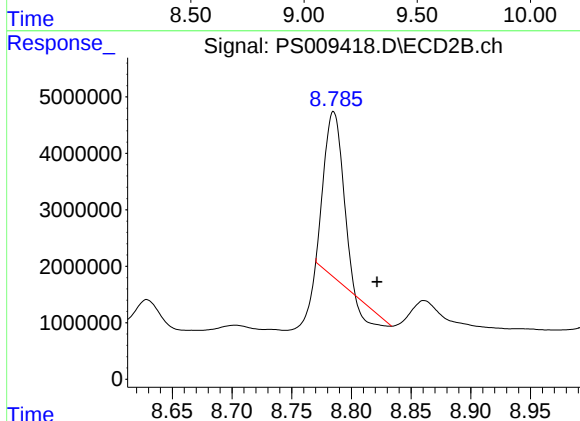


#11 2,4,5-TP (SILVEX)

R.T.: 8.785 min
Delta R.T.: -0.036 min
Response: 29313113
Conc: 9.83 ng/ml

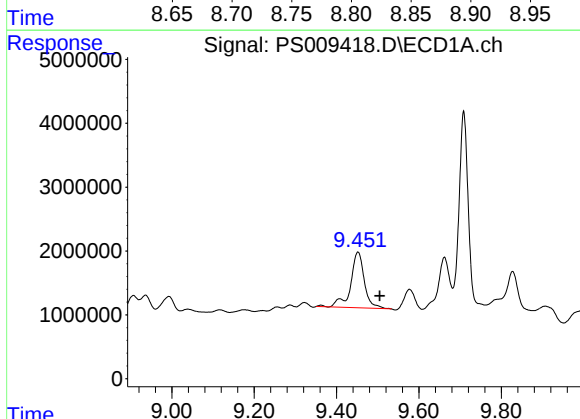


#12 2,4,5-T

R.T.: 9.452 min
Delta R.T.: -0.053 min
Response: 20154074
Conc: 7.92 ng/ml

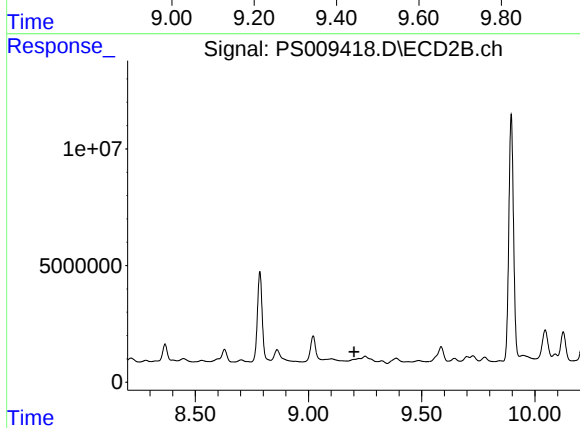

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

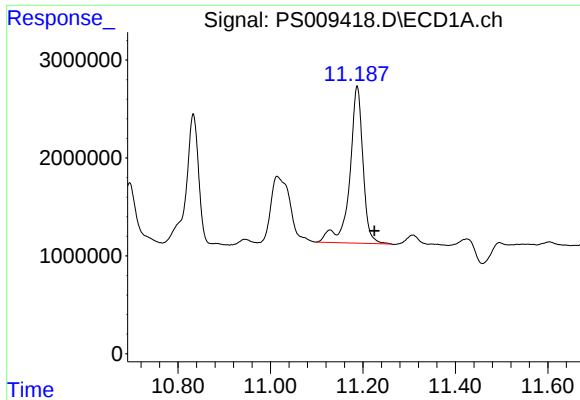

#14 DINOSEB


R.T.: 11.188 min
Delta R.T.: -0.038 min
Response: 32095184
Conc: 15.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

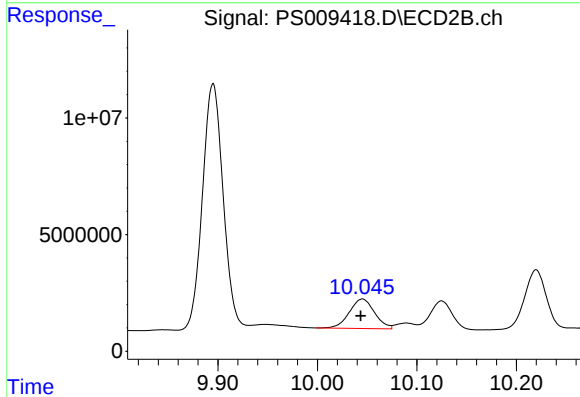


#14 DINOSEB

R.T.: 10.045 min
Delta R.T.: 0.002 min
Response: 22324868
Conc: 10.16 ng/ml

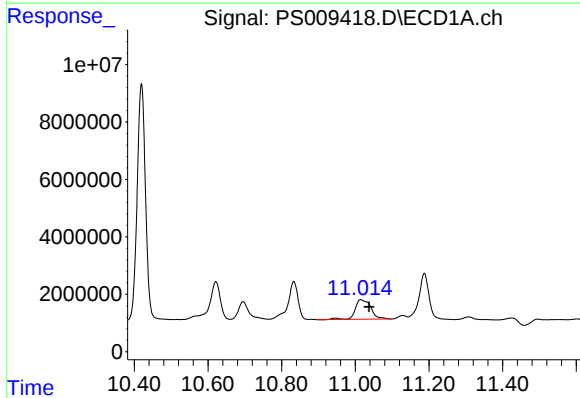


#15 Picloram

R.T.: 11.015 min
Delta R.T.: -0.022 min
Response: 20204344
Conc: 6.66 ng/ml

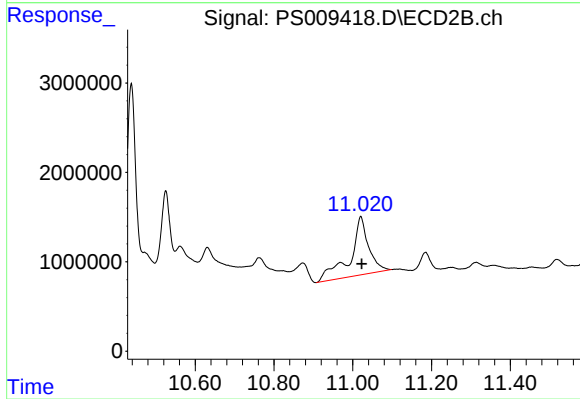

#15 Picloram


R.T.: 11.020 min
Delta R.T.: -0.003 min
Response: 21402349
Conc: 5.26 ng/ml

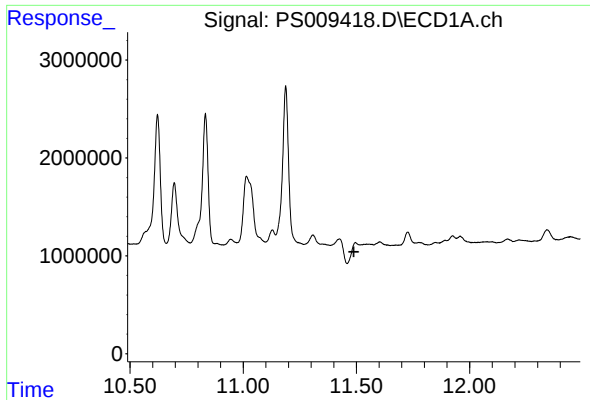

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

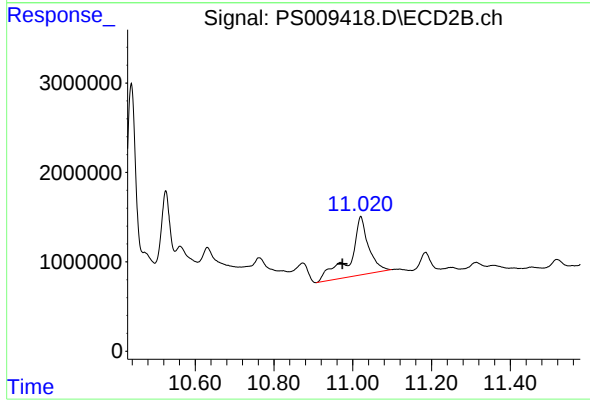

#16 DCPA

R.T.: 11.020 min
Delta R.T.: 0.046 min
Response: 21402349
Conc: 5.53 ng/ml