

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
 Data File : PS009420.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2020 18:59
 Operator : DD\AJ
 Sample : PB127787TB
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 02:43:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.931	323.4E6	264.4E6	584.546	481.462
Target Compounds							
1) T	Dalapon	3.007	2.589	17494997	55893369	22.434	70.988 #
2) T	3,5-DICHL...	0.000	6.108	0	59909840	N.D.	73.662
3) T	4-Nitroph...	7.116	0.000	25475362	0	106.720	N.D. #
8) T	DICHLORPROP	0.000	7.751	0	45753072	N.D.	82.464
11) T	2,4,5-TP ...	0.000	8.859	0	3340644	N.D.	1.121
12) T	2,4,5-T	9.445	0.000	49901282	0	19.616	N.D. #
14) T	DINOSEB	11.186	10.085	27153650	46175685	13.284	21.023 #
15) T	Picloram	11.013	11.020	29024740	11736924	9.564	2.882 #
16) T	DCPA	0.000	11.020	0	11736924	N.D.	3.030



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
Data File : PS009420.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2020 18:59
Operator : DD\AJ
Sample : PB127787TB
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 02:43:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

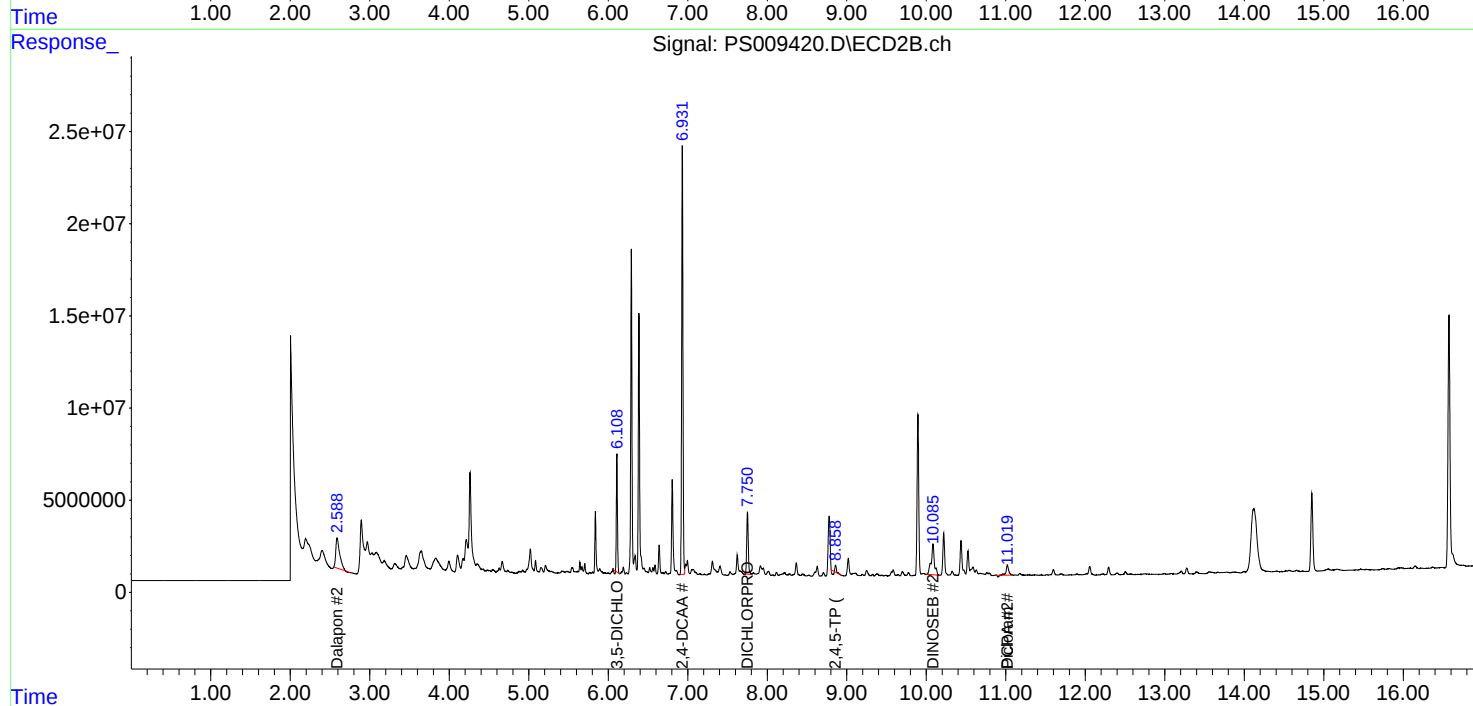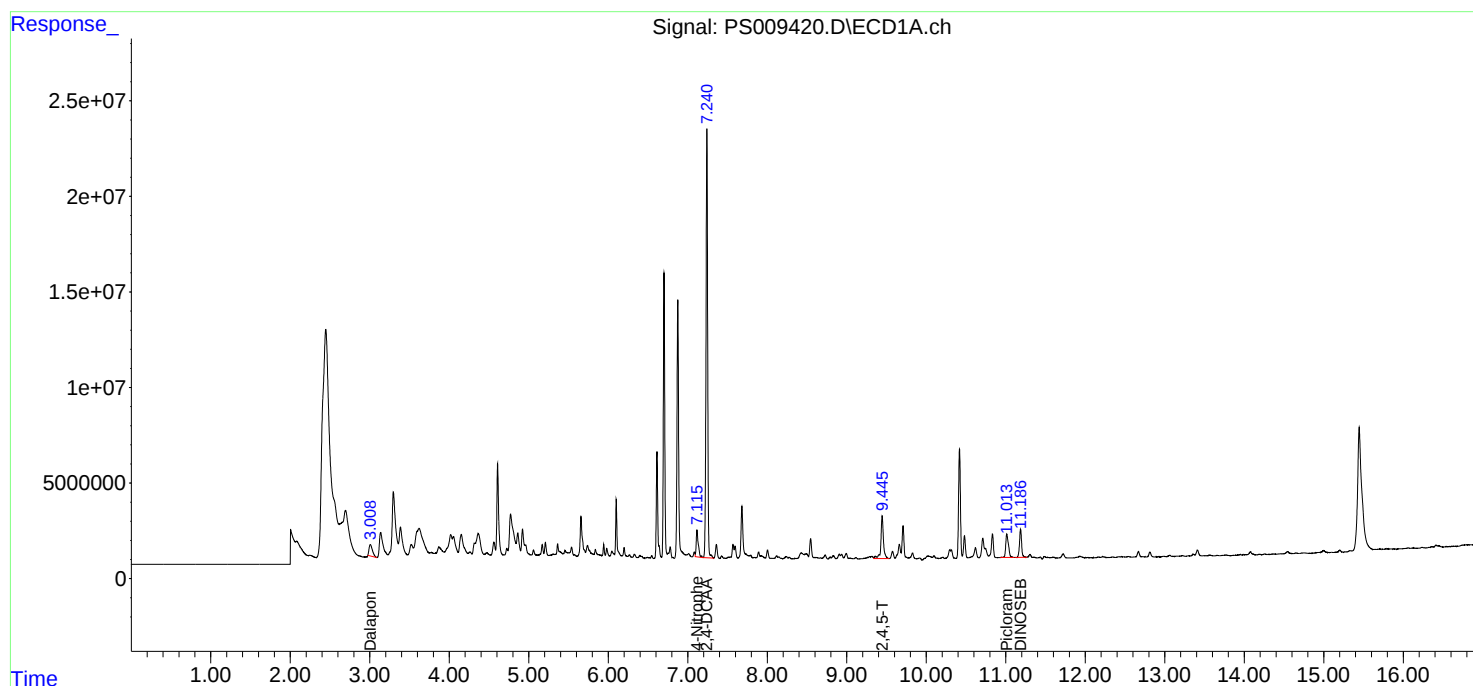


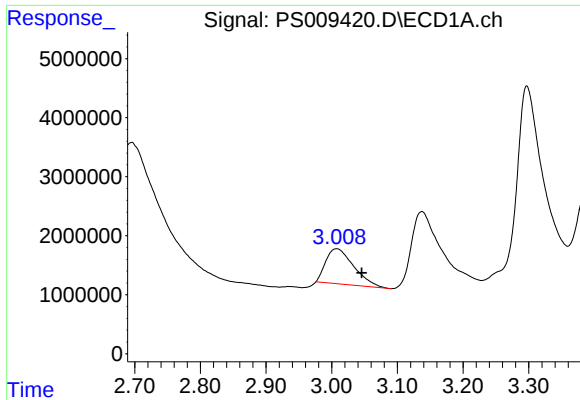

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 17494997
Conc: 22.43 ng/ml

Instrument :
ECD_S
ClientSampleId :

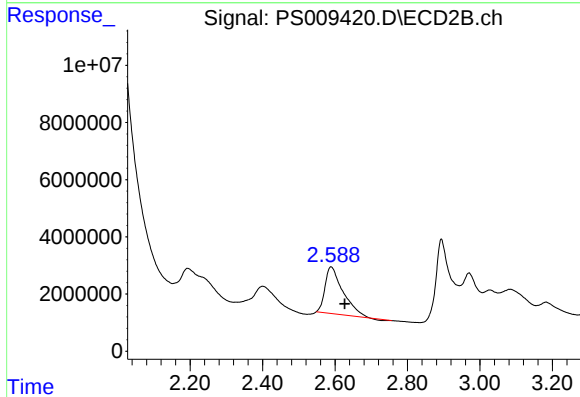


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 55893369
Conc: 70.99 ng/ml

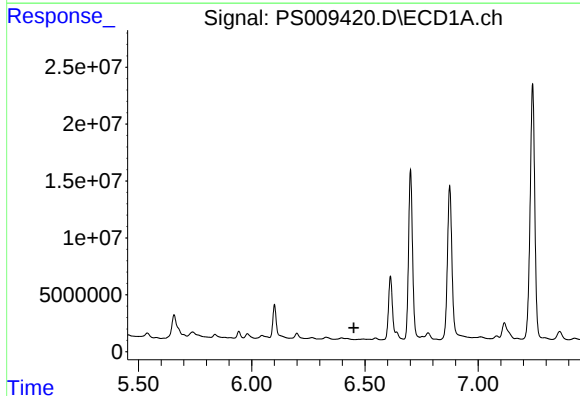


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

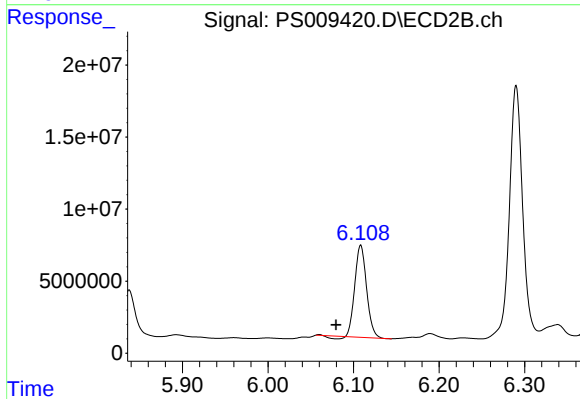

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.108 min
Delta R.T.: 0.029 min
Response: 59909840
Conc: 73.66 ng/ml

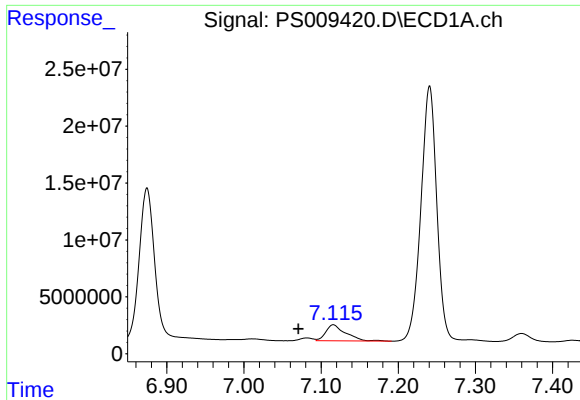

#3 4-Nitrophenol


R.T.: 7.116 min
Delta R.T.: 0.045 min
Response: 25475362
Conc: 106.72 ng/ml

Instrument :
ECD_S
ClientSampleId :

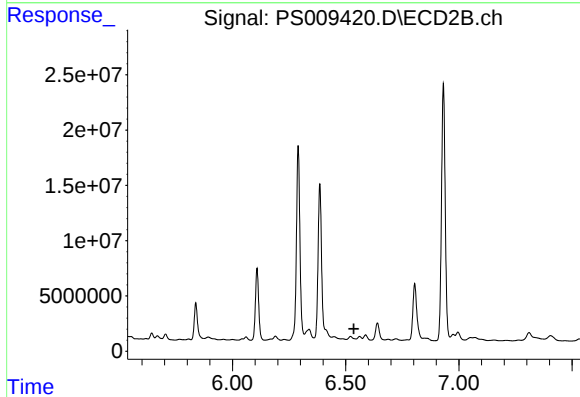


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.536 min
Response: 0
Conc: N.D.

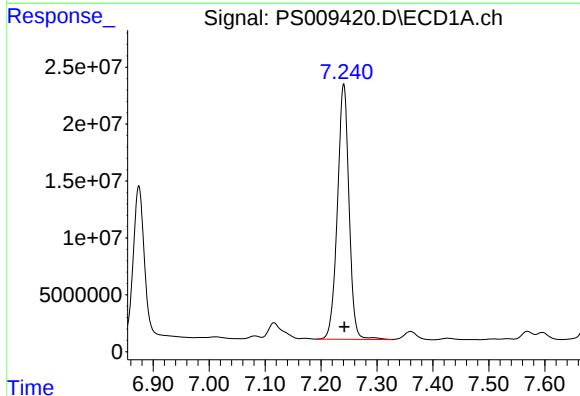


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: -0.001 min
Response: 323353585
Conc: 584.55 ng/ml

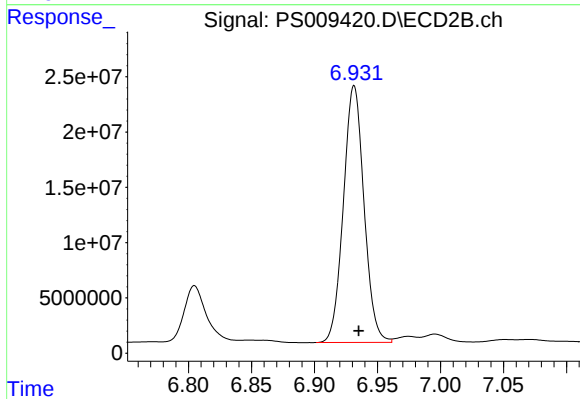

#4 2,4-DCAA


R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 264417667
Conc: 481.46 ng/ml

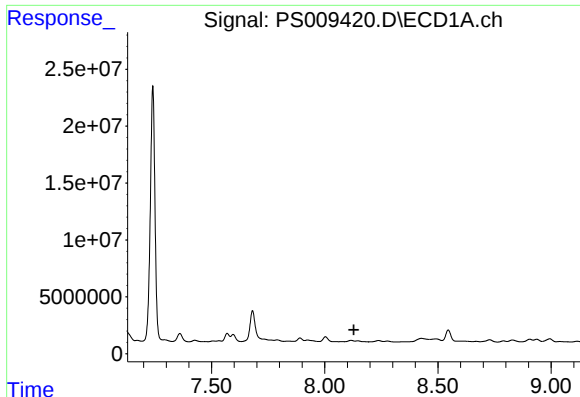

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

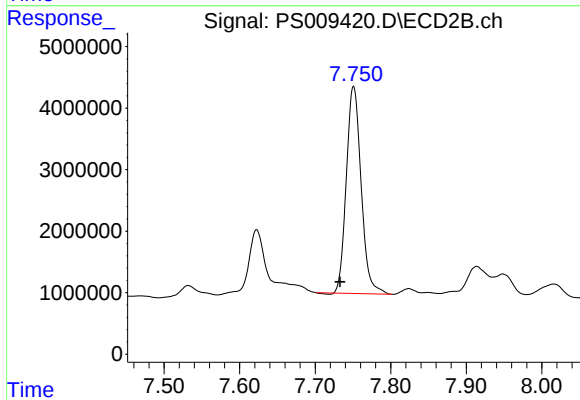


#8 DICHLORPROP

R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 45753072
Conc: 82.46 ng/ml

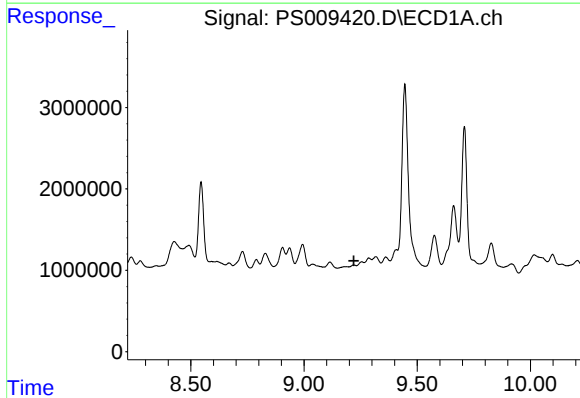


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

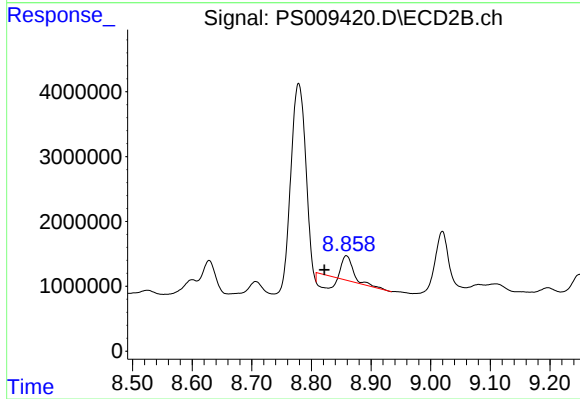

#11 2,4,5-TP (SILVEX)


R.T.: 8.859 min
Delta R.T.: 0.037 min
Response: 3340644
Conc: 1.12 ng/ml

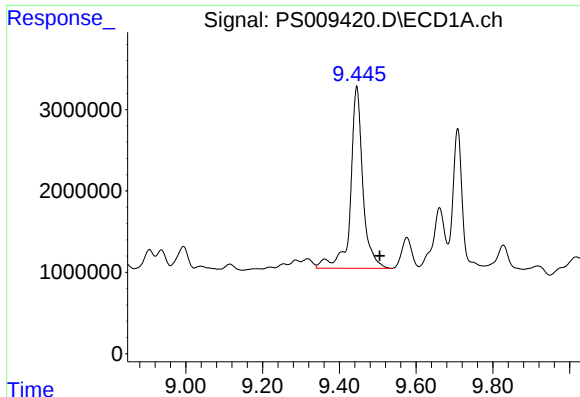

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 49901282
Conc: 19.62 ng/ml

Instrument :
ECD_S
ClientSampleId :

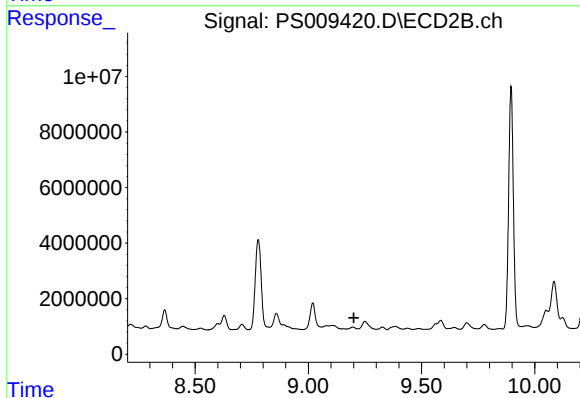


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

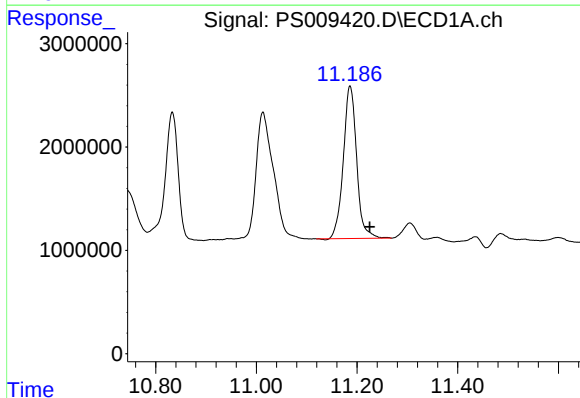


#14 DINOSEB

R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 27153650
Conc: 13.28 ng/ml

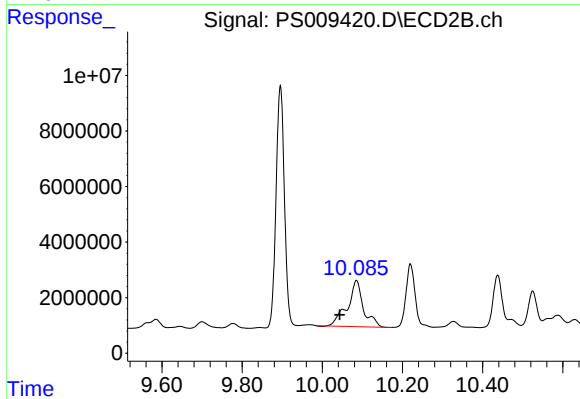

#14 DINOSEB


R.T.: 10.085 min
Delta R.T.: 0.041 min
Response: 46175685
Conc: 21.02 ng/ml

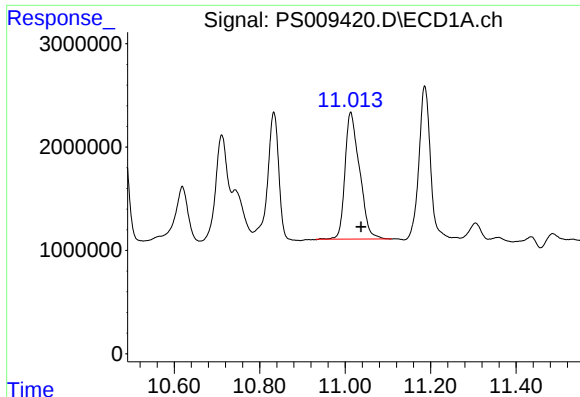

#15 Picloram


R.T.: 11.013 min
Delta R.T.: -0.024 min
Response: 29024740
Conc: 9.56 ng/ml

Instrument :
ECD_S
ClientSampleId :

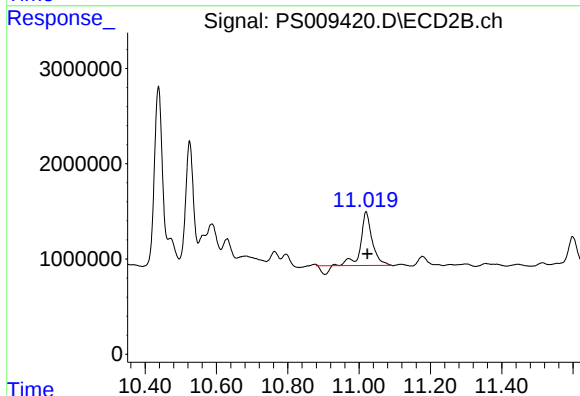


#15 Picloram

R.T.: 11.020 min
Delta R.T.: -0.004 min
Response: 11736924
Conc: 2.88 ng/ml

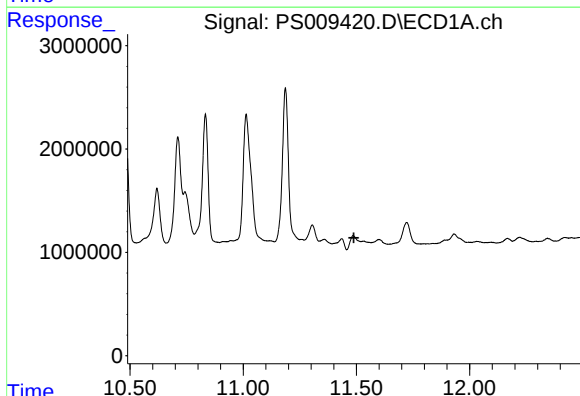

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

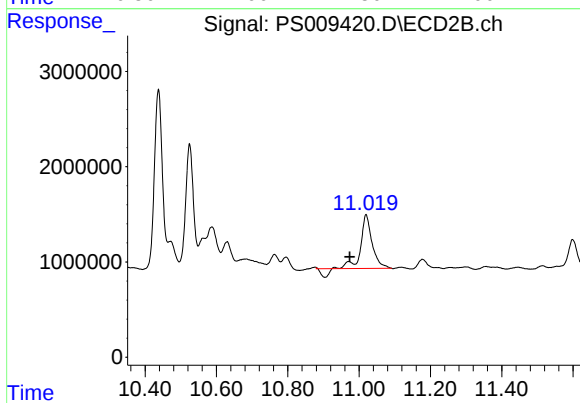

#16 DCPA

R.T.: 11.020 min
Delta R.T.: 0.046 min
Response: 11736924
Conc: 3.03 ng/ml