

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
 Data File : PS009424.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2020 20:30
 Operator : DD\AJ
 Sample : L1994-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 02:45:08 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.931	316.9E6	270.9E6	572.932	493.247
Target Compounds							
1) T	Dalapon	3.007	2.589	18873136	73238821	24.201	93.018 #
2) T	3,5-DICHL...	0.000	6.108	0	67883051	N.D.	83.466
3) T	4-Nitroph...	7.116	0.000	17662016	0	73.989	N.D. #
8) T	DICHLORPROP	0.000	7.751	0	41155012	N.D.	74.177
9) T	2,4-D	8.295	0.000	17760387	0	33.687	N.D. #
12) T	2,4,5-T	9.445	9.249	41048209	24909337	16.136	8.438 #
14) T	DINOSEB	11.187	10.084	30762625	61813548	15.049	28.142 #
15) T	Picloram	11.034	11.019	94200632	99314803	31.039	24.389
16) T	DCPA	0.000	11.019	0	99314803	N.D.	25.643



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
Data File : PS009424.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2020 20:30
Operator : DD\AJ
Sample : L1994-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 02:45:08 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

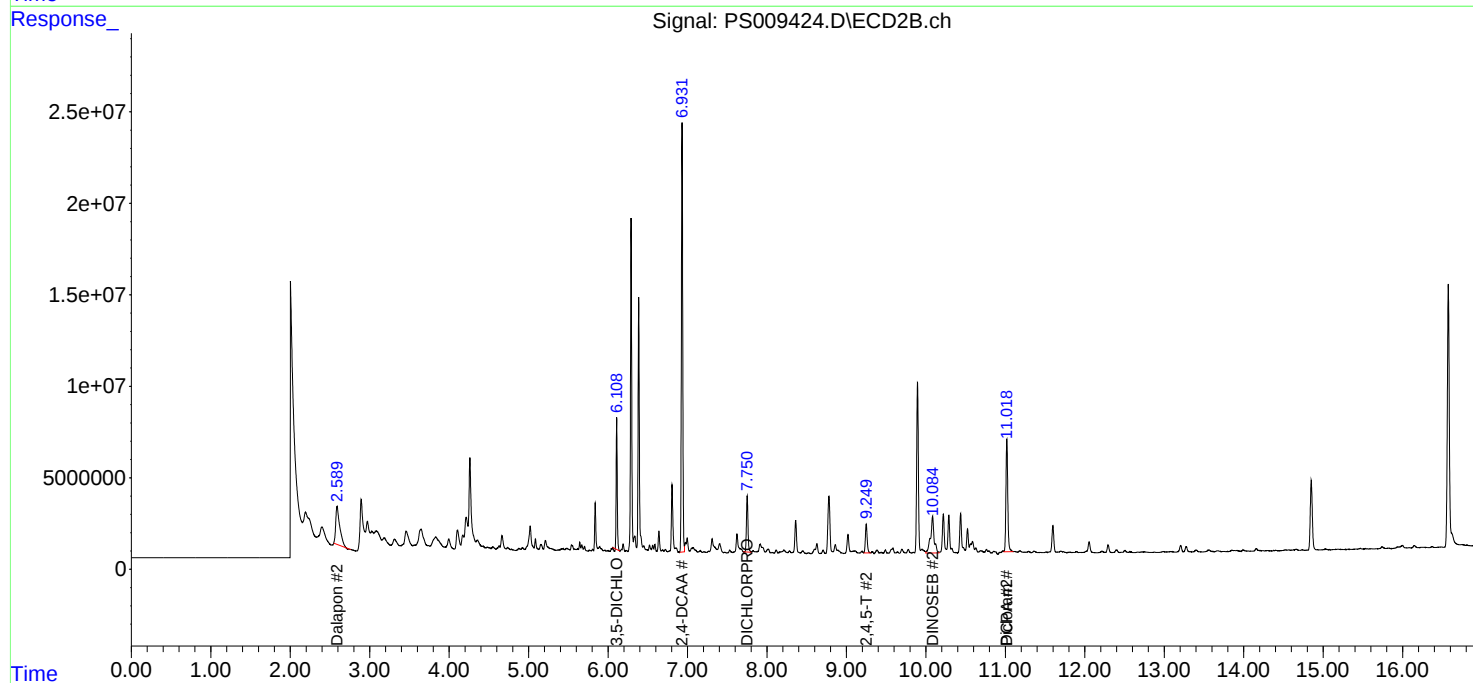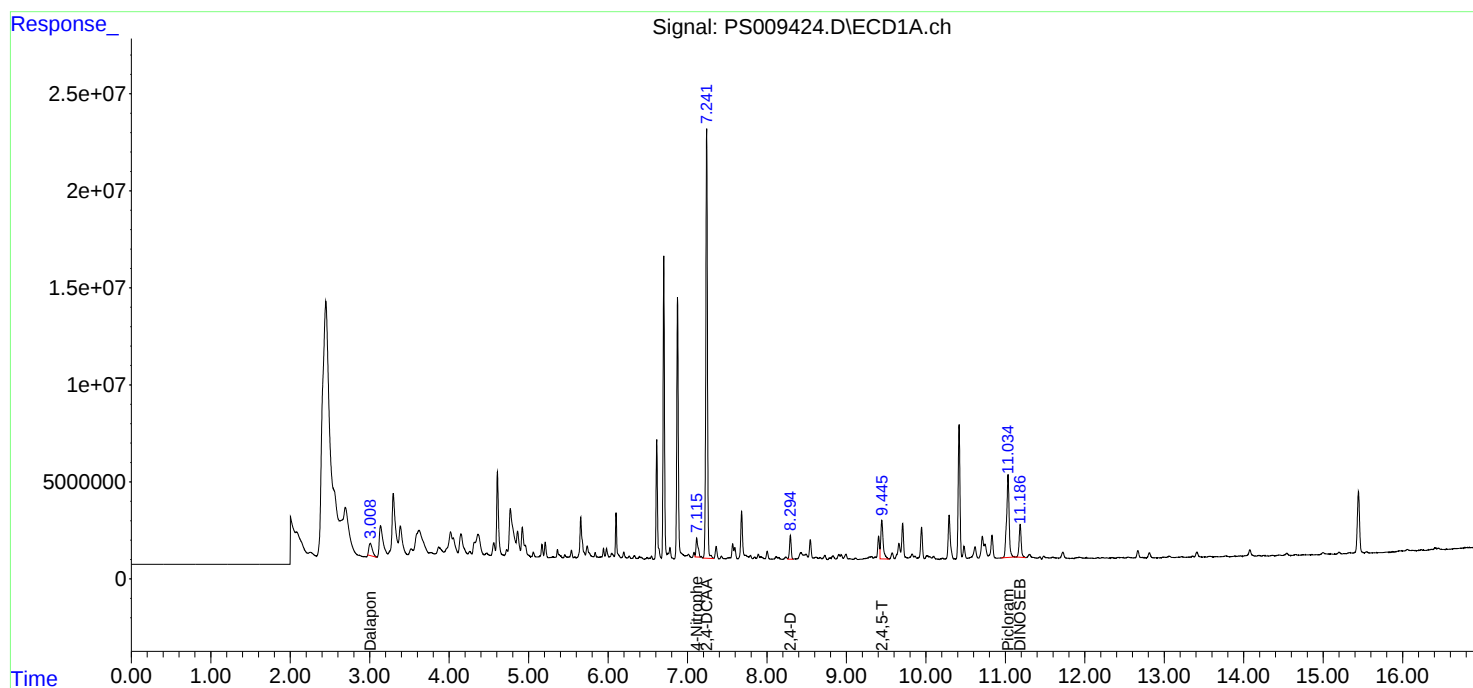


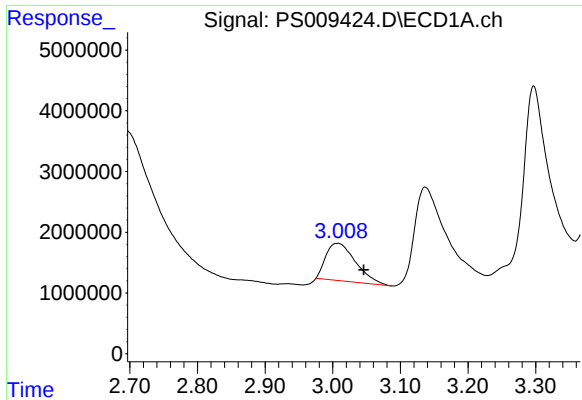

#1 Dalapon


R.T.: 3.007 min
Delta R.T.: -0.039 min
Response: 18873136
Conc: 24.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

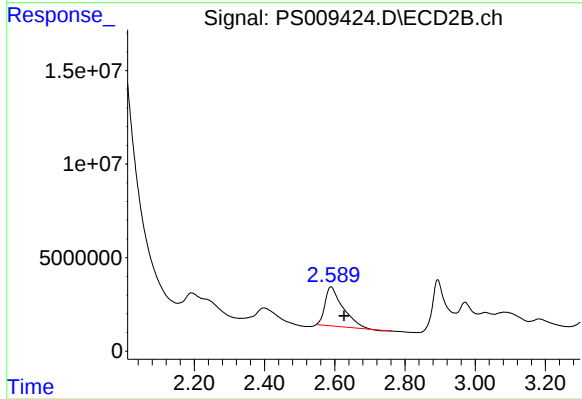


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 73238821
Conc: 93.02 ng/ml

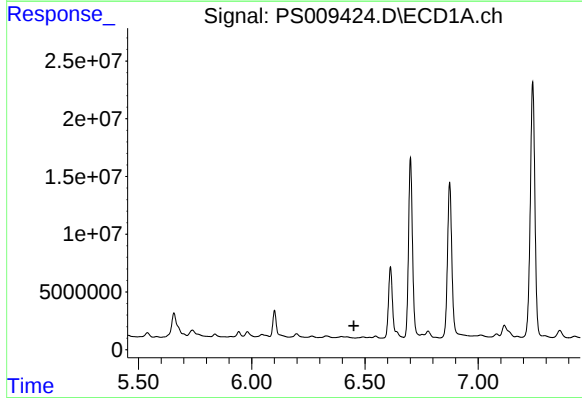


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

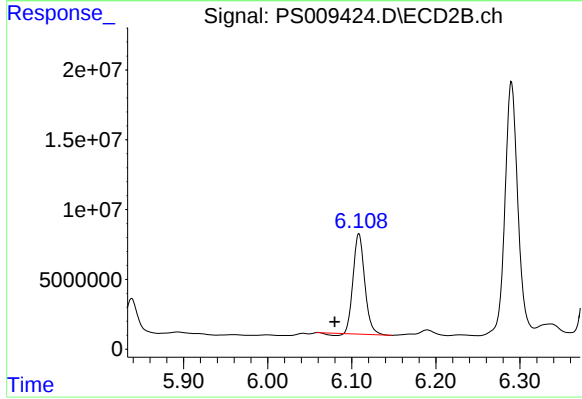

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.108 min
Delta R.T.: 0.029 min
Response: 67883051
Conc: 83.47 ng/ml

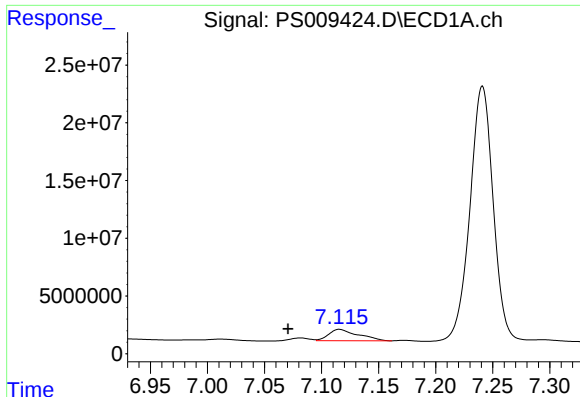

#3 4-Nitrophenol


R.T.: 7.116 min
Delta R.T.: 0.045 min
Response: 17662016
Conc: 73.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

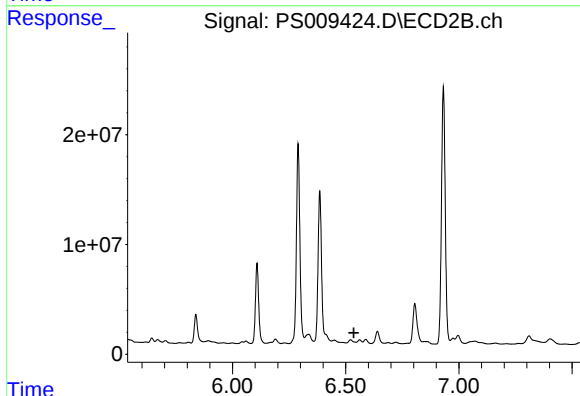


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.536 min
Response: 0
Conc: N.D.

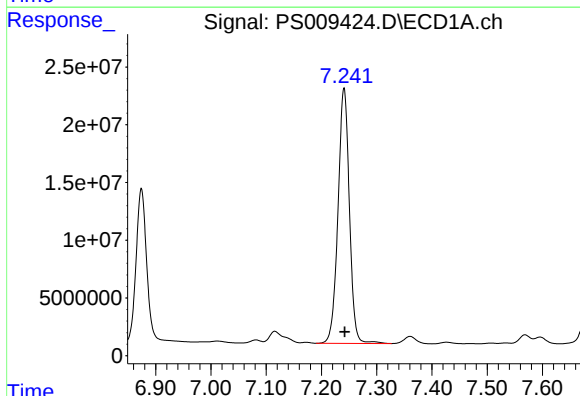


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: -0.001 min
Response: 316928625
Conc: 572.93 ng/ml

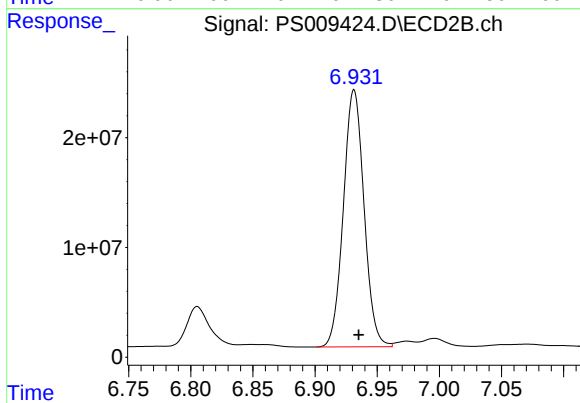

#4 2,4-DCAA


R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 270889992
Conc: 493.25 ng/ml

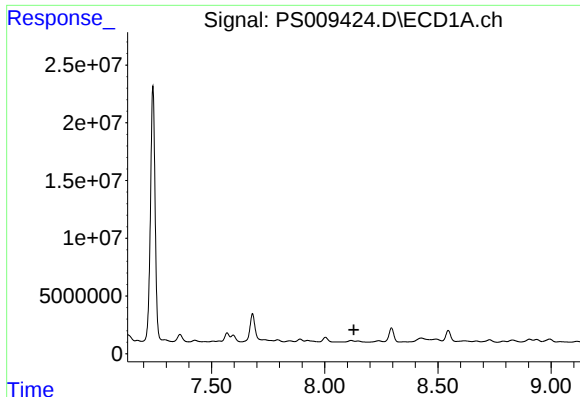

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

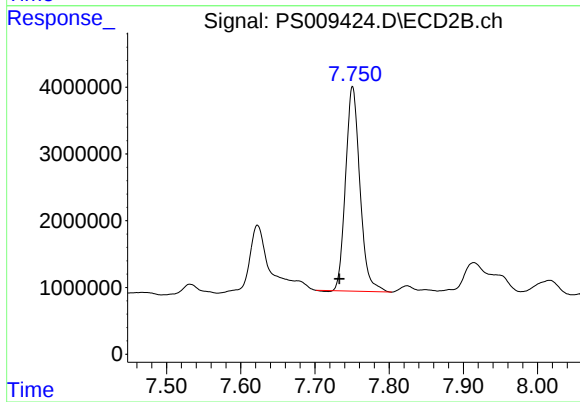


#8 DICHLORPROP

R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 41155012
Conc: 74.18 ng/ml

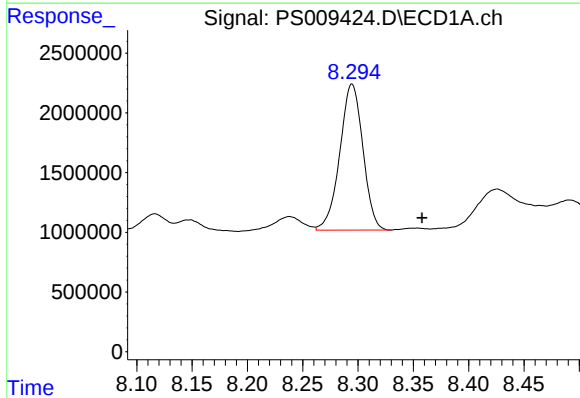


#9 2,4-D

R.T.: 8.295 min
Delta R.T.: -0.063 min
Response: 17760387
Conc: 33.69 ng/ml

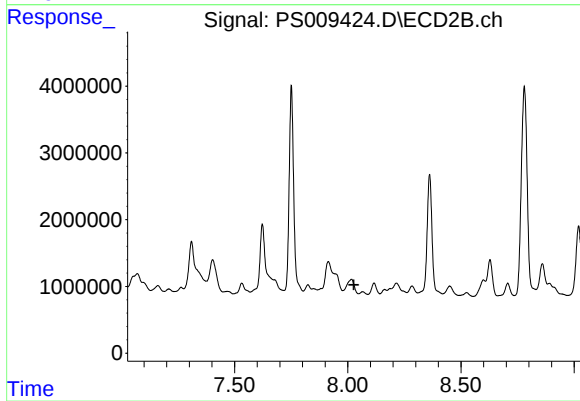

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

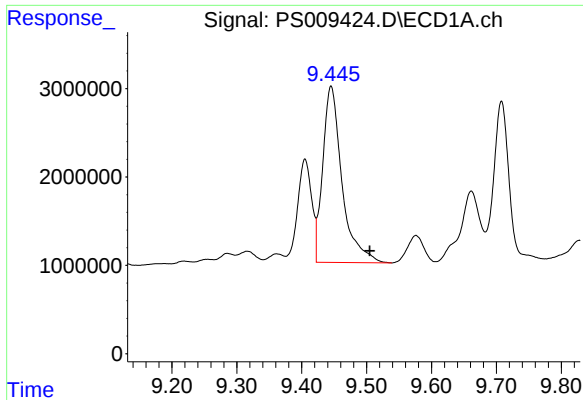

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 41048209
Conc: 16.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

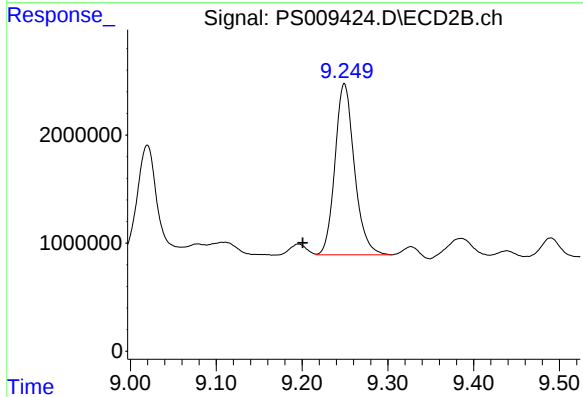


#12 2,4,5-T

R.T.: 9.249 min
Delta R.T.: 0.049 min
Response: 24909337
Conc: 8.44 ng/ml

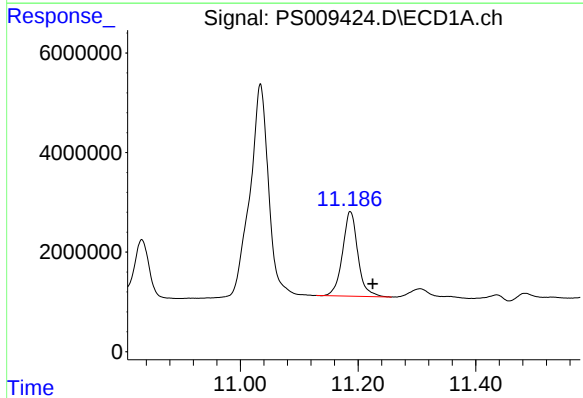


#14 DINOSEB

R.T.: 11.187 min
Delta R.T.: -0.038 min
Response: 30762625
Conc: 15.05 ng/ml

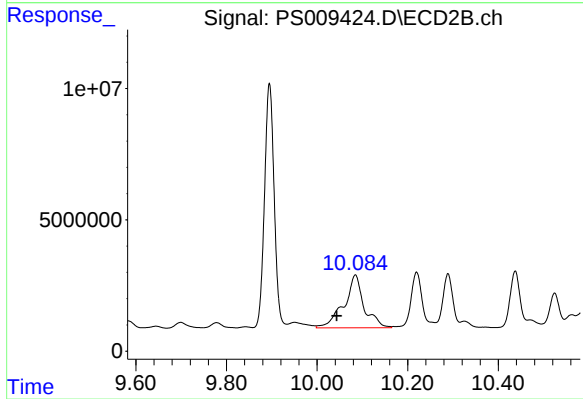

#14 DINOSEB


R.T.: 10.084 min
Delta R.T.: 0.041 min
Response: 61813548
Conc: 28.14 ng/ml

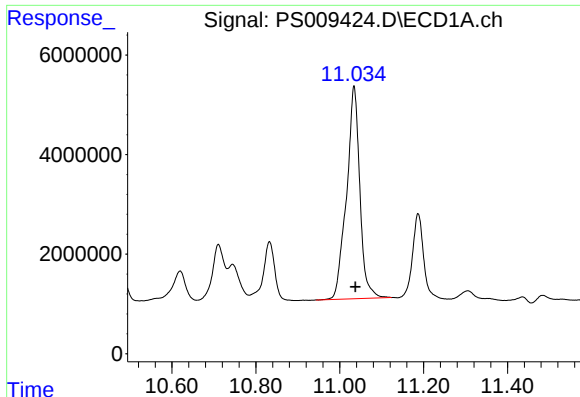

#15 Picloram


R.T.: 11.034 min
Delta R.T.: -0.003 min
Response: 94200632
Conc: 31.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

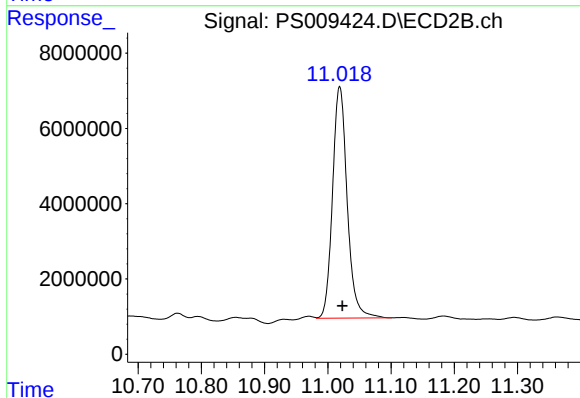


#15 Picloram

R.T.: 11.019 min
Delta R.T.: -0.004 min
Response: 99314803
Conc: 24.39 ng/ml

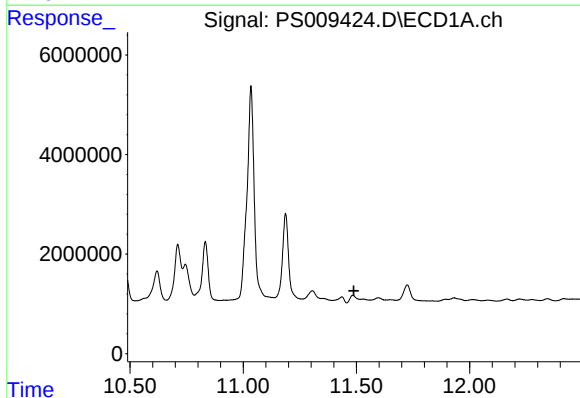

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

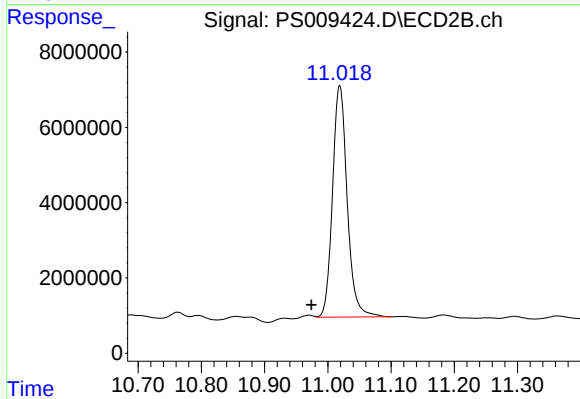

#16 DCPA

R.T.: 11.019 min
Delta R.T.: 0.045 min
Response: 99314803
Conc: 25.64 ng/ml