

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
 Data File : PS009428.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2020 22:02
 Operator : DD\AJ
 Sample : L2011-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 02:46:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.931	300.5E6	263.9E6	543.261	480.560
Target Compounds							
1) T	Dalapon	3.005	2.588	18409556	69971810	23.607	88.869 #
2) T	3,5-DICHL...	0.000	6.108	0	61953528	N.D.	76.175
3) T	4-Nitroph...	7.114	0.000	15307916	0	64.127	N.D. #
8) T	DICHLORPROP	0.000	7.750	0	52288891	N.D.	94.244
9) T	2,4-D	8.426	0.000	12032360	0	22.822	N.D. #
12) T	2,4,5-T	9.444	0.000	53878351	0	21.180	N.D. #
14) T	DINOSEB	11.186	10.050	25538335	11245862	12.493	5.120 #
15) T	Picloram	11.011	0.000	29631240	0	9.763	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
Data File : PS009428.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2020 22:02
Operator : DD\AJ
Sample : L2011-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 02:46:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

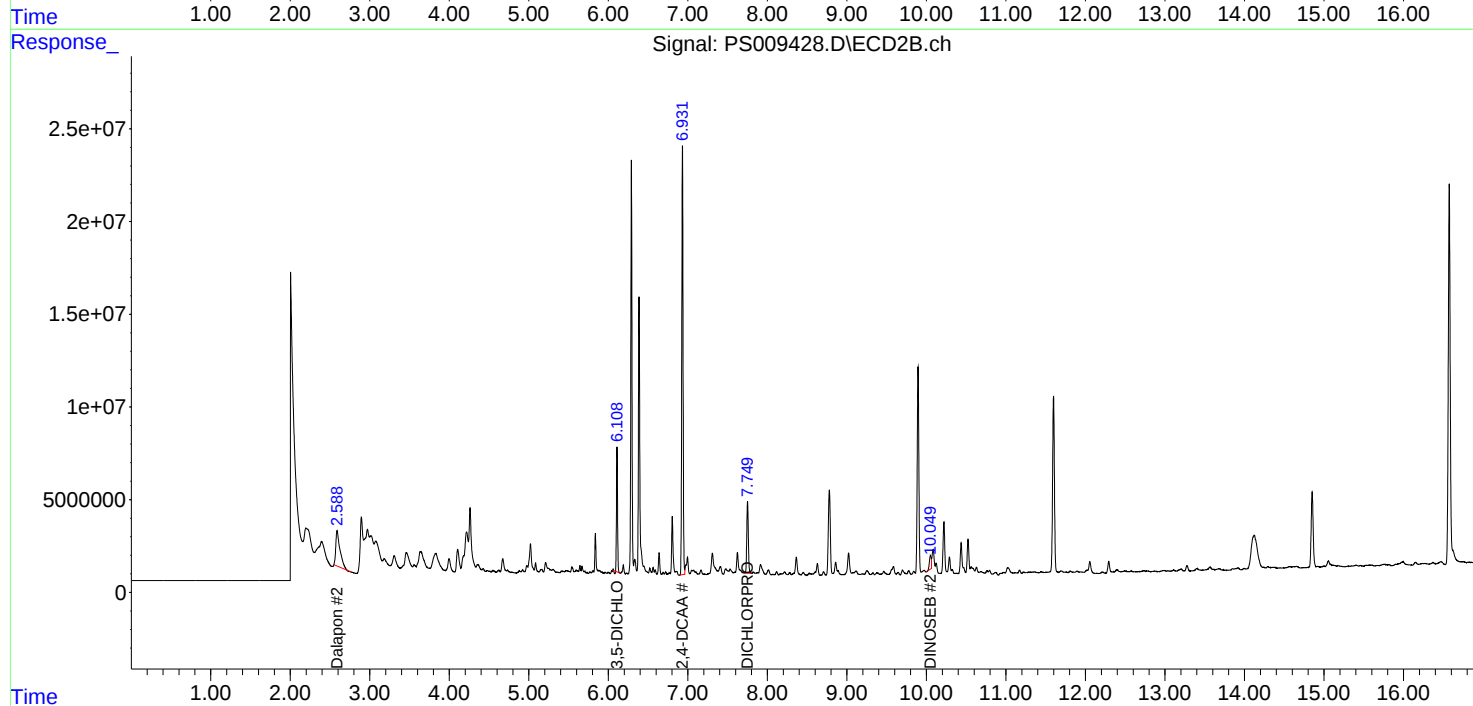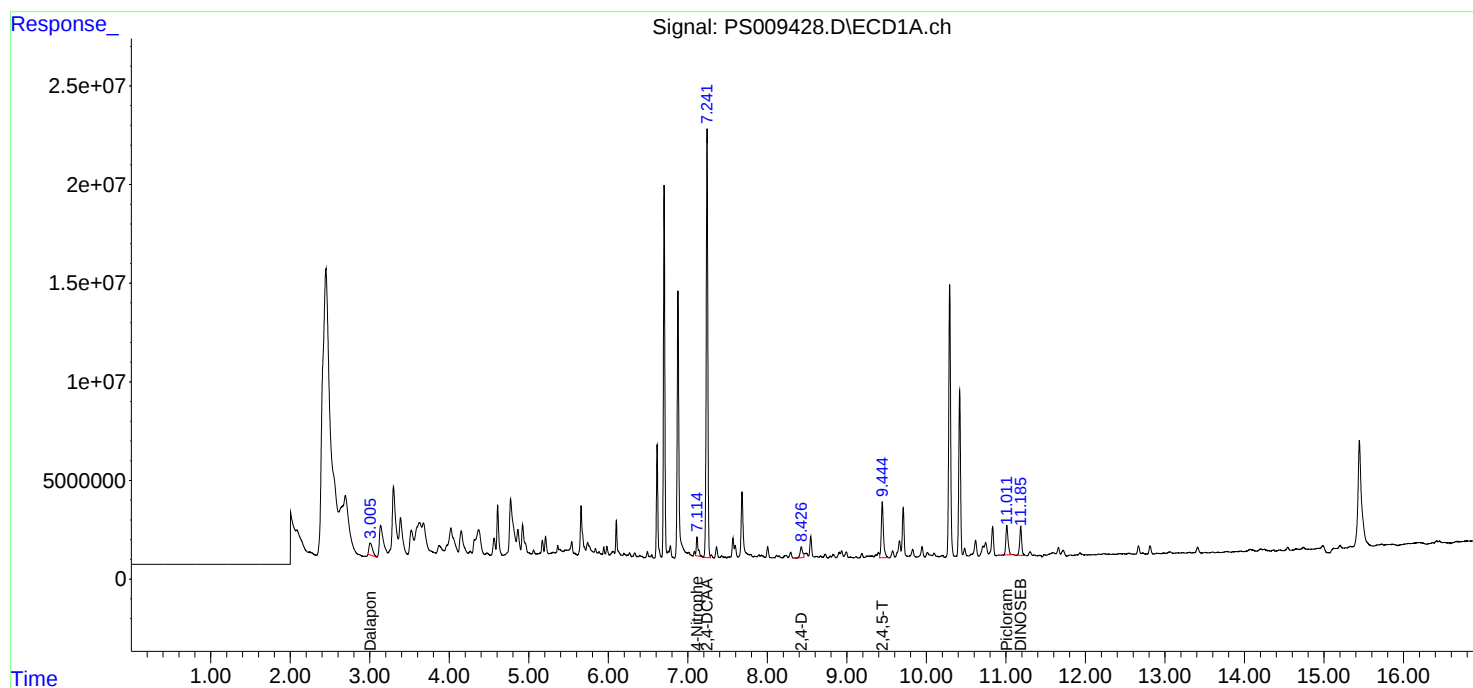


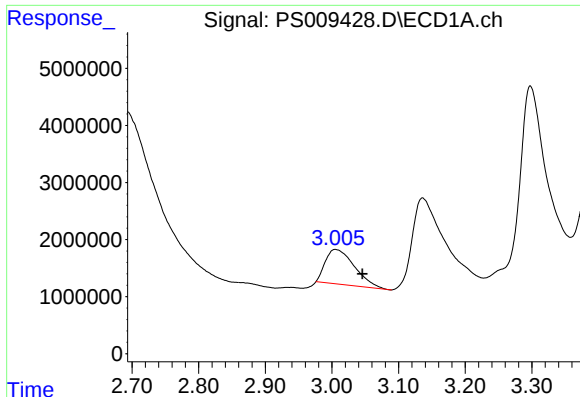

#1 Dalapon


R.T.: 3.005 min
Delta R.T.: -0.041 min
Response: 18409556
Conc: 23.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

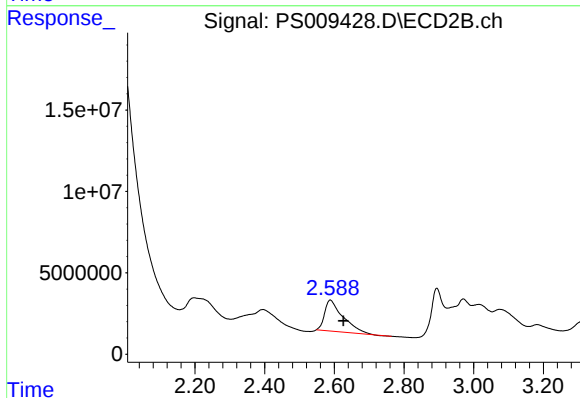


#1 Dalapon

R.T.: 2.588 min
Delta R.T.: -0.038 min
Response: 69971810
Conc: 88.87 ng/ml

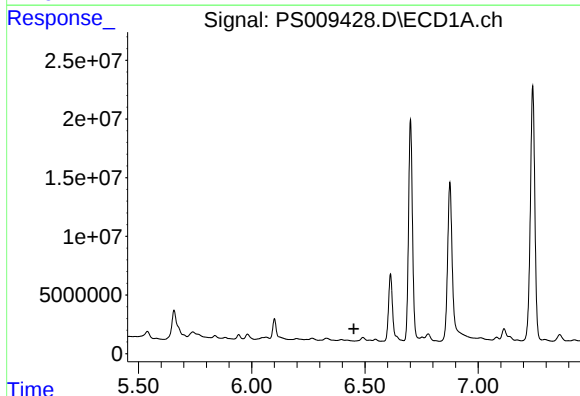


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

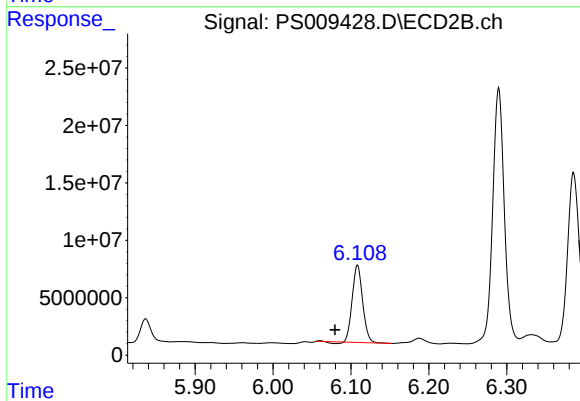

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.108 min
Delta R.T.: 0.029 min
Response: 61953528
Conc: 76.17 ng/ml

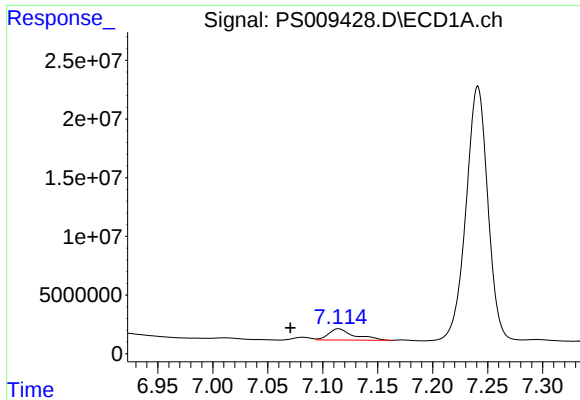

#3 4-Nitrophenol


R.T.: 7.114 min
Delta R.T.: 0.044 min
Response: 15307916
Conc: 64.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

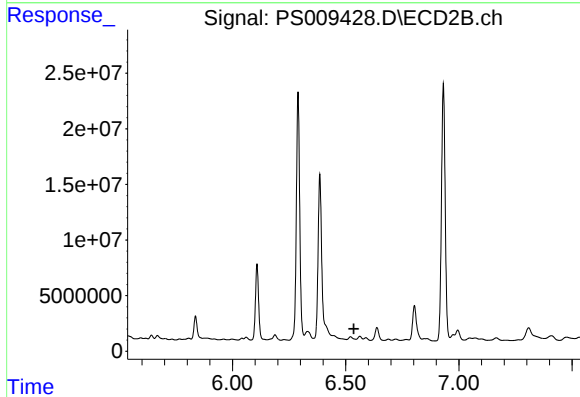


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.536 min
Response: 0
Conc: N.D.

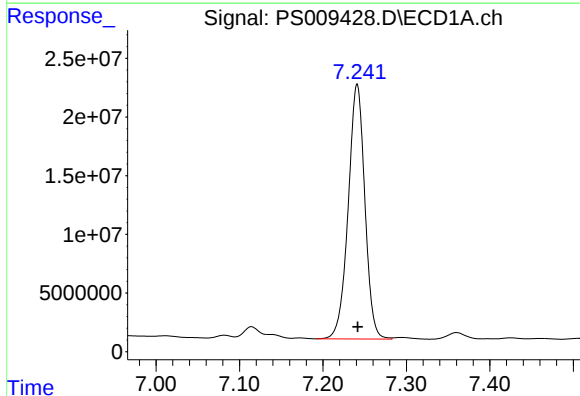


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 300515892
Conc: 543.26 ng/ml

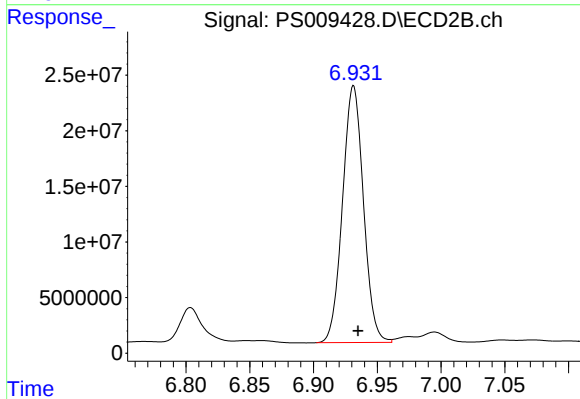

#4 2,4-DCAA


R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 263922199
Conc: 480.56 ng/ml

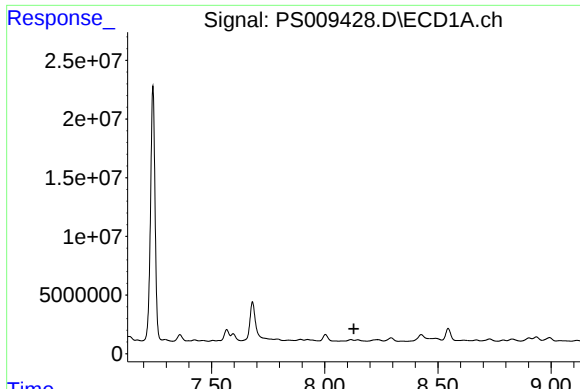

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

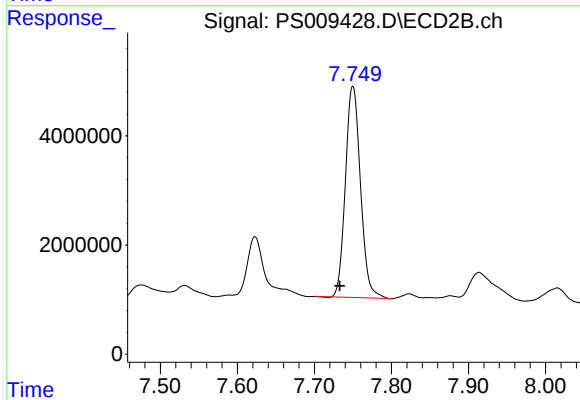


#8 DICHLORPROP

R.T.: 7.750 min
Delta R.T.: 0.017 min
Response: 52288891
Conc: 94.24 ng/ml

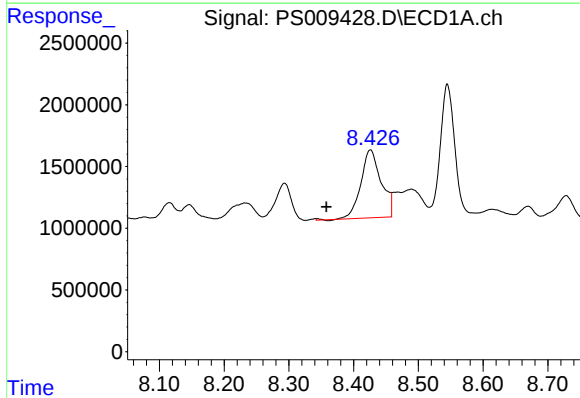


#9 2,4-D

R.T.: 8.426 min
Delta R.T.: 0.068 min
Response: 12032360
Conc: 22.82 ng/ml

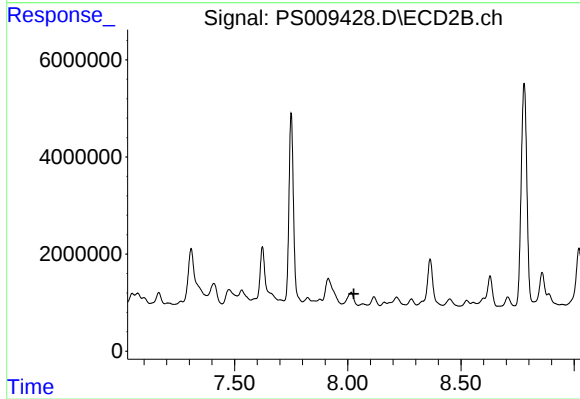

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

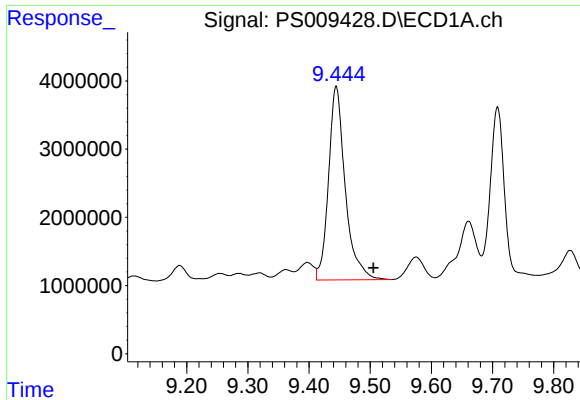

#12 2,4,5-T


R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 53878351
Conc: 21.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

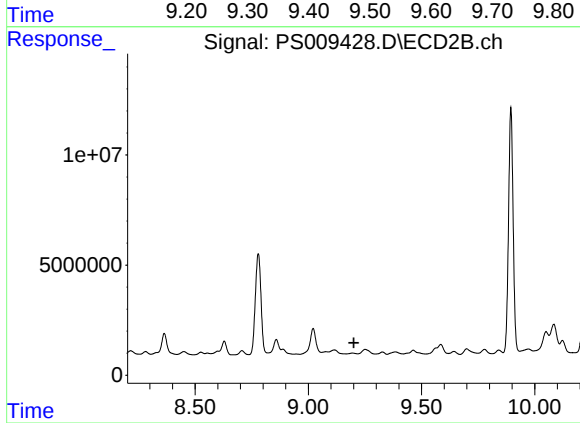


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

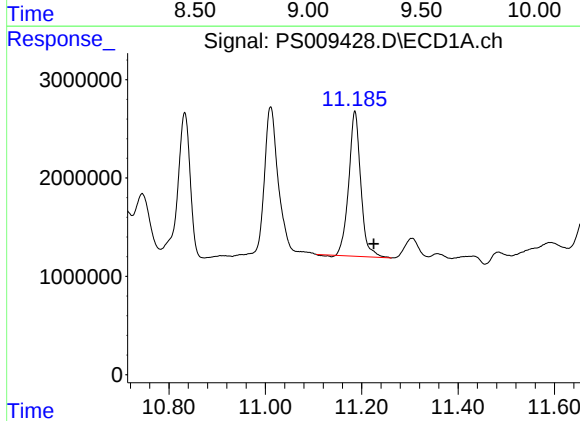


#14 DINOSEB

R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 25538335
Conc: 12.49 ng/ml

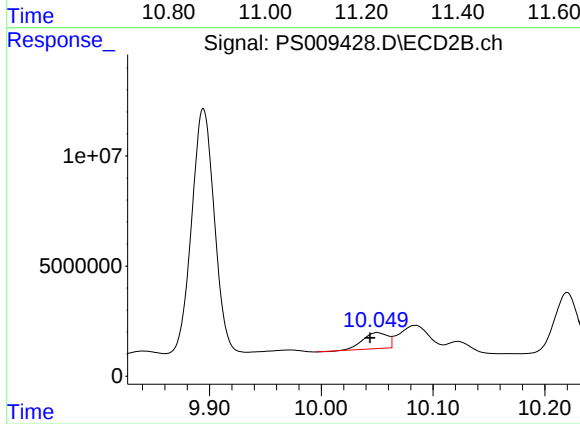

#14 DINOSEB


R.T.: 10.050 min
Delta R.T.: 0.006 min
Response: 11245862
Conc: 5.12 ng/ml

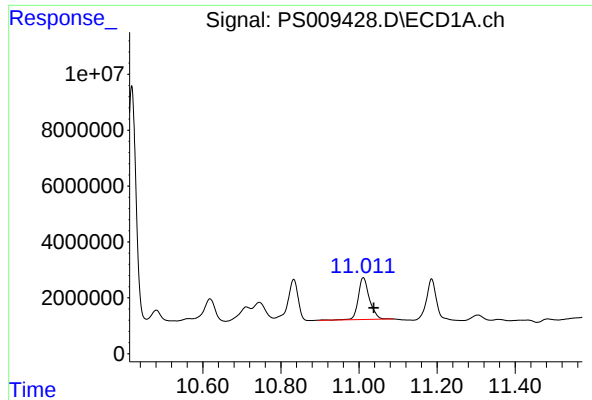

#15 Picloram

R.T.: 11.011 min
Delta R.T.: -0.026 min
Response: 29631240
Conc: 9.76 ng/ml

Instrument :
ECD_S
ClientSampleId :

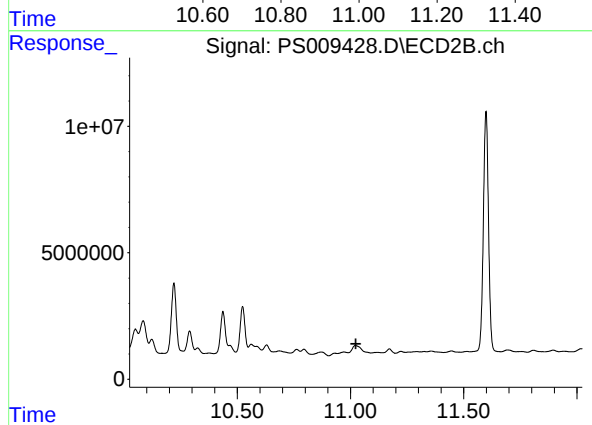

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.