

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
 Data File : PS009429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2020 22:25
 Operator : DD\AJ
 Sample : L2011-02
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 02:46:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	6.931	313.4E6	262.9E6	566.597	478.690
Target Compounds							
1) T	Dalapon	3.006	2.589	17446285	62649046	22.372	79.568 #
2) T	3,5-DICHL...	0.000	6.108	0	55985025	N.D.	68.836
3) T	4-Nitroph...	7.114	0.000	21017987	0	88.047	N.D. #
8) T	DICHLORPROP	0.000	7.750	0	38114142	N.D.	68.696
9) T	2,4-D	8.426	0.000	17696431	0	33.565	N.D. #
12) T	2,4,5-T	9.446	0.000	38002441	0	14.939	N.D. #
14) T	DINOSEB	11.186	10.084	29742910	34219605	14.550	15.579
15) T	Picloram	11.011	10.965	26957036	6499753	8.882	1.596 #
16) T	DCPA	0.000	10.965	0	6499753	N.D.	1.678



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032420\
Data File : PS009429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2020 22:25
Operator : DD\AJ
Sample : L2011-02
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 02:46:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

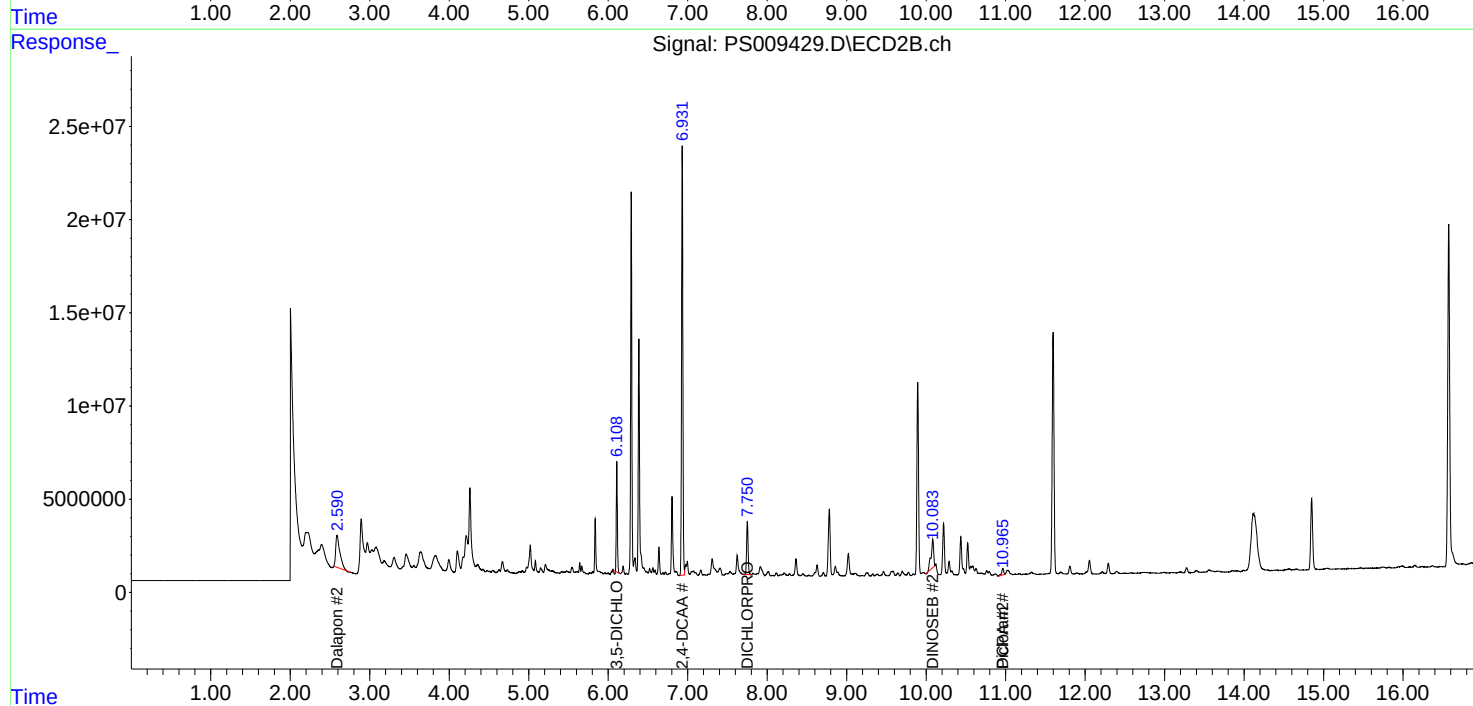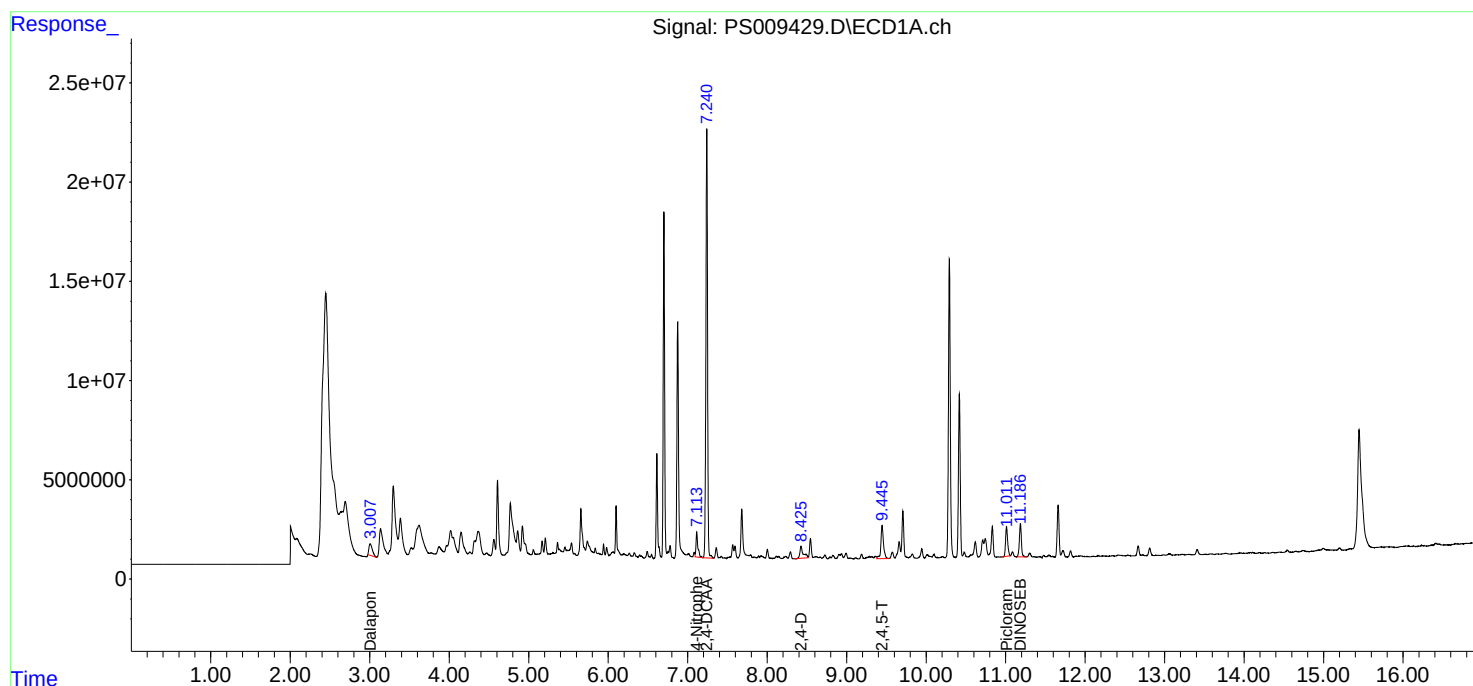


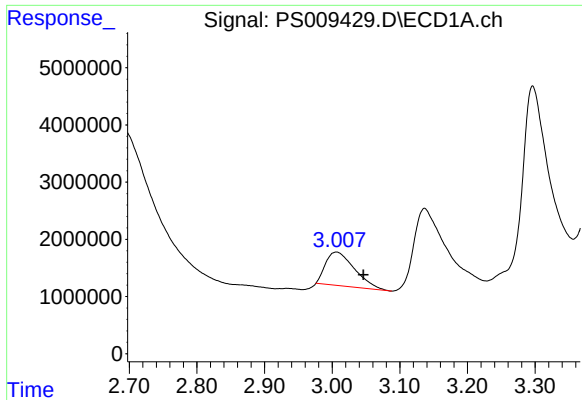

#1 Dalapon


R.T.: 3.006 min
Delta R.T.: -0.040 min
Response: 17446285
Conc: 22.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

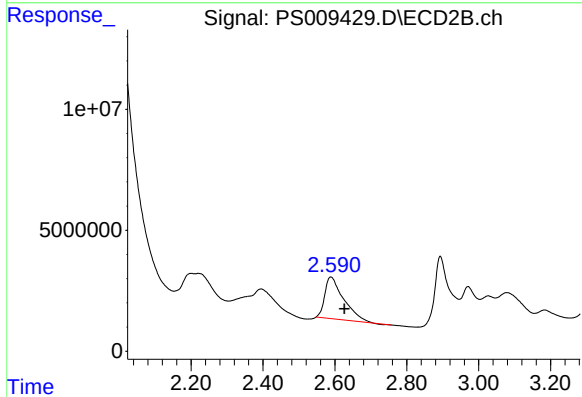


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.037 min
Response: 62649046
Conc: 79.57 ng/ml

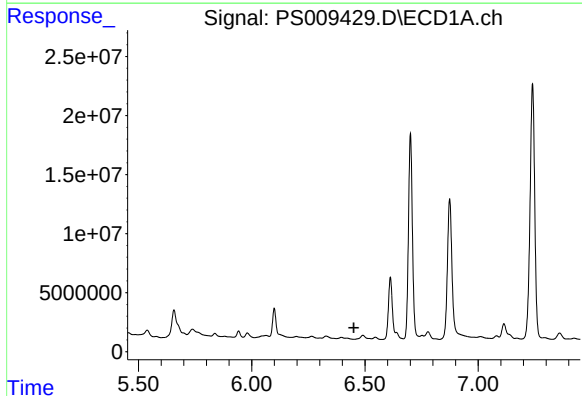


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

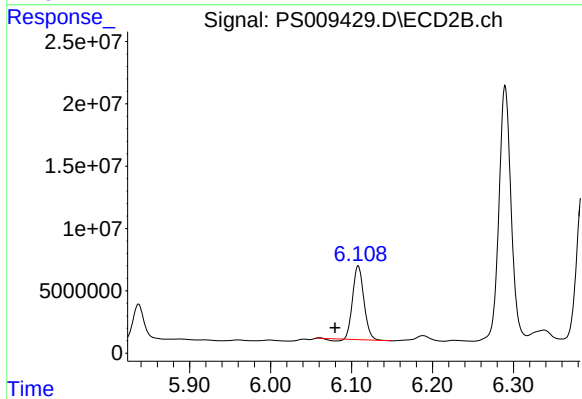

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.108 min
Delta R.T.: 0.029 min
Response: 55985025
Conc: 68.84 ng/ml

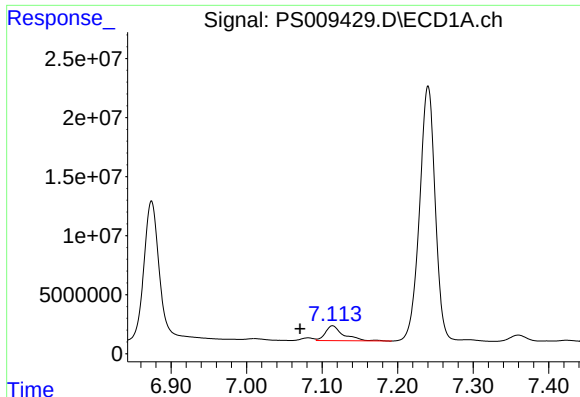

#3 4-Nitrophenol


R.T.: 7.114 min
Delta R.T.: 0.043 min
Response: 21017987
Conc: 88.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

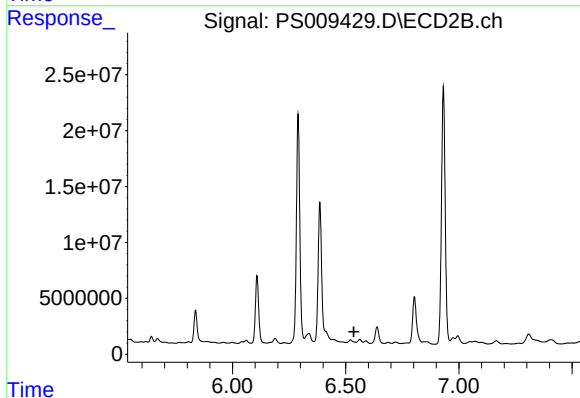


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 6.536 min
Response: 0
Conc: N.D.

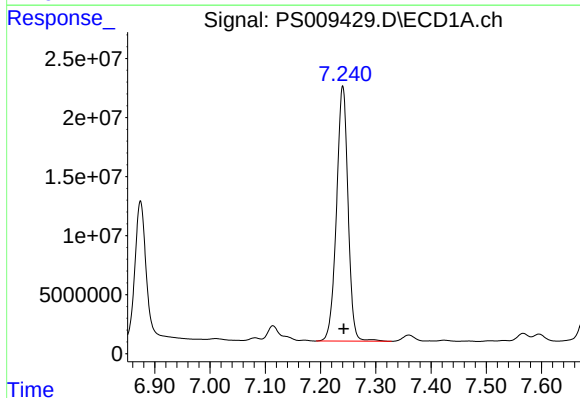


#4 2,4-DCAA

R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 313424675
Conc: 566.60 ng/ml

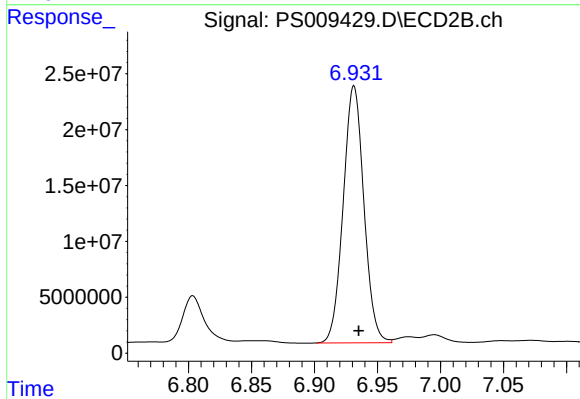

#4 2,4-DCAA


R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 262895680
Conc: 478.69 ng/ml

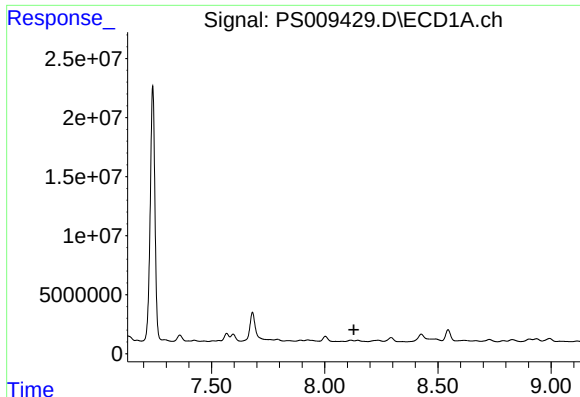

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

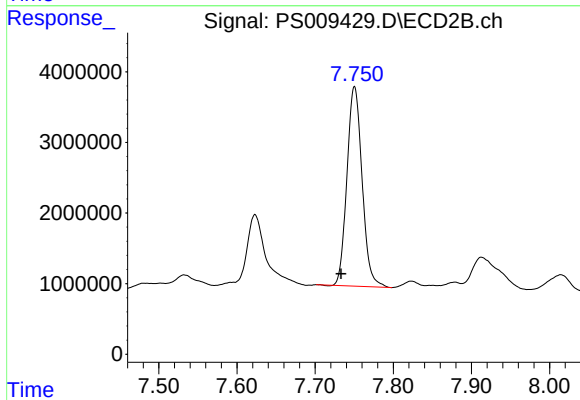


#8 DICHLORPROP

R.T.: 7.750 min
Delta R.T.: 0.017 min
Response: 38114142
Conc: 68.70 ng/ml

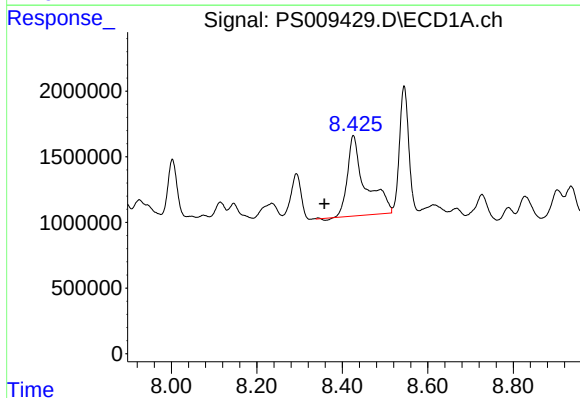


#9 2,4-D

R.T.: 8.426 min
Delta R.T.: 0.068 min
Response: 17696431
Conc: 33.57 ng/ml

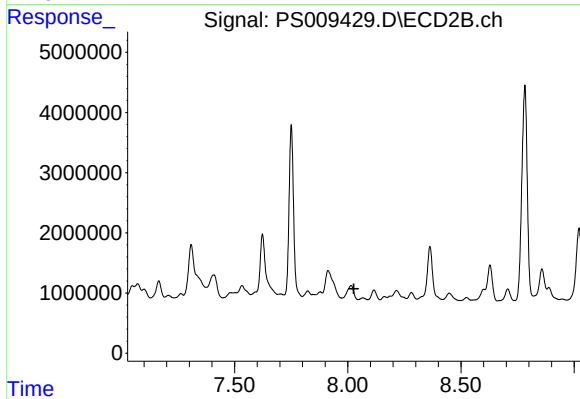

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

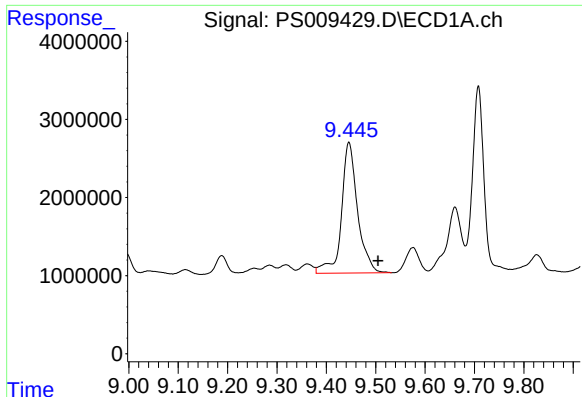

#12 2,4,5-T


R.T.: 9.446 min
Delta R.T.: -0.059 min
Response: 38002441
Conc: 14.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

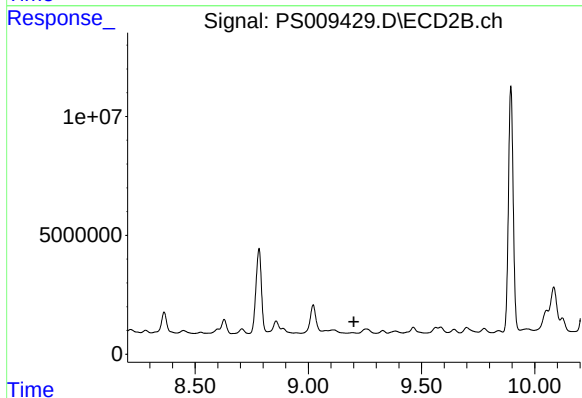


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

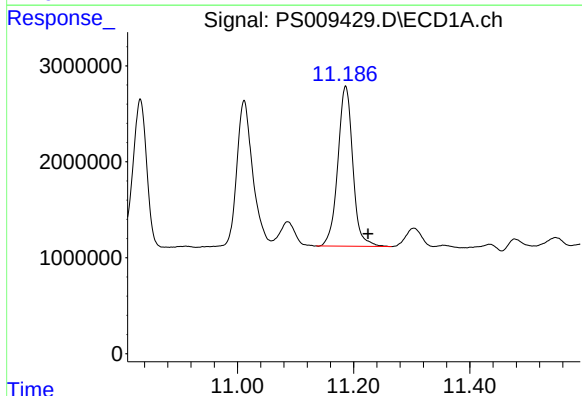


#14 DINOSEB

R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 29742910
Conc: 14.55 ng/ml

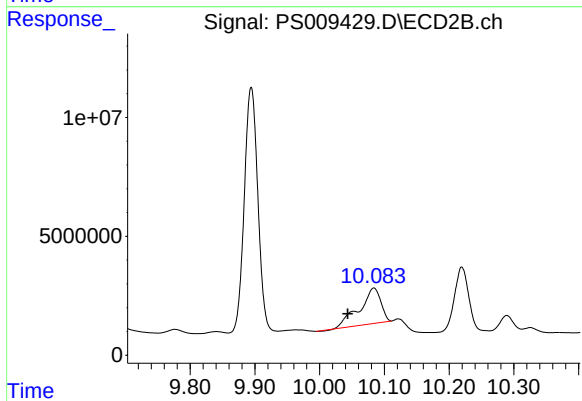

#14 DINOSEB


R.T.: 10.084 min
Delta R.T.: 0.040 min
Response: 34219605
Conc: 15.58 ng/ml

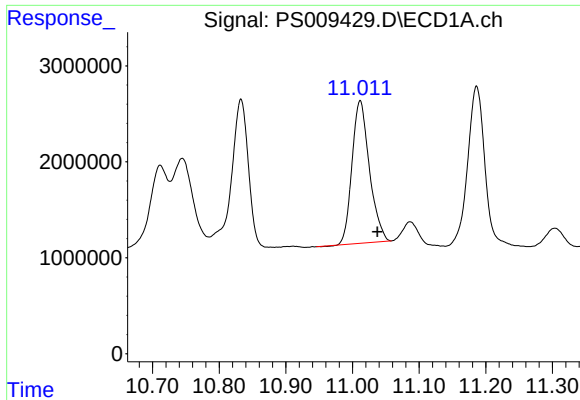

#15 Picloram


R.T.: 11.011 min
Delta R.T.: -0.026 min
Response: 26957036
Conc: 8.88 ng/ml

Instrument :
ECD_S
ClientSampleId :

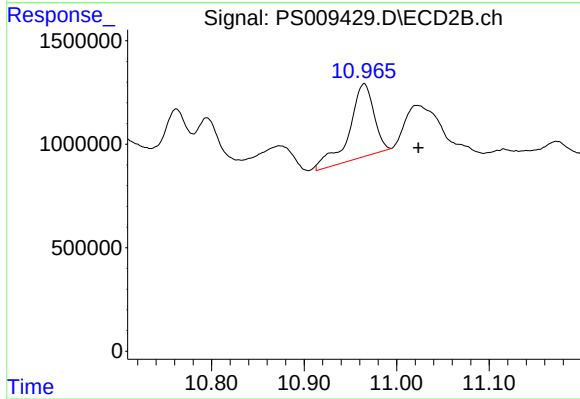


#15 Picloram

R.T.: 10.965 min
Delta R.T.: -0.059 min
Response: 6499753
Conc: 1.60 ng/ml

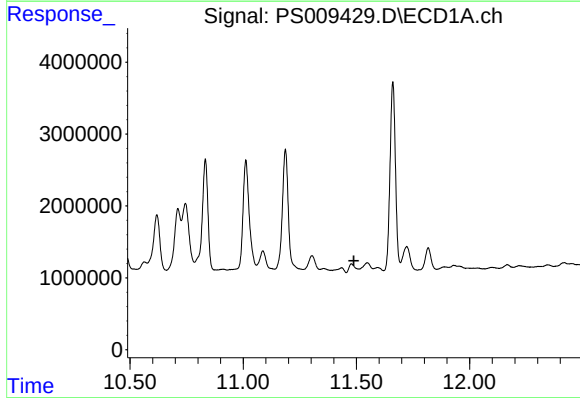

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

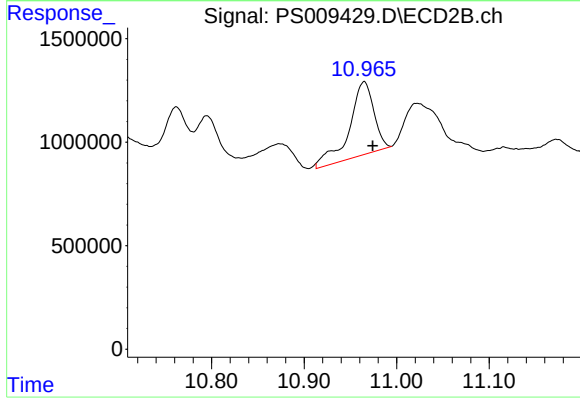

#16 DCPA

R.T.: 10.965 min
Delta R.T.: -0.009 min
Response: 6499753
Conc: 1.68 ng/ml