

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032421\
 Data File : PS014341.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2021 09:29
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 12:54:57 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
2) T	3,5-DICHL...	6.429	0.000	222.1E6	0	115.067	N.D. #
3) T	4-Nitroph...	6.956f	0.000	341061	0	<MDL	N.D. #
5) T	DICAMBA	7.426f	7.118f	30695776	86810099	5.708	43.333 #
6) T	MCP	0.000	7.118	0	86810099	N.D.	52.135
7) T	MCPA	7.650	0.000	7884803	0	1.371	N.D. #
8) T	DICHLORPROP	0.000	7.734f	0	1127165	N.D.	2.212
9) T	2,4-D	8.343f	0.000	142.8E6	0	96.849	N.D. #
13) T	2,4-DB	9.919f	0.000	25921137	0	16.762	N.D. #
15) T	Picloram	10.951	10.983	10985655	12344345	1.052	3.254 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032421\
Data File : PS014341.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2021 09:29
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 12:54:57 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

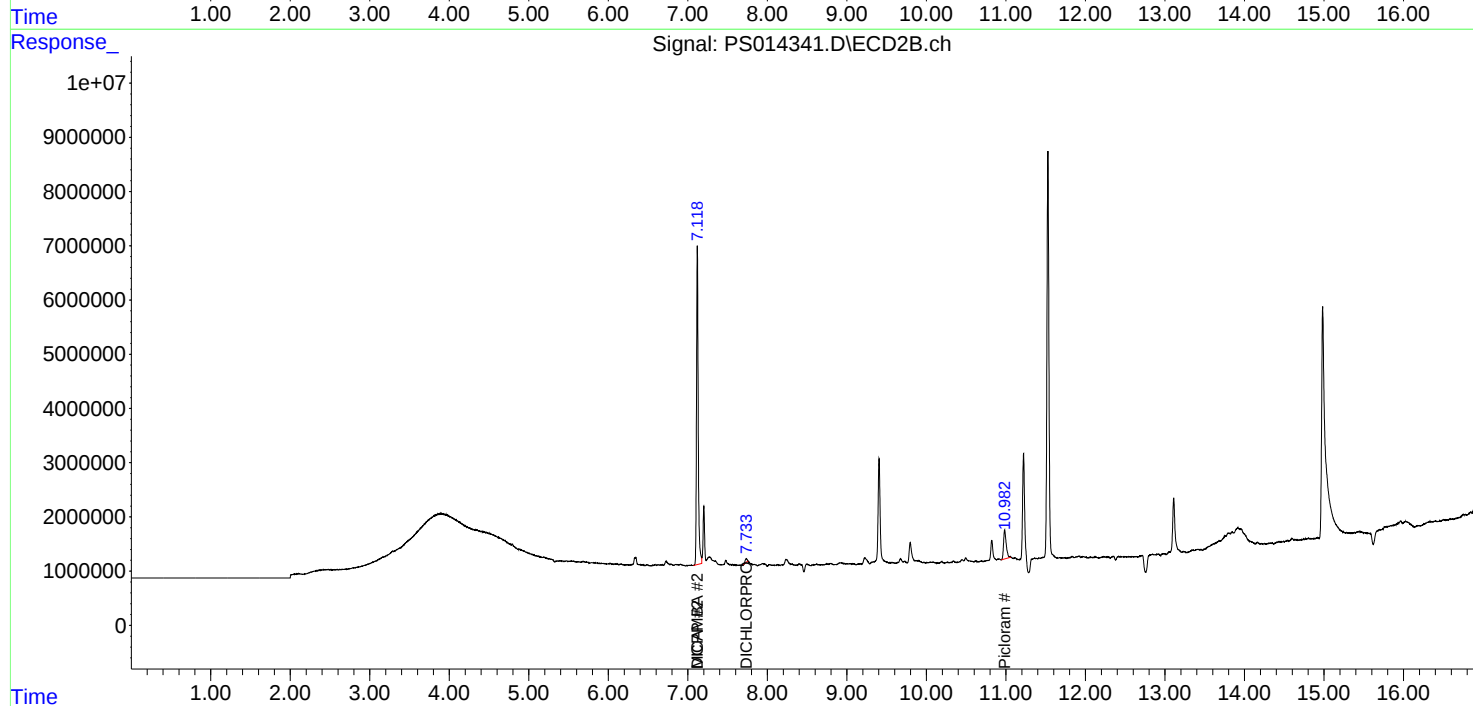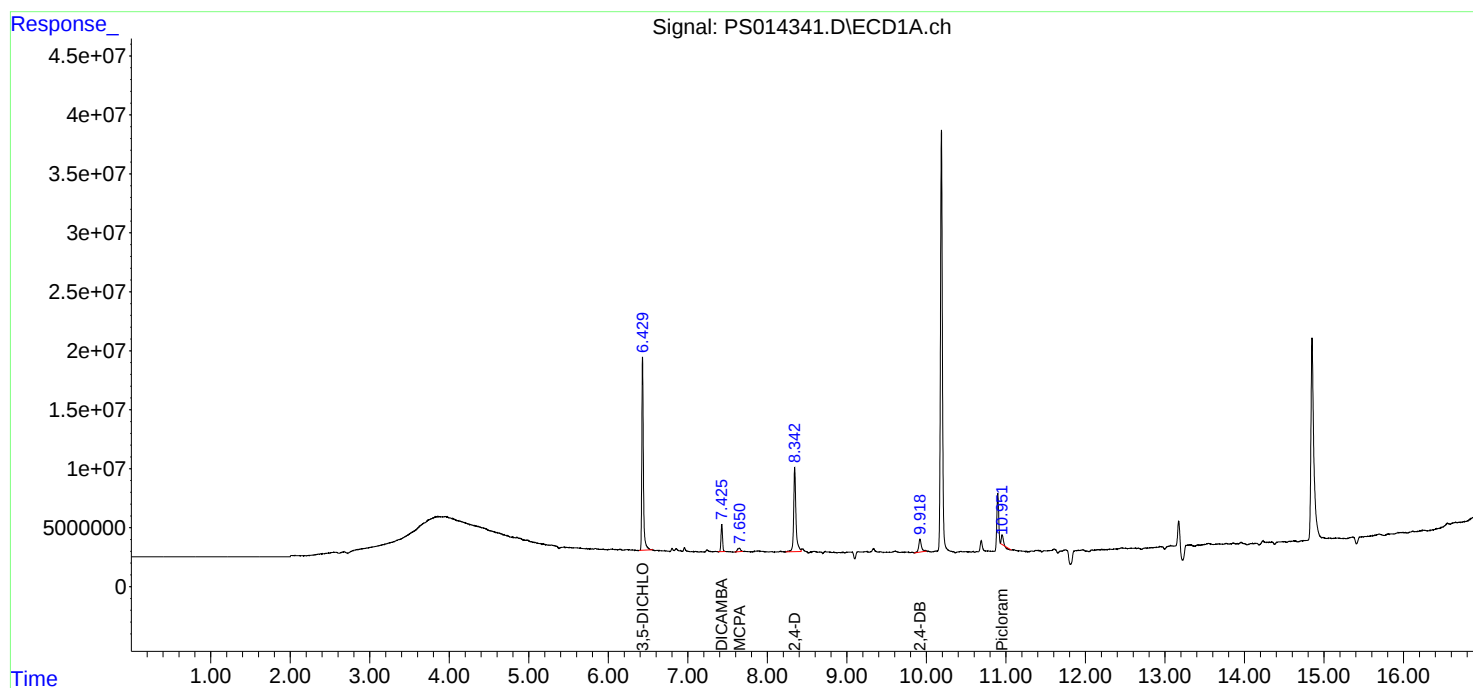


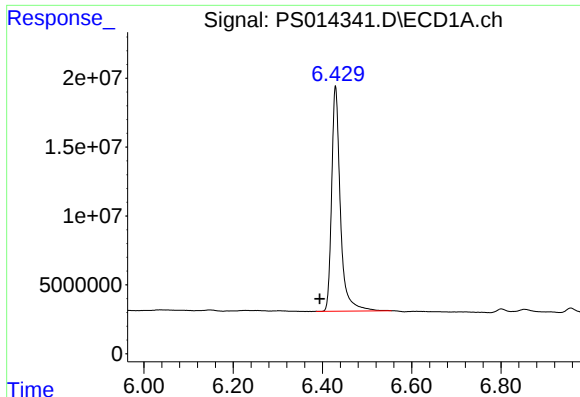

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.429 min
Delta R.T.: 0.035 min
Response: 222142646
Conc: 115.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

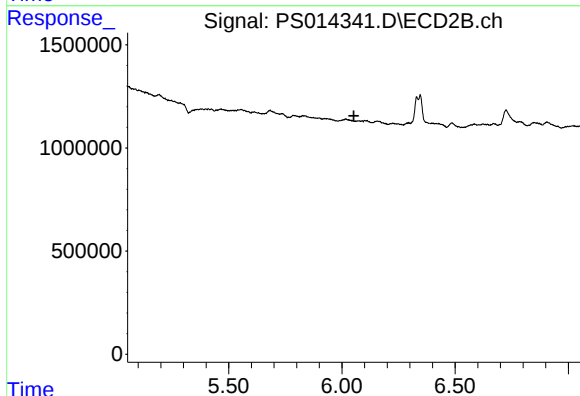


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.053 min
Response: 0
Conc: N.D.

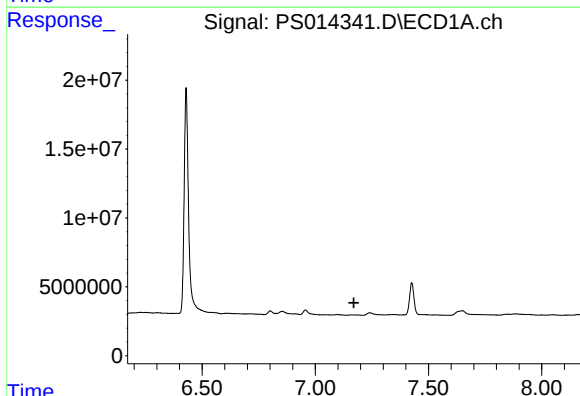


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.170 min
Response: 0
Conc: N.D.

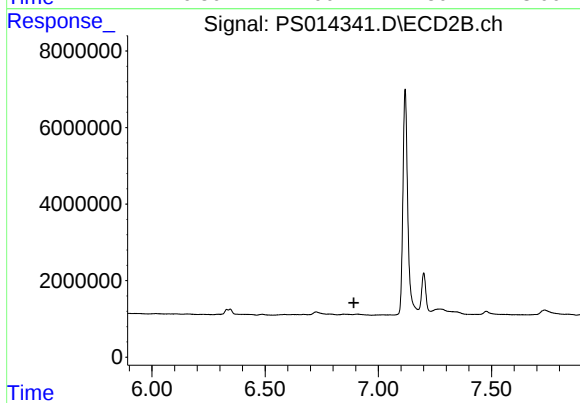

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.892 min
Response: 0
Conc: N.D.

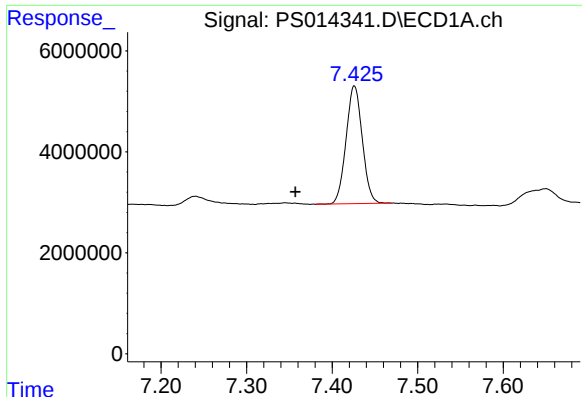

#5 DICAMBA


R.T.: 7.426 min
Delta R.T.: 0.069 min
Response: 30695776
Conc: 5.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

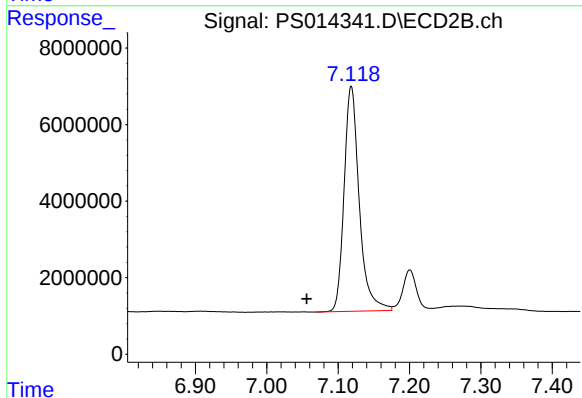


#5 DICAMBA

R.T.: 7.118 min
Delta R.T.: 0.062 min
Response: 86810099
Conc: 43.33 ng/ml

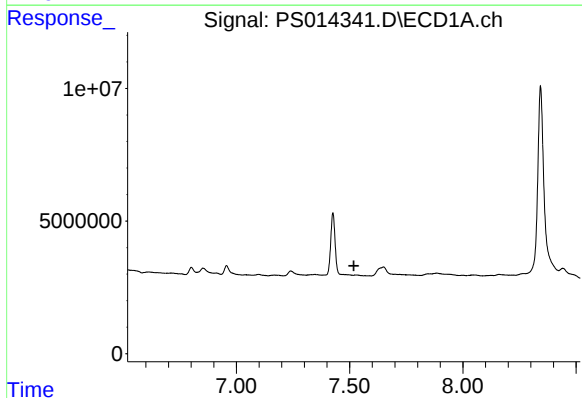


#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.518 min
Response: 0
Conc: N.D.

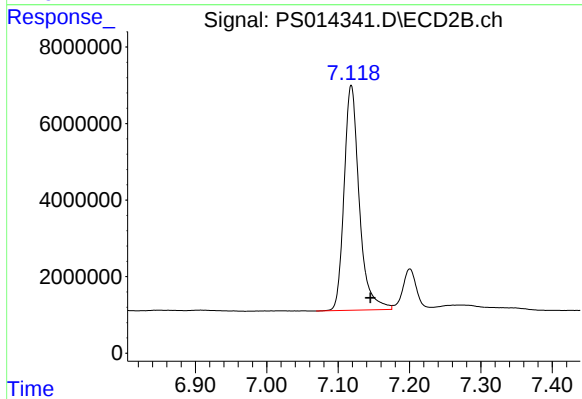

#6 MCP


R.T.: 7.118 min
Delta R.T.: -0.027 min
Response: 86810099
Conc: 52.13 ug/ml

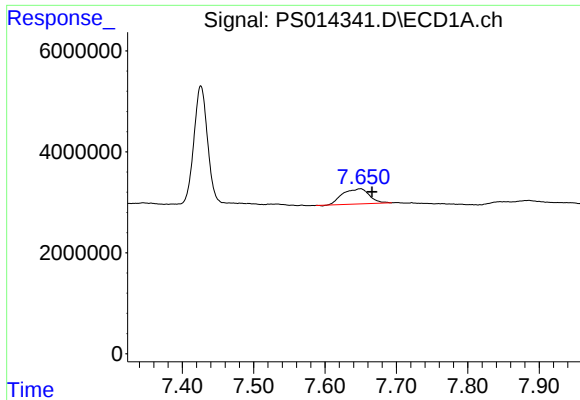

#7 MCPA


R.T.: 7.650 min
Delta R.T.: -0.016 min
Response: 7884803
Conc: 1.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

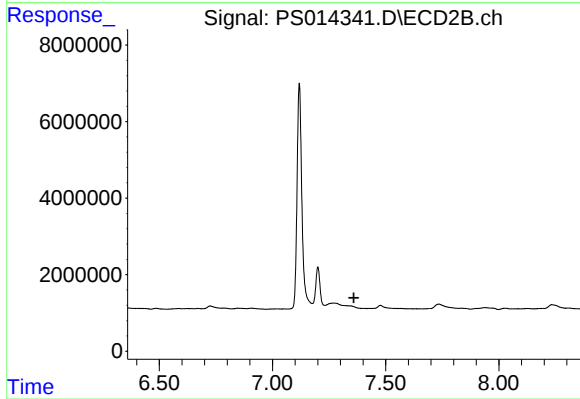


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.359 min
Response: 0
Conc: N.D.

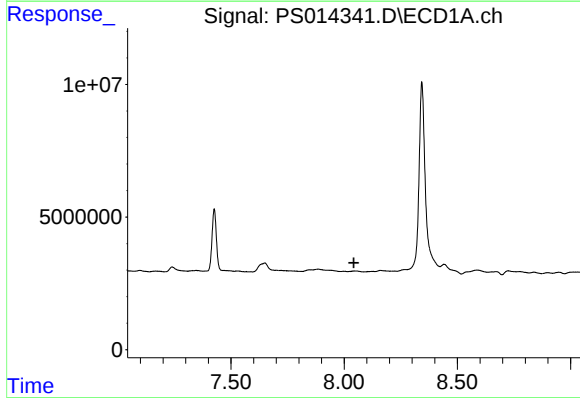


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.043 min
Response: 0
Conc: N.D.

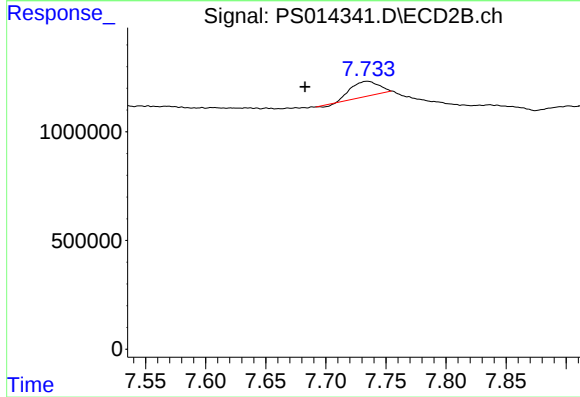

#8 DICHLORPROP


R.T.: 7.734 min
Delta R.T.: 0.052 min
Response: 1127165
Conc: 2.21 ng/ml

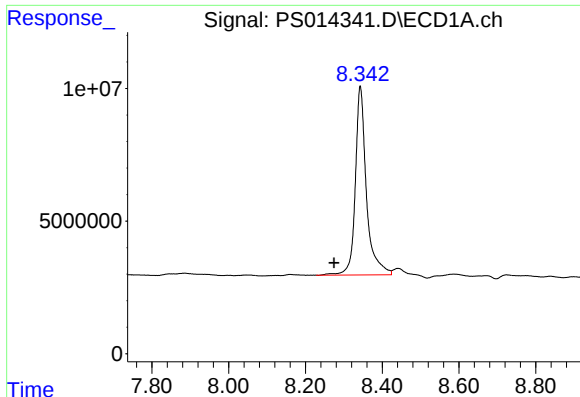

#9 2,4-D


R.T.: 8.343 min
Delta R.T.: 0.068 min
Response: 142753637
Conc: 96.85 ng/ml

Instrument :
ECD_S
ClientSampleId :

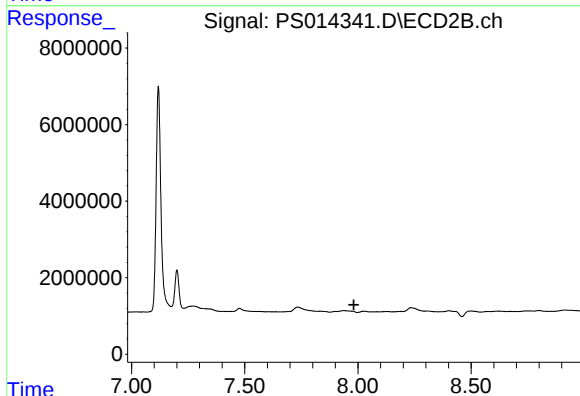


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.982 min
Response: 0
Conc: N.D.

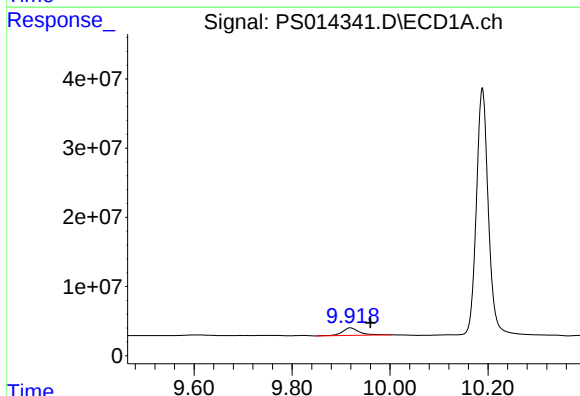


#13 2,4-DB

R.T.: 9.919 min
Delta R.T.: -0.041 min
Response: 25921137
Conc: 16.76 ng/ml

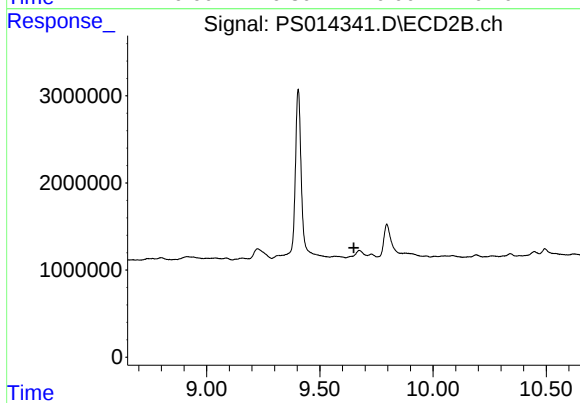

#13 2,4-DB


R.T.: 0.000 min
Exp R.T. : 9.651 min
Response: 0
Conc: N.D.

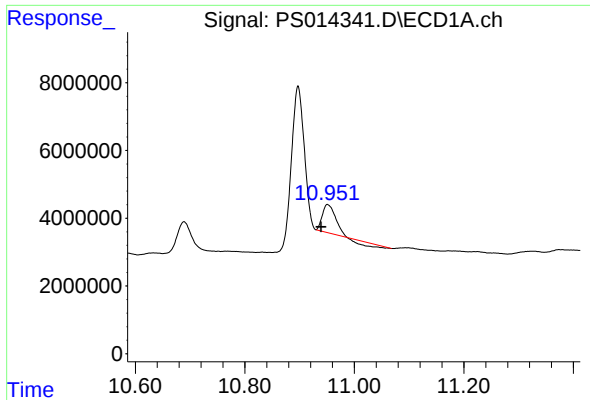

#15 Picloram

R.T.: 10.951 min
Delta R.T.: 0.011 min
Response: 10985655
Conc: 1.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

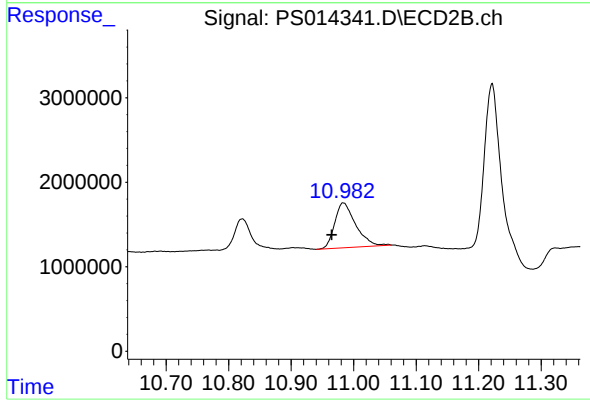

#15 Picloram

R.T.: 10.983 min
Delta R.T.: 0.019 min
Response: 12344345
Conc: 3.25 ng/ml