

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032421\
 Data File : PS014342.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2021 09:58
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 12:55:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.164	6.888	640.7E6	252.5E6	448.387	535.319
Target Compounds							
9) T	2,4-D	8.332f	0.000	16624471	0	11.279	N.D. #
15) T	Picloram	10.962	10.990	20967340	7698523	2.008	2.029



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032421\
Data File : PS014342.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2021 09:58
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 12:55:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

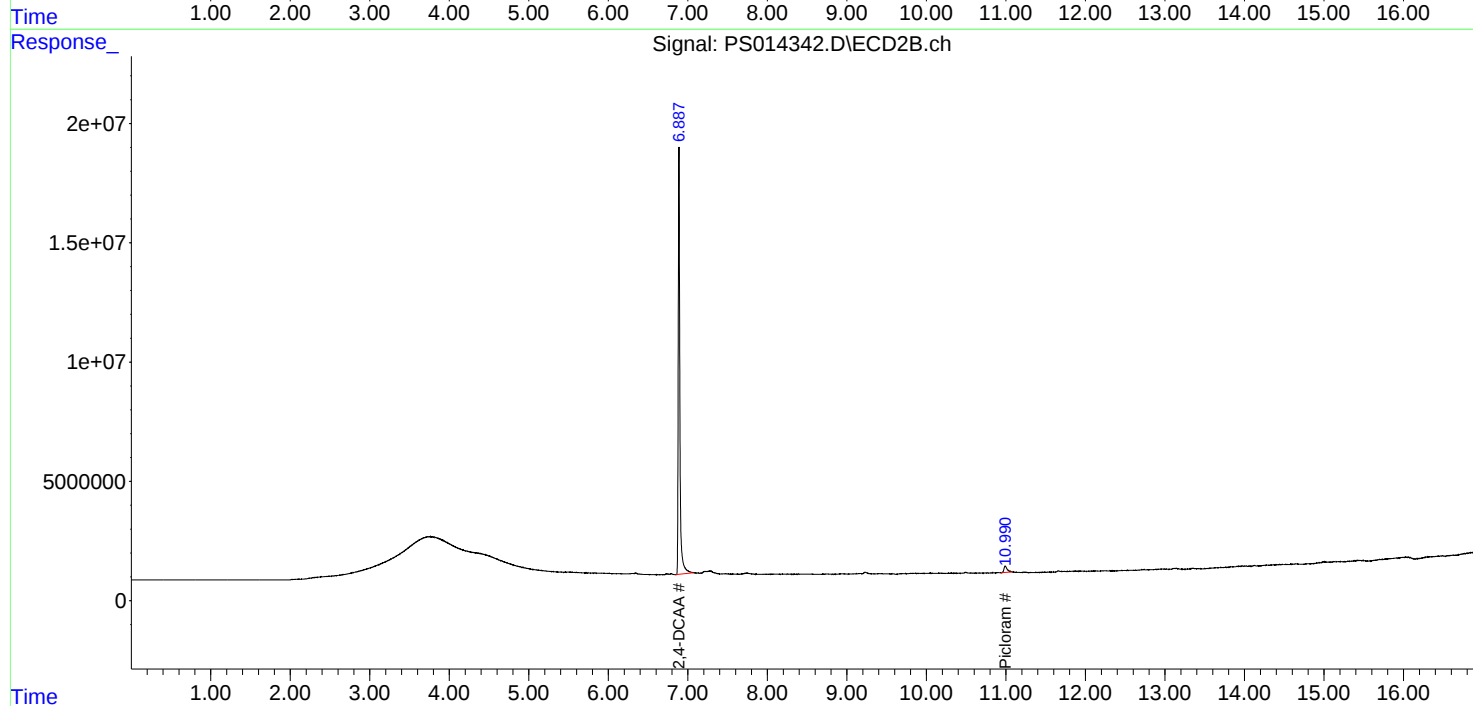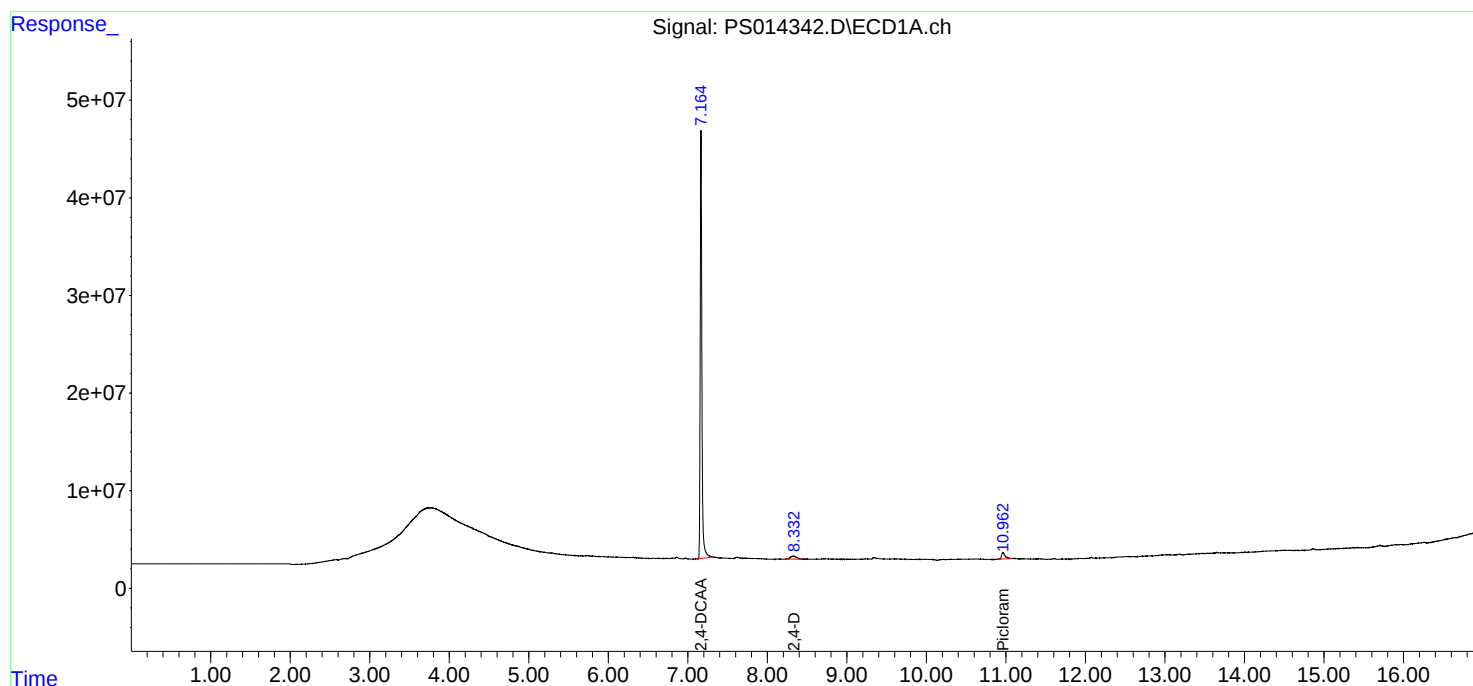


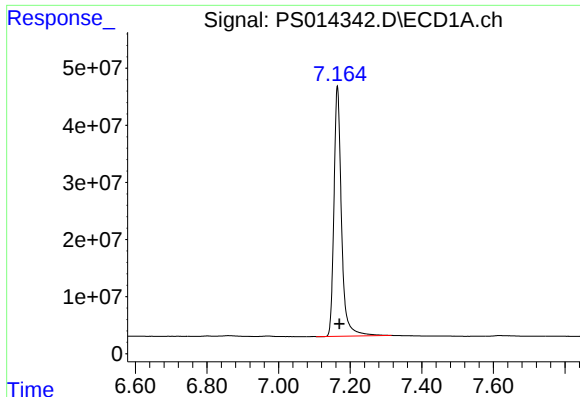

#4 2,4-DCAA


R.T.: 7.164 min
Delta R.T.: -0.006 min
Response: 640674336
Conc: 448.39 ng/ml

Instrument :
ECD_S
ClientSampleId :

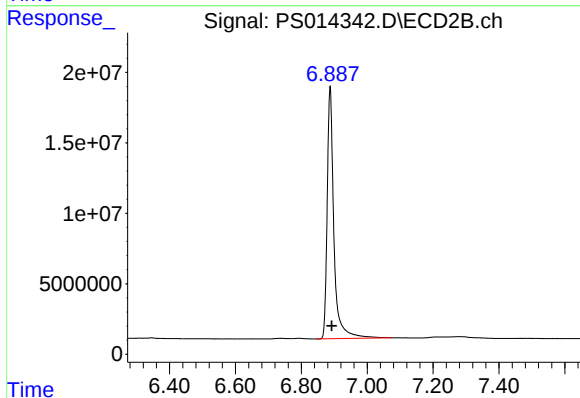


#4 2,4-DCAA

R.T.: 6.888 min
Delta R.T.: -0.004 min
Response: 252546854
Conc: 535.32 ng/ml

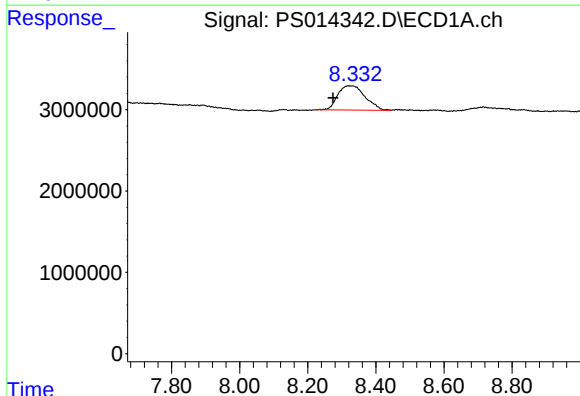


#9 2,4-D

R.T.: 8.332 min
Delta R.T.: 0.057 min
Response: 16624471
Conc: 11.28 ng/ml

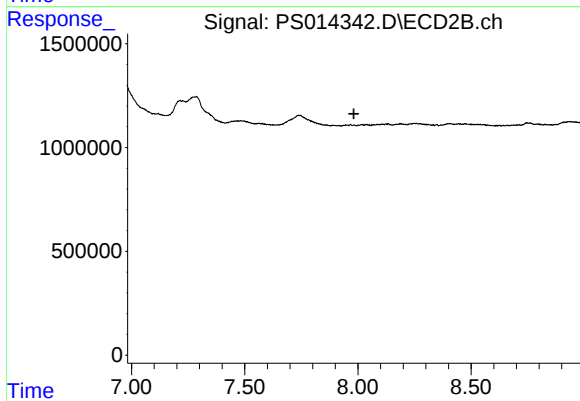

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.982 min
Response: 0
Conc: N.D.

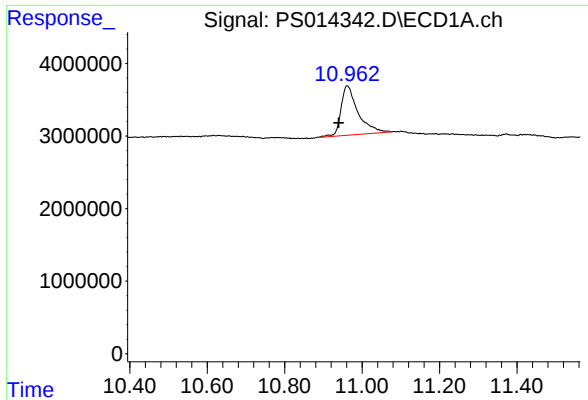

#15 Picloram

R.T.: 10.962 min
Delta R.T.: 0.022 min
Response: 20967340
Conc: 2.01 ng/ml

Instrument :
ECD_S
ClientSampleId :

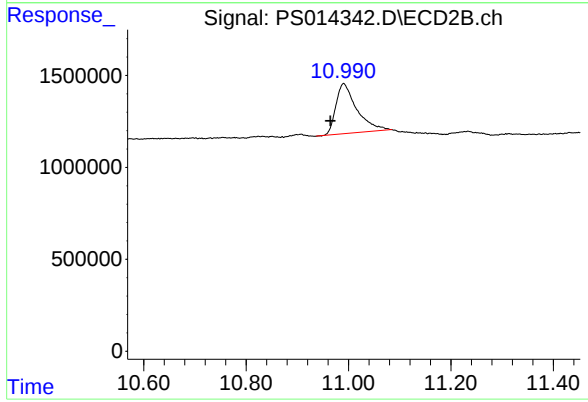

#15 Picloram

R.T.: 10.990 min
Delta R.T.: 0.026 min
Response: 7698523
Conc: 2.03 ng/ml