

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032421\
 Data File : PS014349.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2021 15:30
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 16:19:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.164	6.886	638.8E6	247.1E6	447.052	523.681
Target Compounds							
5) T	DICAMBA	0.000	6.996f	0	313872	N.D.	<MDL
7) T	MCPA	7.621f	0.000	6835147	0	1.188	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032421\
Data File : PS014349.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2021 15:30
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 16:19:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

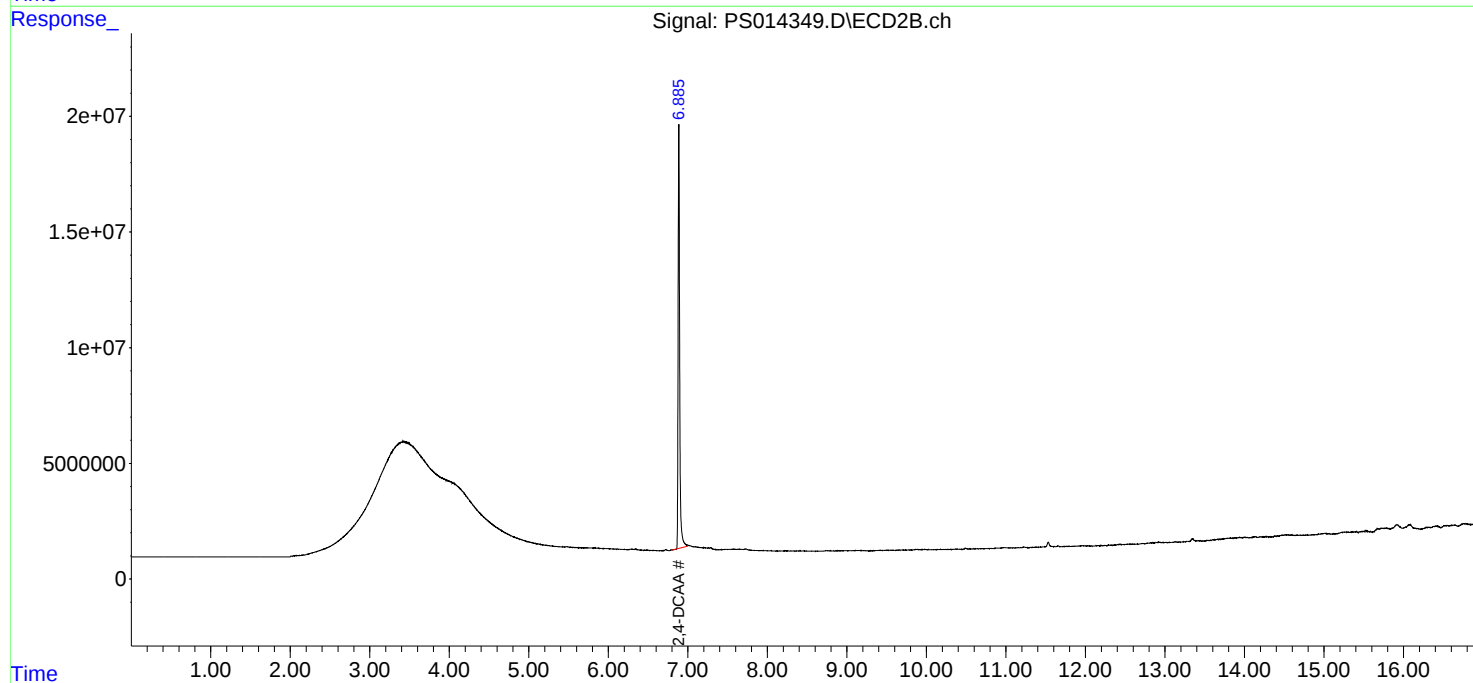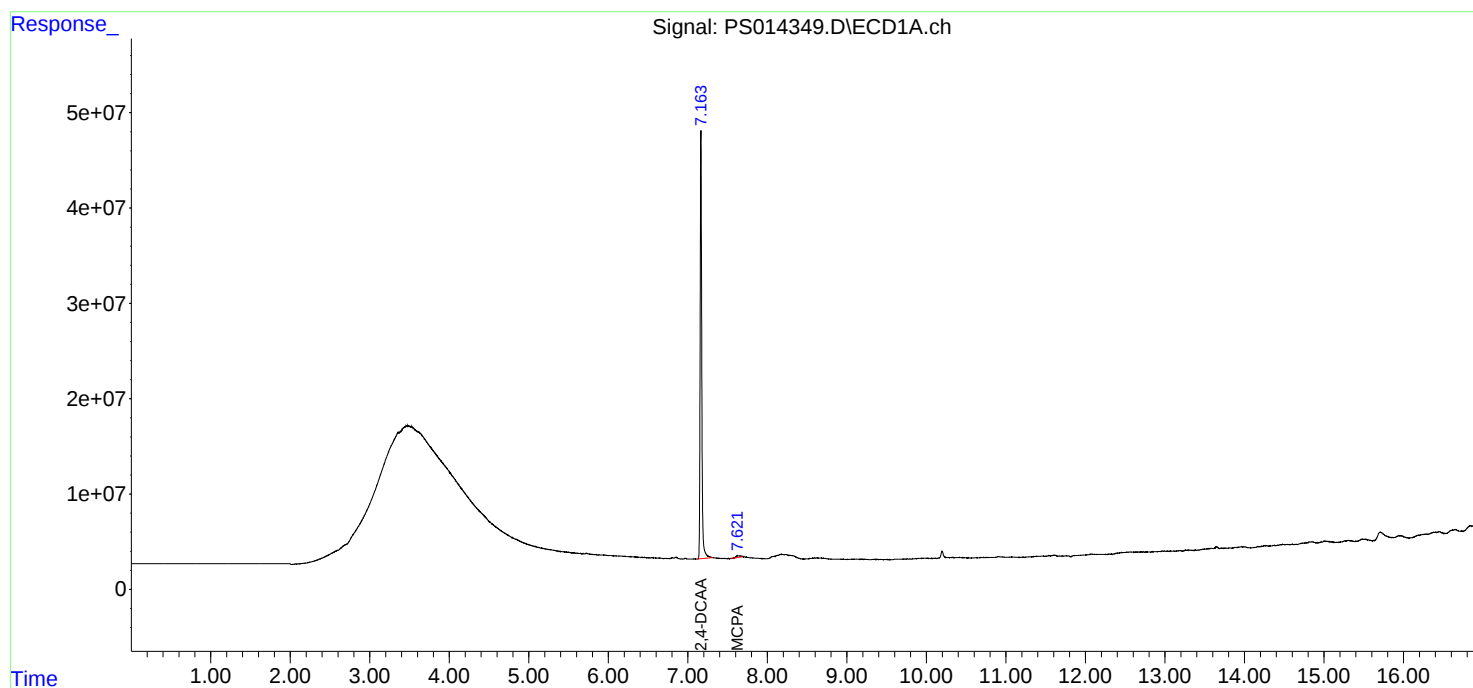


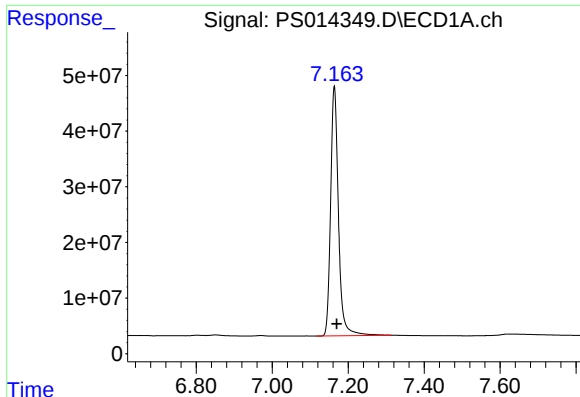

#4 2,4-DCAA


R.T.: 7.164 min
Delta R.T.: -0.007 min
Response: 638766465
Conc: 447.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

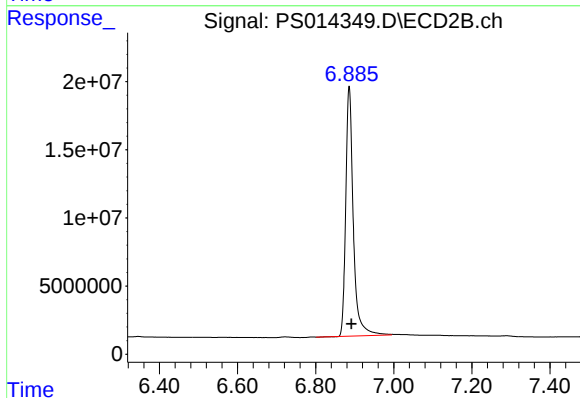


#4 2,4-DCAA

R.T.: 6.886 min
Delta R.T.: -0.006 min
Response: 247056167
Conc: 523.68 ng/ml

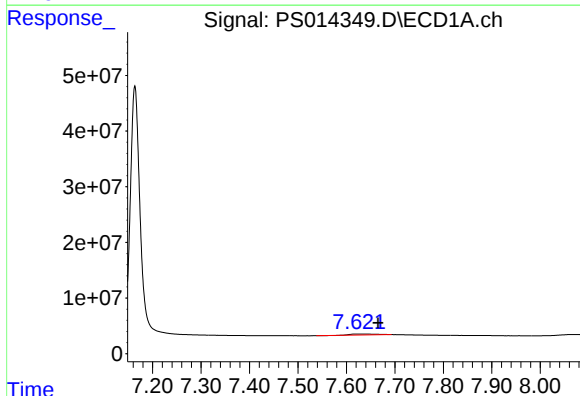

#7 MCPA

R.T.: 7.621 min
Delta R.T.: -0.045 min
Response: 6835147
Conc: 1.19 ug/ml

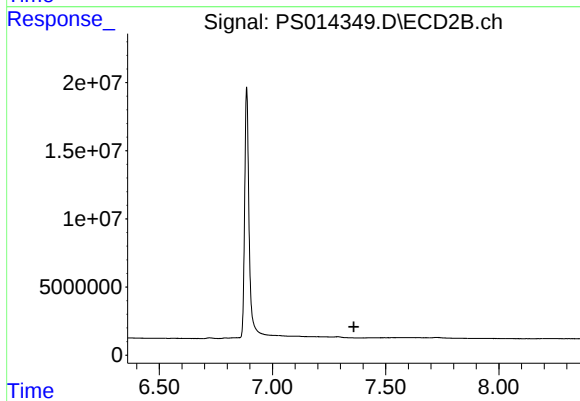

#7 MCPA

R.T.: 0.000 min
Exp R.T.: 7.359 min
Response: 0
Conc: N.D.