

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032422\
 Data File : PS018730.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 09:17
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 15:32:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.236	6.813	4688581	1891687	1.647	2.688 #
Target Compounds							
2) T	3,5-DICHL...	6.476	0.000	411.2E6	0	106.706	N.D. #
3) T	4-Nitroph...	7.019f	0.000	3805961	0	2.209	N.D. #
5) T	DICAMBA	7.383f	7.034f	-1574941	95537726	N.D.	32.075
6) T	MCP	0.000	7.034f	0	95537726	N.D.	39.025
7) T	MCPA	7.770	0.000	3845950	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.623	0	32327590	N.D.	40.838
9) T	2,4-D	8.408f	0.000	275.2E6	0	82.145	N.D. #
10) T	Pentachlo...	8.664	8.370f	7697013	4492317	<MDL	<MDL #
11) T	2,4,5-TP ...	9.274f	8.638f	17470987	3761674	1.149	<MDL #
12) T	2,4,5-T	9.474	9.040	3334749	3915460	<MDL	<MDL #
13) T	2,4-DB	9.999f	0.000	1508047	0	<MDL	N.D. #
15) T	Picloram	10.999	10.875	413.7E6	21852456	20.126	4.111 #
16) T	DCPA	0.000	10.875f	0	21852456	N.D.	4.155



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032422\
Data File : PS018730.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 09:17
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 15:32:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

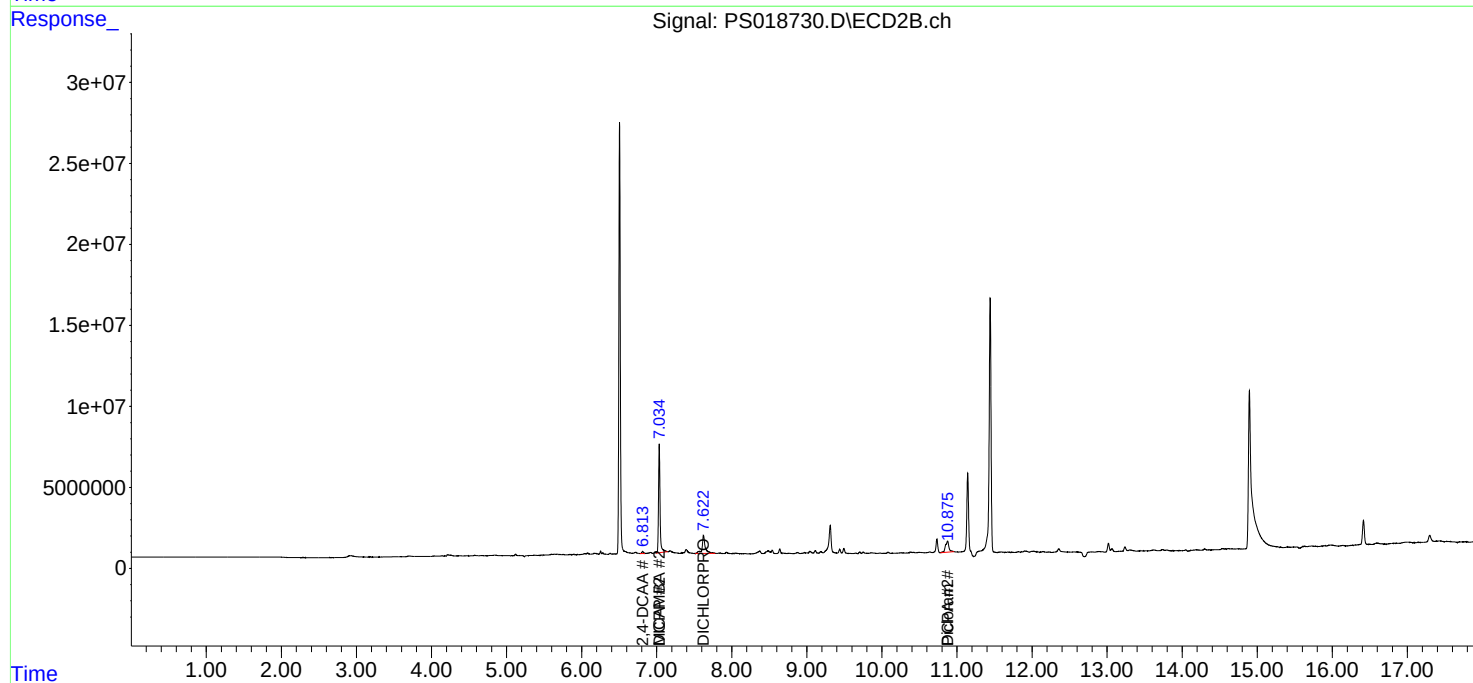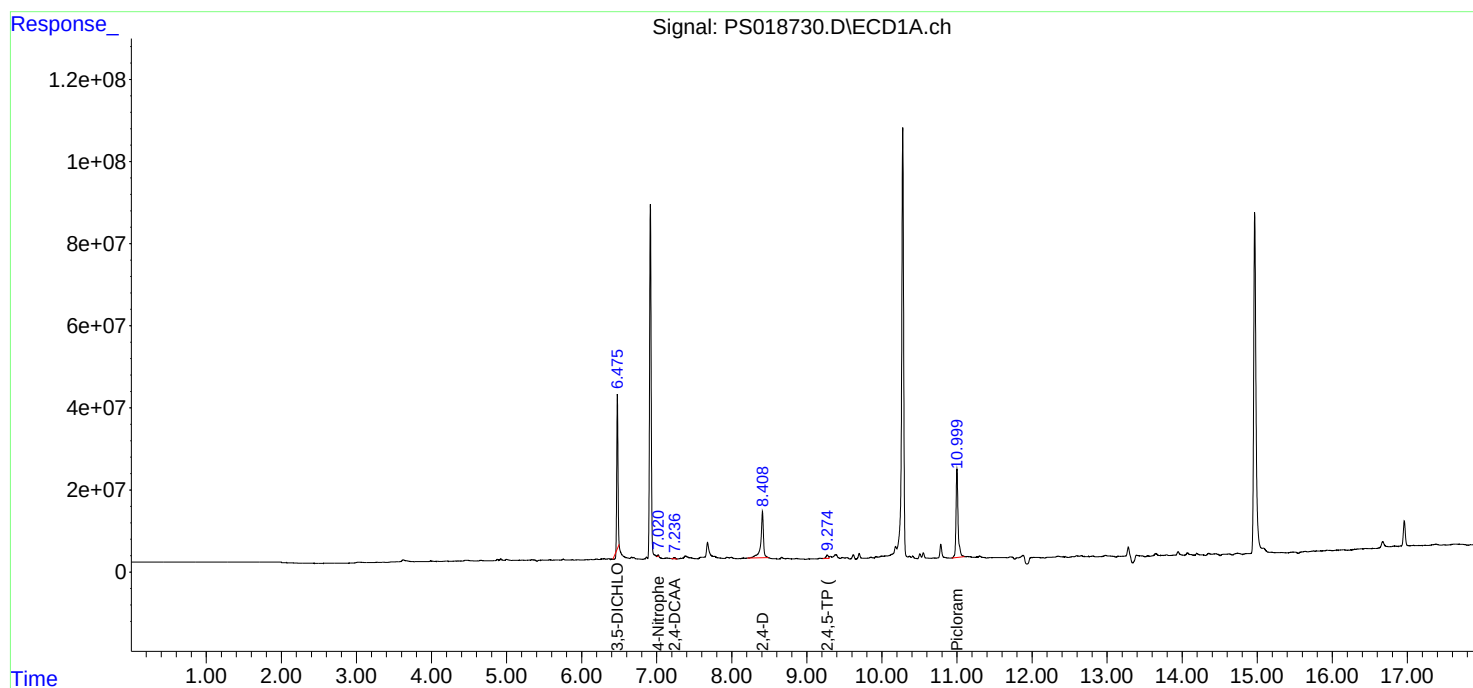


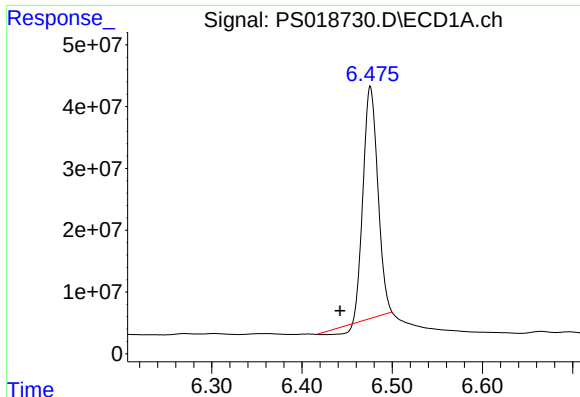

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.476 min
Delta R.T.: 0.034 min
Response: 411198748
Conc: 106.71 ng/ml

Instrument :
ECD_S
ClientSampleId :

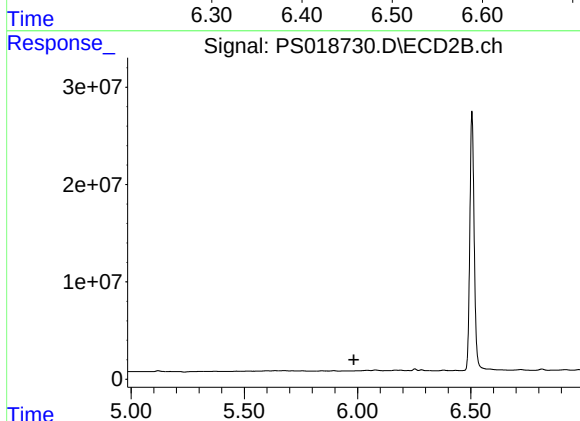


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.984 min
Response: 0
Conc: N.D.

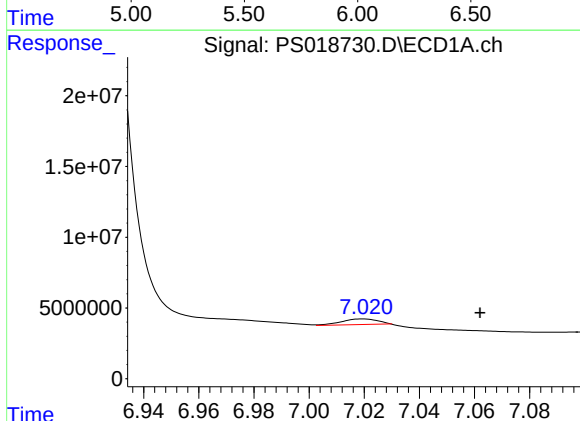


#3 4-Nitrophenol

R.T.: 7.019 min
Delta R.T.: -0.043 min
Response: 3805961
Conc: 2.21 ng/ml

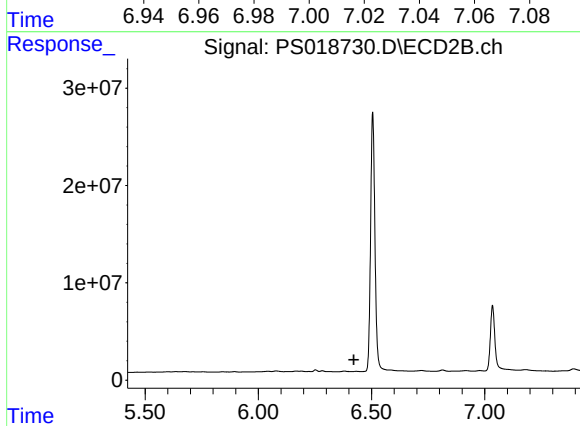

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.422 min
Response: 0
Conc: N.D.

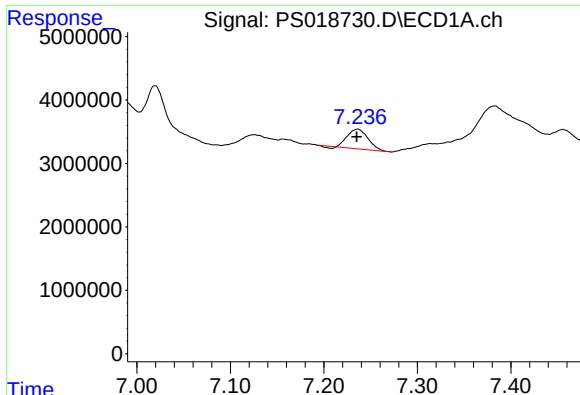

#4 2,4-DCAA


R.T.: 7.236 min
Delta R.T.: 0.001 min
Response: 4688581
Conc: 1.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

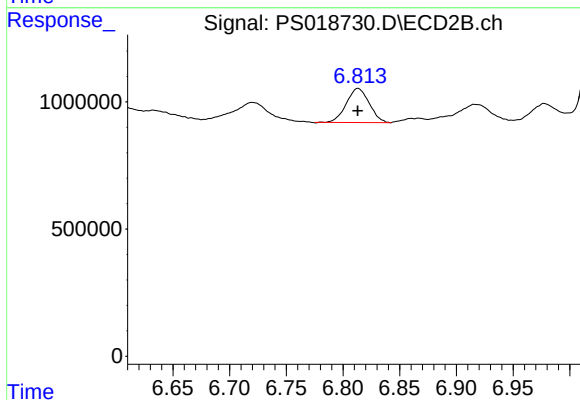


#4 2,4-DCAA

R.T.: 6.813 min
Delta R.T.: 0.000 min
Response: 1891687
Conc: 2.69 ng/ml

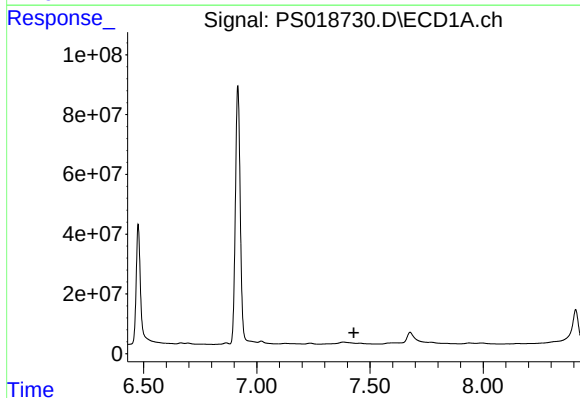


#5 DICAMBA

R.T.: 7.383 min
Delta R.T.: -0.046 min
Response: -1574941
Conc: N.D.

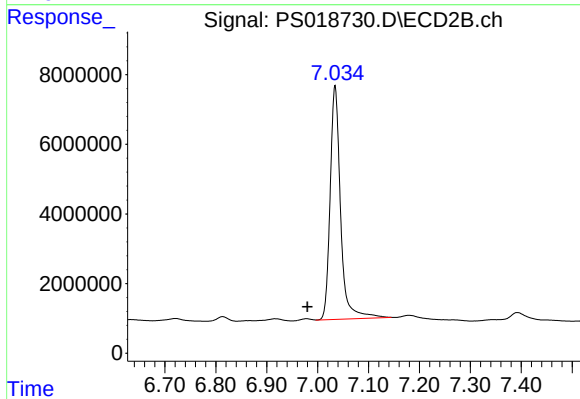

#5 DICAMBA


R.T.: 7.034 min
Delta R.T.: 0.054 min
Response: 95537726
Conc: 32.08 ng/ml

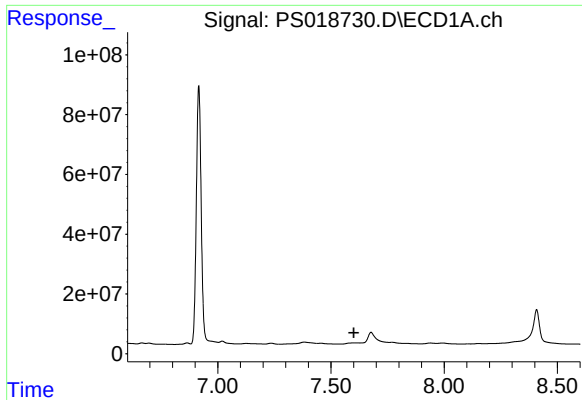

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.601 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

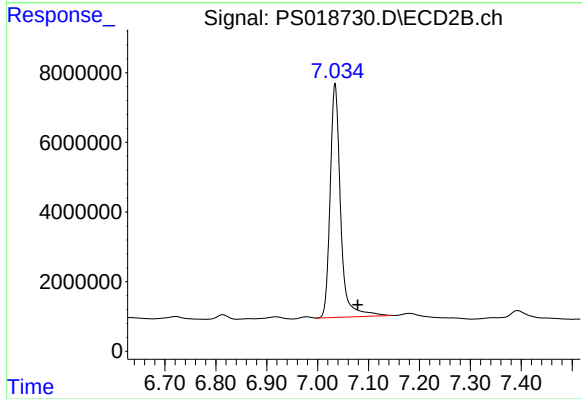


#6 MCP

R.T.: 7.034 min
Delta R.T.: -0.045 min
Response: 95537726
Conc: 39.03 ug/ml

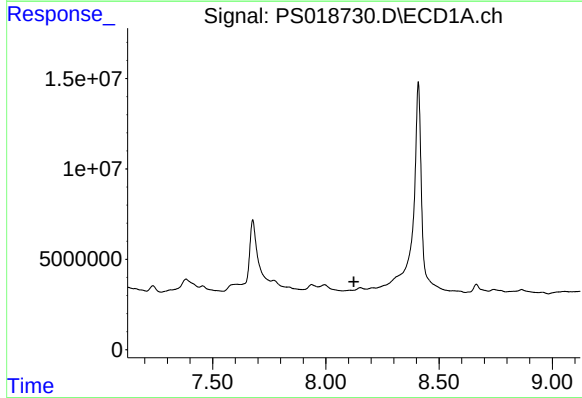


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

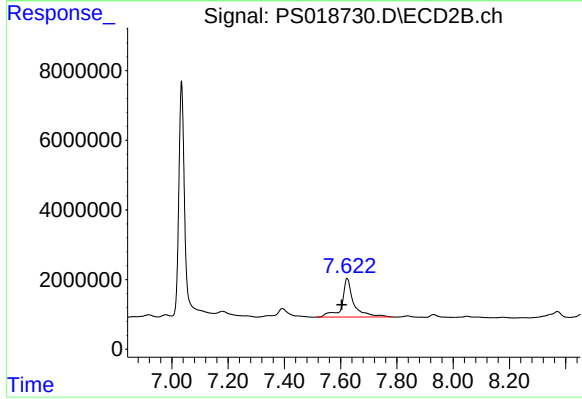

#8 DICHLORPROP


R.T.: 7.623 min
Delta R.T.: 0.019 min
Response: 32327590
Conc: 40.84 ng/ml

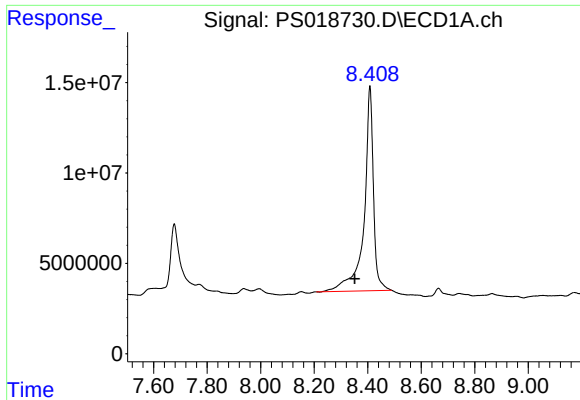

#9 2,4-D


R.T.: 8.408 min
Delta R.T.: 0.056 min
Response: 275237745
Conc: 82.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

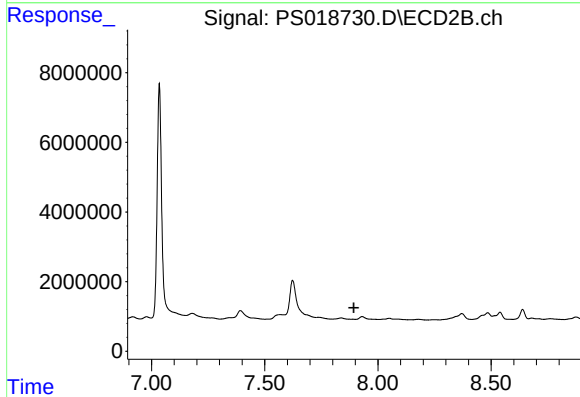


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.894 min
Response: 0
Conc: N.D.

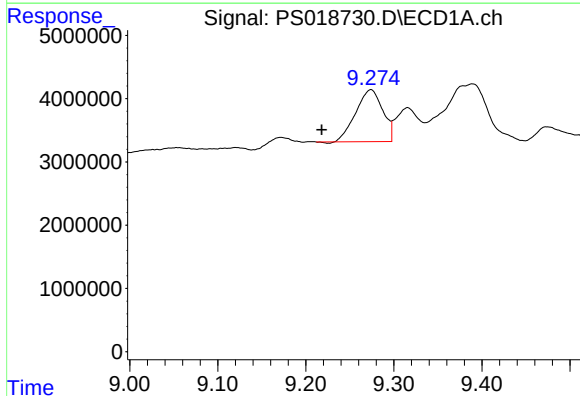


#11 2,4,5-TP (SILVEX)

R.T.: 9.274 min
Delta R.T.: 0.056 min
Response: 17470987
Conc: 1.15 ng/ml

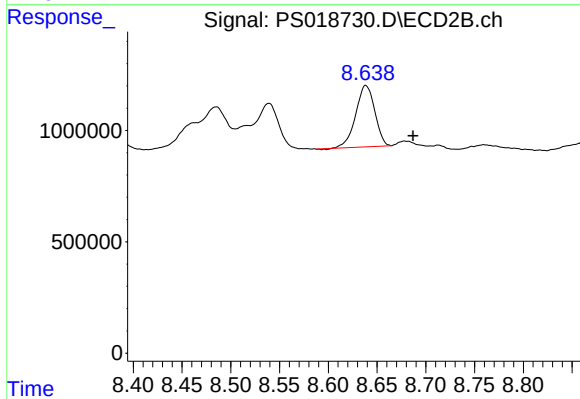

#11 2,4,5-TP (SILVEX)


R.T.: 8.638 min
Delta R.T.: -0.049 min
Response: 3761674
Conc: N.D.

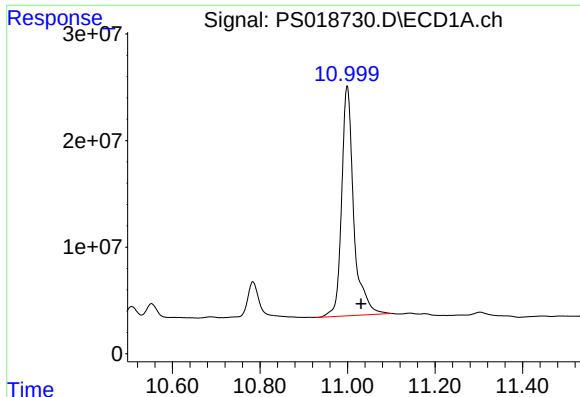

#15 Picloram


R.T.: 10.999 min
Delta R.T.: -0.032 min
Response: 413696250
Conc: 20.13 ng/ml

Instrument :
ECD_S
ClientSampleId :

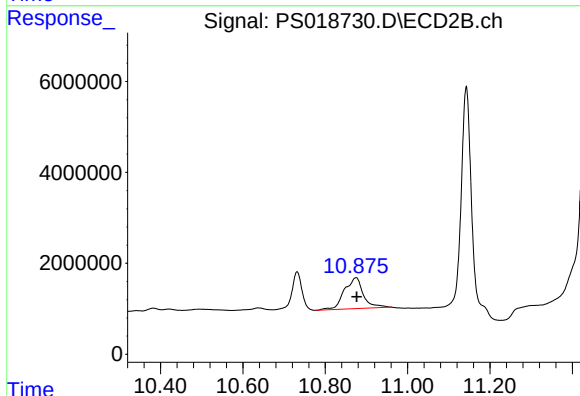


#15 Picloram

R.T.: 10.875 min
Delta R.T.: 0.000 min
Response: 21852456
Conc: 4.11 ng/ml

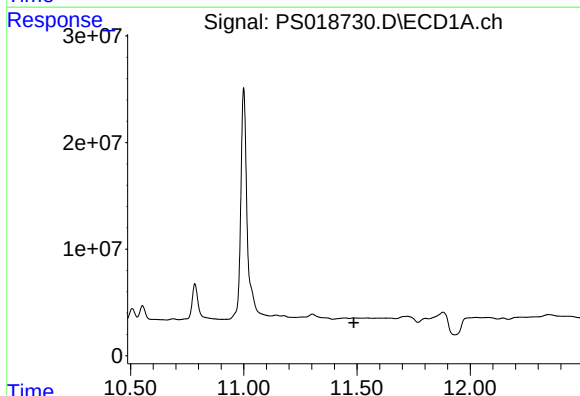

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.486 min
Response: 0
Conc: N.D.

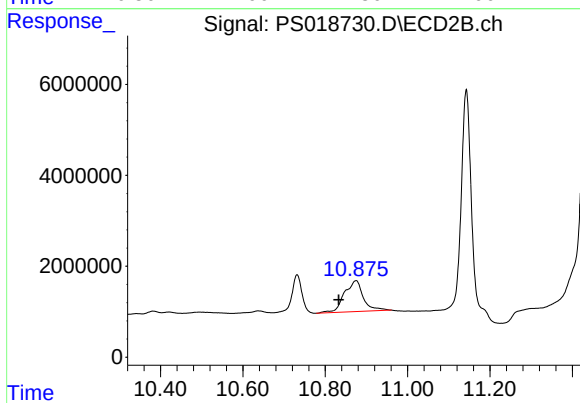

#16 DCPA

R.T.: 10.875 min
Delta R.T.: 0.042 min
Response: 21852456
Conc: 4.16 ng/ml