

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032422\
 Data File : PS018739.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 14:34
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 16:08:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.808	1312.6E6	371.6E6	461.229	528.054
Target Compounds							
2) T	3,5-DICHL...	6.437	0.000	2417235	0	<MDL	N.D. #
3) T	4-Nitroph...	0.000	6.473f	0	1406442	N.D.	3.462
5) T	DICAMBA	7.420	6.975	8995517	2433835	<MDL	<MDL #
8) T	DICHLORPROP	0.000	7.623	0	12758416	N.D.	16.117
9) T	2,4-D	8.347	0.000	3019793	0	<MDL	N.D. #
10) T	Pentachlo...	8.655	8.320	30314924	7226068	<MDL	<MDL #
11) T	2,4,5-TP ...	9.209	8.682	15143791	5499934	<MDL	1.261 #
12) T	2,4,5-T	9.492	9.060	19463866	3746378	1.303	<MDL #
14) T	DINOSEB	11.210	9.895	9976074	2571155	<MDL	<MDL #
15) T	Picloram	11.031	10.879	43606020	12827383	2.121	2.413
16) T	DCPA	11.476	10.827	17884292	5334769	<MDL	1.014 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032422\
Data File : PS018739.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 14:34
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 16:08:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

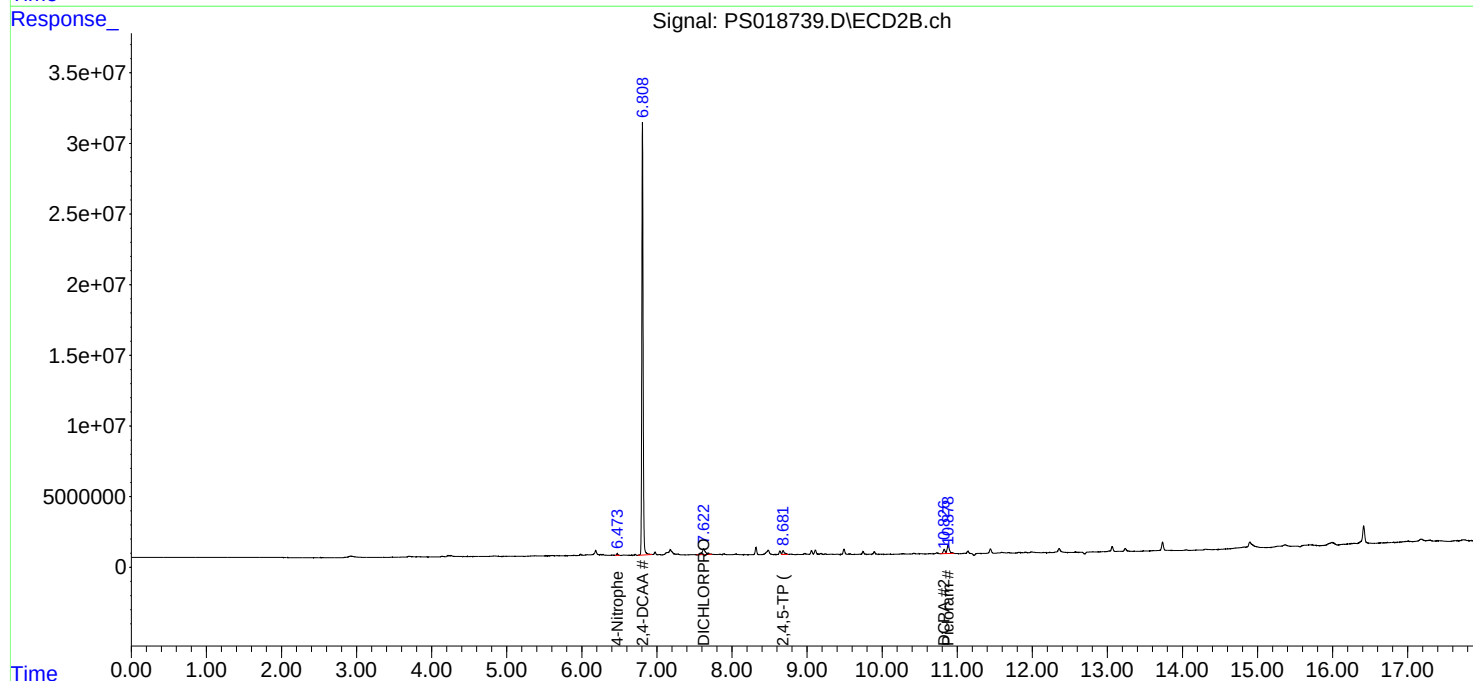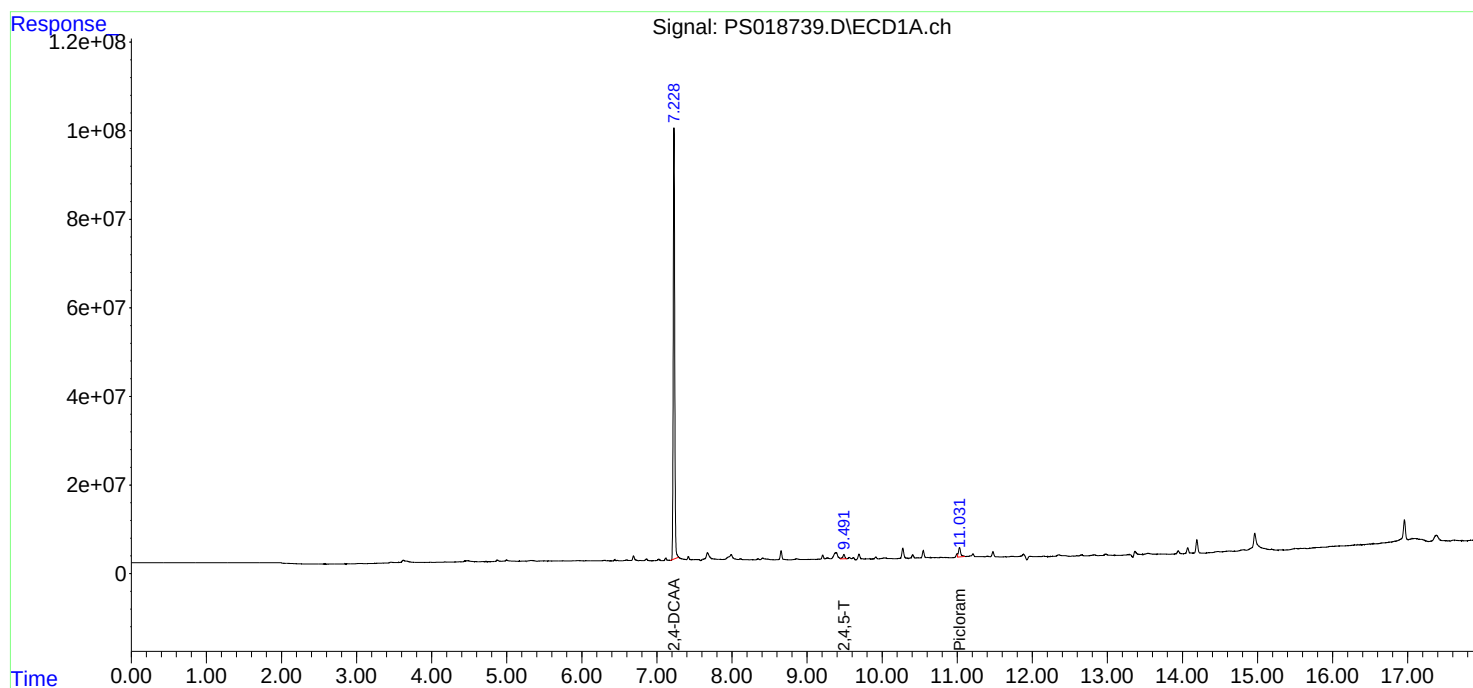


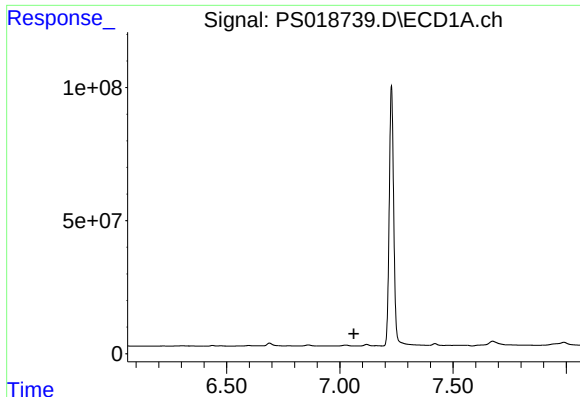

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.062 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

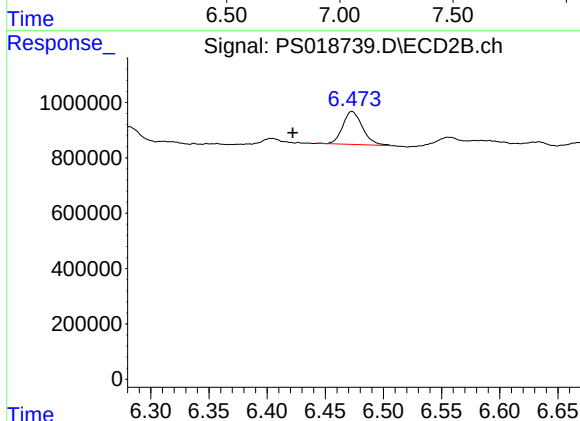


#3 4-Nitrophenol

R.T.: 6.473 min
Delta R.T.: 0.051 min
Response: 1406442
Conc: 3.46 ng/ml

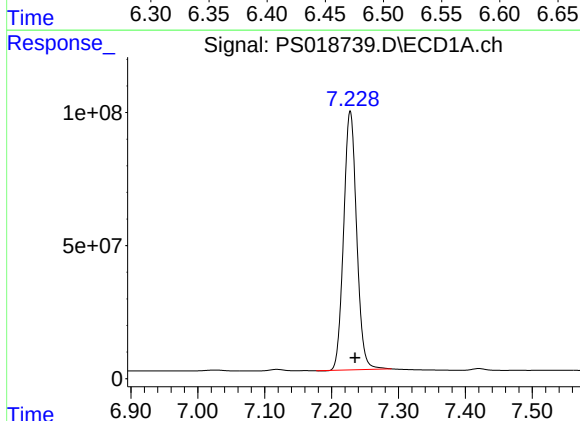


#4 2,4-DCAA

R.T.: 7.228 min
Delta R.T.: -0.007 min
Response: 1312620435
Conc: 461.23 ng/ml

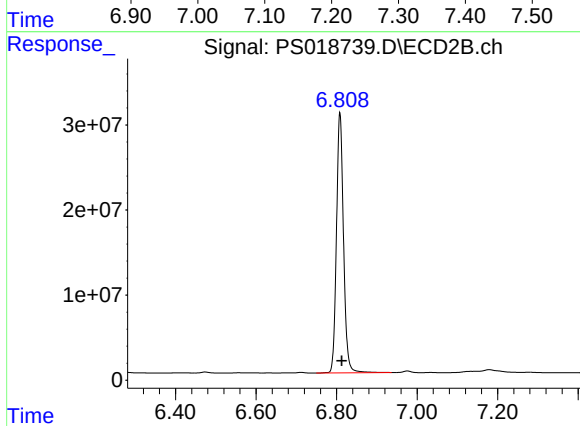

#4 2,4-DCAA


R.T.: 6.808 min
Delta R.T.: -0.005 min
Response: 371567646
Conc: 528.05 ng/ml

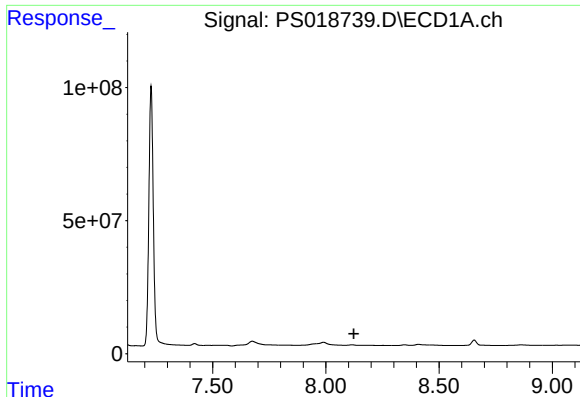

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.124 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

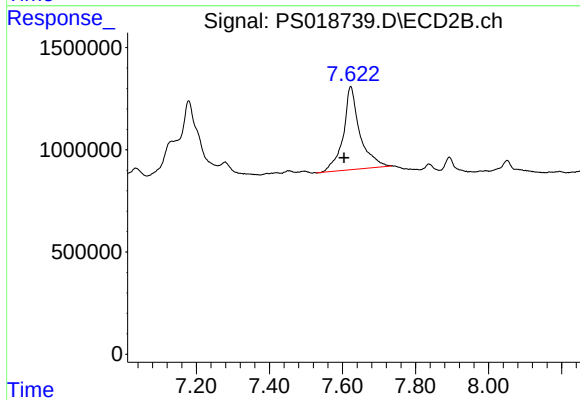


#8 DICHLORPROP

R.T.: 7.623 min
Delta R.T.: 0.019 min
Response: 12758416
Conc: 16.12 ng/ml

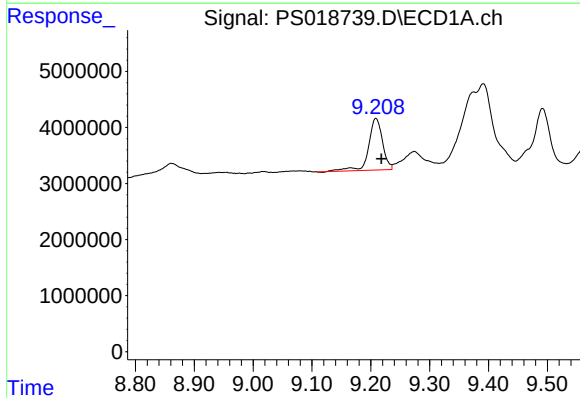


#11 2,4,5-TP (SILVEX)

R.T.: 9.209 min
Delta R.T.: -0.009 min
Response: 15143791
Conc: N.D.

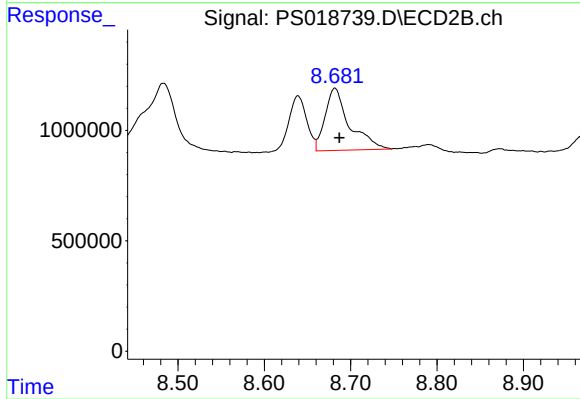

#11 2,4,5-TP (SILVEX)


R.T.: 8.682 min
Delta R.T.: -0.005 min
Response: 5499934
Conc: 1.26 ng/ml

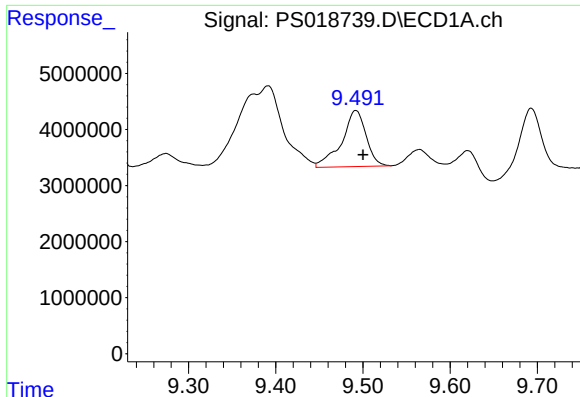

#12 2,4,5-T


R.T.: 9.492 min
Delta R.T.: -0.008 min
Response: 19463866
Conc: 1.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

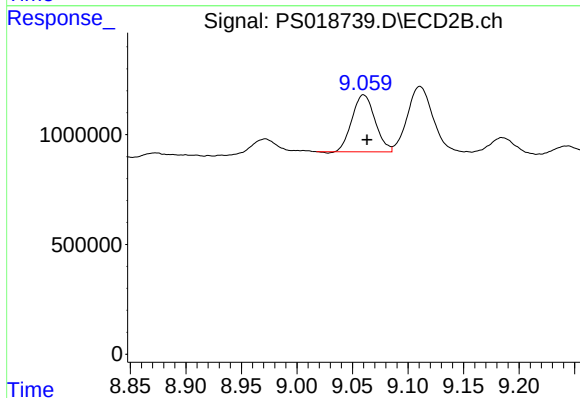


#12 2,4,5-T

R.T.: 9.060 min
Delta R.T.: -0.003 min
Response: 3746378
Conc: N.D.

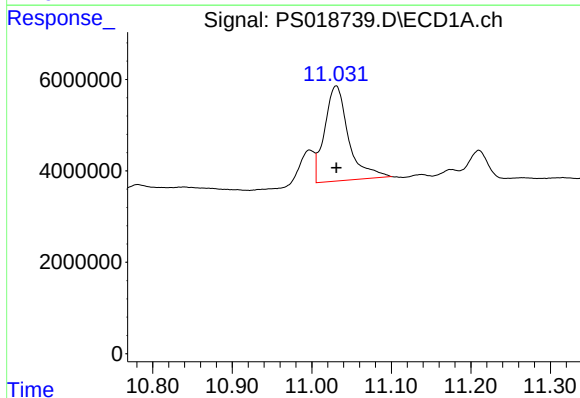


#15 Picloram

R.T.: 11.031 min
Delta R.T.: 0.000 min
Response: 43606020
Conc: 2.12 ng/ml

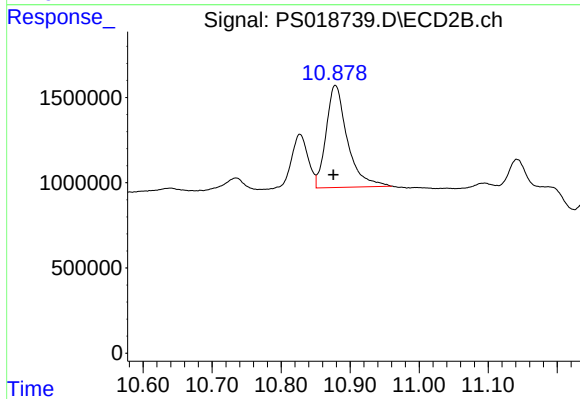

#15 Picloram


R.T.: 10.879 min
Delta R.T.: 0.003 min
Response: 12827383
Conc: 2.41 ng/ml

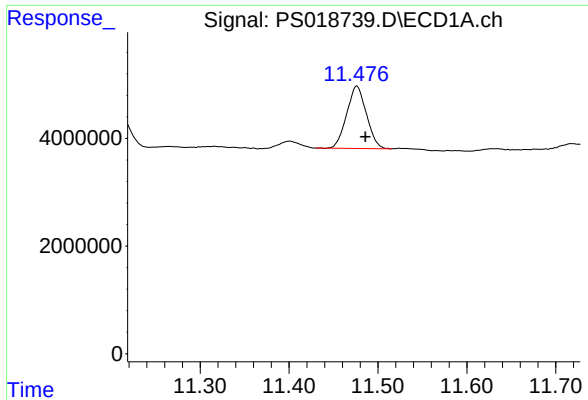

#16 DCPA

R.T.: 11.476 min
Delta R.T.: -0.010 min
Response: 17884292
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

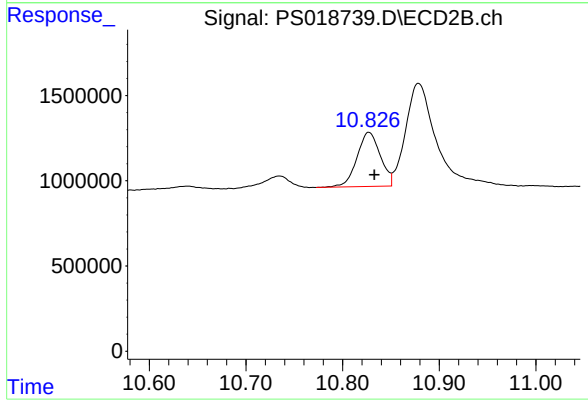

#16 DCPA

R.T.: 10.827 min
Delta R.T.: -0.006 min
Response: 5334769
Conc: 1.01 ng/ml