

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032422\
 Data File : PS018751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2022 20:37
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 01:24:15 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.228	6.810	1311.2E6	373.7E6	460.745	531.071
Target Compounds							
5) T	DICAMBA	7.420	0.000	4500131	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.624	0	8650234	N.D.	10.927
9) T	2,4-D	8.411f	0.000	12305871	0	3.673	N.D. #
10) T	Pentachlo...	8.654	8.321	5238651	1465342	<MDL	<MDL #
11) T	2,4,5-TP ...	9.210	8.640f	3469507	8868317	<MDL	2.033 #
12) T	2,4,5-T	9.493	9.062	9919910	1670962	<MDL	<MDL #
14) T	DINOSEB	11.176f	0.000	5303152	0	<MDL	N.D. #
15) T	Picloram	11.034	10.881	34009919	8966894	1.655	1.687
16) T	DCPA	11.477	10.827	17057537	3408246	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032422\
Data File : PS018751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2022 20:37
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 01:24:15 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

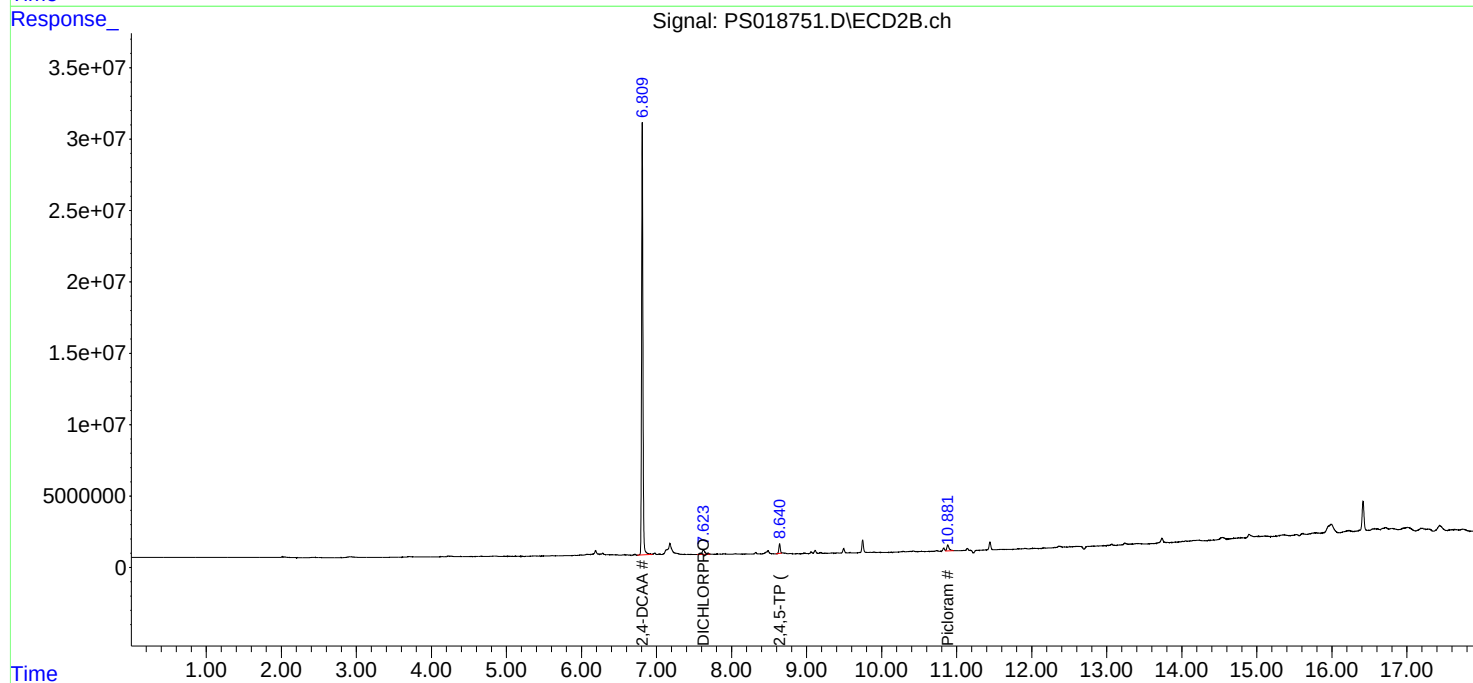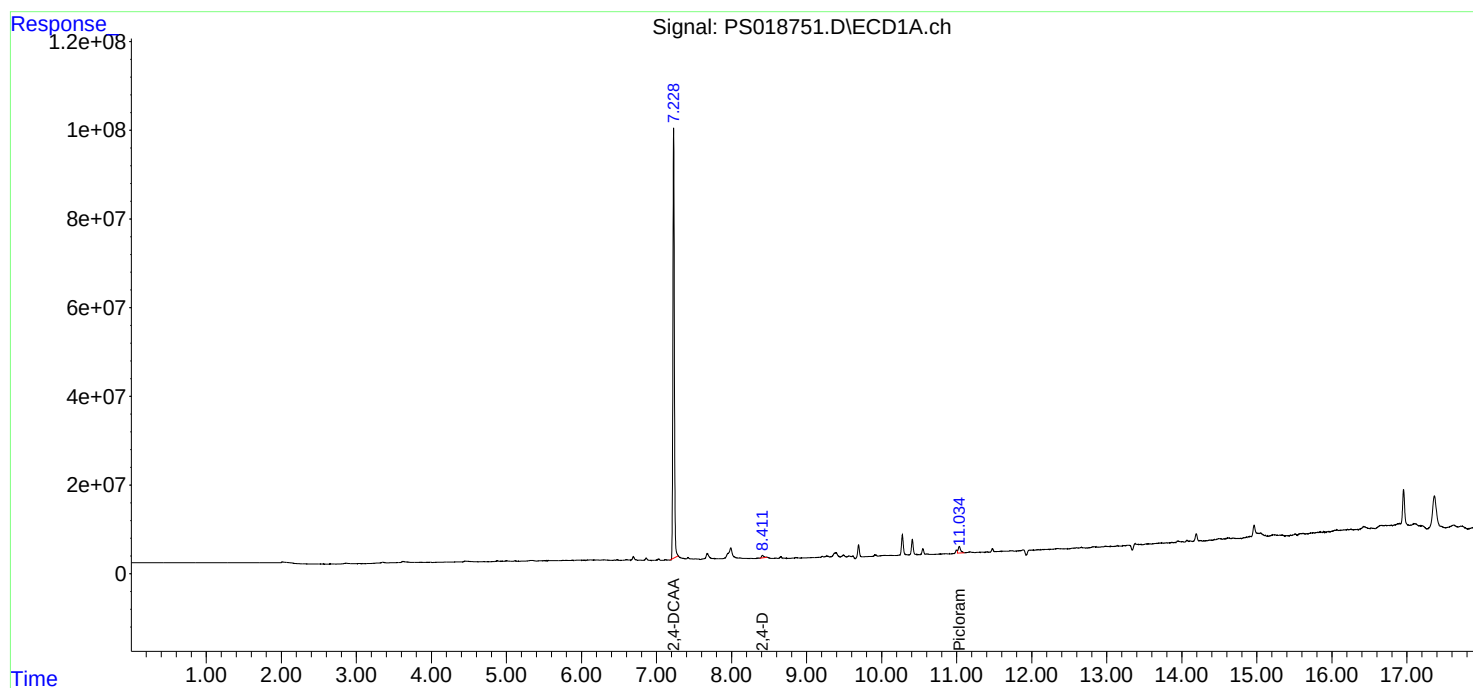


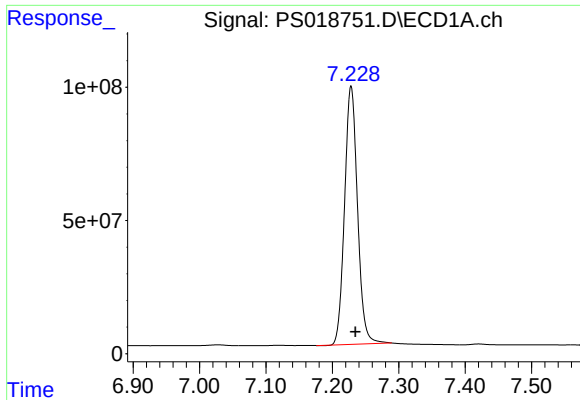

#4 2,4-DCAA


R.T.: 7.228 min
Delta R.T.: -0.007 min
Response: 1311240429
Conc: 460.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

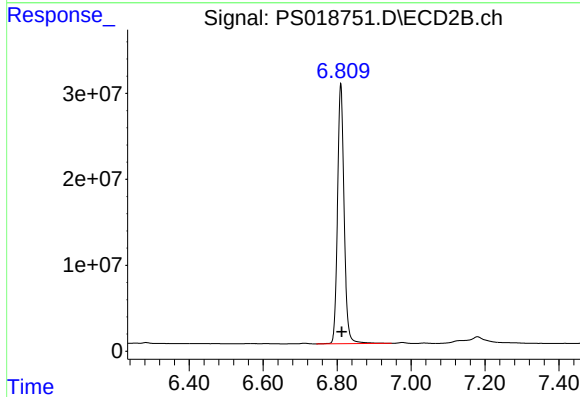


#4 2,4-DCAA

R.T.: 6.810 min
Delta R.T.: -0.003 min
Response: 373690670
Conc: 531.07 ng/ml

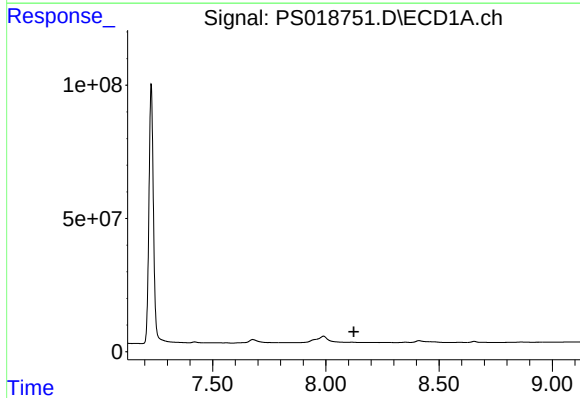


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.124 min
Response: 0
Conc: N.D.

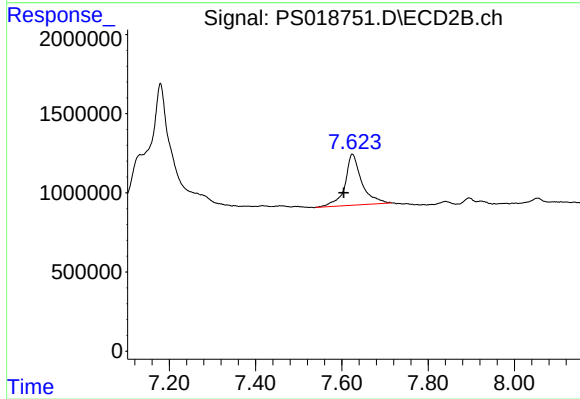

#8 DICHLORPROP


R.T.: 7.624 min
Delta R.T.: 0.020 min
Response: 8650234
Conc: 10.93 ng/ml

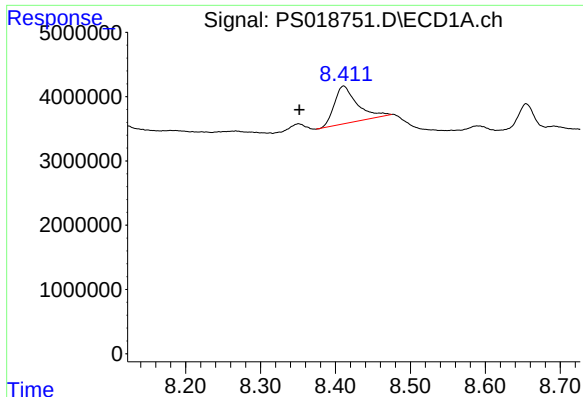

#9 2,4-D


R.T.: 8.411 min
Delta R.T.: 0.059 min
Response: 12305871
Conc: 3.67 ng/ml

Instrument :
ECD_S
ClientSampleId :

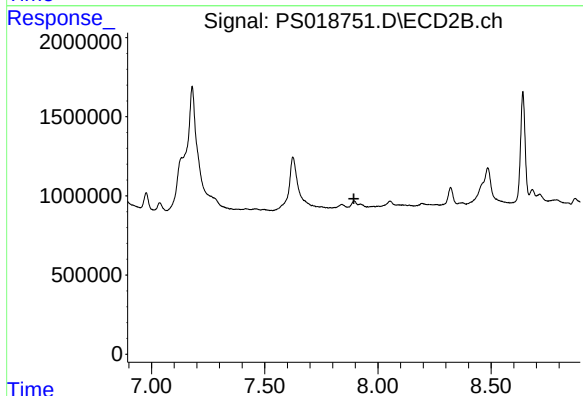


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.894 min
Response: 0
Conc: N.D.

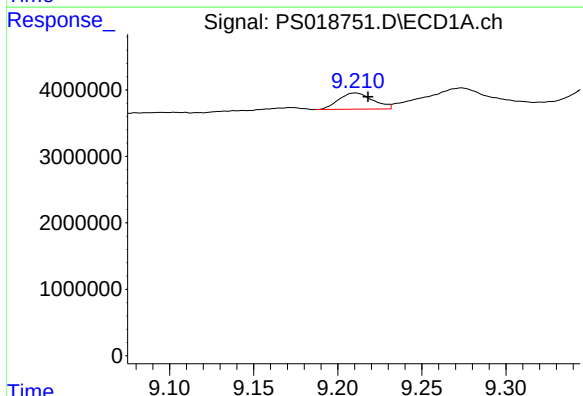


#11 2,4,5-TP (SILVEX)

R.T.: 9.210 min
Delta R.T.: -0.008 min
Response: 3469507
Conc: N.D.

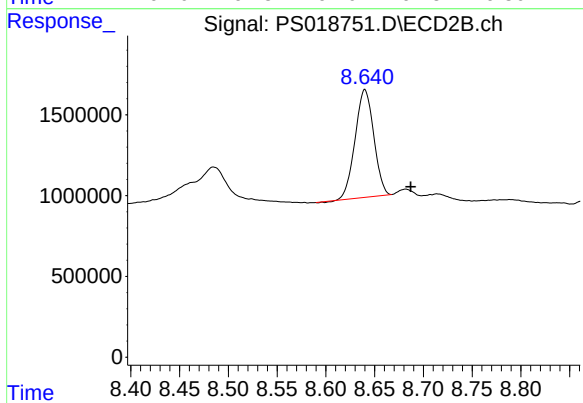

#11 2,4,5-TP (SILVEX)


R.T.: 8.640 min
Delta R.T.: -0.047 min
Response: 8868317
Conc: 2.03 ng/ml

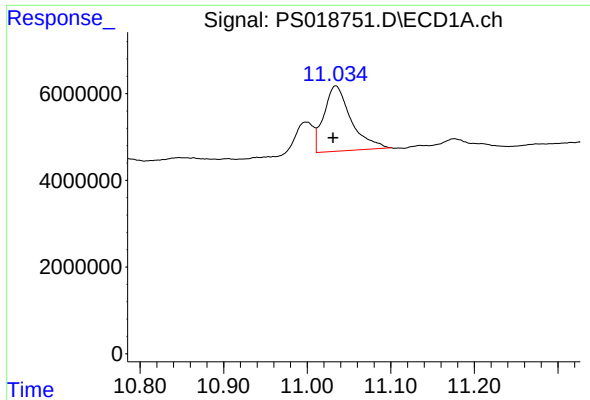

#15 Picloram

R.T.: 11.034 min
Delta R.T.: 0.003 min
Response: 34009919
Conc: 1.65 ng/ml

Instrument :
ECD_S
ClientSampleId :

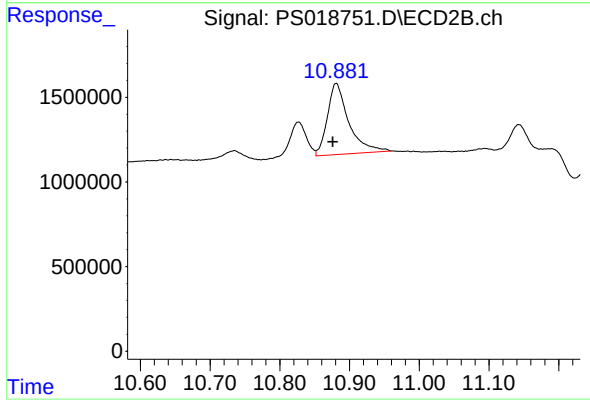

#15 Picloram

R.T.: 10.881 min
Delta R.T.: 0.005 min
Response: 8966894
Conc: 1.69 ng/ml