

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032422\
 Data File : PS018756.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2022 00:36
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 01:25:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.809	1346.7E6	386.4E6	473.213	549.127
Target Compounds							
2) T	3,5-DICHL...	6.474	0.000	3739339	0	<MDL	N.D. #
5) T	DICAMBA	7.474f	7.036f	14030210	1108772	1.286	<MDL #
6) T	MCP	0.000	7.036f	0	1108772	N.D.	<MDL
8) T	DICHLORPROP	8.103	7.620	3366814	63060373	1.222	79.661 #
9) T	2,4-D	8.408f	0.000	6945668	0	2.073	N.D. #
11) T	2,4,5-TP ...	9.271f	8.709	30295511	2963133	1.992	<MDL #
12) T	2,4,5-T	9.467	9.111f	7175148	1887072	<MDL	<MDL #
14) T	DINOSEB	11.262f	0.000	29449362	0	2.754	N.D. #
15) T	Picloram	11.029	10.879	20195824	10549543	<MDL	1.984 #
16) T	DCPA	0.000	10.828	0	1822529	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032422\
Data File : PS018756.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2022 00:36
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 01:25:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

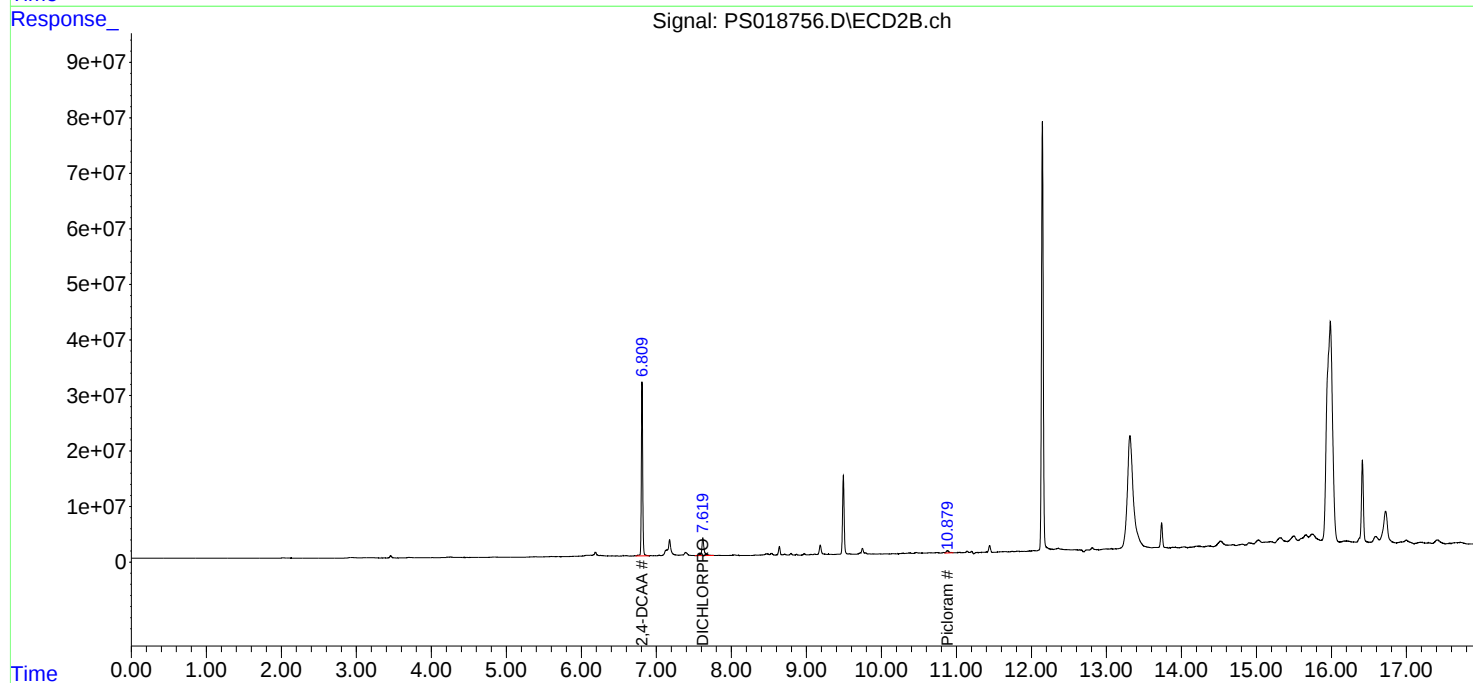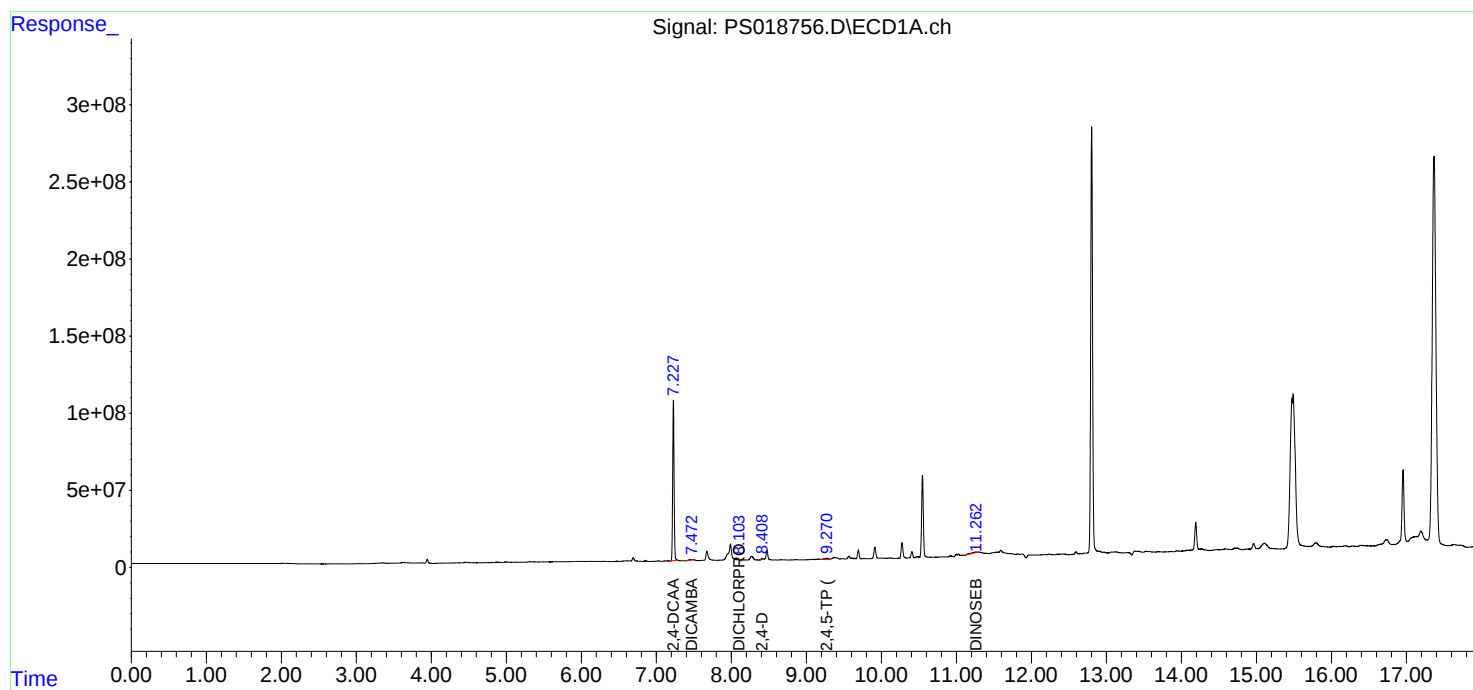


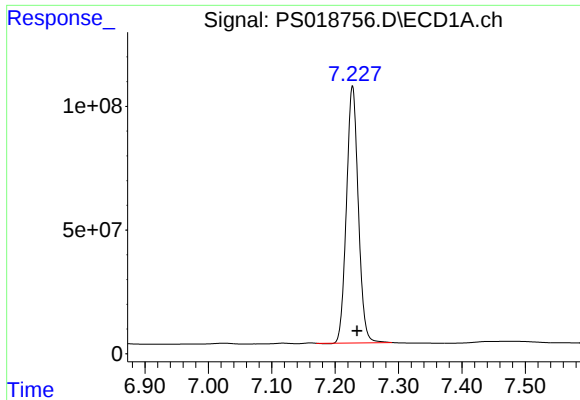

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: -0.008 min
Response: 1346723967
Conc: 473.21 ng/ml

Instrument :
ECD_S
ClientSampleId :

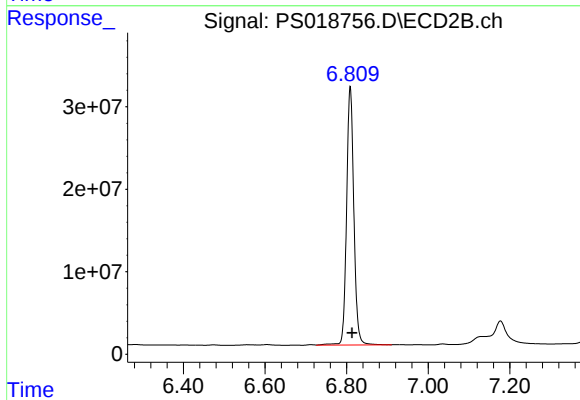


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.004 min
Response: 386396018
Conc: 549.13 ng/ml

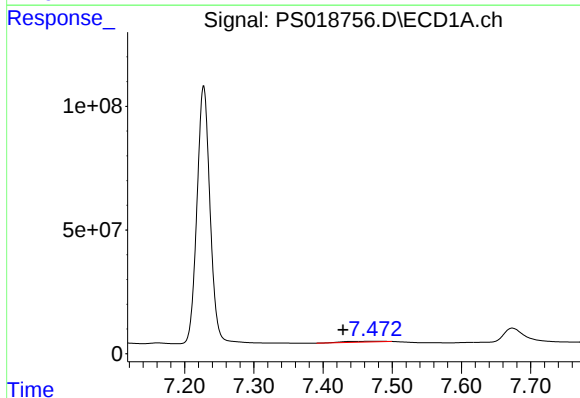


#5 DICAMBA

R.T.: 7.474 min
Delta R.T.: 0.045 min
Response: 14030210
Conc: 1.29 ng/ml

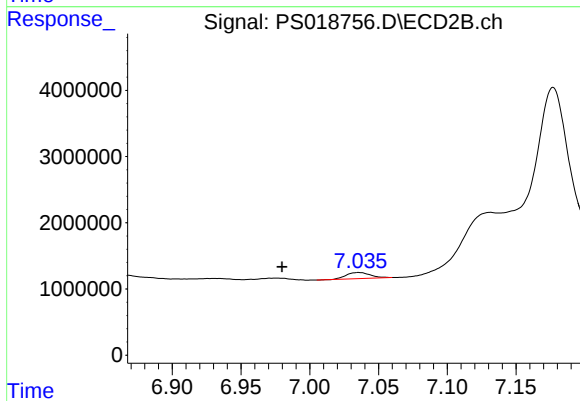

#5 DICAMBA


R.T.: 7.036 min
Delta R.T.: 0.056 min
Response: 1108772
Conc: N.D.

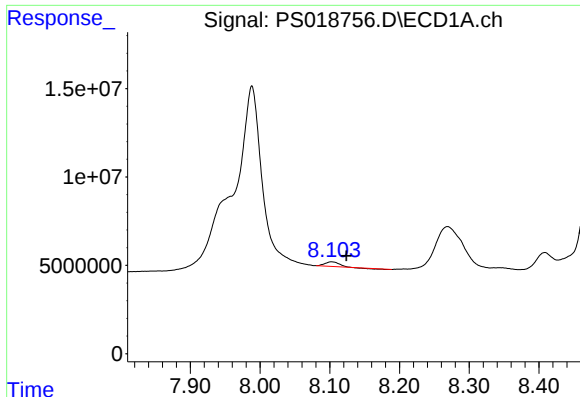

#8 DICHLORPROP


R.T.: 8.103 min
Delta R.T.: -0.021 min
Response: 3366814
Conc: 1.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

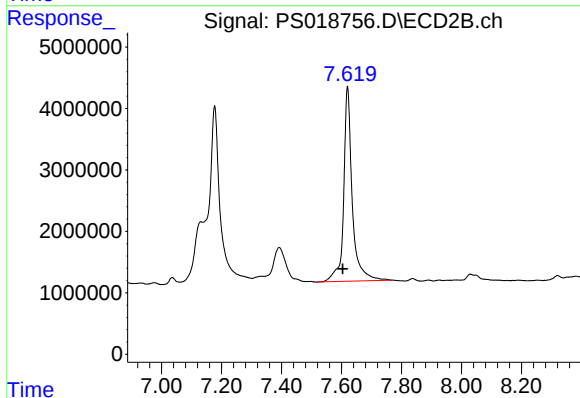


#8 DICHLORPROP

R.T.: 7.620 min
Delta R.T.: 0.016 min
Response: 63060373
Conc: 79.66 ng/ml

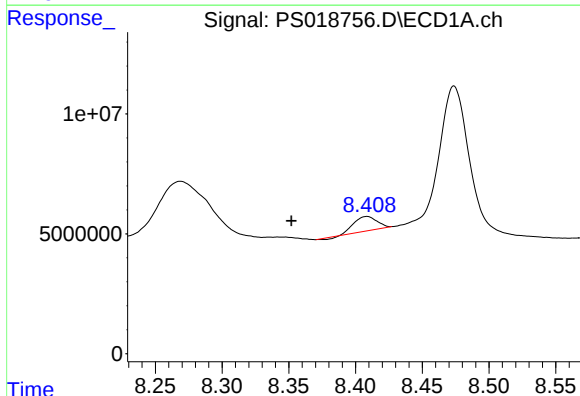


#9 2,4-D

R.T.: 8.408 min
Delta R.T.: 0.056 min
Response: 6945668
Conc: 2.07 ng/ml

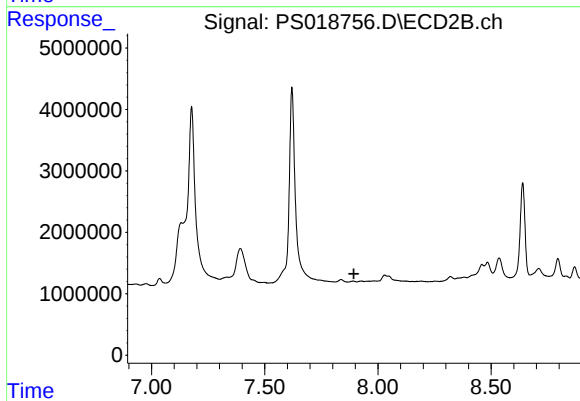

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.894 min
Response: 0
Conc: N.D.

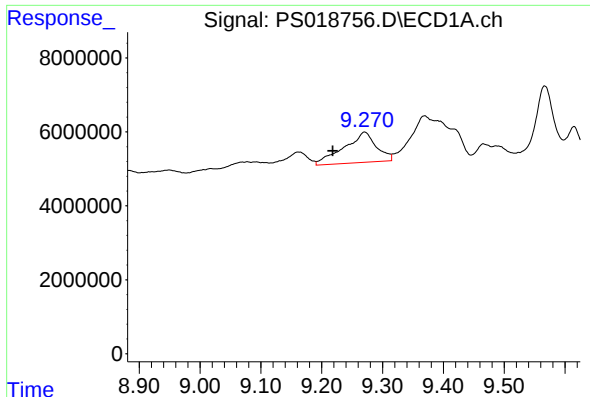

#11 2,4,5-TP (SILVEX)


R.T.: 9.271 min
Delta R.T.: 0.053 min
Response: 30295511
Conc: 1.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

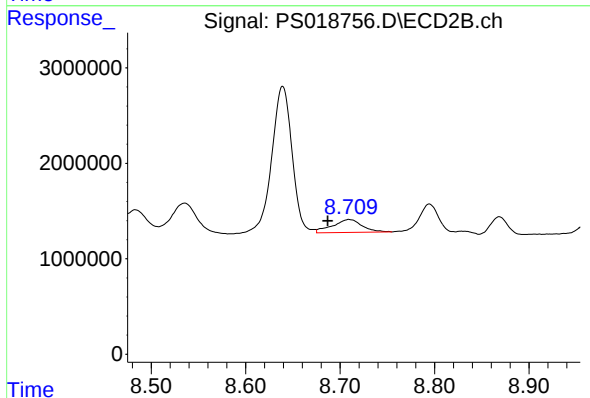


#11 2,4,5-TP (SILVEX)

R.T.: 8.709 min
Delta R.T.: 0.022 min
Response: 2963133
Conc: N.D.

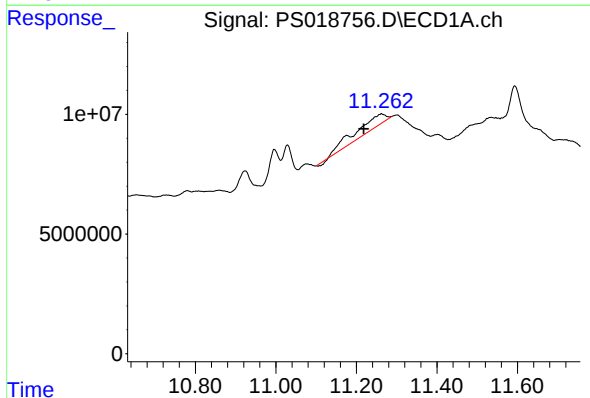


#14 DINOSEB

R.T.: 11.262 min
Delta R.T.: 0.044 min
Response: 29449362
Conc: 2.75 ng/ml

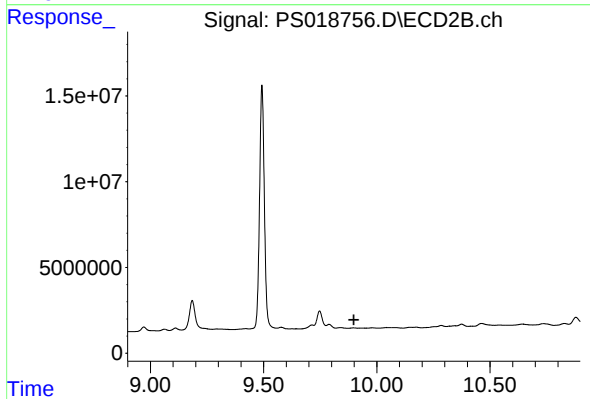

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.899 min
Response: 0
Conc: N.D.

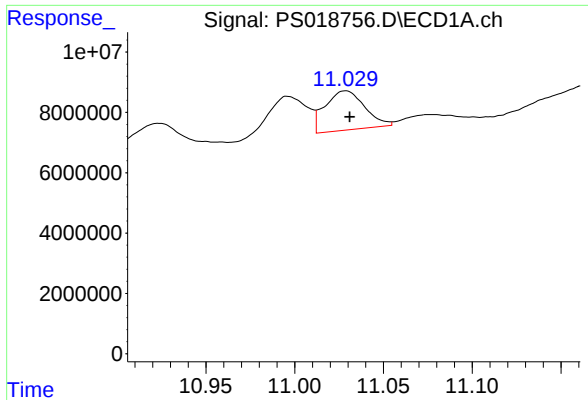

#15 Picloram

R.T.: 11.029 min
Delta R.T.: -0.002 min
Response: 20195824
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

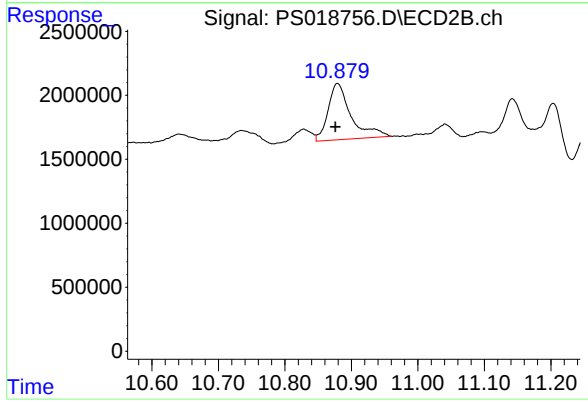

#15 Picloram

R.T.: 10.879 min
Delta R.T.: 0.003 min
Response: 10549543
Conc: 1.98 ng/ml