

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032423\
 Data File : PS022502.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2023 09:35
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 12:29:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.297	6.719	1269.7E6	1184.1E6	519.446	574.912
Target Compounds							
1) T	Dalapon	2.379	2.518	1340692	462170	<MDL	<MDL #
3) T	4-Nitroph...	6.149	0.000	4740941	0	3.460	N.D. #
5) T	DICAMBA	0.000	6.879	0	8761345	N.D.	<MDL
6) T	MCP	6.618	7.019	-1478080	3759592	N.D.	<MDL
8) T	DICHLORPROP	7.036	7.519	1363493	26895260	<MDL	10.801 #
9) T	2,4-D	0.000	7.758	0	2550643	N.D.	<MDL
10) T	Pentachlo...	7.445	8.209	11016748	10666035	<MDL	<MDL #
11) T	2,4,5-TP ...	7.980	8.574	6848269	2714088	<MDL	<MDL #
12) T	2,4,5-T	8.191	8.967	20135524	6578884	1.226	<MDL #
13) T	2,4-DB	8.714	0.000	1786881	0	<MDL	N.D. #
14) T	DINOSEB	0.000	9.775	0	2573790	N.D.	<MDL
15) T	Picloram	0.000	10.777	0	37478748	N.D.	1.868
16) T	DCPA	10.041	10.699	6040182	4394134	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032423\
Data File : PS022502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2023 09:35
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 12:29:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

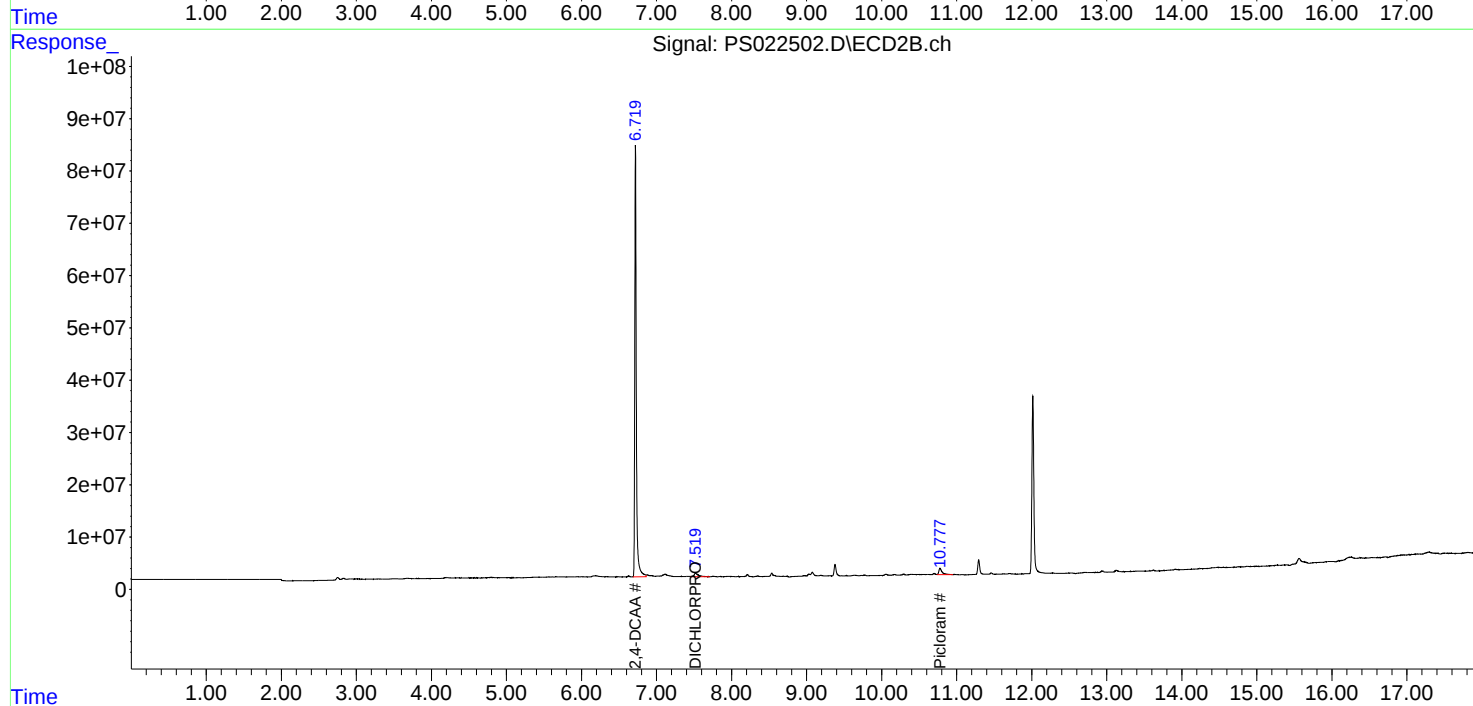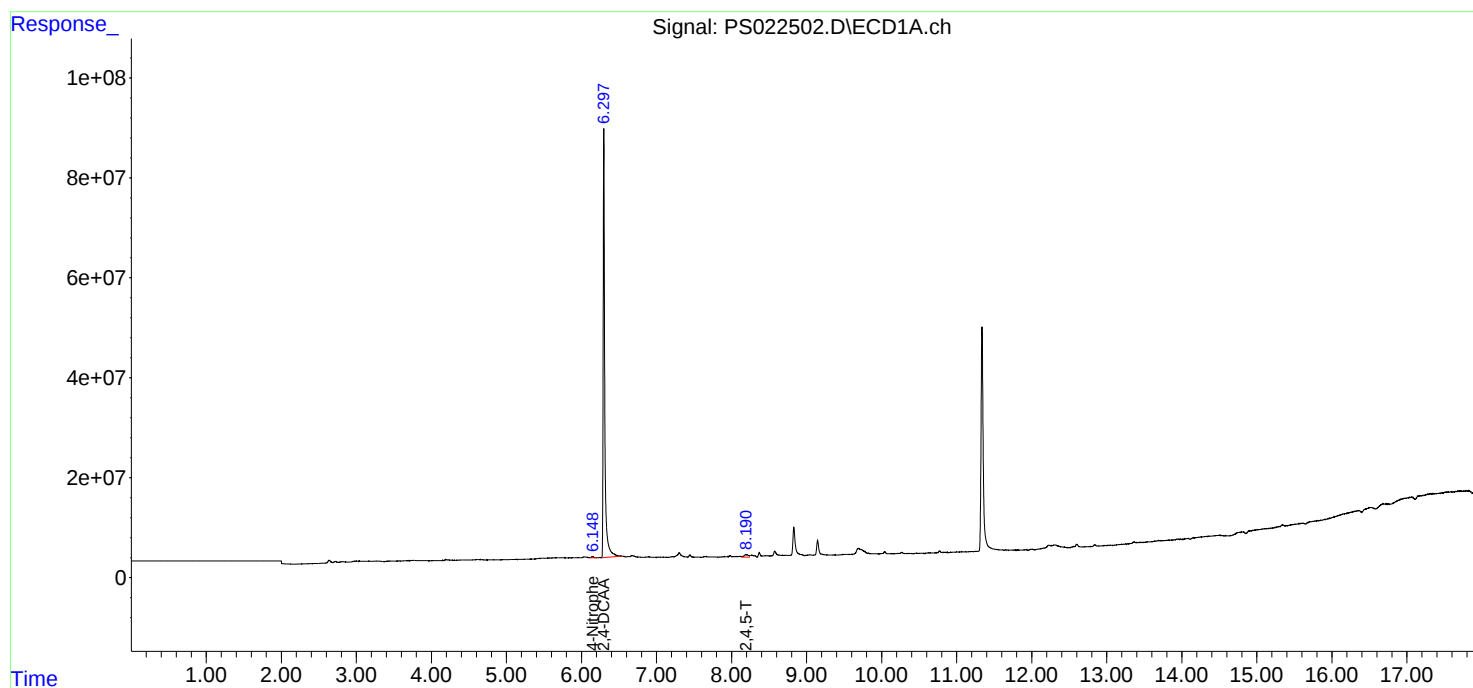


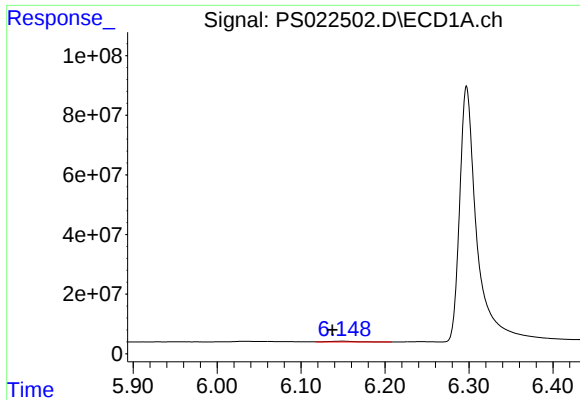

#3 4-Nitrophenol


R.T.: 6.149 min
Delta R.T.: 0.012 min
Response: 4740941
Conc: 3.46 ng/ml

Instrument :
ECD_S
ClientSampleId :

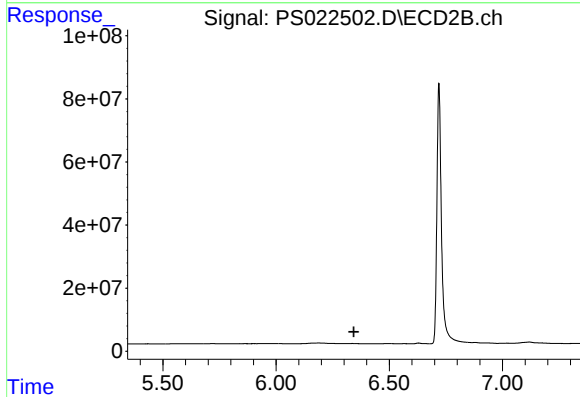


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

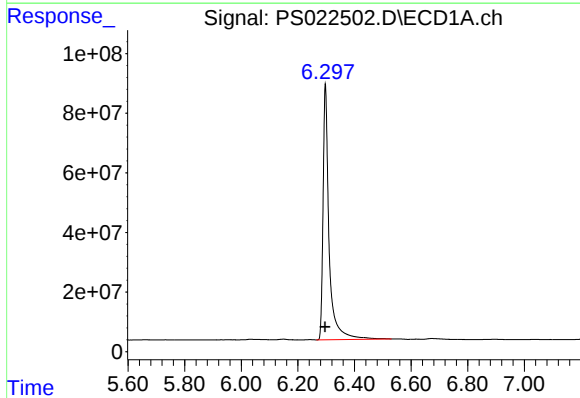


#4 2,4-DCAA

R.T.: 6.297 min
Delta R.T.: 0.001 min
Response: 1269724799
Conc: 519.45 ng/ml

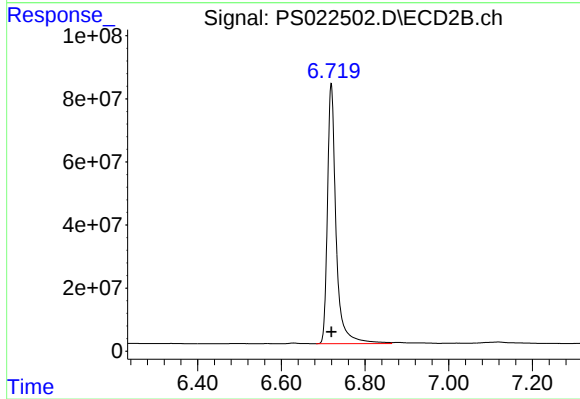

#4 2,4-DCAA


R.T.: 6.719 min
Delta R.T.: 0.000 min
Response: 1184137601
Conc: 574.91 ng/ml

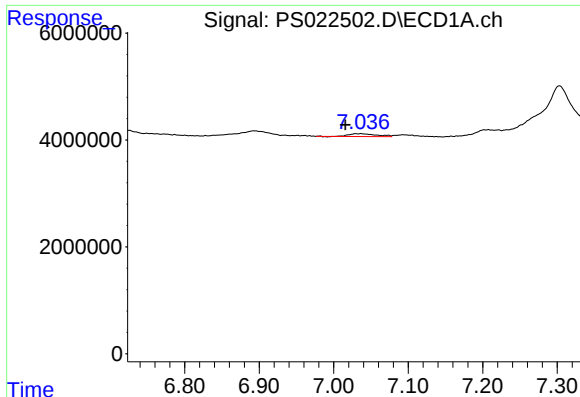

#8 DICHLORPROP


R.T.: 7.036 min
Delta R.T.: 0.020 min
Response: 1363493
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

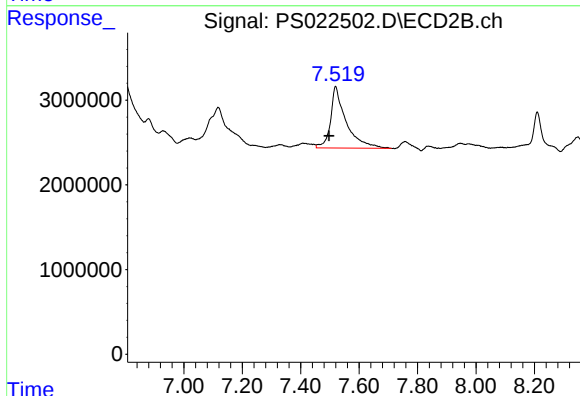


#8 DICHLORPROP

R.T.: 7.519 min
Delta R.T.: 0.022 min
Response: 26895260
Conc: 10.80 ng/ml

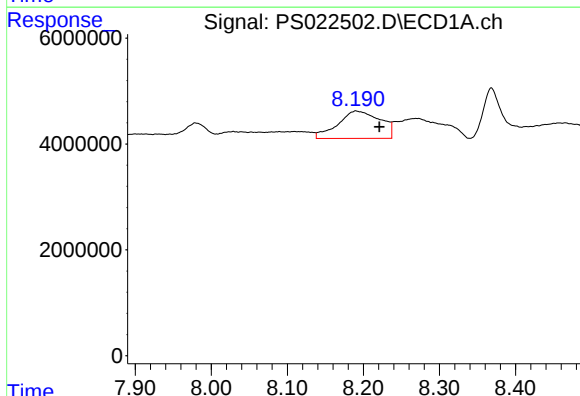


#12 2,4,5-T

R.T.: 8.191 min
Delta R.T.: -0.030 min
Response: 20135524
Conc: 1.23 ng/ml

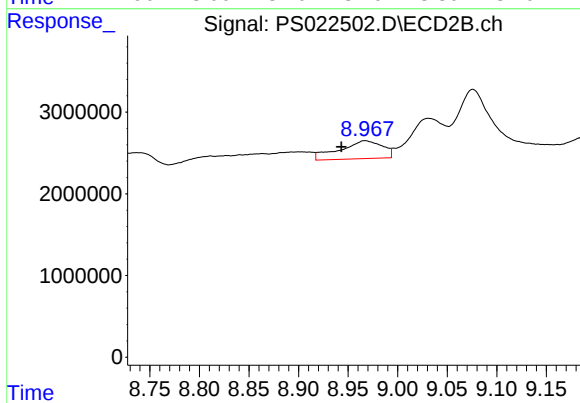

#12 2,4,5-T


R.T.: 8.967 min
Delta R.T.: 0.024 min
Response: 6578884
Conc: N.D.

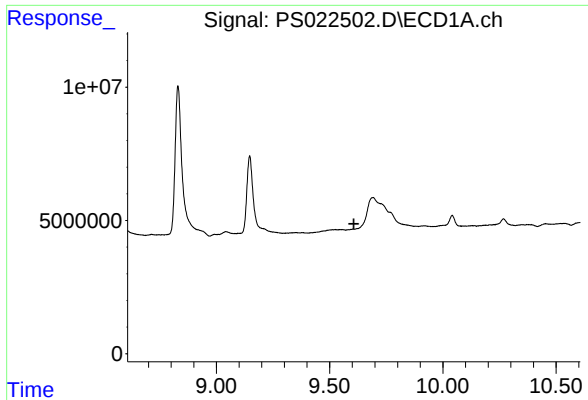

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.607 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

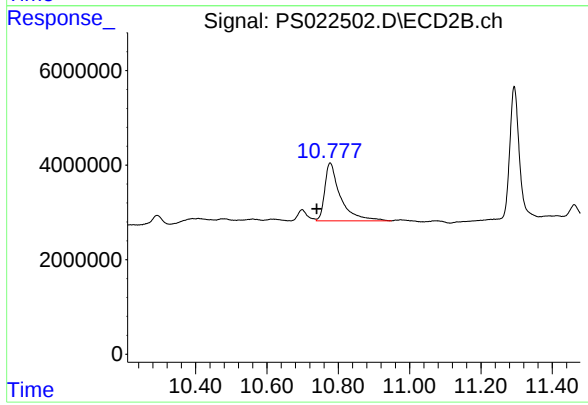

#15 Picloram

R.T.: 10.777 min
Delta R.T.: 0.038 min
Response: 37478748
Conc: 1.87 ng/ml