

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032423\
 Data File : PS022508.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2023 13:10
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 21:40:32 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 20 15:46:44 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.298	6.719	1264.1E6	1192.3E6	517.162	578.896
Target Compounds							
1) T	Dalapon	2.431	2.510	1158791	-362191	<MDL	N.D. #
3) T	4-Nitroph...	6.149	0.000	4847069	0	3.538	N.D. #
5) T	DICAMBA	6.435	6.880	16100348	9588375	1.566	<MDL #
6) T	MCP	6.630	7.024f	-2563454	4120205	N.D.	<MDL
8) T	DICHLORPROP	7.034	7.518	1993711	30113018	<MDL	12.093 #
9) T	2,4-D	7.206	7.757	14647428	2157956	4.467	<MDL #
10) T	Pentachlo...	7.446	8.210	12495803	15031331	<MDL	<MDL #
11) T	2,4,5-TP ...	7.981	8.575	11678268	4820636	<MDL	<MDL #
12) T	2,4,5-T	8.188	8.967	53873051	10222148	3.281	<MDL #
14) T	DINOSEB	0.000	9.774	0	4189723	N.D.	<MDL
15) T	Picloram	0.000	10.772	0	141.2E6	N.D.	7.036
16) T	DCPA	10.040	10.697	10078669	6346524	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032423\
Data File : PS022508.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2023 13:10
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 21:40:32 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032023.M
Quant Title : 8080.M
QLast Update : Mon Mar 20 15:46:44 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

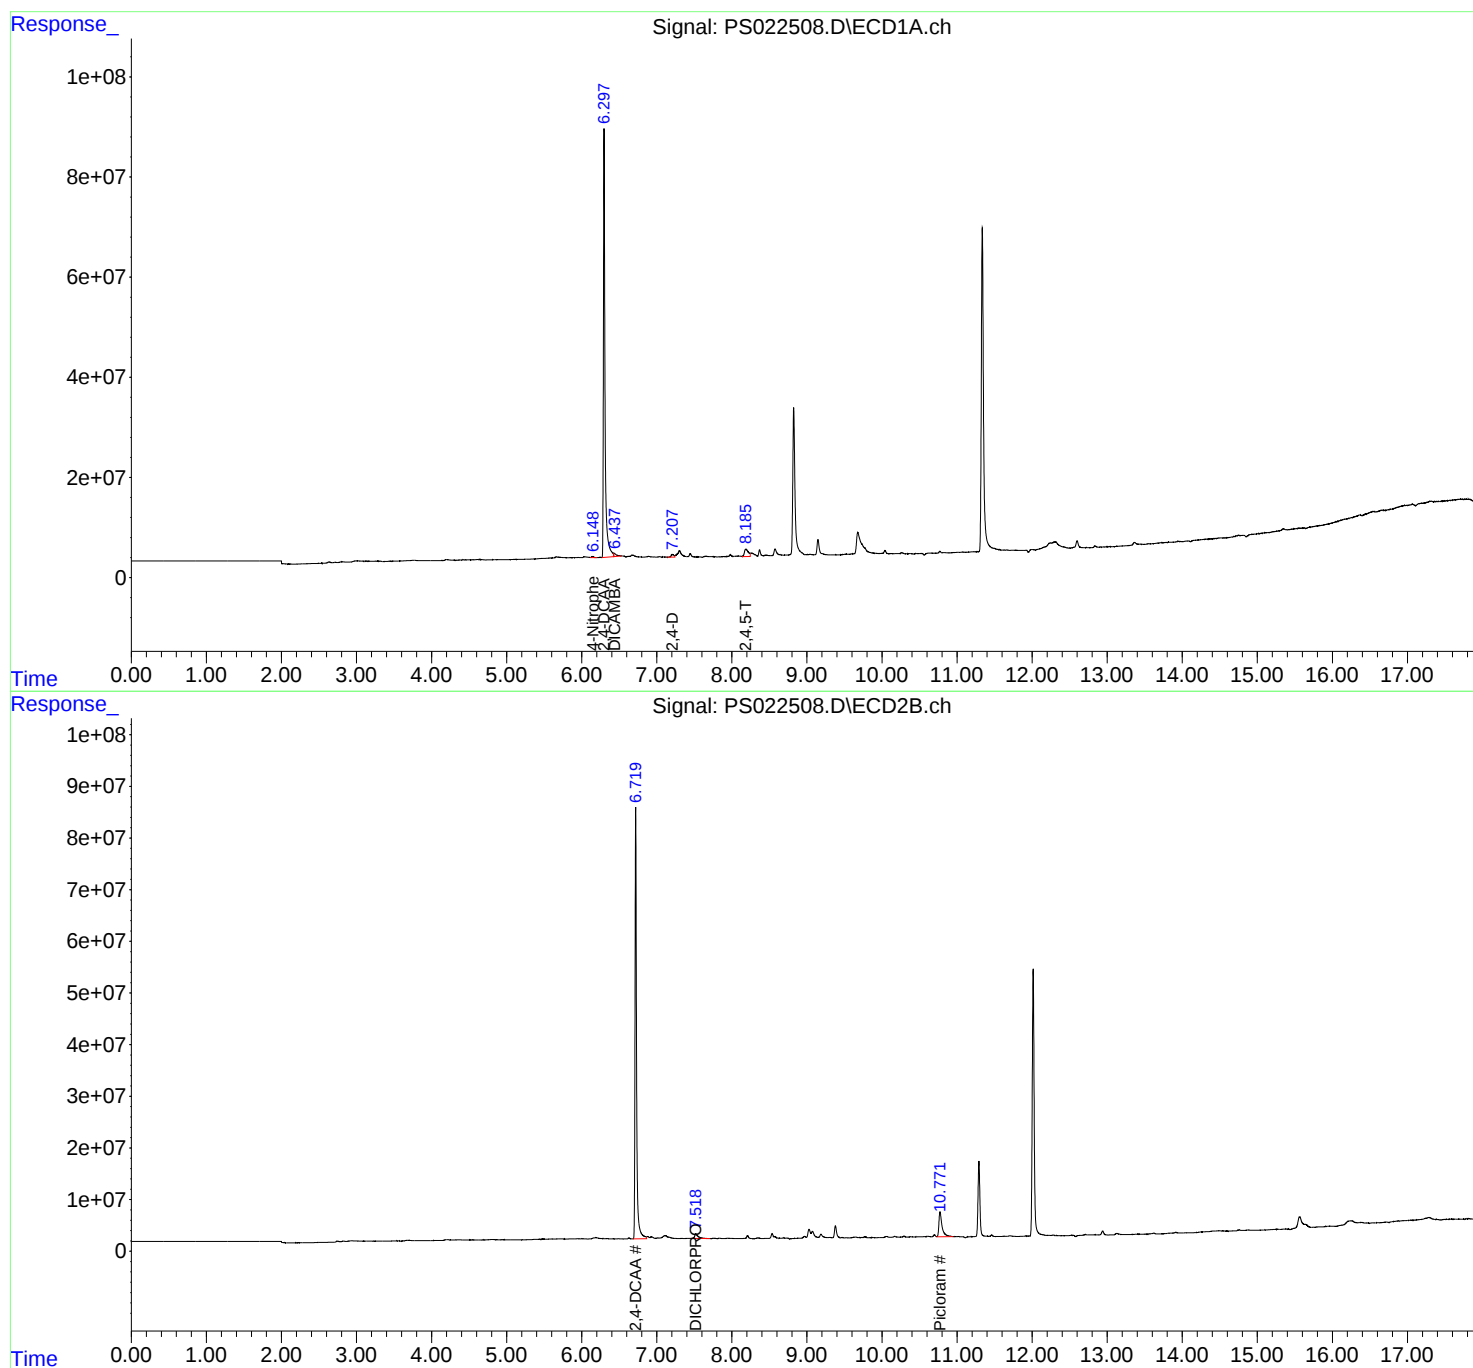


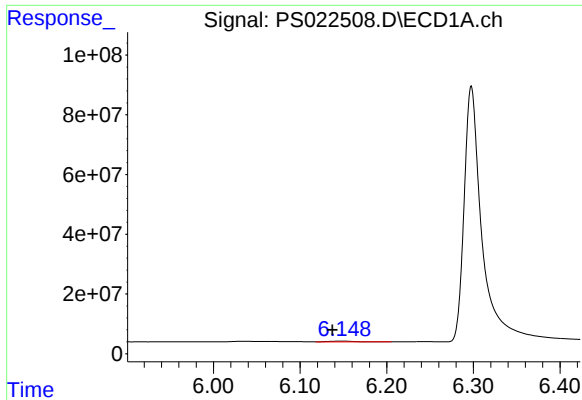

#3 4-Nitrophenol


R.T.: 6.149 min
Delta R.T.: 0.011 min
Response: 4847069
Conc: 3.54 ng/ml

Instrument :
ECD_S
ClientSampleId :

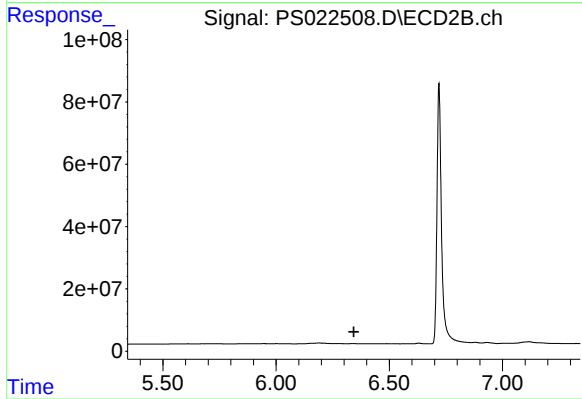


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.344 min
Response: 0
Conc: N.D.

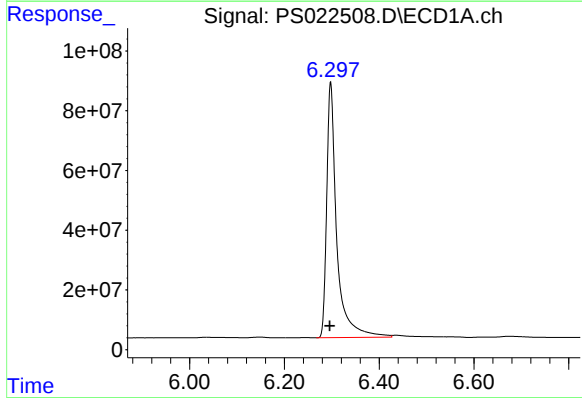


#4 2,4-DCAA

R.T.: 6.298 min
Delta R.T.: 0.002 min
Response: 1264141684
Conc: 517.16 ng/ml

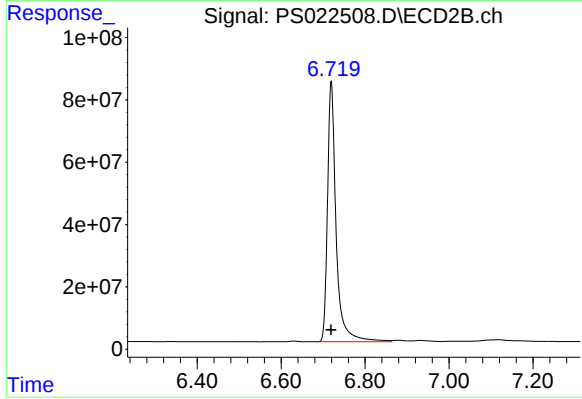

#4 2,4-DCAA


R.T.: 6.719 min
Delta R.T.: 0.000 min
Response: 1192344595
Conc: 578.90 ng/ml

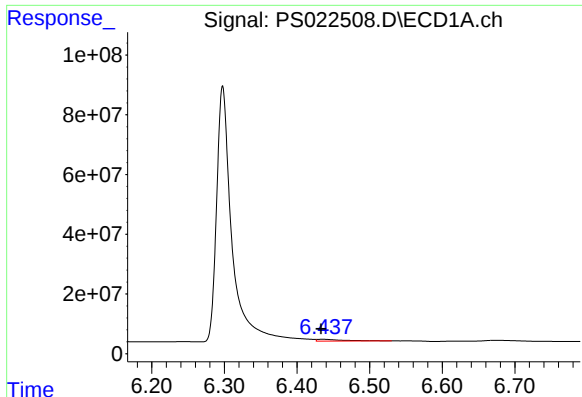

#5 DICAMBA


R.T.: 6.435 min
Delta R.T.: 0.002 min
Response: 16100348
Conc: 1.57 ng/ml

Instrument :
ECD_S
ClientSampleId :

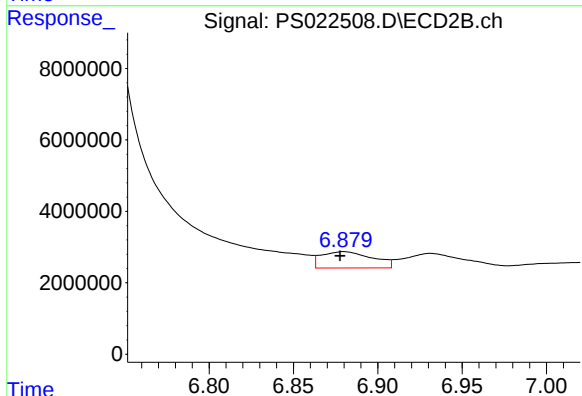


#5 DICAMBA

R.T.: 6.880 min
Delta R.T.: 0.002 min
Response: 9588375
Conc: N.D.

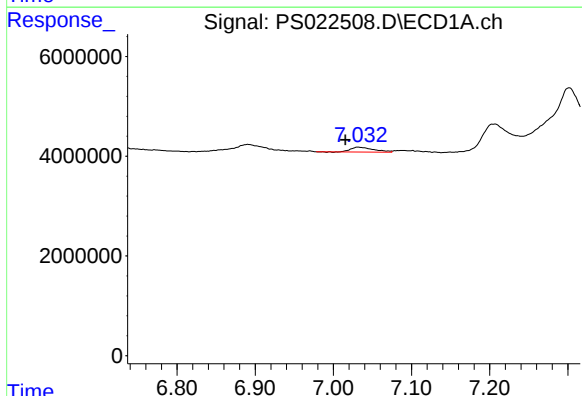


#8 DICHLORPROP

R.T.: 7.034 min
Delta R.T.: 0.018 min
Response: 1993711
Conc: N.D.

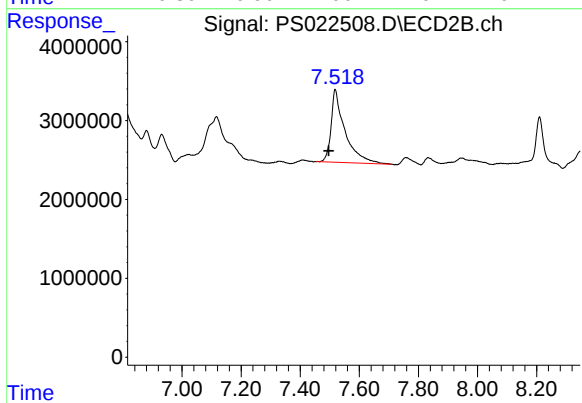

#8 DICHLORPROP


R.T.: 7.518 min
Delta R.T.: 0.021 min
Response: 30113018
Conc: 12.09 ng/ml

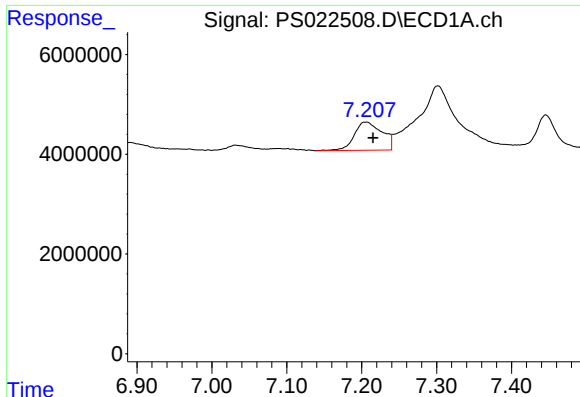

#9 2,4-D


R.T.: 7.206 min
Delta R.T.: -0.009 min
Response: 14647428
Conc: 4.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

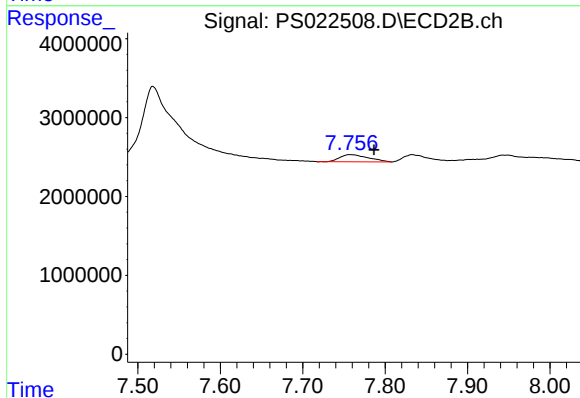


#9 2,4-D

R.T.: 7.757 min
Delta R.T.: -0.030 min
Response: 2157956
Conc: N.D.

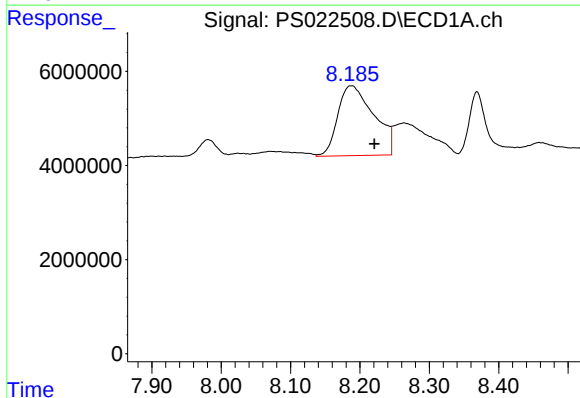


#12 2,4,5-T

R.T.: 8.188 min
Delta R.T.: -0.033 min
Response: 53873051
Conc: 3.28 ng/ml

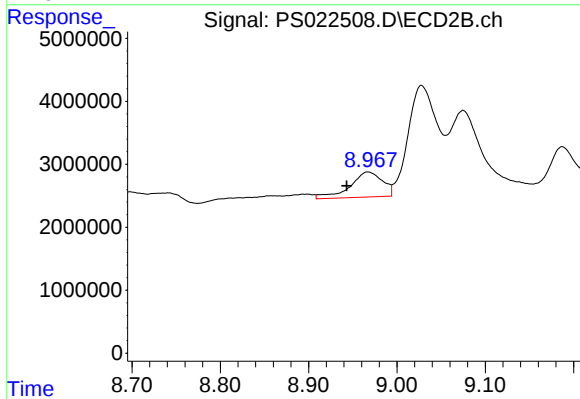

#12 2,4,5-T


R.T.: 8.967 min
Delta R.T.: 0.024 min
Response: 10222148
Conc: N.D.

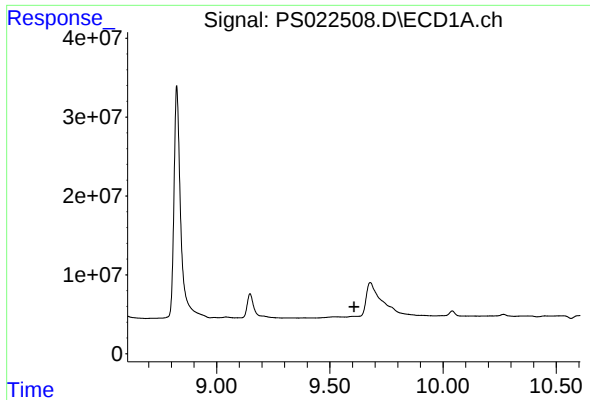

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 9.607 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

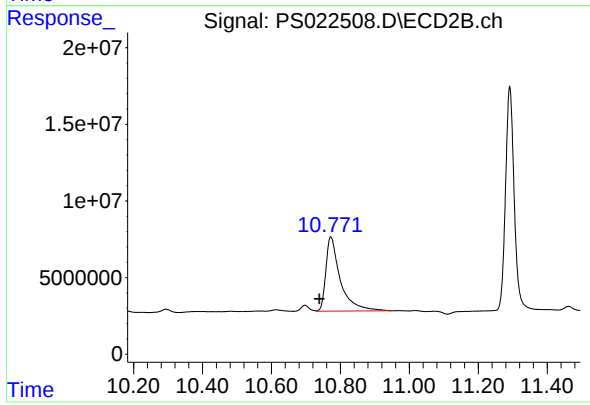

#15 Picloram

R.T.: 10.772 min
Delta R.T.: 0.033 min
Response: 141185294
Conc: 7.04 ng/ml