

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032425\
 Data File : PS029515.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 24 Mar 2025 08:27
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 24 12:29:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032025.M
 Quant Title : 8080.M
 QLast Update : Fri Mar 21 04:46:07 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.151	7.578	2295.4E6	450.9E6	554.701	518.626
Target Compounds							
1) T	Dalapon	0.000	2.672f	0	12086909	N.D.	5.989
2) T	3,5-DICHL...	6.346	0.000	992834	0	<MDL	N.D. #
3) T	4-Nitroph...	6.940	0.000	22408975	0	11.883	N.D. #
5) T	DICAMBA	0.000	7.766	0	4868691	N.D.	<MDL
6) T	MCPD	7.470f	0.000	1589515	0	<MDL	N.D. #
7) T	MCPA	7.685	0.000	2556724	0	<MDL	N.D. #
8) T	DICHLORPROP	8.023	8.523f	15536266	6804586	3.365	5.622 #
10) T	Pentachlo...	8.543	9.309	7357500	10034518	<MDL	<MDL #
11) T	2,4,5-TP ...	9.108f	0.000	8538136	0	<MDL	N.D. #
12) T	2,4,5-T	9.438	0.000	9755207	0	<MDL	N.D. #
13) T	2,4-DB	9.986	0.000	1304792	0	<MDL	N.D. #
14) T	DINOSEB	11.175	11.087f	5388687	4443696	<MDL	<MDL #
15) T	Picloram	11.030	12.112	63796113	31626349	2.118	2.787 #
16) T	DCPA	11.477	12.112f	2958179	31626349	<MDL	2.645 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032425\
Data File : PS029515.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 24 Mar 2025 08:27
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 24 12:29:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032025.M
Quant Title : 8080.M
QLast Update : Fri Mar 21 04:46:07 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

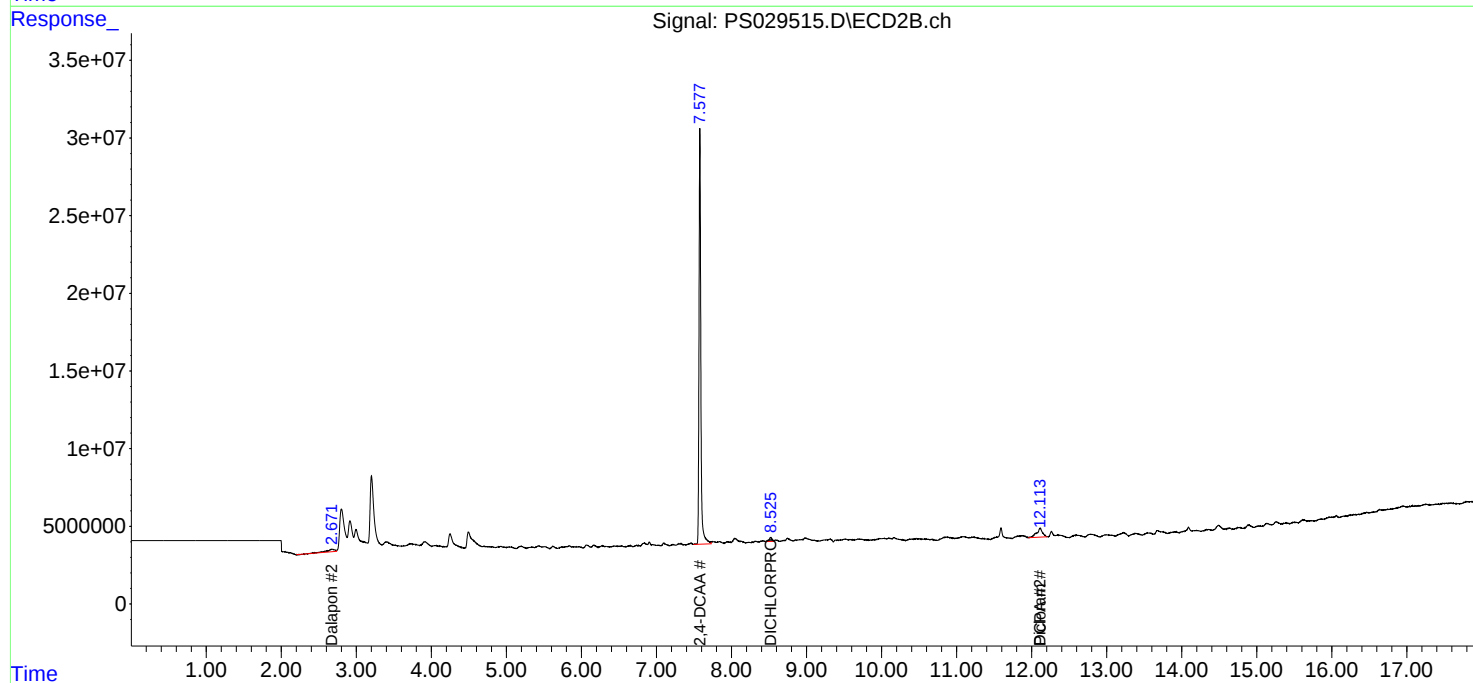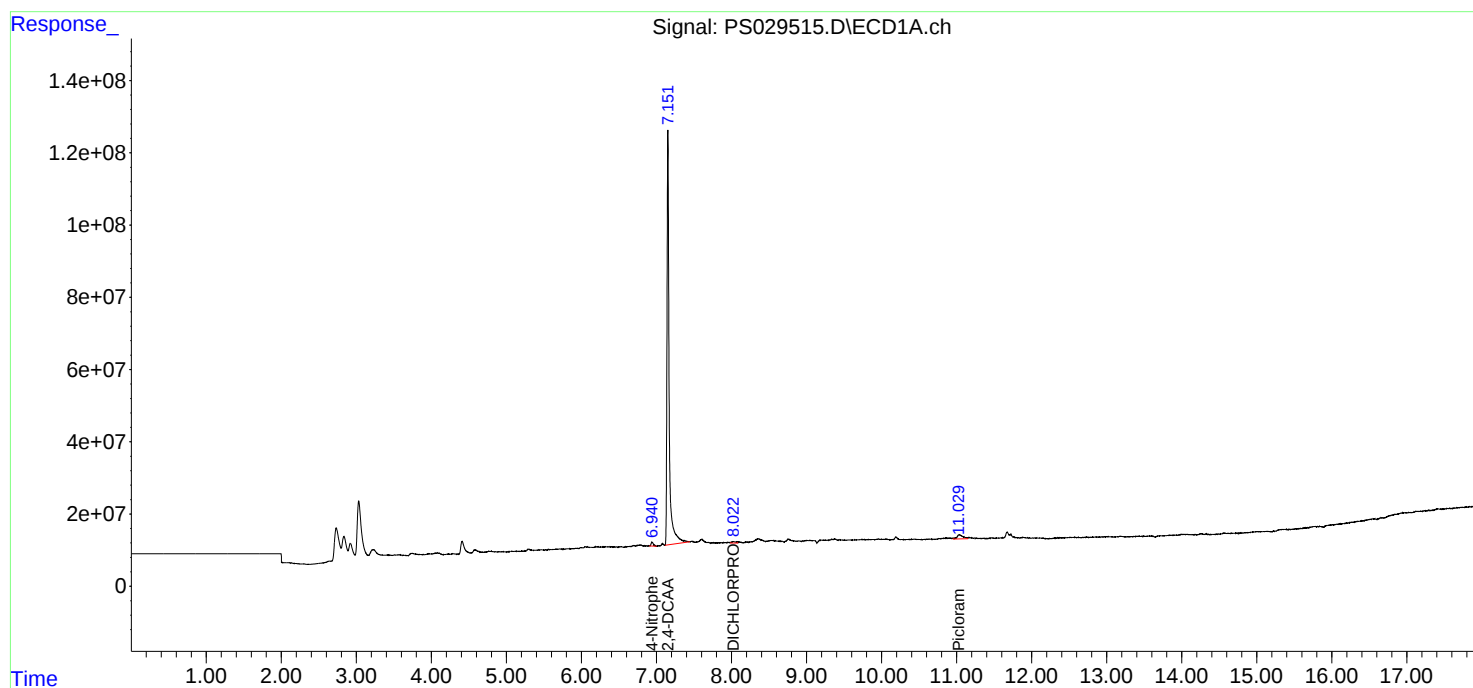


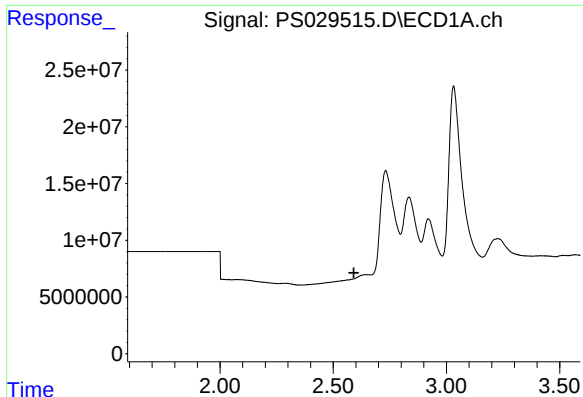

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.591 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

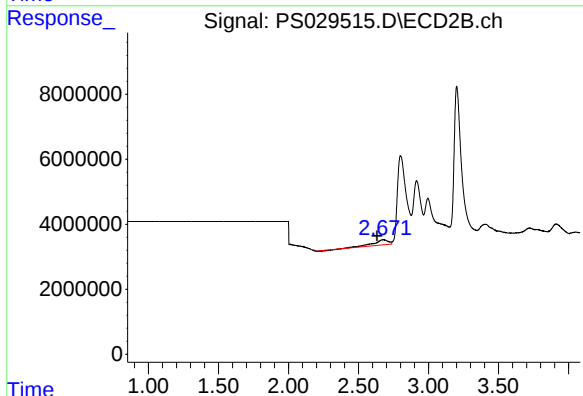


#1 Dalapon

R.T.: 2.672 min
Delta R.T.: 0.040 min
Response: 12086909
Conc: 5.99 ng/ml

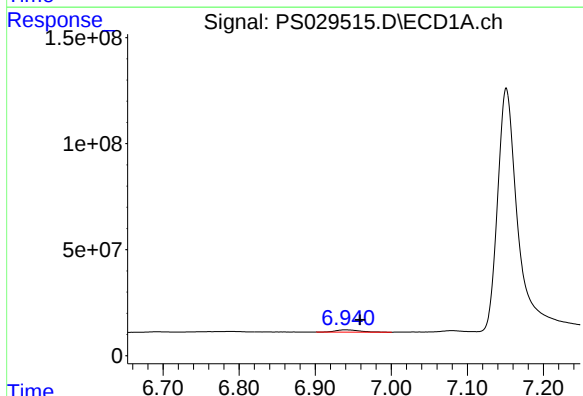


#3 4-Nitrophenol

R.T.: 6.940 min
Delta R.T.: -0.019 min
Response: 22408975
Conc: 11.88 ng/ml

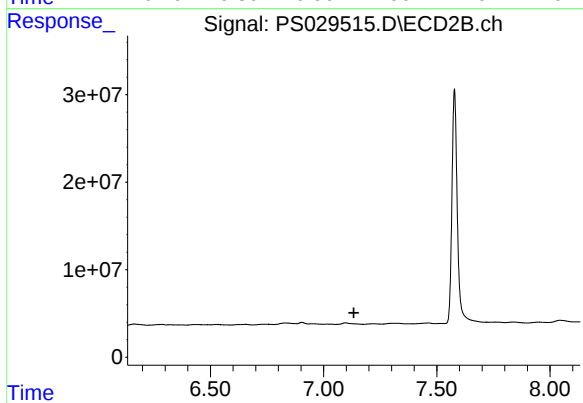

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 7.133 min
Response: 0
Conc: N.D.

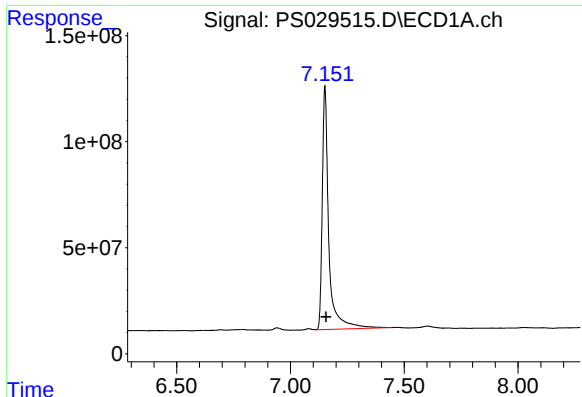

#4 2,4-DCAA


R.T.: 7.151 min
Delta R.T.: -0.006 min
Response: 2295367126
Conc: 554.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

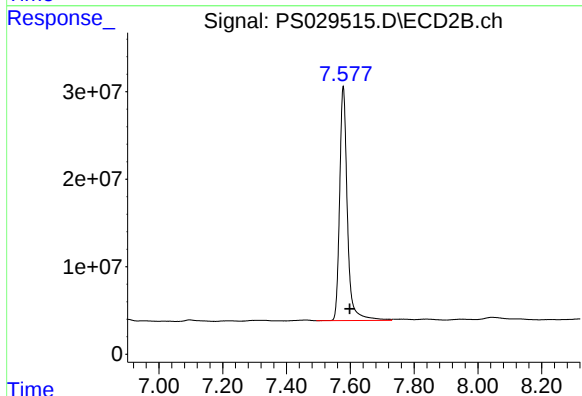


#4 2,4-DCAA

R.T.: 7.578 min
Delta R.T.: -0.021 min
Response: 450940492
Conc: 518.63 ng/ml

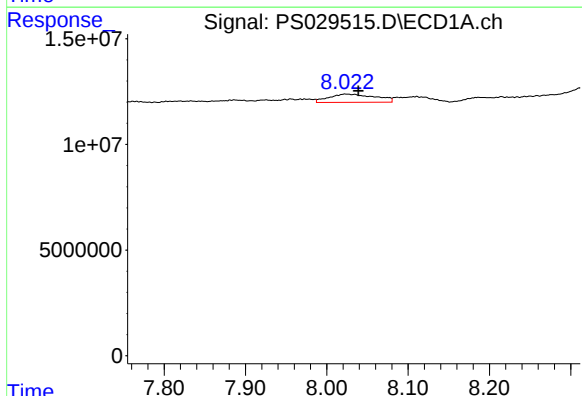


#8 DICHLORPROP

R.T.: 8.023 min
Delta R.T.: -0.016 min
Response: 15536266
Conc: 3.36 ng/ml

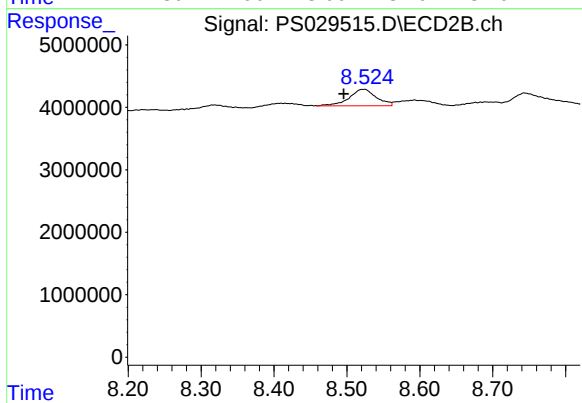

#8 DICHLORPROP


R.T.: 8.523 min
Delta R.T.: 0.027 min
Response: 6804586
Conc: 5.62 ng/ml

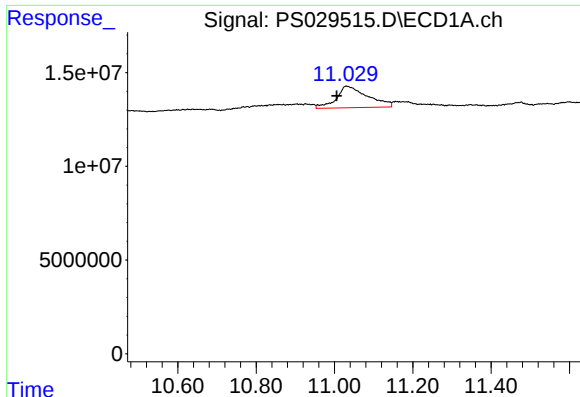

#15 Picloram


R.T.: 11.030 min
Delta R.T.: 0.025 min
Response: 63796113
Conc: 2.12 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

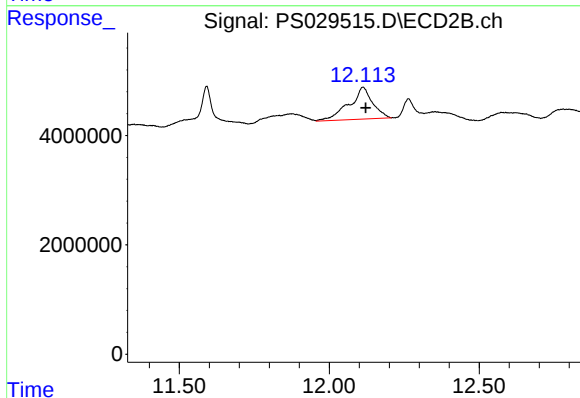


#15 Picloram

R.T.: 12.112 min
Delta R.T.: -0.010 min
Response: 31626349
Conc: 2.79 ng/ml

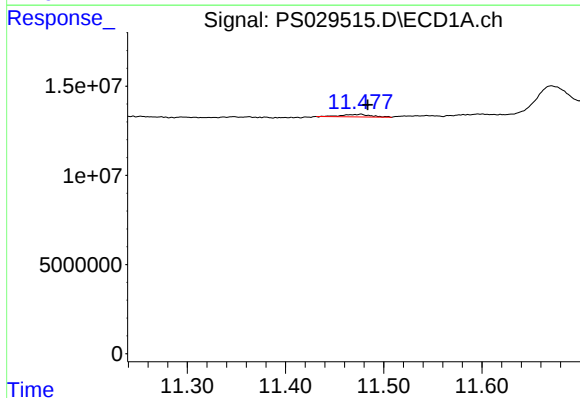

#16 DCPA

R.T.: 11.477 min
Delta R.T.: -0.007 min
Response: 2958179
Conc: N.D.

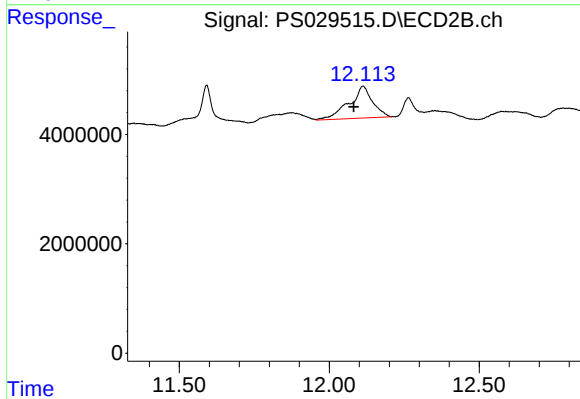

#16 DCPA

R.T.: 12.112 min
Delta R.T.: 0.030 min
Response: 31626349
Conc: 2.65 ng/ml