

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032519\
 Data File : PS003709.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2019 09:09
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 17:07:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	0.000	10.780	0	562502	N.D.	1.198 #
Target Compounds							
2) T	3,5-DICHL...	0.000	8.935	0	369608	N.D.	0.599 #
3) T	4-Nitroph...	0.000	9.925	0	125456	N.D.	0.558 #
6) T	MCP	0.000	11.300	0	223287	N.D.	0.189 #
7) T	MCPA	0.000	11.688	0	11374	N.D.	0.007 #
9) T	2,4-D	0.000	12.628	0	50090	N.D.	0.095 #
10) T	Pentachlo...	0.000	13.194	0	49045	N.D.	0.007 #
14) T	DINOSEB	0.000	15.431	0	472970	N.D.	0.265 #
16) T	DCPA	0.000	16.604	0	1235561	N.D.	0.397 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032519\
Data File : PS003709.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2019 09:09
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 17:07:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

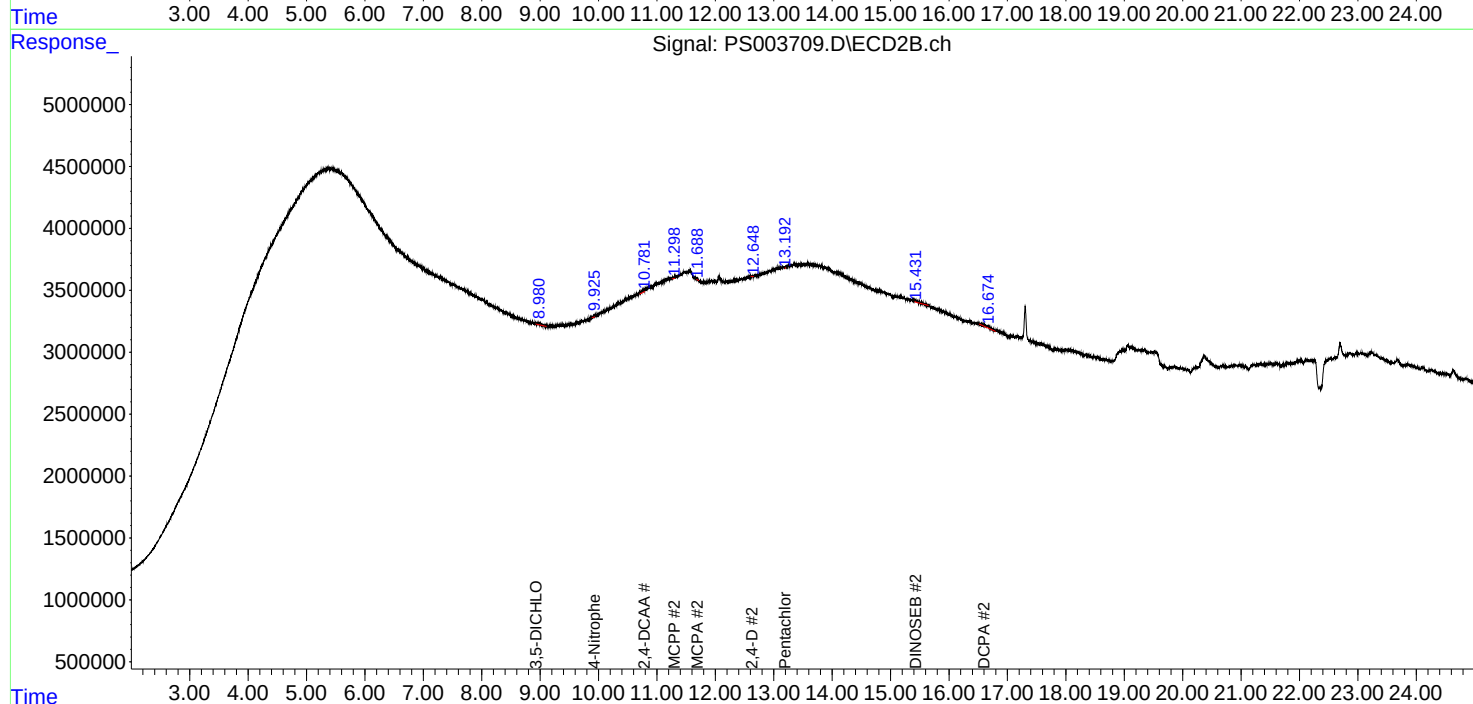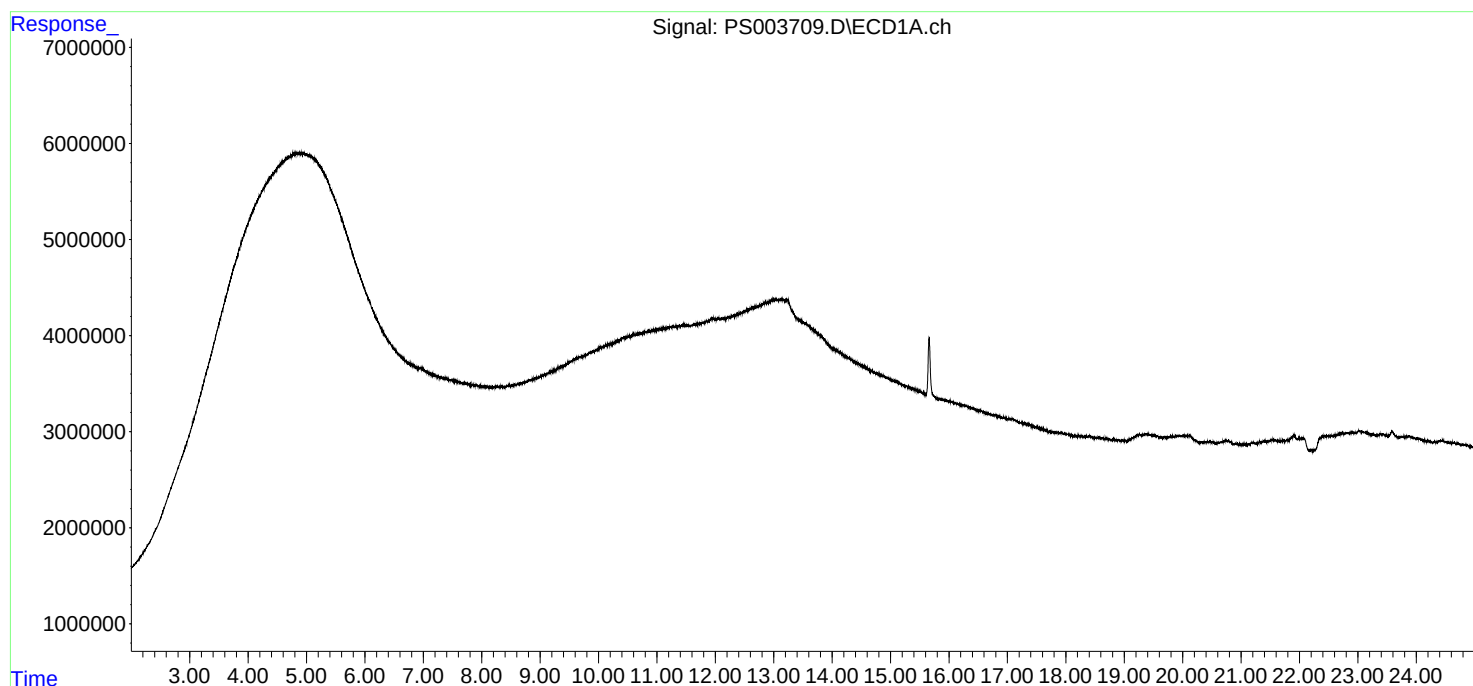


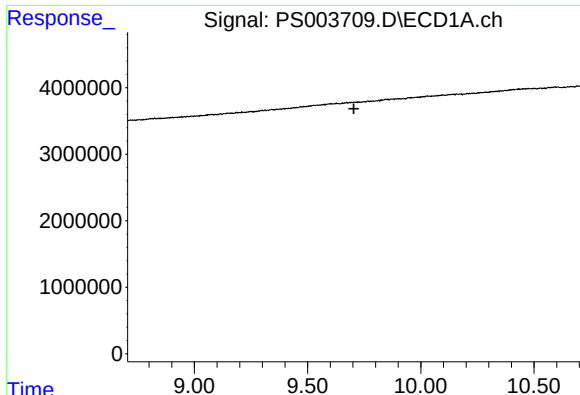

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

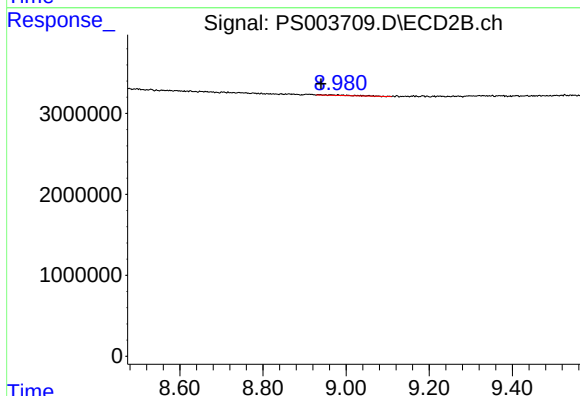


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.935 min
Delta R.T.: -0.004 min
Response: 369608
Conc: 0.60 ng/ml

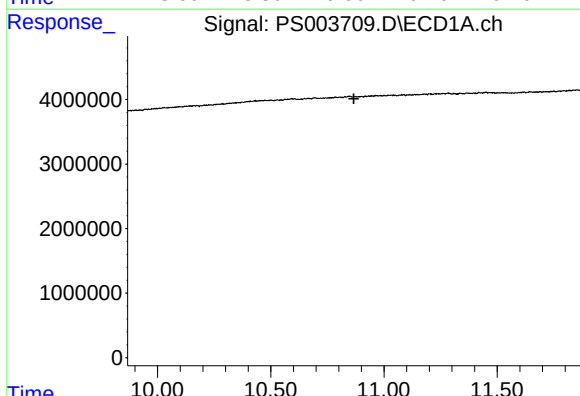


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

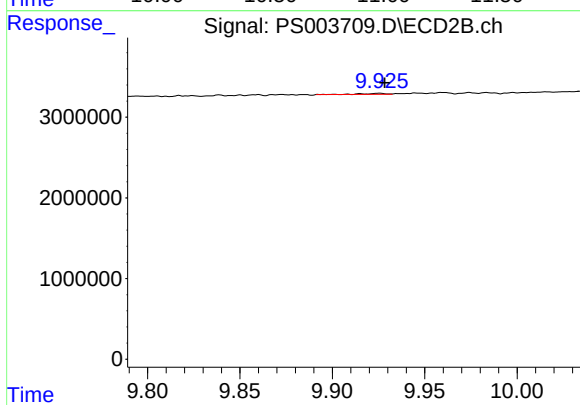

#3 4-Nitrophenol


R.T.: 9.925 min
Delta R.T.: -0.003 min
Response: 125456
Conc: 0.56 ng/ml

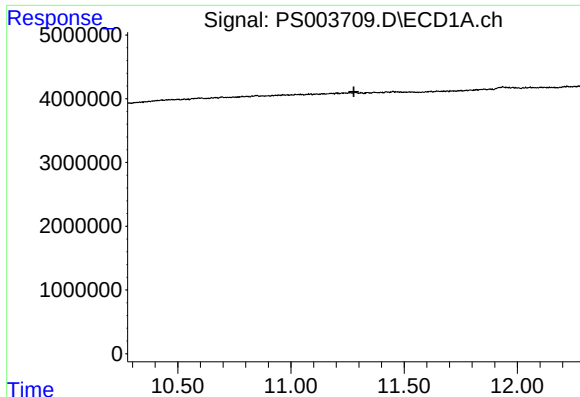

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 11.278 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

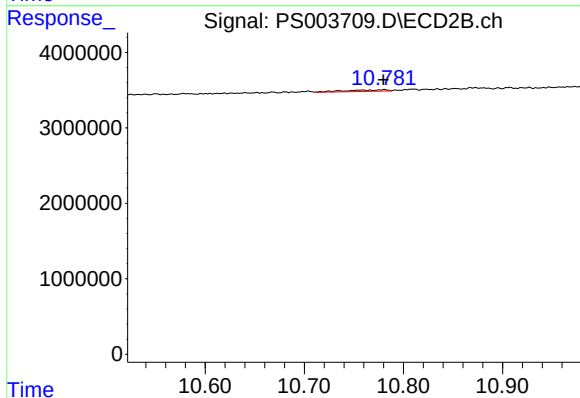


#4 2,4-DCAA

R.T.: 10.780 min
Delta R.T.: 0.000 min
Response: 562502
Conc: 1.20 ng/ml

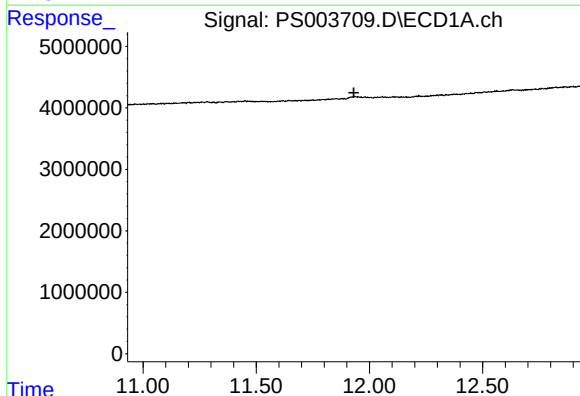


#6 MCP

R.T.: 0.000 min
Exp R.T.: 11.931 min
Response: 0
Conc: N.D.

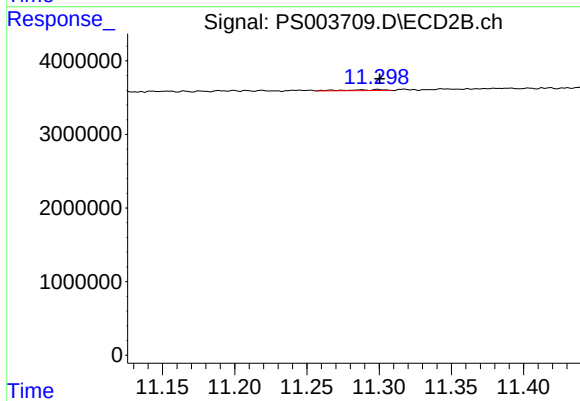

#6 MCP


R.T.: 11.300 min
Delta R.T.: 0.000 min
Response: 223287
Conc: 0.19 ug/ml

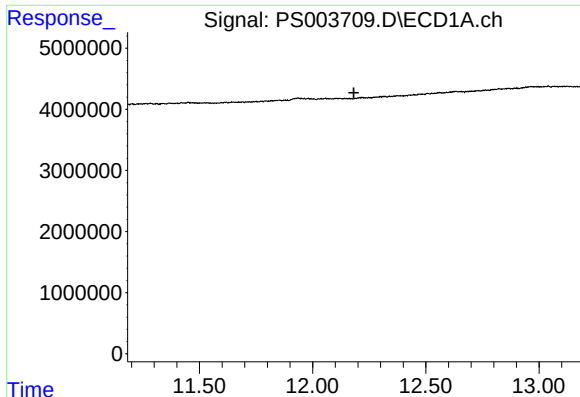

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

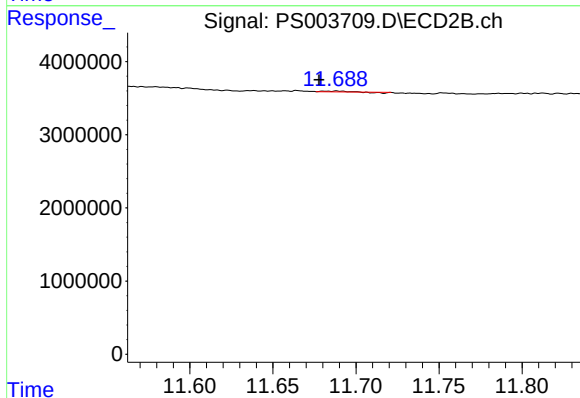


#7 MCPA

R.T.: 11.688 min
Delta R.T.: 0.010 min
Response: 11374
Conc: 0.01 ug/ml

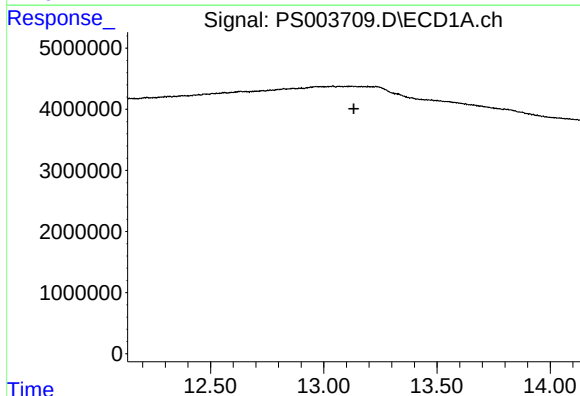


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.133 min
Response: 0
Conc: N.D.

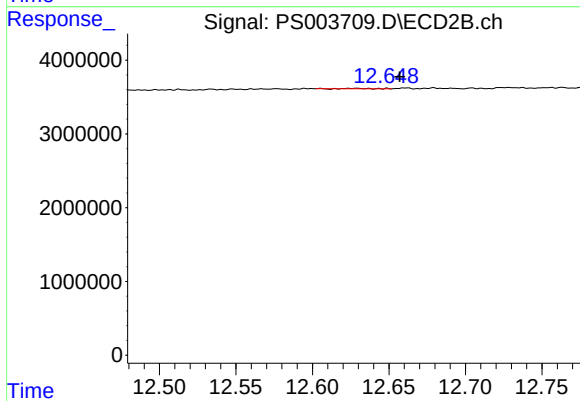

#9 2,4-D


R.T.: 12.628 min
Delta R.T.: -0.029 min
Response: 50090
Conc: 0.10 ng/ml

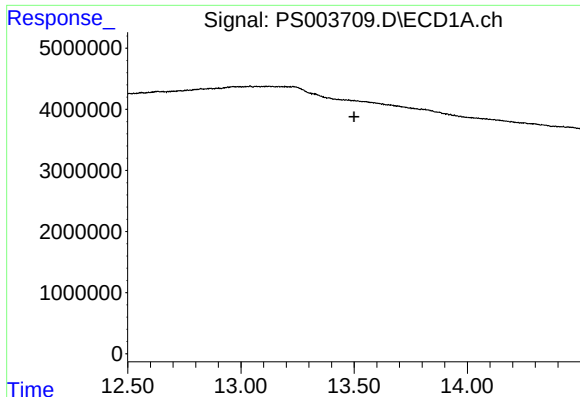

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

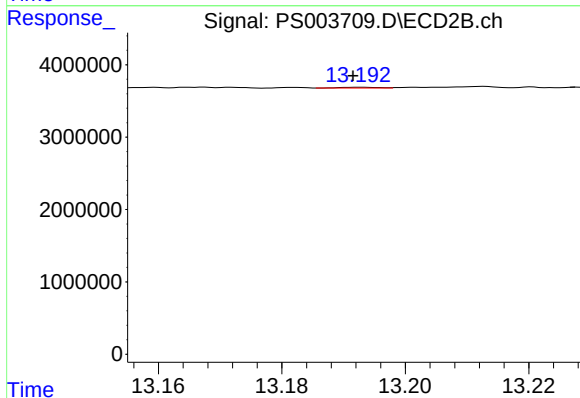


#10 Pentachlorophenol

R.T.: 13.194 min
Delta R.T.: 0.002 min
Response: 49045
Conc: 0.01 ng/ml

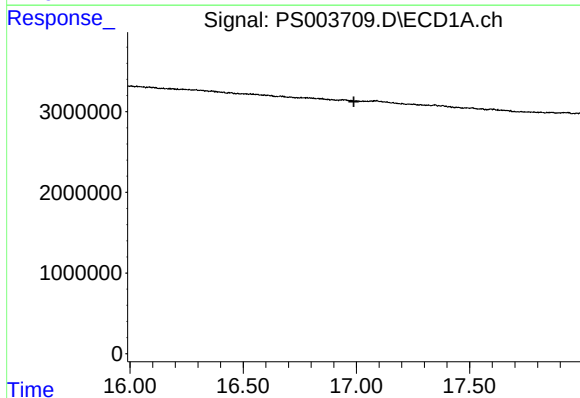


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 16.989 min
Response: 0
Conc: N.D.

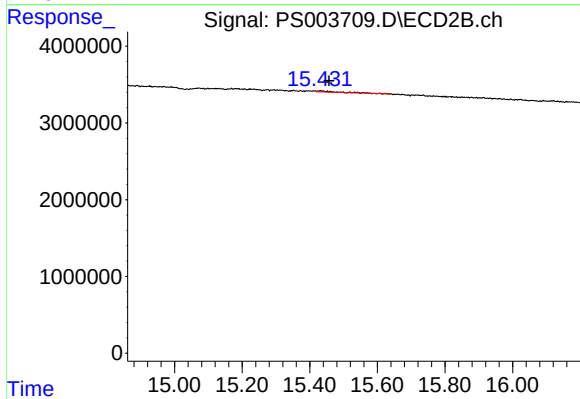

#14 DINOSEB


R.T.: 15.431 min
Delta R.T.: -0.026 min
Response: 472970
Conc: 0.26 ng/ml

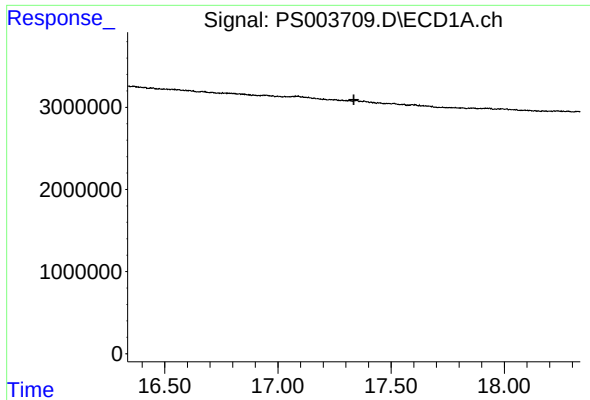

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

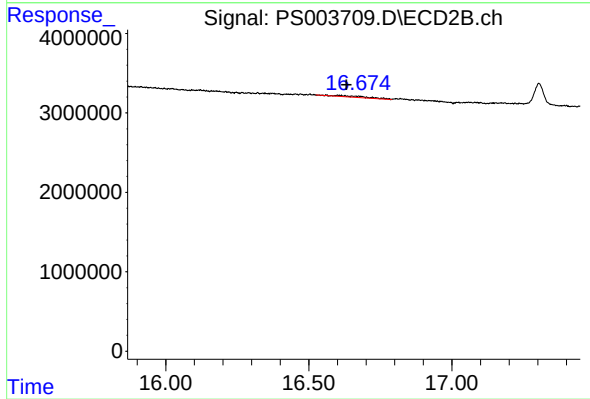

#16 DCPA

R.T.: 16.604 min
Delta R.T.: -0.028 min
Response: 1235561
Conc: 0.40 ng/ml