

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS032519\  
 Data File : PS003710.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 25 Mar 2019 09:40  
 Operator : EI\SJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Mar 25 17:07:02 2019  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS022719.M  
 Quant Title : 8080.M  
 QLast Update : Thu Feb 28 03:00:19 2019  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1   | RT#2   | Resp#1  | Resp#2  | ng/ml   | ng/ml   |
|-----------------------------|--------------|--------|--------|---------|---------|---------|---------|
| -----                       |              |        |        |         |         |         |         |
| System Monitoring Compounds |              |        |        |         |         |         |         |
| 4) S                        | 2,4-DCAA     | 11.289 | 10.774 | 227.0E6 | 214.1E6 | 517.031 | 456.001 |
| Target Compounds            |              |        |        |         |         |         |         |
| 8) T                        | DICHLORPROP  | 0.000  | 12.193 | 0       | 675213  | N.D.    | 1.634 # |
| 10) T                       | Pentachlo... | 0.000  | 13.186 | 0       | 727664  | N.D.    | 0.110 # |
| 12) T                       | 2,4,5-T      | 0.000  | 14.325 | 0       | 383102  | N.D.    | 0.190 # |
| 13) T                       | 2,4-DB       | 0.000  | 14.990 | 0       | 100401  | N.D.    | 0.393 # |
| 14) T                       | DINOSEB      | 0.000  | 15.497 | 0       | 282100  | N.D.    | 0.158 # |
| 15) T                       | Picloram     | 0.000  | 16.618 | 0       | 1010828 | N.D.    | 0.398 # |
| 16) T                       | DCPA         | 0.000  | 16.618 | 0       | 1010828 | N.D.    | 0.325 # |
| -----                       |              |        |        |         |         |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS032519\  
Data File : PS003710.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 25 Mar 2019 09:40  
Operator : EI\SJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Mar 25 17:07:02 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS022719.M  
Quant Title : 8080.M  
QLast Update : Thu Feb 28 03:00:19 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

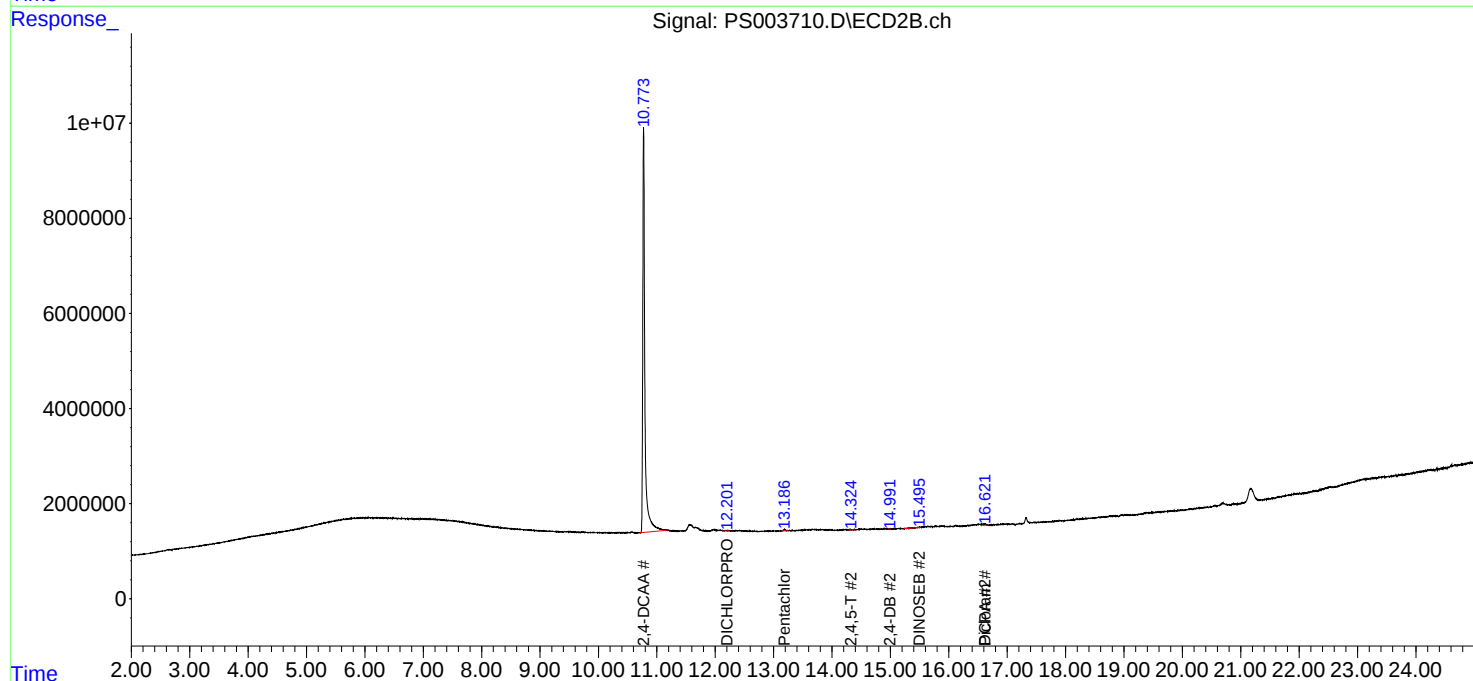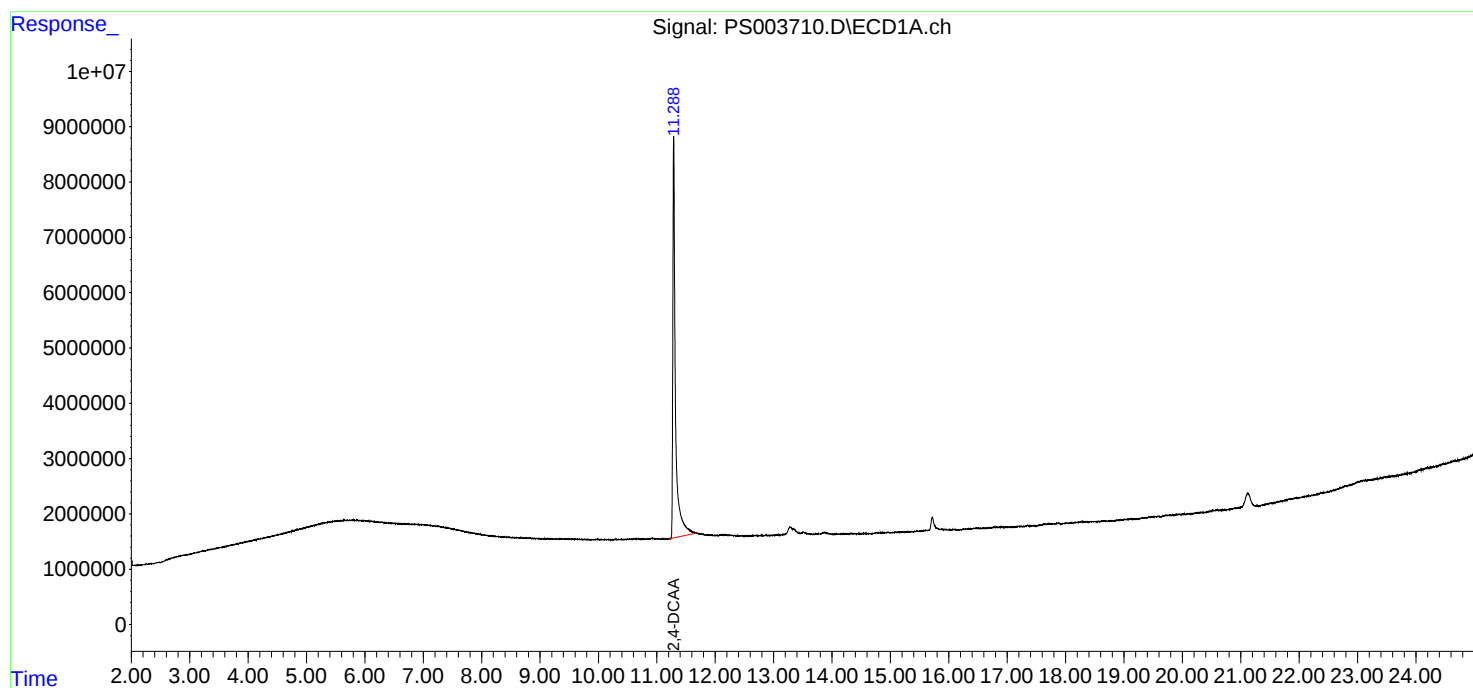


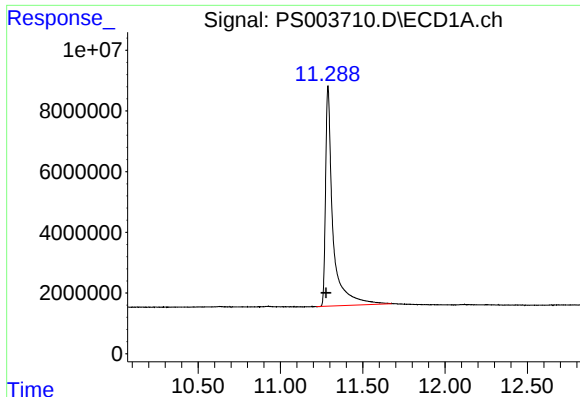

#4 2,4-DCAA


R.T.: 11.289 min  
Delta R.T.: 0.011 min  
Response: 226989281  
Conc: 517.03 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

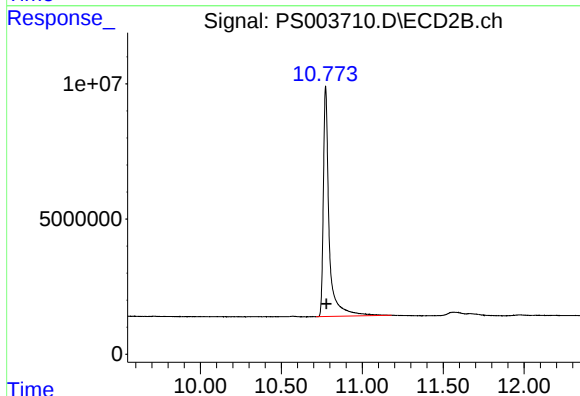


#4 2,4-DCAA

R.T.: 10.774 min  
Delta R.T.: -0.006 min  
Response: 214123965  
Conc: 456.00 ng/ml

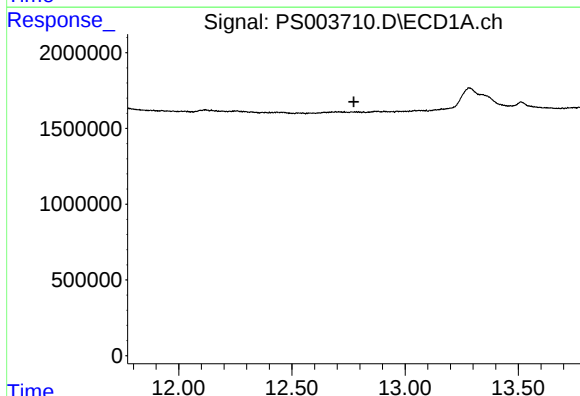


#8 DICHLORPROP

R.T.: 0.000 min  
Exp R.T. : 12.773 min  
Response: 0  
Conc: N.D.

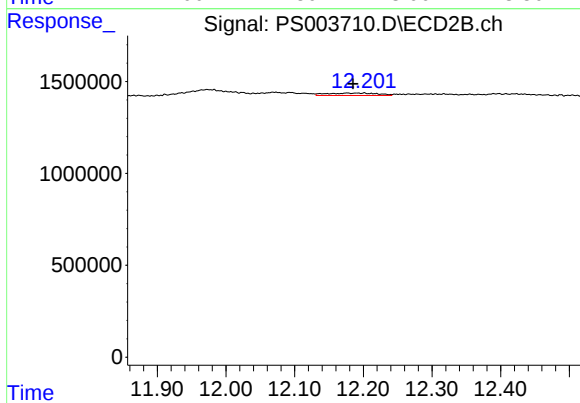

#8 DICHLORPROP


R.T.: 12.193 min  
Delta R.T.: 0.008 min  
Response: 675213  
Conc: 1.63 ng/ml

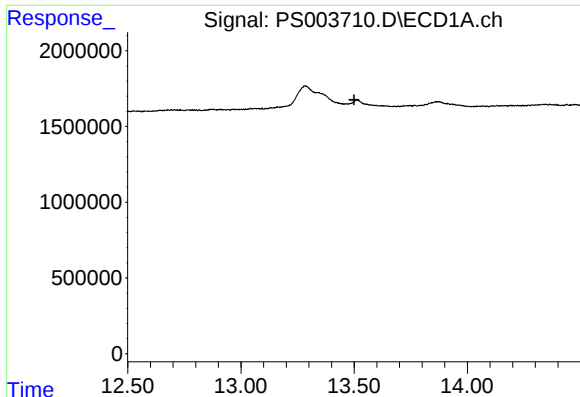

#10 Pentachlorophenol


R.T.: 0.000 min  
Exp R.T.: 13.499 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

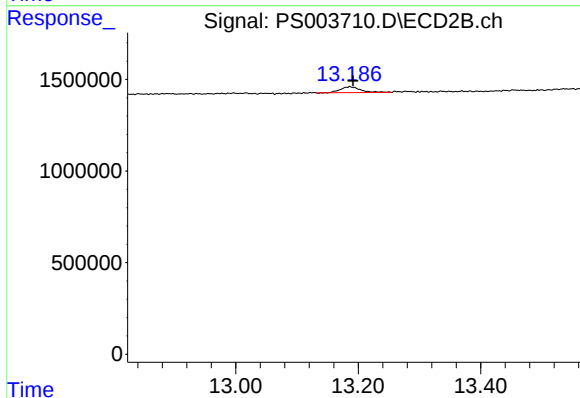


#10 Pentachlorophenol

R.T.: 13.186 min  
Delta R.T.: -0.005 min  
Response: 727664  
Conc: 0.11 ng/ml

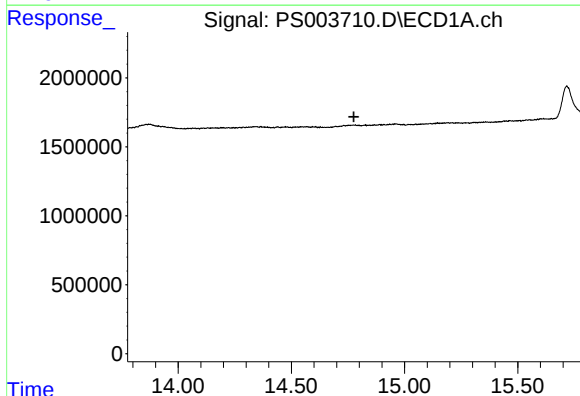


#12 2,4,5-T

R.T.: 0.000 min  
Exp R.T.: 14.776 min  
Response: 0  
Conc: N.D.

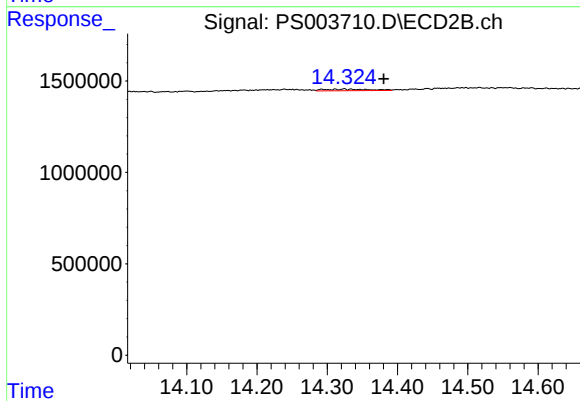

#12 2,4,5-T


R.T.: 14.325 min  
Delta R.T.: -0.056 min  
Response: 383102  
Conc: 0.19 ng/ml

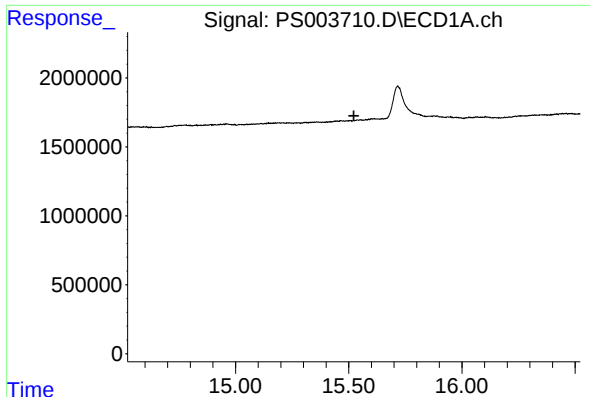

#13 2,4-DB


R.T.: 0.000 min  
Exp R.T.: 15.523 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

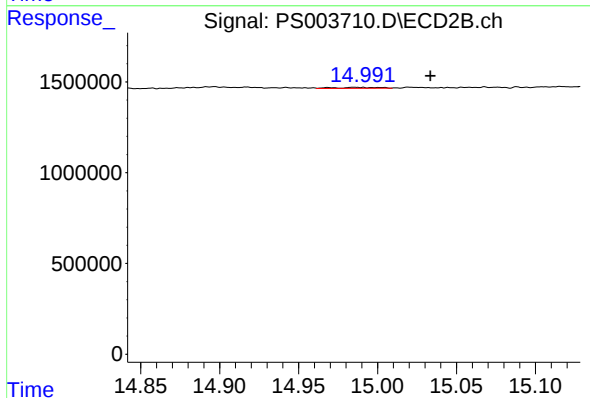


#13 2,4-DB

R.T.: 14.990 min  
Delta R.T.: -0.043 min  
Response: 100401  
Conc: 0.39 ng/ml

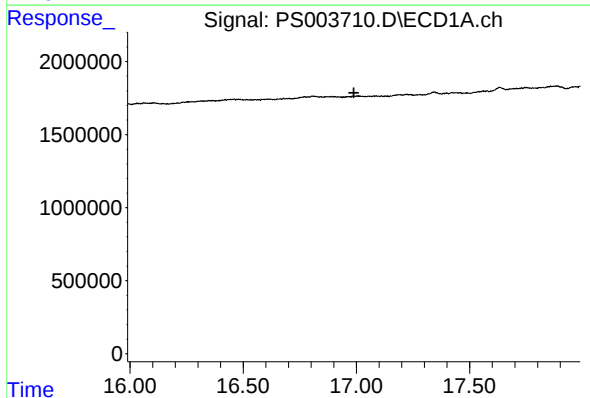


#14 DINOSEB

R.T.: 0.000 min  
Exp R.T.: 16.989 min  
Response: 0  
Conc: N.D.

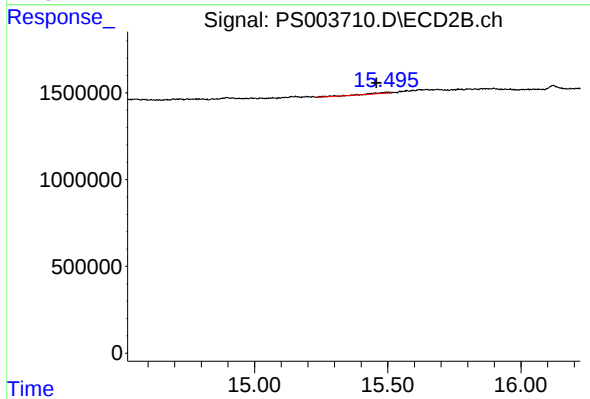

#14 DINOSEB


R.T.: 15.497 min  
Delta R.T.: 0.041 min  
Response: 282100  
Conc: 0.16 ng/ml

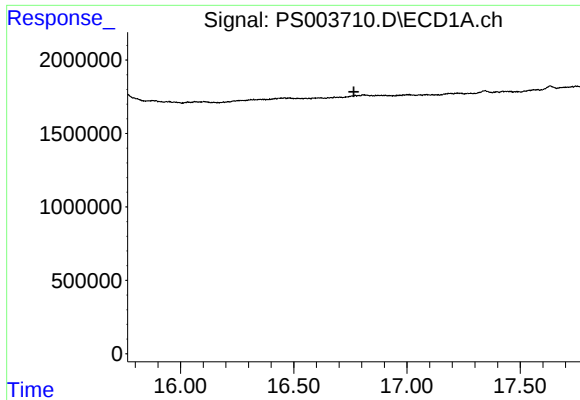

#15 Picloram


R.T.: 0.000 min  
Exp R.T. : 16.765 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

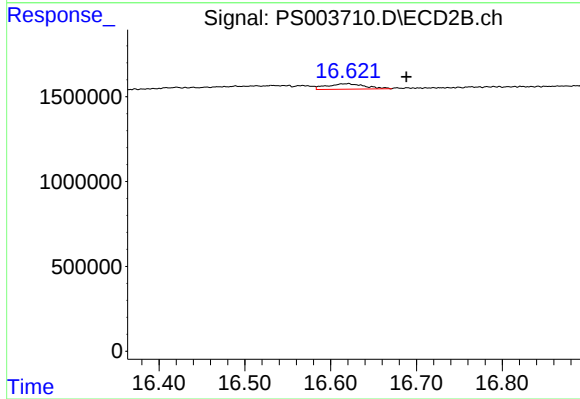


#15 Picloram

R.T.: 16.618 min  
Delta R.T.: -0.070 min  
Response: 1010828  
Conc: 0.40 ng/ml

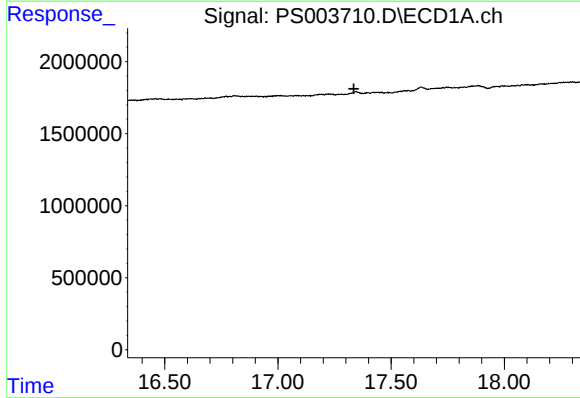

#16 DCPA

R.T.: 0.000 min  
Exp R.T. : 17.335 min  
Response: 0  
Conc: N.D.

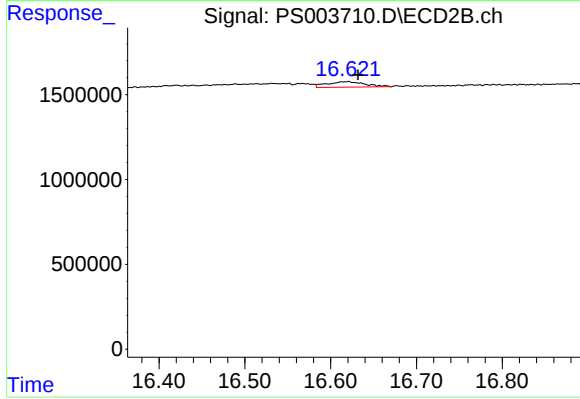

#16 DCPA

R.T.: 16.618 min  
Delta R.T.: -0.014 min  
Response: 1010828  
Conc: 0.32 ng/ml