

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032519\
 Data File : PS003738.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 01:54
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 05:17:23 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.263	10.769	244.2E6	226.3E6	556.168	481.928
Target Compounds							
2) T	3,5-DICHL...	0.000	8.944	0	77066	N.D.	0.125 #
3) T	4-Nitroph...	0.000	9.939	0	61813	N.D.	0.275 #
6) T	MCP	0.000	11.293	0	48761	N.D.	0.041 #
7) T	MCPA	0.000	11.661	0	56385	N.D.	0.033 #
10) T	Pentachlo...	0.000	13.177	0	786384	N.D.	0.119 #
13) T	2,4-DB	0.000	14.998	0	685567	N.D.	2.685 #
14) T	DINOSEB	0.000	15.493	0	316259	N.D.	0.177 #
15) T	Picloram	0.000	16.709	0	916003	N.D.	0.361 #
16) T	DCPA	0.000	16.618	0	1501483	N.D.	0.483 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032519\
Data File : PS003738.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 01:54
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 05:17:23 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

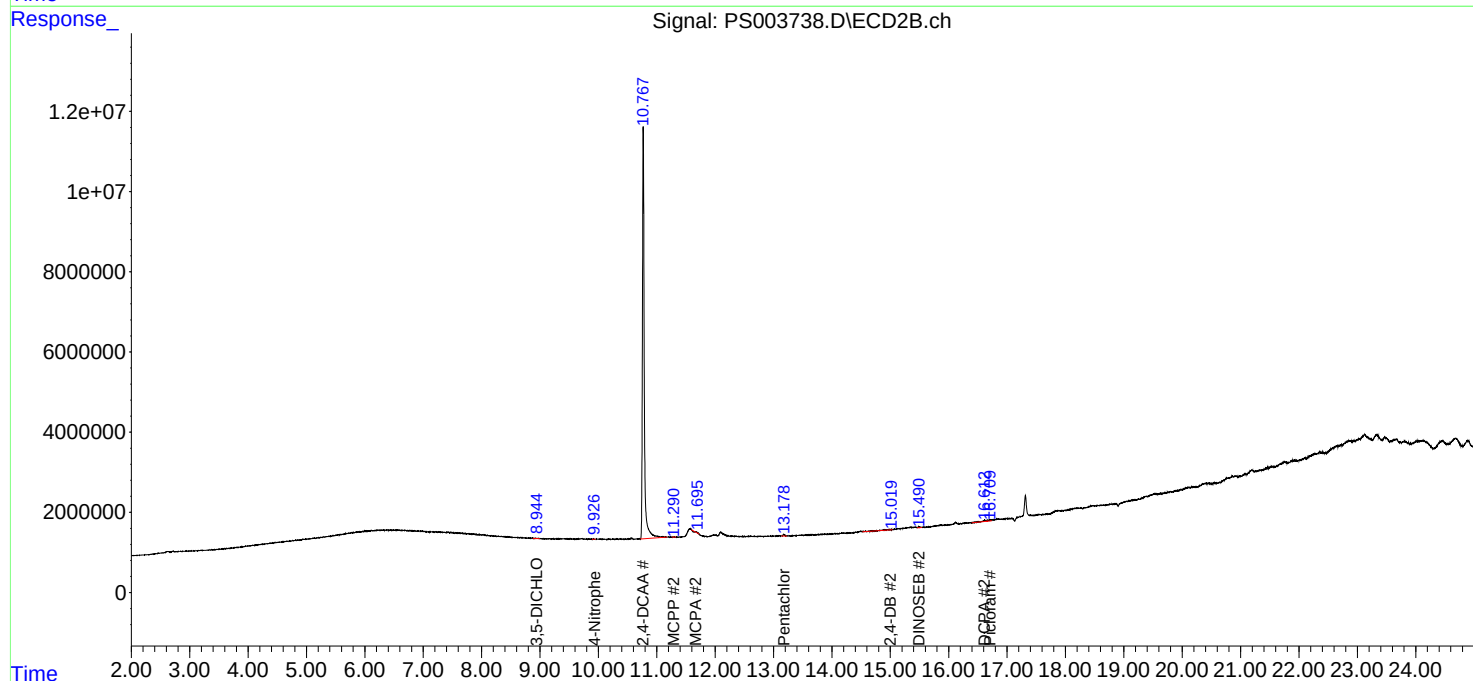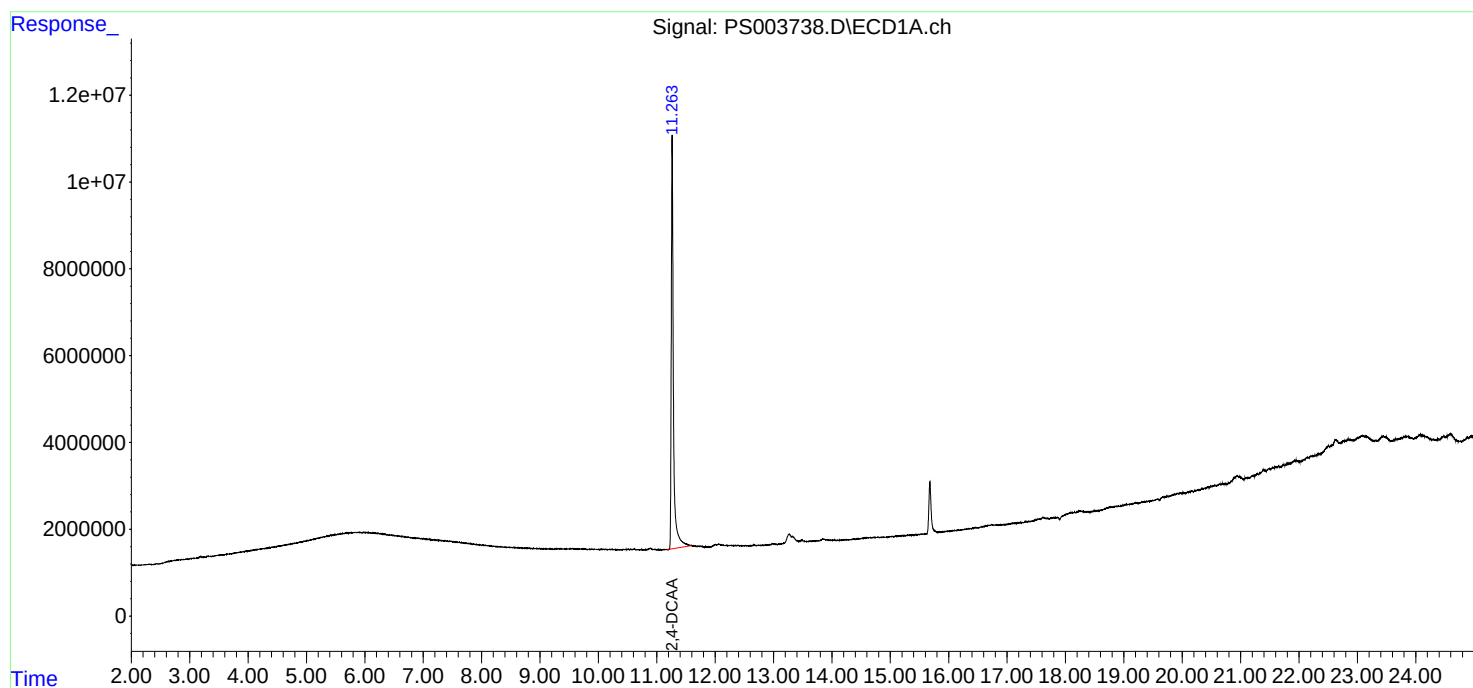


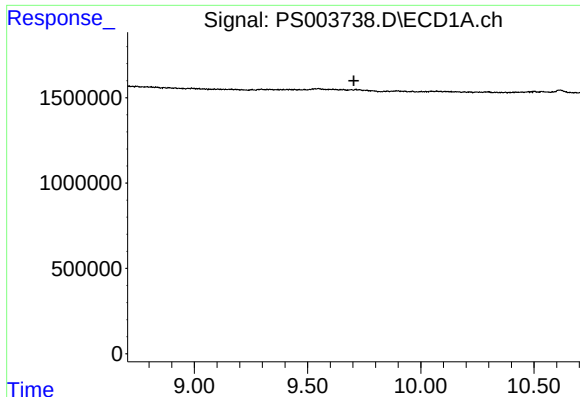

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

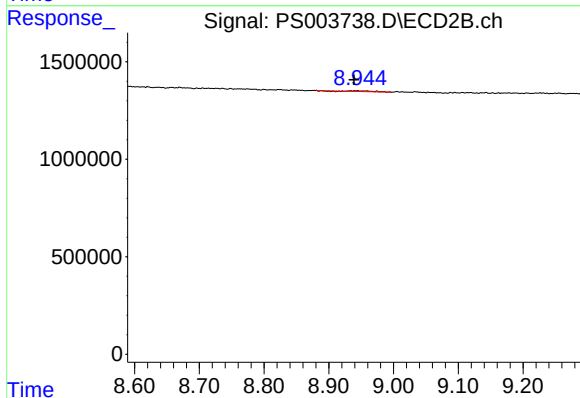


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.944 min
Delta R.T.: 0.004 min
Response: 77066
Conc: 0.12 ng/ml

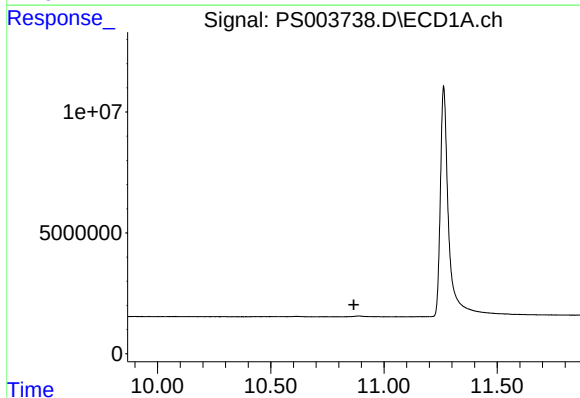


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

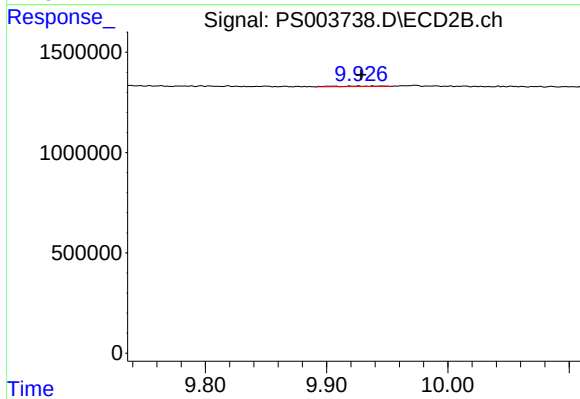

#3 4-Nitrophenol


R.T.: 9.939 min
Delta R.T.: 0.011 min
Response: 61813
Conc: 0.27 ng/ml

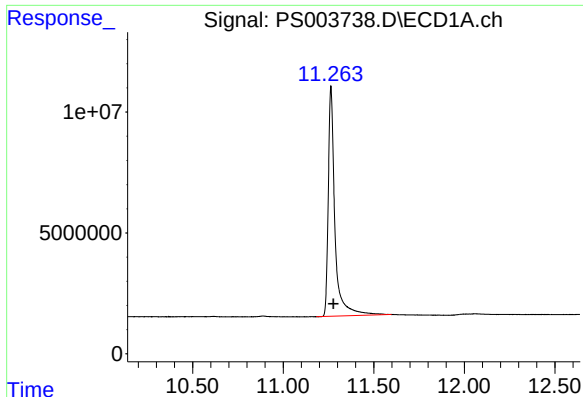

#4 2,4-DCAA


R.T.: 11.263 min
Delta R.T.: -0.014 min
Response: 244171384
Conc: 556.17 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

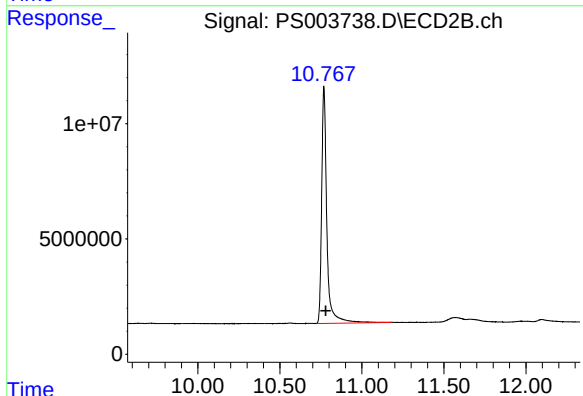


#4 2,4-DCAA

R.T.: 10.769 min
Delta R.T.: -0.011 min
Response: 226298377
Conc: 481.93 ng/ml

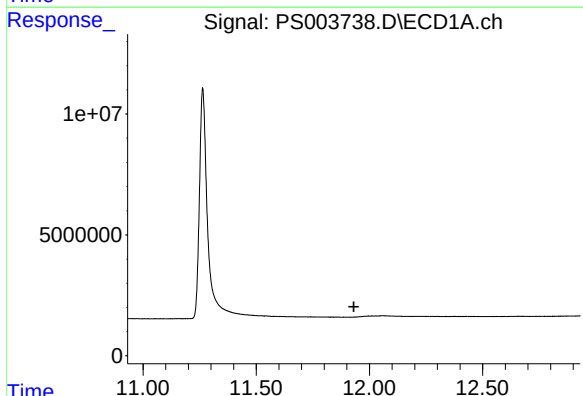


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.931 min
Response: 0
Conc: N.D.

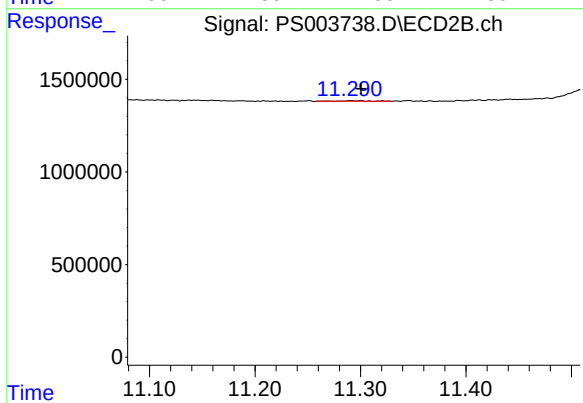

#6 MCP


R.T.: 11.293 min
Delta R.T.: -0.008 min
Response: 48761
Conc: 0.04 ug/ml

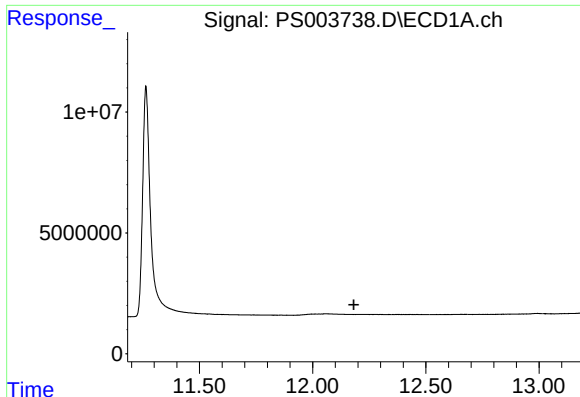

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

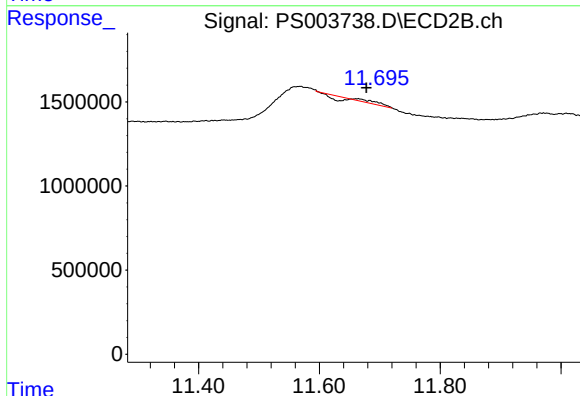


#7 MCPA

R.T.: 11.661 min
Delta R.T.: -0.017 min
Response: 56385
Conc: 0.03 ug/ml

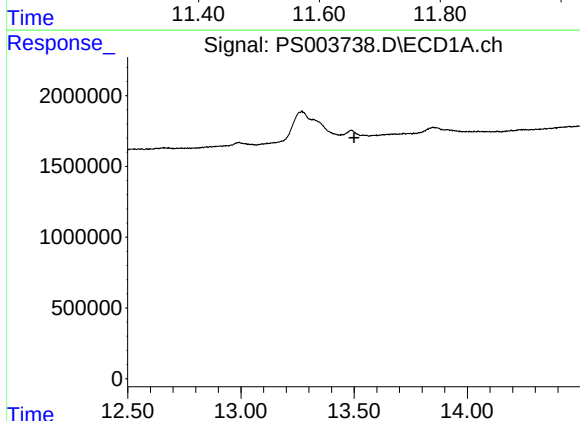


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.499 min
Response: 0
Conc: N.D.

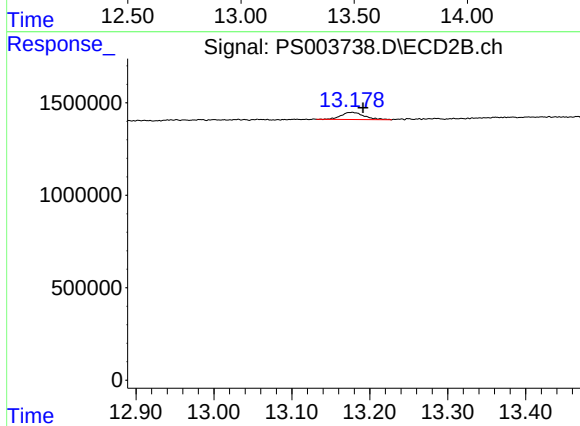

#10 Pentachlorophenol


R.T.: 13.177 min
Delta R.T.: -0.014 min
Response: 786384
Conc: 0.12 ng/ml

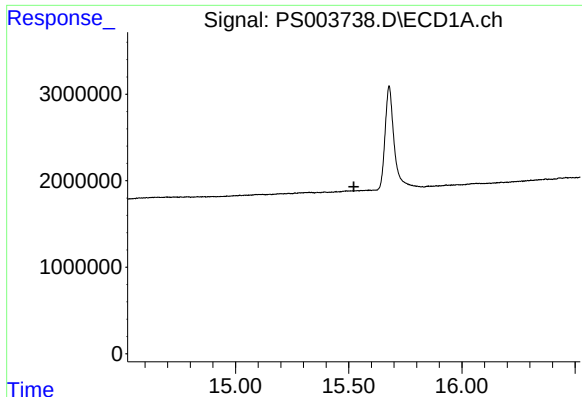

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

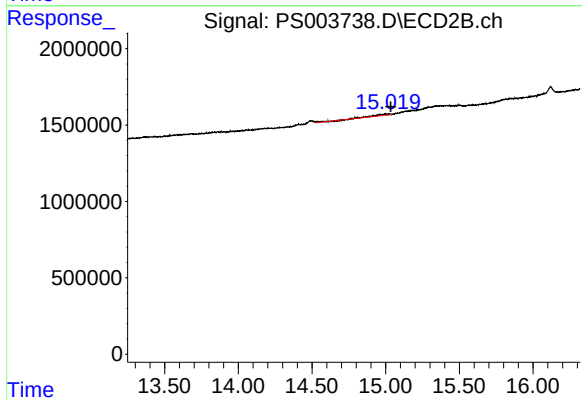


#13 2,4-DB

R.T.: 14.998 min
Delta R.T.: -0.035 min
Response: 685567
Conc: 2.68 ng/ml

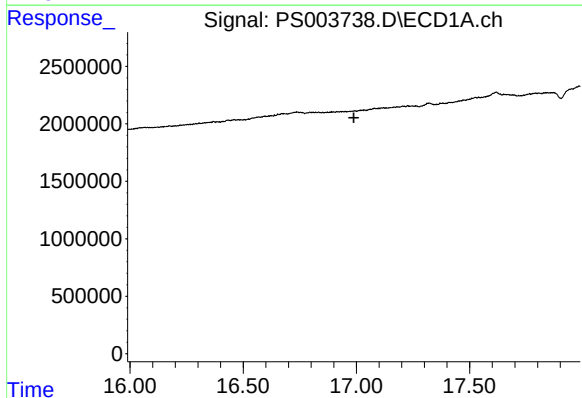


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

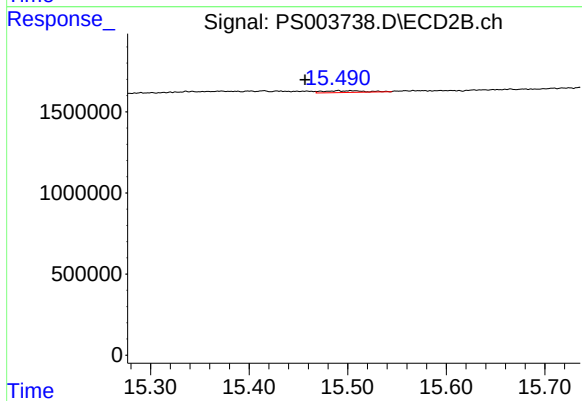

#14 DINOSEB


R.T.: 15.493 min
Delta R.T.: 0.036 min
Response: 316259
Conc: 0.18 ng/ml

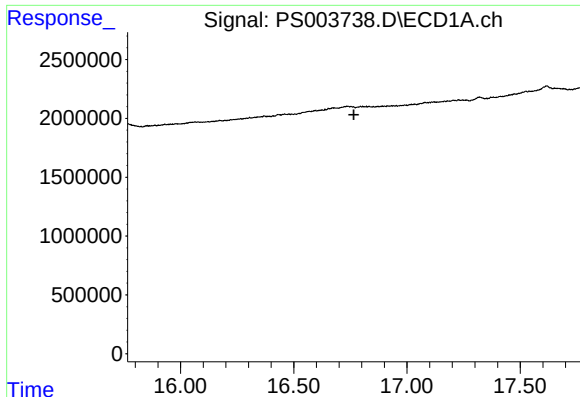

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

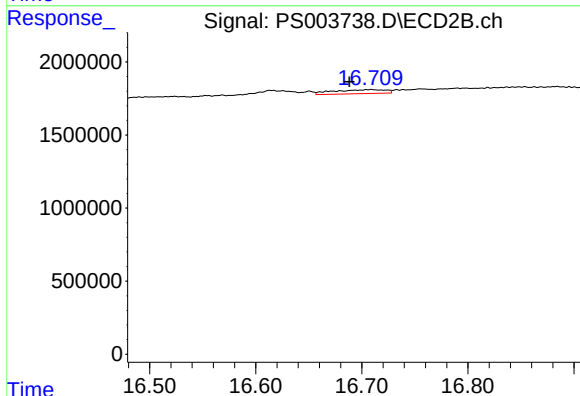


#15 Picloram

R.T.: 16.709 min
Delta R.T.: 0.020 min
Response: 916003
Conc: 0.36 ng/ml

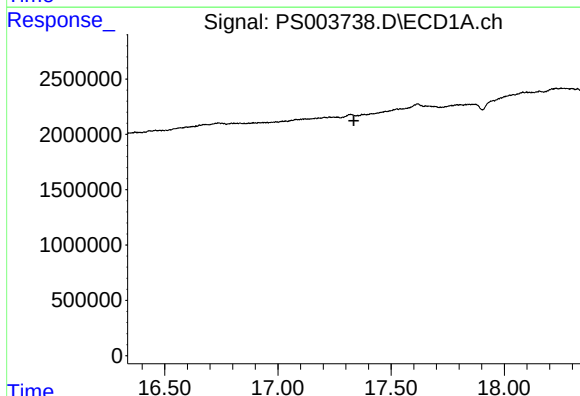

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

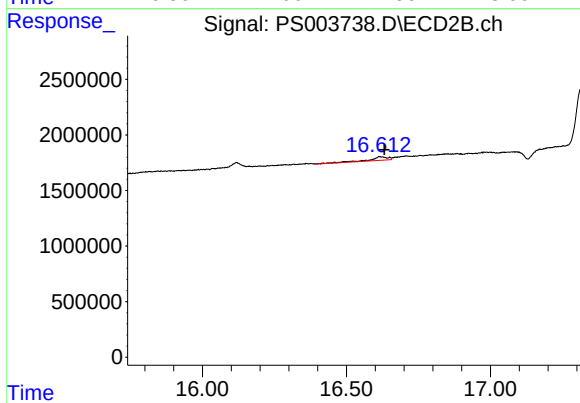

#16 DCPA

R.T.: 16.618 min
Delta R.T.: -0.014 min
Response: 1501483
Conc: 0.48 ng/ml