

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032519\
 Data File : PS003743.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 04:30
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 05:27:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.299	10.803	248.0E6	228.0E6	564.945	485.502
Target Compounds							
2) T	3,5-DICHL...	0.000	8.969	0	5189	N.D.	0.008 #
3) T	4-Nitroph...	0.000	9.950	0	43716	N.D.	0.194 #
6) T	MCP	0.000	11.350	0	77797	N.D.	0.066 #
7) T	MCPA	0.000	11.689	0	389328	N.D.	0.226 #
8) T	DICHLORPROP	0.000	12.132	0	10898591	N.D.	26.373 #
10) T	Pentachlo...	0.000	13.214	0	982412	N.D.	0.149 #
11) T	2,4,5-TP ...	0.000	13.848	0	203436	N.D.	0.080 #
13) T	2,4-DB	0.000	15.043	0	621482	N.D.	2.434 #
14) T	DINOSEB	0.000	15.477	0	849211	N.D.	0.476 #
15) T	Picloram	0.000	16.651	0	781450	N.D.	0.308 #
16) T	DCPA	0.000	16.651	0	781450	N.D.	0.251 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032519\
Data File : PS003743.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 04:30
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 05:27:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

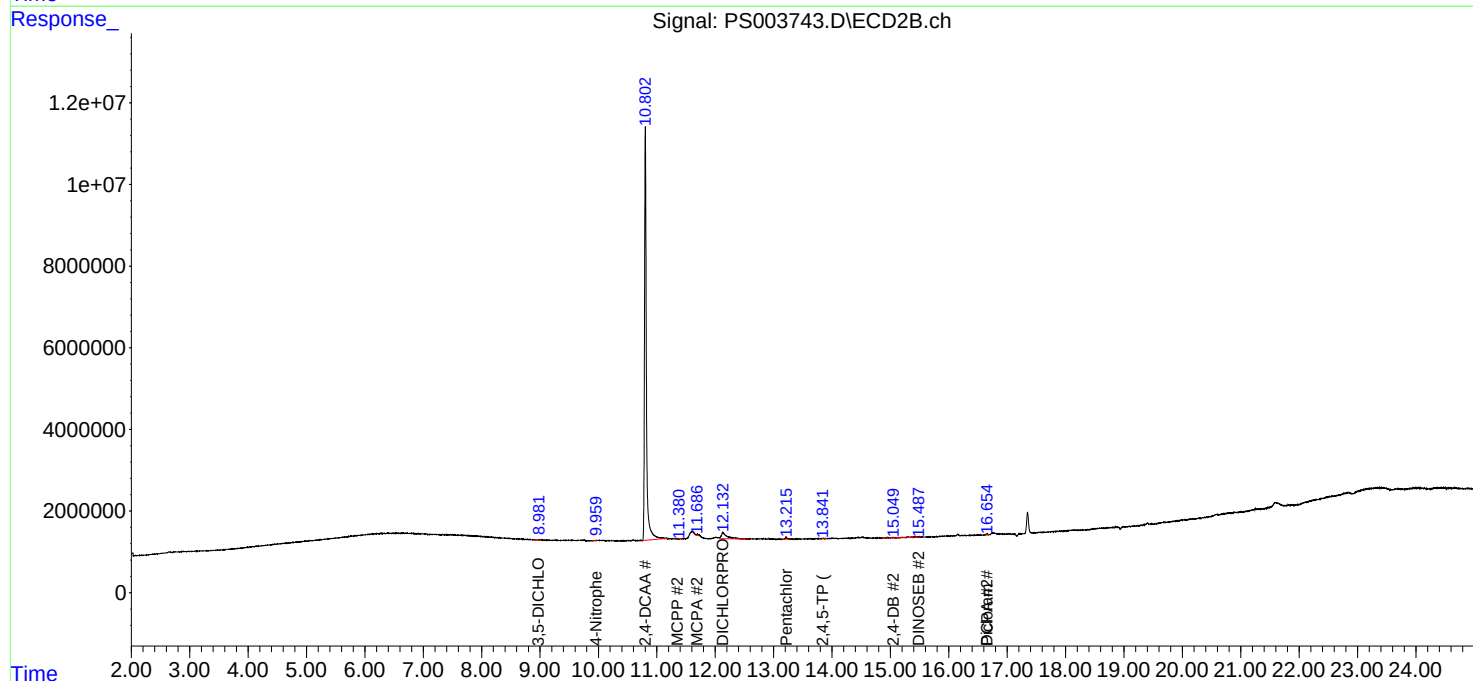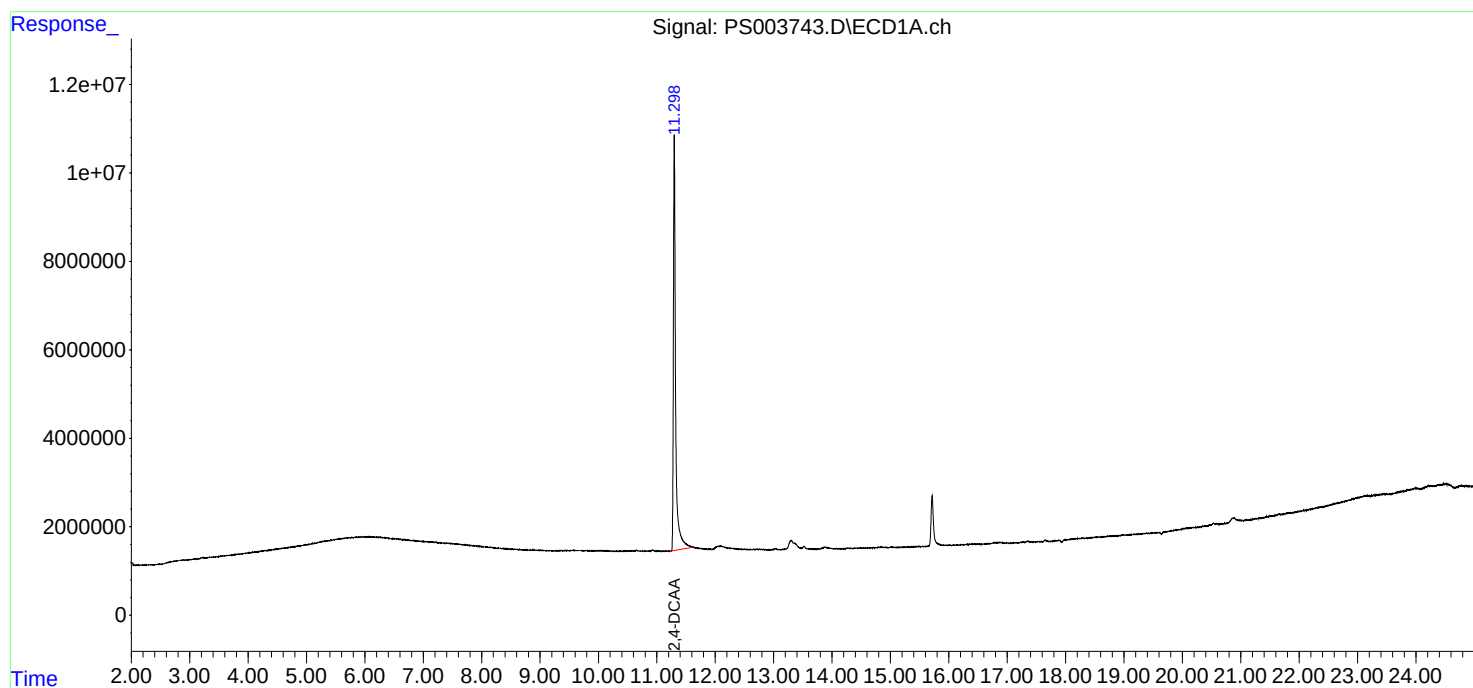


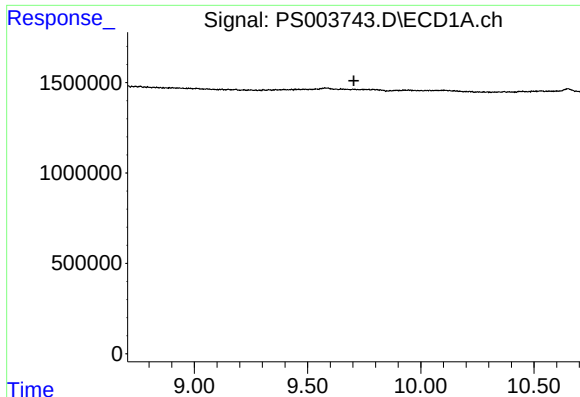

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.705 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

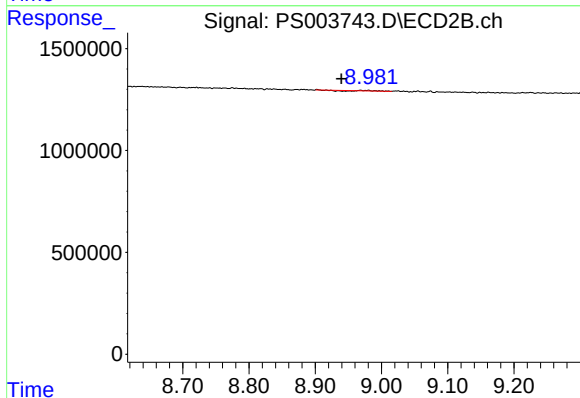


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.969 min
Delta R.T.: 0.029 min
Response: 5189
Conc: 0.01 ng/ml

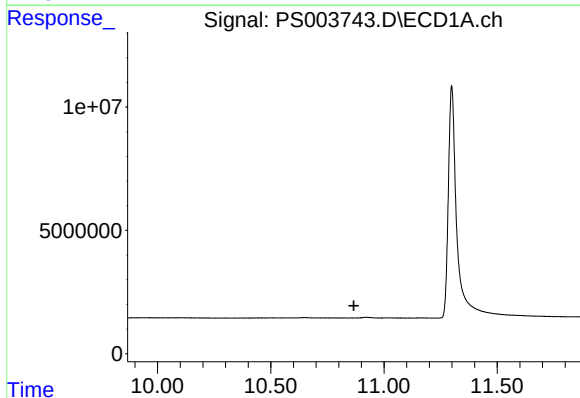


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.867 min
Response: 0
Conc: N.D.

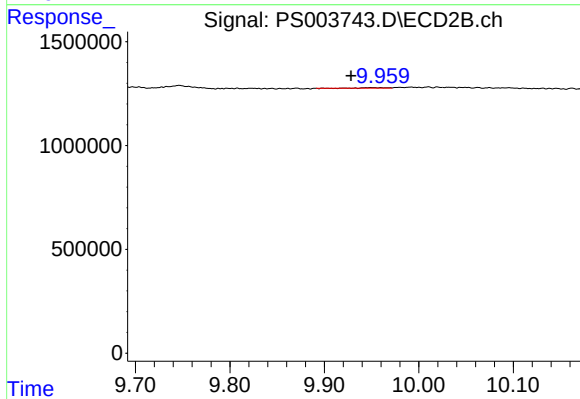

#3 4-Nitrophenol


R.T.: 9.950 min
Delta R.T.: 0.021 min
Response: 43716
Conc: 0.19 ng/ml

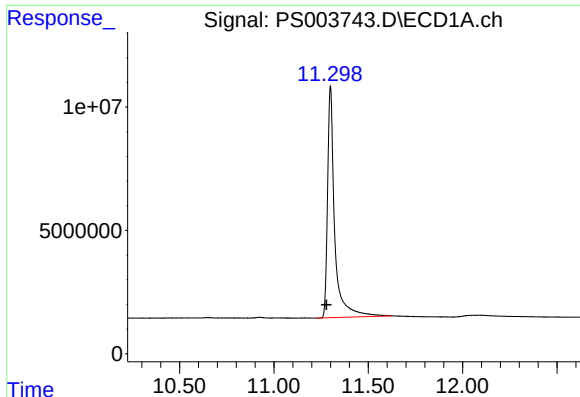

#4 2,4-DCAA


R.T.: 11.299 min
Delta R.T.: 0.021 min
Response: 248024761
Conc: 564.95 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

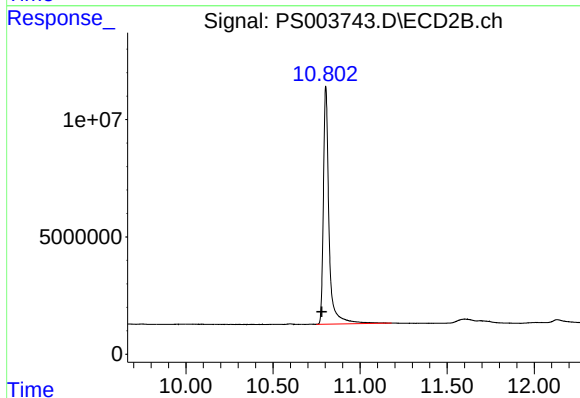


#4 2,4-DCAA

R.T.: 10.803 min
Delta R.T.: 0.024 min
Response: 227976814
Conc: 485.50 ng/ml

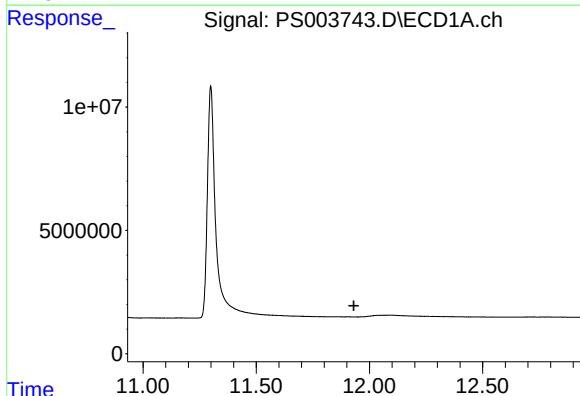


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.931 min
Response: 0
Conc: N.D.

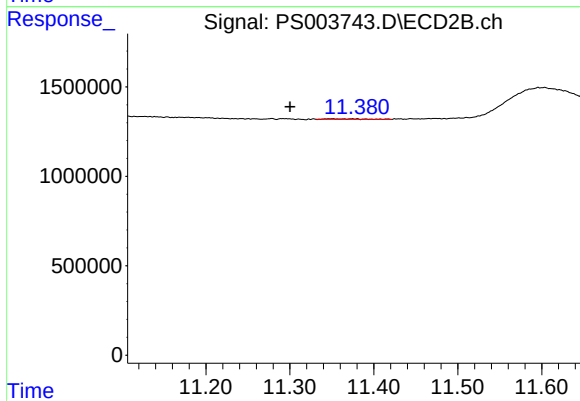

#6 MCP


R.T.: 11.350 min
Delta R.T.: 0.050 min
Response: 77797
Conc: 0.07 ug/ml

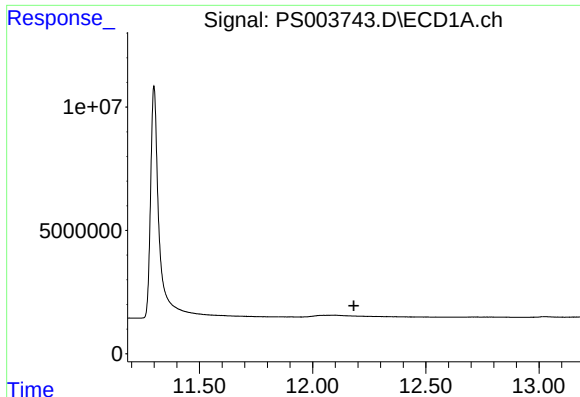

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.182 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

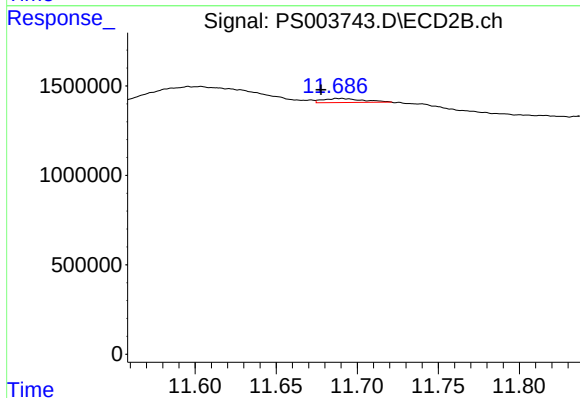


#7 MCPA

R.T.: 11.689 min
Delta R.T.: 0.012 min
Response: 389328
Conc: 0.23 ug/ml

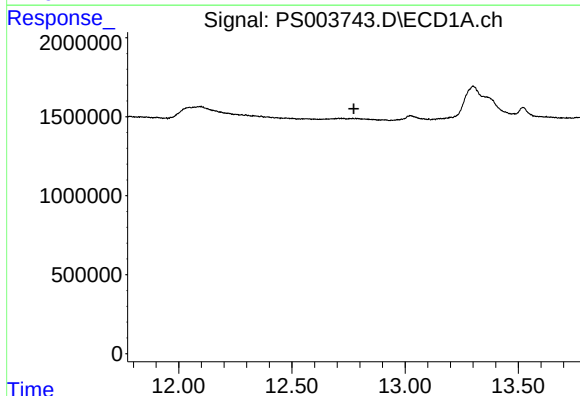


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 12.773 min
Response: 0
Conc: N.D.

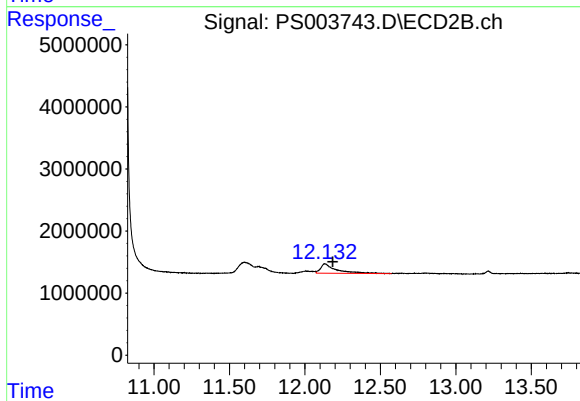

#8 DICHLORPROP


R.T.: 12.132 min
Delta R.T.: -0.053 min
Response: 10898591
Conc: 26.37 ng/ml

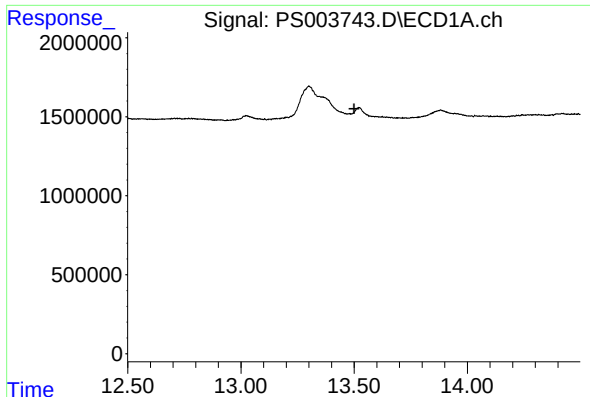

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.499 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

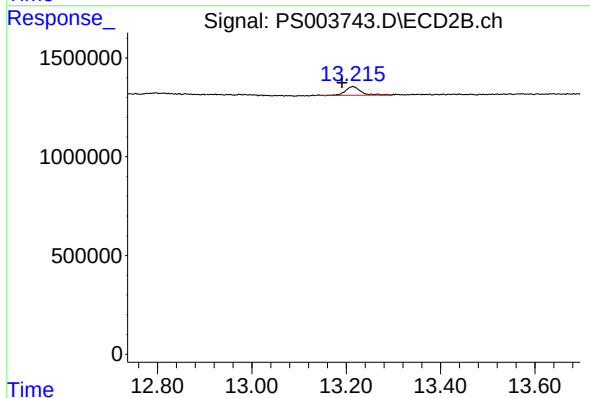


#10 Pentachlorophenol

R.T.: 13.214 min
Delta R.T.: 0.023 min
Response: 982412
Conc: 0.15 ng/ml

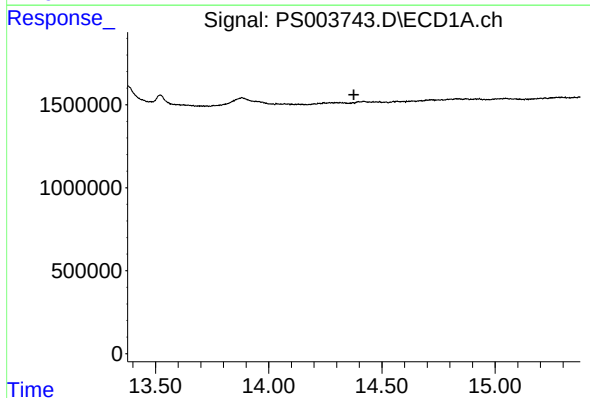


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.376 min
Response: 0
Conc: N.D.

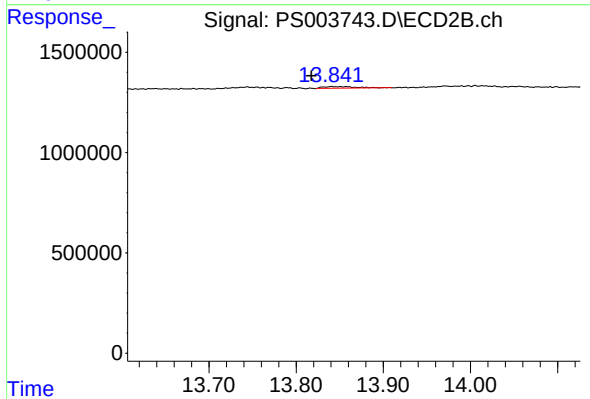

#11 2,4,5-TP (SILVEX)


R.T.: 13.848 min
Delta R.T.: 0.030 min
Response: 203436
Conc: 0.08 ng/ml

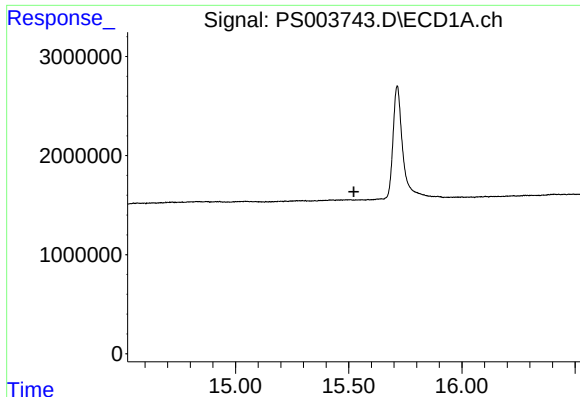

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.523 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

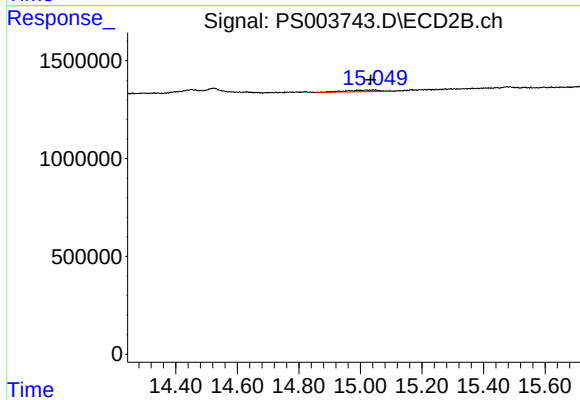


#13 2,4-DB

R.T.: 15.043 min
Delta R.T.: 0.010 min
Response: 621482
Conc: 2.43 ng/ml

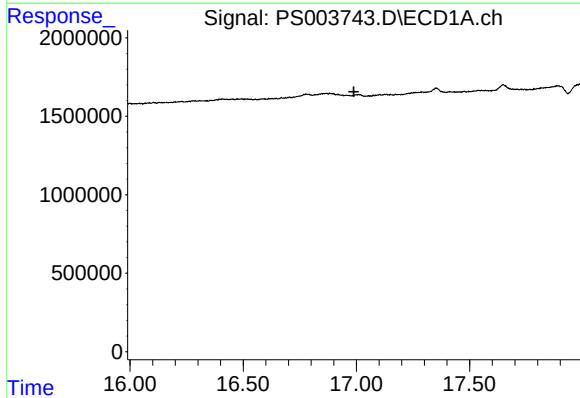


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.989 min
Response: 0
Conc: N.D.

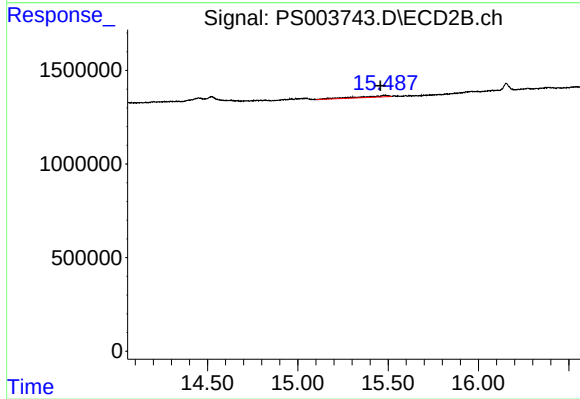

#14 DINOSEB


R.T.: 15.477 min
Delta R.T.: 0.021 min
Response: 849211
Conc: 0.48 ng/ml

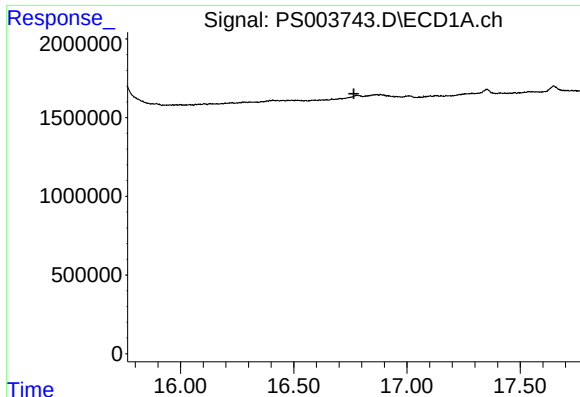

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.765 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

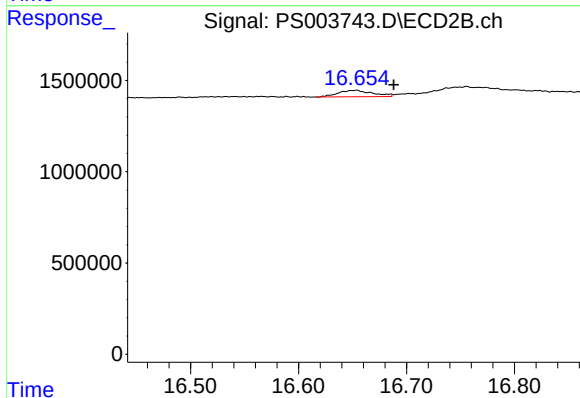


#15 Picloram

R.T.: 16.651 min
Delta R.T.: -0.037 min
Response: 781450
Conc: 0.31 ng/ml

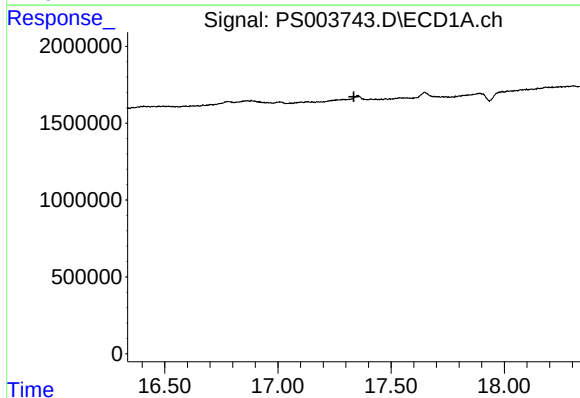

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.335 min
Response: 0
Conc: N.D.

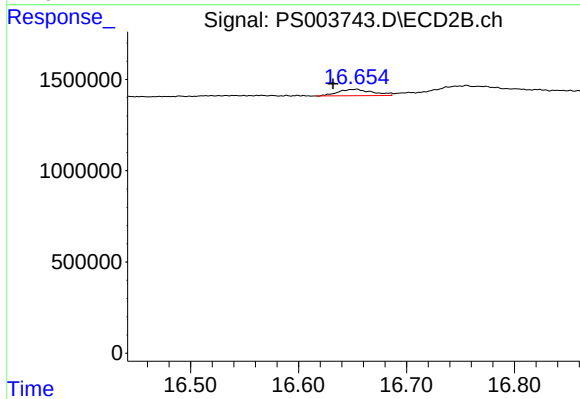

#16 DCPA

R.T.: 16.651 min
Delta R.T.: 0.019 min
Response: 781450
Conc: 0.25 ng/ml