

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032519\
 Data File : PS003737.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 01:23
 Operator : EI\SJ
 Sample : K2004-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SB-23(4-5)

Manual Integrations
 APPROVED

Sohil
 3/26/2019 1:43:58 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 05:17:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
 Quant Title : 8080.M
 QLast Update : Thu Feb 28 03:00:19 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	11.262	10.768	213.7E6	196.9E6	486.842m	419.389

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032519\
Data File : PS003737.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 01:23
Operator : EI\SJ
Sample : K2004-12
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SB-23(4-5)


Manual Integrations
APPROVED

Sohil
3/26/2019 1:43:58 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 05:17:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS022719.M
Quant Title : 8080.M
QLast Update : Thu Feb 28 03:00:19 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

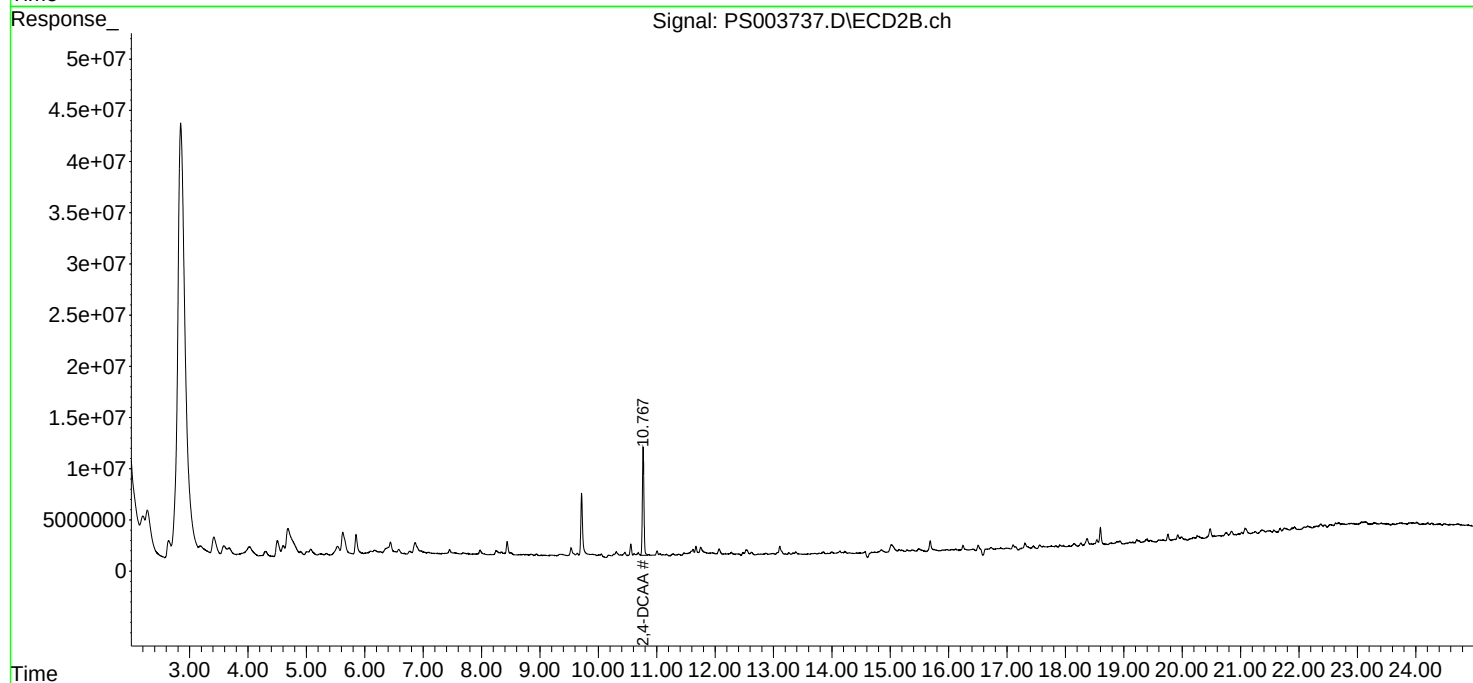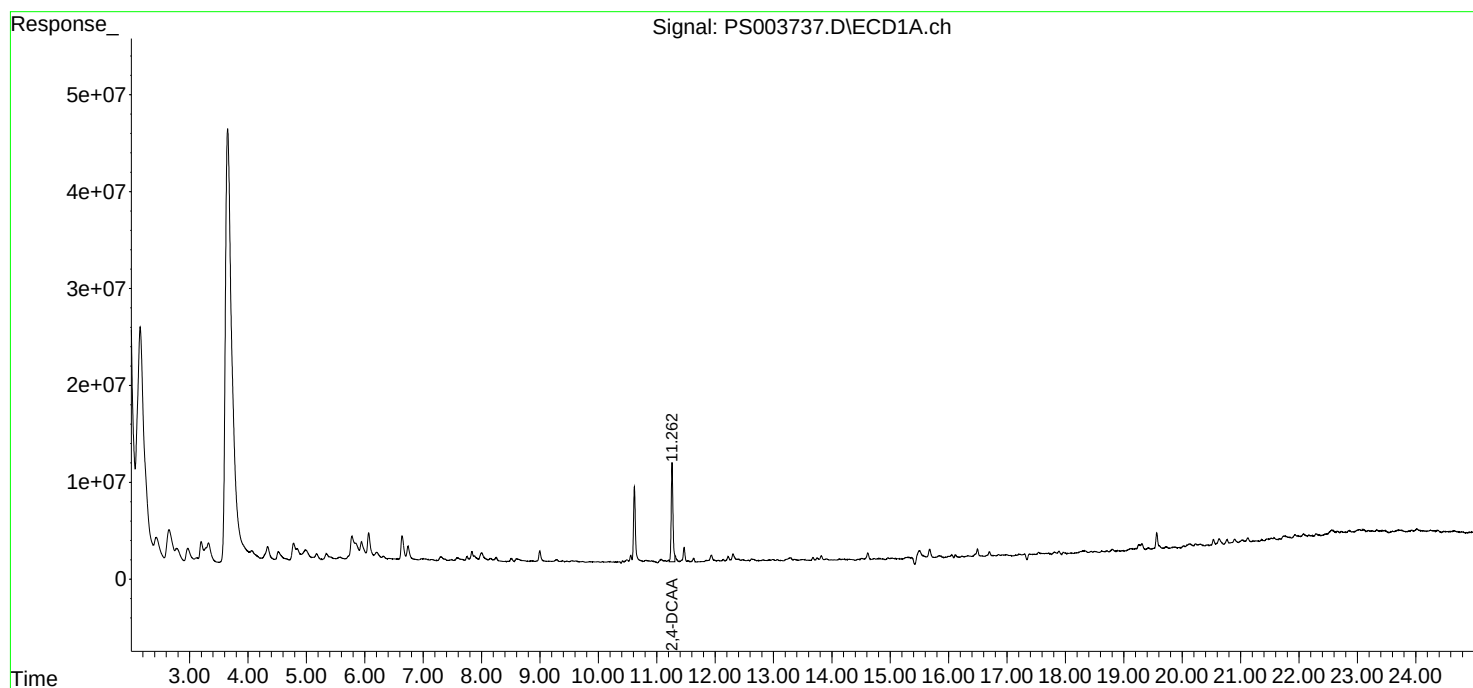

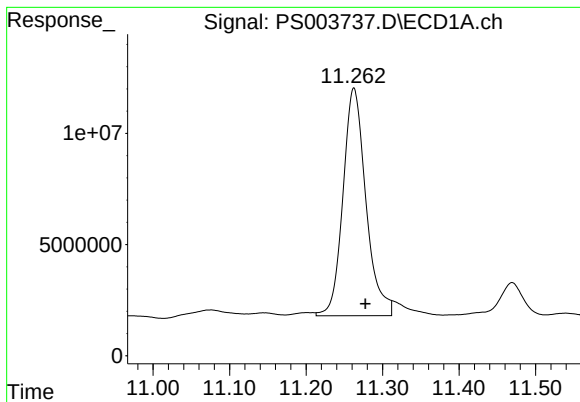


#4 2,4-DCAA

R.T.: 11.262 min
Delta R.T.: -0.016 min
Response: 213735420
Conc: 486.84 ng/ml m

Instrument :
ECD_S
ClientSampleId :
SB-23(4-5)

Manual Integrations
APPROVED

Sohil
3/26/2019 1:43:58 PM

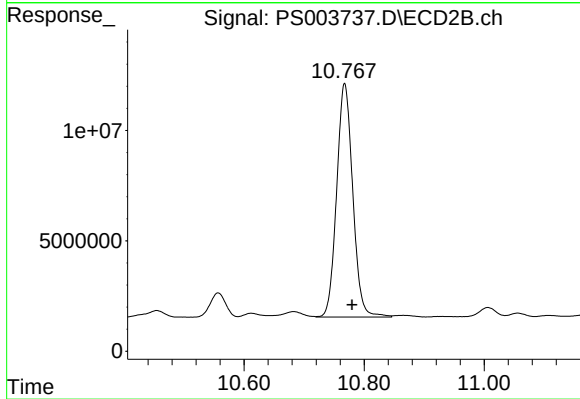

#4 2,4-DCAA

R.T.: 10.768 min
Delta R.T.: -0.012 min
Response: 196932031
Conc: 419.39 ng/ml