

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032522\
 Data File : PS018759.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2022 09:28
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 22:01:07 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.229	6.810	1277.7E6	370.8E6	448.953	527.026
Target Compounds							
5) T	DICAMBA	7.420	0.000	4782068	0	<MDL	N.D. #
8) T	DICHLORPROP	0.000	7.620	0	19213922	N.D.	24.272
9) T	2,4-D	8.350	7.895	7113620	2406666	2.123	2.571
10) T	Pentachlo...	8.656	8.321	6086294	1628073	<MDL	<MDL #
11) T	2,4,5-TP ...	9.210	8.681	7500934	1746823	<MDL	<MDL #
12) T	2,4,5-T	9.493	9.061	38807723	7298528	2.598	1.762 #
13) T	2,4-DB	10.047	0.000	13330153	0	4.873	N.D. #
14) T	DINOSEB	11.210	9.896	3558526	2550546	<MDL	<MDL #
15) T	Picloram	11.032	10.878	523.9E6	139.3E6	25.487	26.212
16) T	DCPA	11.476	10.827	11706189	1871112	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032522\
Data File : PS018759.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2022 09:28
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 22:01:07 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

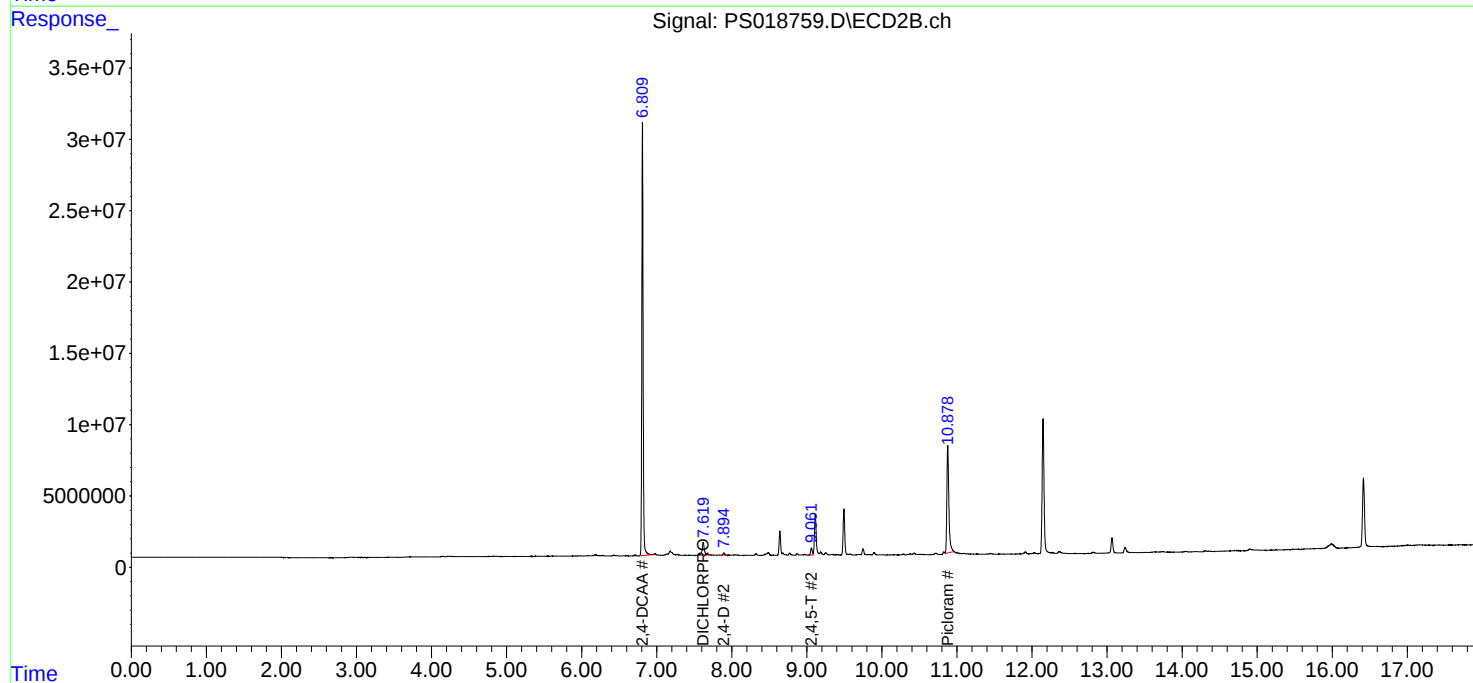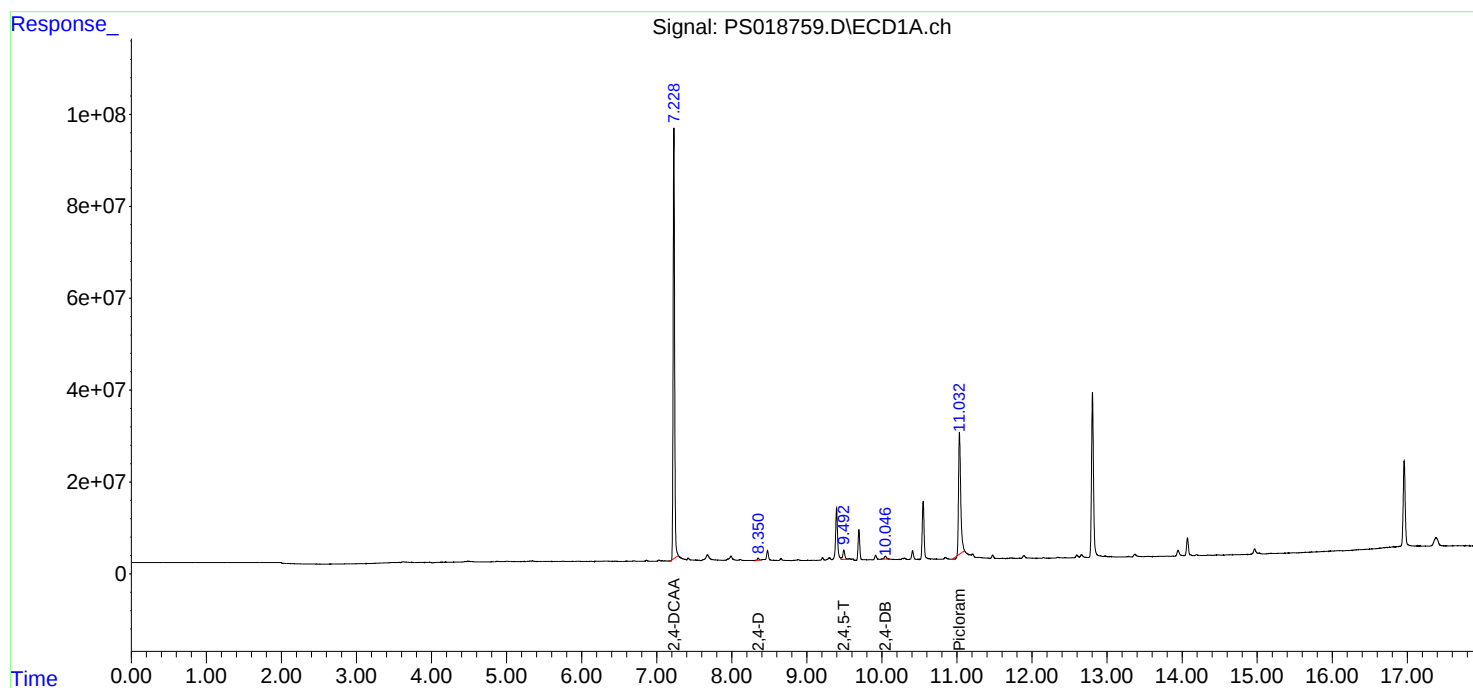


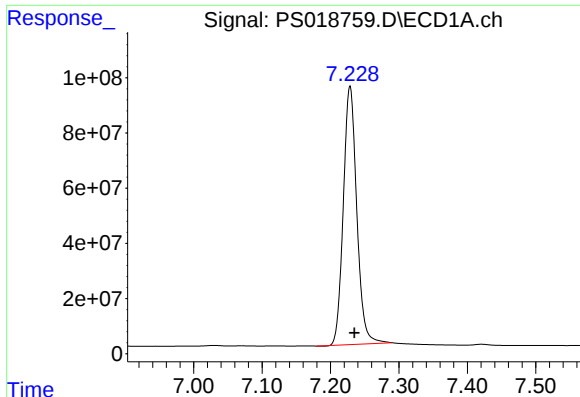

#4 2,4-DCAA


R.T.: 7.229 min
Delta R.T.: -0.006 min
Response: 1277683388
Conc: 448.95 ng/ml

Instrument :
ECD_S
ClientSampleId :

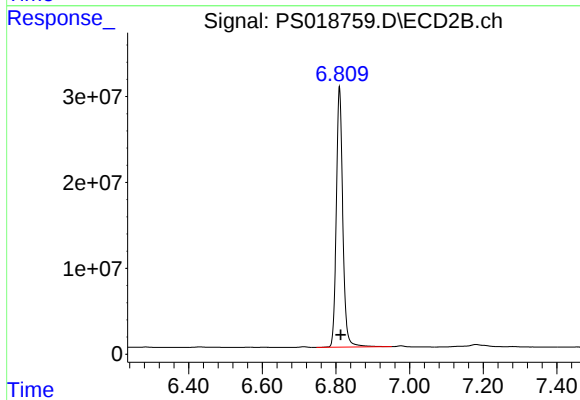


#4 2,4-DCAA

R.T.: 6.810 min
Delta R.T.: -0.003 min
Response: 370844807
Conc: 527.03 ng/ml

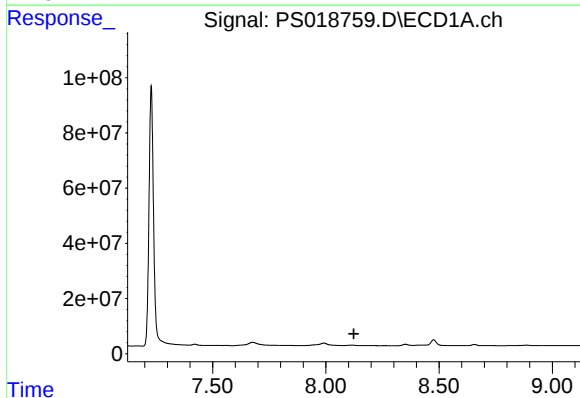


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.124 min
Response: 0
Conc: N.D.

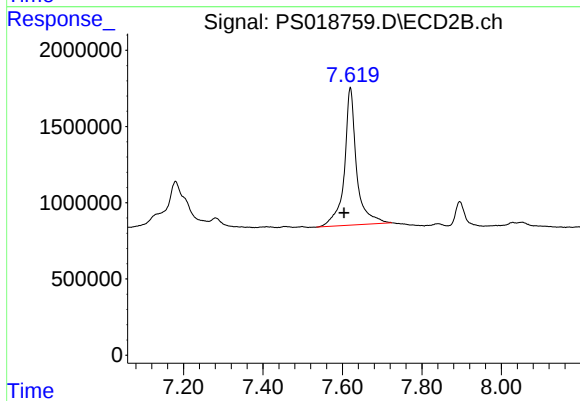

#8 DICHLORPROP


R.T.: 7.620 min
Delta R.T.: 0.016 min
Response: 19213922
Conc: 24.27 ng/ml

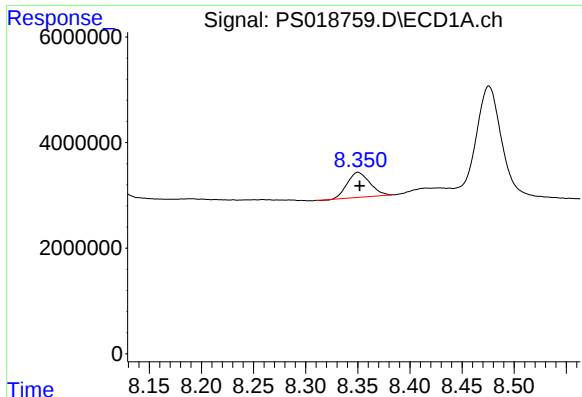

#9 2,4-D


R.T.: 8.350 min
Delta R.T.: -0.002 min
Response: 7113620
Conc: 2.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

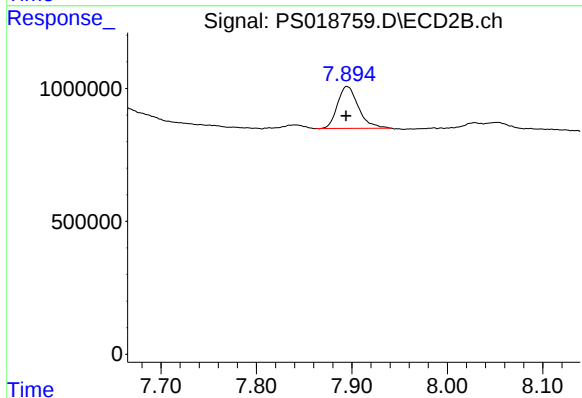


#9 2,4-D

R.T.: 7.895 min
Delta R.T.: 0.001 min
Response: 2406666
Conc: 2.57 ng/ml

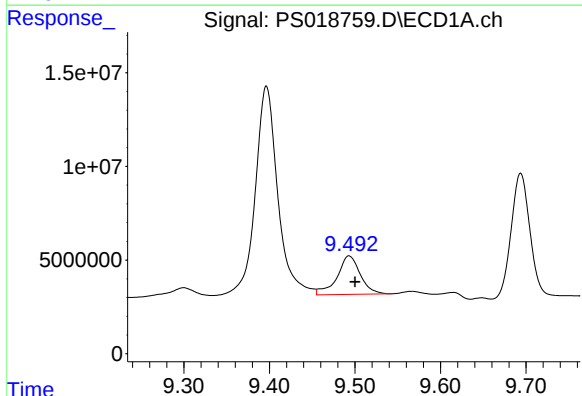


#12 2,4,5-T

R.T.: 9.493 min
Delta R.T.: -0.007 min
Response: 38807723
Conc: 2.60 ng/ml

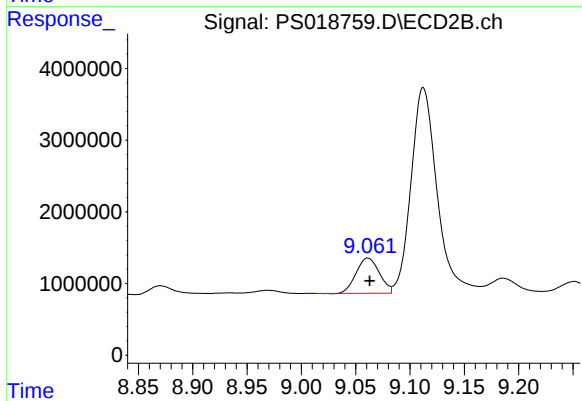

#12 2,4,5-T


R.T.: 9.061 min
Delta R.T.: -0.002 min
Response: 7298528
Conc: 1.76 ng/ml

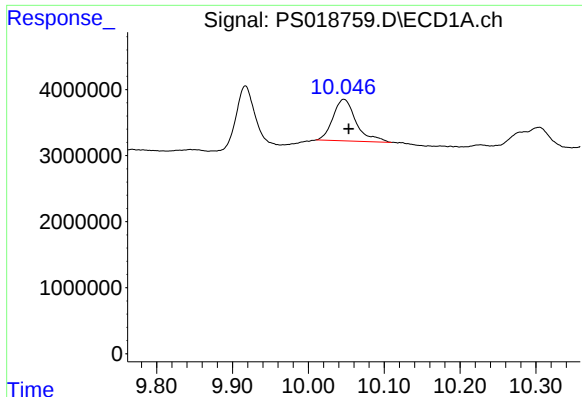

#13 2,4-DB


R.T.: 10.047 min
Delta R.T.: -0.006 min
Response: 13330153
Conc: 4.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

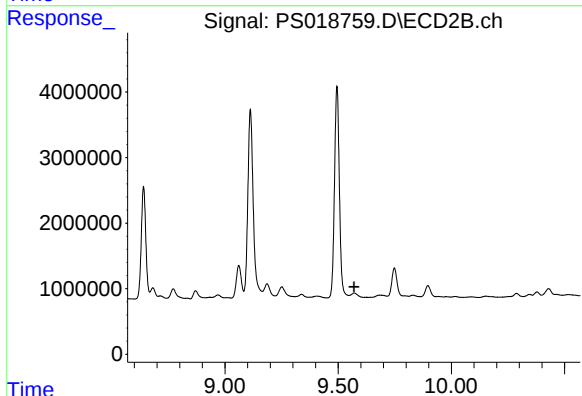


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.570 min
Response: 0
Conc: N.D.

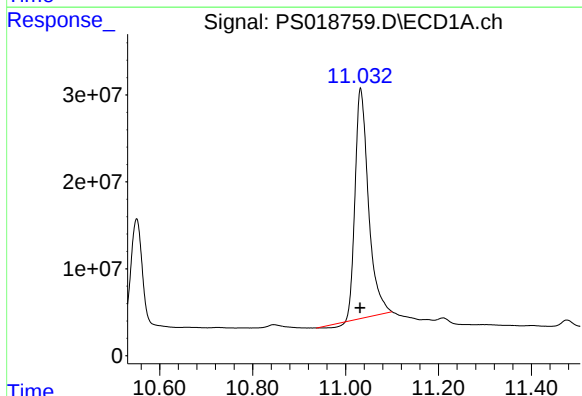

#15 Picloram

R.T.: 11.032 min
Delta R.T.: 0.001 min
Response: 523903051
Conc: 25.49 ng/ml

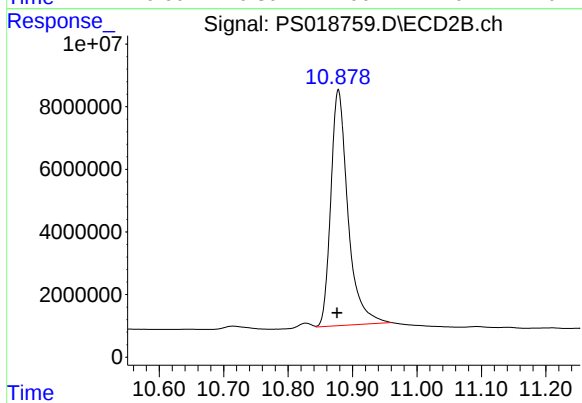

#15 Picloram

R.T.: 10.878 min
Delta R.T.: 0.002 min
Response: 139343809
Conc: 26.21 ng/ml