

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032522\
 Data File : PS018764.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2022 15:52
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 22:02:27 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.232	6.809	1340.9E6	374.4E6	471.169	532.067
Target Compounds							
8) T	DICHLORPROP	0.000	7.620	0	57471872	N.D.	72.601
9) T	2,4-D	8.352	0.000	7647845	0	2.283	N.D. #
10) T	Pentachlo...	8.733f	0.000	1943145	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.217	8.680	12696549	3782997	<MDL	<MDL #
12) T	2,4,5-T	9.500	9.061	24431727	24826330	1.635	5.994 #
13) T	2,4-DB	10.038	0.000	8814479	0	3.222	N.D. #
14) T	DINOSEB	11.183	9.900	11648457	1187133	1.089	<MDL #
15) T	Picloram	11.034	10.878	346.0E6	83761596	16.832	15.756
16) T	DCPA	11.495	10.830	180.6E6	2836049	10.093	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032522\
Data File : PS018764.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2022 15:52
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 22:02:27 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

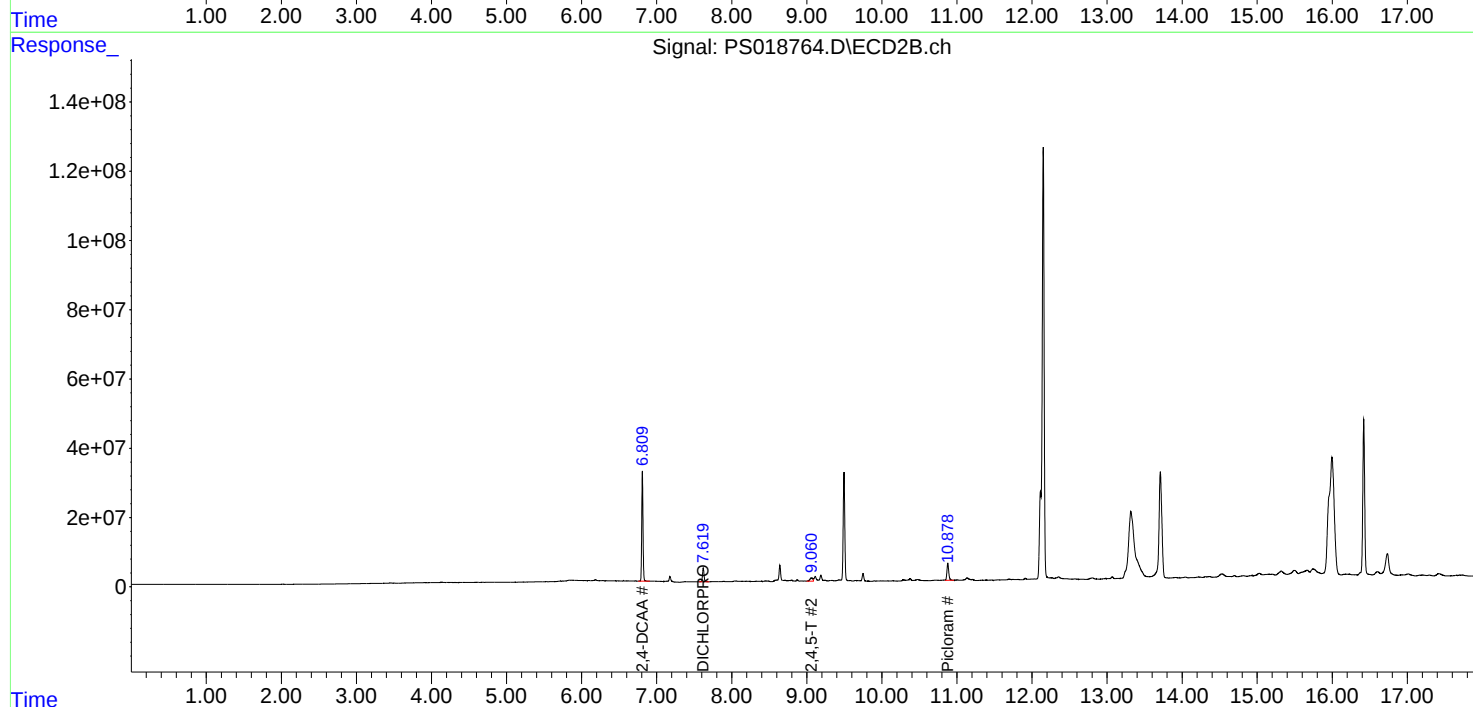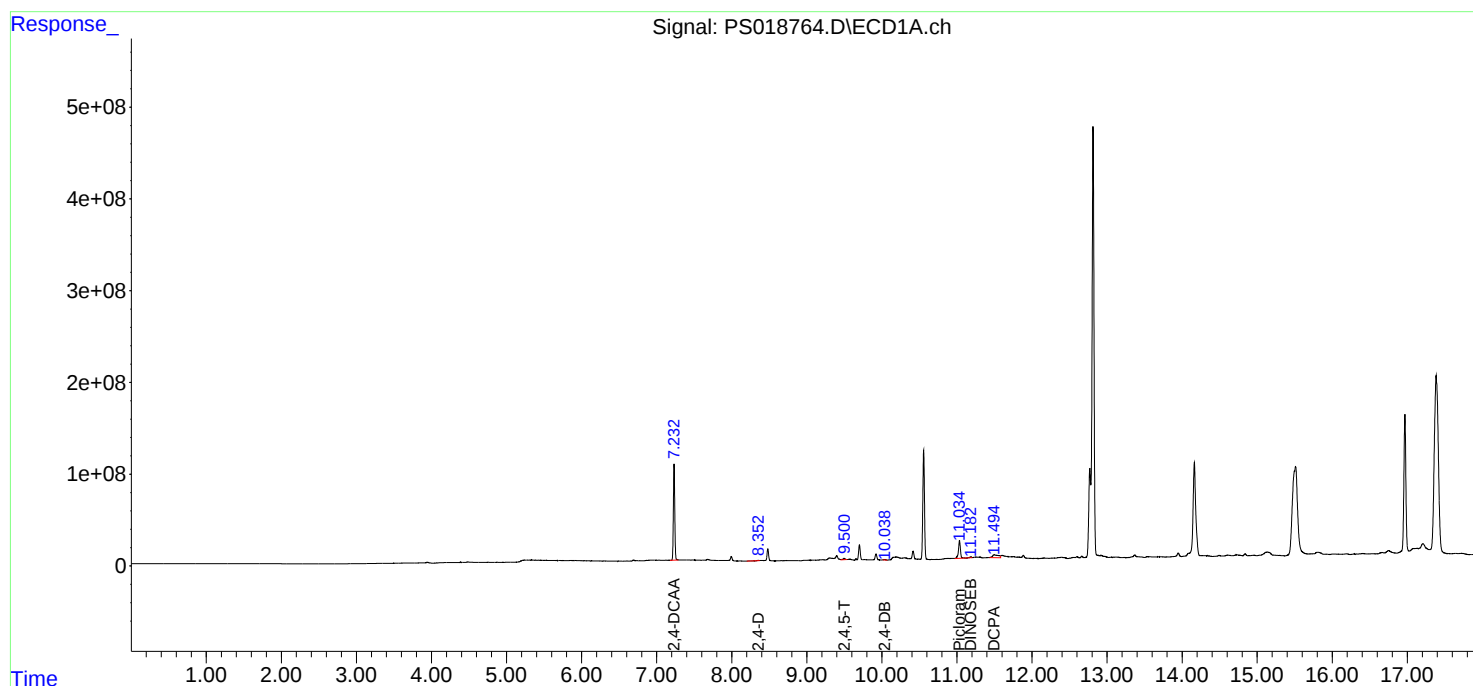


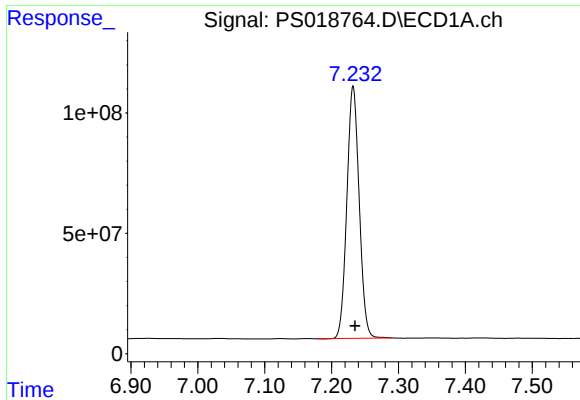

#4 2,4-DCAA


R.T.: 7.232 min
Delta R.T.: -0.003 min
Response: 1340908120
Conc: 471.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

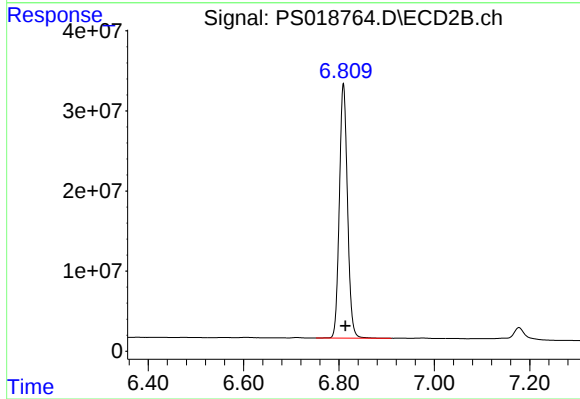


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.004 min
Response: 374391831
Conc: 532.07 ng/ml

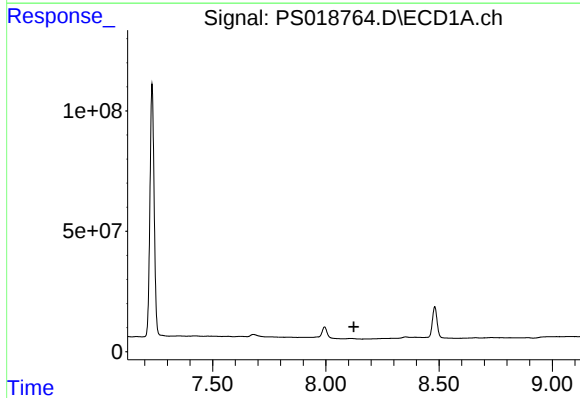


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.124 min
Response: 0
Conc: N.D.

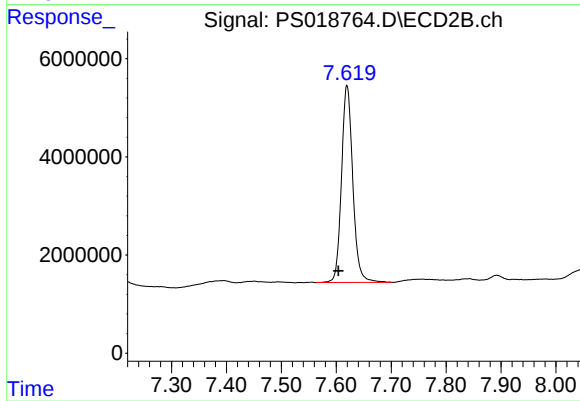

#8 DICHLORPROP


R.T.: 7.620 min
Delta R.T.: 0.016 min
Response: 57471872
Conc: 72.60 ng/ml

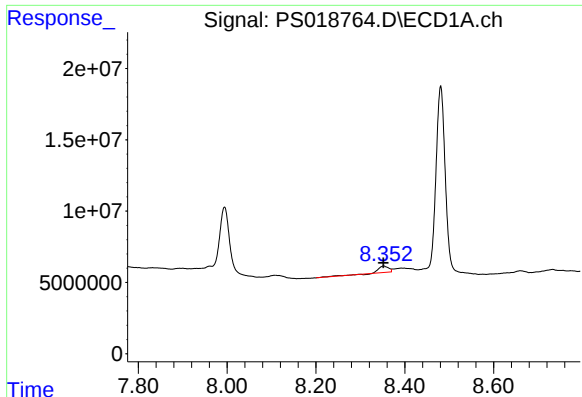

#9 2,4-D


R.T.: 8.352 min
Delta R.T.: 0.000 min
Response: 7647845
Conc: 2.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

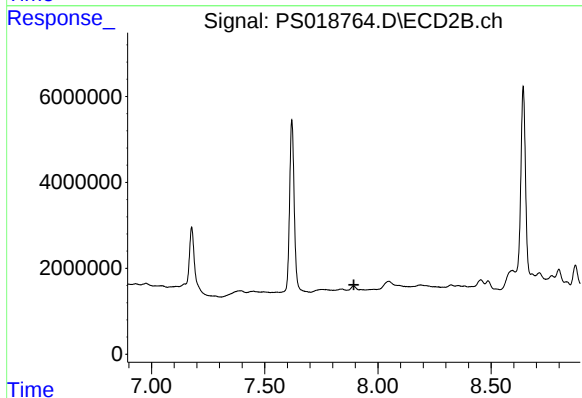


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.894 min
Response: 0
Conc: N.D.

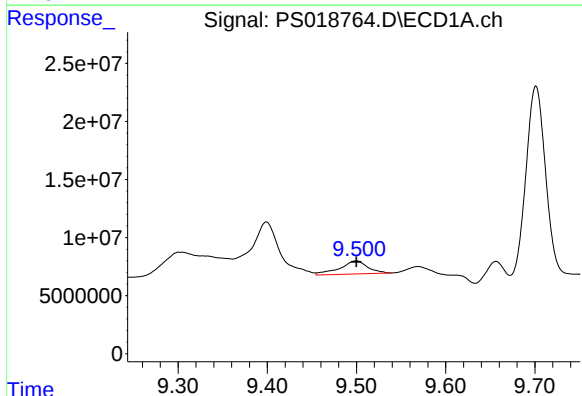


#12 2,4,5-T

R.T.: 9.500 min
Delta R.T.: 0.000 min
Response: 24431727
Conc: 1.64 ng/ml

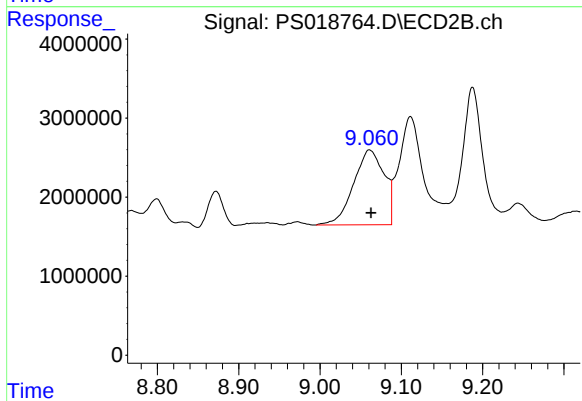

#12 2,4,5-T


R.T.: 9.061 min
Delta R.T.: -0.002 min
Response: 24826330
Conc: 5.99 ng/ml

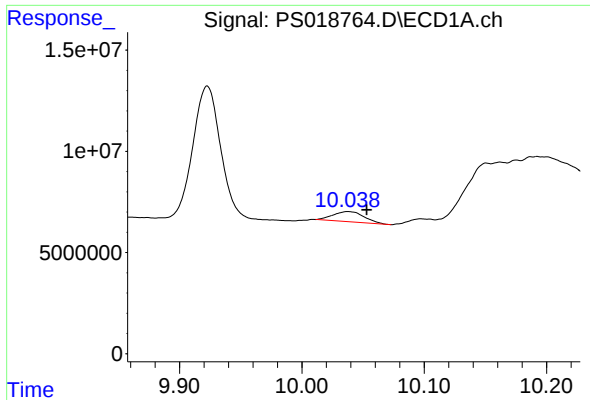

#13 2,4-DB


R.T.: 10.038 min
Delta R.T.: -0.015 min
Response: 8814479
Conc: 3.22 ng/ml

Instrument :
ECD_S
ClientSampleId :

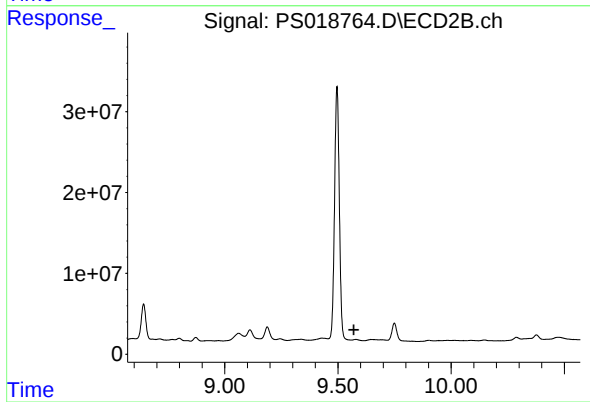


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 9.570 min
Response: 0
Conc: N.D.

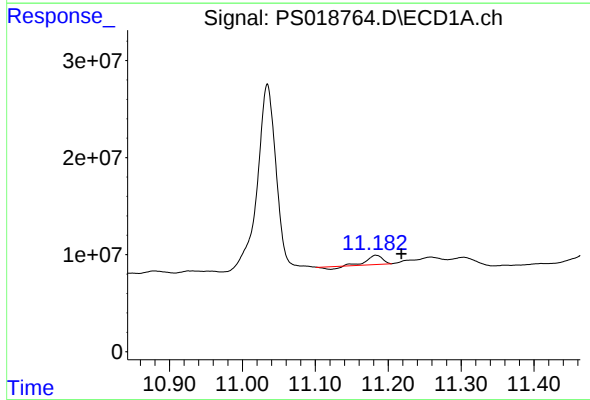


#14 DINOSEB

R.T.: 11.183 min
Delta R.T.: -0.035 min
Response: 11648457
Conc: 1.09 ng/ml

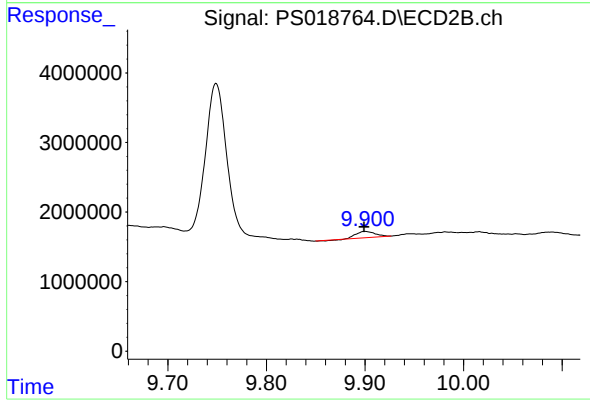

#14 DINOSEB


R.T.: 9.900 min
Delta R.T.: 0.001 min
Response: 1187133
Conc: N.D.

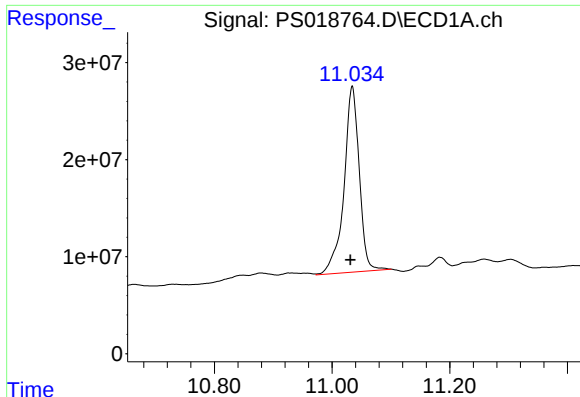

#15 Picloram


R.T.: 11.034 min
Delta R.T.: 0.003 min
Response: 345988304
Conc: 16.83 ng/ml

Instrument :
ECD_S
ClientSampleId :

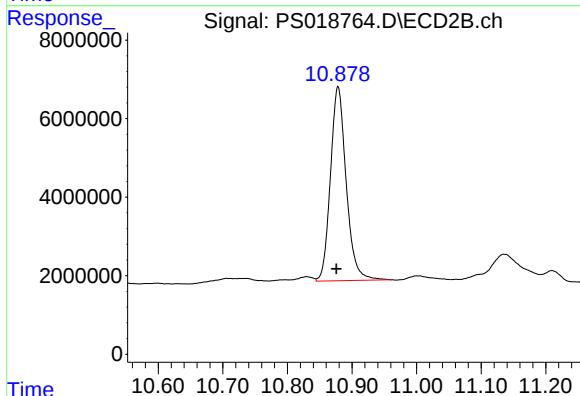


#15 Picloram

R.T.: 10.878 min
Delta R.T.: 0.002 min
Response: 83761596
Conc: 15.76 ng/ml

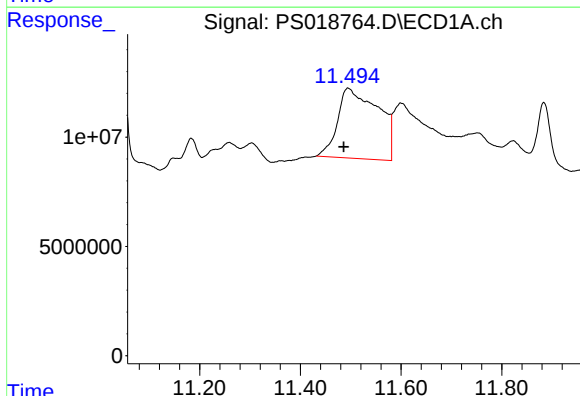

#16 DCPA

R.T.: 11.495 min
Delta R.T.: 0.009 min
Response: 180574084
Conc: 10.09 ng/ml

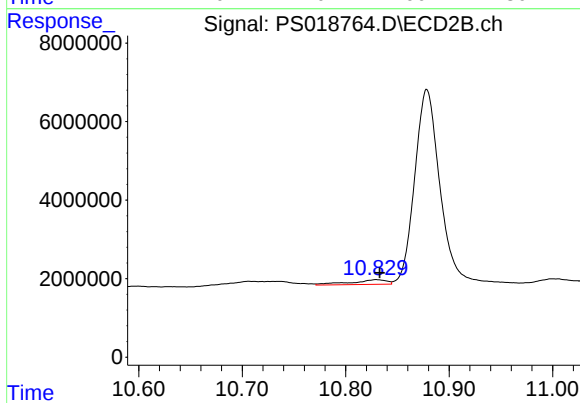

#16 DCPA

R.T.: 10.830 min
Delta R.T.: -0.003 min
Response: 2836049
Conc: N.D.