

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032522\
 Data File : PS018776.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 25 Mar 2022 20:40
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 25 22:05:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.809	1379.1E6	388.5E6	484.586	552.141
Target Compounds							
5) T	DICAMBA	7.475f	0.000	5617020	0	<MDL	N.D. #
8) T	DICHLORPROP	8.103	7.619	3271001	53847402	1.188	68.022 #
11) T	2,4,5-TP ...	9.270f	8.708	62391420	4964572	4.102	1.138 #
12) T	2,4,5-T	9.491	9.062	8427271	2605164	<MDL	<MDL #
13) T	2,4-DB	0.000	9.576	0	1374895	N.D.	2.422
14) T	DINOSEB	11.175f	0.000	8307582	0	<MDL	N.D. #
15) T	Picloram	11.028	10.876	85320032	26547080	4.151	4.994
16) T	DCPA	0.000	10.829	0	2482489	N.D.	<MDL



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032522\
Data File : PS018776.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 25 Mar 2022 20:40
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 25 22:05:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

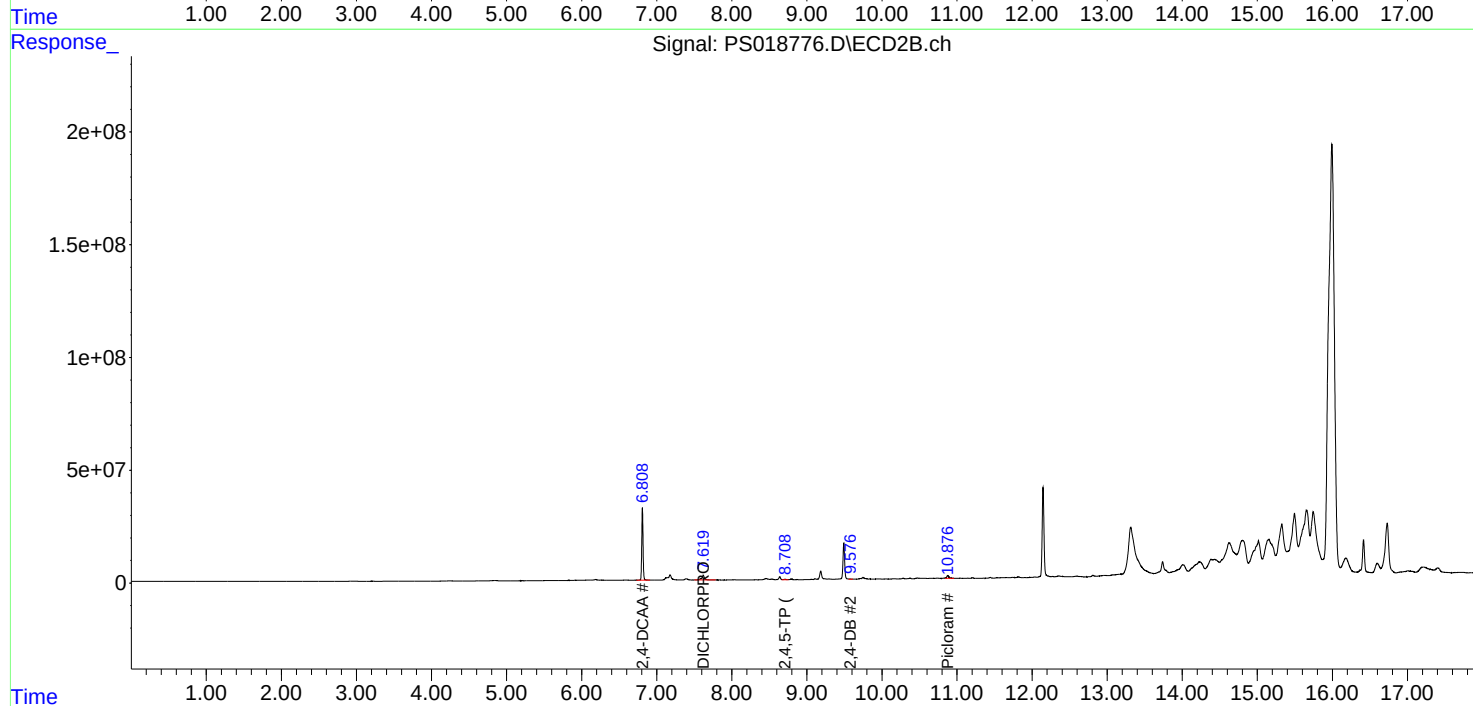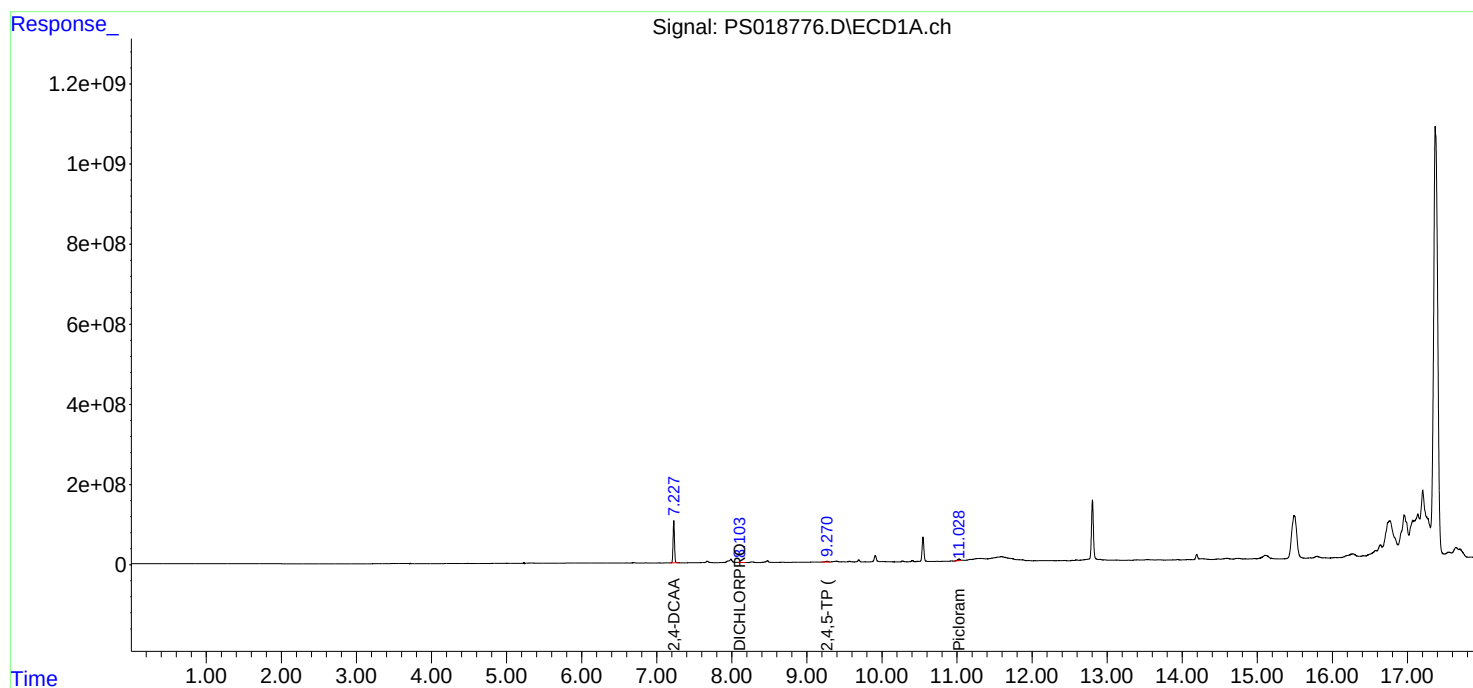


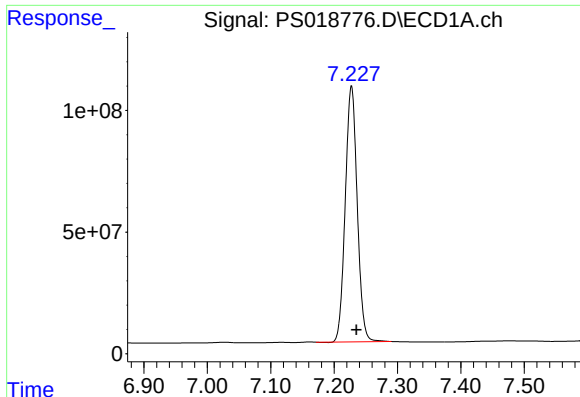

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: -0.008 min
Response: 1379090480
Conc: 484.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

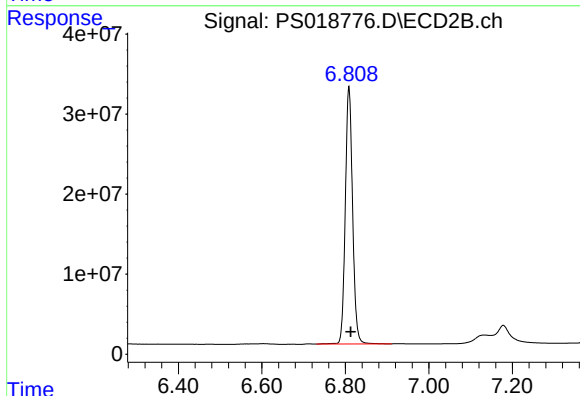


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.004 min
Response: 388517147
Conc: 552.14 ng/ml

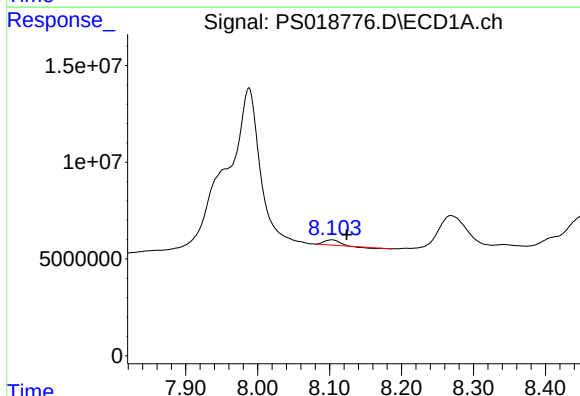


#8 DICHLORPROP

R.T.: 8.103 min
Delta R.T.: -0.021 min
Response: 3271001
Conc: 1.19 ng/ml

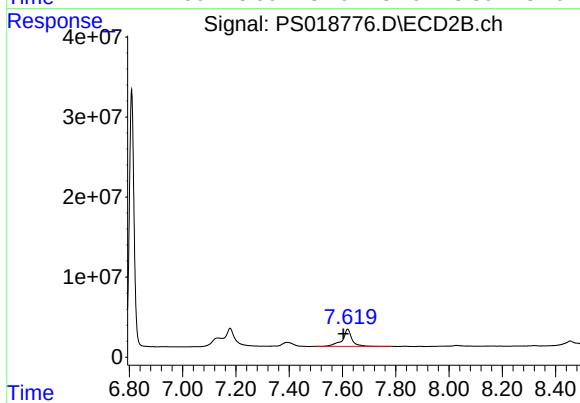

#8 DICHLORPROP


R.T.: 7.619 min
Delta R.T.: 0.015 min
Response: 53847402
Conc: 68.02 ng/ml

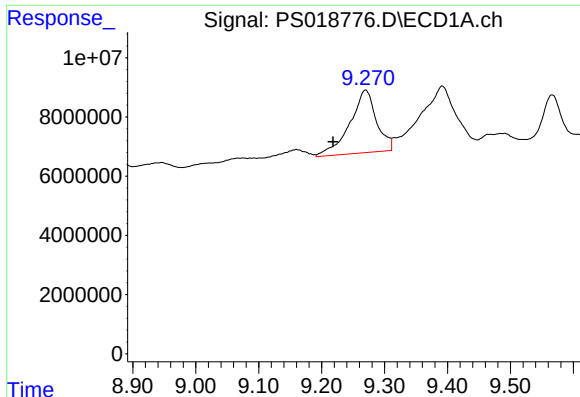

#11 2,4,5-TP (SILVEX)


R.T.: 9.270 min
Delta R.T.: 0.052 min
Response: 62391420
Conc: 4.10 ng/ml

Instrument :
ECD_S
ClientSampleId :

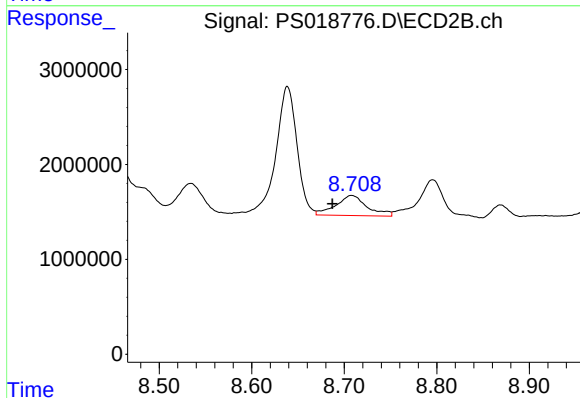


#11 2,4,5-TP (SILVEX)

R.T.: 8.708 min
Delta R.T.: 0.021 min
Response: 4964572
Conc: 1.14 ng/ml

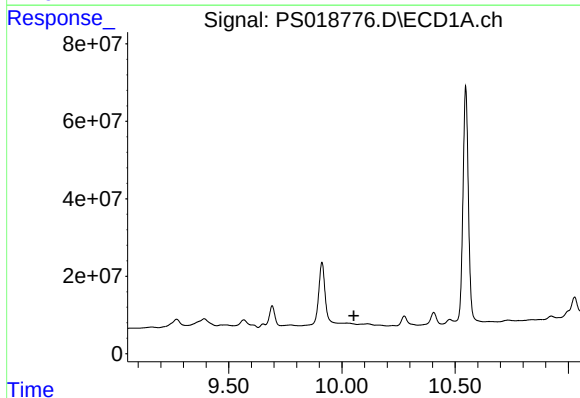


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.053 min
Response: 0
Conc: N.D.

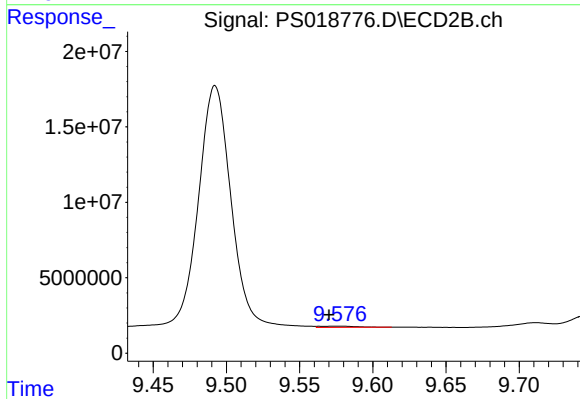

#13 2,4-DB


R.T.: 9.576 min
Delta R.T.: 0.006 min
Response: 1374895
Conc: 2.42 ng/ml

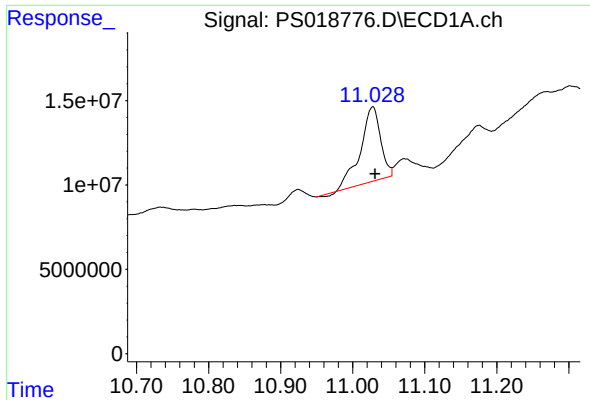

#15 Picloram

R.T.: 11.028 min
Delta R.T.: -0.003 min
Response: 85320032
Conc: 4.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

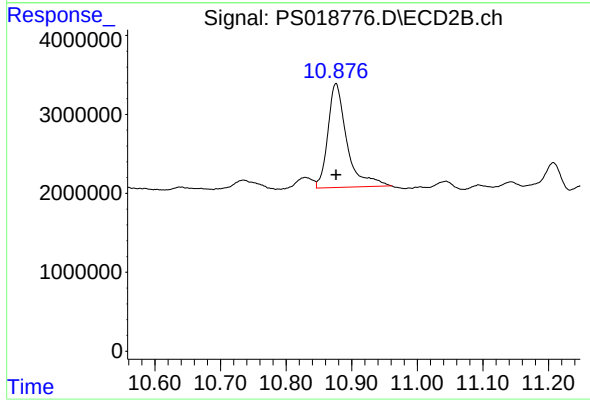

#15 Picloram

R.T.: 10.876 min
Delta R.T.: 0.000 min
Response: 26547080
Conc: 4.99 ng/ml