

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032522\
 Data File : PS018786.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2022 04:13
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 05:41:18 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
 Quant Title : 8080.M
 QLast Update : Mon Mar 14 11:41:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.227	6.809	1389.6E6	394.0E6	488.277	559.990
Target Compounds							
8) T	DICHLORPROP	0.000	7.619	0	39461800	N.D.	49.850
9) T	2,4-D	8.344	0.000	1444517	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.271f	8.709	63494923	2620718	4.175	<MDL #
12) T	2,4,5-T	9.486	9.061	7241252	3579059	<MDL	<MDL #
14) T	DINOSEB	11.261f	0.000	25116632	0	2.349	N.D. #
15) T	Picloram	11.029	10.879	68429997	23189561	3.329	4.362 #
16) T	DCPA	11.554f	10.829	209.1E6	2280013	11.688	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032522\
Data File : PS018786.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2022 04:13
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 05:41:18 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031422.M
Quant Title : 8080.M
QLast Update : Mon Mar 14 11:41:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

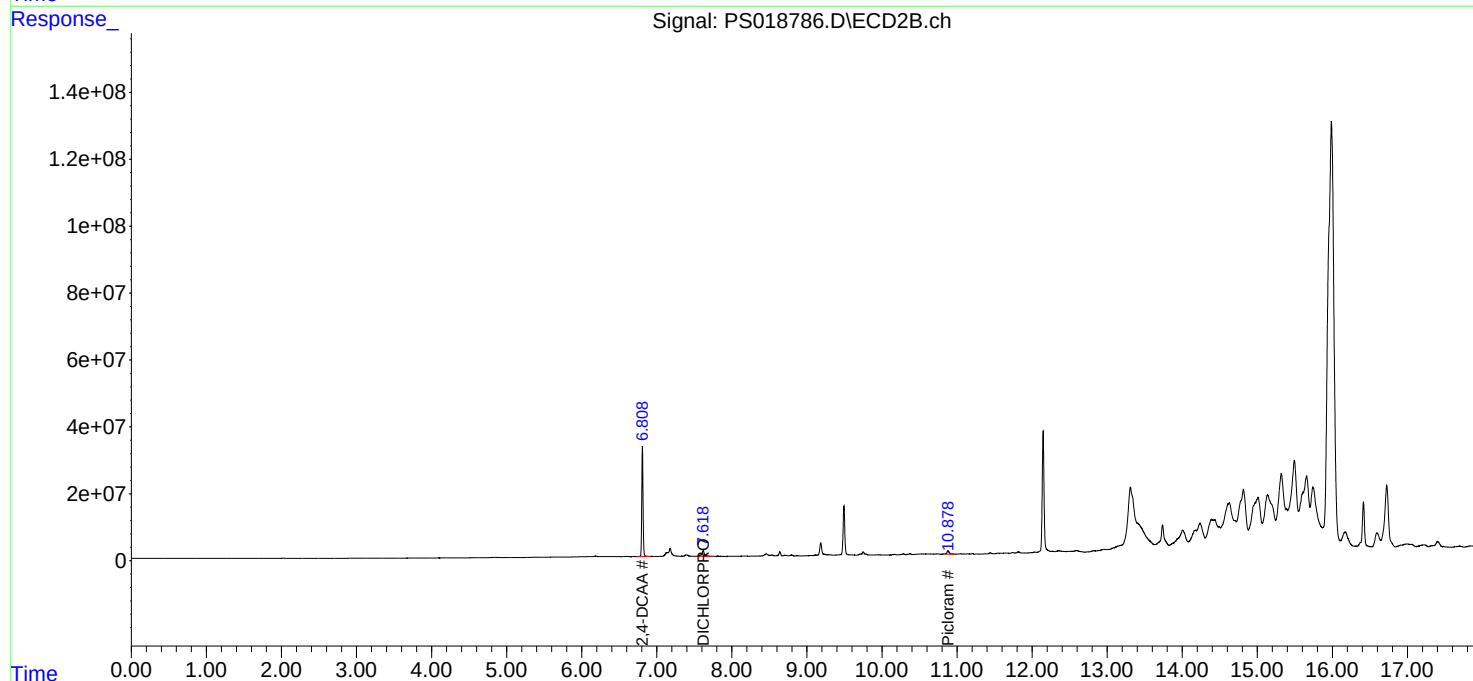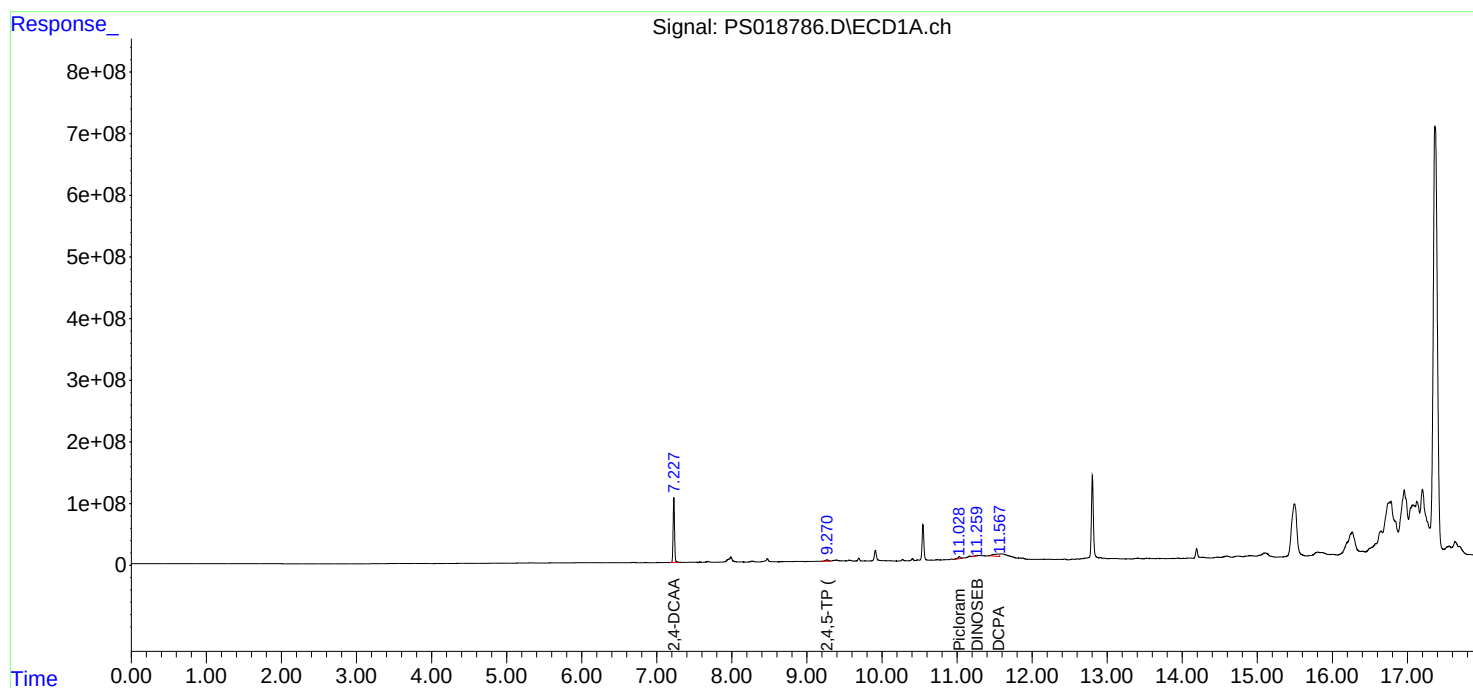


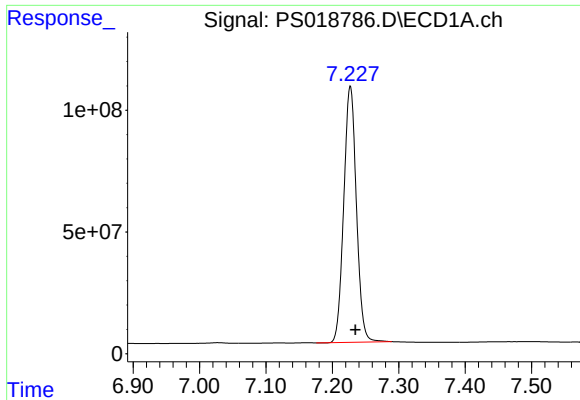

#4 2,4-DCAA


R.T.: 7.227 min
Delta R.T.: -0.008 min
Response: 1389595686
Conc: 488.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

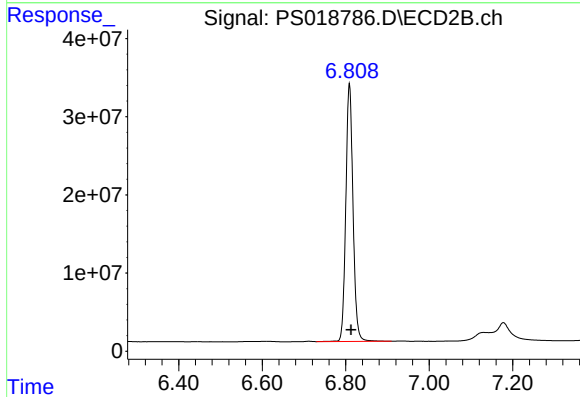


#4 2,4-DCAA

R.T.: 6.809 min
Delta R.T.: -0.004 min
Response: 394039693
Conc: 559.99 ng/ml

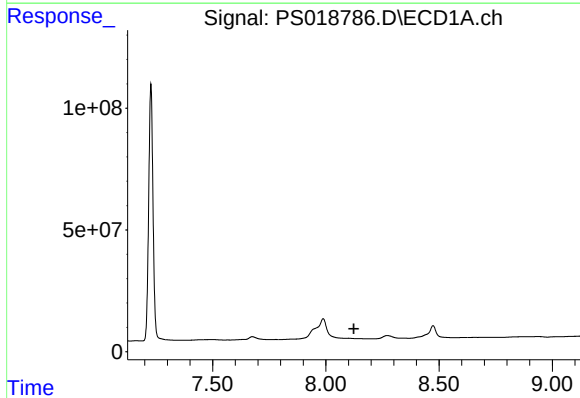


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.124 min
Response: 0
Conc: N.D.

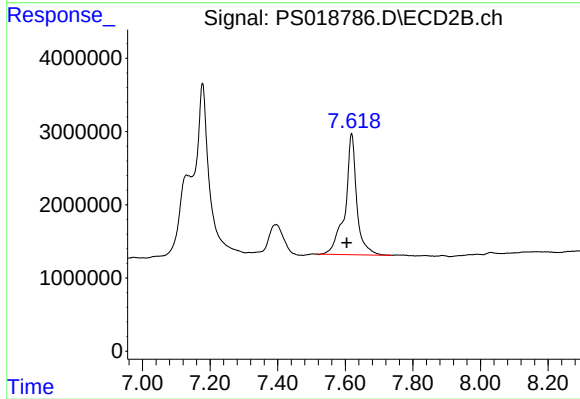

#8 DICHLORPROP


R.T.: 7.619 min
Delta R.T.: 0.015 min
Response: 39461800
Conc: 49.85 ng/ml

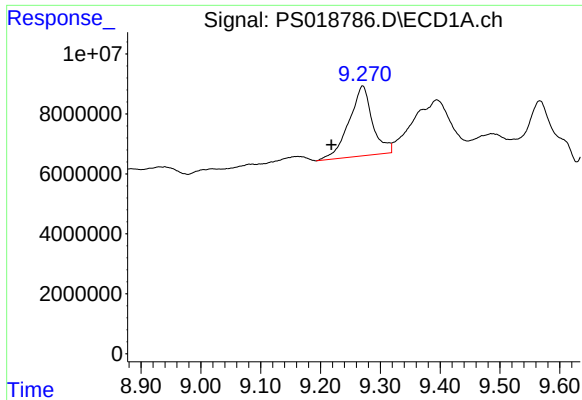

#11 2,4,5-TP (SILVEX)


R.T.: 9.271 min
Delta R.T.: 0.053 min
Response: 63494923
Conc: 4.18 ng/ml

Instrument :
ECD_S
ClientSampleId :

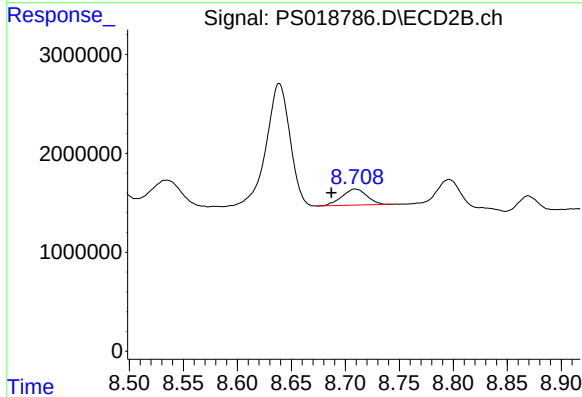


#11 2,4,5-TP (SILVEX)

R.T.: 8.709 min
Delta R.T.: 0.022 min
Response: 2620718
Conc: N.D.

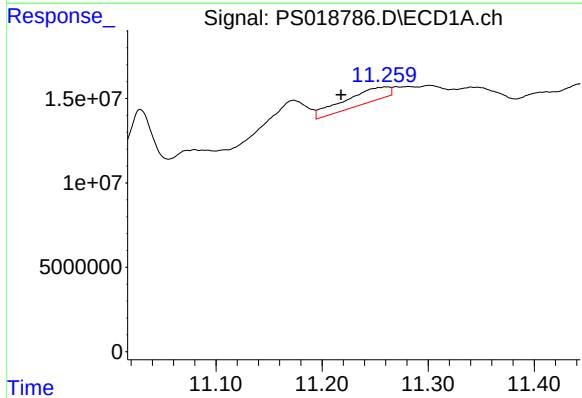


#14 DINOSEB

R.T.: 11.261 min
Delta R.T.: 0.043 min
Response: 25116632
Conc: 2.35 ng/ml

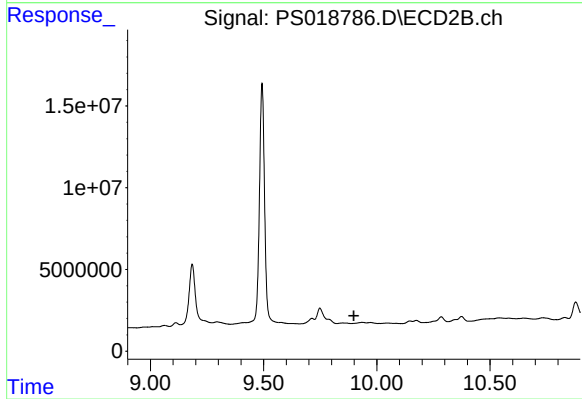

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.899 min
Response: 0
Conc: N.D.

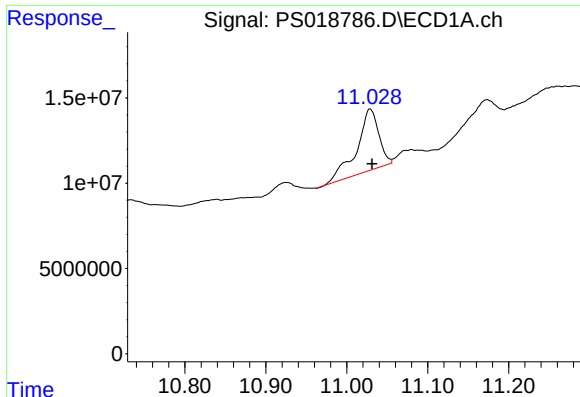

#15 Picloram


R.T.: 11.029 min
Delta R.T.: -0.002 min
Response: 68429997
Conc: 3.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

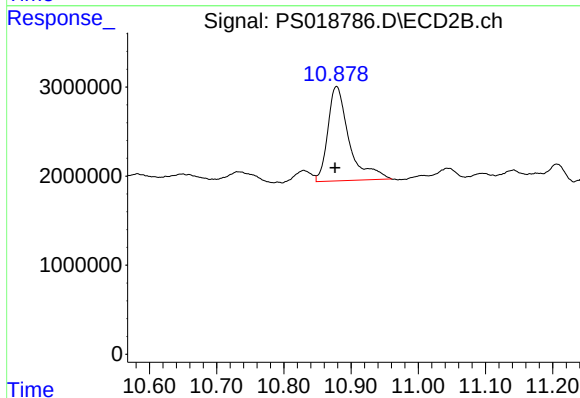


#15 Picloram

R.T.: 10.879 min
Delta R.T.: 0.003 min
Response: 23189561
Conc: 4.36 ng/ml

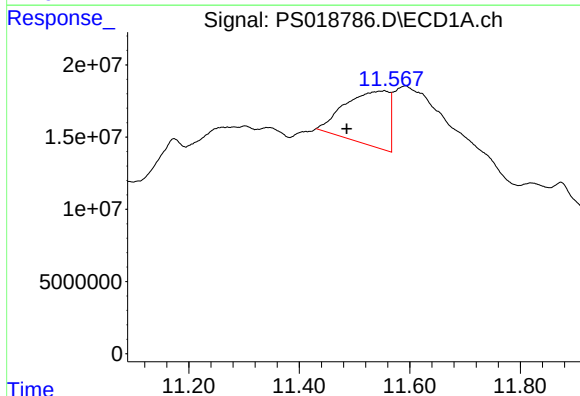

#16 DCPA

R.T.: 11.554 min
Delta R.T.: 0.068 min
Response: 209104021
Conc: 11.69 ng/ml

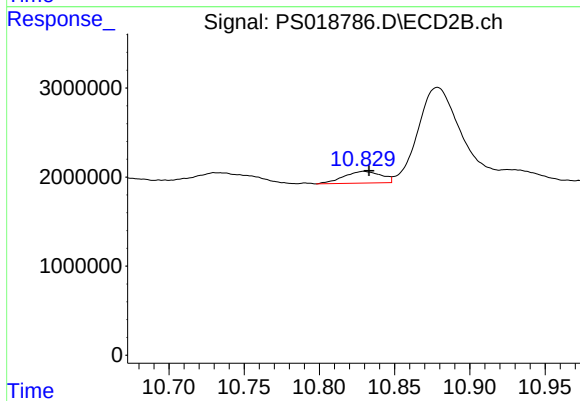

#16 DCPA

R.T.: 10.829 min
Delta R.T.: -0.004 min
Response: 2280013
Conc: N.D.