

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032619\
 Data File : PS003745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 15:40
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 05:53:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
3) T	4-Nitroph...	0.000	9.981	0	478049	N.D. 2.106 #
7) T	MCPA	0.000	11.665	0	810482	N.D. 0.454 #
8) T	DICHLORPROP	0.000	12.125	0	4384285	N.D. 9.418 #
9) T	2,4-D	0.000	12.637	0	140841	N.D. 0.265 #
10) T	Pentachlo...	0.000	13.169	0	208739	N.D. 0.030 #
11) T	2,4,5-TP ...	0.000	13.855	0	1977715	N.D. 0.747 #
13) T	2,4-DB	0.000	15.043	0	1442092	N.D. 4.856 #
14) T	DINOSEB	0.000	15.451	0	3584817	N.D. 1.868 #
15) T	Picloram	16.734	0.000	28567064	0	8.409 N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032619\
Data File : PS003745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 15:40
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 05:53:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

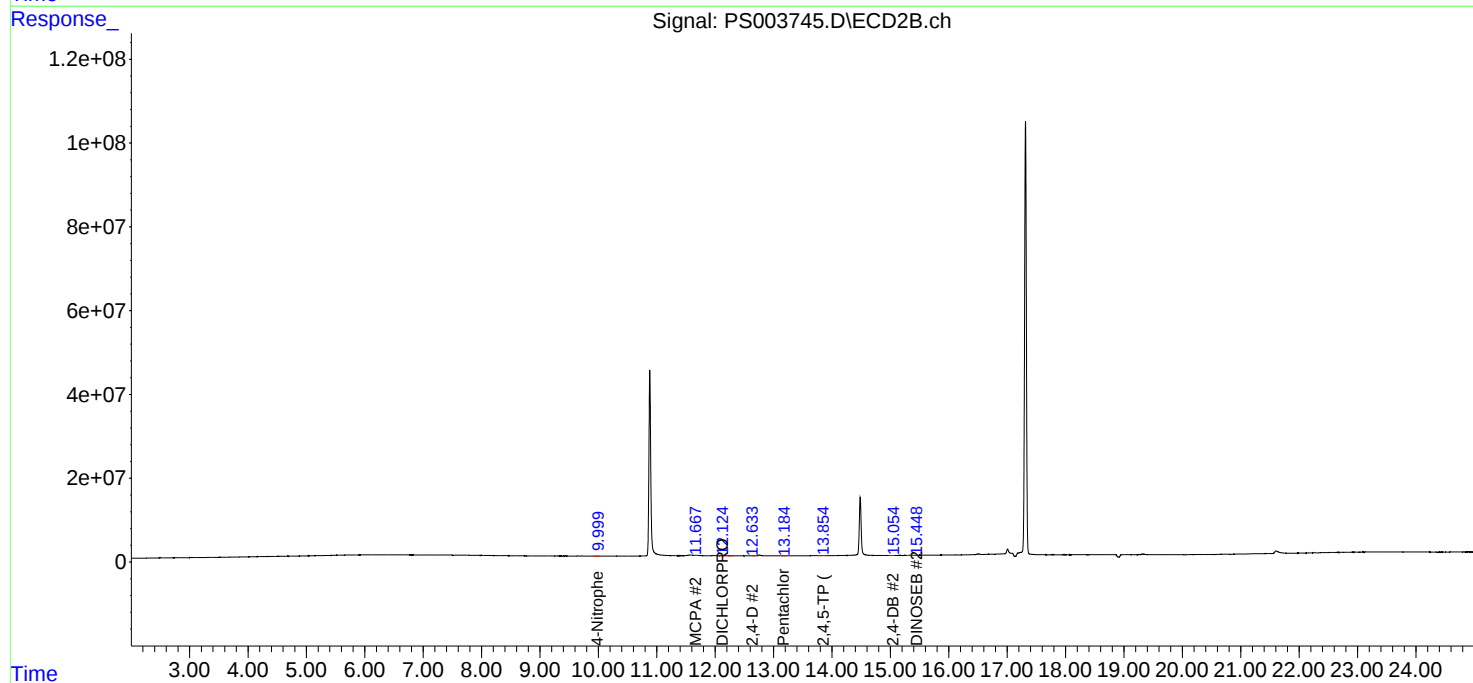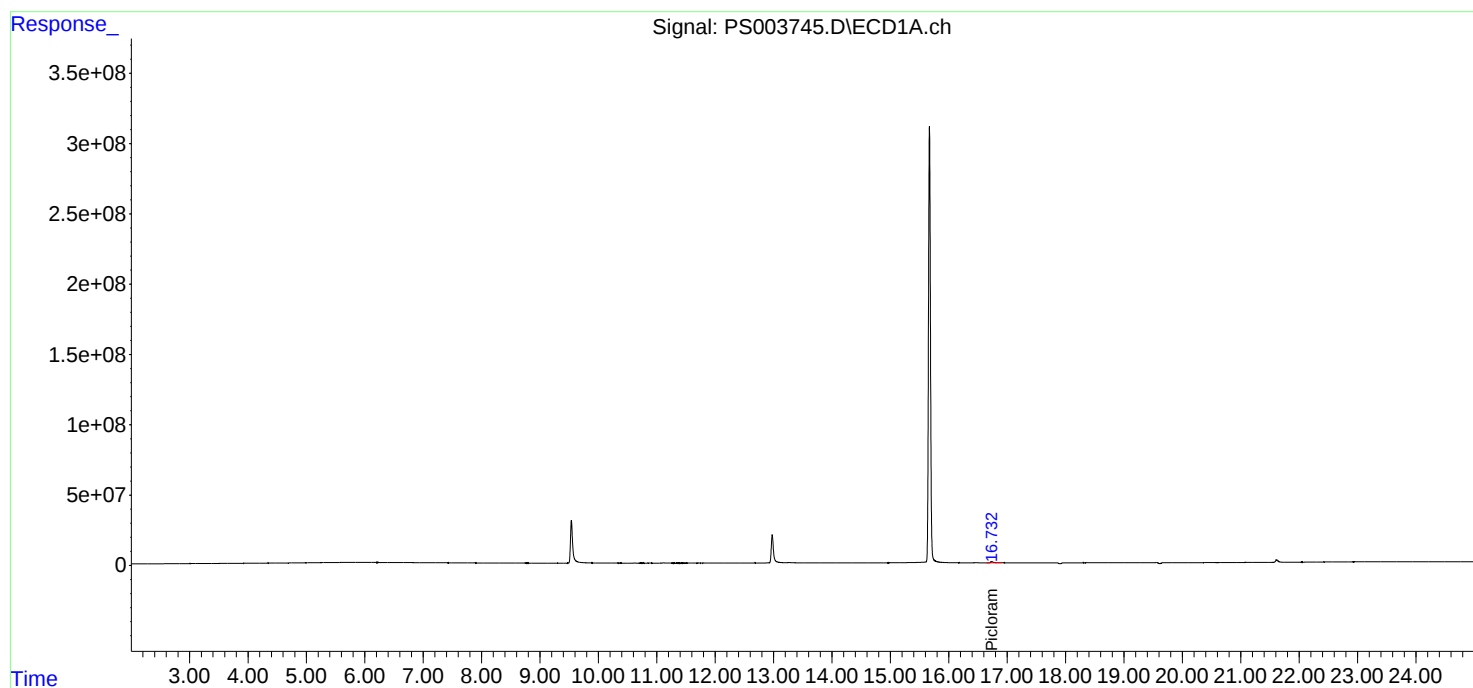


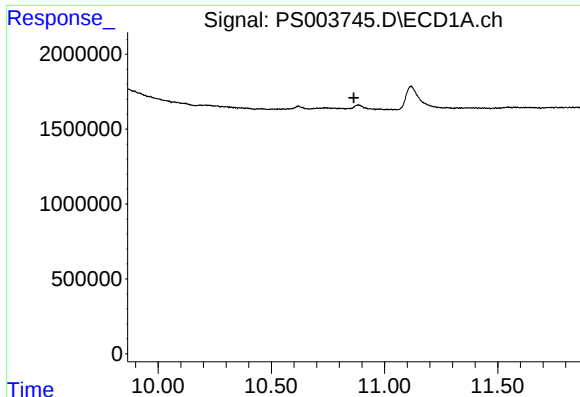

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

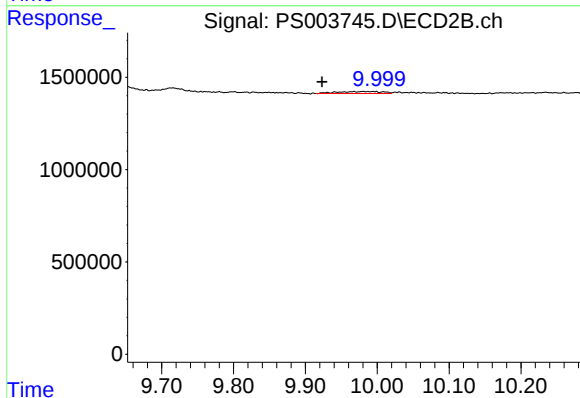


#3 4-Nitrophenol

R.T.: 9.981 min
Delta R.T.: 0.058 min
Response: 478049
Conc: 2.11 ng/ml

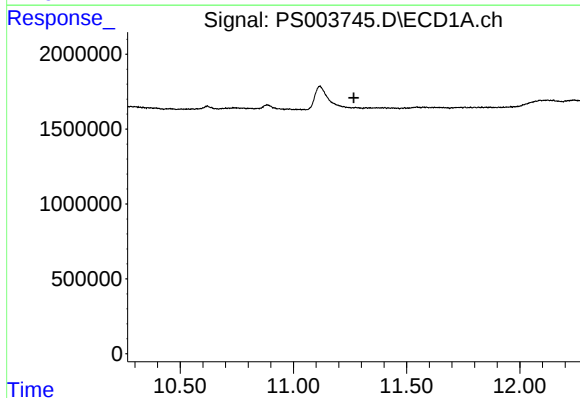


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 11.267 min
Response: 0
Conc: N.D.

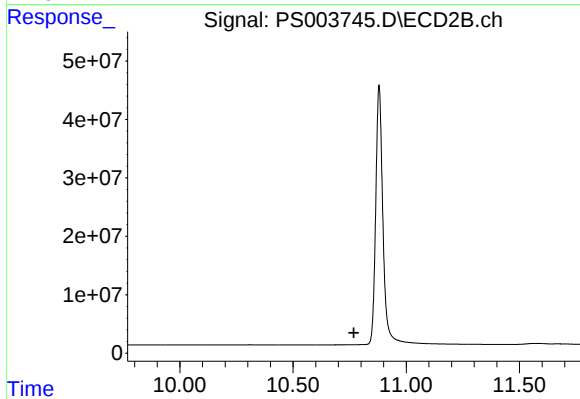

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 10.769 min
Response: 0
Conc: N.D.

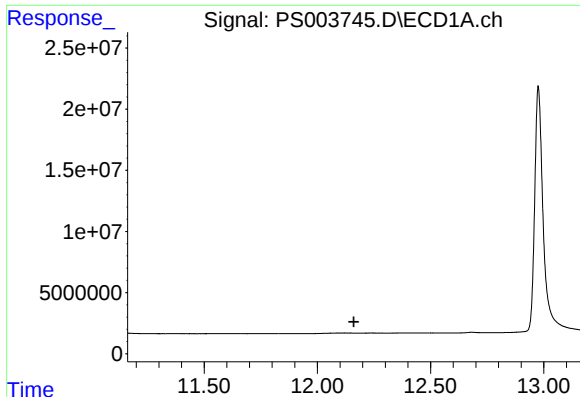

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

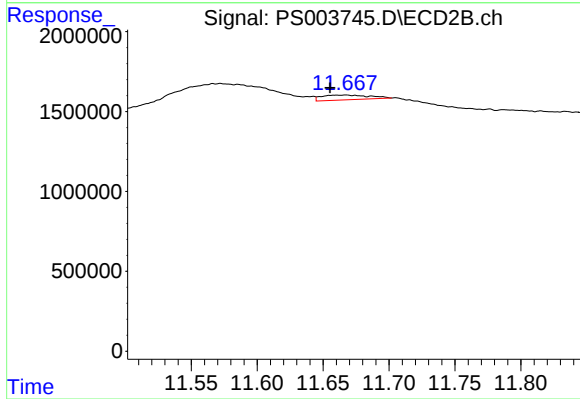


#7 MCPA

R.T.: 11.665 min
Delta R.T.: 0.010 min
Response: 810482
Conc: 0.45 ug/ml

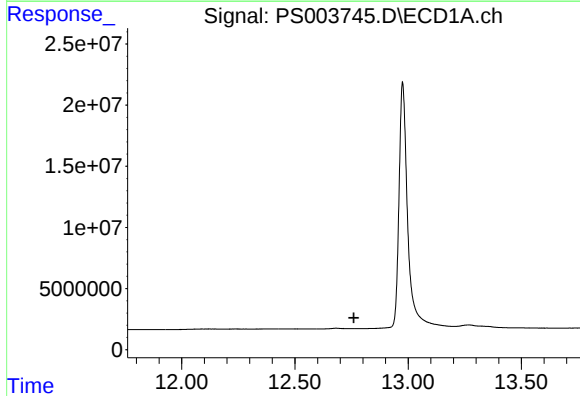


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

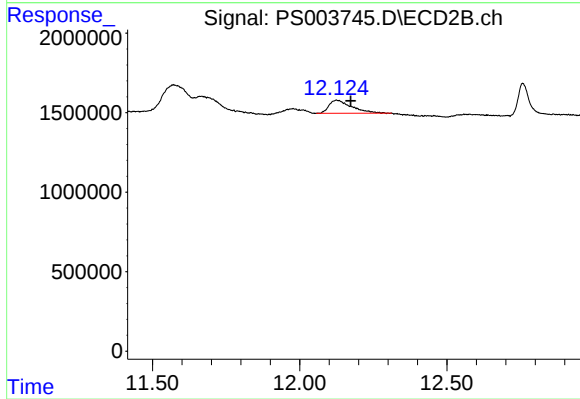

#8 DICHLORPROP


R.T.: 12.125 min
Delta R.T.: -0.048 min
Response: 4384285
Conc: 9.42 ng/ml

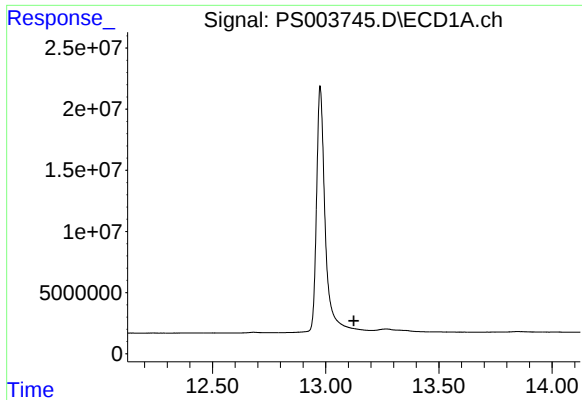

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

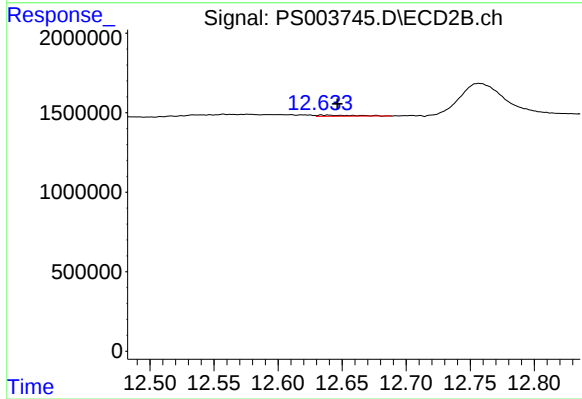


#9 2,4-D

R.T.: 12.637 min
Delta R.T.: -0.009 min
Response: 140841
Conc: 0.26 ng/ml

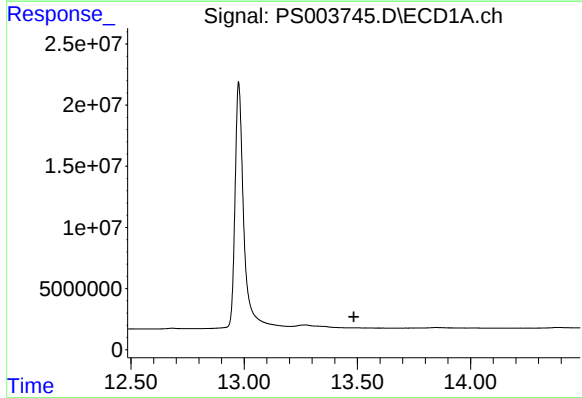


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.485 min
Response: 0
Conc: N.D.

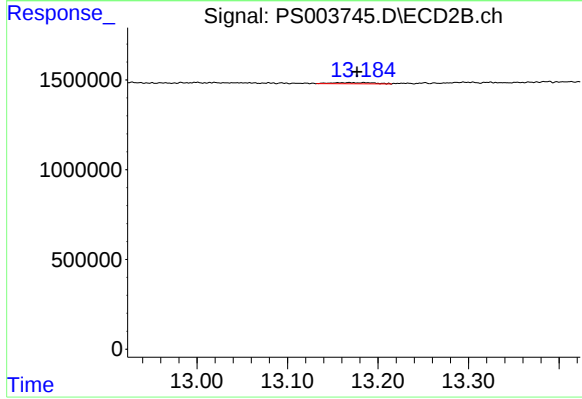

#10 Pentachlorophenol


R.T.: 13.169 min
Delta R.T.: -0.008 min
Response: 208739
Conc: 0.03 ng/ml

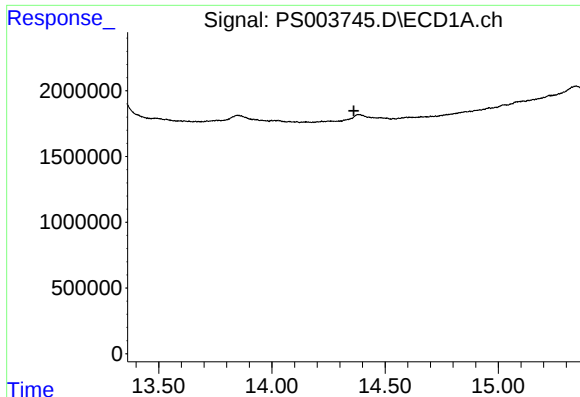

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

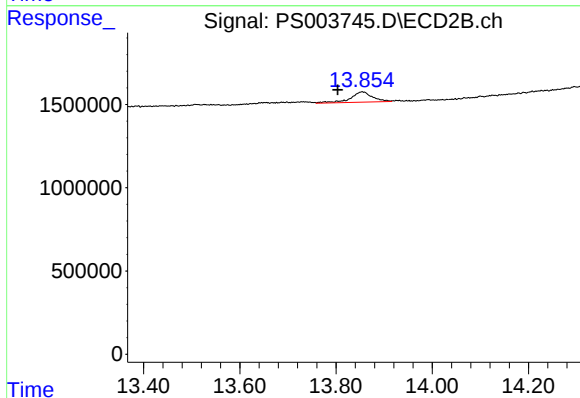


#11 2,4,5-TP (SILVEX)

R.T.: 13.855 min
Delta R.T.: 0.051 min
Response: 1977715
Conc: 0.75 ng/ml

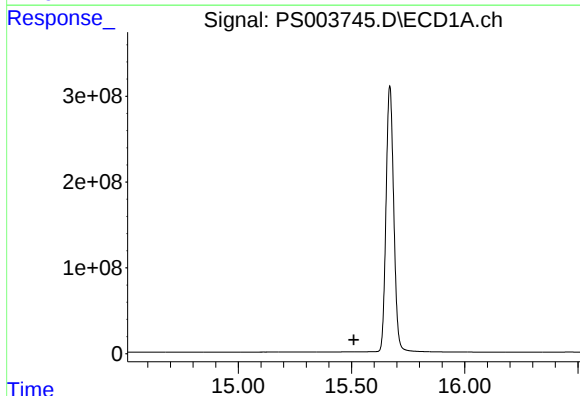


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

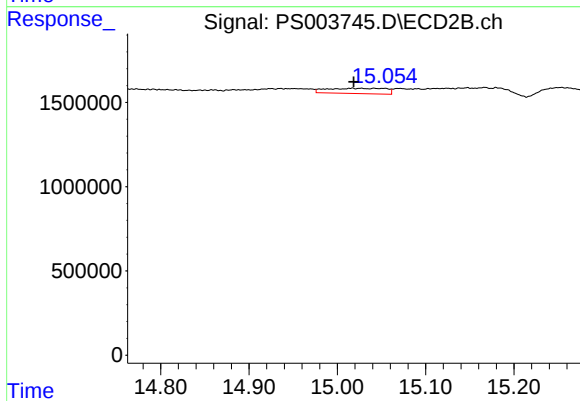

#13 2,4-DB


R.T.: 15.043 min
Delta R.T.: 0.024 min
Response: 1442092
Conc: 4.86 ng/ml

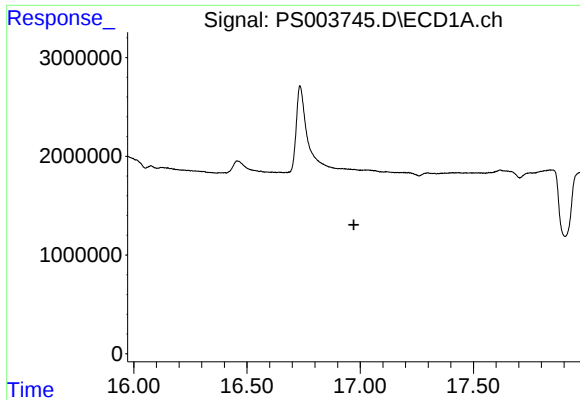

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

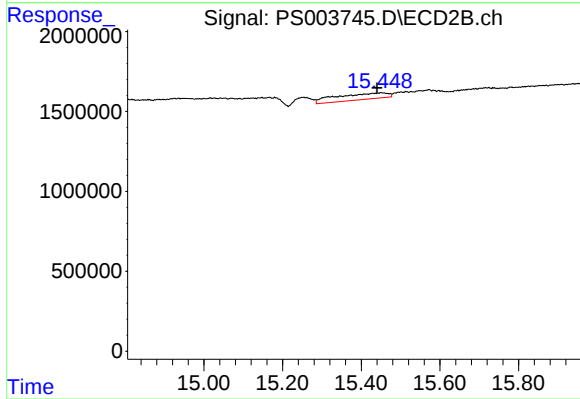


#14 DINOSEB

R.T.: 15.451 min
Delta R.T.: 0.011 min
Response: 3584817
Conc: 1.87 ng/ml

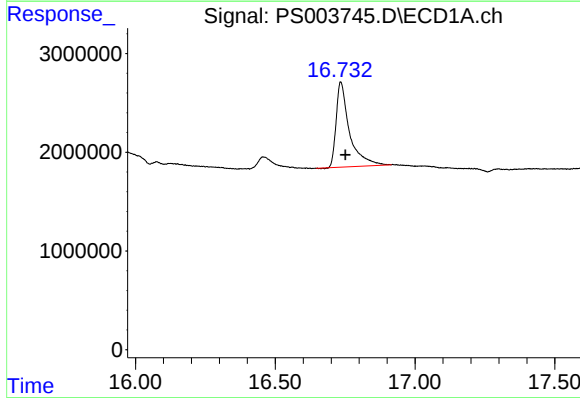

#15 Picloram

R.T.: 16.734 min
Delta R.T.: -0.018 min
Response: 28567064
Conc: 8.41 ng/ml

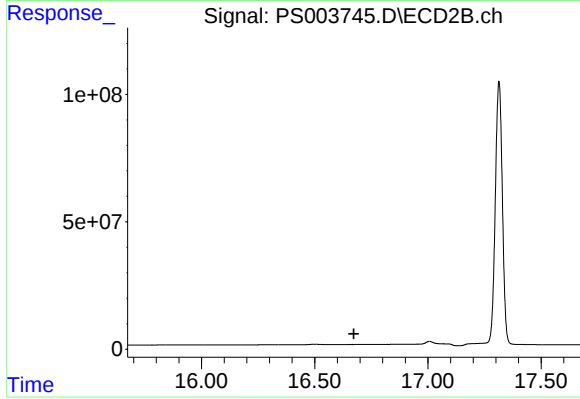

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.673 min
Response: 0
Conc: N.D.