

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032619\
 Data File : PS003761.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2019 00:00
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 06:40:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.274	10.776	226.7E6	197.9E6	519.795	403.245
Target Compounds							
2) T	3,5-DICHL...	0.000	8.931	0	14641	N.D.	0.023 #
3) T	4-Nitroph...	0.000	9.956	0	223091	N.D.	0.983 #
7) T	MCPA	0.000	11.672	0	1136372	N.D.	0.637 #
8) T	DICHLORPROP	0.000	12.130	0	3042541	N.D.	6.536 #
9) T	2,4-D	0.000	12.645	0	72341	N.D.	0.136 #
10) T	Pentachlo...	0.000	13.188	0	1957551	N.D.	0.283 #
11) T	2,4,5-TP ...	0.000	13.783	0	45702	N.D.	0.017 #
12) T	2,4,5-T	0.000	14.340	0	30642	N.D.	0.014 #
13) T	2,4-DB	0.000	15.023	0	533163	N.D.	1.795 #
14) T	DINOSEB	0.000	15.451	0	391444	N.D.	0.204 #
15) T	Picloram	16.761	16.624	6045380	1539066	1.780	0.485 #
16) T	DCPA	0.000	16.624	0	1539066	N.D.	0.455 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032619\
Data File : PS003761.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2019 00:00
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 06:40:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

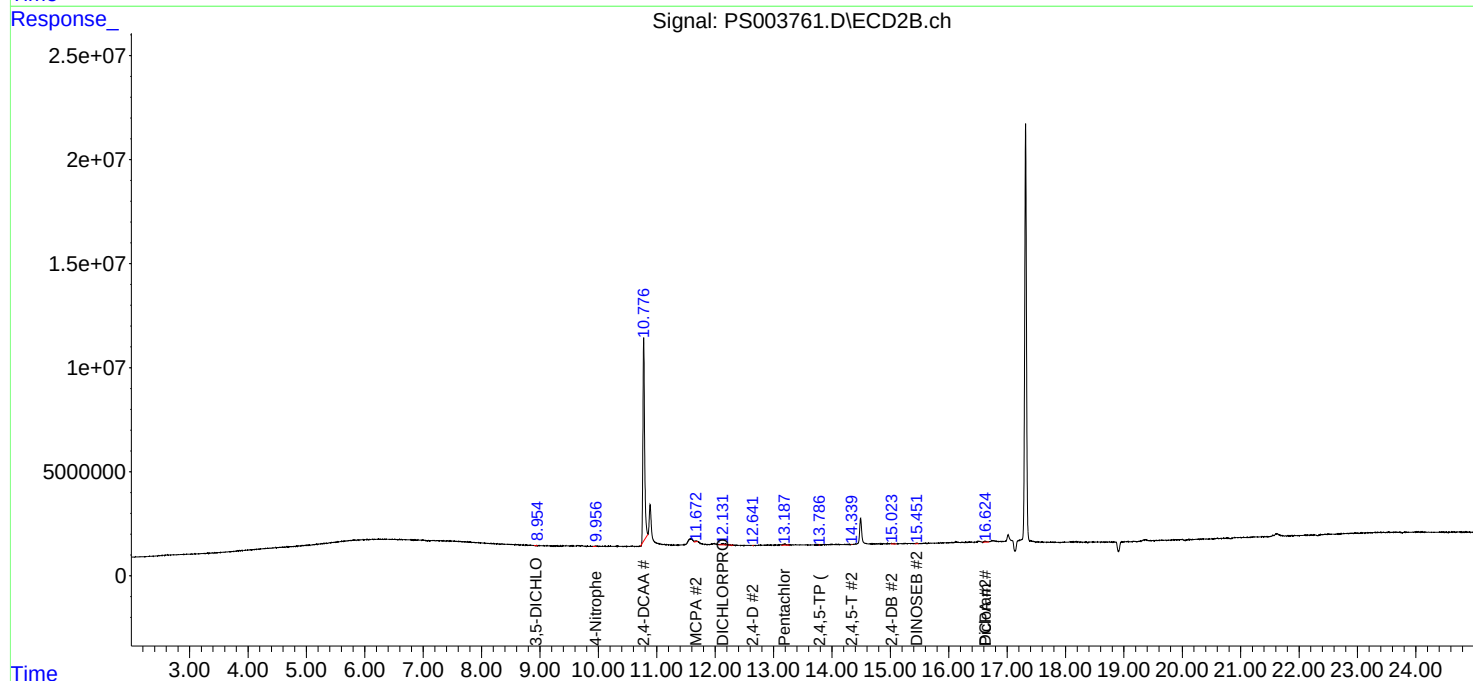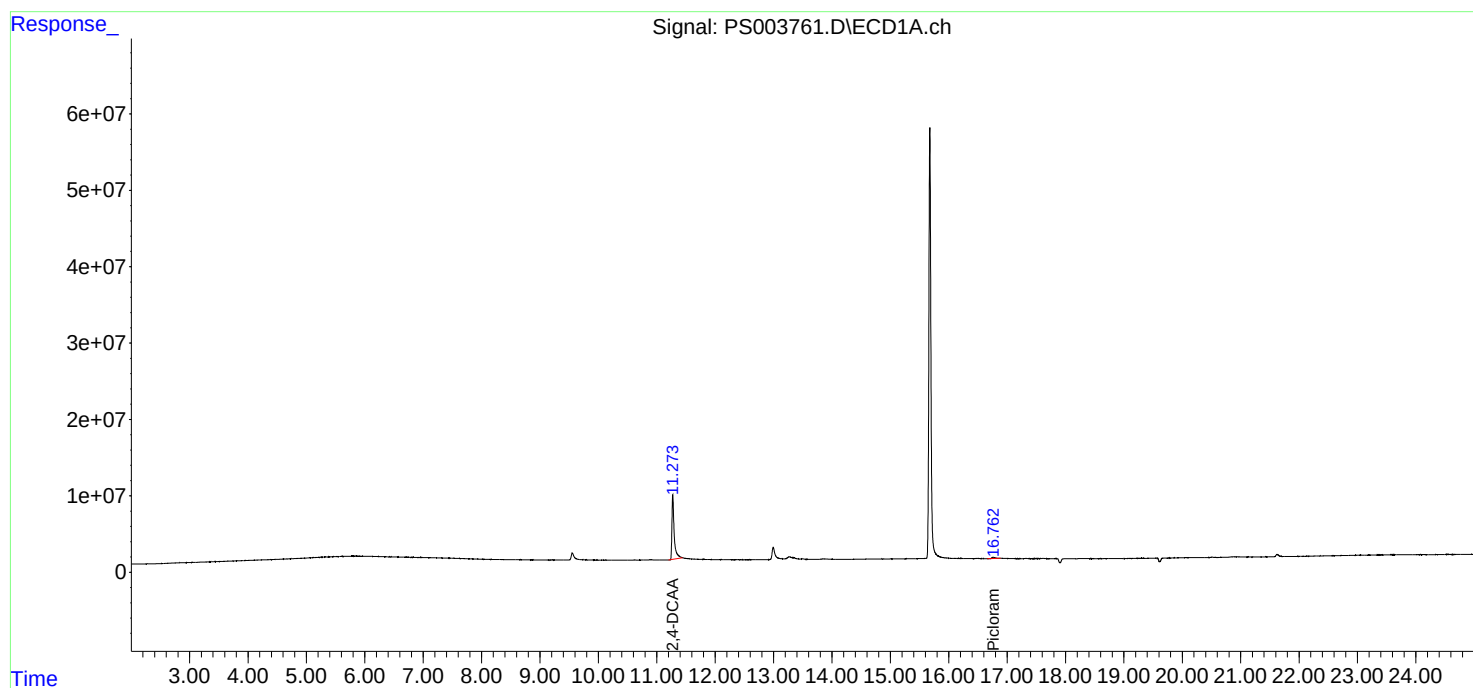


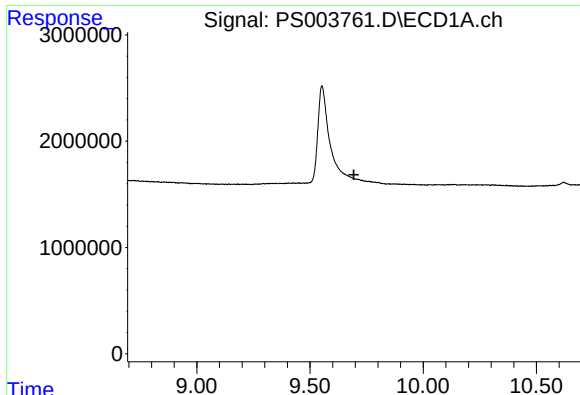

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

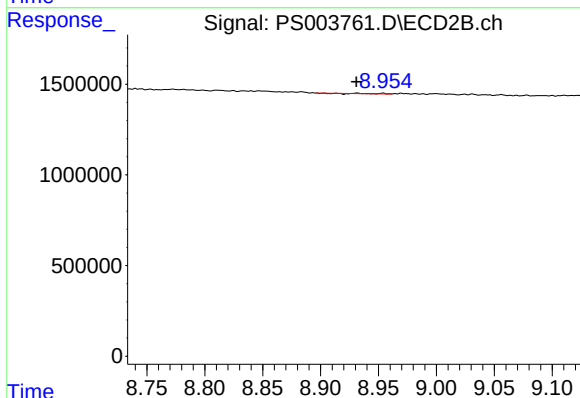


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.931 min
Delta R.T.: 0.000 min
Response: 14641
Conc: 0.02 ng/ml

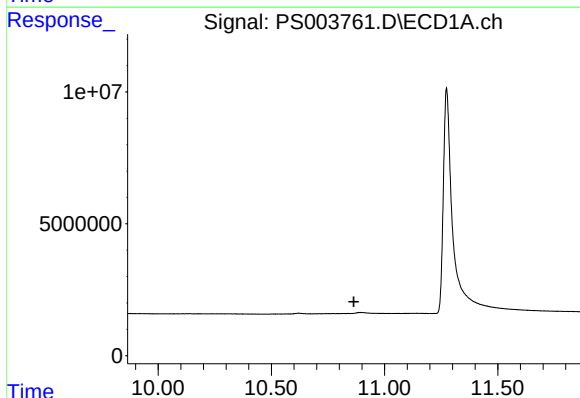


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

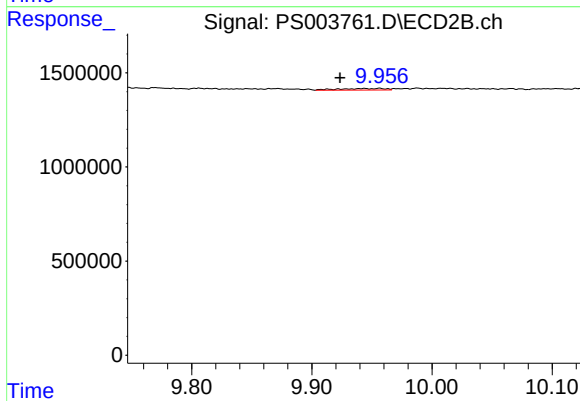

#3 4-Nitrophenol


R.T.: 9.956 min
Delta R.T.: 0.033 min
Response: 223091
Conc: 0.98 ng/ml

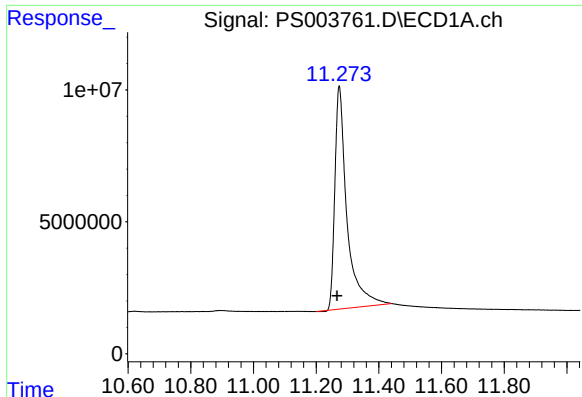

#4 2,4-DCAA


R.T.: 11.274 min
Delta R.T.: 0.007 min
Response: 226740974
Conc: 519.79 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

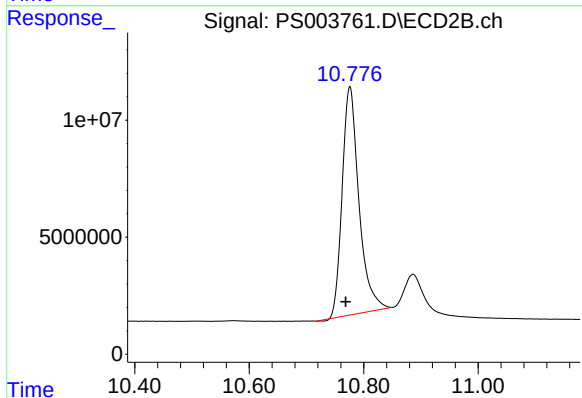


#4 2,4-DCAA

R.T.: 10.776 min
Delta R.T.: 0.007 min
Response: 197855628
Conc: 403.25 ng/ml

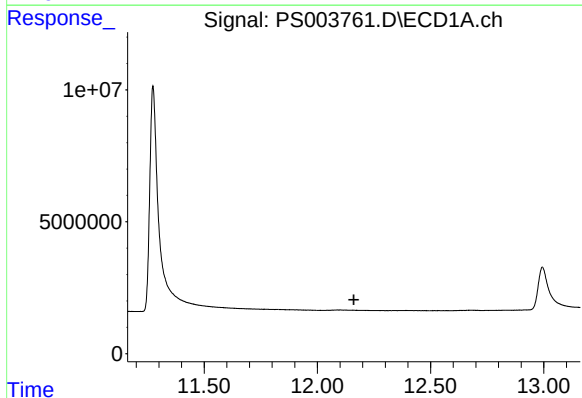


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

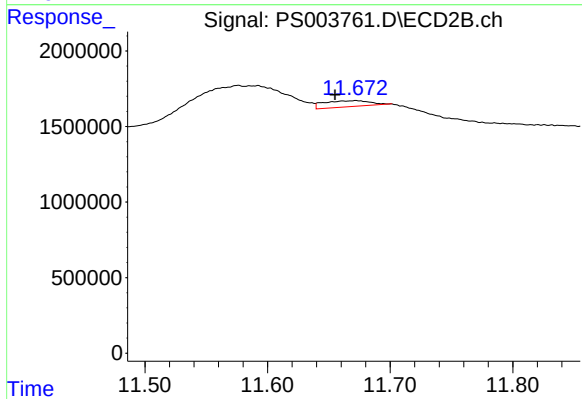

#7 MCPA


R.T.: 11.672 min
Delta R.T.: 0.017 min
Response: 1136372
Conc: 0.64 ug/ml

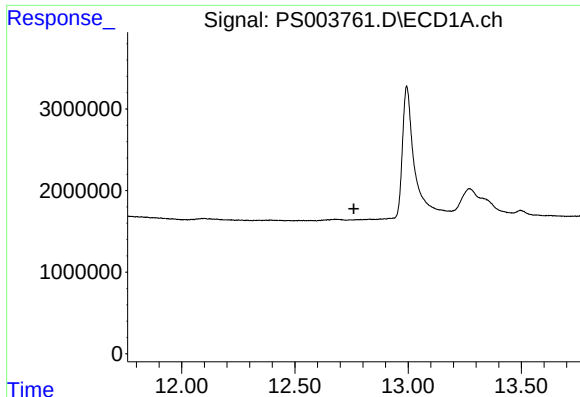

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

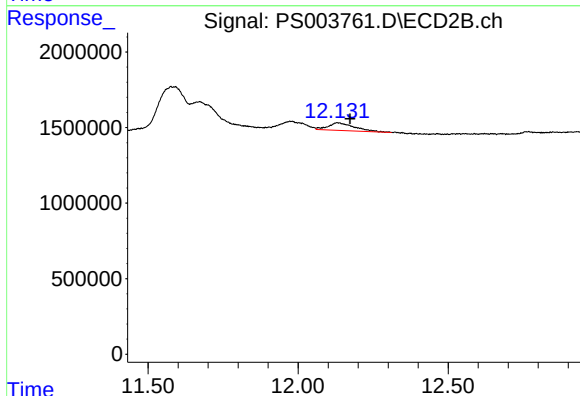


#8 DICHLORPROP

R.T.: 12.130 min
Delta R.T.: -0.043 min
Response: 3042541
Conc: 6.54 ng/ml

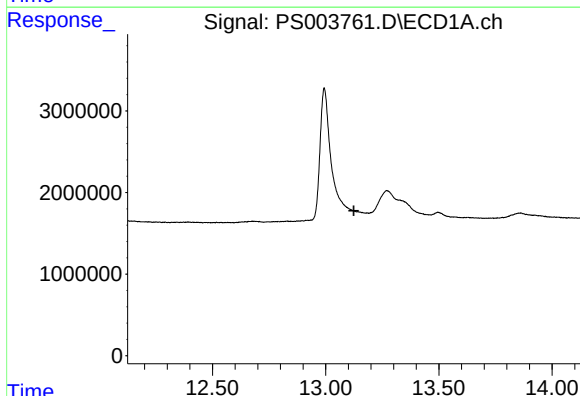


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

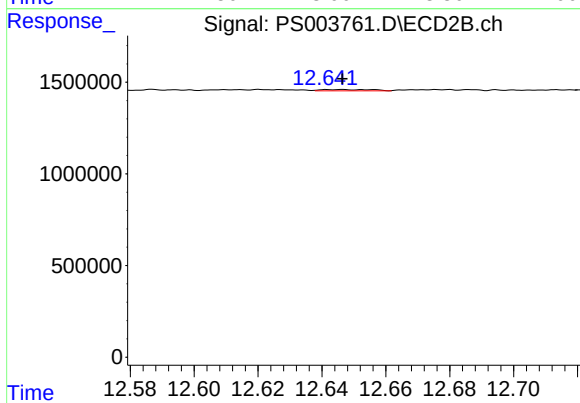

#9 2,4-D


R.T.: 12.645 min
Delta R.T.: -0.001 min
Response: 72341
Conc: 0.14 ng/ml

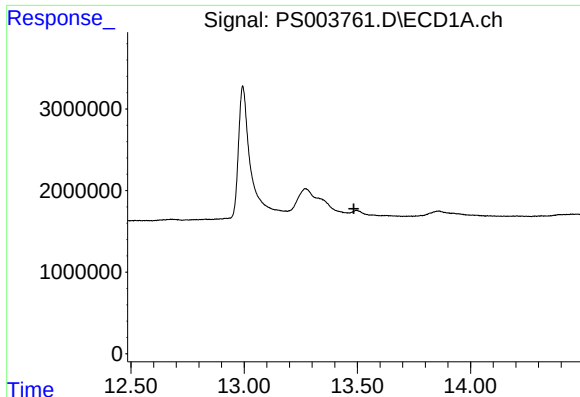

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

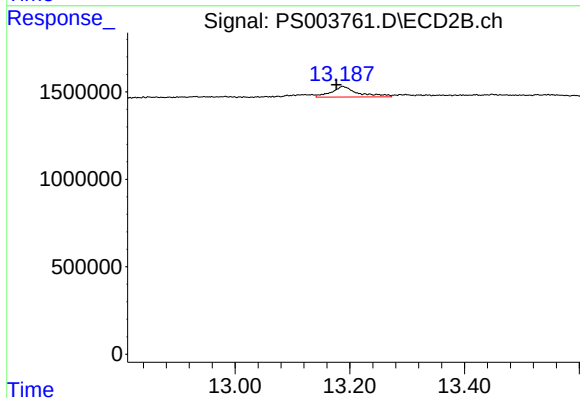


#10 Pentachlorophenol

R.T.: 13.188 min
Delta R.T.: 0.011 min
Response: 1957551
Conc: 0.28 ng/ml

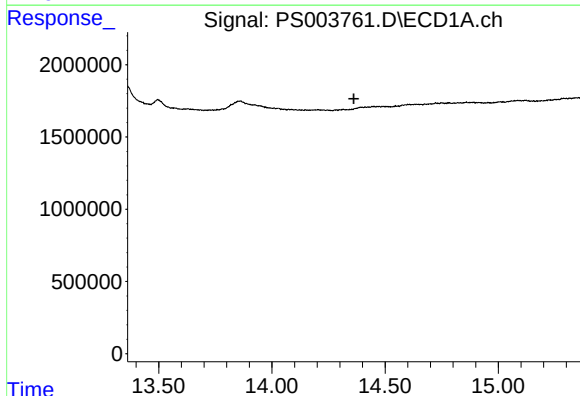


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

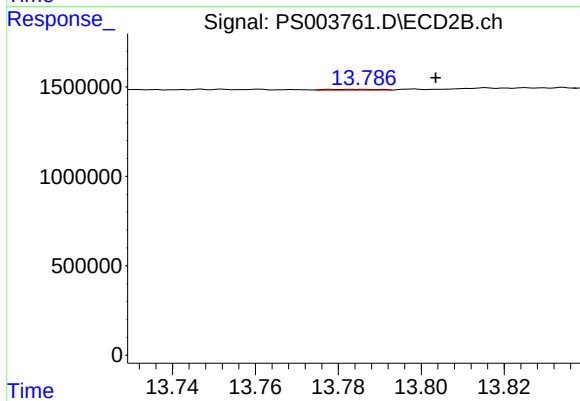

#11 2,4,5-TP (SILVEX)


R.T.: 13.783 min
Delta R.T.: -0.020 min
Response: 45702
Conc: 0.02 ng/ml

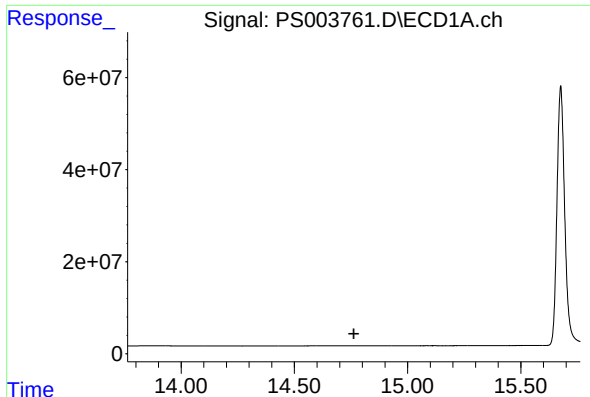

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

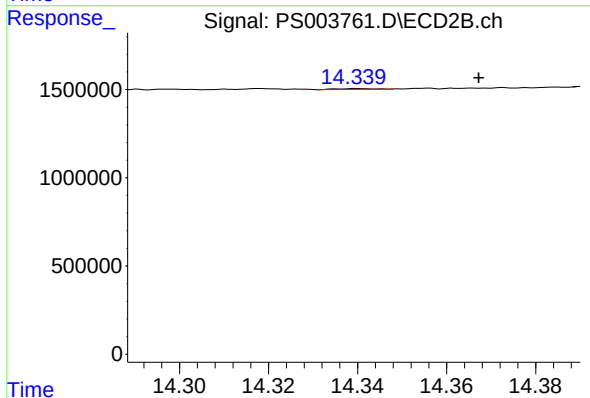


#12 2,4,5-T

R.T.: 14.340 min
Delta R.T.: -0.027 min
Response: 30642
Conc: 0.01 ng/ml

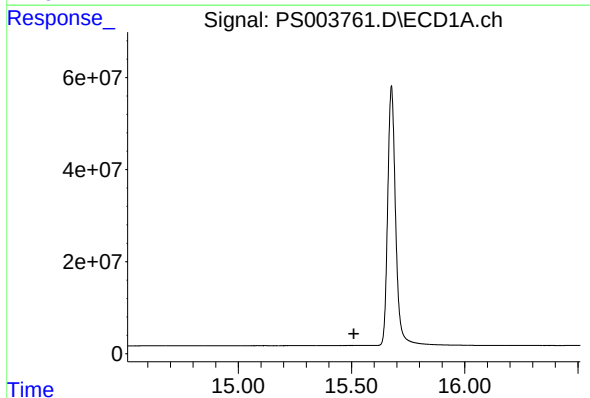


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

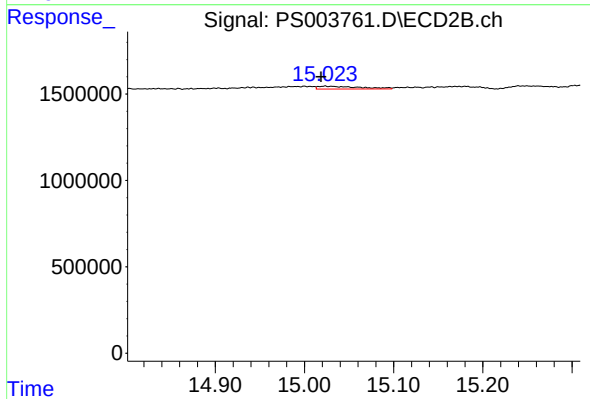

#13 2,4-DB


R.T.: 15.023 min
Delta R.T.: 0.005 min
Response: 533163
Conc: 1.80 ng/ml

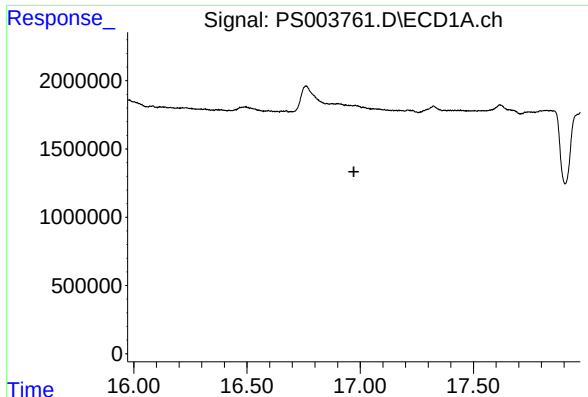

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

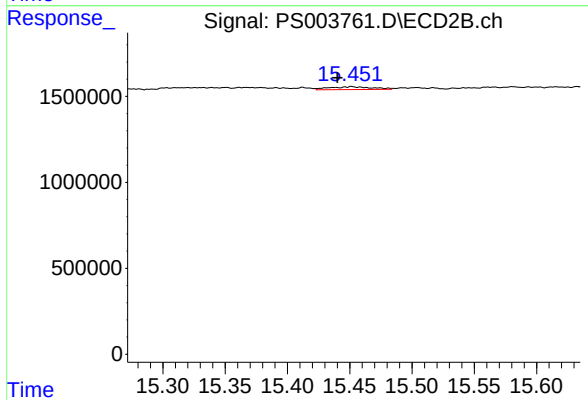


#14 DINOSEB

R.T.: 15.451 min
Delta R.T.: 0.011 min
Response: 391444
Conc: 0.20 ng/ml

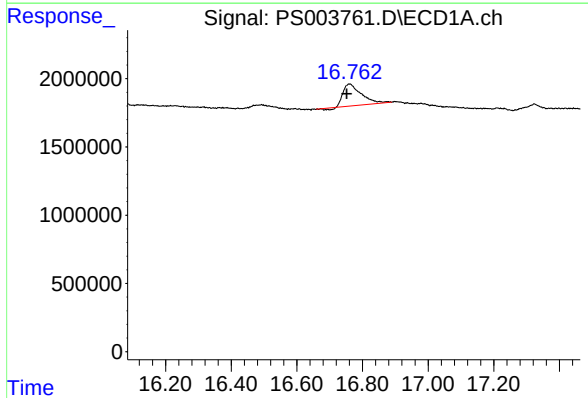


#15 Picloram

R.T.: 16.761 min
Delta R.T.: 0.009 min
Response: 6045380
Conc: 1.78 ng/ml

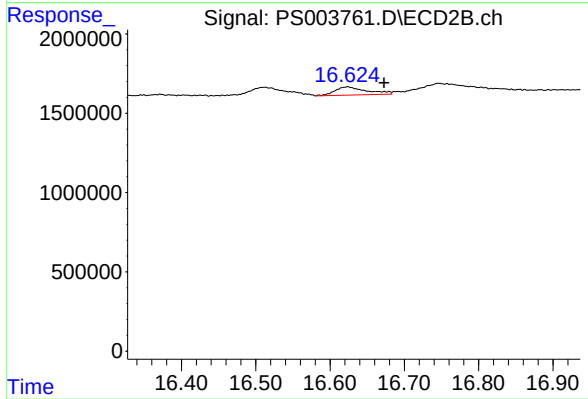

#15 Picloram


R.T.: 16.624 min
Delta R.T.: -0.049 min
Response: 1539066
Conc: 0.49 ng/ml

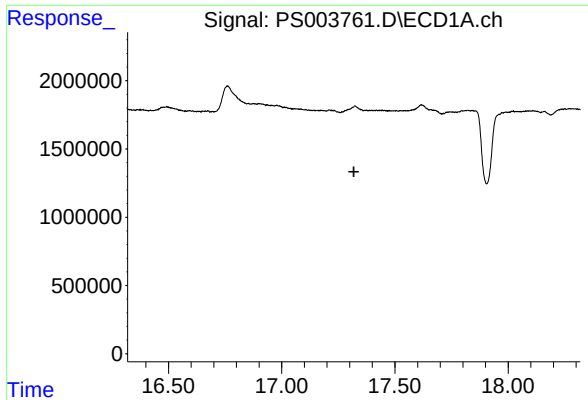

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

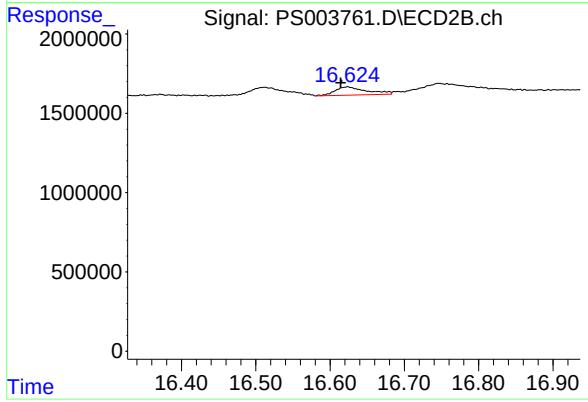

#16 DCPA

R.T.: 16.624 min
Delta R.T.: 0.009 min
Response: 1539066
Conc: 0.46 ng/ml