

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032619\
 Data File : PS003777.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2019 08:20
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 10:32:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.268	10.771	224.6E6	192.1E6	514.920	391.425
Target Compounds							
3) T	4-Nitroph...	0.000	9.931	0	290383	N.D.	1.279 #
7) T	MCPA	0.000	11.662	0	1325154	N.D.	0.743 #
8) T	DICHLORPROP	0.000	12.137	0	3949409	N.D.	8.484 #
9) T	2,4-D	0.000	12.649	0	81069	N.D.	0.152 #
10) T	Pentachlo...	0.000	13.184	0	1855483	N.D.	0.268 #
11) T	2,4,5-TP ...	0.000	13.843	0	926309	N.D.	0.350 #
12) T	2,4,5-T	0.000	14.325	0	26668	N.D.	0.012 #
13) T	2,4-DB	0.000	15.027	0	270652	N.D.	0.911 #
14) T	DINOSEB	0.000	15.464	0	818979	N.D.	0.427 #
15) T	Picloram	16.751	16.619	10948114	1098168	3.223	0.346 #
16) T	DCPA	0.000	16.619	0	1098168	N.D.	0.325 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032619\
Data File : PS003777.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2019 08:20
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 10:32:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

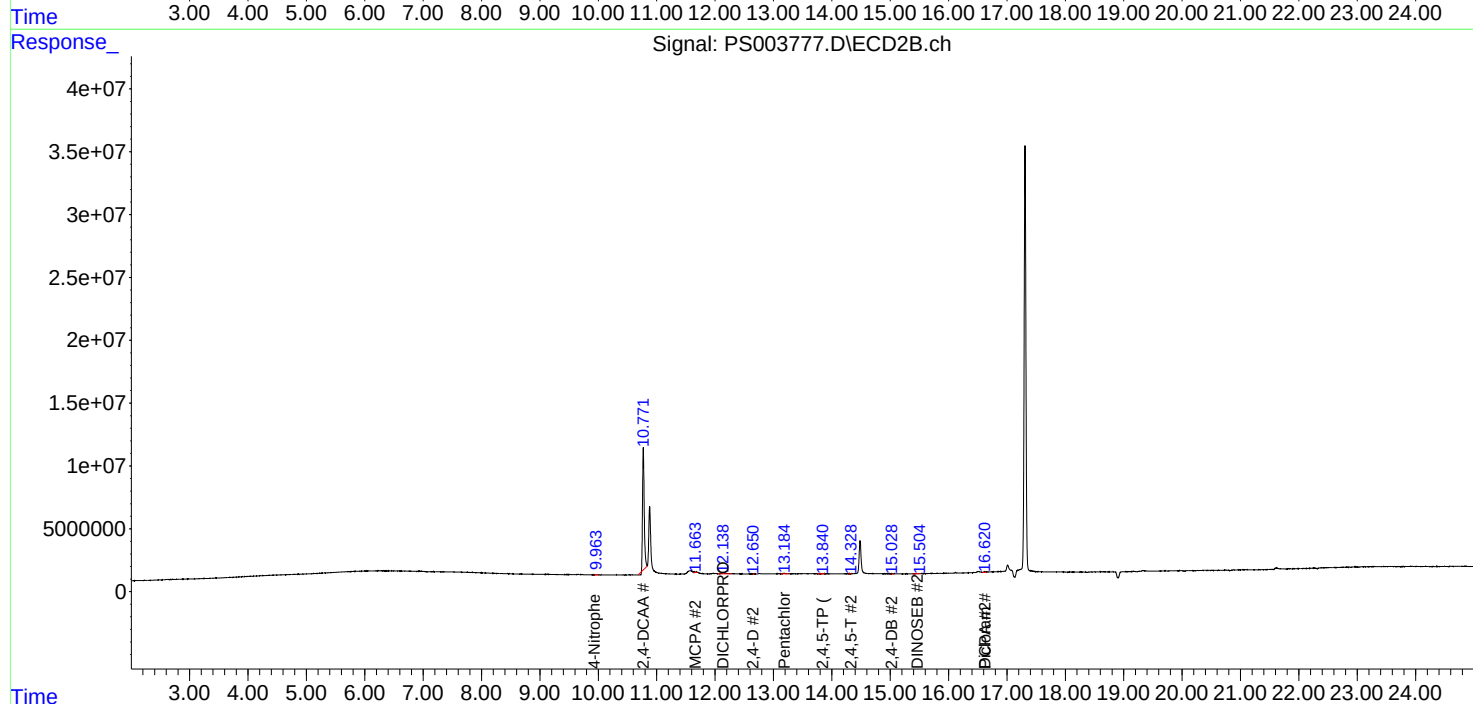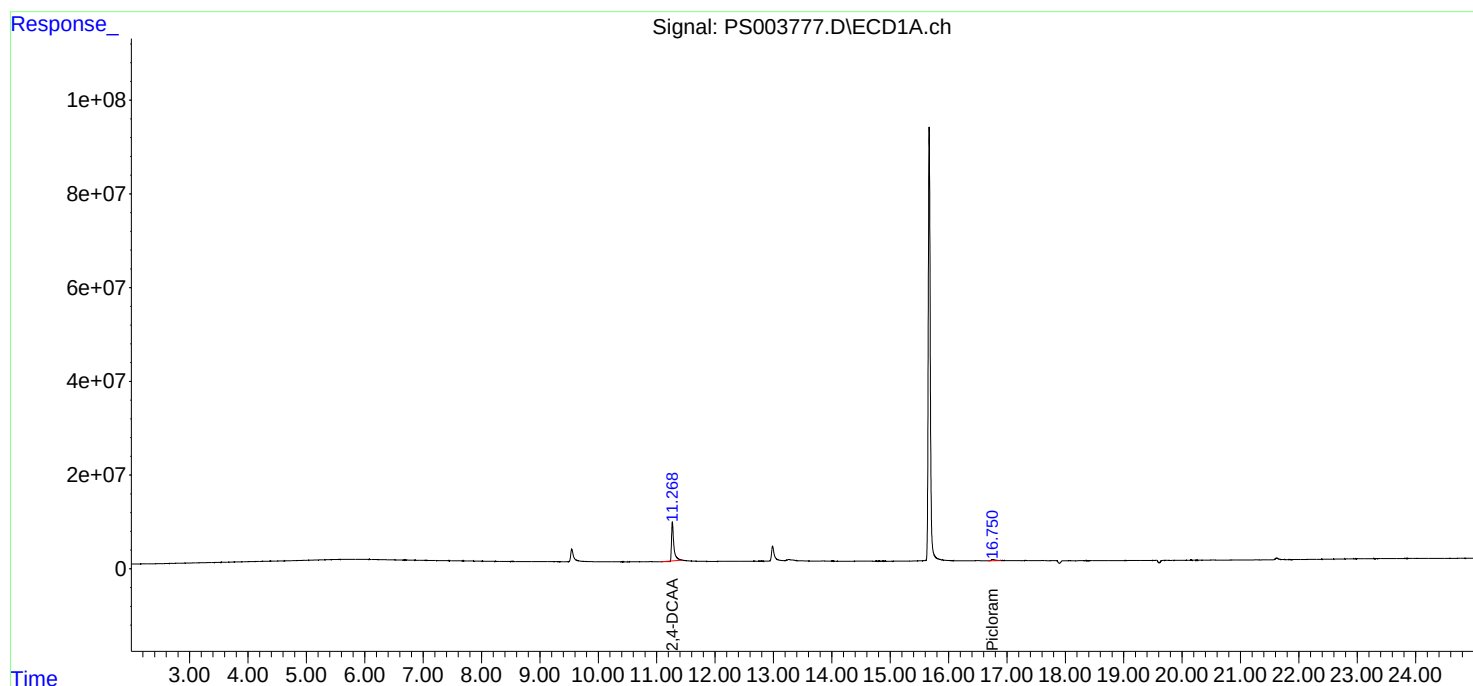


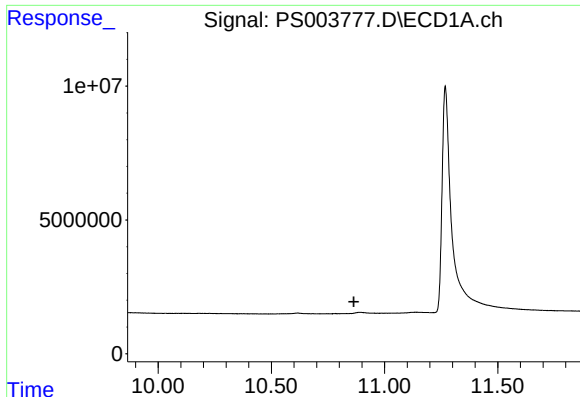

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

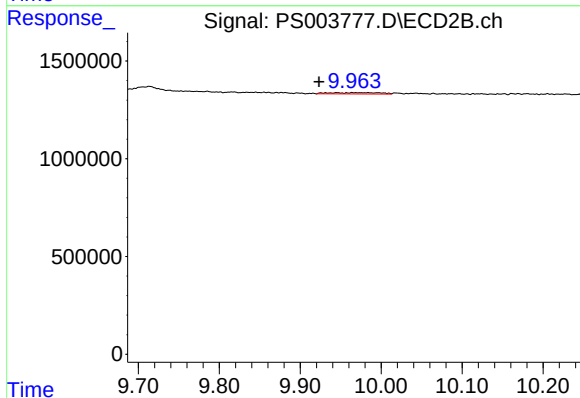


#3 4-Nitrophenol

R.T.: 9.931 min
Delta R.T.: 0.008 min
Response: 290383
Conc: 1.28 ng/ml

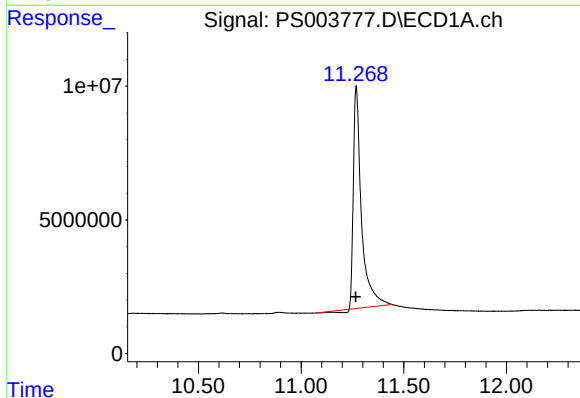


#4 2,4-DCAA

R.T.: 11.268 min
Delta R.T.: 0.001 min
Response: 224614488
Conc: 514.92 ng/ml

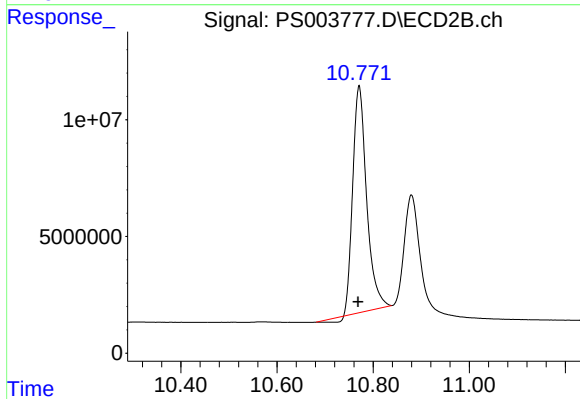

#4 2,4-DCAA


R.T.: 10.771 min
Delta R.T.: 0.002 min
Response: 192055736
Conc: 391.42 ng/ml

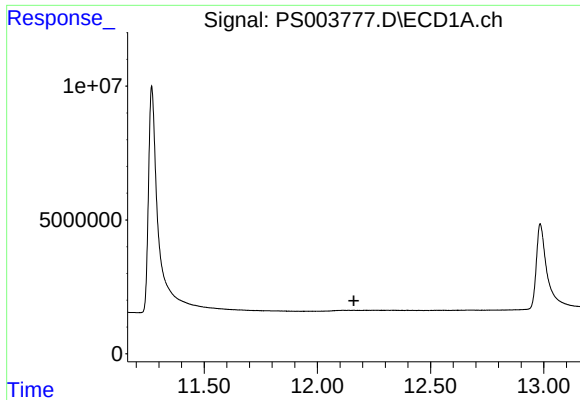

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

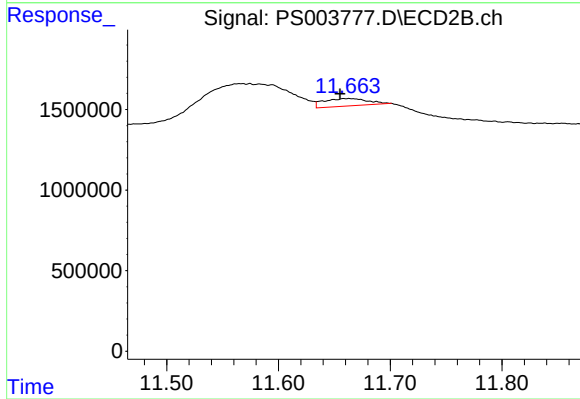


#7 MCPA

R.T.: 11.662 min
Delta R.T.: 0.007 min
Response: 1325154
Conc: 0.74 ug/ml

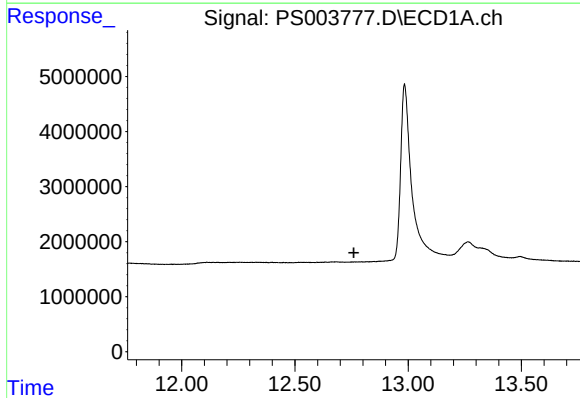


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

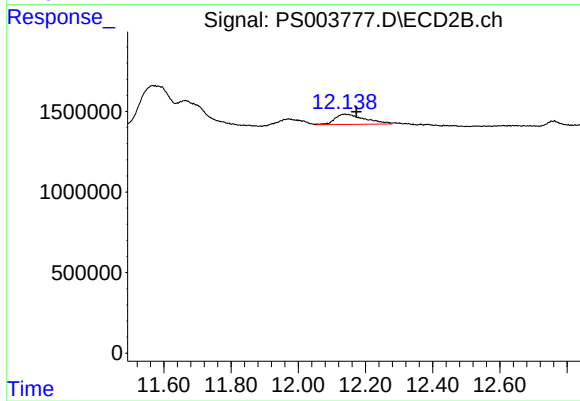

#8 DICHLORPROP


R.T.: 12.137 min
Delta R.T.: -0.036 min
Response: 3949409
Conc: 8.48 ng/ml

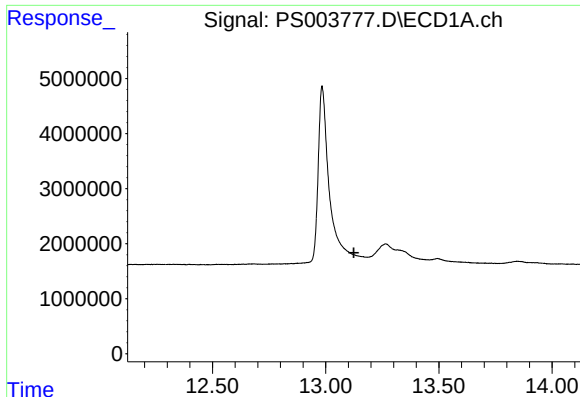

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

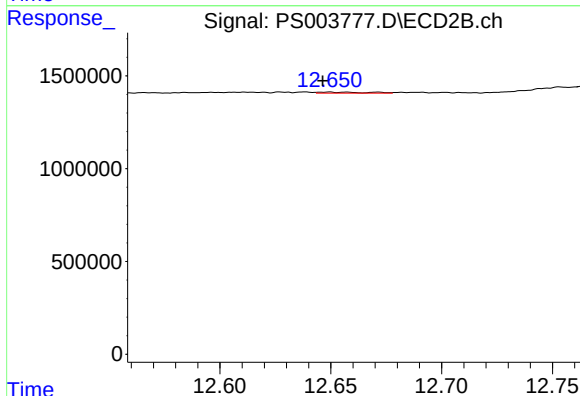


#9 2,4-D

R.T.: 12.649 min
Delta R.T.: 0.002 min
Response: 81069
Conc: 0.15 ng/ml

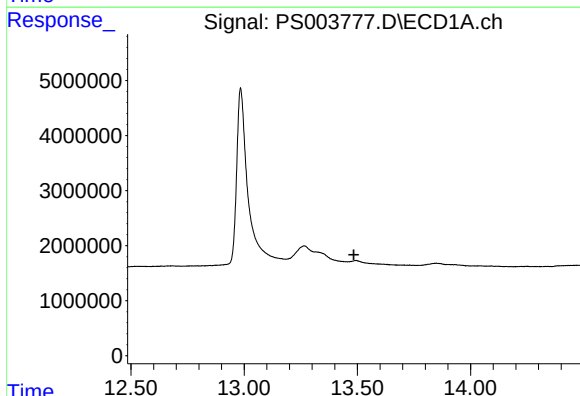


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.485 min
Response: 0
Conc: N.D.

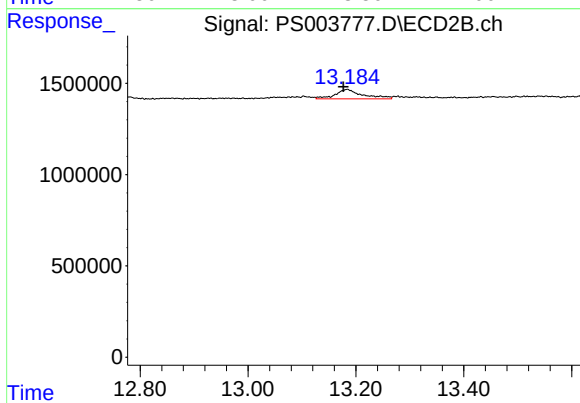

#10 Pentachlorophenol


R.T.: 13.184 min
Delta R.T.: 0.007 min
Response: 1855483
Conc: 0.27 ng/ml

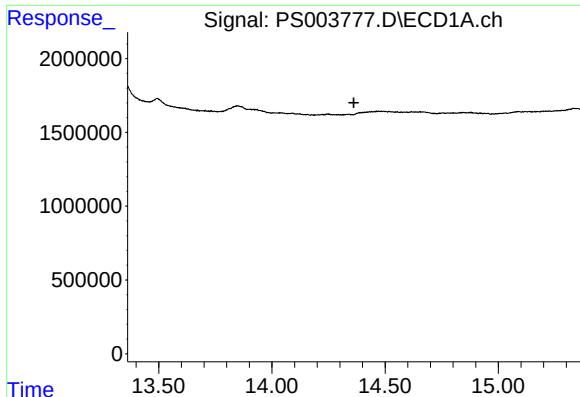

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

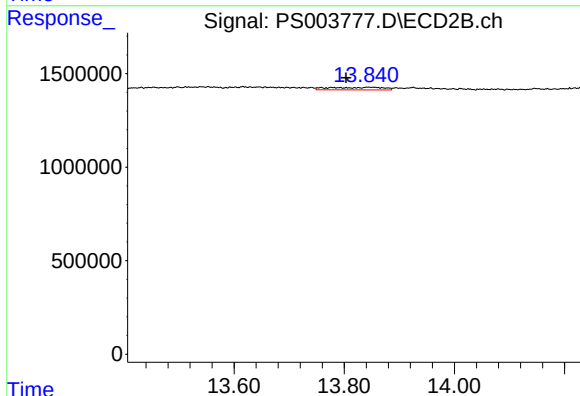


#11 2,4,5-TP (SILVEX)

R.T.: 13.843 min
Delta R.T.: 0.040 min
Response: 926309
Conc: 0.35 ng/ml

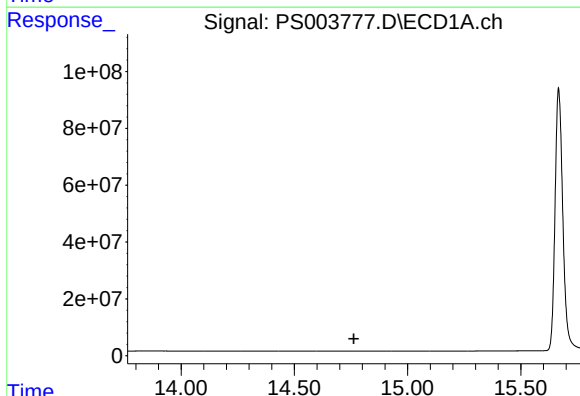


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

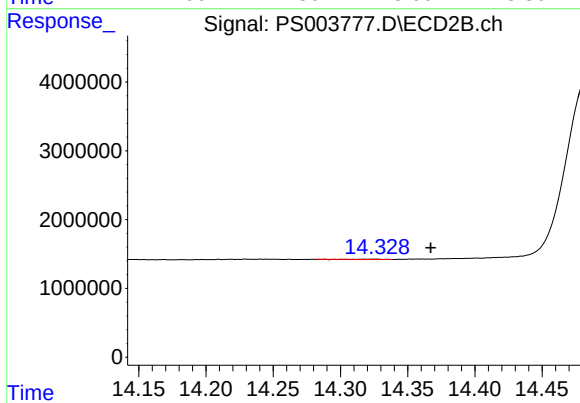

#12 2,4,5-T


R.T.: 14.325 min
Delta R.T.: -0.043 min
Response: 26668
Conc: 0.01 ng/ml

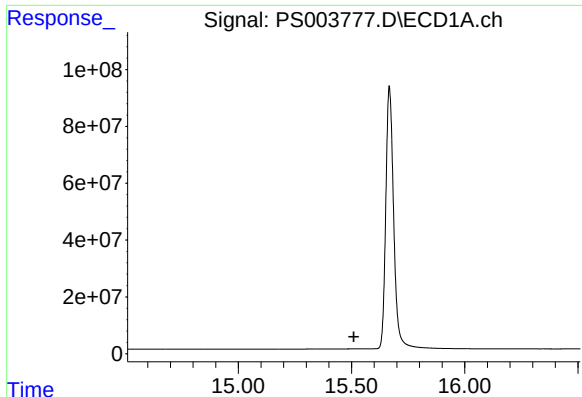

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

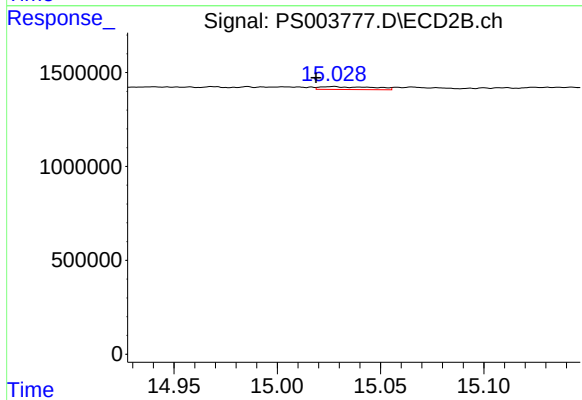


#13 2,4-DB

R.T.: 15.027 min
Delta R.T.: 0.008 min
Response: 270652
Conc: 0.91 ng/ml

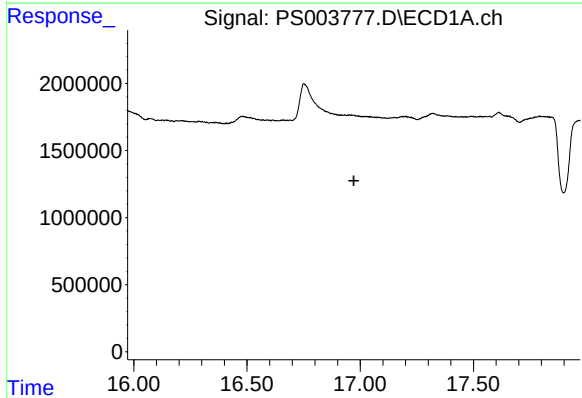


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

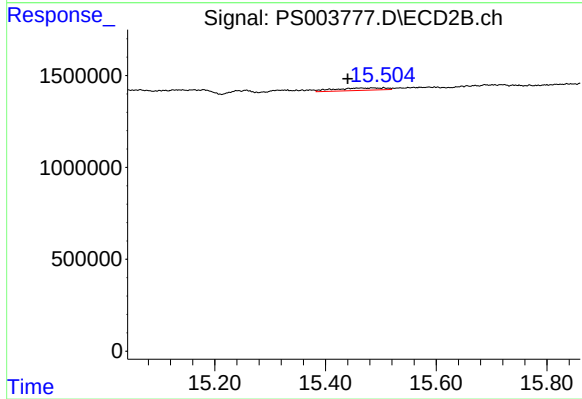

#14 DINOSEB


R.T.: 15.464 min
Delta R.T.: 0.024 min
Response: 818979
Conc: 0.43 ng/ml

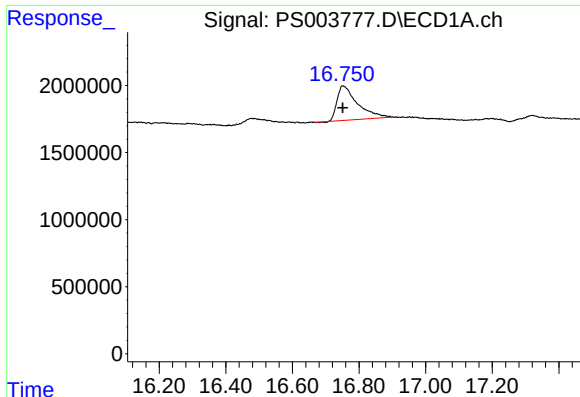

#15 Picloram


R.T.: 16.751 min
Delta R.T.: 0.000 min
Response: 10948114
Conc: 3.22 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

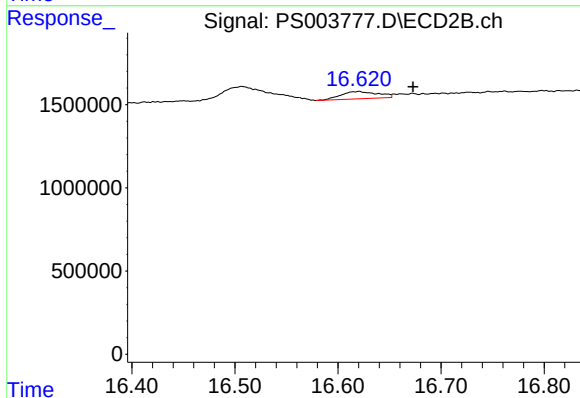


#15 Picloram

R.T.: 16.619 min
Delta R.T.: -0.054 min
Response: 1098168
Conc: 0.35 ng/ml

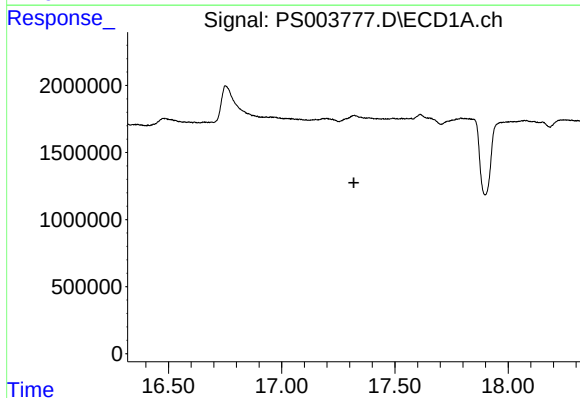

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.319 min
Response: 0
Conc: N.D.

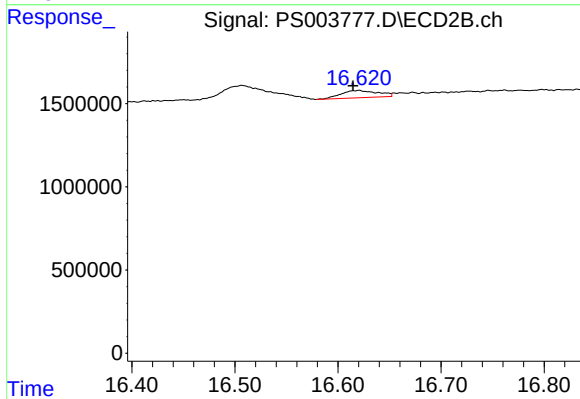

#16 DCPA

R.T.: 16.619 min
Delta R.T.: 0.005 min
Response: 1098168
Conc: 0.32 ng/ml