

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032619\
 Data File : PS003749.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2019 17:45
 Operator : EI\SJ
 Sample : HSTDICC750
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HSTDICC750

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 05:30:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:26:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.267	10.769	334.8E6	374.6E6	750.000	750.000
Target Compounds							
1) T	Dalapon	2.835	2.310	519.2E6	497.7E6	682.500	682.500
2) T	3,5-DICHL...	9.693	8.931	486.8E6	447.8E6	697.500	697.500
3) T	4-Nitroph...	10.865	9.923	159.6E6	158.8E6	682.500	682.500
5) T	DICAMBA	11.569	11.047	1480.9E6	1341.9E6	705.000	705.000
6) T	MCPD	11.911	11.280	101.7E6	86127832	70.500	70.500
7) T	MCPA	12.162	11.655	151.3E6	128.6E6	69.750	69.750
8) T	DICHLORPROP	12.760	12.173	351.7E6	330.8E6	705.000	705.000
9) T	2,4-D	13.125	12.646	356.5E6	380.2E6	705.000	705.000
10) T	Pentachlo...	13.485	13.177	5610.3E6	5024.2E6	712.500	712.500
11) T	2,4,5-TP ...	14.362	13.803	2089.4E6	1914.7E6	712.500	712.500
12) T	2,4,5-T	14.763	14.367	2081.0E6	1563.3E6	712.500	712.500
13) T	2,4-DB	15.510	15.019	224.2E6	214.5E6	712.500	712.500
14) T	DINOSEB	16.972	15.440	1694.8E6	1373.6E6	705.000	705.000
15) T	Picloram	16.752	16.673	2548.3E6	2361.2E6	712.500	712.500
16) T	DCPA	17.319	16.615	2642.9E6	2475.9E6	720.000	720.000



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032619\
Data File : PS003749.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2019 17:45
Operator : EI\SJ
Sample : HSTDICC750
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 05:30:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:26:07 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

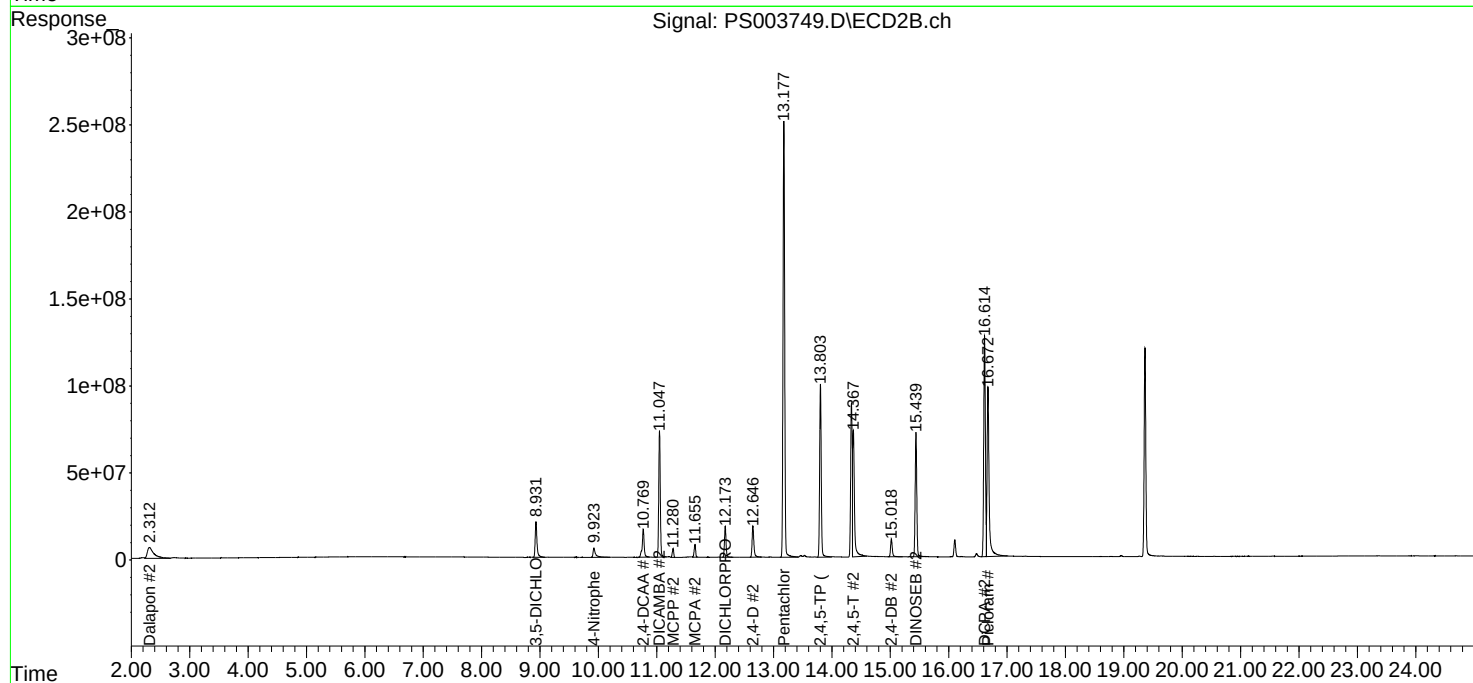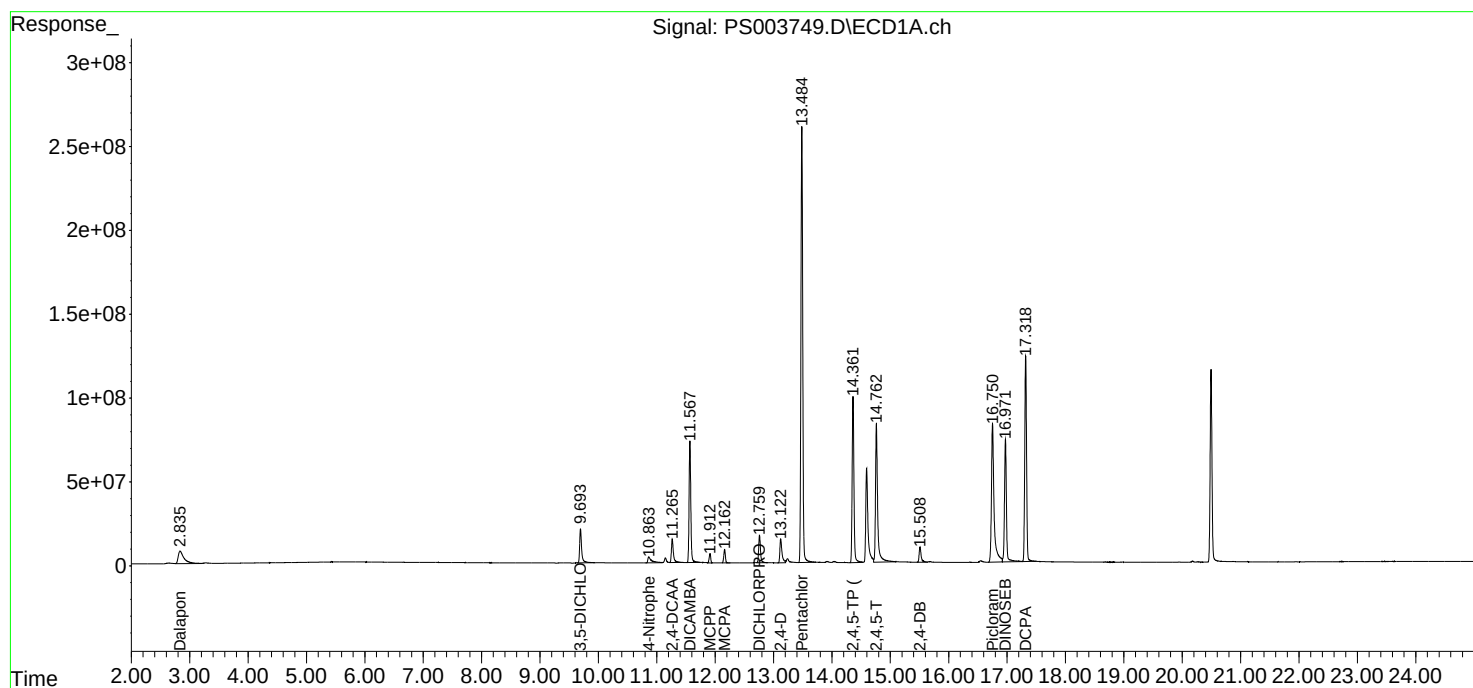


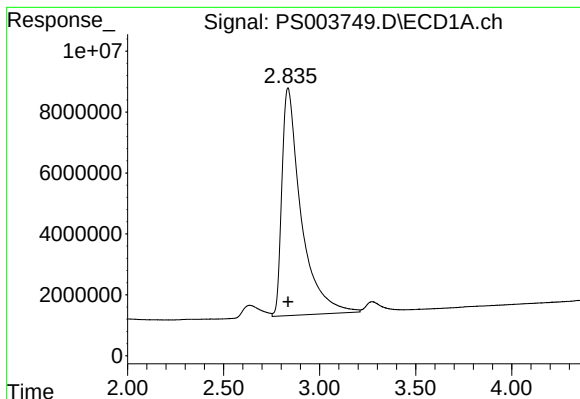

#1 Dalapon


R.T.: 2.835 min
Delta R.T.: 0.000 min
Response: 519162892
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

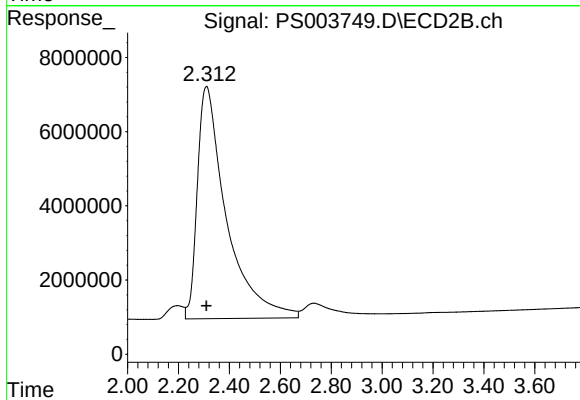


#1 Dalapon

R.T.: 2.310 min
Delta R.T.: 0.000 min
Response: 497668061
Conc: 682.50 ng/ml

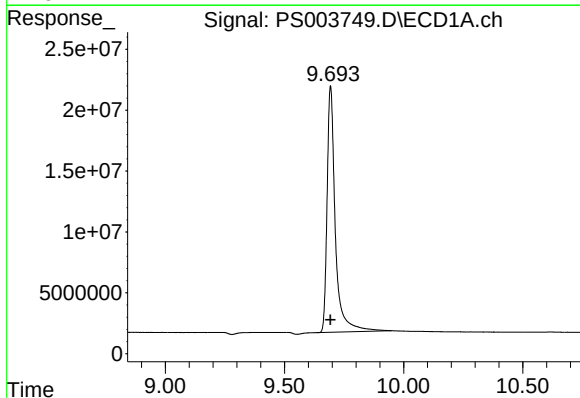


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 9.693 min
Delta R.T.: 0.000 min
Response: 486787130
Conc: 697.50 ng/ml

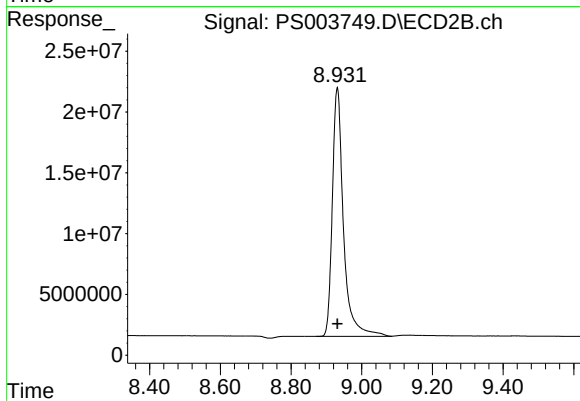

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.931 min
Delta R.T.: 0.000 min
Response: 447784927
Conc: 697.50 ng/ml

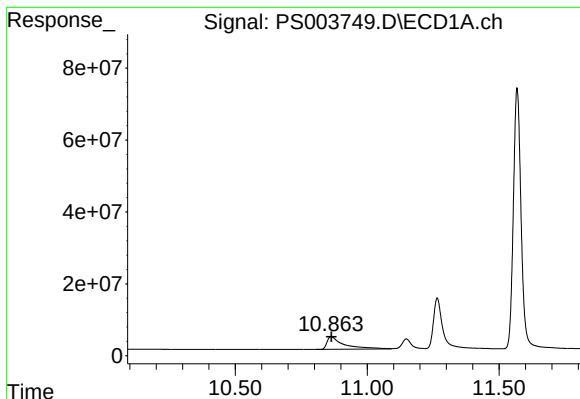

#3 4-Nitrophenol


R.T.: 10.865 min
Delta R.T.: 0.000 min
Response: 159557851
Conc: 682.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

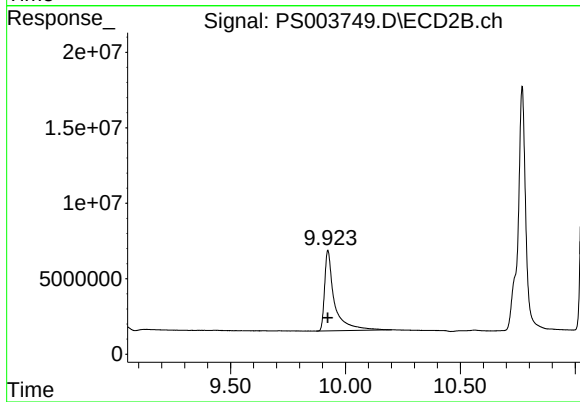


#3 4-Nitrophenol

R.T.: 9.923 min
Delta R.T.: 0.000 min
Response: 158831168
Conc: 682.50 ng/ml

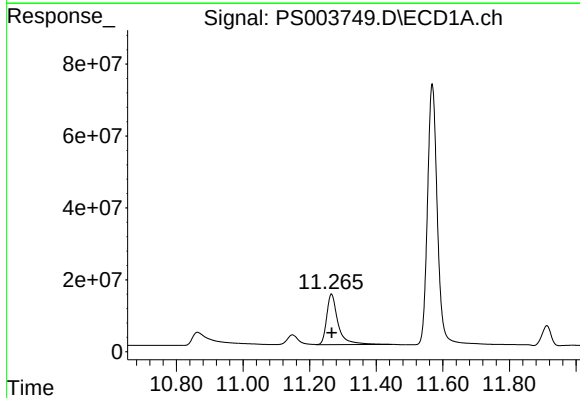


#4 2,4-DCAA

R.T.: 11.267 min
Delta R.T.: 0.000 min
Response: 334773352
Conc: 750.00 ng/ml

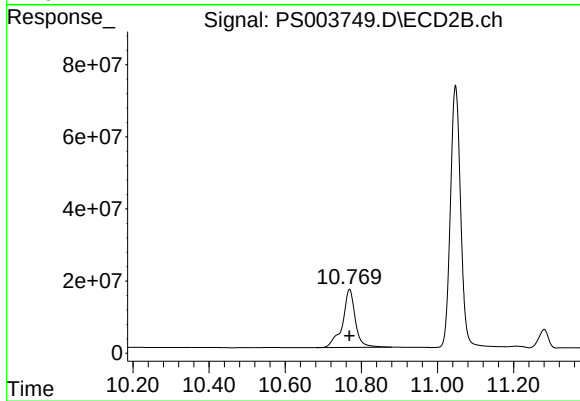

#4 2,4-DCAA


R.T.: 10.769 min
Delta R.T.: 0.000 min
Response: 374552278
Conc: 750.00 ng/ml

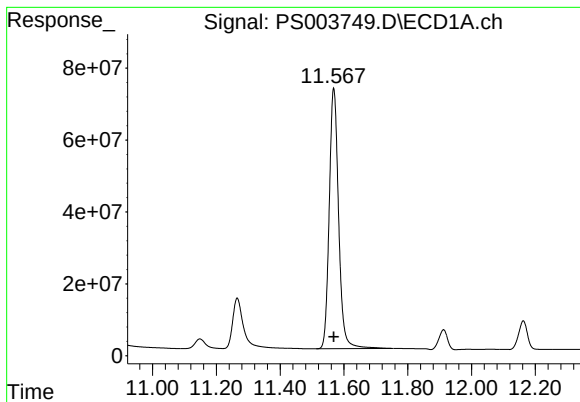

#5 DICAMBA


R.T.: 11.569 min
Delta R.T.: 0.000 min
Response: 1480895071
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

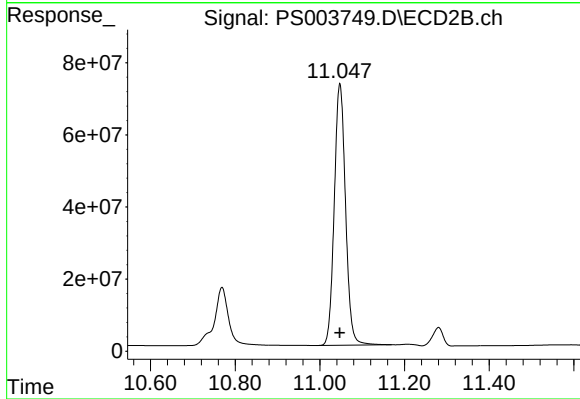


#5 DICAMBA

R.T.: 11.047 min
Delta R.T.: 0.000 min
Response: 1341927969
Conc: 705.00 ng/ml

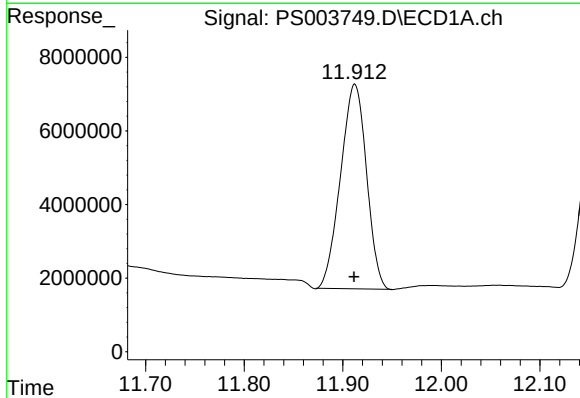


#6 MCP

R.T.: 11.911 min
Delta R.T.: 0.000 min
Response: 101710820
Conc: 70.50 ug/ml

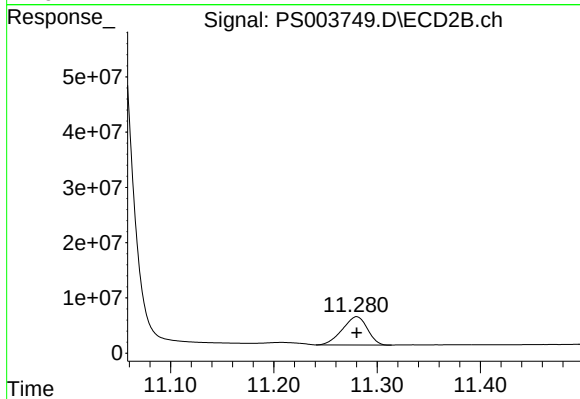

#6 MCP


R.T.: 11.280 min
Delta R.T.: 0.000 min
Response: 86127832
Conc: 70.50 ug/ml

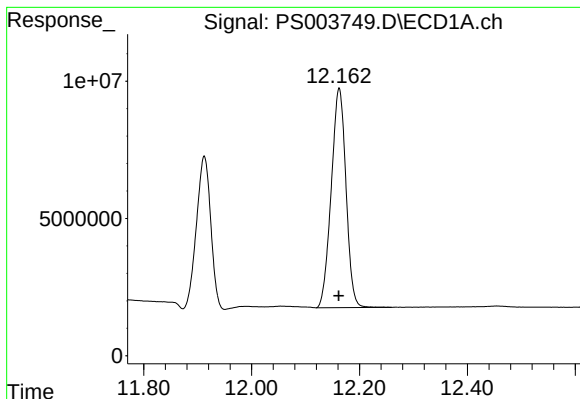

#7 MCPA


R.T.: 12.162 min
Delta R.T.: 0.000 min
Response: 151319986
Conc: 69.75 ug/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

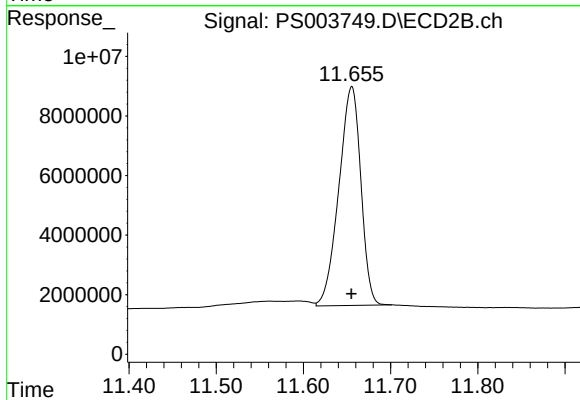


#7 MCPA

R.T.: 11.655 min
Delta R.T.: 0.000 min
Response: 128573847
Conc: 69.75 ug/ml

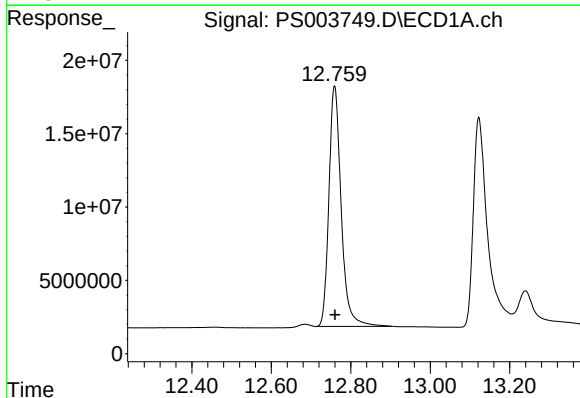


#8 DICHLORPROP

R.T.: 12.760 min
Delta R.T.: 0.000 min
Response: 351705482
Conc: 705.00 ng/ml

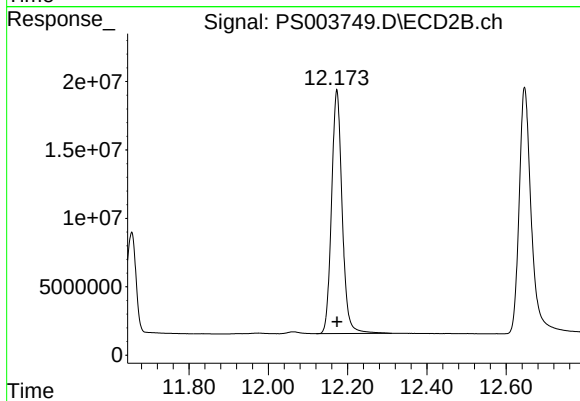

#8 DICHLORPROP


R.T.: 12.173 min
Delta R.T.: 0.000 min
Response: 330777622
Conc: 705.00 ng/ml

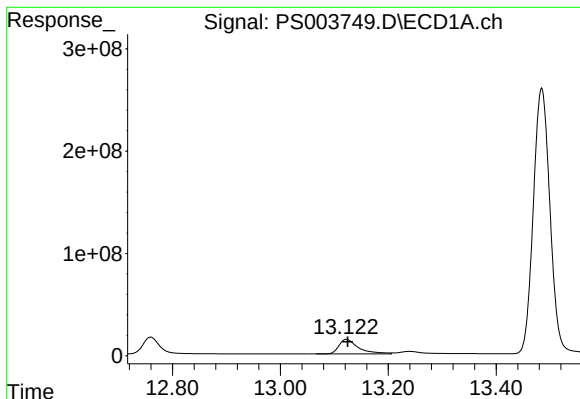

#9 2,4-D


R.T.: 13.125 min
Delta R.T.: 0.000 min
Response: 356545293
Conc: 705.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

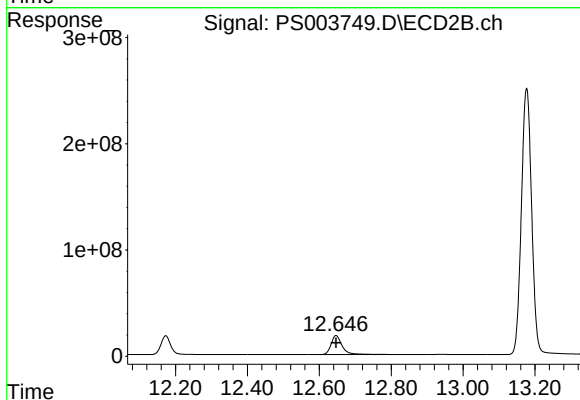


#9 2,4-D

R.T.: 12.646 min
Delta R.T.: 0.000 min
Response: 380200827
Conc: 705.00 ng/ml

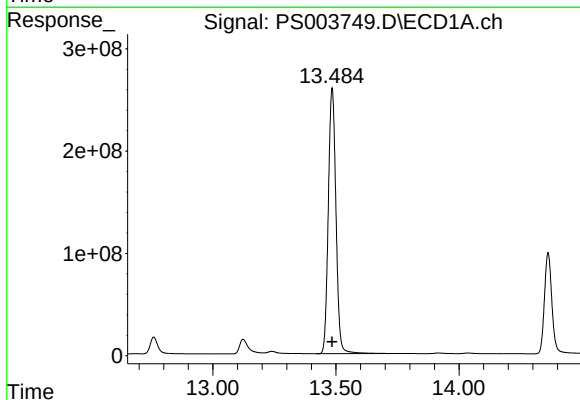


#10 Pentachlorophenol

R.T.: 13.485 min
Delta R.T.: 0.000 min
Response: 5610334506
Conc: 712.50 ng/ml

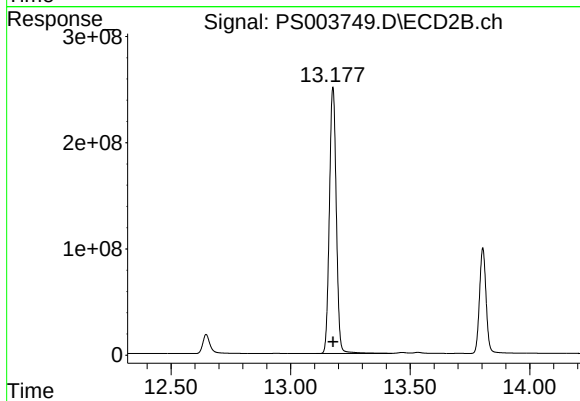

#10 Pentachlorophenol


R.T.: 13.177 min
Delta R.T.: 0.000 min
Response: 5024172964
Conc: 712.50 ng/ml

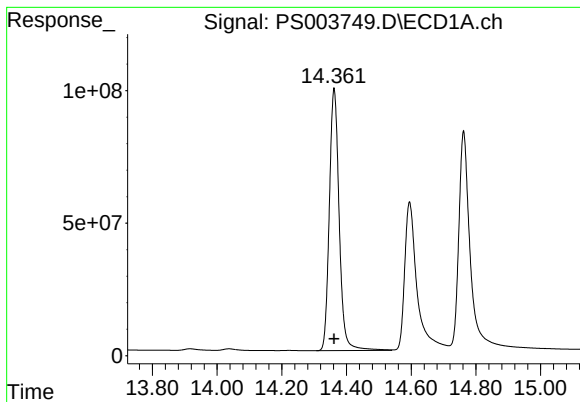

#11 2,4,5-TP (SILVEX)


R.T.: 14.362 min
Delta R.T.: 0.000 min
Response: 2089357163
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

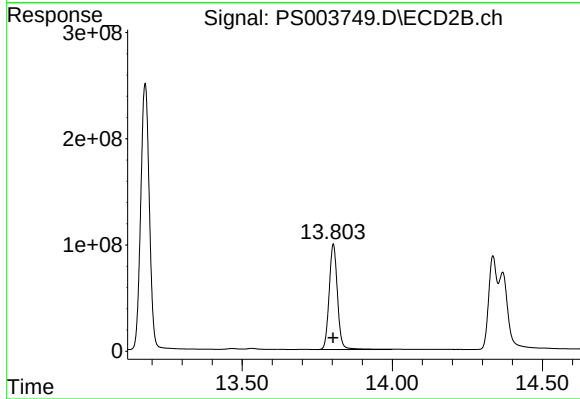


#11 2,4,5-TP (SILVEX)

R.T.: 13.803 min
Delta R.T.: 0.000 min
Response: 1914679201
Conc: 712.50 ng/ml

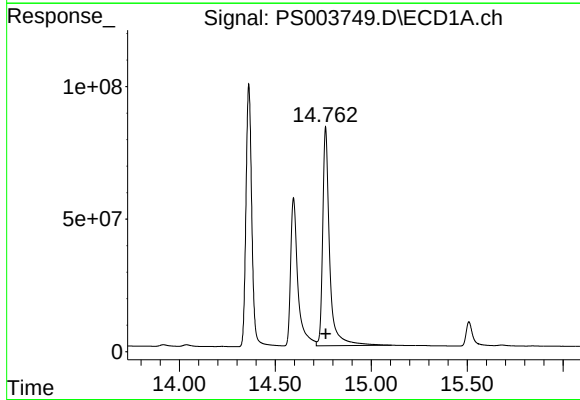


#12 2,4,5-T

R.T.: 14.763 min
Delta R.T.: 0.000 min
Response: 2080961252
Conc: 712.50 ng/ml

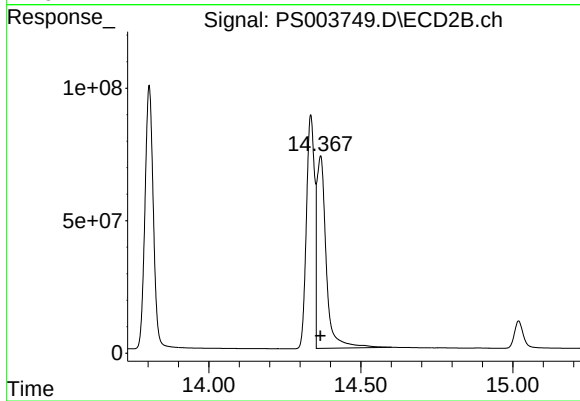

#12 2,4,5-T


R.T.: 14.367 min
Delta R.T.: 0.000 min
Response: 1563260381
Conc: 712.50 ng/ml

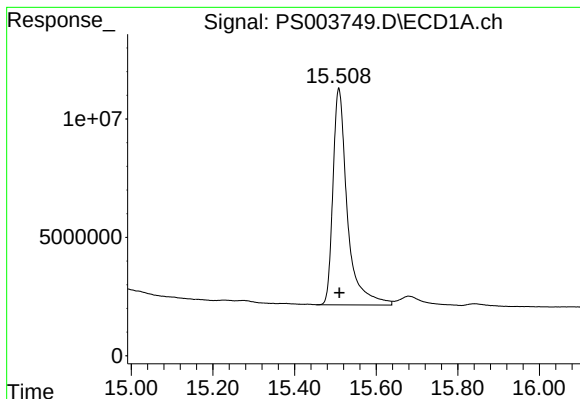

#13 2,4-DB


R.T.: 15.510 min
Delta R.T.: 0.000 min
Response: 224186450
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

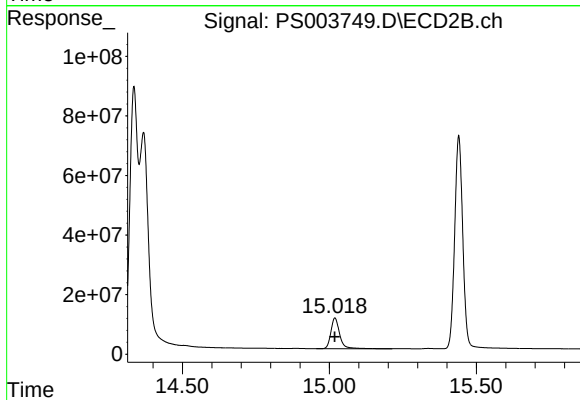


#13 2,4-DB

R.T.: 15.019 min
Delta R.T.: 0.000 min
Response: 214462403
Conc: 712.50 ng/ml

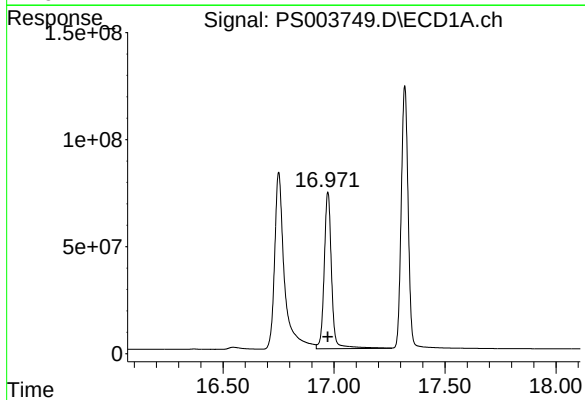


#14 DINOSEB

R.T.: 16.972 min
Delta R.T.: 0.000 min
Response: 1694751291
Conc: 705.00 ng/ml

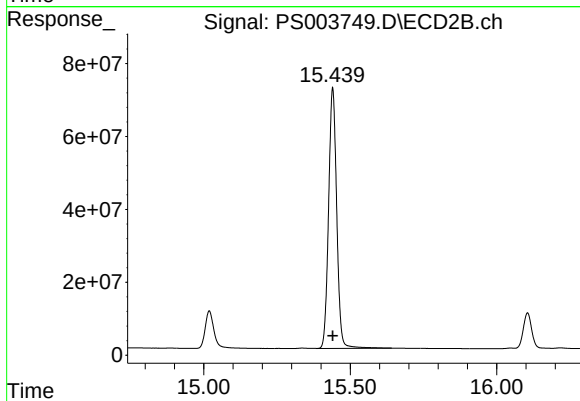

#14 DINOSEB


R.T.: 15.440 min
Delta R.T.: 0.000 min
Response: 1373606290
Conc: 705.00 ng/ml

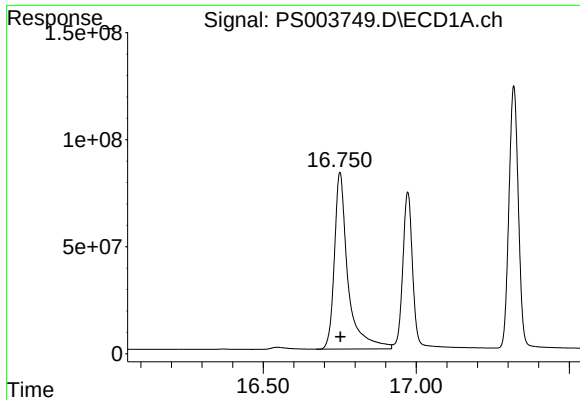

#15 Picloram


R.T.: 16.752 min
Delta R.T.: 0.000 min
Response: 2548276365
Conc: 712.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
HSTDICC750

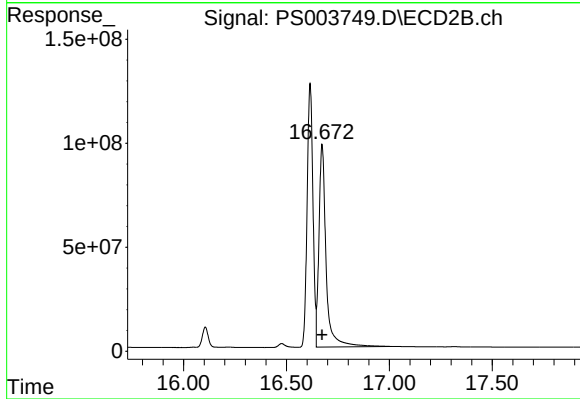


#15 Picloram

R.T.: 16.673 min
Delta R.T.: 0.000 min
Response: 2361246796
Conc: 712.50 ng/ml

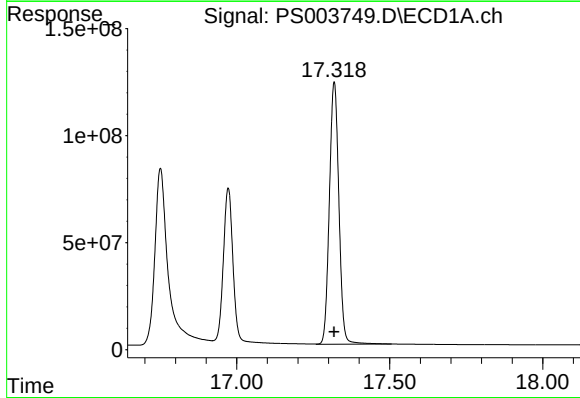

#16 DCPA

R.T.: 17.319 min
Delta R.T.: 0.000 min
Response: 2642893228
Conc: 720.00 ng/ml

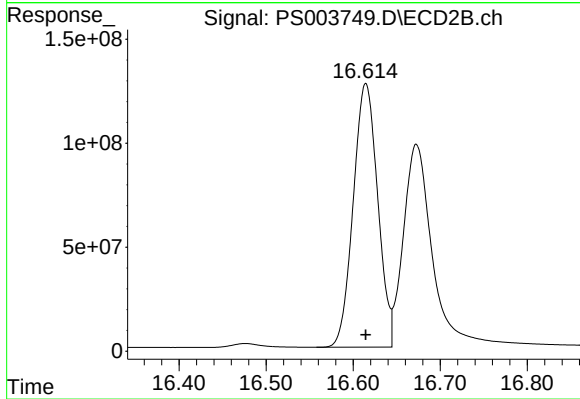

#16 DCPA

R.T.: 16.615 min
Delta R.T.: 0.000 min
Response: 2475932760
Conc: 720.00 ng/ml