

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
 Data File : PS009437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 16:40
 Operator : DD\AJ
 Sample : PB127761BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 17:56:33 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.930	323.7E6	307.3E6	585.194	559.602
Target Compounds							
2) T	3,5-DICHL...	0.000	6.106	0 50342286		N.D.	61.898
6) T	MCP	7.602	0.000	7114801	0	2.891	N.D. #
7) T	MCPA	7.797	7.397	69809562	34759621	22.921	12.881 #
8) T	DICHLORPROP	0.000	7.749	0 28073351		N.D.	50.599
11) T	2,4,5-TP ...	0.000	8.784	0 37157251		N.D.	12.464
12) T	2,4,5-T	9.456	0.000	17525653	0	6.889	N.D. #
13) T	2,4-DB	0.000	9.644	0 6834450		N.D.	18.004
14) T	DINOSEB	11.193	10.046	11993677	17266666	5.867	7.861 #
15) T	Picloram	11.041	11.020	28949145	37686962	9.539	9.255
16) T	DCPA	0.000	11.020	0 37686962		N.D.	9.731



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
Data File : PS009437.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 16:40
Operator : DD\AJ
Sample : PB127761BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 17:56:33 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

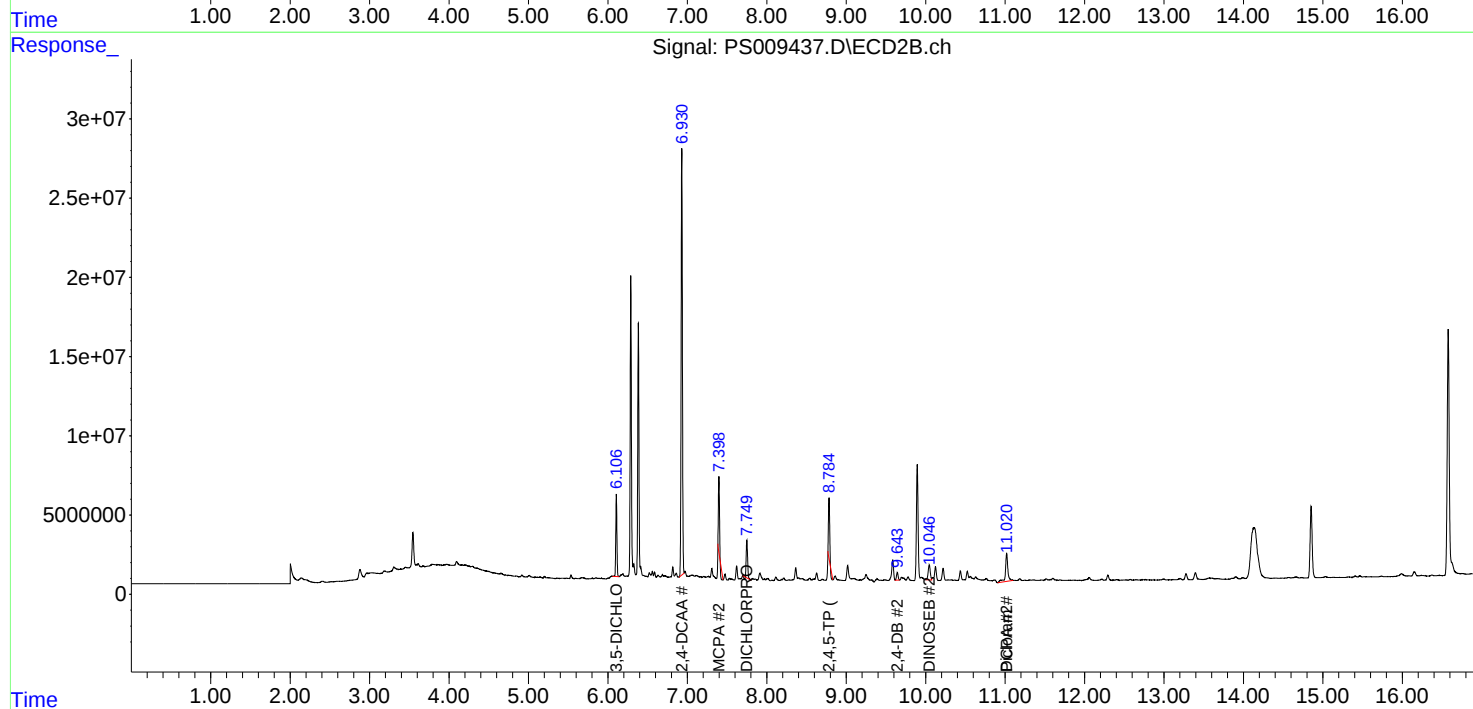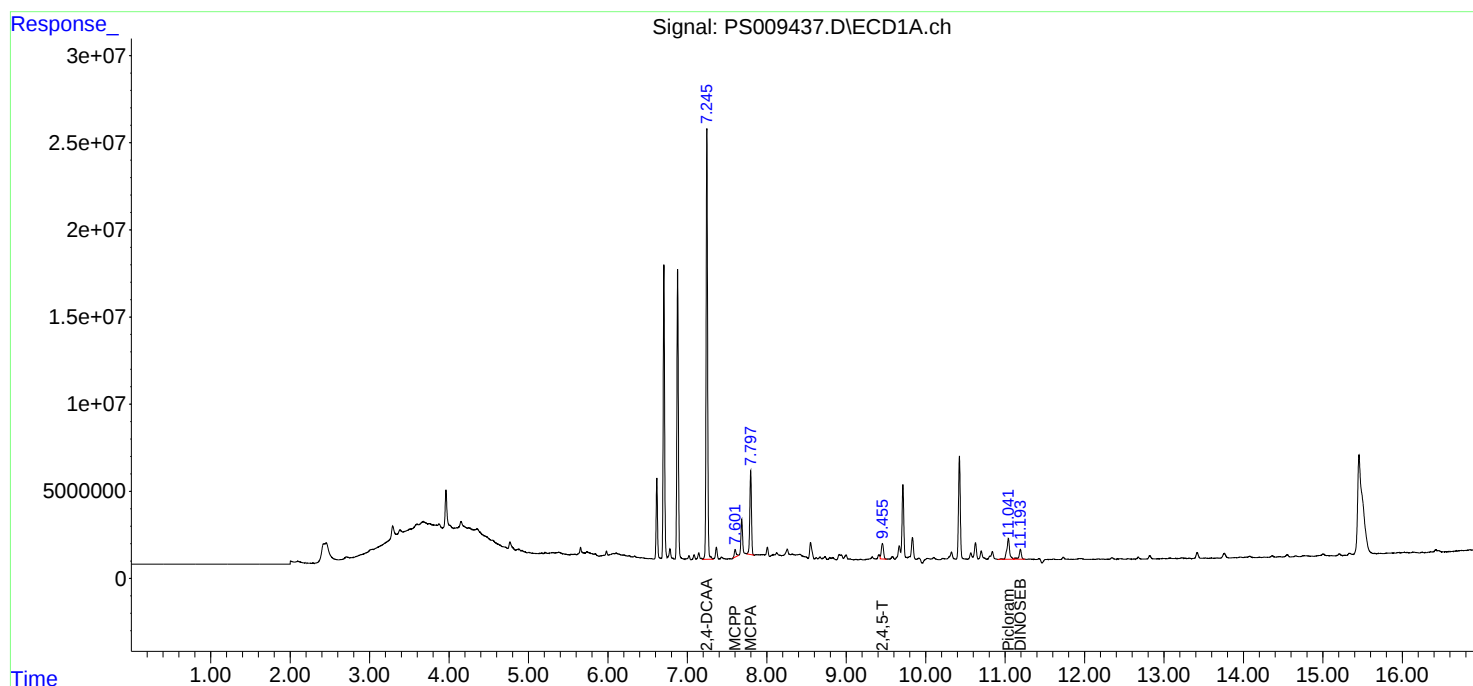


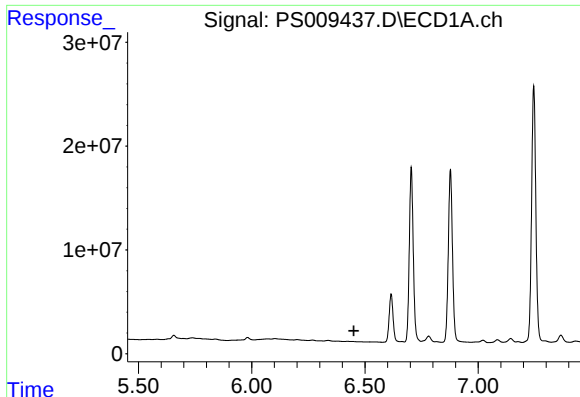

#2 3,5-DICHLORO BENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

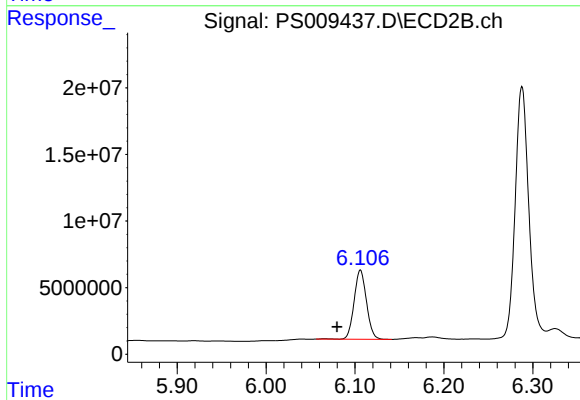


#2 3,5-DICHLORO BENZOIC ACID

R.T.: 6.106 min
Delta R.T.: 0.026 min
Response: 50342286
Conc: 61.90 ng/ml

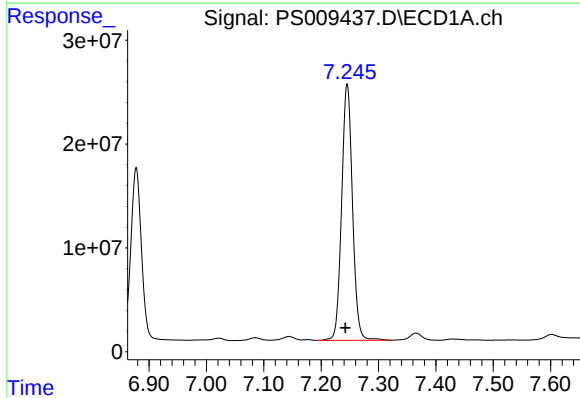


#4 2,4-DCAA

R.T.: 7.245 min
Delta R.T.: 0.004 min
Response: 323711831
Conc: 585.19 ng/ml

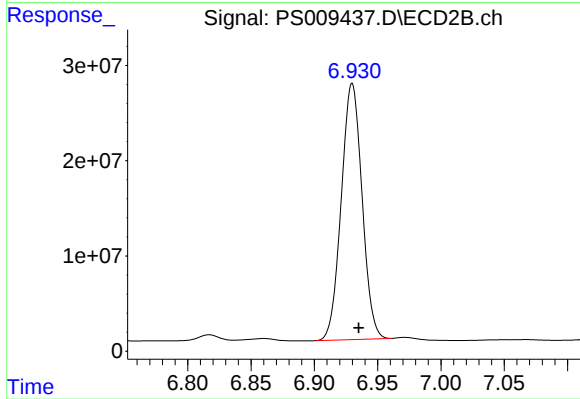

#4 2,4-DCAA


R.T.: 6.930 min
Delta R.T.: -0.005 min
Response: 307332016
Conc: 559.60 ng/ml

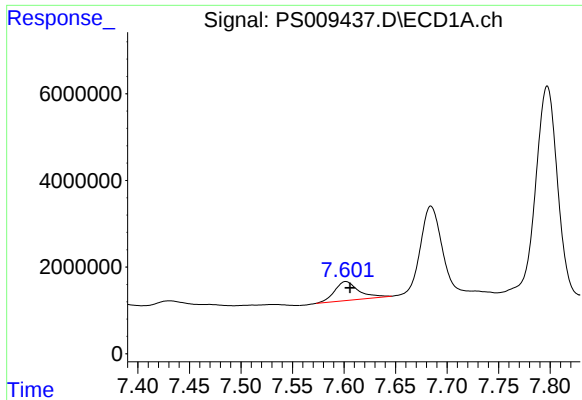

#6 MCPP


R.T.: 7.602 min
Delta R.T.: -0.004 min
Response: 7114801
Conc: 2.89 ug/ml

Instrument :
ECD_S
ClientSampleId :

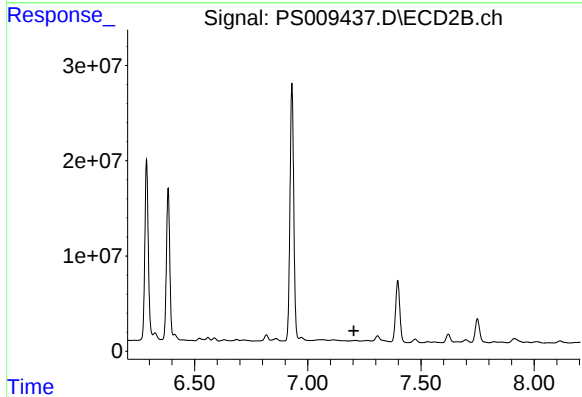


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 7.204 min
Response: 0
Conc: N.D.

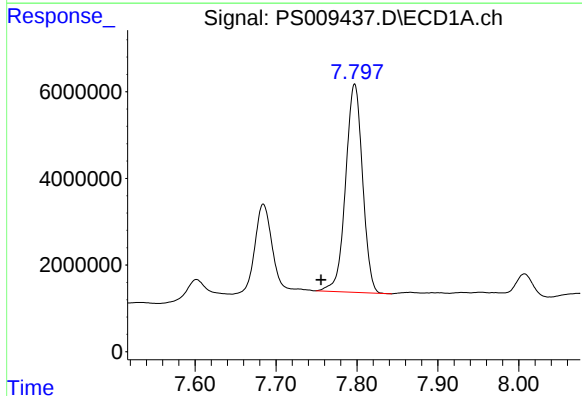


#7 MCPA

R.T.: 7.797 min
Delta R.T.: 0.042 min
Response: 69809562
Conc: 22.92 ug/ml

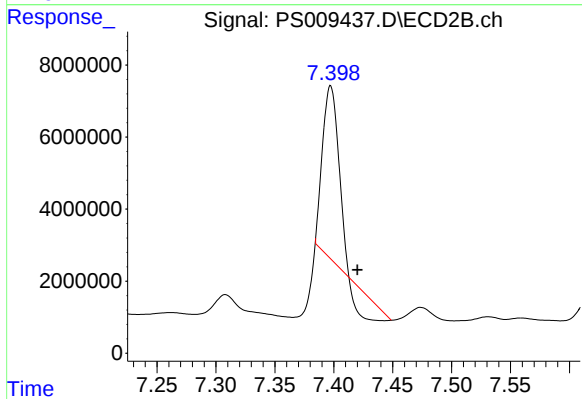

#7 MCPA


R.T.: 7.397 min
Delta R.T.: -0.023 min
Response: 34759621
Conc: 12.88 ug/ml

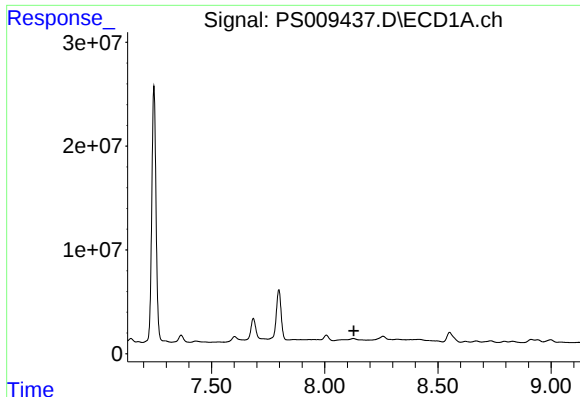

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

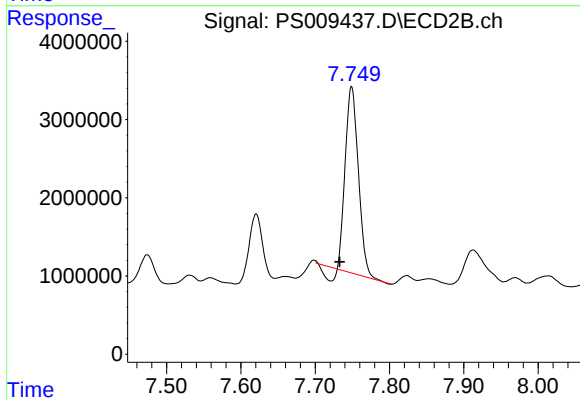


#8 DICHLORPROP

R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 28073351
Conc: 50.60 ng/ml

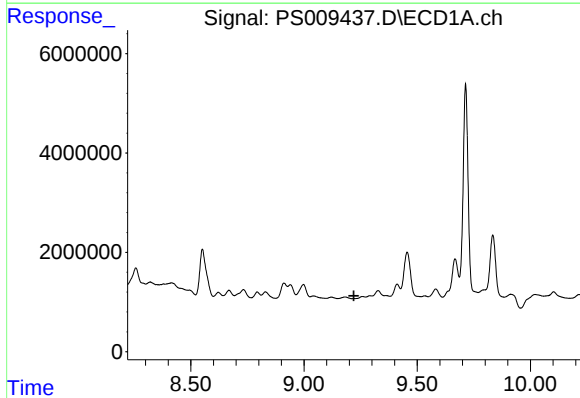


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

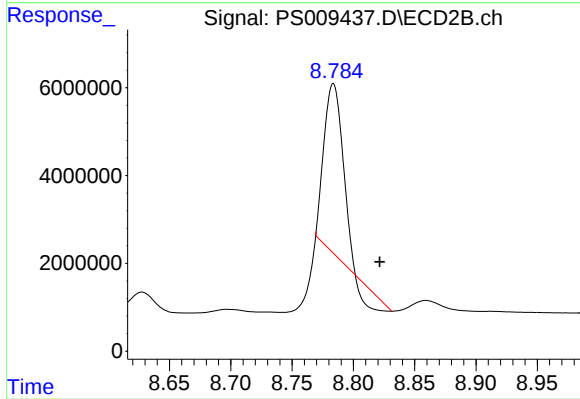

#11 2,4,5-TP (SILVEX)


R.T.: 8.784 min
Delta R.T.: -0.038 min
Response: 37157251
Conc: 12.46 ng/ml

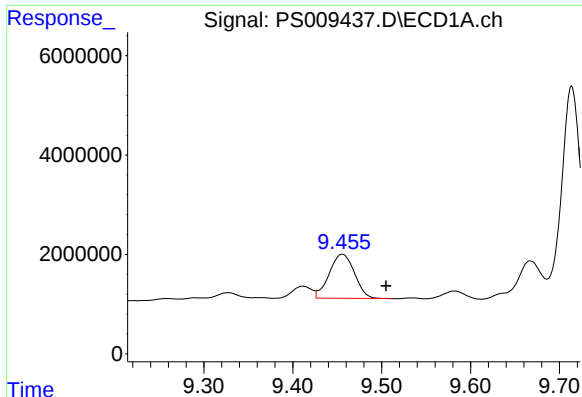

#12 2,4,5-T


R.T.: 9.456 min
Delta R.T.: -0.049 min
Response: 17525653
Conc: 6.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

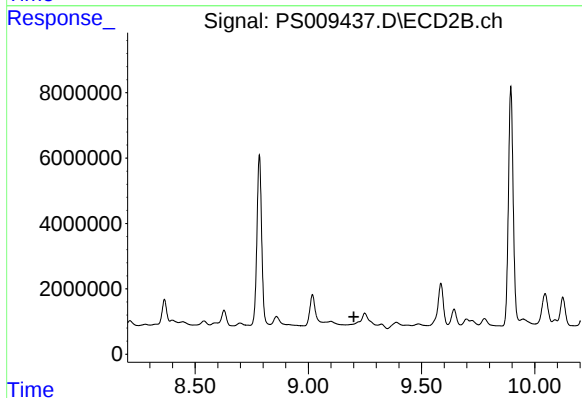


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

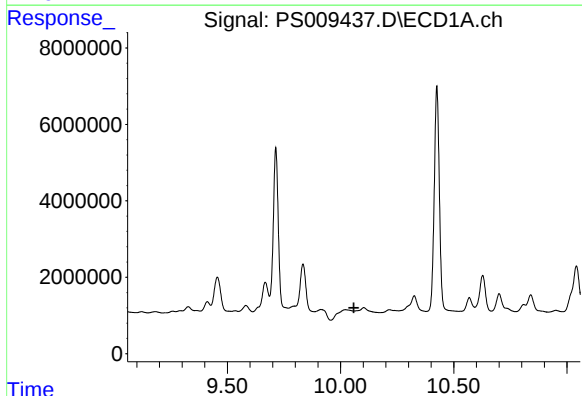


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.059 min
Response: 0
Conc: N.D.

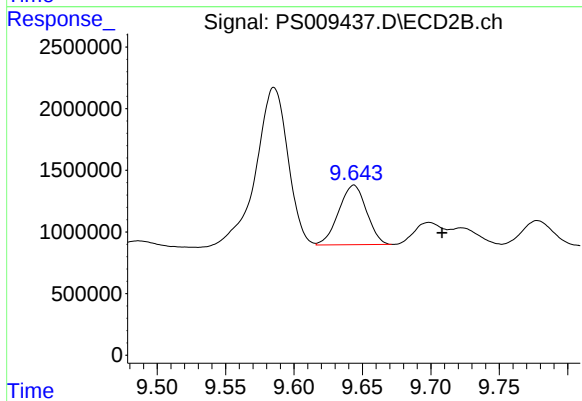

#13 2,4-DB


R.T.: 9.644 min
Delta R.T.: -0.064 min
Response: 6834450
Conc: 18.00 ng/ml

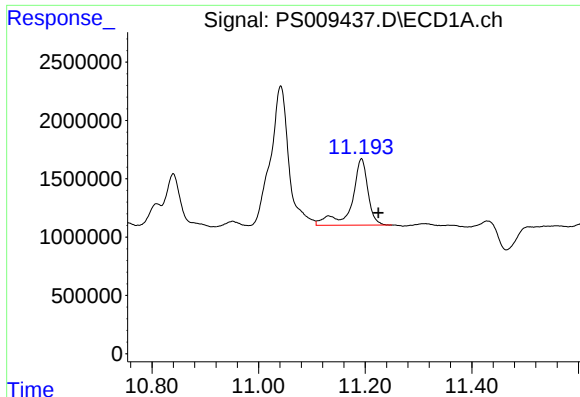

#14 DINOSEB


R.T.: 11.193 min
Delta R.T.: -0.032 min
Response: 11993677
Conc: 5.87 ng/ml

Instrument :
ECD_S
ClientSampleId :

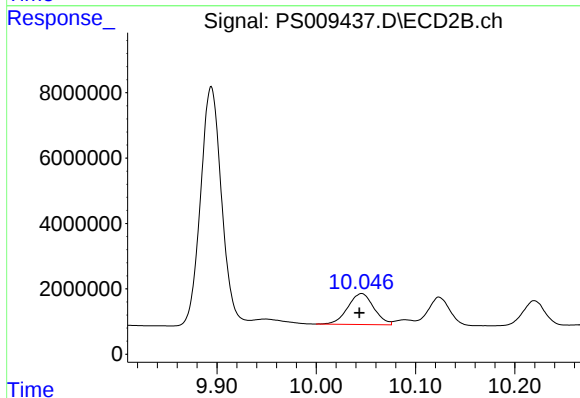


#14 DINOSEB

R.T.: 10.046 min
Delta R.T.: 0.002 min
Response: 17266666
Conc: 7.86 ng/ml

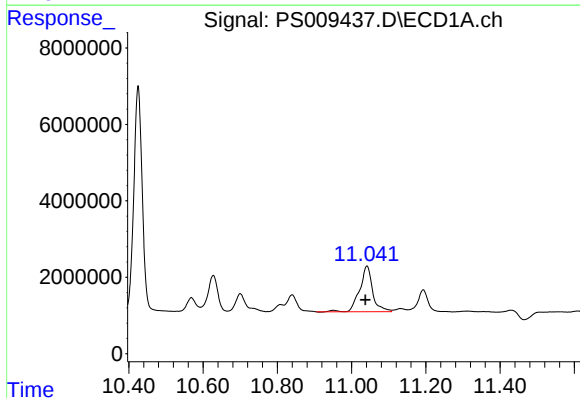


#15 Picloram

R.T.: 11.041 min
Delta R.T.: 0.004 min
Response: 28949145
Conc: 9.54 ng/ml

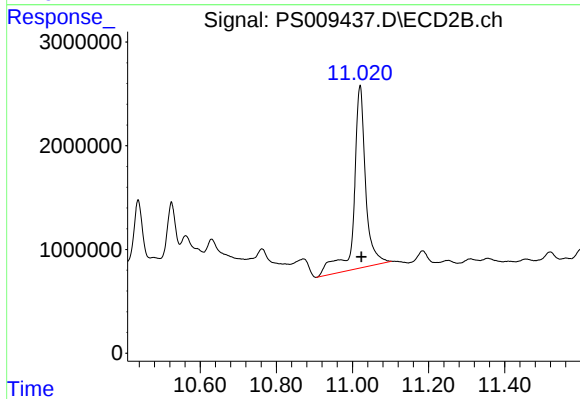

#15 Picloram


R.T.: 11.020 min
Delta R.T.: -0.003 min
Response: 37686962
Conc: 9.25 ng/ml

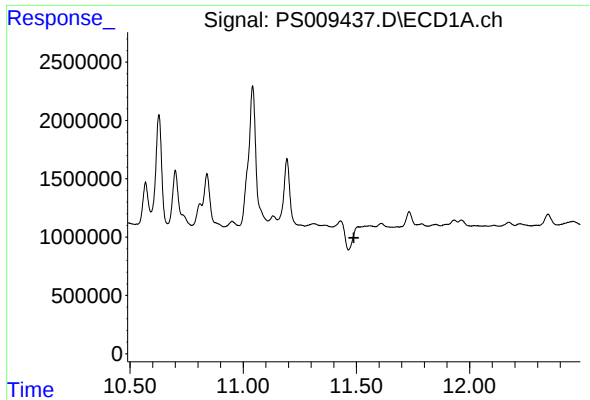

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

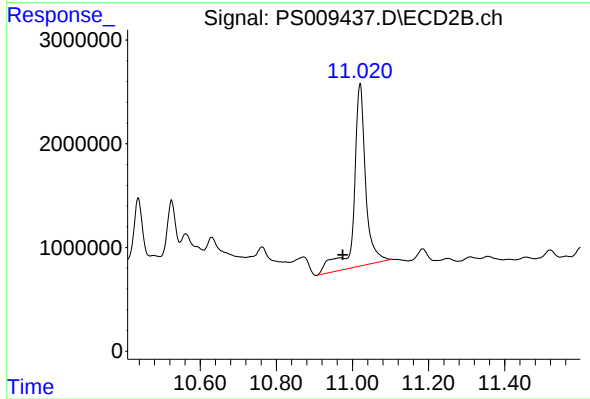

#16 DCPA

R.T.: 11.020 min
Delta R.T.: 0.046 min
Response: 37686962
Conc: 9.73 ng/ml