

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
 Data File : PS009448.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 20:52
 Operator : DD\AJ
 Sample : PB127812BL
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB127812BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:28:48 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.931	328.0E6	313.5E6	592.912	570.821
Target Compounds							
2) T	3,5-DICHL...	0.000	6.108	0 78394140		N.D.	96.389
5) T	DICAMBA	0.000	7.066	0 11379436		N.D.	4.957
6) T	MCP	7.596	0.000	10006017	0	4.066	N.D. #
7) T	MCPA	7.792	7.399	71980277	41215146	23.634	15.273 #
8) T	DICHLORPROP	0.000	7.750	0 28741434		N.D.	51.803
11) T	2,4,5-TP ...	0.000	8.785	0 29424371		N.D.	9.870
12) T	2,4,5-T	9.528	9.249	6867625	28736824	2.700	9.734 #
14) T	DINOSEB	0.000	10.049	0 10652843		N.D.	4.850
15) T	Picloram	11.036	11.018	97433833	136.3E6	32.104	33.461
16) T	DCPA	0.000	11.018	0 136.3E6		N.D.	35.181



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
Data File : PS009448.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 20:52
Operator : DD\AJ
Sample : PB127812BL
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB127812BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:28:48 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

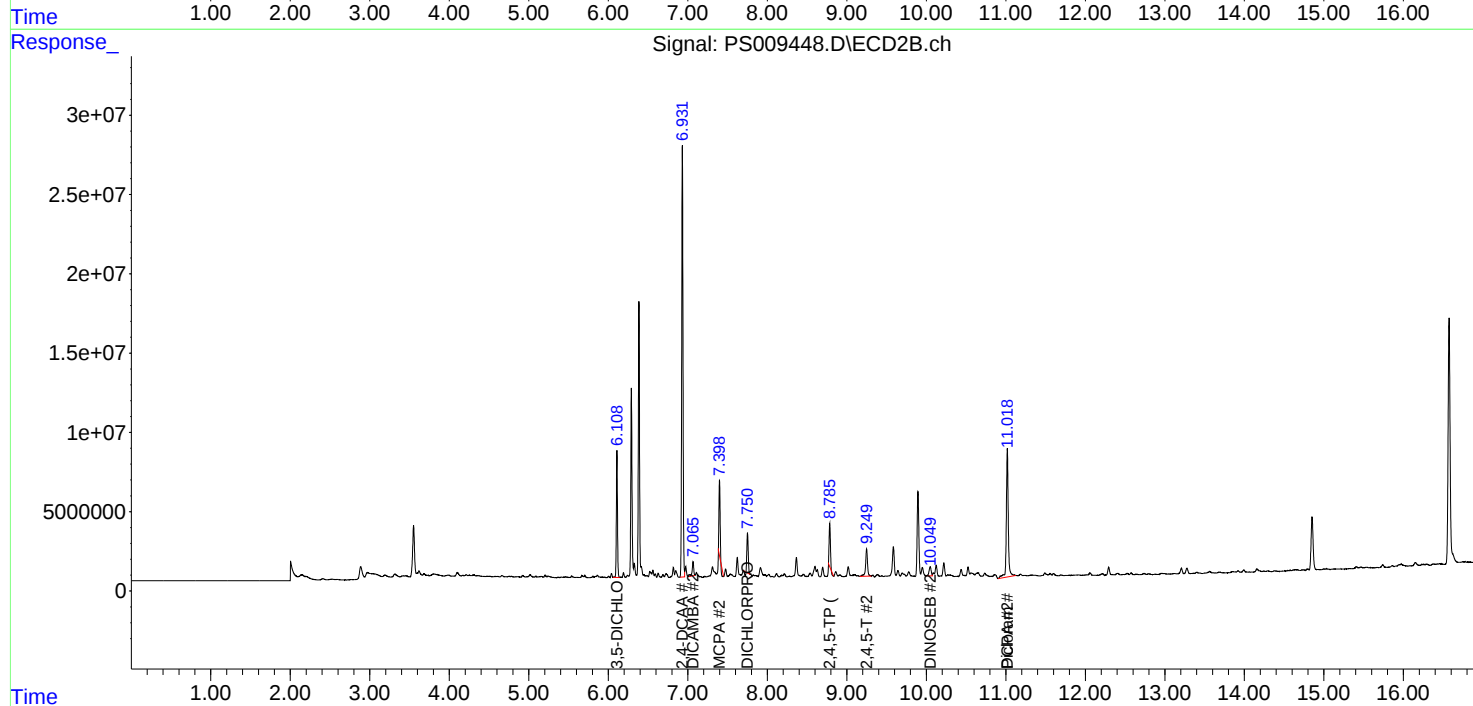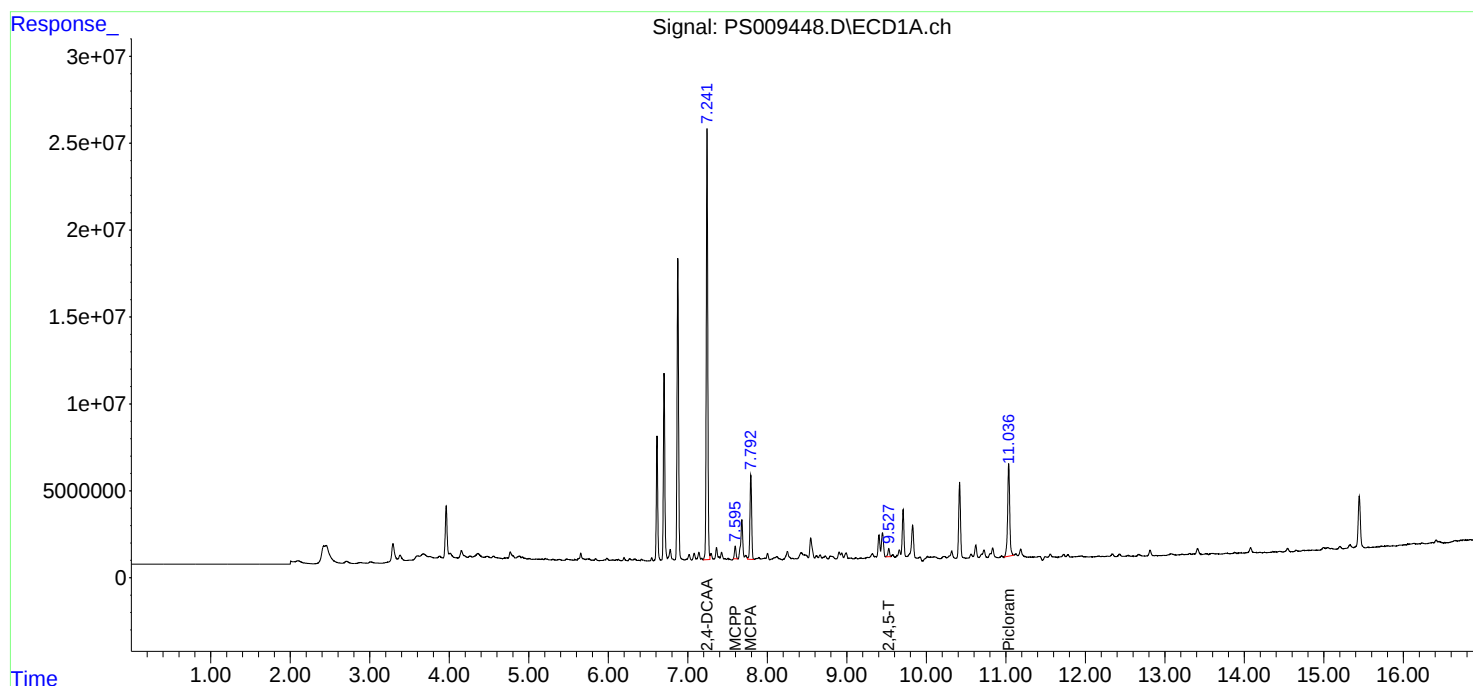


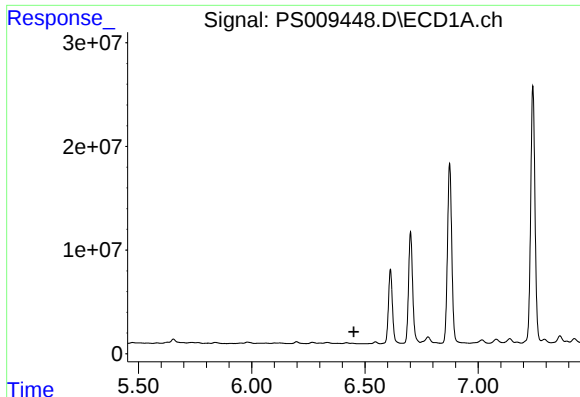

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127812BL

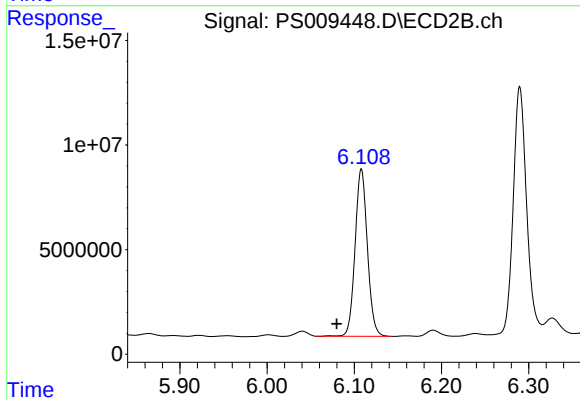


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.108 min
Delta R.T.: 0.028 min
Response: 78394140
Conc: 96.39 ng/ml

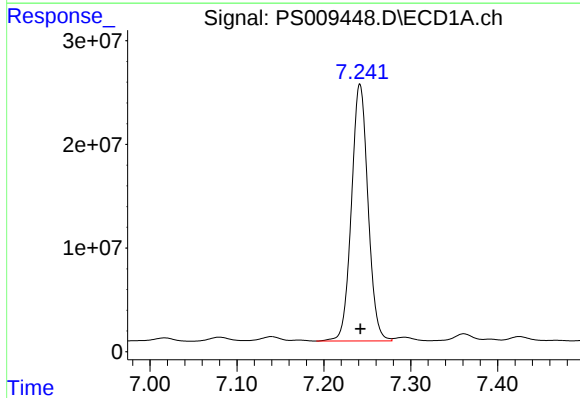


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 327981199
Conc: 592.91 ng/ml

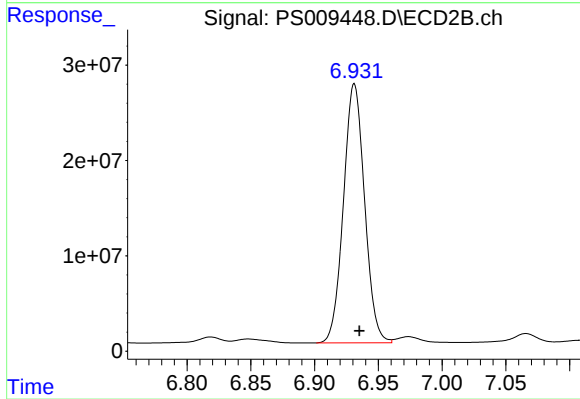

#4 2,4-DCAA


R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 313493528
Conc: 570.82 ng/ml

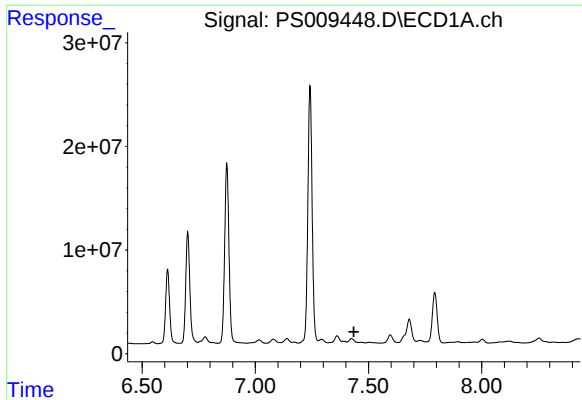

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 7.435 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127812BL

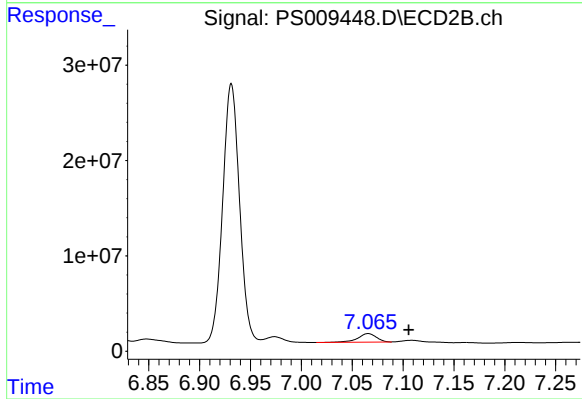


#5 DICAMBA

R.T.: 7.066 min
Delta R.T.: -0.040 min
Response: 11379436
Conc: 4.96 ng/ml

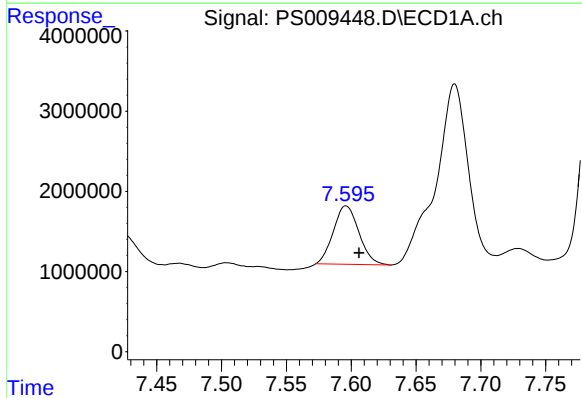


#6 MCP

R.T.: 7.596 min
Delta R.T.: -0.010 min
Response: 10006017
Conc: 4.07 ug/ml

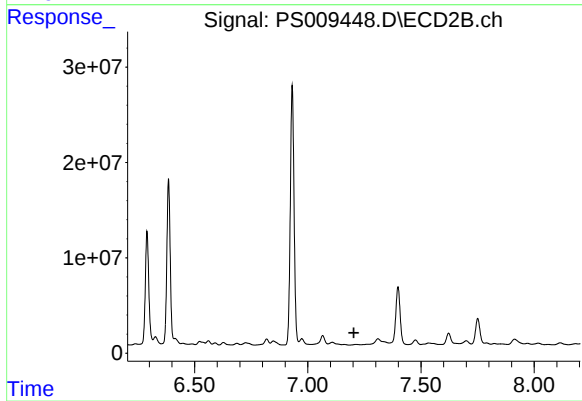

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

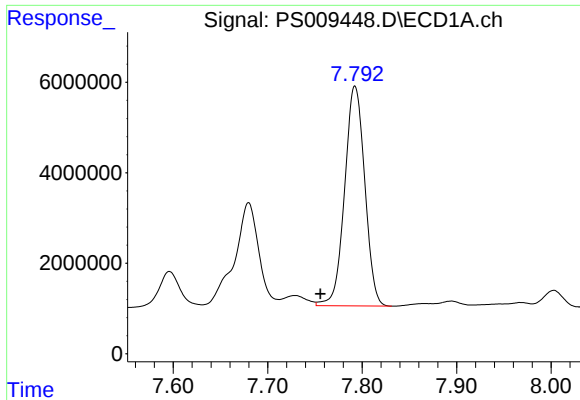

#7 MCPA


R.T.: 7.792 min
Delta R.T.: 0.037 min
Response: 71980277
Conc: 23.63 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB127812BL

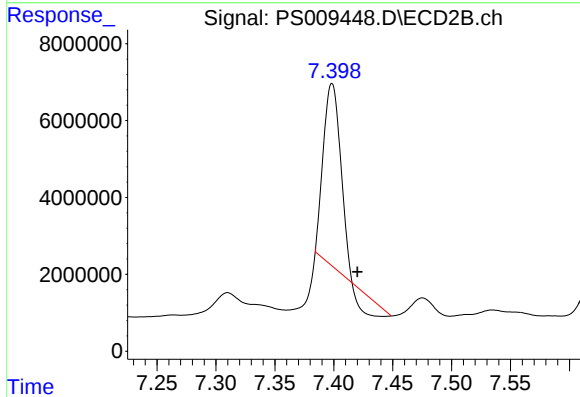


#7 MCPA

R.T.: 7.399 min
Delta R.T.: -0.021 min
Response: 41215146
Conc: 15.27 ug/ml

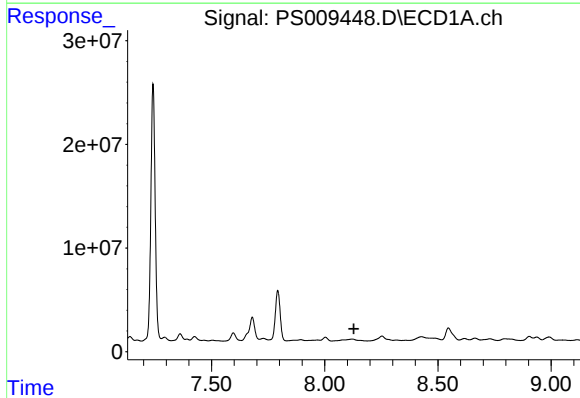


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

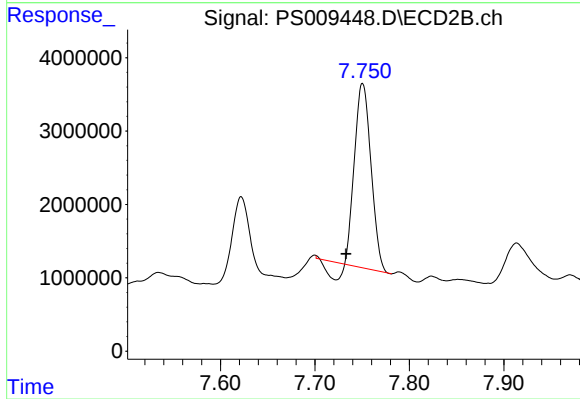

#8 DICHLORPROP


R.T.: 7.750 min
Delta R.T.: 0.017 min
Response: 28741434
Conc: 51.80 ng/ml

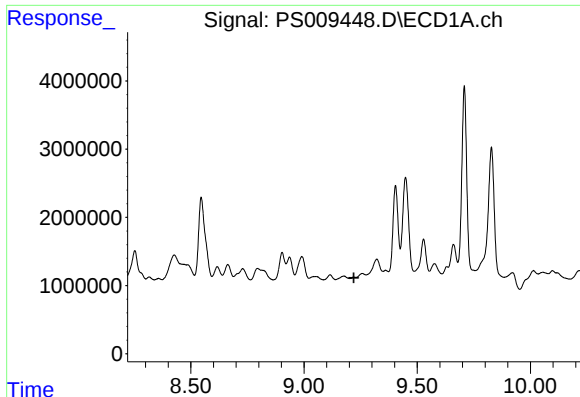

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 9.221 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127812BL

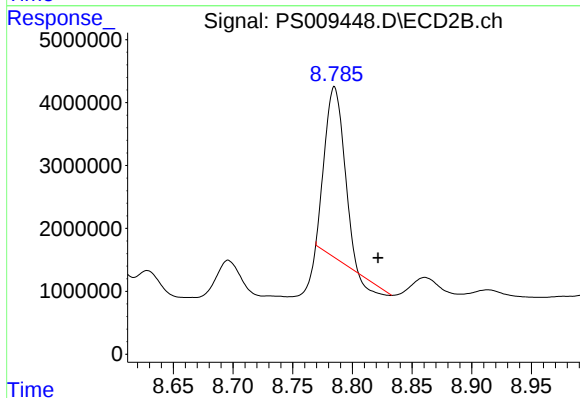


#11 2,4,5-TP (SILVEX)

R.T.: 8.785 min
Delta R.T.: -0.037 min
Response: 29424371
Conc: 9.87 ng/ml

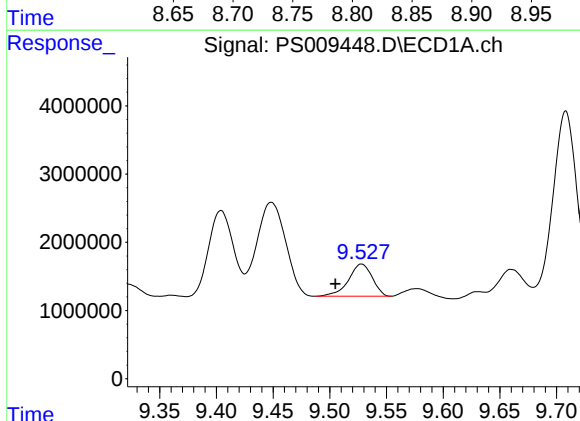


#12 2,4,5-T

R.T.: 9.528 min
Delta R.T.: 0.023 min
Response: 6867625
Conc: 2.70 ng/ml

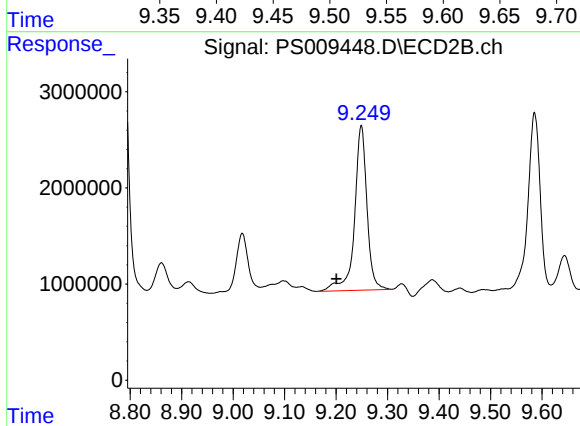

#12 2,4,5-T


R.T.: 9.249 min
Delta R.T.: 0.048 min
Response: 28736824
Conc: 9.73 ng/ml

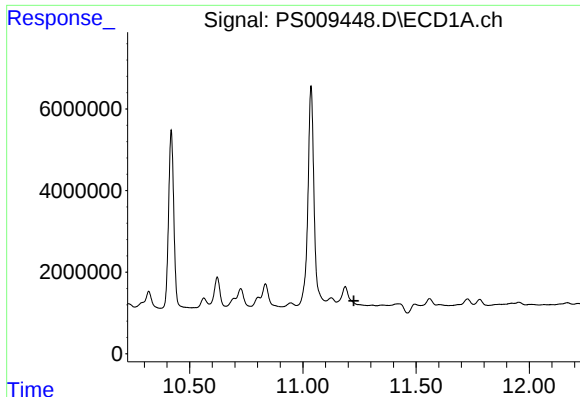

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 11.225 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127812BL

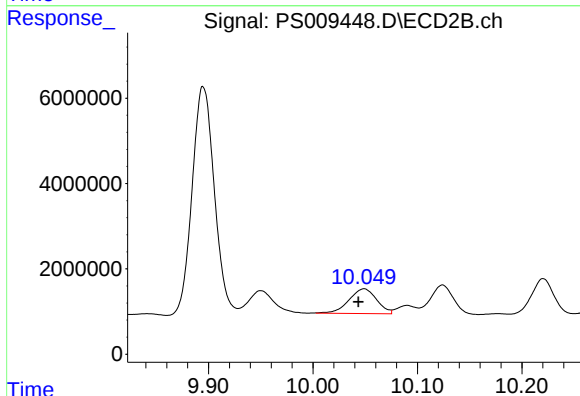


#14 DINOSEB

R.T.: 10.049 min
Delta R.T.: 0.005 min
Response: 10652843
Conc: 4.85 ng/ml

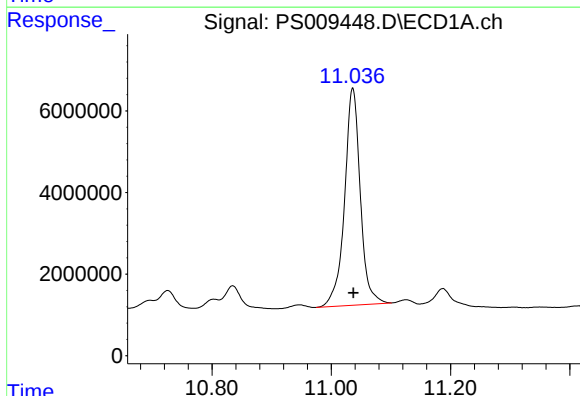


#15 Picloram

R.T.: 11.036 min
Delta R.T.: -0.001 min
Response: 97433833
Conc: 32.10 ng/ml

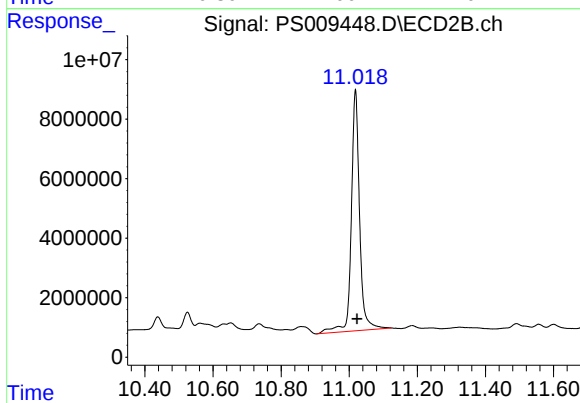

#15 Picloram


R.T.: 11.018 min
Delta R.T.: -0.005 min
Response: 136258945
Conc: 33.46 ng/ml

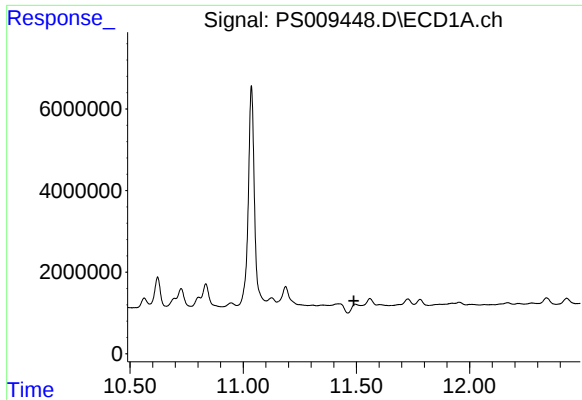

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB127812BL

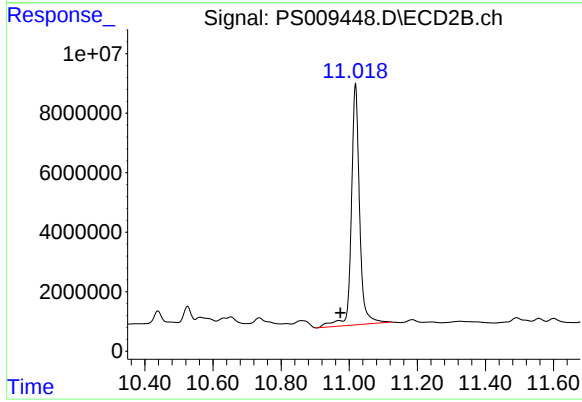

#16 DCPA

R.T.: 11.018 min
Delta R.T.: 0.044 min
Response: 136258945
Conc: 35.18 ng/ml