

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
 Data File : PS009451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 22:01
 Operator : DD\AJ
 Sample : L1754-04
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 NB-08-032420

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:29:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.242	6.932	269.9E6	252.3E6	487.910	459.365
Target Compounds							
2) T	3,5-DICHL...	0.000	6.109	0 61040239		N.D.	75.052
8) T	DICHLORPROP	0.000	7.751	0 36063112		N.D.	64.999
9) T	2,4-D	8.294	0.000	7321222	0	13.886	N.D. #
12) T	2,4,5-T	9.444	0.000	69047935	0	27.143	N.D. #
15) T	Picloram	0.000	11.020	0 6039010		N.D.	1.483
16) T	DCPA	0.000	11.020	0 6039010		N.D.	1.559



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
Data File : PS009451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 22:01
Operator : DD\AJ
Sample : L1754-04
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
NB-08-032420

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:29:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

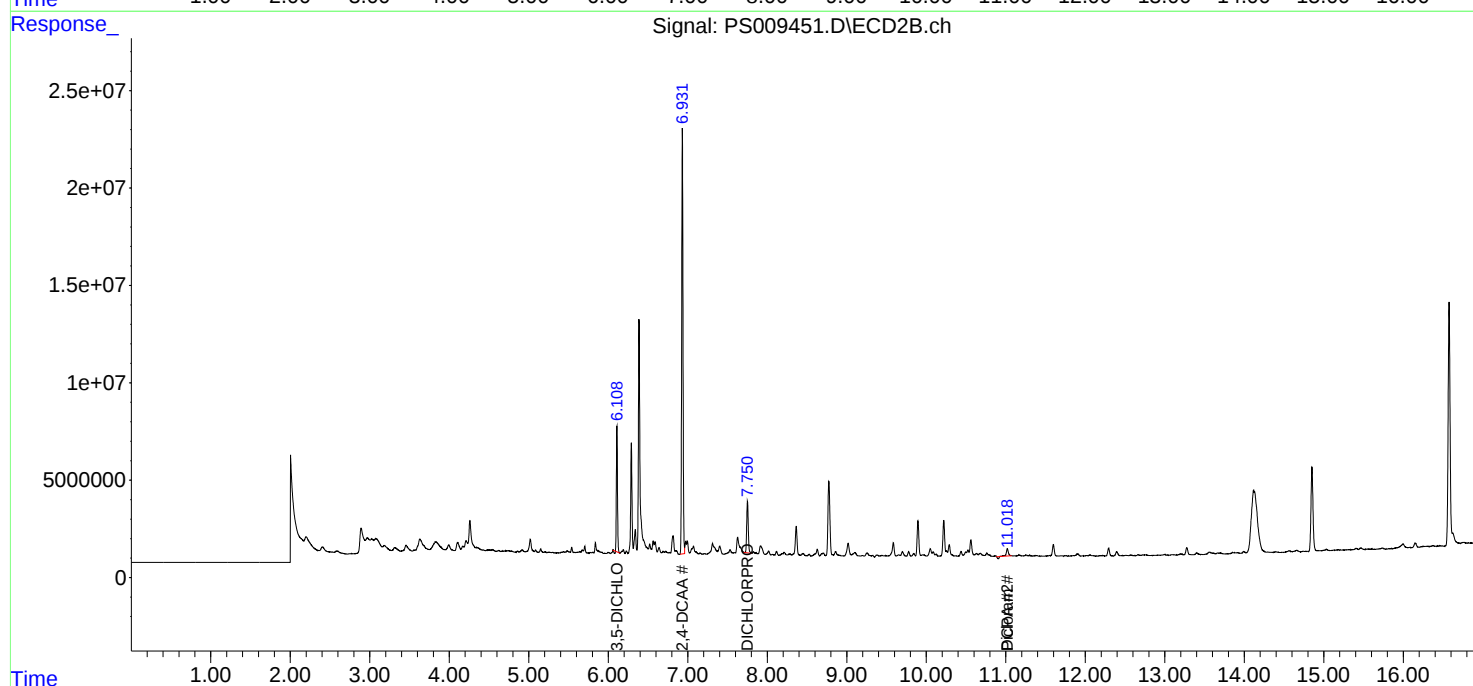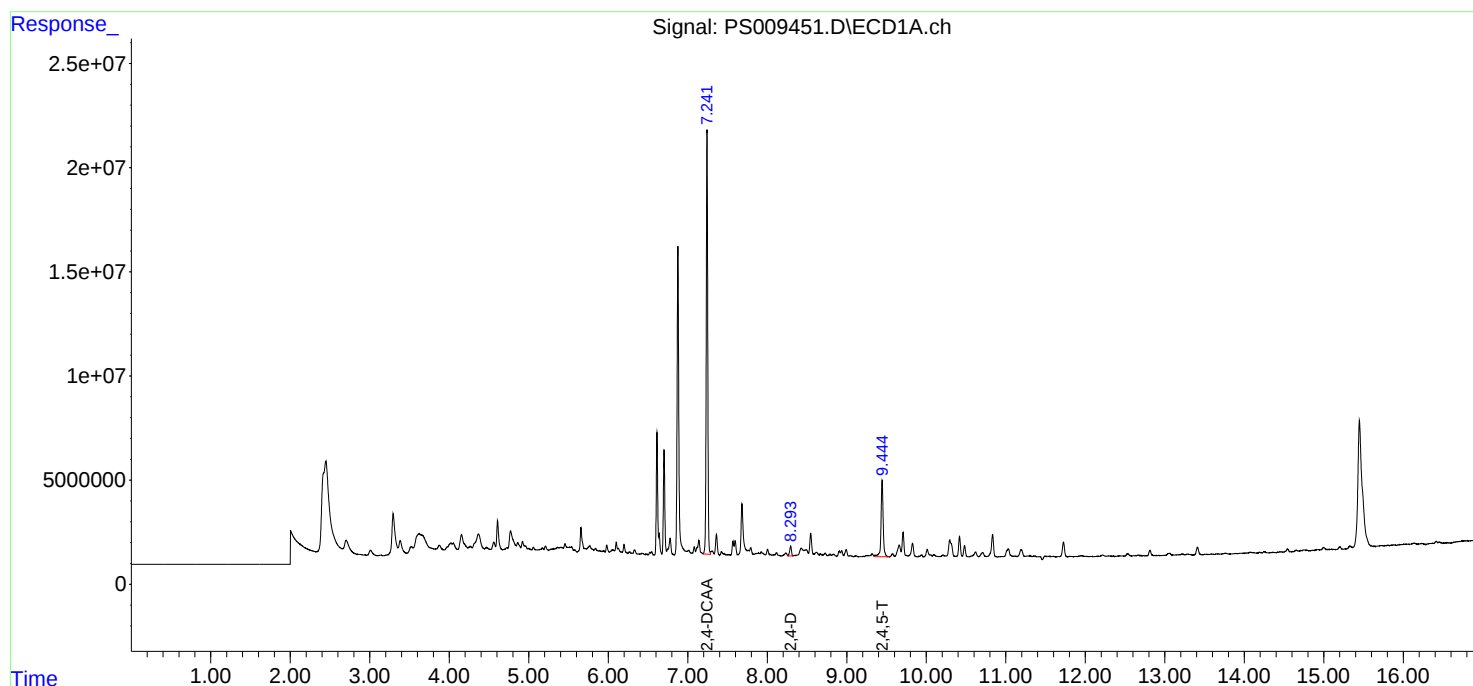


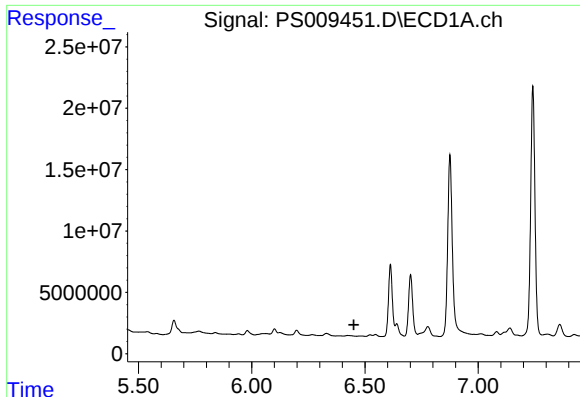

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
NB-08-032420

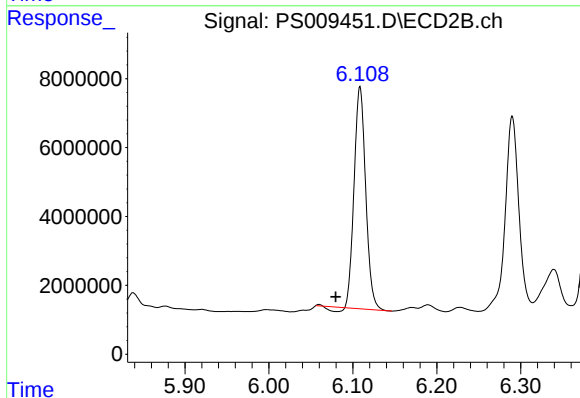


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.109 min
Delta R.T.: 0.029 min
Response: 61040239
Conc: 75.05 ng/ml

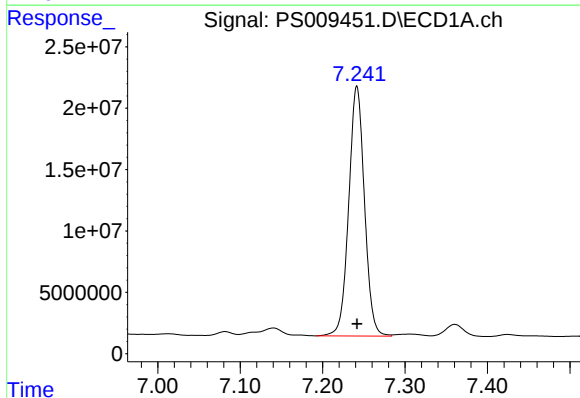


#4 2,4-DCAA

R.T.: 7.242 min
Delta R.T.: 0.000 min
Response: 269897438
Conc: 487.91 ng/ml

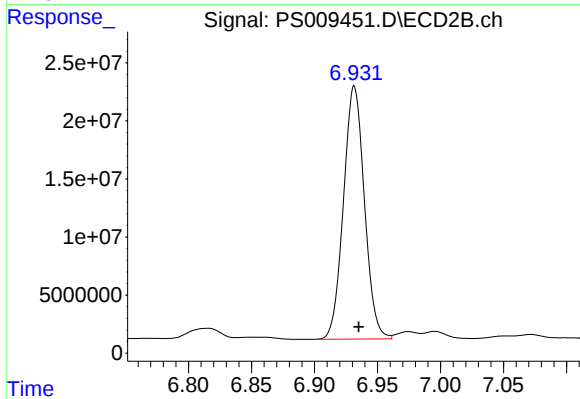

#4 2,4-DCAA


R.T.: 6.932 min
Delta R.T.: -0.003 min
Response: 252282326
Conc: 459.37 ng/ml

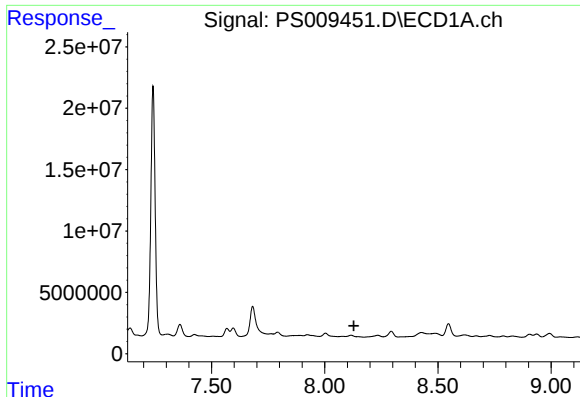

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
NB-08-032420

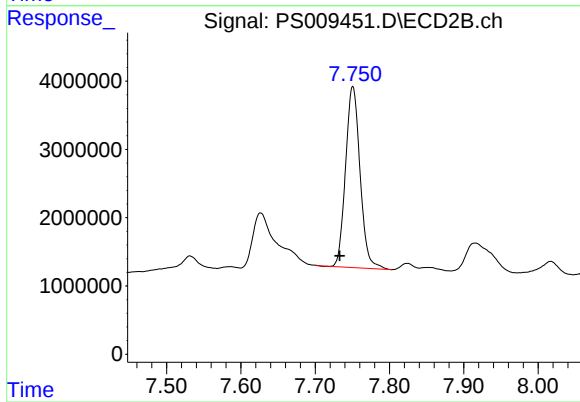


#8 DICHLORPROP

R.T.: 7.751 min
Delta R.T.: 0.018 min
Response: 36063112
Conc: 65.00 ng/ml

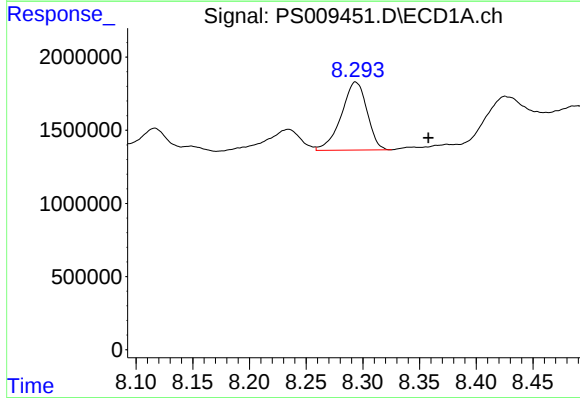


#9 2,4-D

R.T.: 8.294 min
Delta R.T.: -0.064 min
Response: 7321222
Conc: 13.89 ng/ml

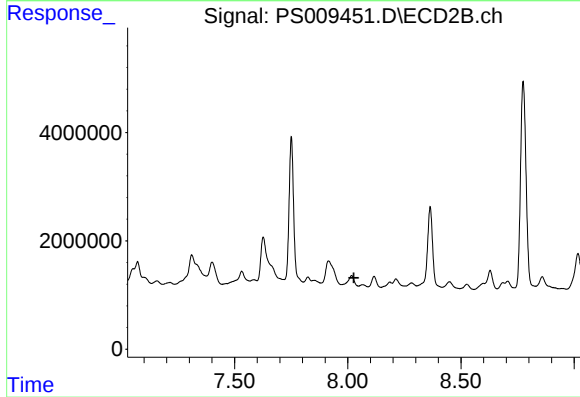

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

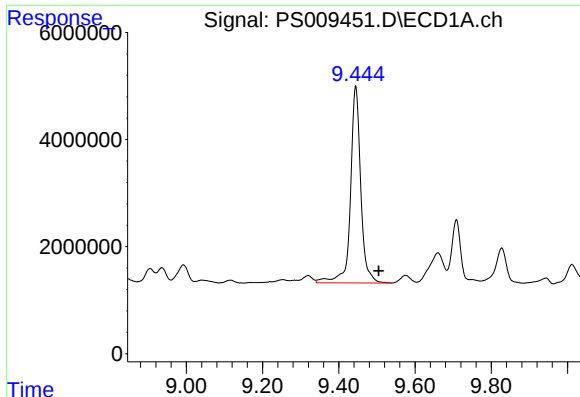

#12 2,4,5-T


R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 69047935
Conc: 27.14 ng/ml

Instrument :
ECD_S
ClientSampleId :
NB-08-032420

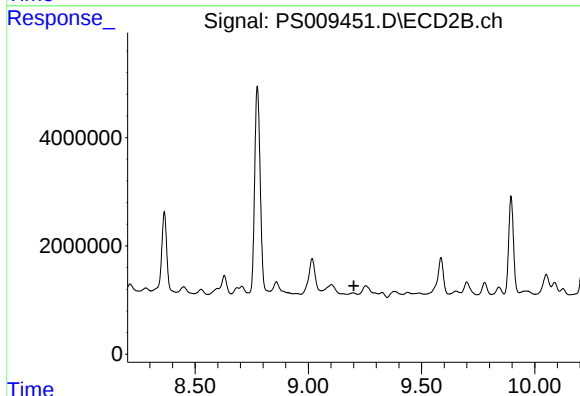


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

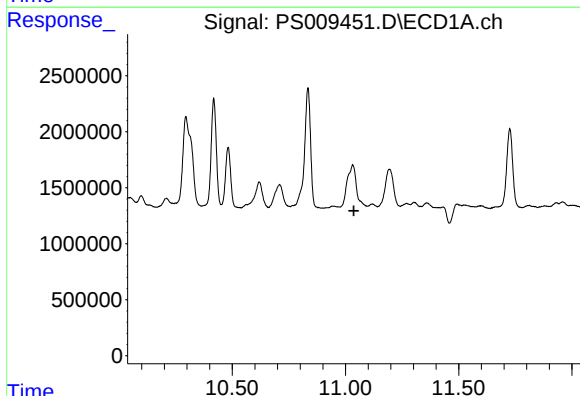


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

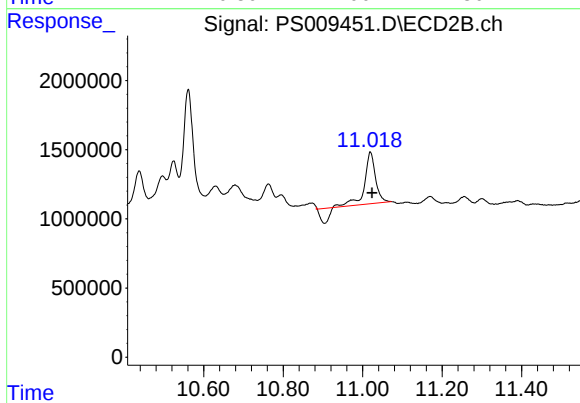

#15 Picloram


R.T.: 11.020 min
Delta R.T.: -0.004 min
Response: 6039010
Conc: 1.48 ng/ml

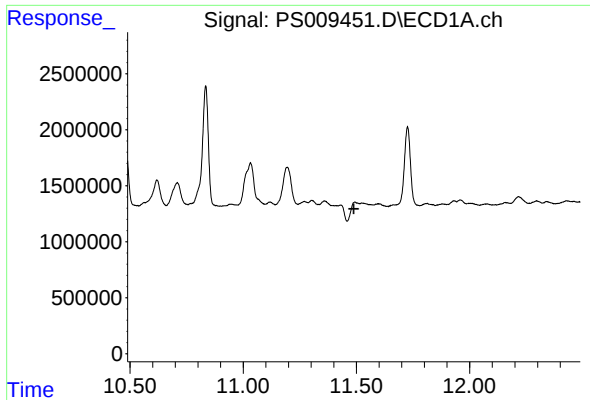

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.489 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
NB-08-032420

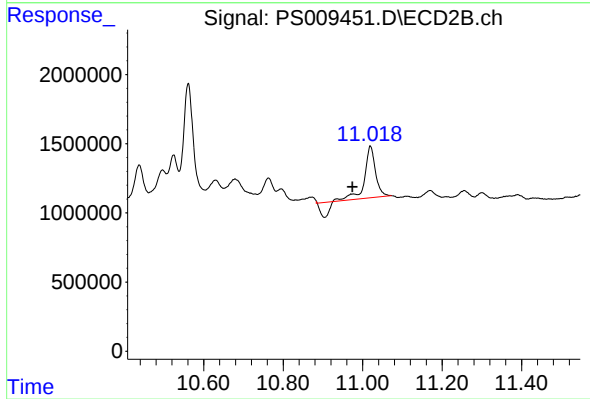

#16 DCPA

R.T.: 11.020 min
Delta R.T.: 0.045 min
Response: 6039010
Conc: 1.56 ng/ml