

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
 Data File : PS009454.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 23:10
 Operator : DD\AJ
 Sample : L1757-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 EO-01-032420

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:30:43 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.931	286.4E6	269.6E6	517.749	490.892
Target Compounds							
2) T	3,5-DICHL...	0.000	6.108	0	61319557	N.D.	75.395
8) T	DICHLORPROP	0.000	7.750	0	35315355	N.D.	63.652
9) T	2,4-D	8.427	0.000	13085493	0	24.820	N.D. #
10) T	Pentachlo...	8.668	8.455	26099809	26107297	3.712	3.440
12) T	2,4,5-T	9.444	0.000	51747303	0	20.342	N.D. #
15) T	Picloram	0.000	11.018	0	7049044	N.D.	1.731
16) T	DCPA	0.000	11.018	0	7049044	N.D.	1.820



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
Data File : PS009454.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 23:10
Operator : DD\AJ
Sample : L1757-11
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
EO-01-032420

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:30:43 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

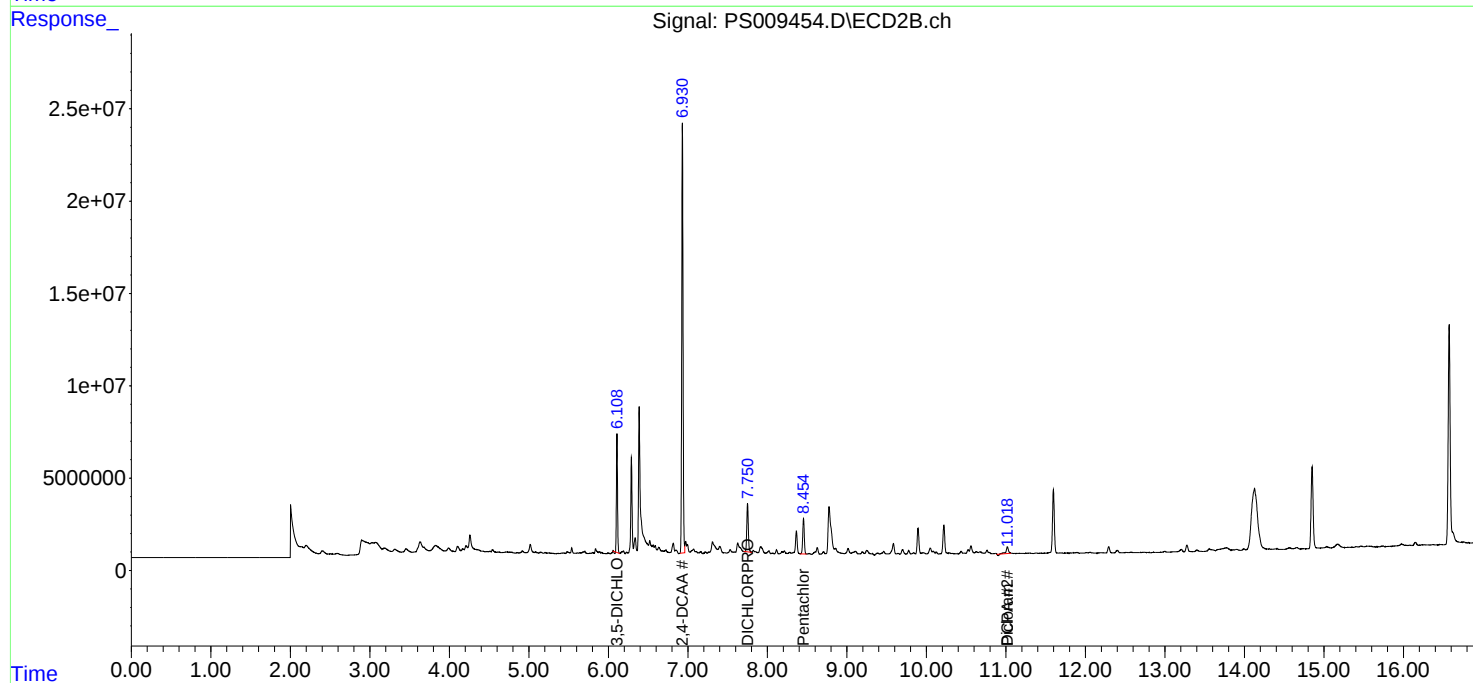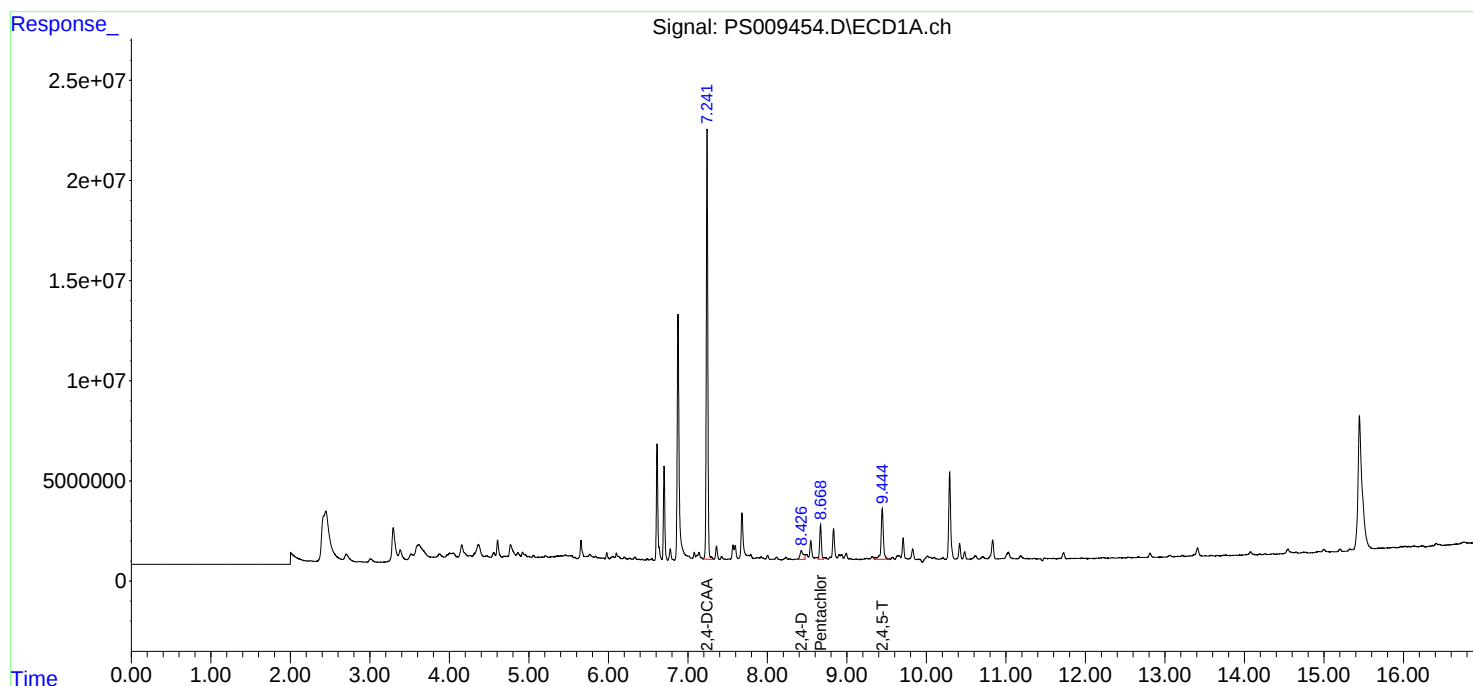


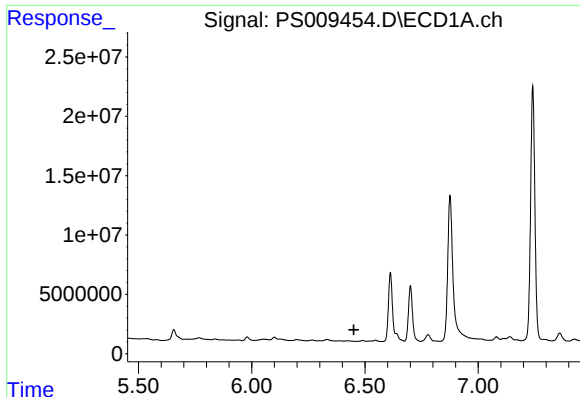

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-01-032420

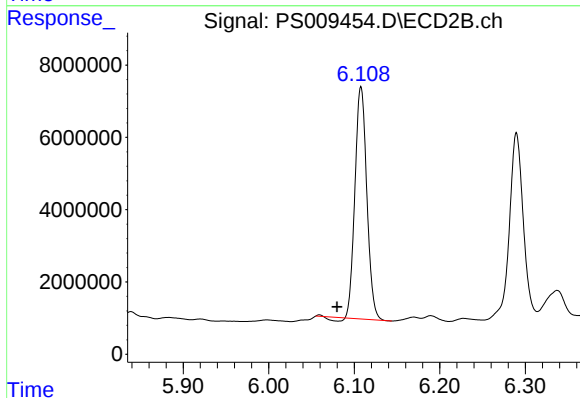


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.108 min
Delta R.T.: 0.028 min
Response: 61319557
Conc: 75.40 ng/ml

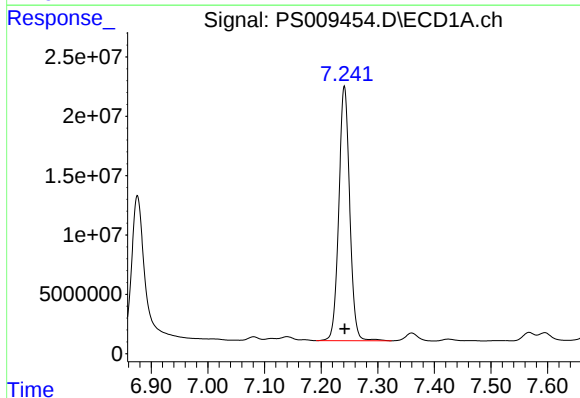


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 286403201
Conc: 517.75 ng/ml

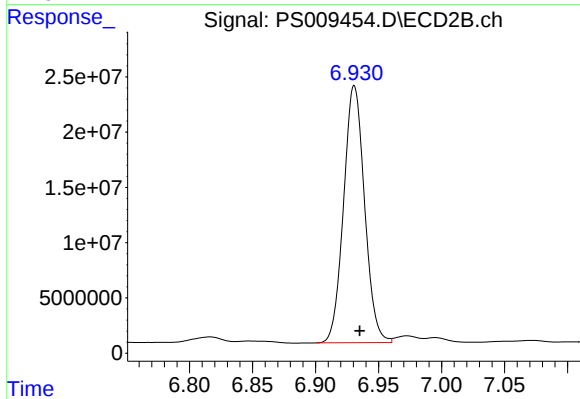

#4 2,4-DCAA


R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 269596580
Conc: 490.89 ng/ml

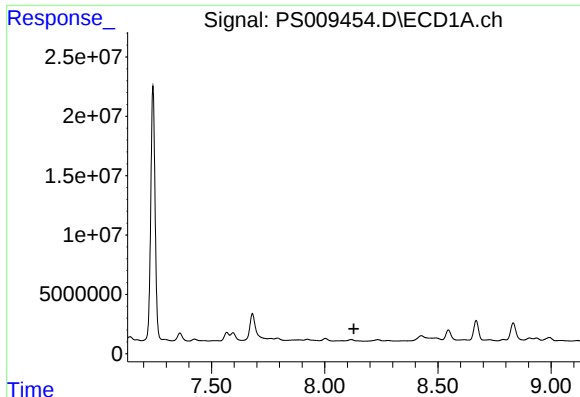

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-01-032420

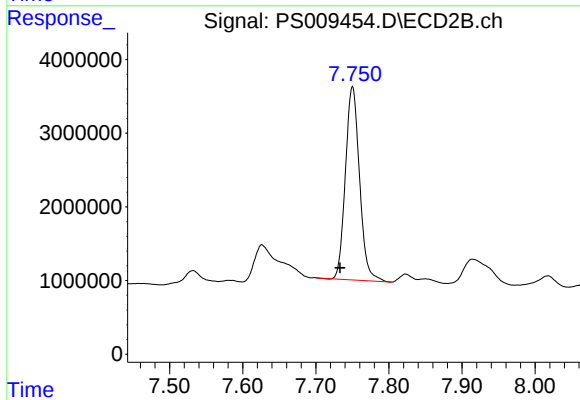


#8 DICHLORPROP

R.T.: 7.750 min
Delta R.T.: 0.017 min
Response: 35315355
Conc: 63.65 ng/ml

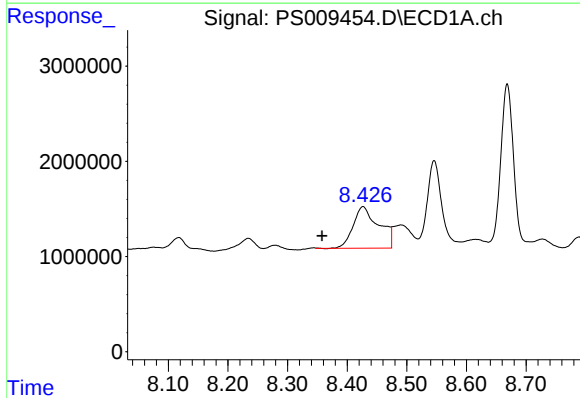


#9 2,4-D

R.T.: 8.427 min
Delta R.T.: 0.069 min
Response: 13085493
Conc: 24.82 ng/ml

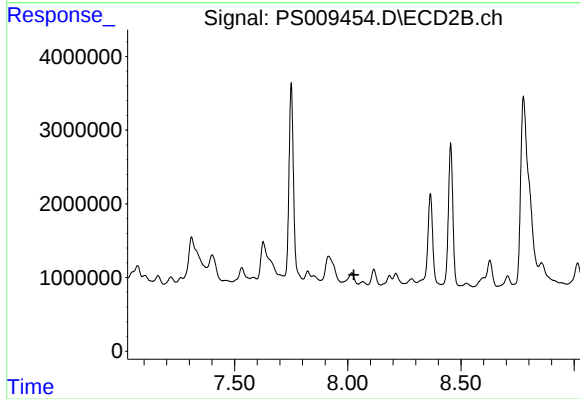

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

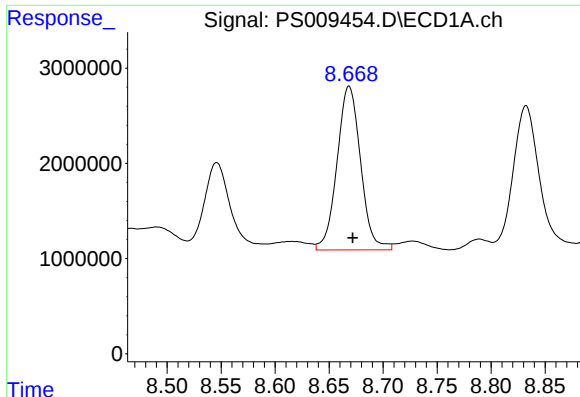

#10 Pentachlorophenol


R.T.: 8.668 min
Delta R.T.: -0.003 min
Response: 26099809
Conc: 3.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
EO-01-032420

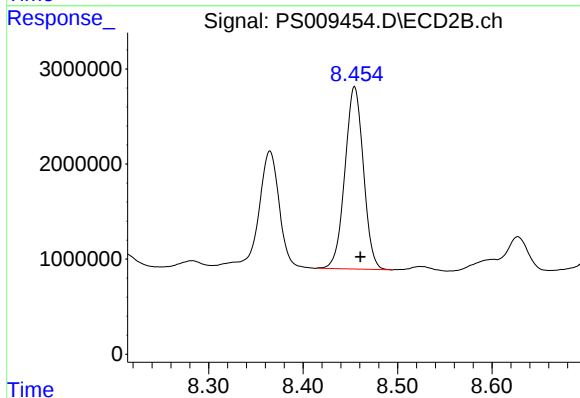


#10 Pentachlorophenol

R.T.: 8.455 min
Delta R.T.: -0.006 min
Response: 26107297
Conc: 3.44 ng/ml

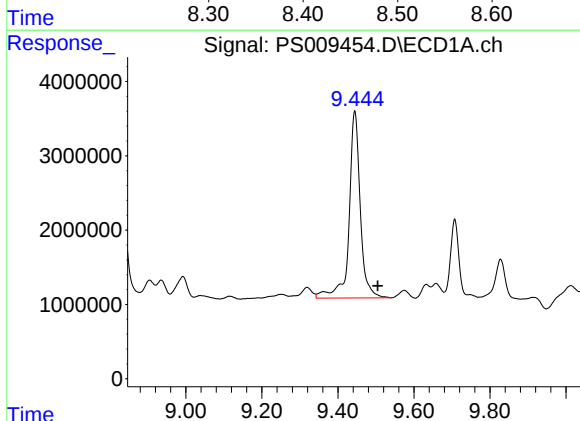


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 51747303
Conc: 20.34 ng/ml

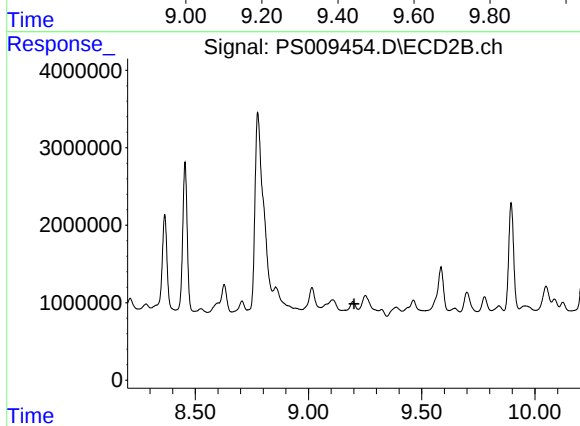

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.201 min
Response: 0
Conc: N.D.

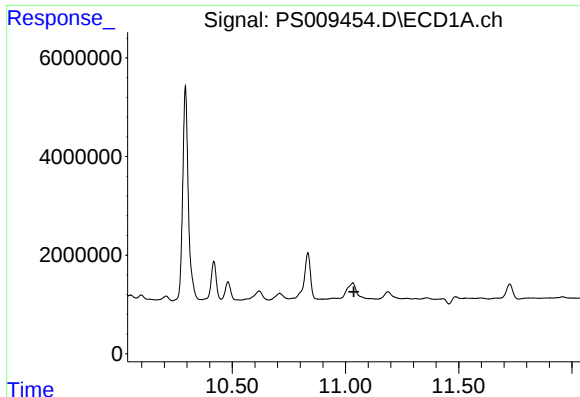

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
EO-01-032420

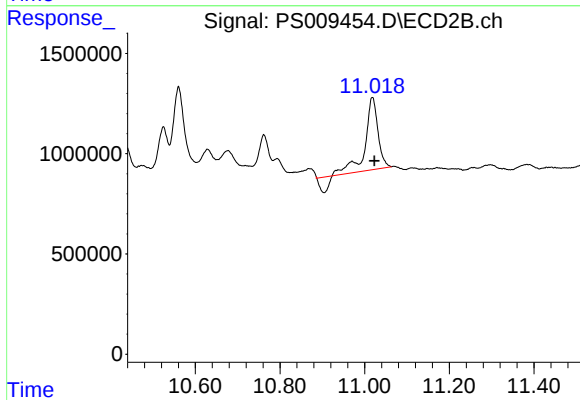


#15 Picloram

R.T.: 11.018 min
Delta R.T.: -0.005 min
Response: 7049044
Conc: 1.73 ng/ml

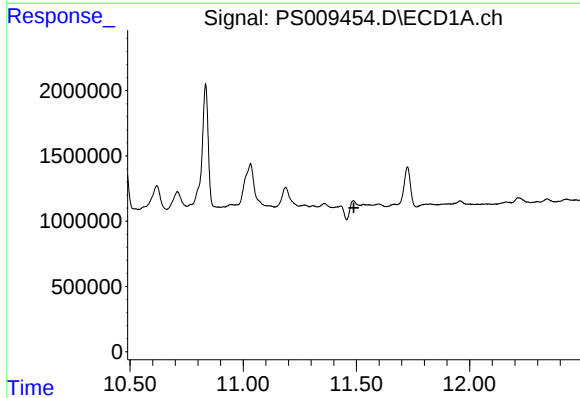

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

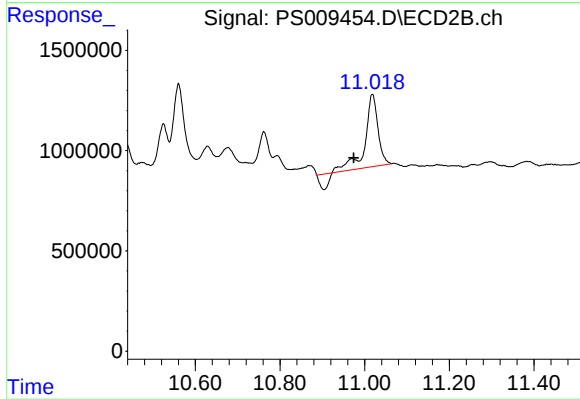

#16 DCPA

R.T.: 11.018 min
Delta R.T.: 0.044 min
Response: 7049044
Conc: 1.82 ng/ml