

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
 Data File : PS009455.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 23:33
 Operator : DD\AJ
 Sample : L2026-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:31:02 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.931	284.1E6	275.9E6	513.590	502.380
Target Compounds							
2) T	3,5-DICHL...	0.000	6.108	0	65073250	N.D.	80.011
5) T	DICAMBA	7.455	0.000	9858721	0	4.632	N.D. #
7) T	MCPA	0.000	7.473	0	19704317	N.D.	7.302
8) T	DICHLORPROP	0.000	7.750	0	45660271	N.D.	82.297
9) T	2,4-D	8.425	0.000	10145133	0	19.243	N.D. #
12) T	2,4,5-T	9.445	0.000	55292186	0	21.736	N.D. #
15) T	Picloram	0.000	11.048	0	18450444	N.D.	4.531



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
Data File : PS009455.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 23:33
Operator : DD\AJ
Sample : L2026-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:31:02 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

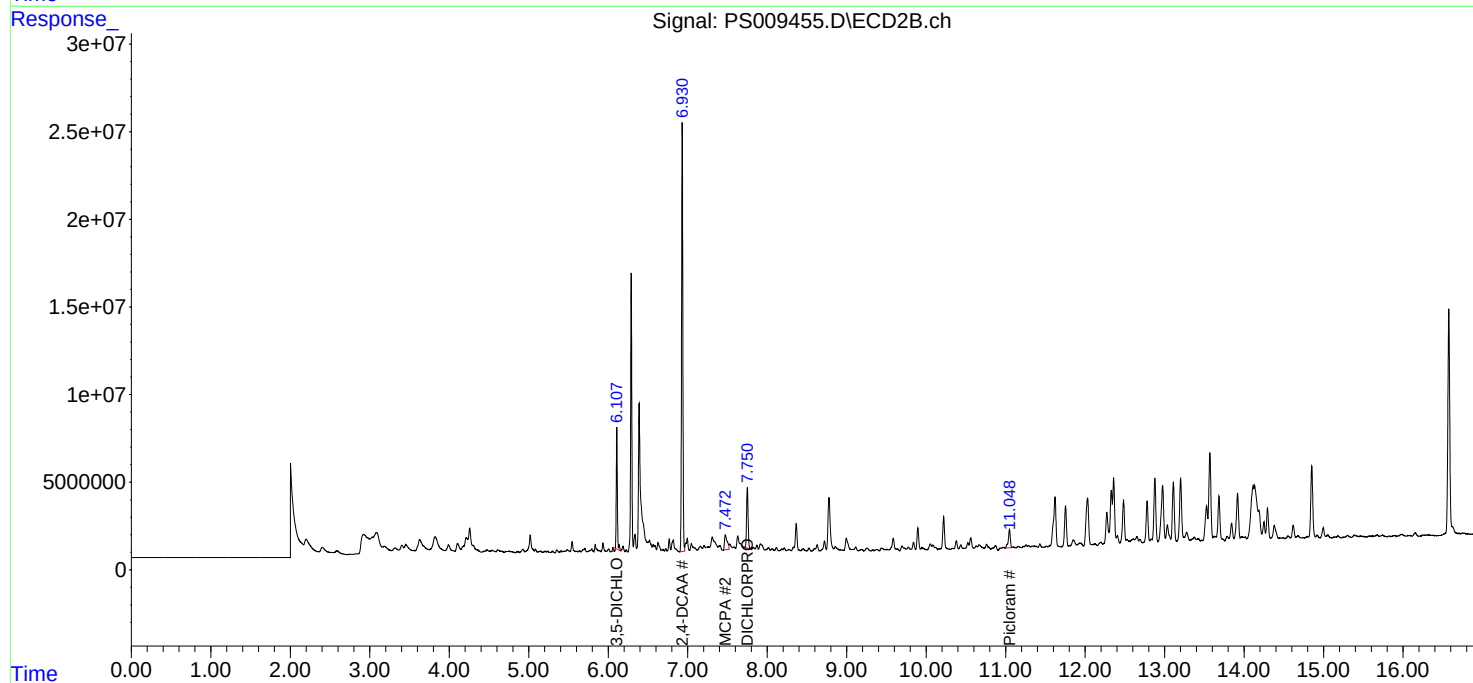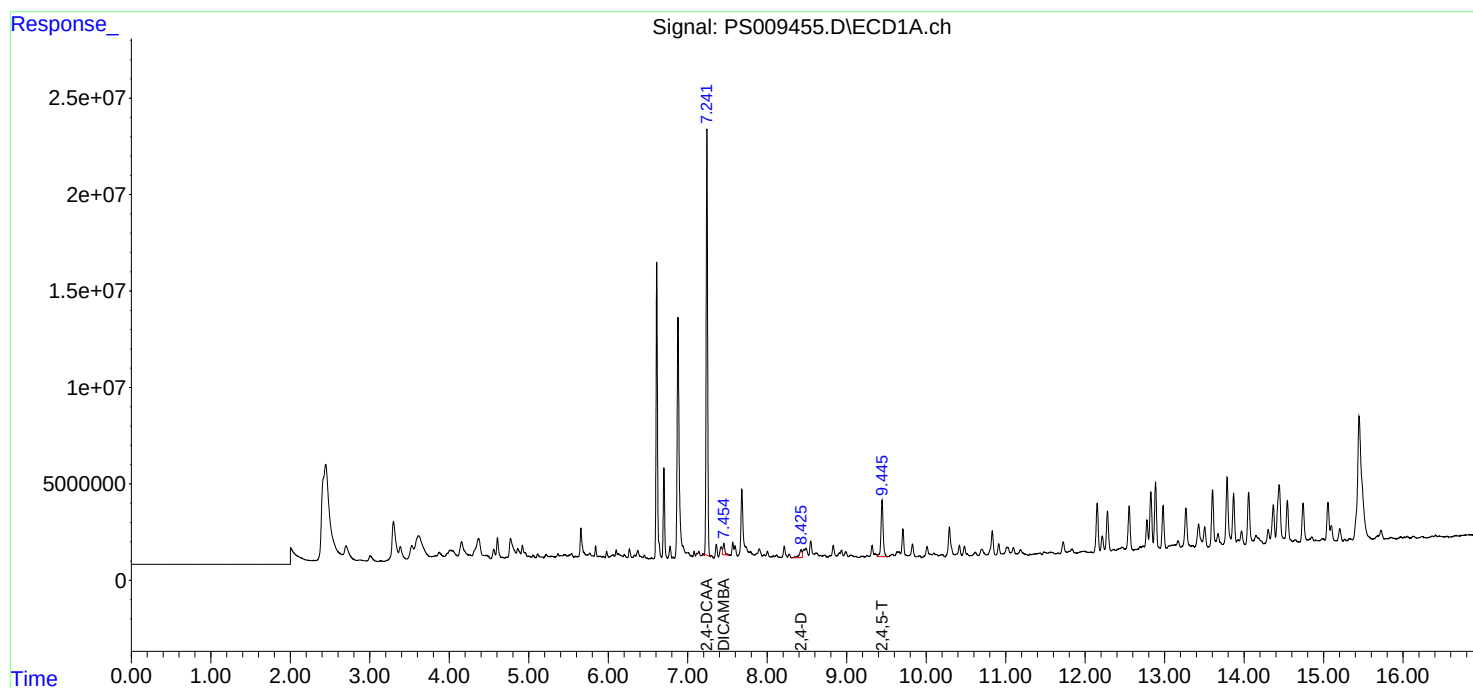


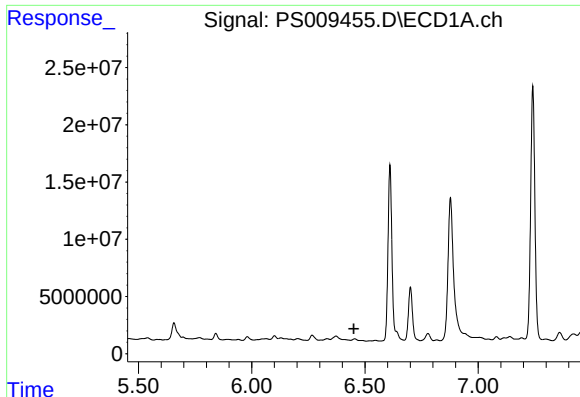

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

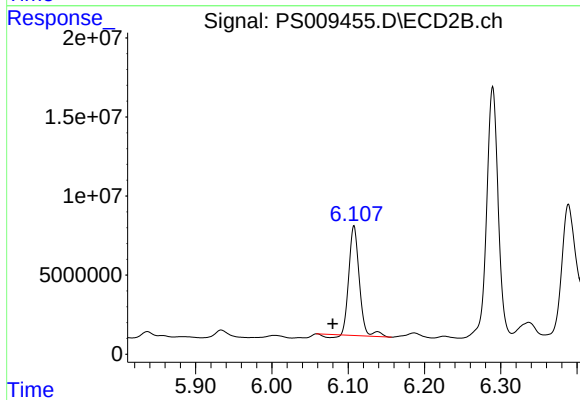


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.108 min
Delta R.T.: 0.028 min
Response: 65073250
Conc: 80.01 ng/ml

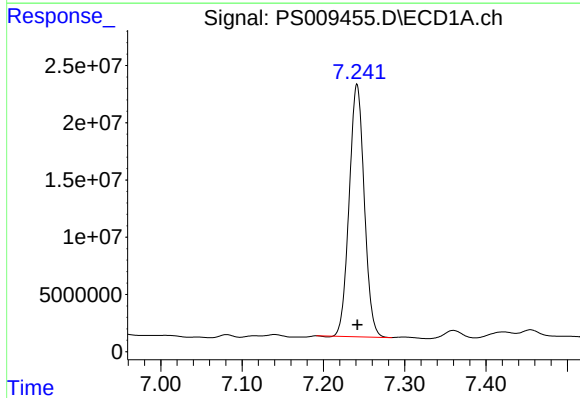


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 284102865
Conc: 513.59 ng/ml

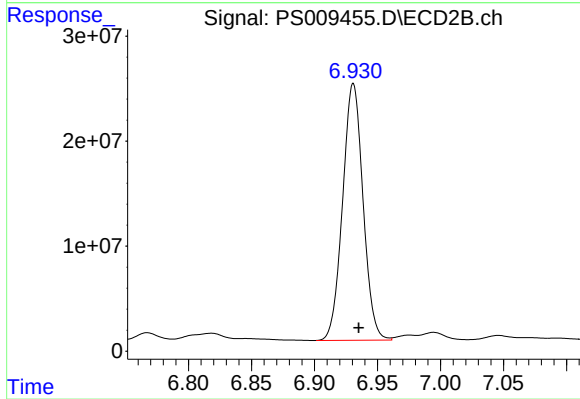

#4 2,4-DCAA


R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 275905713
Conc: 502.38 ng/ml

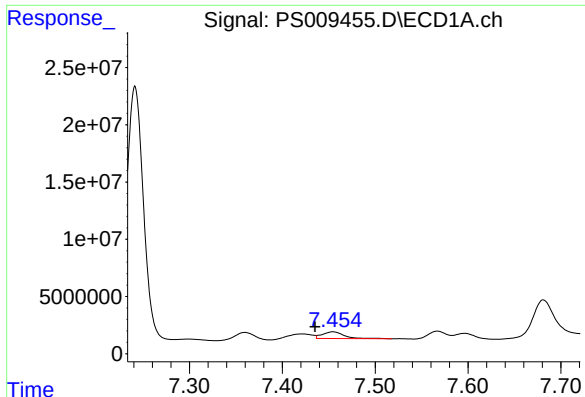

#5 DICAMBA


R.T.: 7.455 min
Delta R.T.: 0.019 min
Response: 9858721
Conc: 4.63 ng/ml

Instrument :
ECD_S
ClientSampleId :

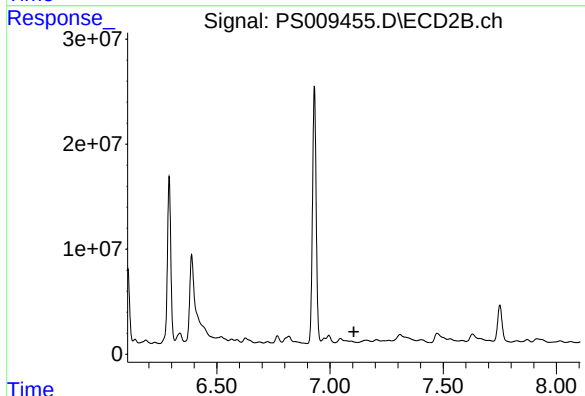


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.106 min
Response: 0
Conc: N.D.

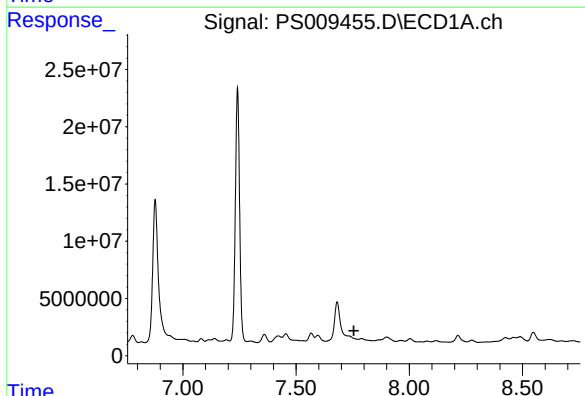


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.756 min
Response: 0
Conc: N.D.

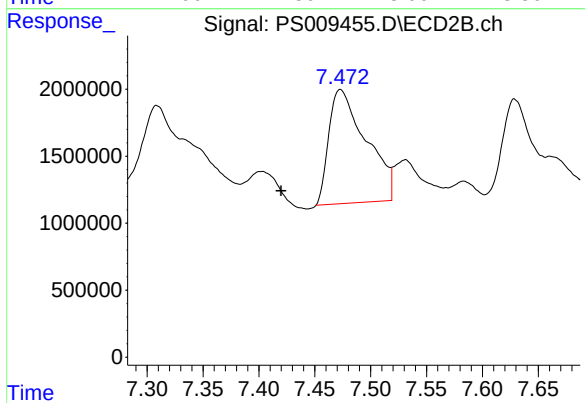

#7 MCPA


R.T.: 7.473 min
Delta R.T.: 0.053 min
Response: 19704317
Conc: 7.30 ug/ml

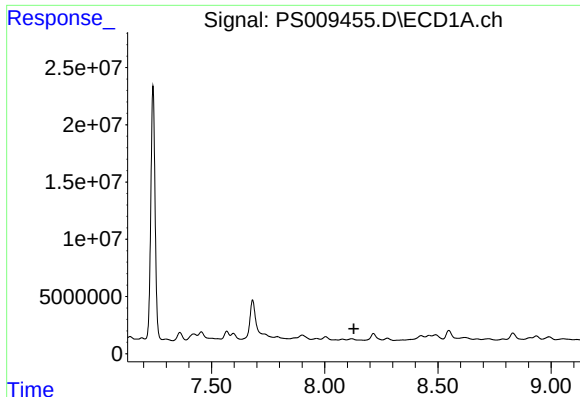

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

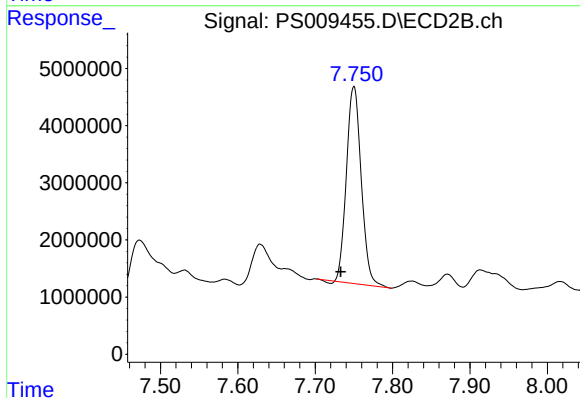


#8 DICHLORPROP

R.T.: 7.750 min
Delta R.T.: 0.017 min
Response: 45660271
Conc: 82.30 ng/ml

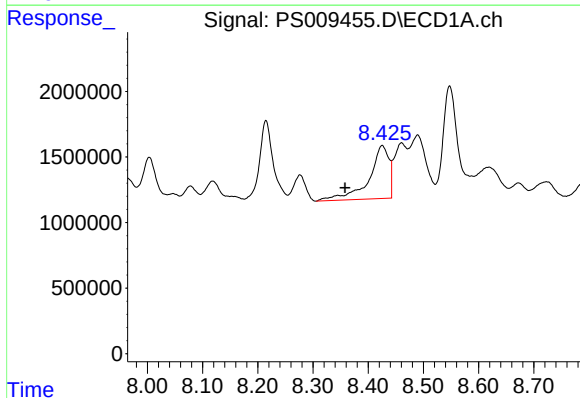


#9 2,4-D

R.T.: 8.425 min
Delta R.T.: 0.068 min
Response: 10145133
Conc: 19.24 ng/ml

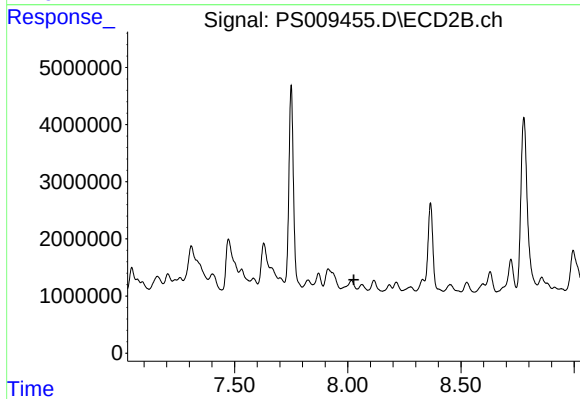

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 8.027 min
Response: 0
Conc: N.D.

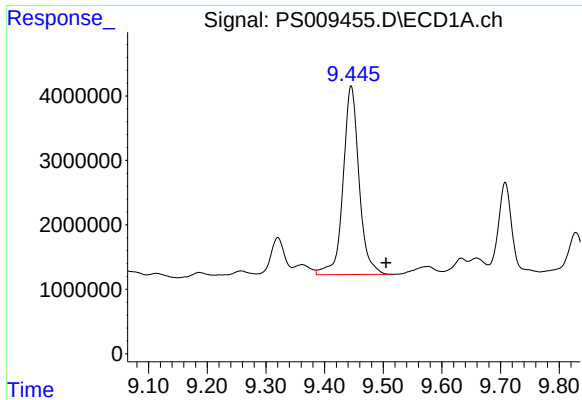

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 55292186
Conc: 21.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

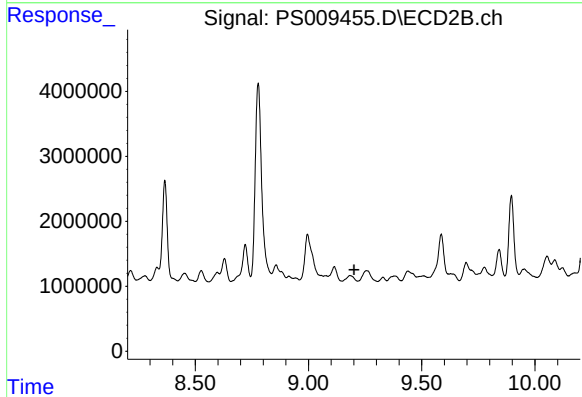


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

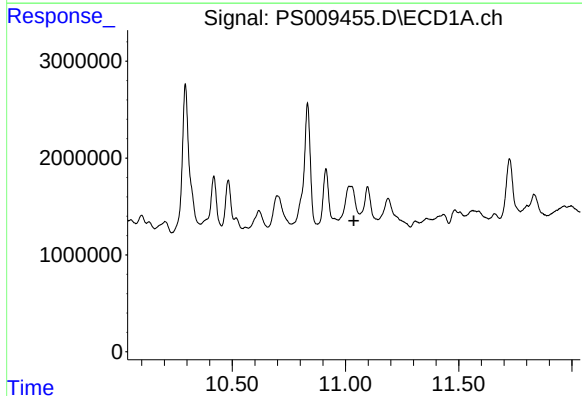

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

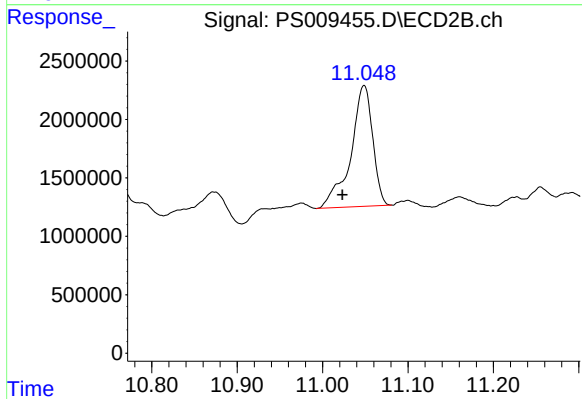

#15 Picloram

R.T.: 11.048 min
Delta R.T.: 0.025 min
Response: 18450444
Conc: 4.53 ng/ml