

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
 Data File : PS009456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2020 23:56
 Operator : DD\AJ
 Sample : L2026-02
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BUS-WASH

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:31:21 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.931	252.5E6	219.7E6	456.452	400.007
Target Compounds							
2) T	3,5-DICHL...	0.000	6.108	0 70302300		N.D.	86.440
7) T	MCPA	0.000	7.478	0 8403382		N.D.	3.114
8) T	DICHLORPROP	0.000	7.749	0 43207706		N.D.	77.877
9) T	2,4-D	8.426	0.000	14751202	0	27.979	N.D. #
11) T	2,4,5-TP ...	9.189	0.000	9368095	0	3.418	N.D. #
12) T	2,4,5-T	9.445	0.000	64921132	0	25.521	N.D. #
14) T	DINOSEB	11.186	10.046	10024041	11115830	4.904	5.061
15) T	Picloram	11.012	0.000	16961309	0	5.589	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
Data File : PS009456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2020 23:56
Operator : DD\AJ
Sample : L2026-02
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:31:21 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

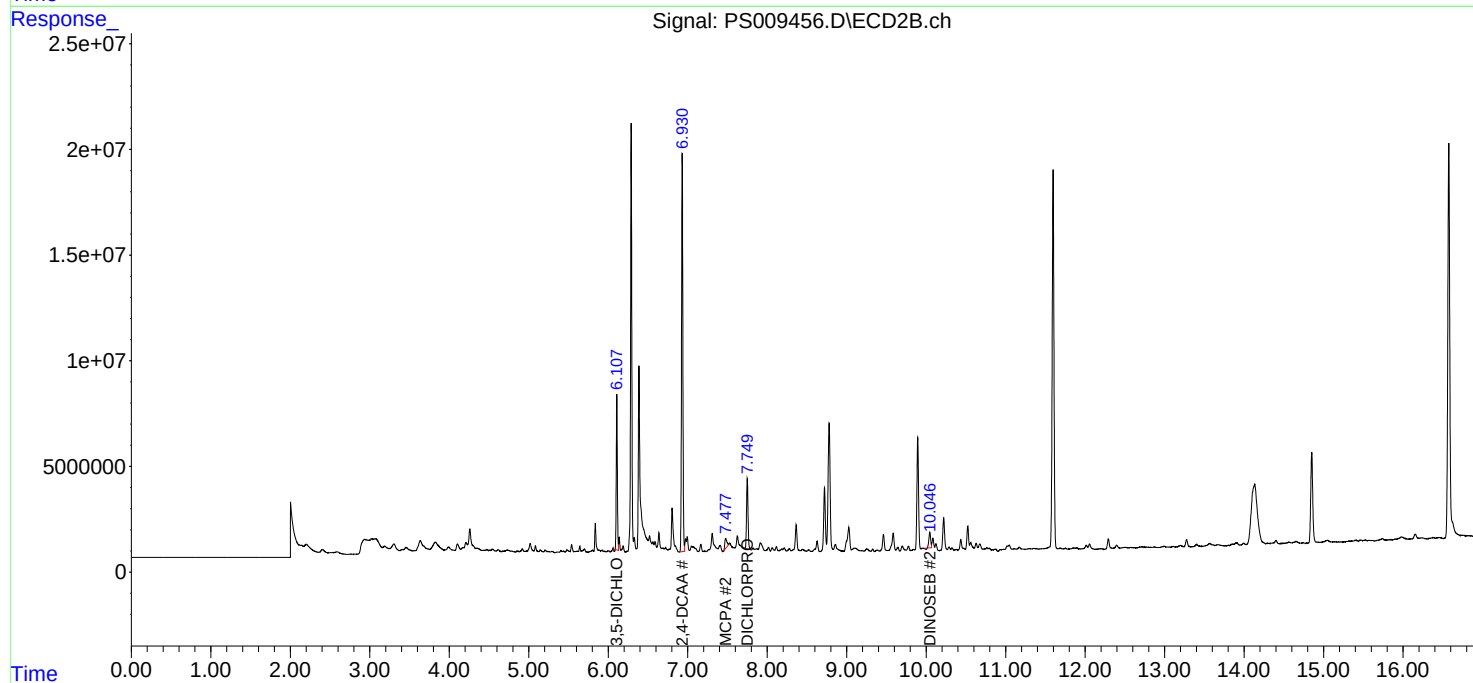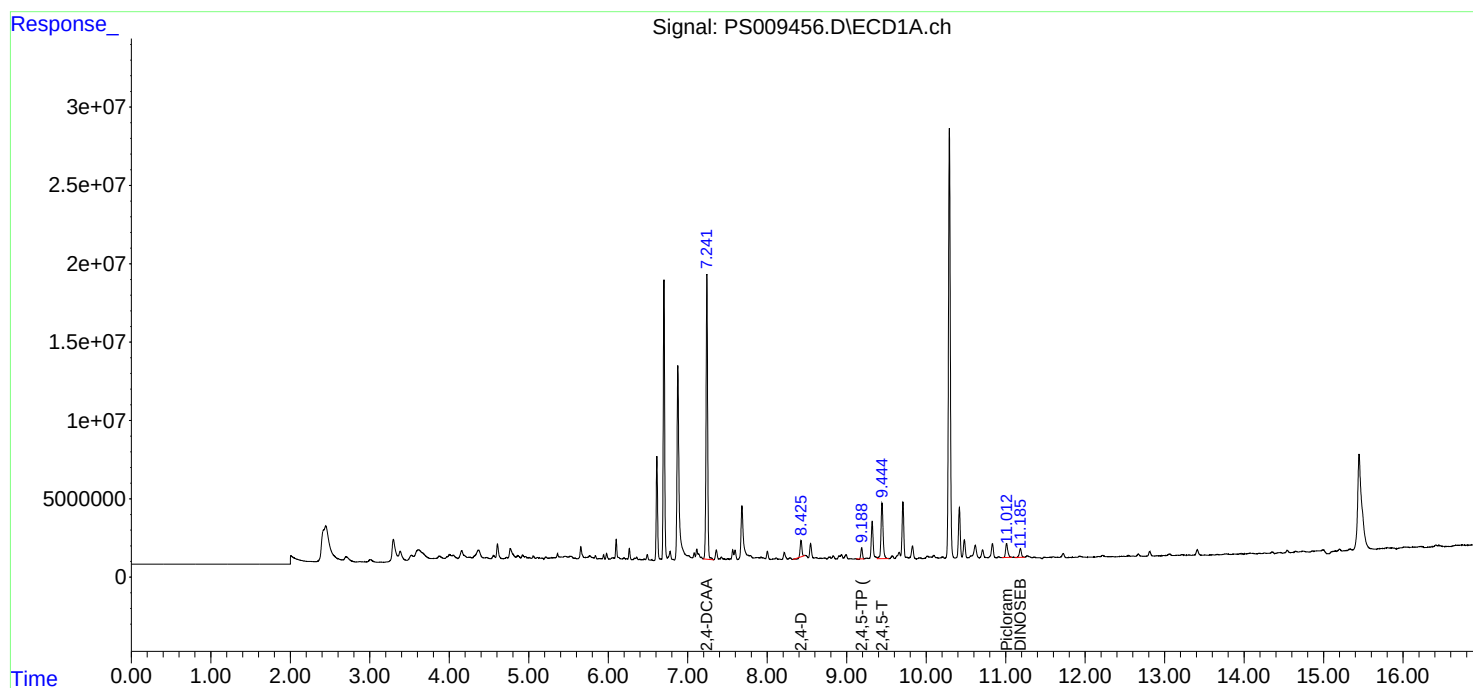


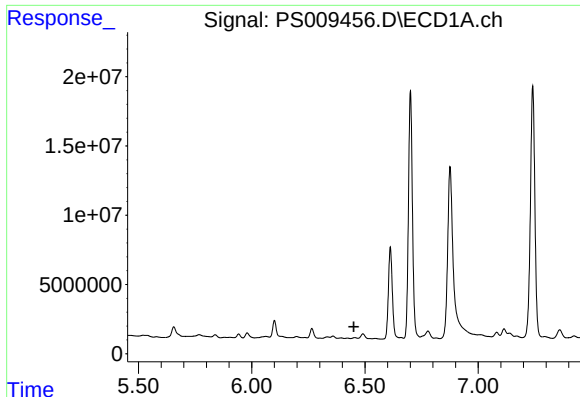

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

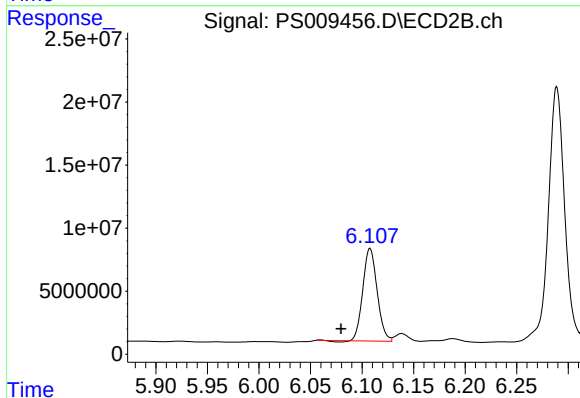


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.108 min
Delta R.T.: 0.028 min
Response: 70302300
Conc: 86.44 ng/ml

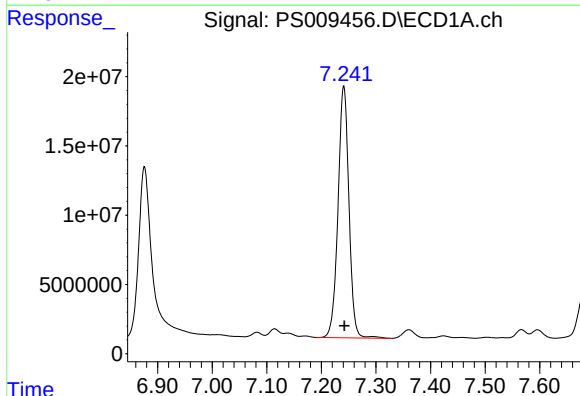


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 252495581
Conc: 456.45 ng/ml

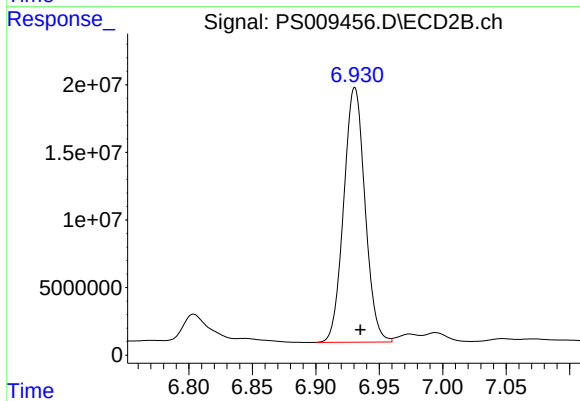

#4 2,4-DCAA


R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 219683037
Conc: 400.01 ng/ml

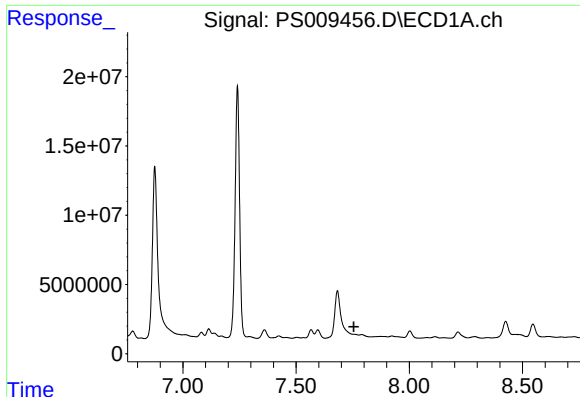

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

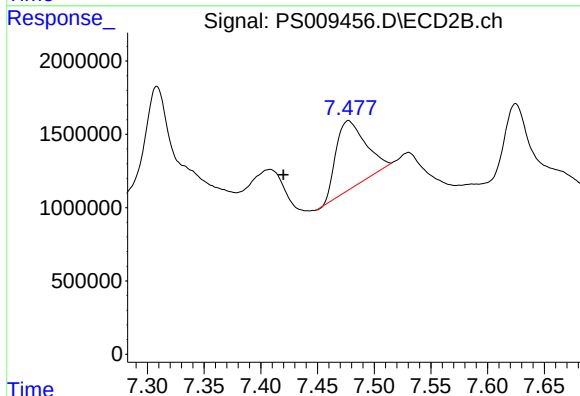


#7 MCPA

R.T.: 7.478 min
Delta R.T.: 0.058 min
Response: 8403382
Conc: 3.11 ug/ml

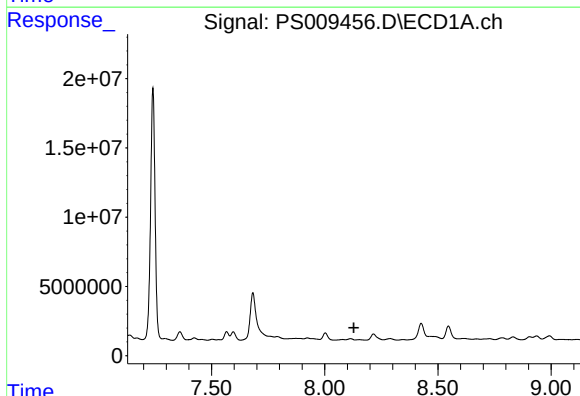


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

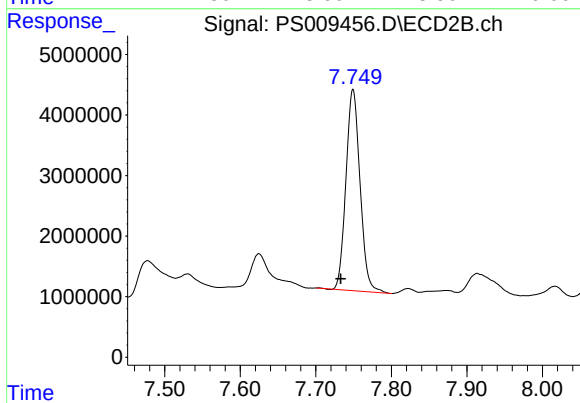

#8 DICHLORPROP


R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 43207706
Conc: 77.88 ng/ml

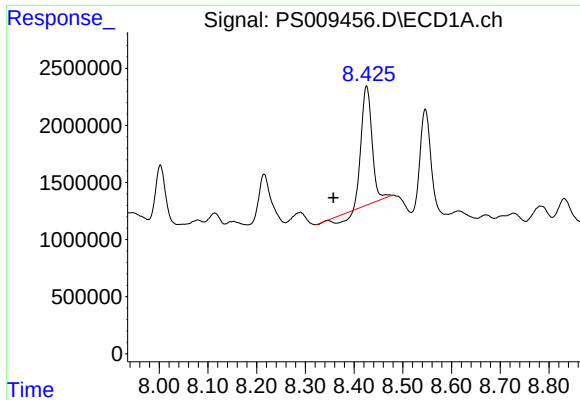

#9 2,4-D


R.T.: 8.426 min
Delta R.T.: 0.068 min
Response: 14751202
Conc: 27.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

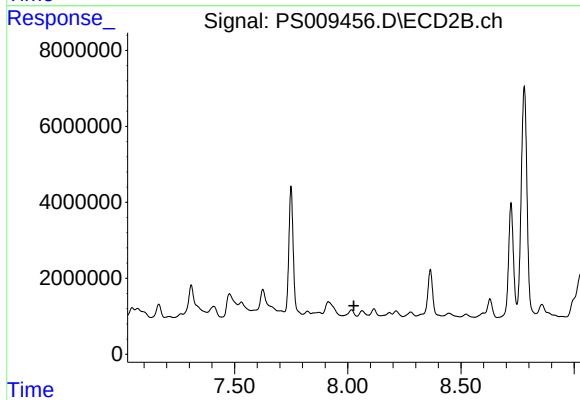


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.027 min
Response: 0
Conc: N.D.

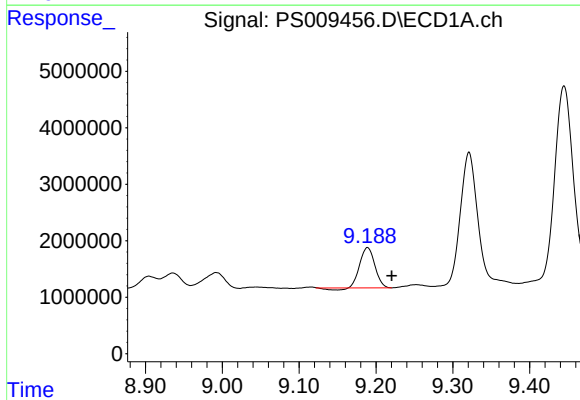


#11 2,4,5-TP (SILVEX)

R.T.: 9.189 min
Delta R.T.: -0.032 min
Response: 9368095
Conc: 3.42 ng/ml

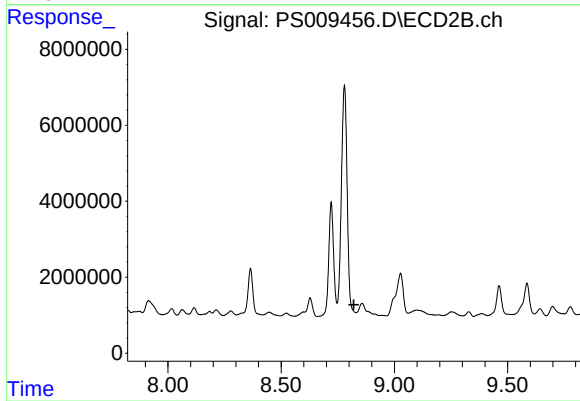

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T. : 8.822 min
Response: 0
Conc: N.D.

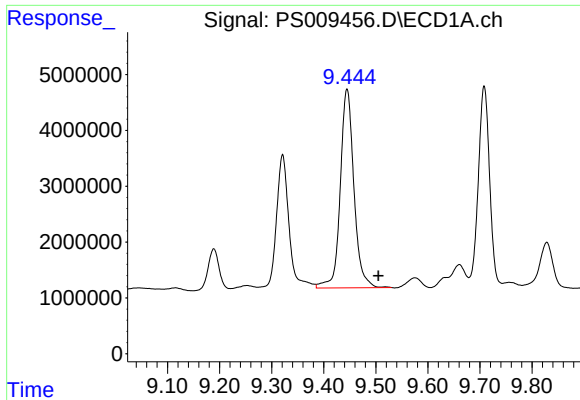

#12 2,4,5-T


R.T.: 9.445 min
Delta R.T.: -0.060 min
Response: 64921132
Conc: 25.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

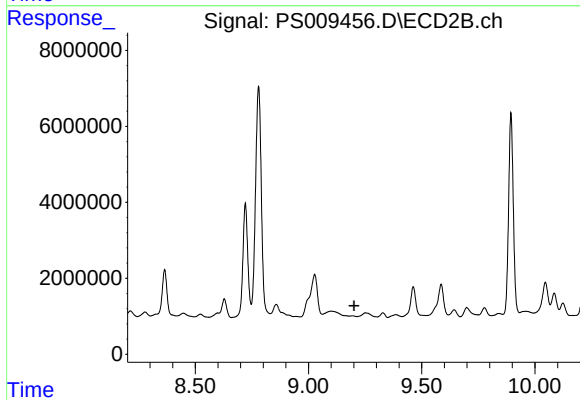


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

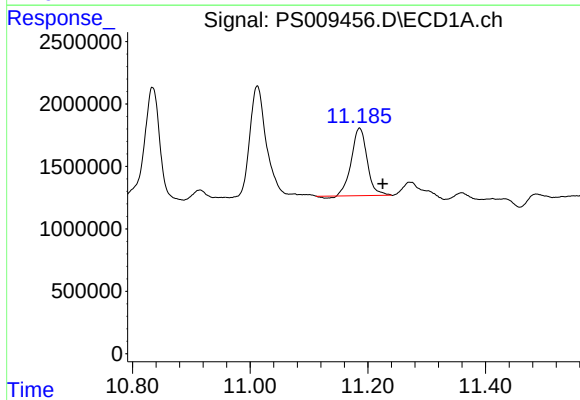


#14 DINOSEB

R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 10024041
Conc: 4.90 ng/ml

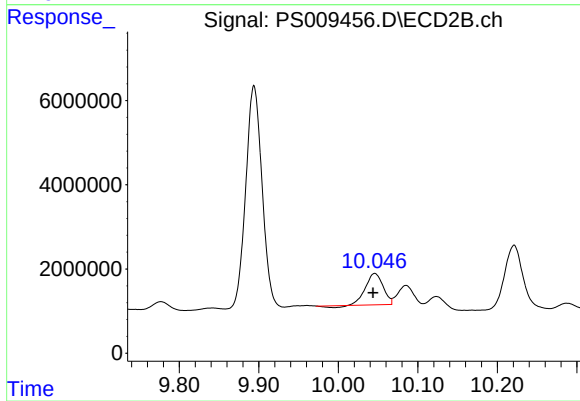

#14 DINOSEB


R.T.: 10.046 min
Delta R.T.: 0.002 min
Response: 11115830
Conc: 5.06 ng/ml

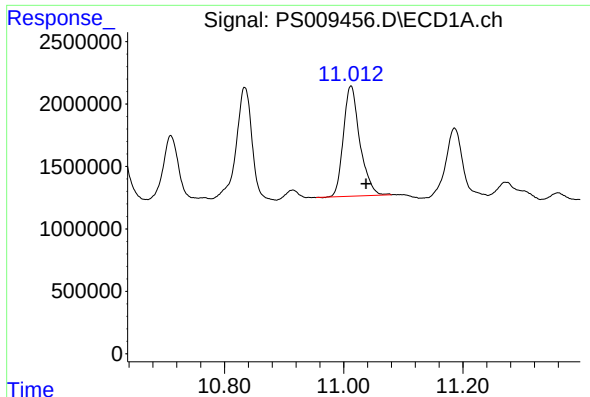

#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.025 min
Response: 16961309
Conc: 5.59 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

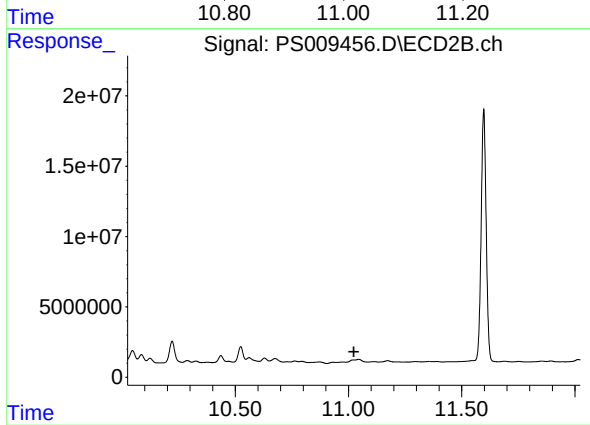

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.023 min
Response: 0
Conc: N.D.