

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
 Data File : PS009457.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 00:18
 Operator : DD\AJ
 Sample : L2026-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SLUDGE-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 01:31:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.931	276.2E6	269.4E6	499.296	490.501
Target Compounds							
2) T	3,5-DICHL...	0.000	6.108	0 83579907		N.D.	102.766
5) T	DICAMBA	7.424	7.065	6411557	29468511	3.013	12.837 #
6) T	MCP	7.598	0.000	9068688	0	3.685	N.D. #
7) T	MCPA	0.000	7.472	0 32447381		N.D.	12.024
8) T	DICHLORPROP	0.000	7.750	0 45792662		N.D.	82.536
9) T	2,4-D	8.424	0.000	9625463	0	18.257	N.D. #
11) T	2,4,5-TP ...	9.188	8.784	6476428	36349918	2.363	12.193 #
12) T	2,4,5-T	9.448	0.000	39696769	0	15.605	N.D. #
14) T	DINOSEB	11.186	10.048	12764291	13304571	6.244	6.057
15) T	Picloram	11.012	11.048	21113458	18380801	6.957	4.514 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032620\
Data File : PS009457.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 00:18
Operator : DD\AJ
Sample : L2026-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 01:31:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

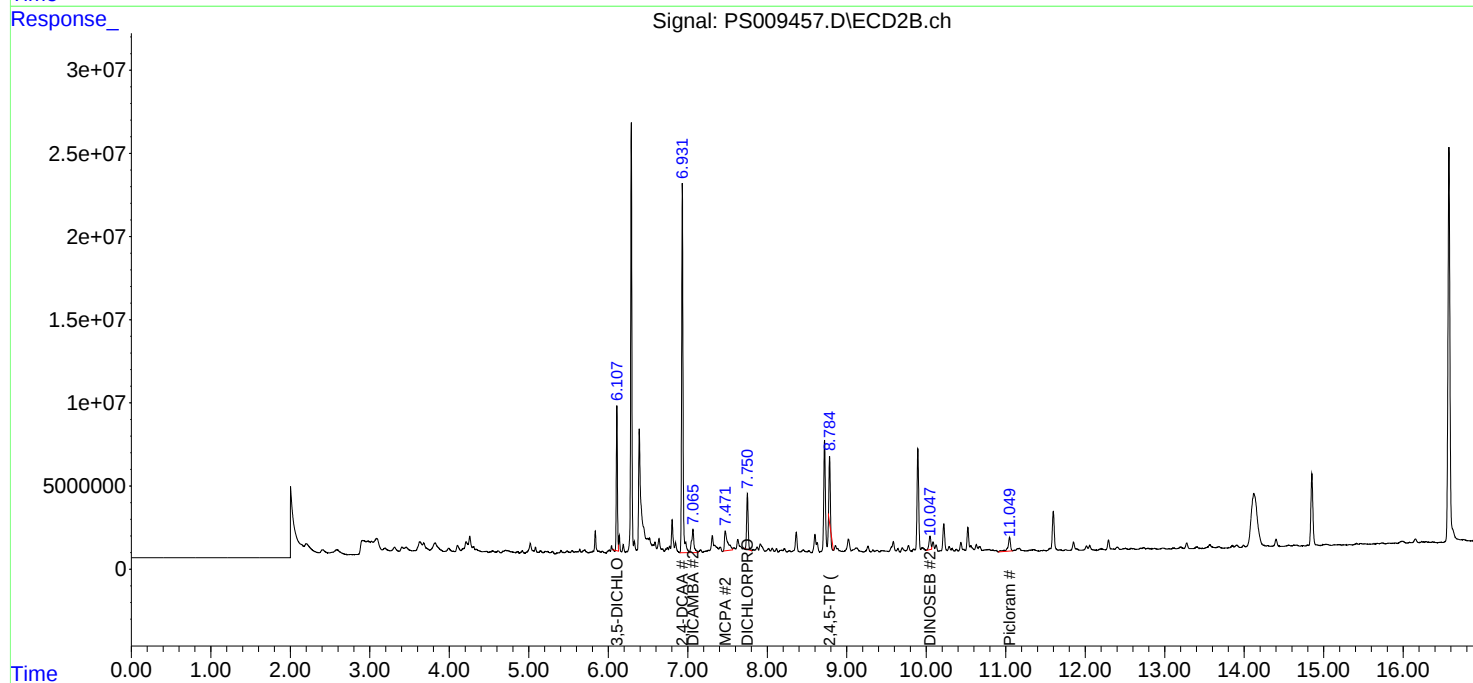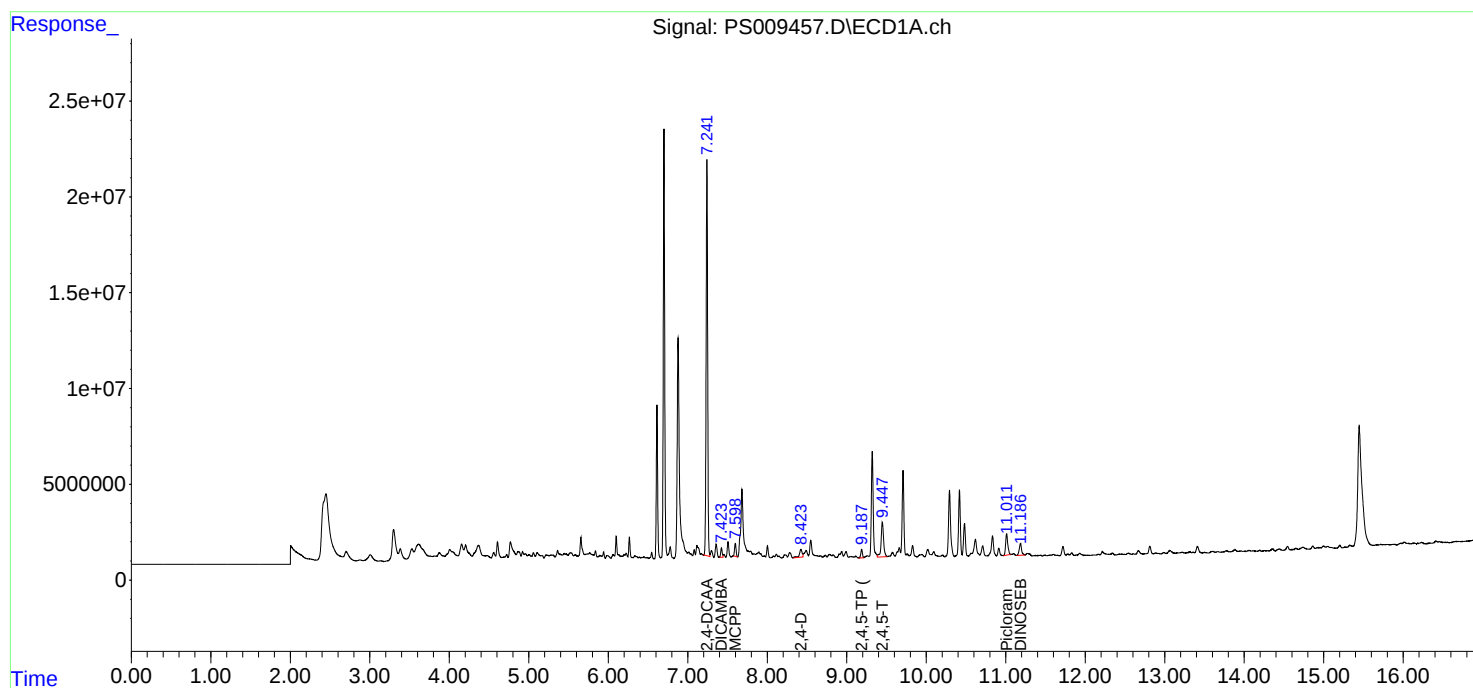


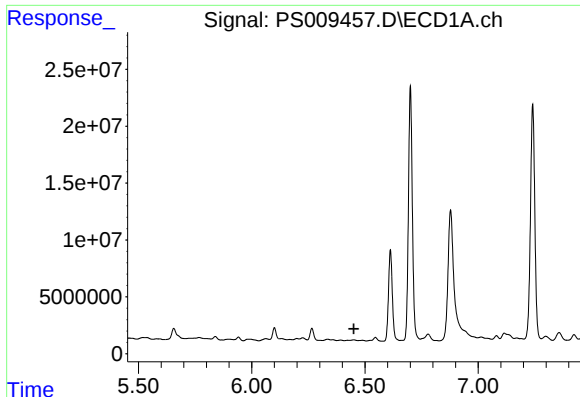

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 6.451 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

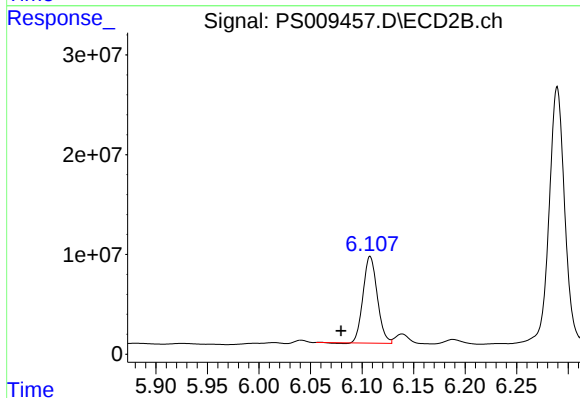


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.108 min
Delta R.T.: 0.028 min
Response: 83579907
Conc: 102.77 ng/ml

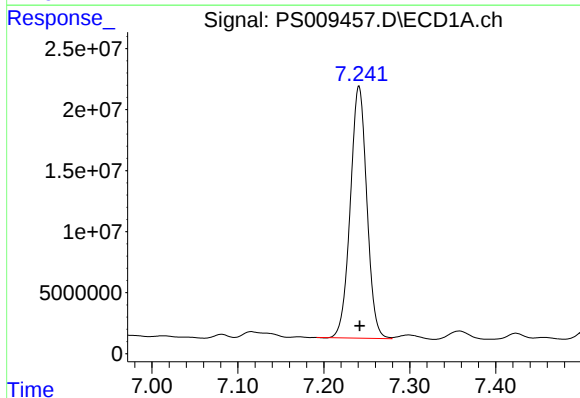


#4 2,4-DCAA

R.T.: 7.241 min
Delta R.T.: -0.001 min
Response: 276195761
Conc: 499.30 ng/ml

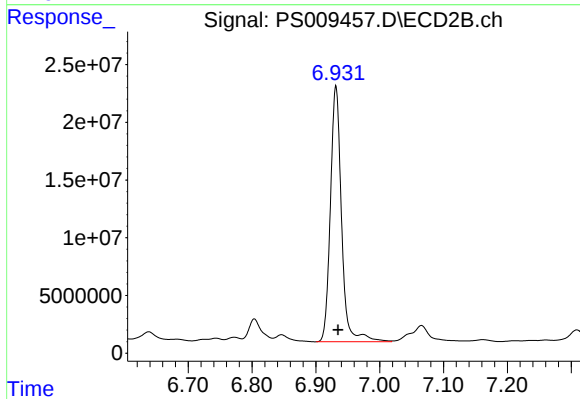

#4 2,4-DCAA


R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 269381764
Conc: 490.50 ng/ml

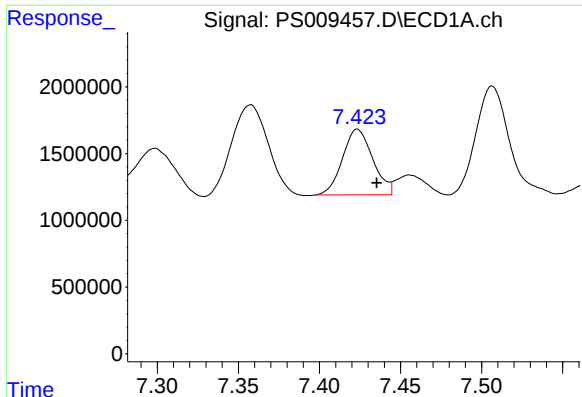

#5 DICAMBA


R.T.: 7.424 min
Delta R.T.: -0.012 min
Response: 6411557
Conc: 3.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

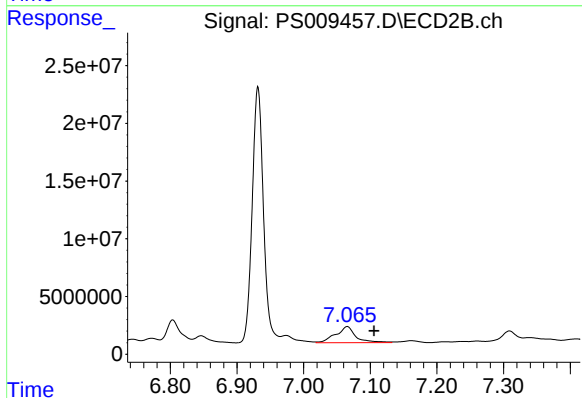


#5 DICAMBA

R.T.: 7.065 min
Delta R.T.: -0.040 min
Response: 29468511
Conc: 12.84 ng/ml

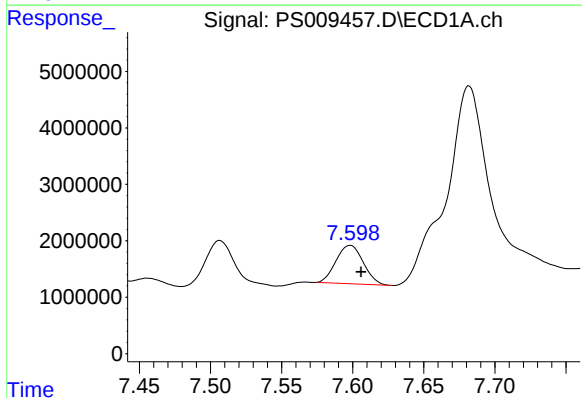


#6 MCP

R.T.: 7.598 min
Delta R.T.: -0.008 min
Response: 9068688
Conc: 3.69 ug/ml

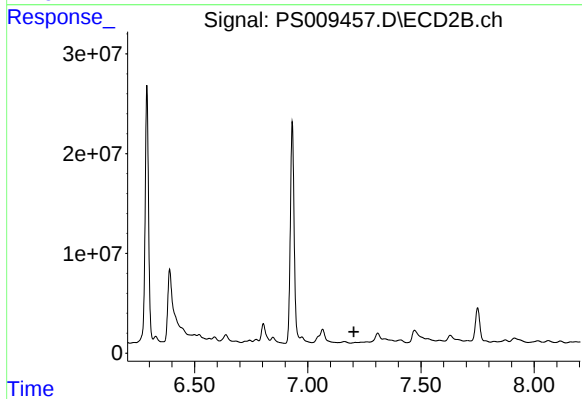

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

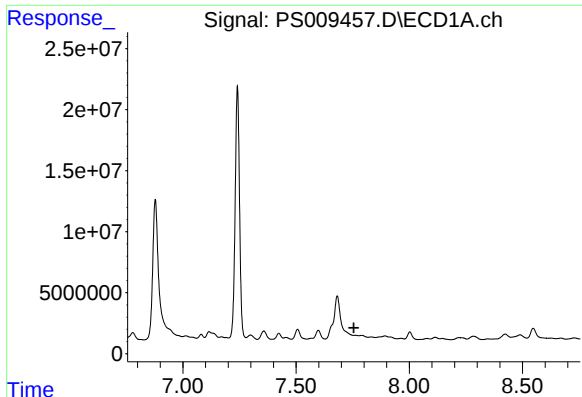

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

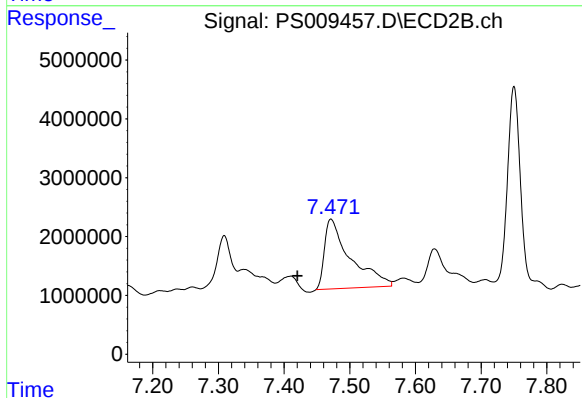


#7 MCPA

R.T.: 7.472 min
Delta R.T.: 0.052 min
Response: 32447381
Conc: 12.02 ug/ml

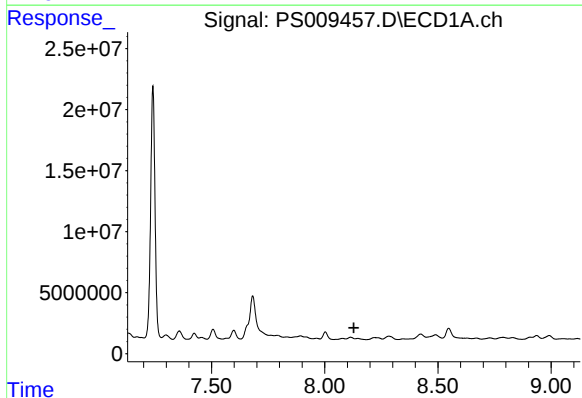


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

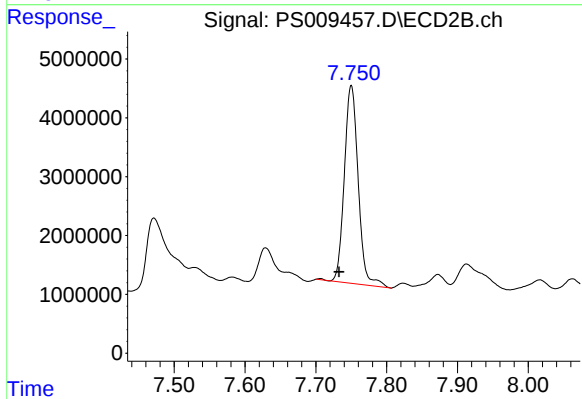

#8 DICHLORPROP


R.T.: 7.750 min
Delta R.T.: 0.017 min
Response: 45792662
Conc: 82.54 ng/ml

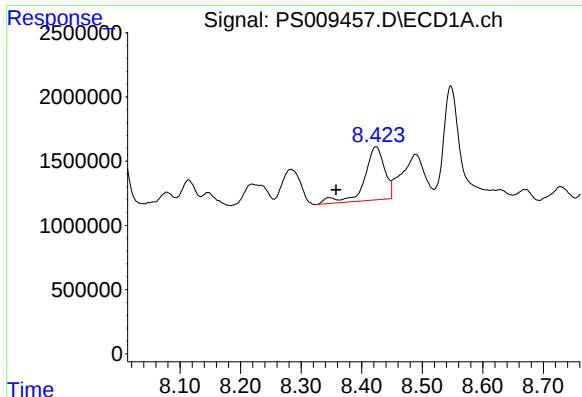

#9 2,4-D


R.T.: 8.424 min
Delta R.T.: 0.066 min
Response: 9625463
Conc: 18.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

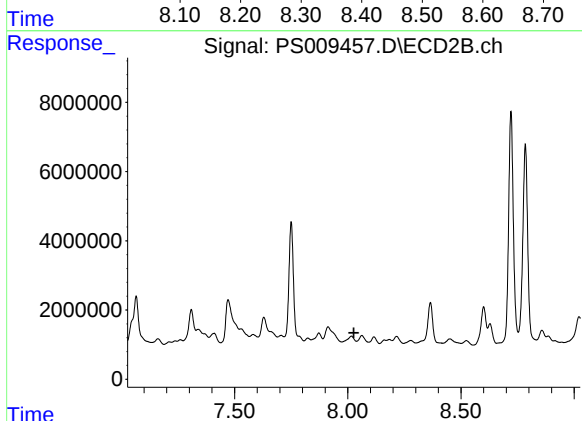


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.027 min
Response: 0
Conc: N.D.

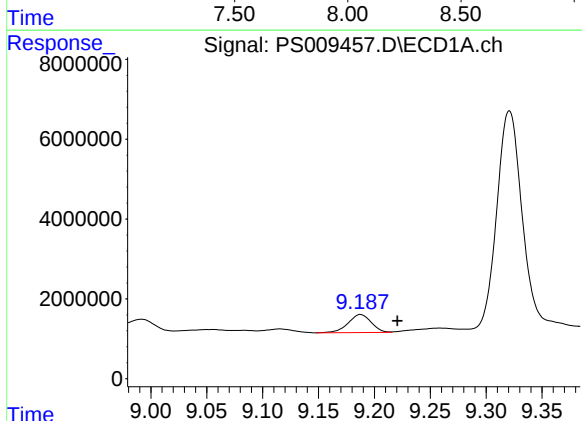


#11 2,4,5-TP (SILVEX)

R.T.: 9.188 min
Delta R.T.: -0.033 min
Response: 6476428
Conc: 2.36 ng/ml

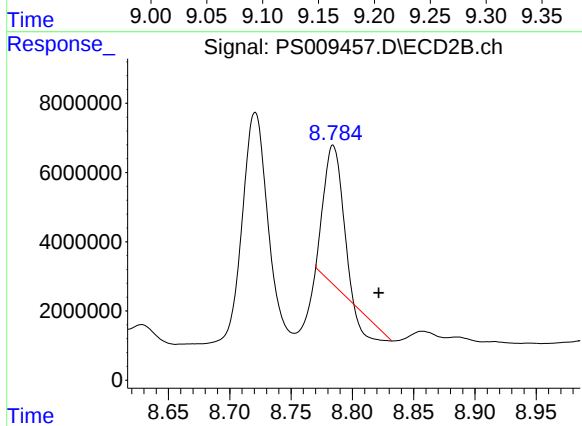

#11 2,4,5-TP (SILVEX)


R.T.: 8.784 min
Delta R.T.: -0.037 min
Response: 36349918
Conc: 12.19 ng/ml

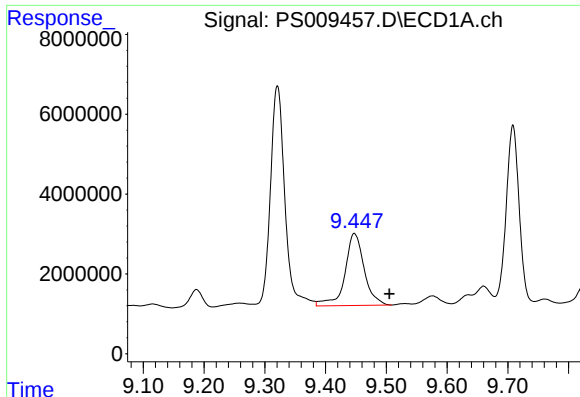

#12 2,4,5-T


R.T.: 9.448 min
Delta R.T.: -0.057 min
Response: 39696769
Conc: 15.60 ng/ml

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

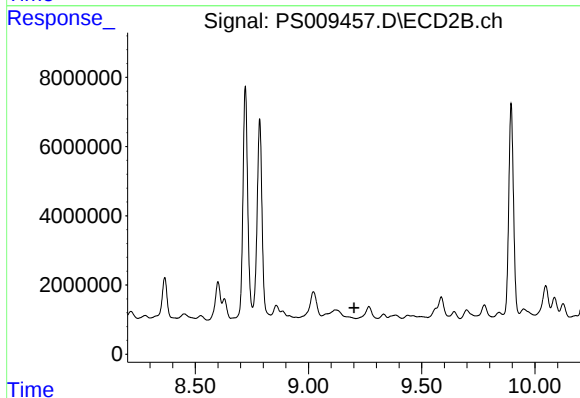


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.201 min
Response: 0
Conc: N.D.

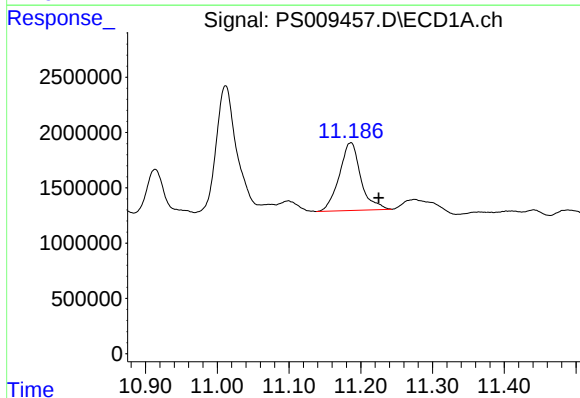


#14 DINOSEB

R.T.: 11.186 min
Delta R.T.: -0.039 min
Response: 12764291
Conc: 6.24 ng/ml

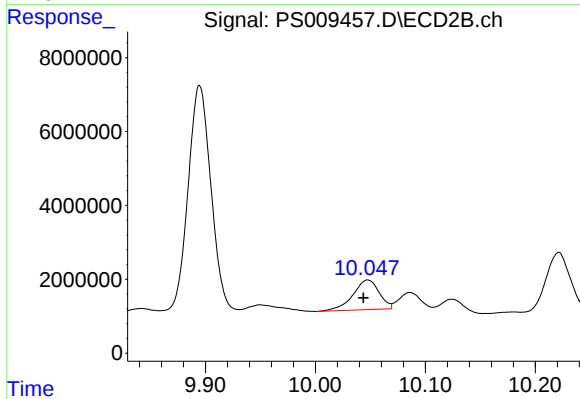

#14 DINOSEB


R.T.: 10.048 min
Delta R.T.: 0.004 min
Response: 13304571
Conc: 6.06 ng/ml

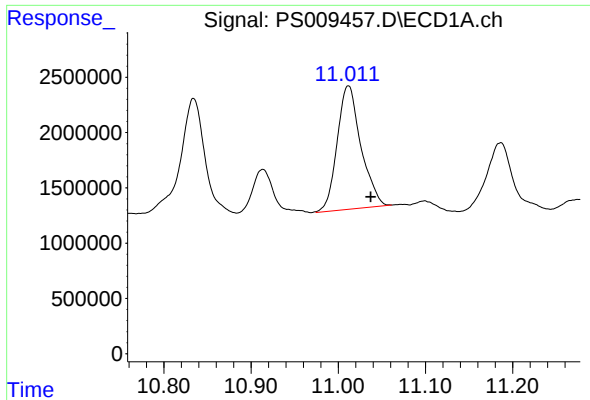

#15 Picloram

R.T.: 11.012 min
Delta R.T.: -0.026 min
Response: 21113458
Conc: 6.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

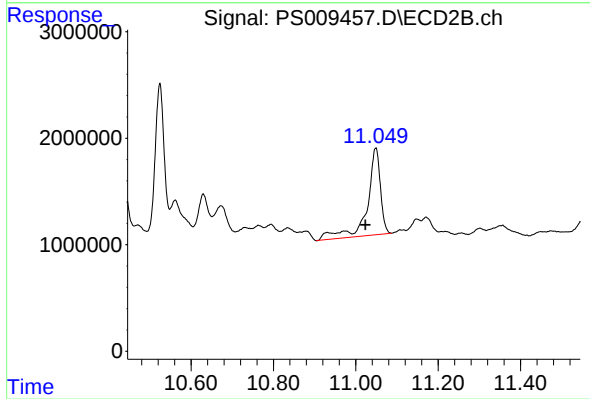

#15 Picloram

R.T.: 11.048 min
Delta R.T.: 0.025 min
Response: 18380801
Conc: 4.51 ng/ml