

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032621\
 Data File : PS014351.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2021 09:20
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 18:58:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
9) T	2,4-D	8.338f	0.000	3565996	0	2.419 N.D. #
15) T	Picloram	10.975	11.004	14673796	5203544	1.405 1.372


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032621\
Data File : PS014351.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2021 09:20
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 18:58:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

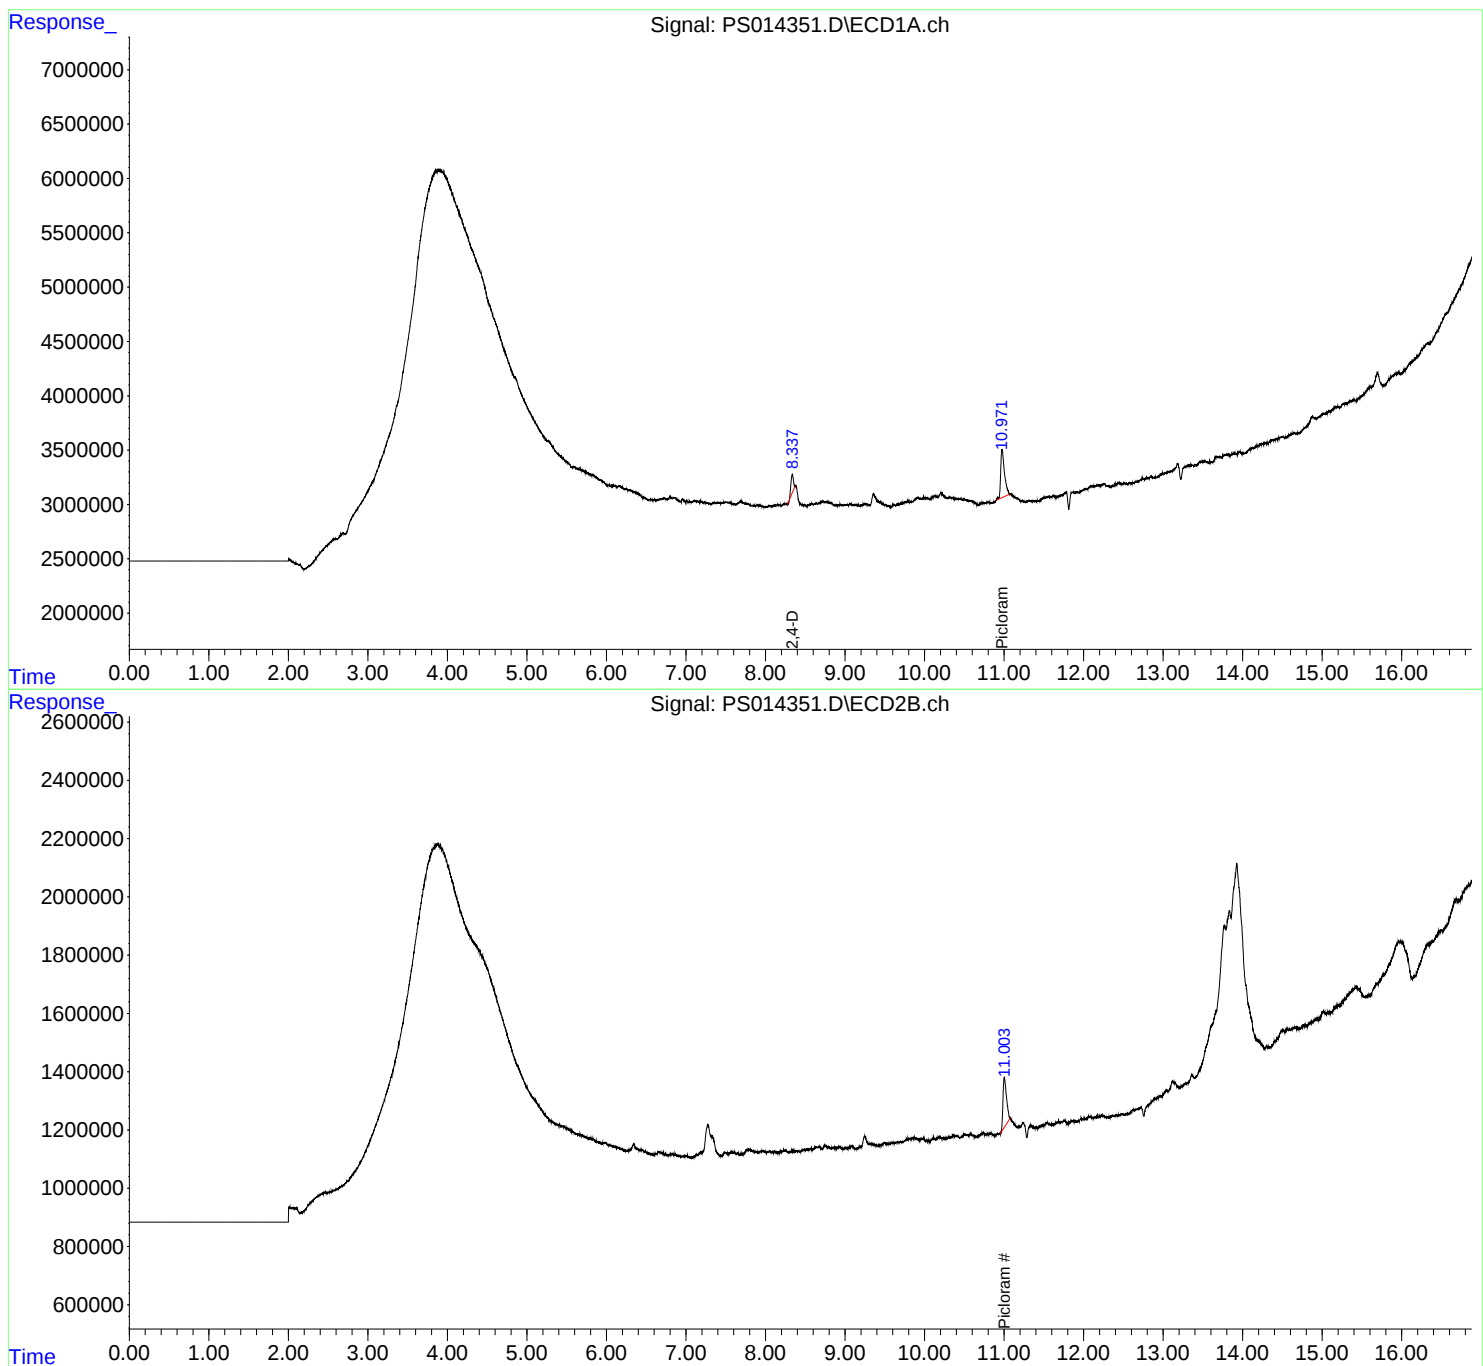


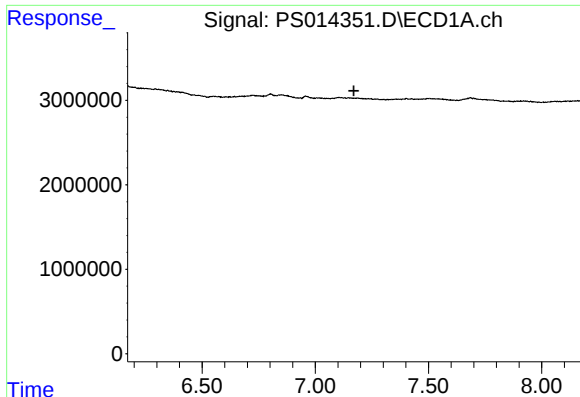

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 7.170 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

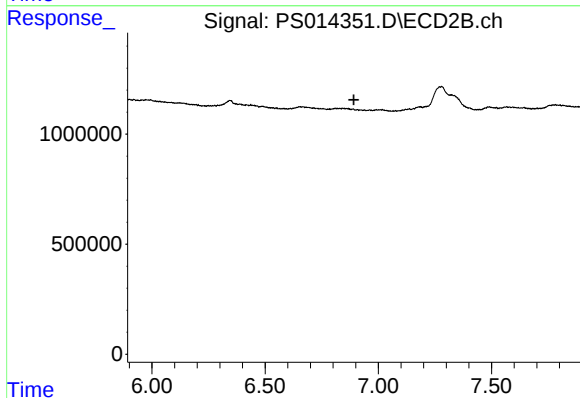


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.892 min
Response: 0
Conc: N.D.

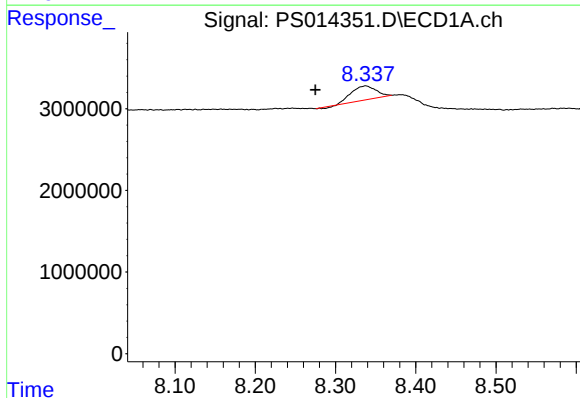


#9 2,4-D

R.T.: 8.338 min
Delta R.T.: 0.063 min
Response: 3565996
Conc: 2.42 ng/ml

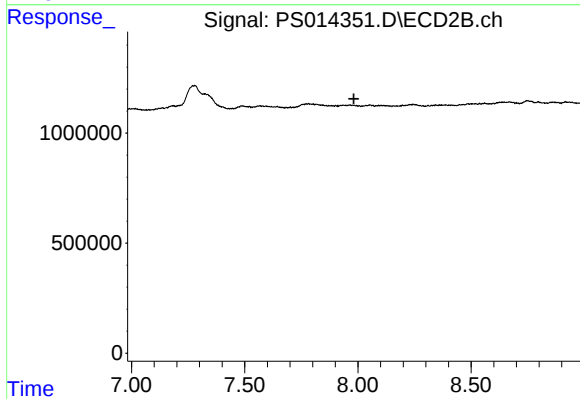

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.982 min
Response: 0
Conc: N.D.

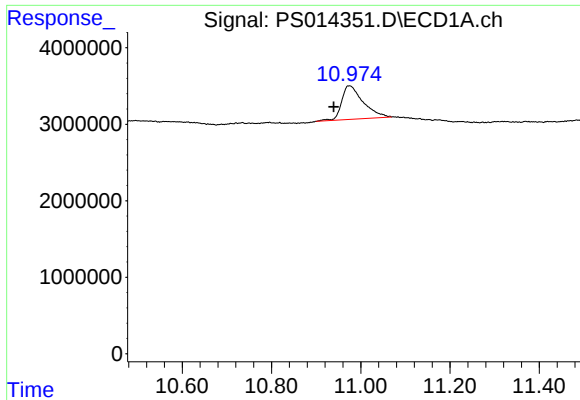

#15 Picloram

R.T.: 10.975 min
Delta R.T.: 0.036 min
Response: 14673796
Conc: 1.41 ng/ml

Instrument :
ECD_S
ClientSampleId :

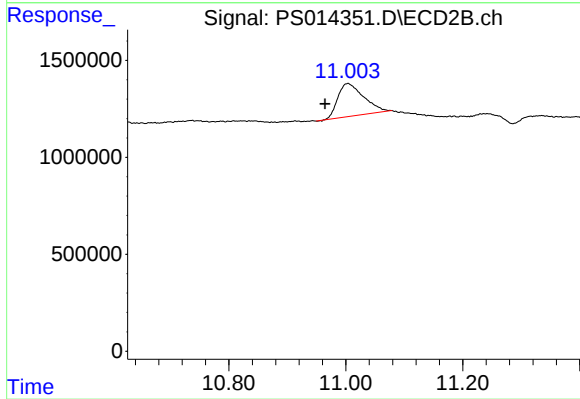

#15 Picloram

R.T.: 11.004 min
Delta R.T.: 0.039 min
Response: 5203544
Conc: 1.37 ng/ml