

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032621\
 Data File : PS014364.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2021 19:23
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 19:46:00 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 18 02:23:19 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.165	6.889	647.2E6	258.9E6	452.941	548.752
Target Compounds							
5) T	DICAMBA	7.354	7.057	3657639	2127692	<MDL	1.062 #
9) T	2,4-D	8.331f	0.000	14295592	0	9.699	N.D. #
10) T	Pentachlo...	8.578	8.405	12180714	4906246	<MDL	<MDL #
11) T	2,4,5-TP ...	9.128	8.771	5597505	3122470	<MDL	1.148 #
12) T	2,4,5-T	9.432	0.000	6849050	0	<MDL	N.D. #
14) T	DINOSEB	11.106	0.000	5251205	0	<MDL	N.D. #
15) T	Picloram	10.973	10.999	12223390	2866431	1.171	<MDL #
16) T	DCPA	11.371	10.904	8176179	2941933	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032621\
Data File : PS014364.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2021 19:23
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 19:46:00 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031721.M
Quant Title : 8080.M
QLast Update : Thu Mar 18 02:23:19 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

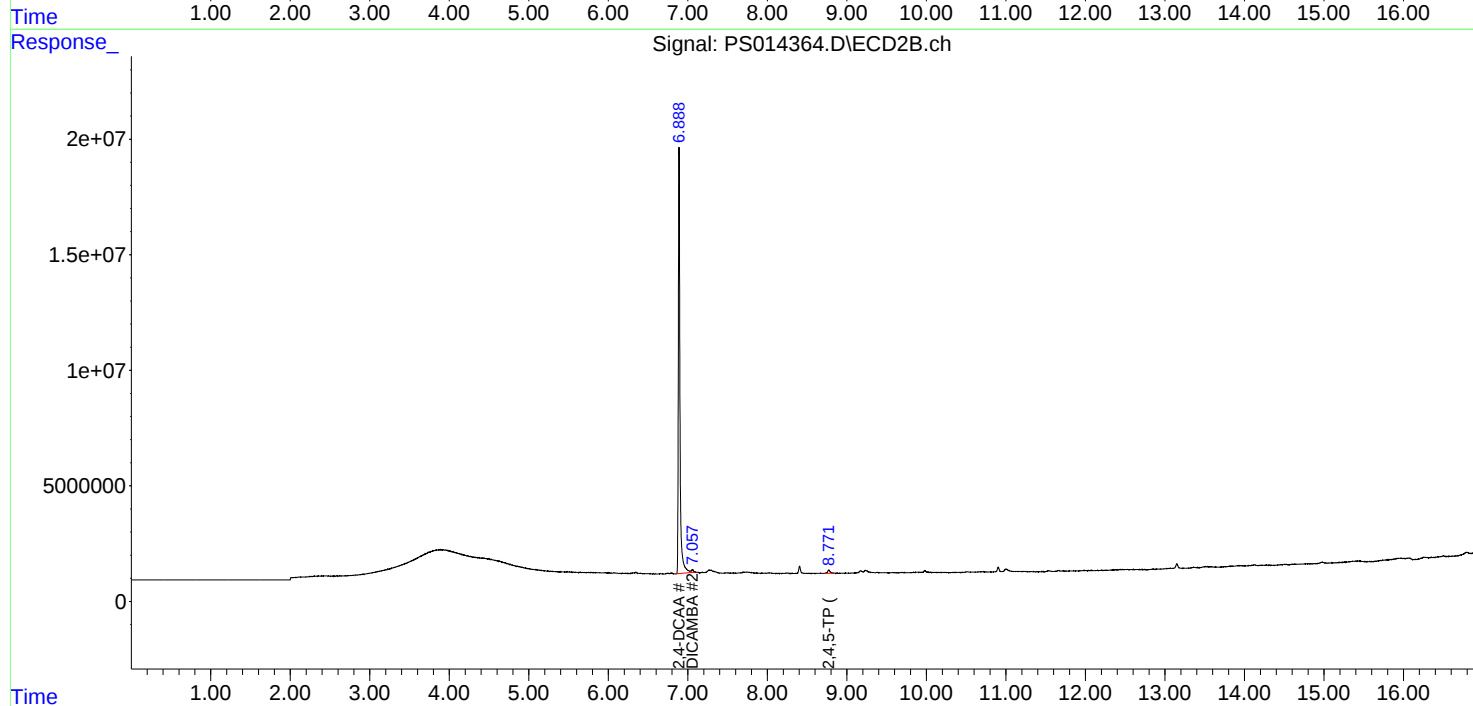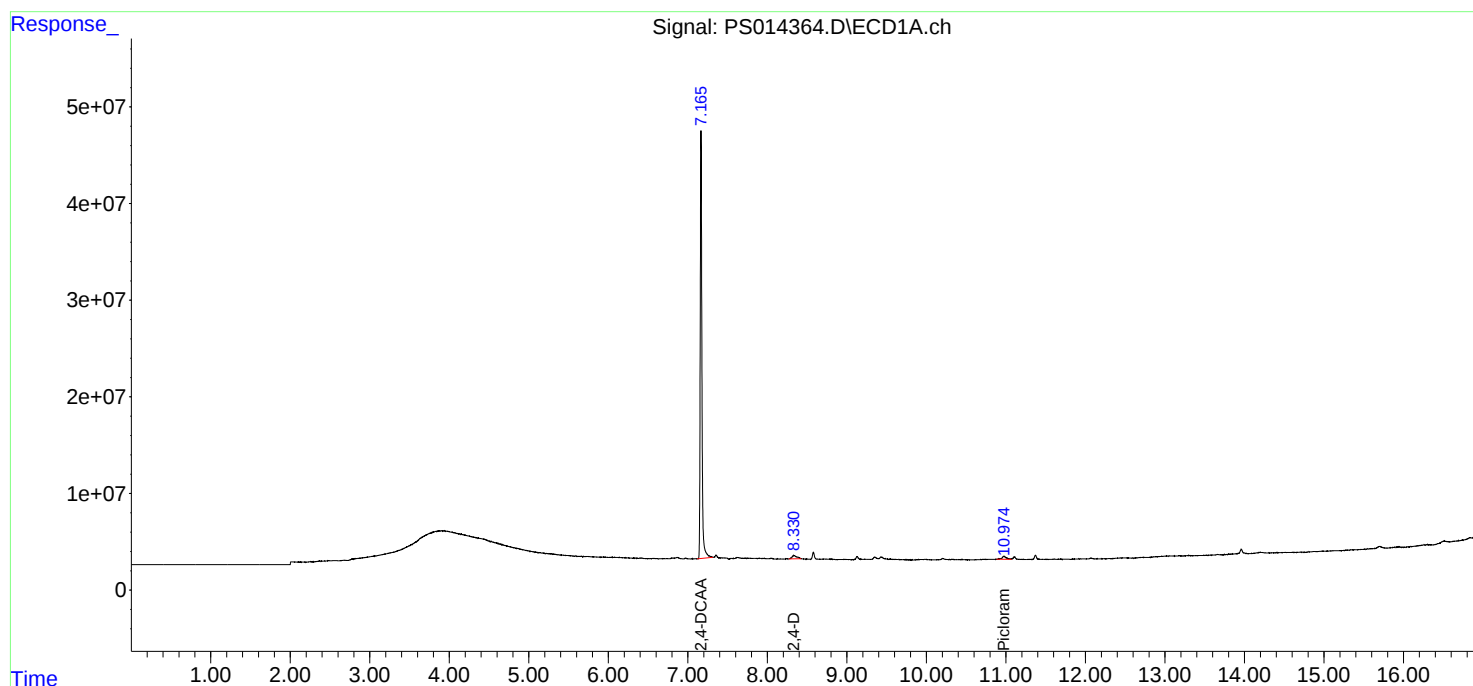


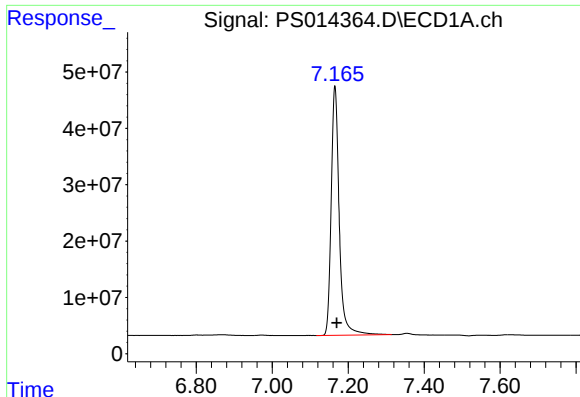

#4 2,4-DCAA


R.T.: 7.165 min
Delta R.T.: -0.005 min
Response: 647181366
Conc: 452.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

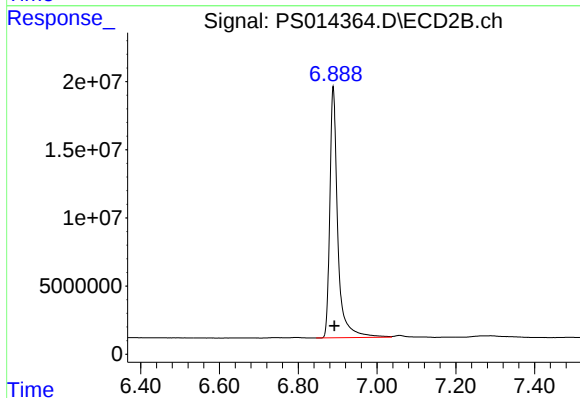


#4 2,4-DCAA

R.T.: 6.889 min
Delta R.T.: -0.003 min
Response: 258884235
Conc: 548.75 ng/ml

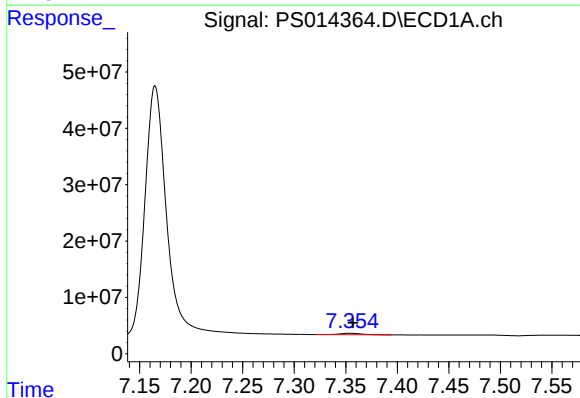


#5 DICAMBA

R.T.: 7.354 min
Delta R.T.: -0.003 min
Response: 3657639
Conc: N.D.

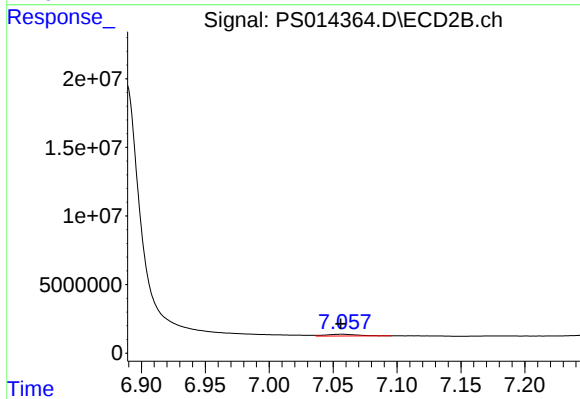

#5 DICAMBA


R.T.: 7.057 min
Delta R.T.: 0.001 min
Response: 2127692
Conc: 1.06 ng/ml

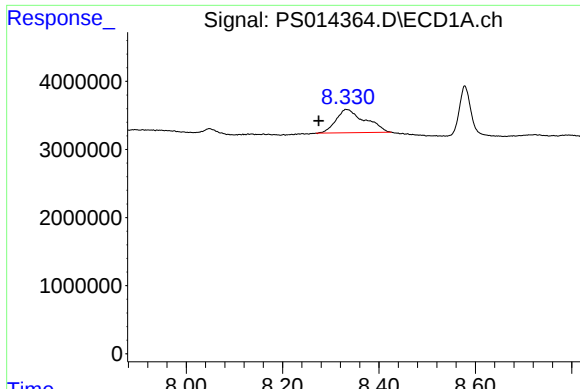

#9 2,4-D


R.T.: 8.331 min
Delta R.T.: 0.057 min
Response: 14295592
Conc: 9.70 ng/ml

Instrument :
ECD_S
ClientSampleId :

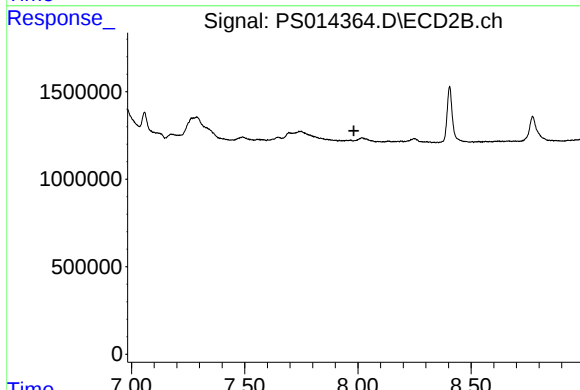


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.982 min
Response: 0
Conc: N.D.

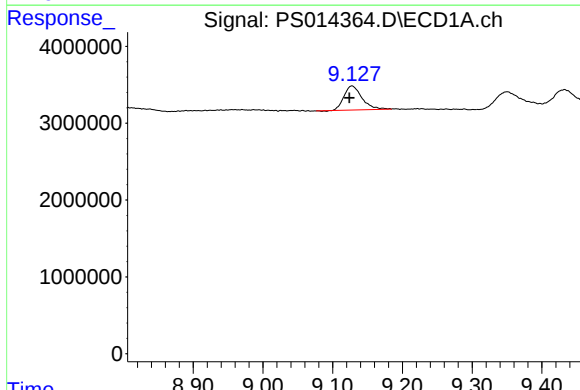


#11 2,4,5-TP (SILVEX)

R.T.: 9.128 min
Delta R.T.: 0.004 min
Response: 5597505
Conc: N.D.

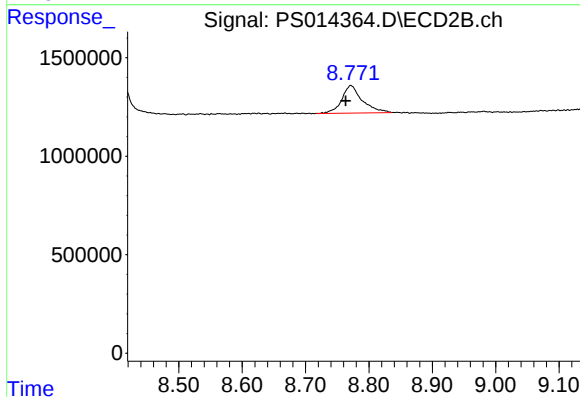

#11 2,4,5-TP (SILVEX)


R.T.: 8.771 min
Delta R.T.: 0.008 min
Response: 3122470
Conc: 1.15 ng/ml

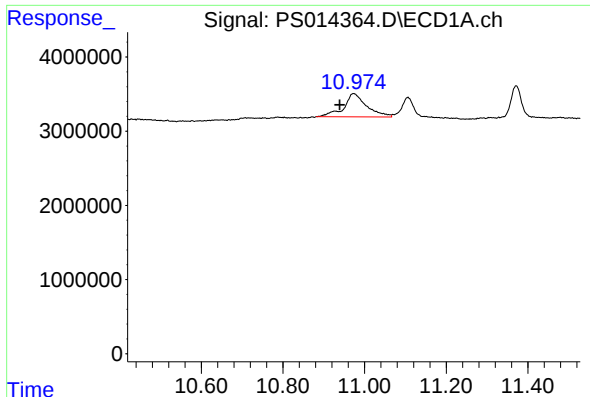

#15 Picloram

R.T.: 10.973 min
Delta R.T.: 0.034 min
Response: 12223390
Conc: 1.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

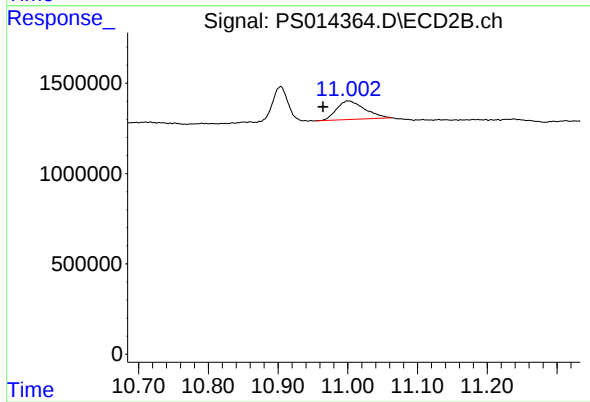

#15 Picloram

R.T.: 10.999 min
Delta R.T.: 0.034 min
Response: 2866431
Conc: N.D.