

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032719\
 Data File : PS003780.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2019 10:34
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 04:53:05 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.300	10.799	176.5E6	160.7E6	404.530	327.596
Target Compounds							
7) T	MCPA	0.000	11.683	0	377210	N.D.	0.212 #
8) T	DICHLORPROP	0.000	12.193	0	1606152	N.D.	3.450 #
9) T	2,4-D	0.000	12.622	0	405207	N.D.	0.762 #
10) T	Pentachlo...	0.000	13.210	0	2231971	N.D.	0.323 #
11) T	2,4,5-TP ...	0.000	13.859	0	225968	N.D.	0.085 #
12) T	2,4,5-T	0.000	14.335	0	596859	N.D.	0.275 #
13) T	2,4-DB	0.000	15.013	0	286929	N.D.	0.966 #
14) T	DINOSEB	0.000	15.468	0	542462	N.D.	0.283 #
15) T	Picloram	0.000	16.645	0	568131	N.D.	0.179 #
16) T	DCPA	0.000	16.645	0	568131	N.D.	0.168 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032719\
Data File : PS003780.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2019 10:34
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 04:53:05 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

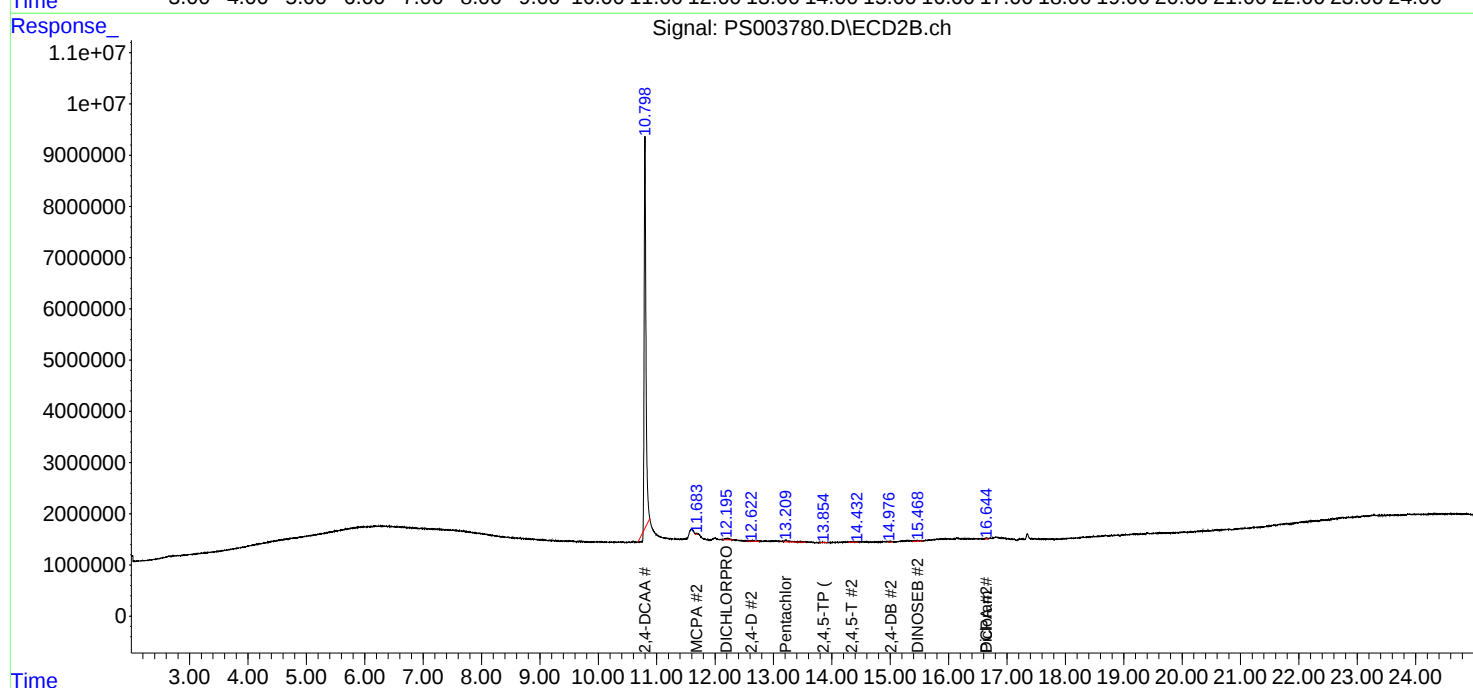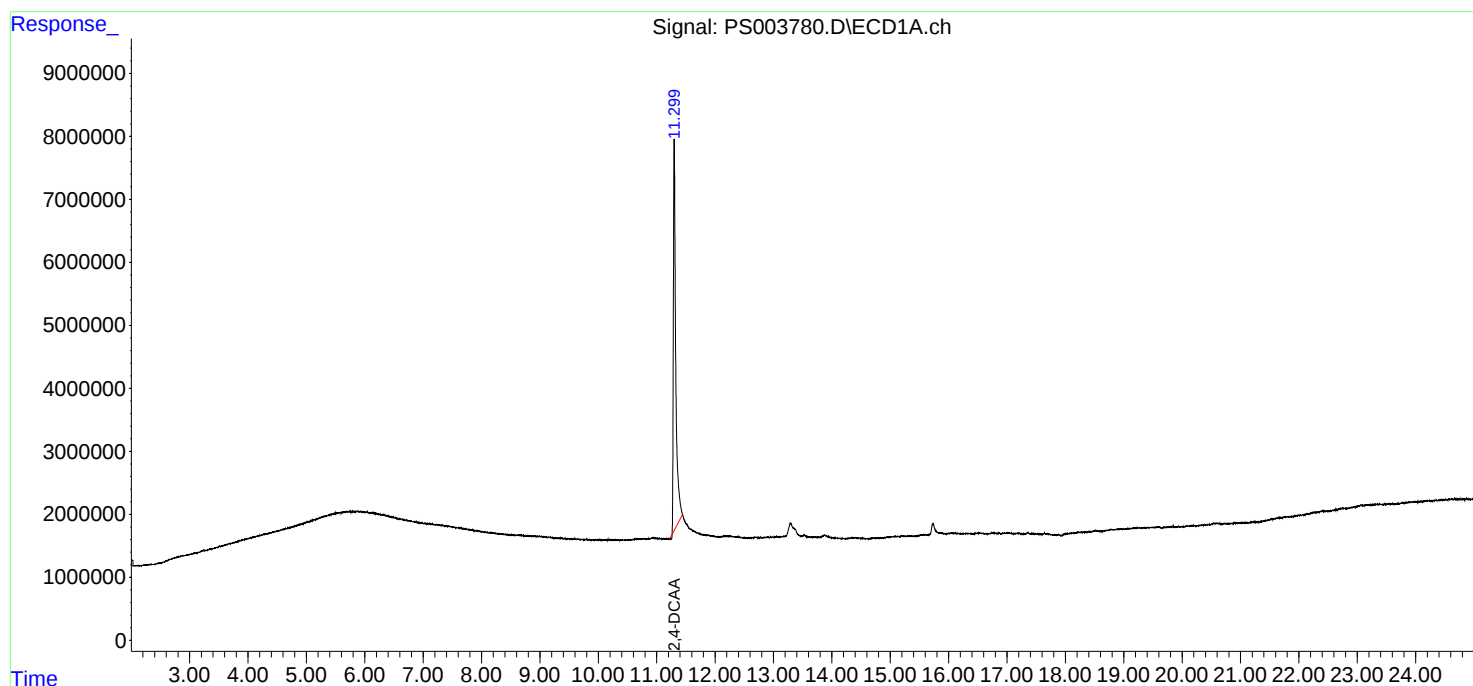


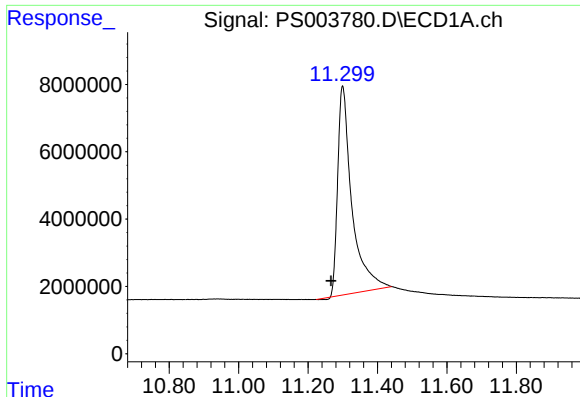

#4 2,4-DCAA


R.T.: 11.300 min
Delta R.T.: 0.033 min
Response: 176461143
Conc: 404.53 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

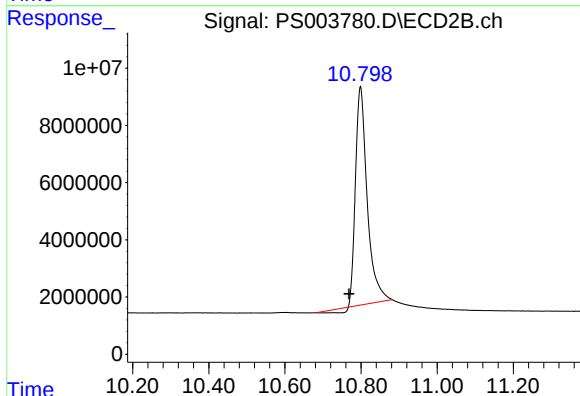


#4 2,4-DCAA

R.T.: 10.799 min
Delta R.T.: 0.030 min
Response: 160737711
Conc: 327.60 ng/ml

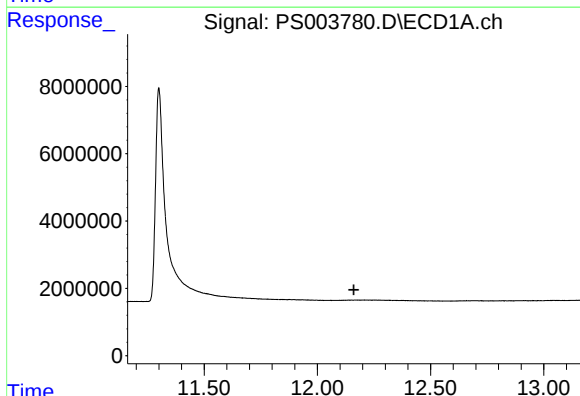


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

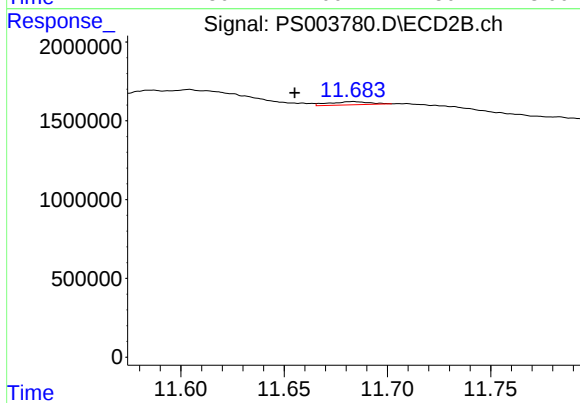

#7 MCPA


R.T.: 11.683 min
Delta R.T.: 0.028 min
Response: 377210
Conc: 0.21 ug/ml

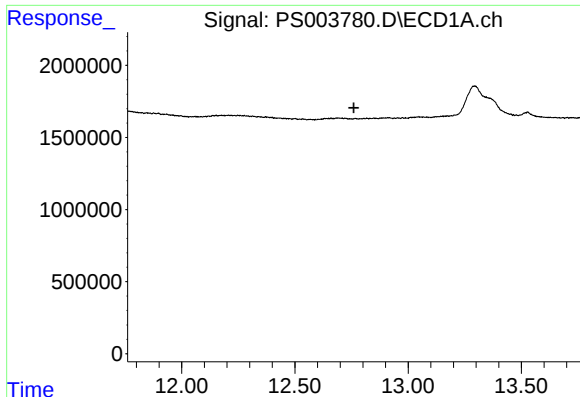

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

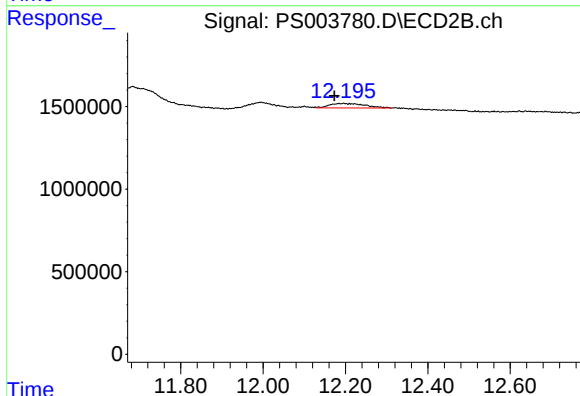


#8 DICHLORPROP

R.T.: 12.193 min
Delta R.T.: 0.020 min
Response: 1606152
Conc: 3.45 ng/ml

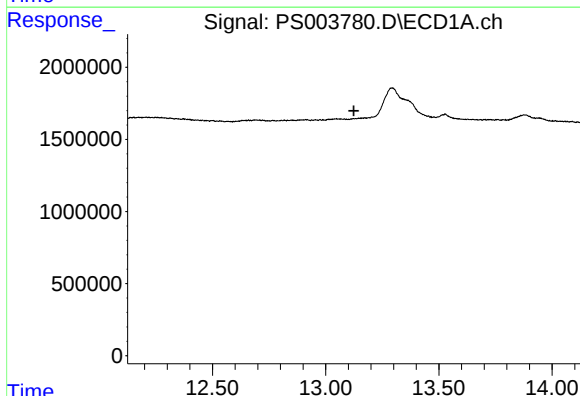


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

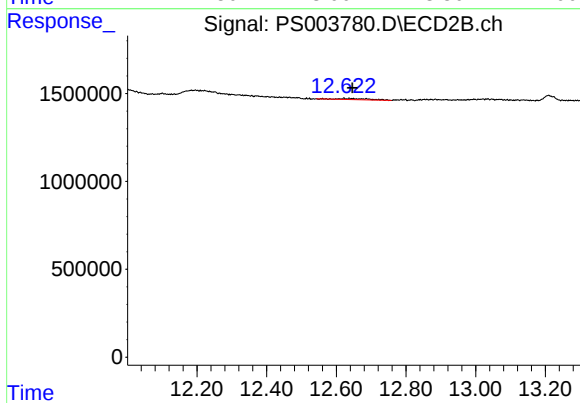

#9 2,4-D


R.T.: 12.622 min
Delta R.T.: -0.024 min
Response: 405207
Conc: 0.76 ng/ml

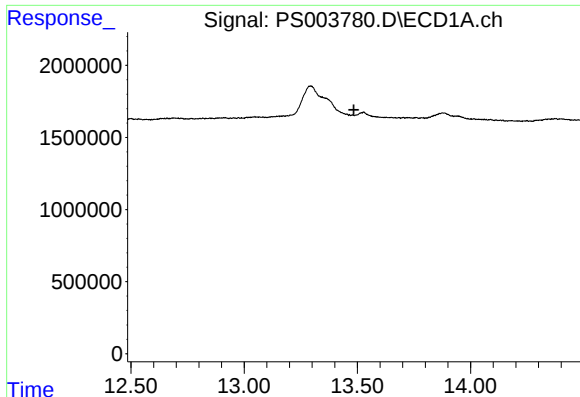

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

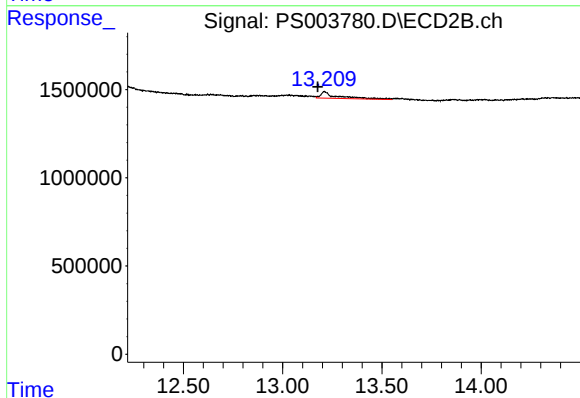


#10 Pentachlorophenol

R.T.: 13.210 min
Delta R.T.: 0.033 min
Response: 2231971
Conc: 0.32 ng/ml

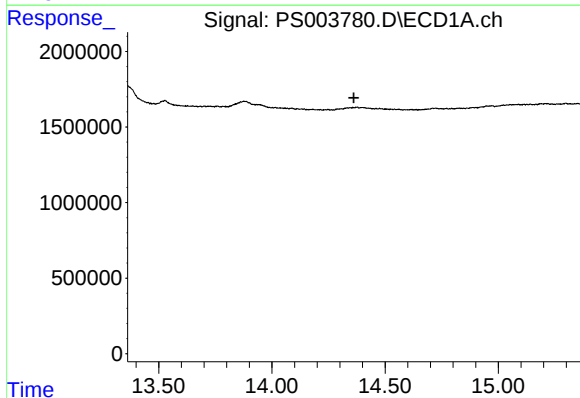


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

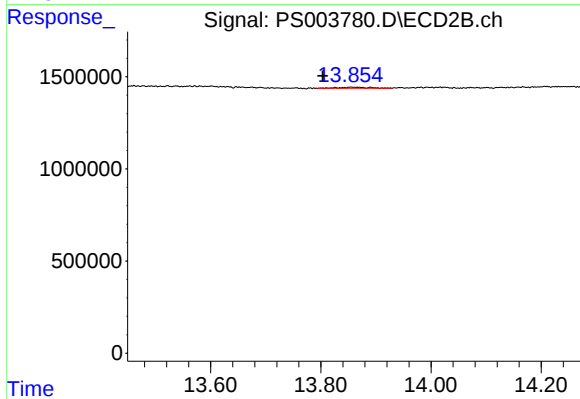

#11 2,4,5-TP (SILVEX)


R.T.: 13.859 min
Delta R.T.: 0.056 min
Response: 225968
Conc: 0.09 ng/ml

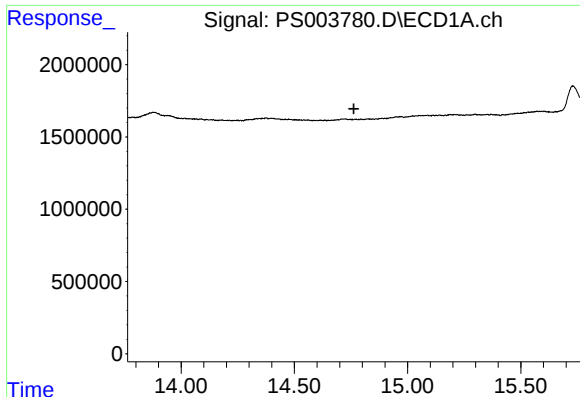

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

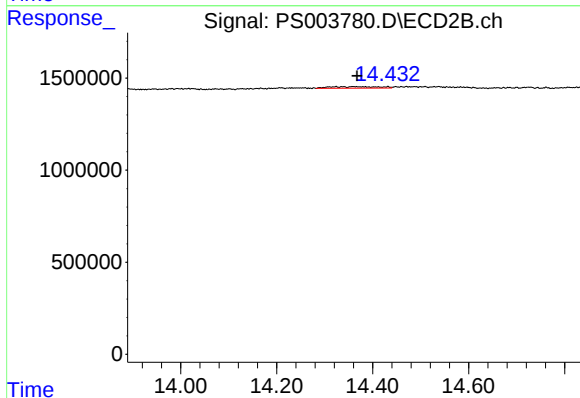


#12 2,4,5-T

R.T.: 14.335 min
Delta R.T.: -0.033 min
Response: 596859
Conc: 0.27 ng/ml

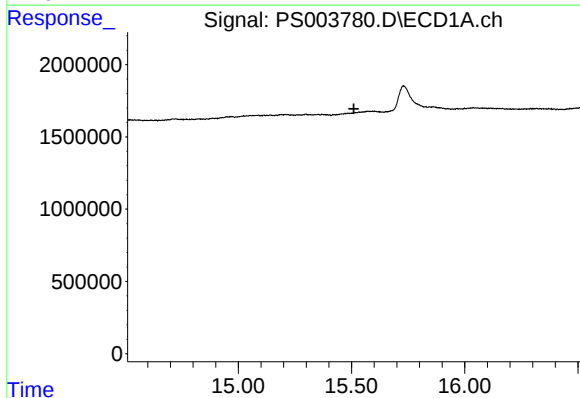


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

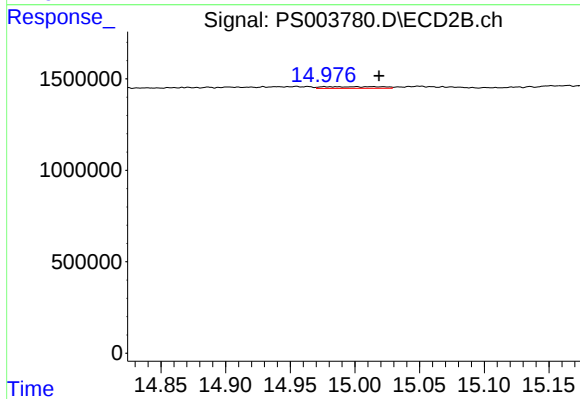

#13 2,4-DB


R.T.: 15.013 min
Delta R.T.: -0.006 min
Response: 286929
Conc: 0.97 ng/ml

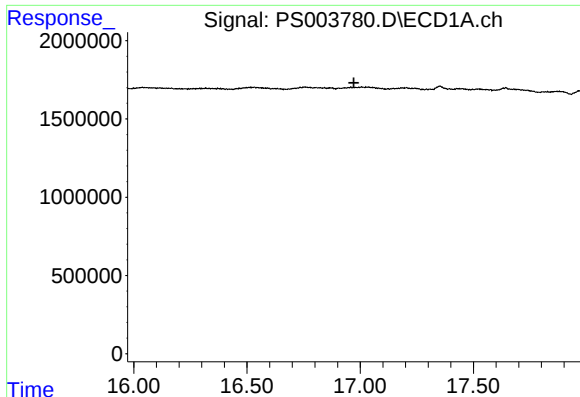

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

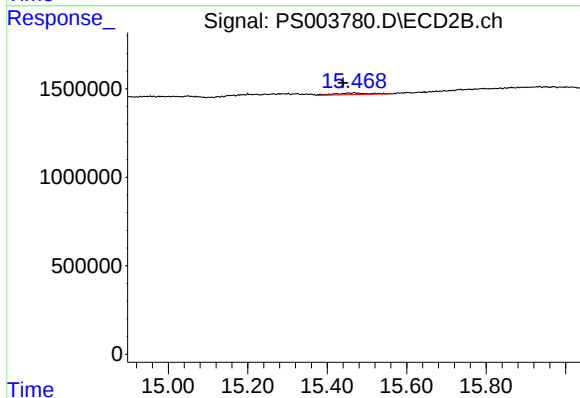


#14 DINOSEB

R.T.: 15.468 min
Delta R.T.: 0.028 min
Response: 542462
Conc: 0.28 ng/ml

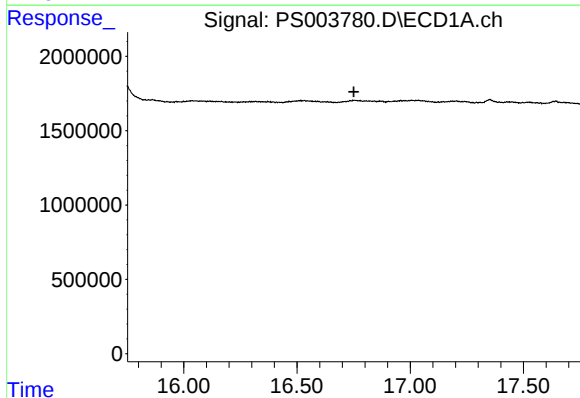


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

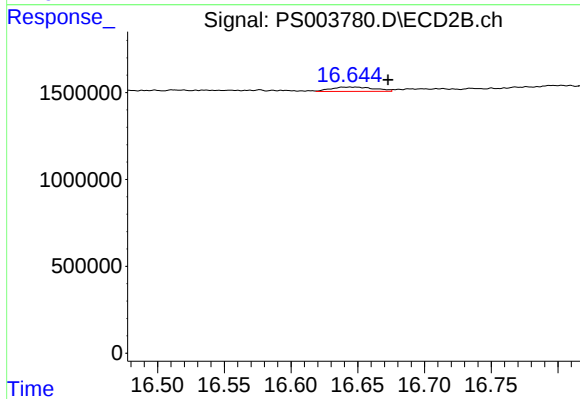

#15 Picloram


R.T.: 16.645 min
Delta R.T.: -0.027 min
Response: 568131
Conc: 0.18 ng/ml

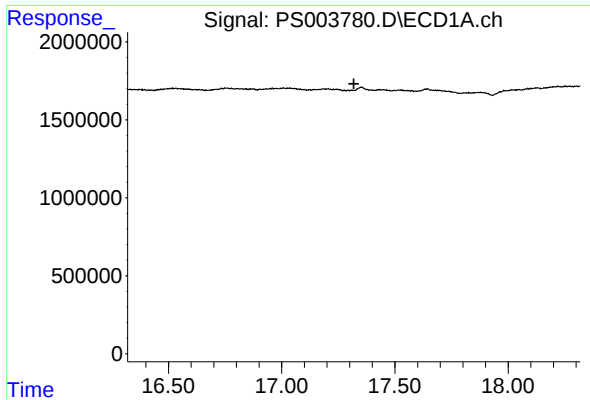

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

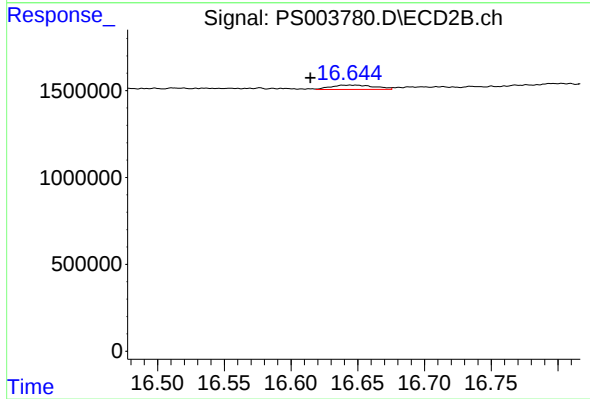

#16 DCPA

R.T.: 16.645 min
Delta R.T.: 0.031 min
Response: 568131
Conc: 0.17 ng/ml