

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032719\
 Data File : PS003785.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2019 13:23
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 04:55:36 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.278	10.778	184.9E6	178.7E6	423.812	364.200
Target Compounds							
2) T	3,5-DICHL...	0.000	8.948	0	7798	N.D.	0.012 #
3) T	4-Nitroph...	0.000	9.953	0	382971	N.D.	1.687 #
7) T	MCPA	0.000	11.663	0	1095790	N.D.	0.614 #
8) T	DICHLORPROP	0.000	12.165	0	2284078	N.D.	4.906 #
9) T	2,4-D	0.000	12.662	0	149221	N.D.	0.281 #
10) T	Pentachlo...	0.000	13.192	0	1344676	N.D.	0.194 #
11) T	2,4,5-TP ...	0.000	13.839	0	326373	N.D.	0.123 #
14) T	DINOSEB	0.000	15.457	0	1026322	N.D.	0.535 #
15) T	Picloram	0.000	16.624	0	898875	N.D.	0.283 #
16) T	DCPA	0.000	16.624	0	898875	N.D.	0.266 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032719\
Data File : PS003785.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2019 13:23
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 04:55:36 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

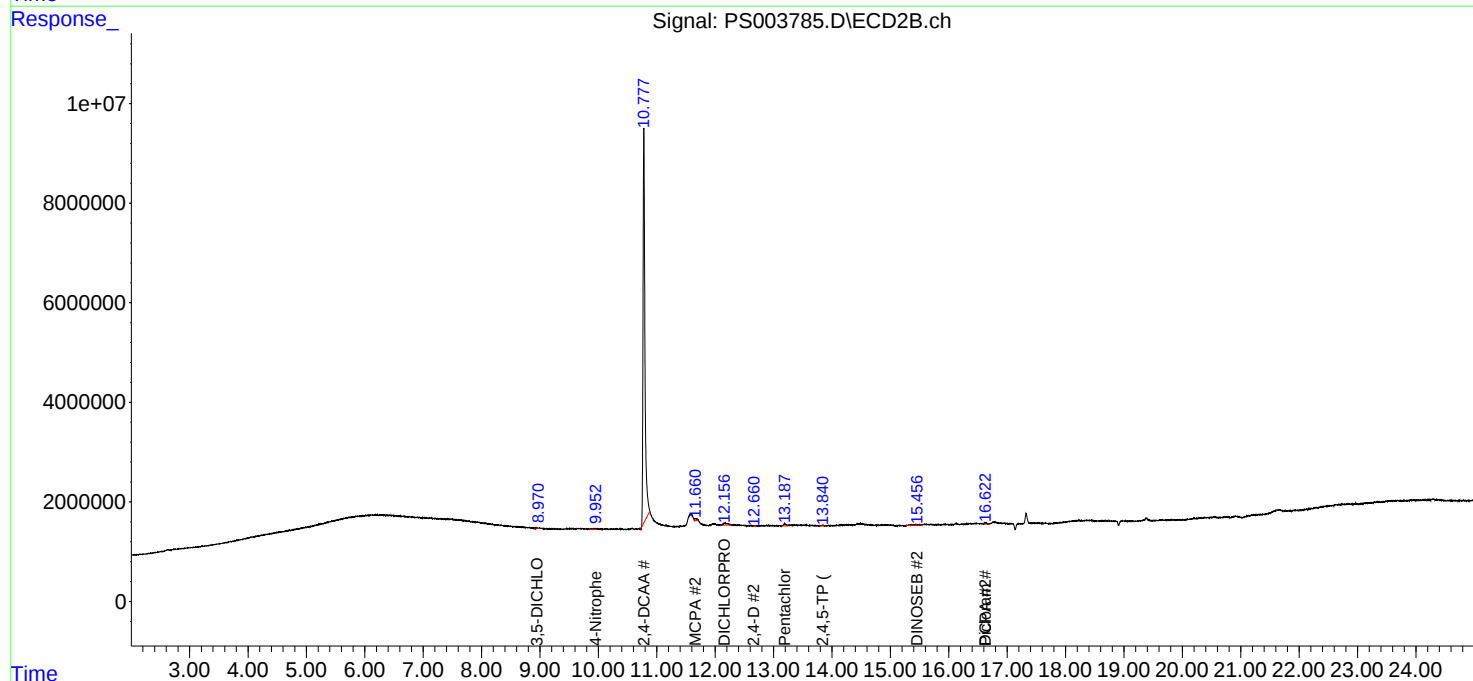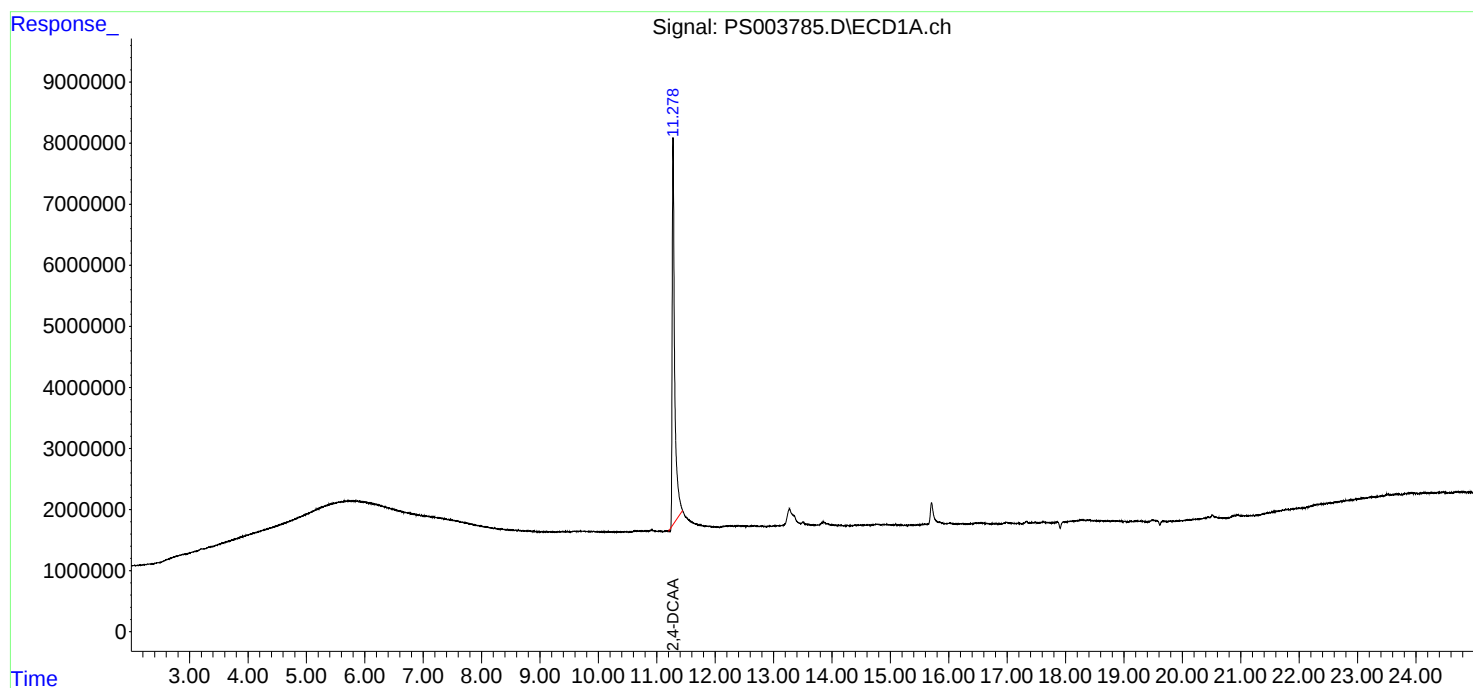


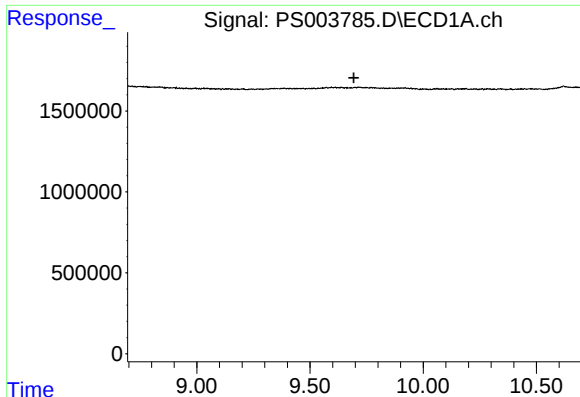

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

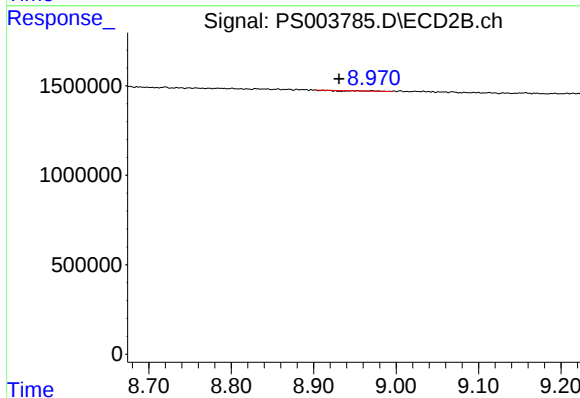


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.948 min
Delta R.T.: 0.017 min
Response: 7798
Conc: 0.01 ng/ml

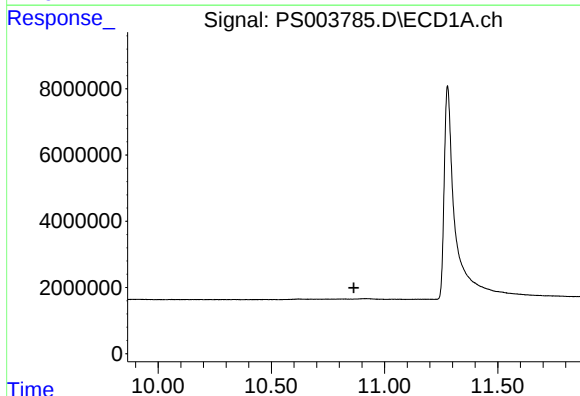


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

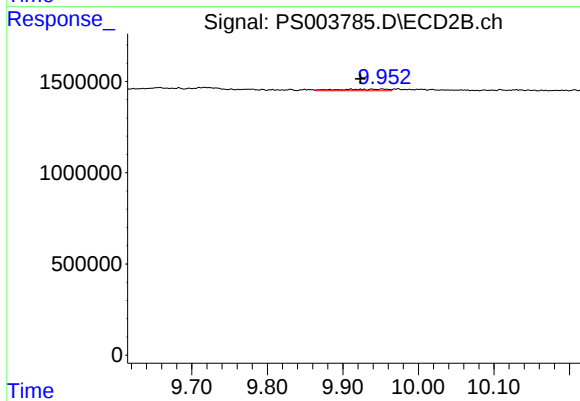

#3 4-Nitrophenol


R.T.: 9.953 min
Delta R.T.: 0.030 min
Response: 382971
Conc: 1.69 ng/ml

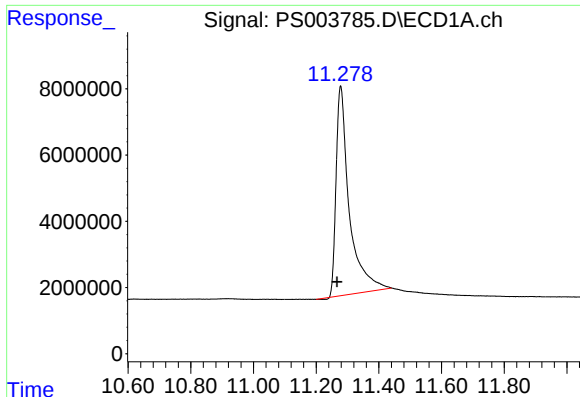

#4 2,4-DCAA


R.T.: 11.278 min
Delta R.T.: 0.011 min
Response: 184872060
Conc: 423.81 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

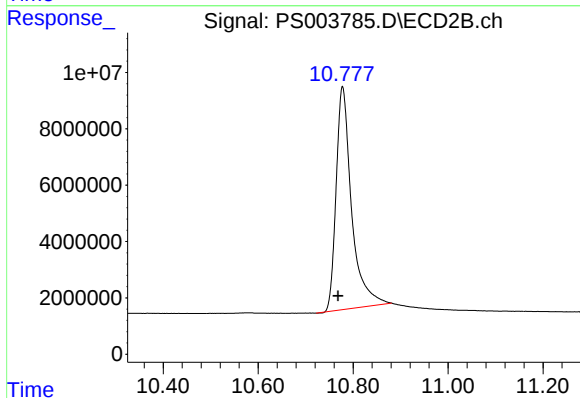


#4 2,4-DCAA

R.T.: 10.778 min
Delta R.T.: 0.009 min
Response: 178697631
Conc: 364.20 ng/ml

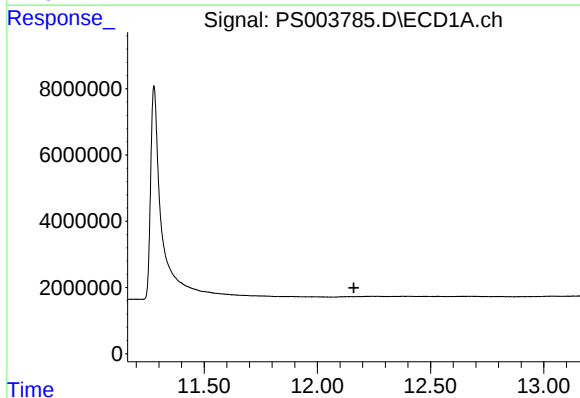


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

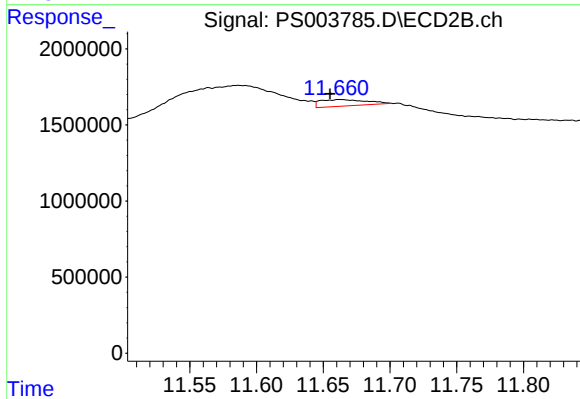

#7 MCPA


R.T.: 11.663 min
Delta R.T.: 0.008 min
Response: 1095790
Conc: 0.61 ug/ml

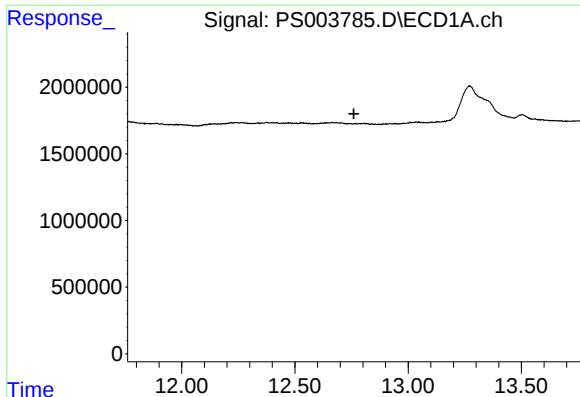

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T. : 12.760 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

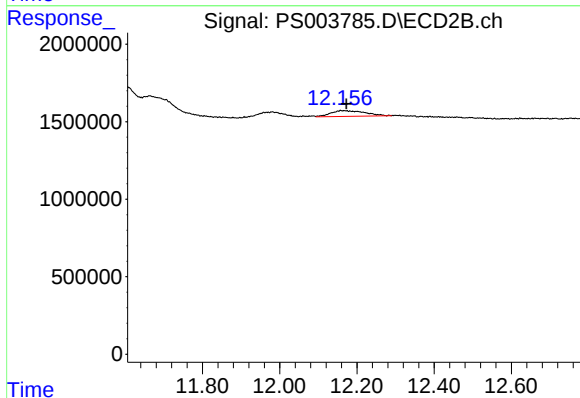


#8 DICHLORPROP

R.T.: 12.165 min
Delta R.T.: -0.008 min
Response: 2284078
Conc: 4.91 ng/ml

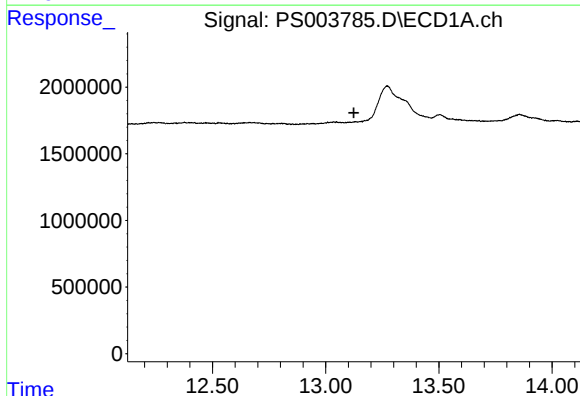


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 13.125 min
Response: 0
Conc: N.D.

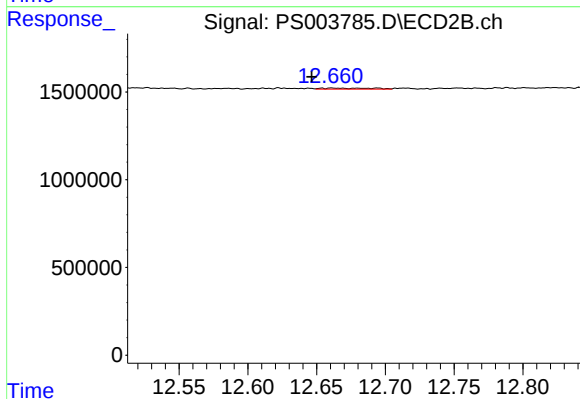

#9 2,4-D


R.T.: 12.662 min
Delta R.T.: 0.016 min
Response: 149221
Conc: 0.28 ng/ml

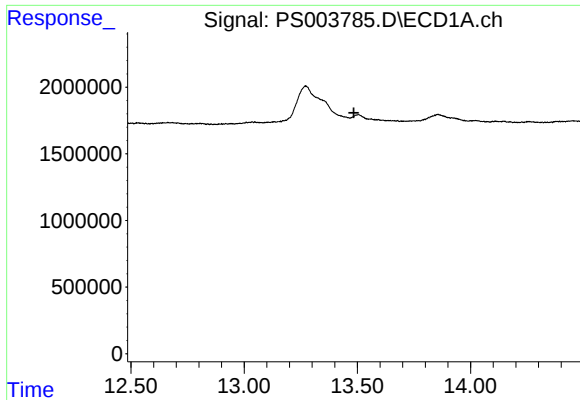

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T. : 13.485 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

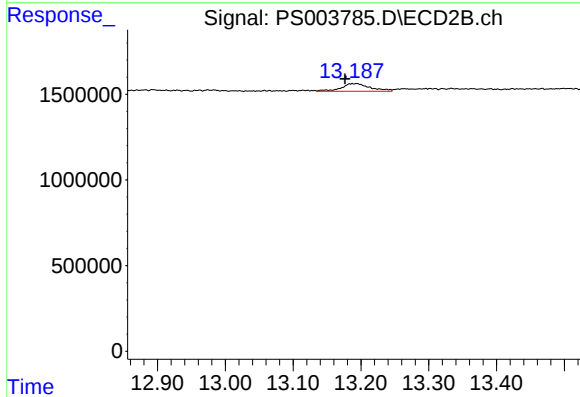


#10 Pentachlorophenol

R.T.: 13.192 min
Delta R.T.: 0.015 min
Response: 1344676
Conc: 0.19 ng/ml

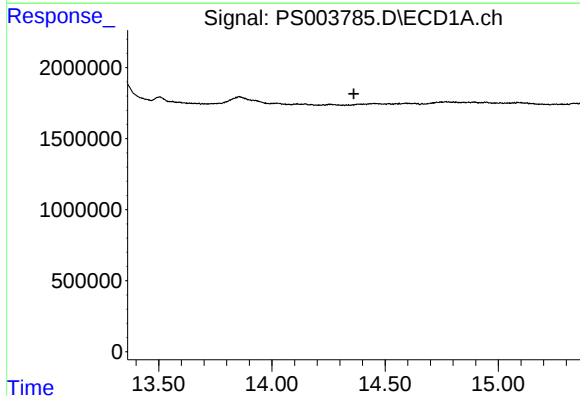


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.362 min
Response: 0
Conc: N.D.

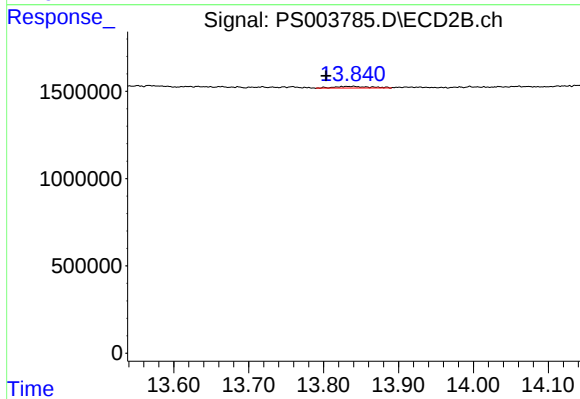

#11 2,4,5-TP (SILVEX)


R.T.: 13.839 min
Delta R.T.: 0.036 min
Response: 326373
Conc: 0.12 ng/ml

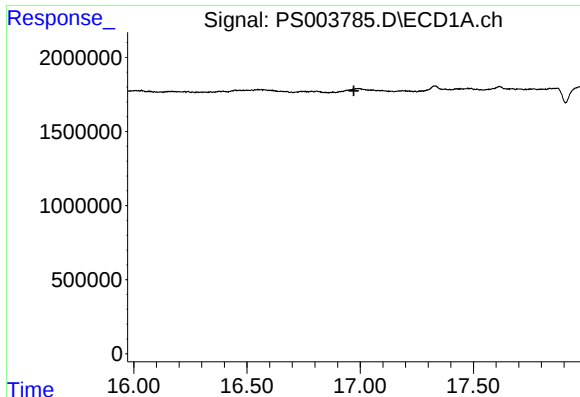

#14 DINoseb


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

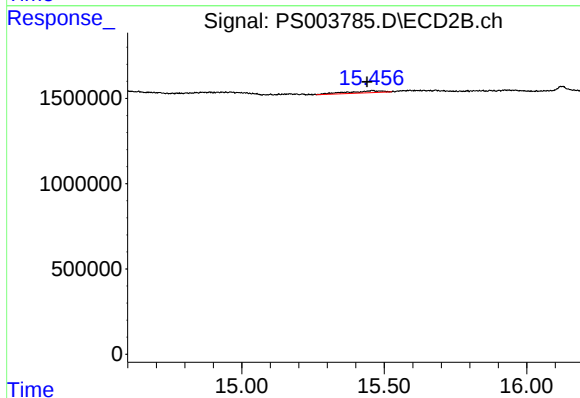


#14 DINoseb

R.T.: 15.457 min
Delta R.T.: 0.017 min
Response: 1026322
Conc: 0.53 ng/ml

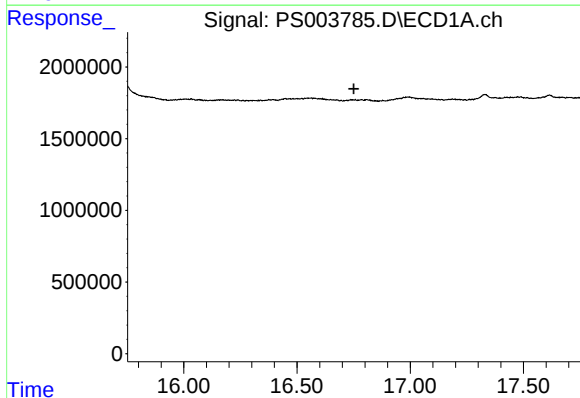


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

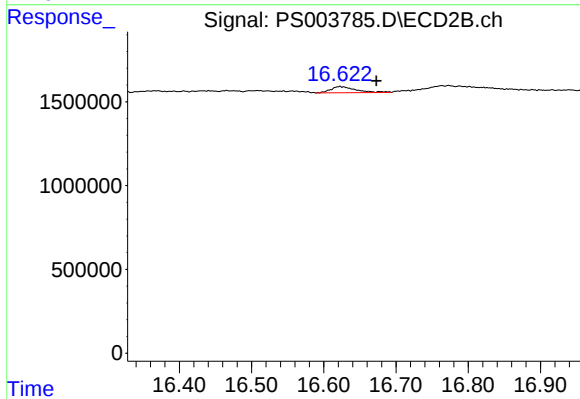

#15 Picloram


R.T.: 16.624 min
Delta R.T.: -0.049 min
Response: 898875
Conc: 0.28 ng/ml

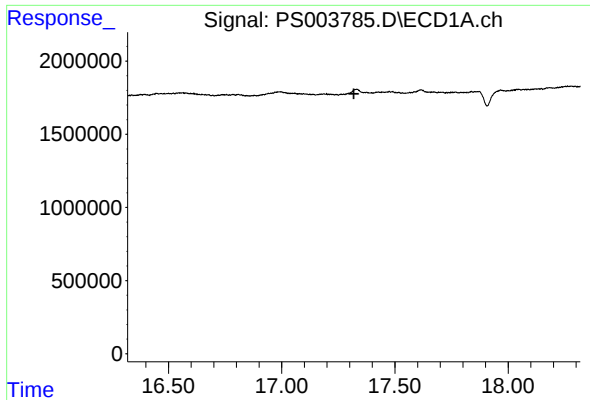

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

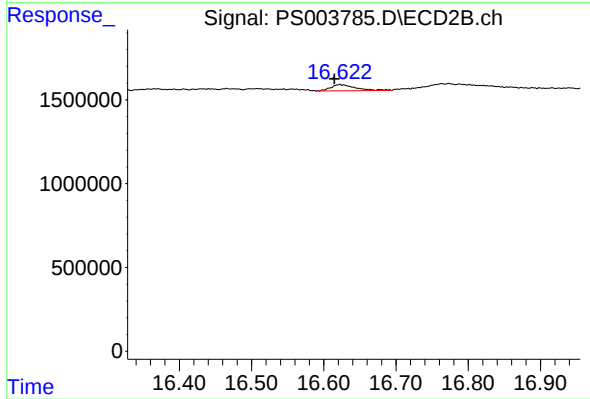

#16 DCPA

R.T.: 16.624 min
Delta R.T.: 0.009 min
Response: 898875
Conc: 0.27 ng/ml