

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032719\
 Data File : PS003802.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 00:25
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 05:03:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.272	10.772	184.4E6	180.2E6	422.714	367.160
Target Compounds							
3) T	4-Nitroph...	0.000	9.939	0	145873	N.D.	0.643 #
6) T	MCP	0.000	11.345	0	105636	N.D.	0.089 #
7) T	MCPA	0.000	11.660	0	1751113	N.D.	0.982 #
9) T	2,4-D	0.000	12.632	0	48185	N.D.	0.091 #
10) T	Pentachlo...	0.000	13.190	0	1391357	N.D.	0.201 #
11) T	2,4,5-TP ...	0.000	13.777	0	292831	N.D.	0.111 #
12) T	2,4,5-T	0.000	14.311	0	187255	N.D.	0.086 #
13) T	2,4-DB	0.000	14.991	0	903361	N.D.	3.042 #
14) T	DINOSEB	0.000	15.467	0	952286	N.D.	0.496 #
15) T	Picloram	0.000	16.621	0	381175	N.D.	0.120 #
16) T	DCPA	0.000	16.621	0	381175	N.D.	0.113 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032719\
Data File : PS003802.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 00:25
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 05:03:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

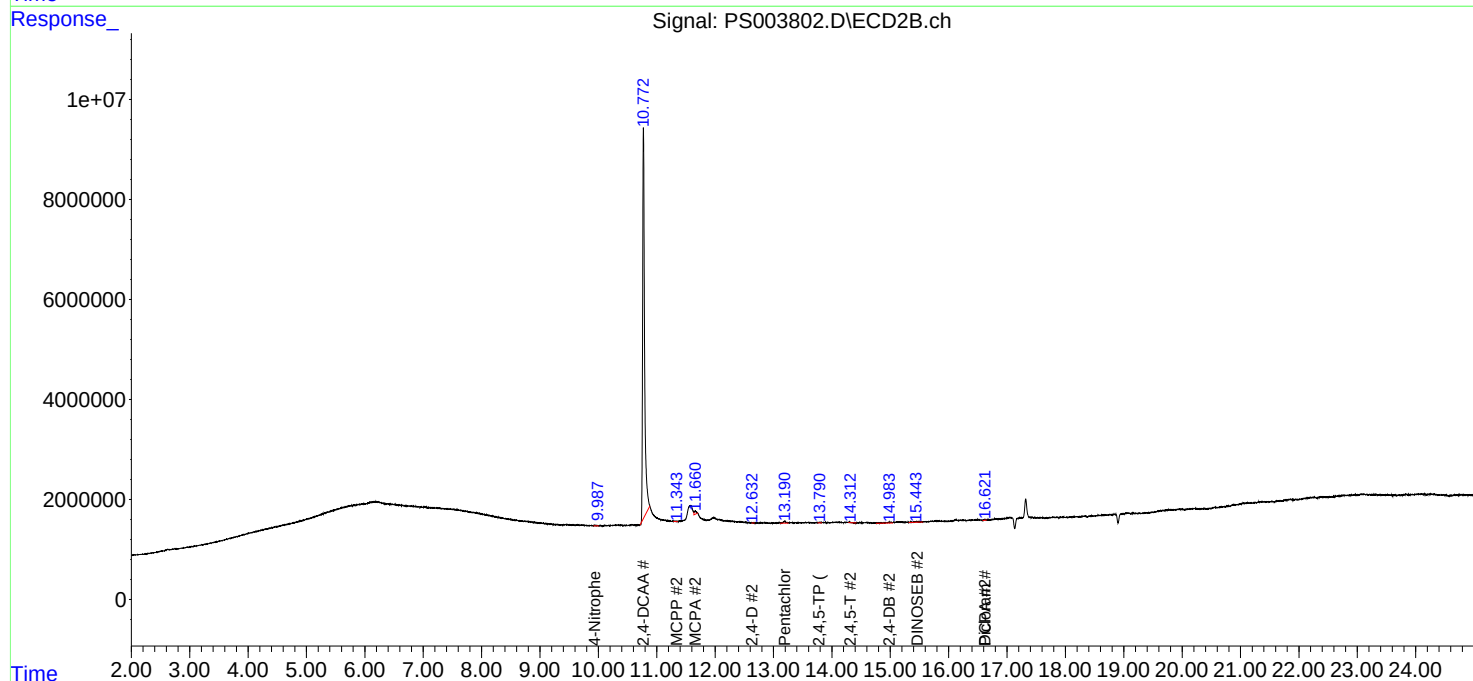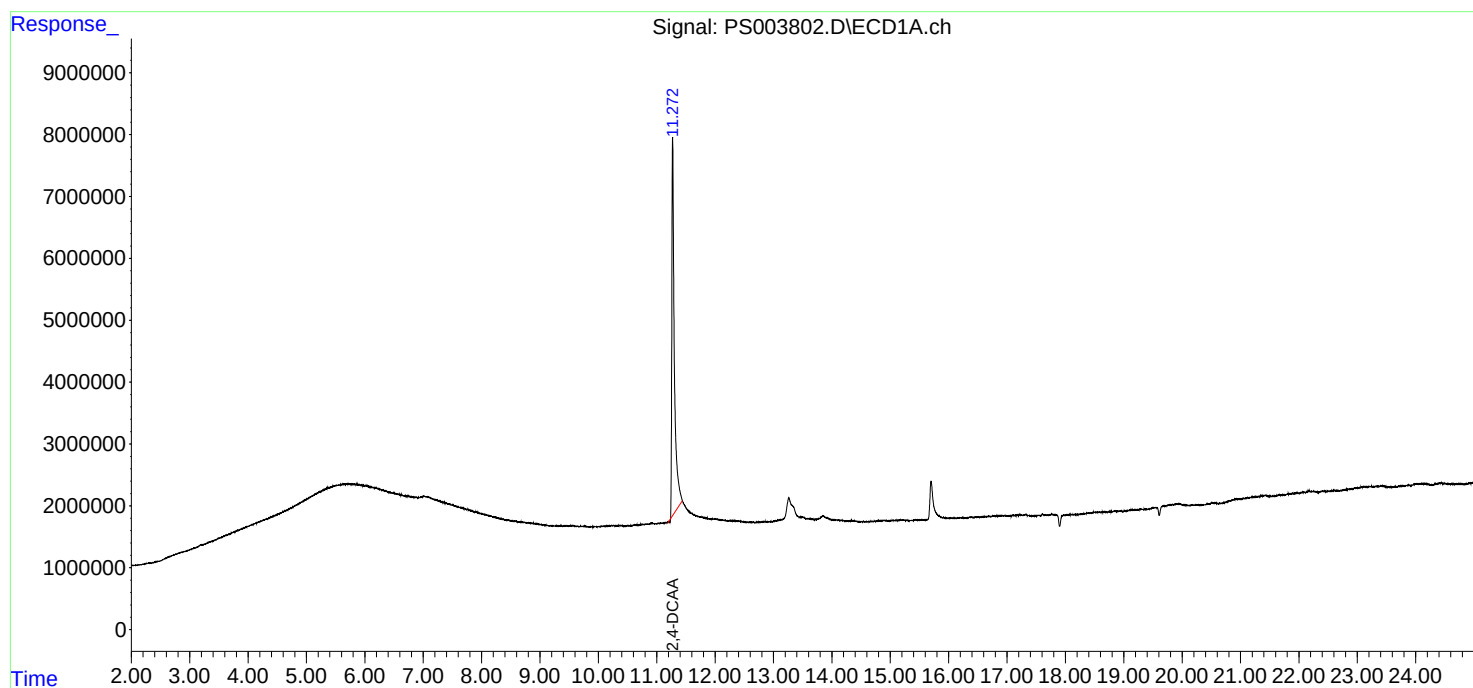


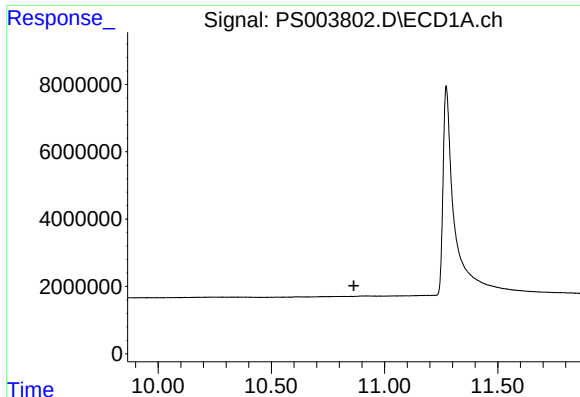

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

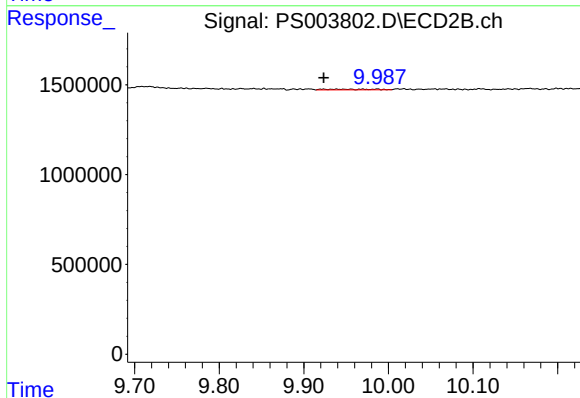


#3 4-Nitrophenol

R.T.: 9.939 min
Delta R.T.: 0.015 min
Response: 145873
Conc: 0.64 ng/ml

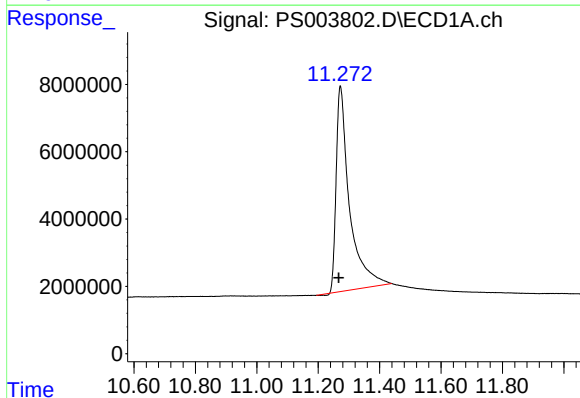


#4 2,4-DCAA

R.T.: 11.272 min
Delta R.T.: 0.006 min
Response: 184393271
Conc: 422.71 ng/ml

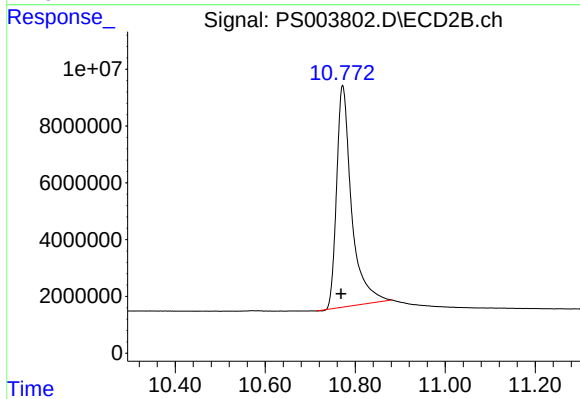

#4 2,4-DCAA


R.T.: 10.772 min
Delta R.T.: 0.004 min
Response: 180150326
Conc: 367.16 ng/ml

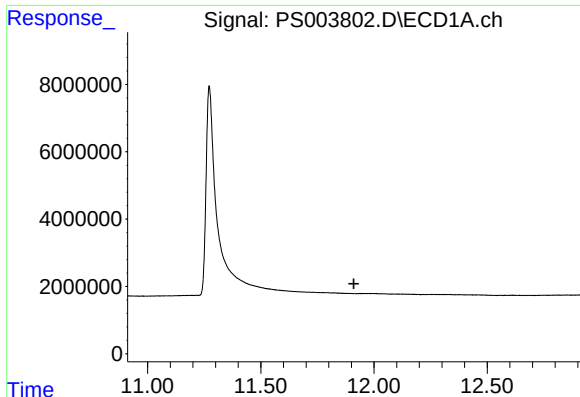

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 11.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

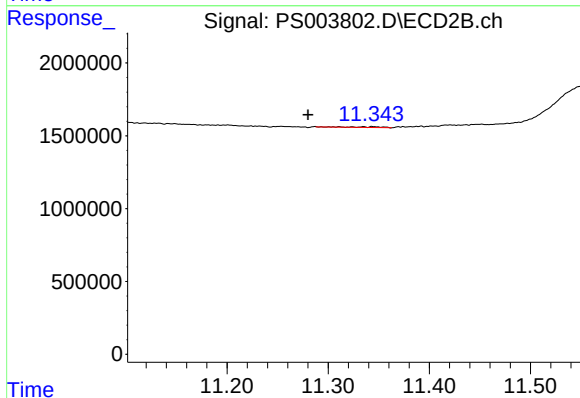


#6 MCPP

R.T.: 11.345 min
Delta R.T.: 0.065 min
Response: 105636
Conc: 0.09 ug/ml

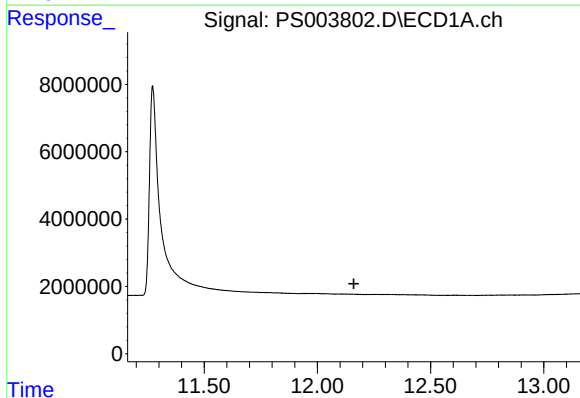


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.162 min
Response: 0
Conc: N.D.

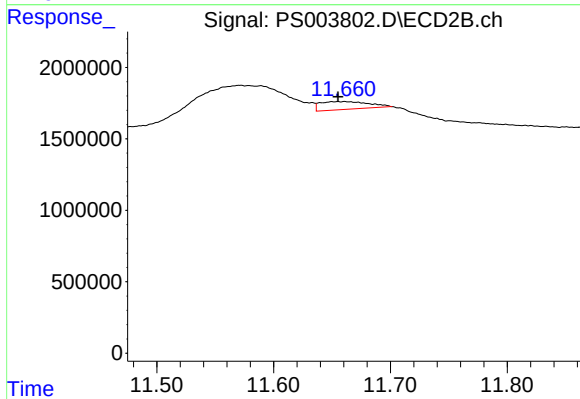

#7 MCPA


R.T.: 11.660 min
Delta R.T.: 0.005 min
Response: 1751113
Conc: 0.98 ug/ml

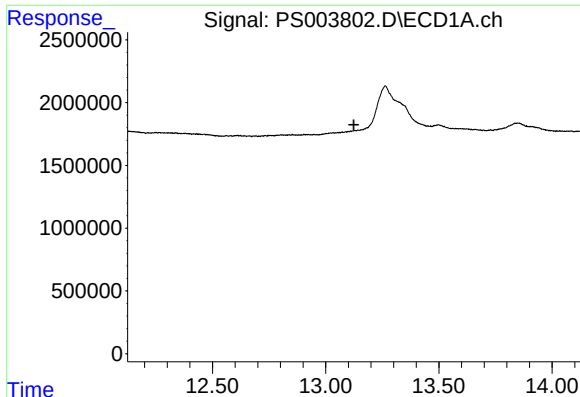

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

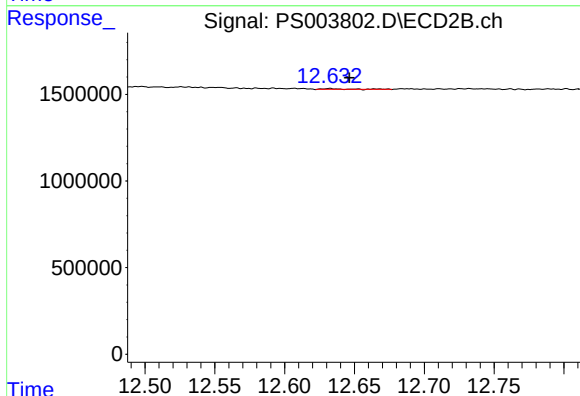


#9 2,4-D

R.T.: 12.632 min
Delta R.T.: -0.014 min
Response: 48185
Conc: 0.09 ng/ml

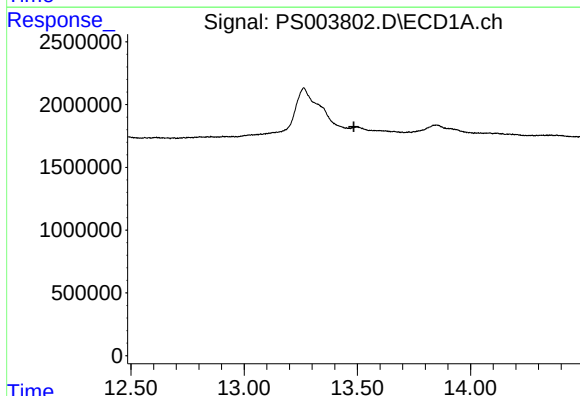


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

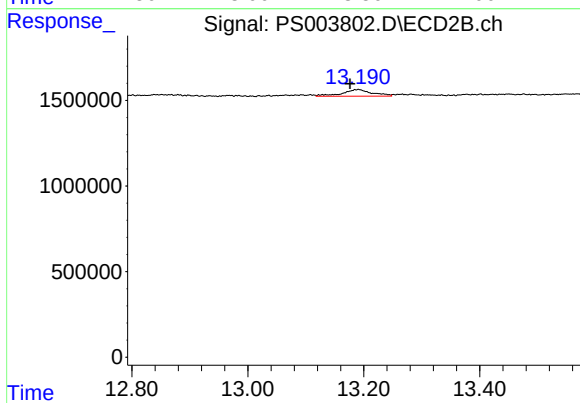

#10 Pentachlorophenol


R.T.: 13.190 min
Delta R.T.: 0.013 min
Response: 1391357
Conc: 0.20 ng/ml

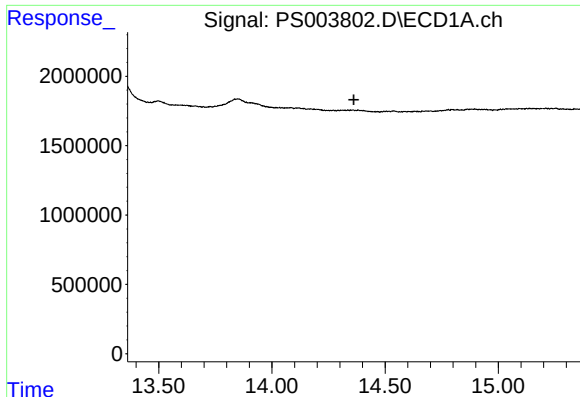

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

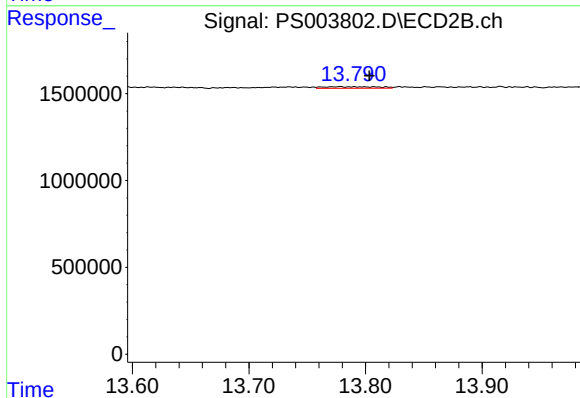


#11 2,4,5-TP (SILVEX)

R.T.: 13.777 min
Delta R.T.: -0.026 min
Response: 292831
Conc: 0.11 ng/ml

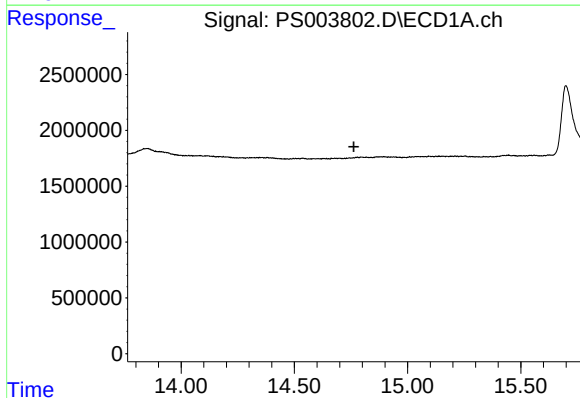


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

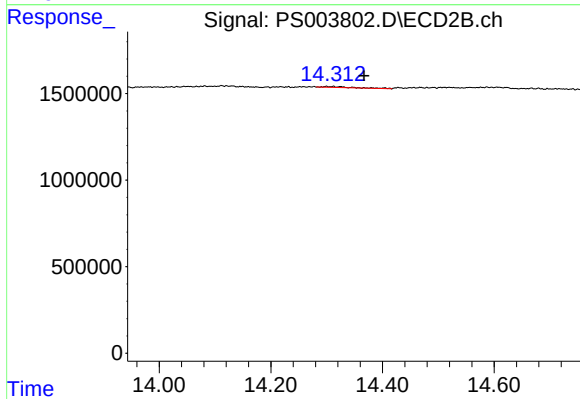

#12 2,4,5-T


R.T.: 14.311 min
Delta R.T.: -0.056 min
Response: 187255
Conc: 0.09 ng/ml

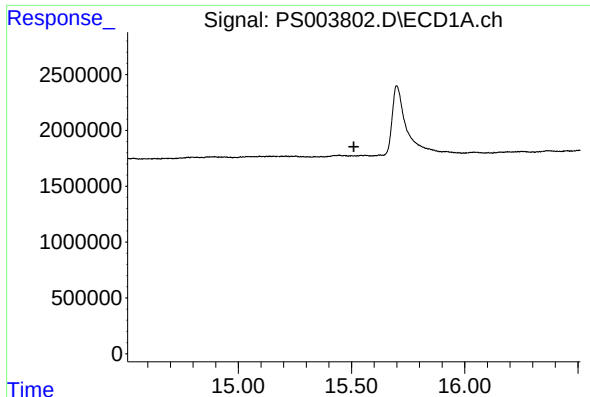

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

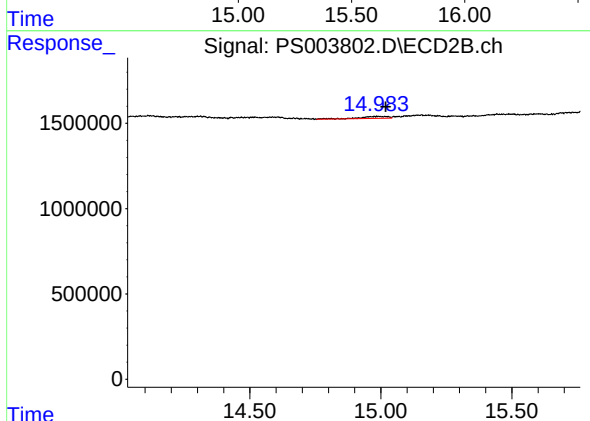


#13 2,4-DB

R.T.: 14.991 min
Delta R.T.: -0.028 min
Response: 903361
Conc: 3.04 ng/ml

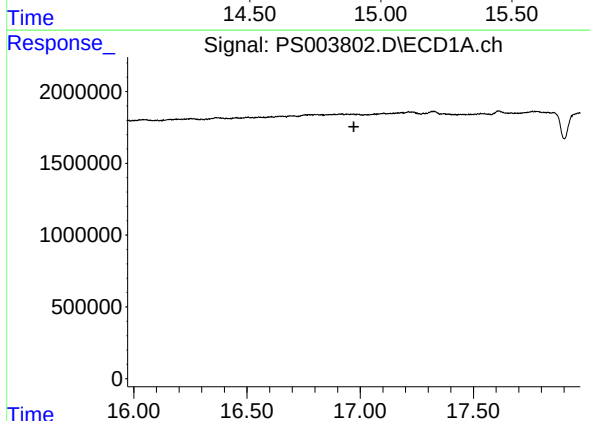


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

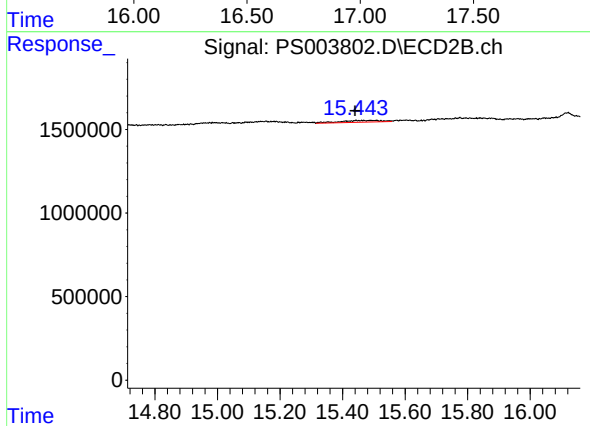

#14 DINOSEB


R.T.: 15.467 min
Delta R.T.: 0.027 min
Response: 952286
Conc: 0.50 ng/ml

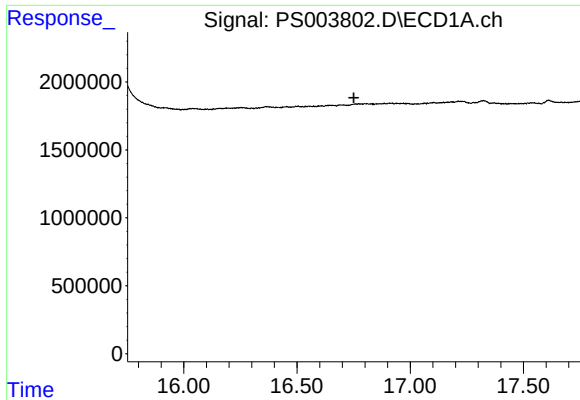

#15 Picloram


R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

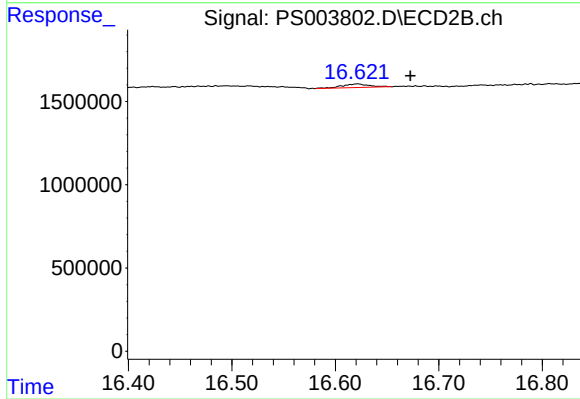


#15 Picloram

R.T.: 16.621 min
Delta R.T.: -0.052 min
Response: 381175
Conc: 0.12 ng/ml

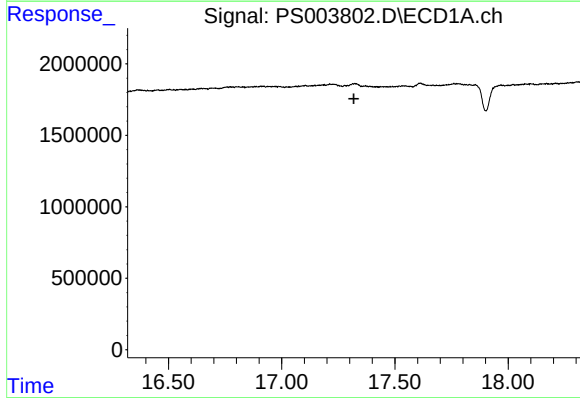

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

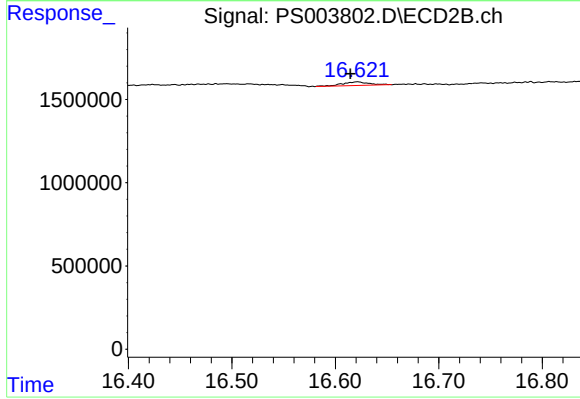

#16 DCPA

R.T.: 16.621 min
Delta R.T.: 0.006 min
Response: 381175
Conc: 0.11 ng/ml