

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032720\
 Data File : PS009463.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 14:57
 Operator : DD\AJ
 Sample : PB127835BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB127835BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 27 15:43:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.245	6.930	316.4E6	299.1E6	571.941	544.557
Target Compounds							
1) T	Dalapon	3.004	2.579	19499270	87539340	25.004	111.180 #
2) T	3,5-DICHL...	0.000	6.106	0	13793562	N.D.	16.960
6) T	MCP	7.600	0.000	6790655	0	2.760	N.D. #
7) T	MCPA	7.797	0.000	84490429	0	27.741	N.D. #
8) T	DICHLORPROP	0.000	7.749	0	26705785	N.D.	48.134
12) T	2,4,5-T	9.455	9.249	20502906	27533763	8.060	9.327
14) T	DINOSEB	11.193	10.047	14861615	12460733	7.270	5.673
15) T	Picloram	11.042	11.019	58760125	78977329	19.361	19.394
16) T	DCPA	0.000	11.019	0	78977329	N.D.	20.392



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032720\
Data File : PS009463.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 14:57
Operator : DD\AJ
Sample : PB127835BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB127835BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 27 15:43:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

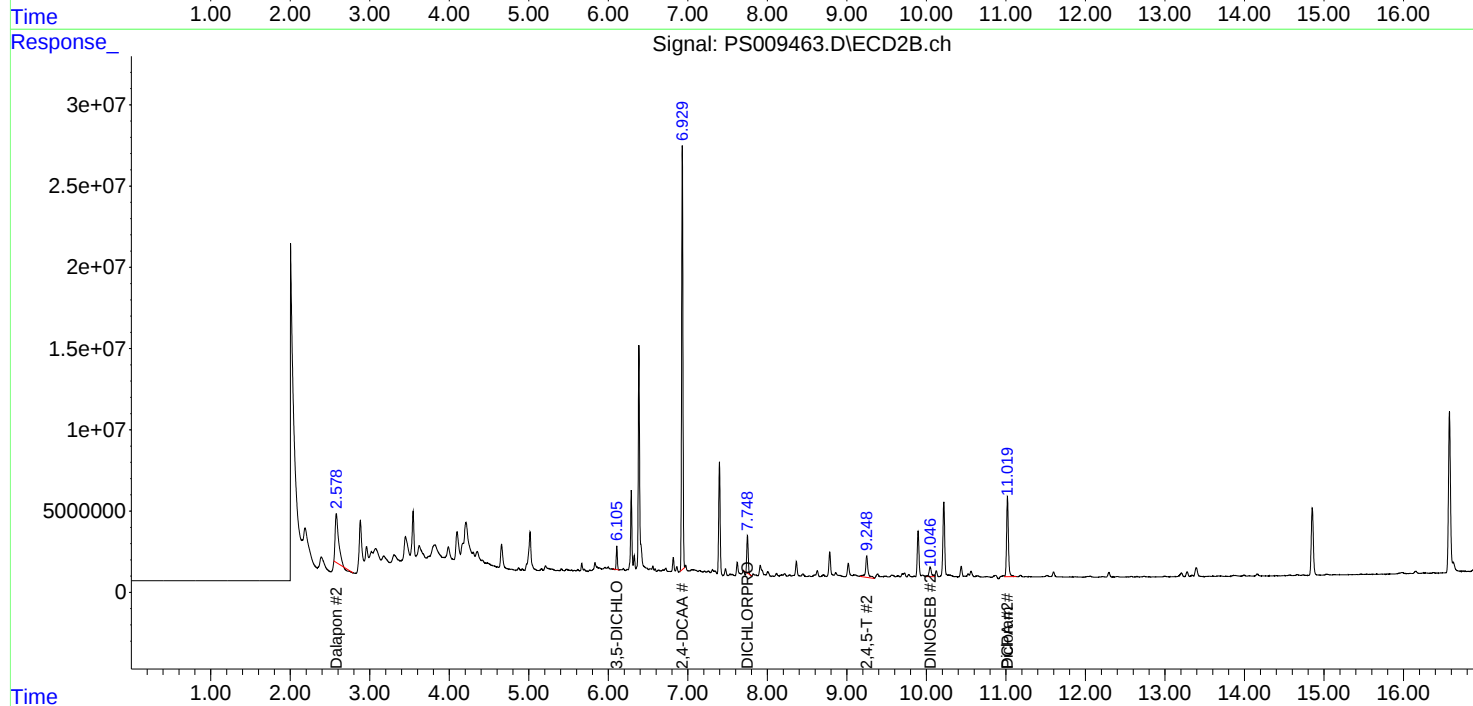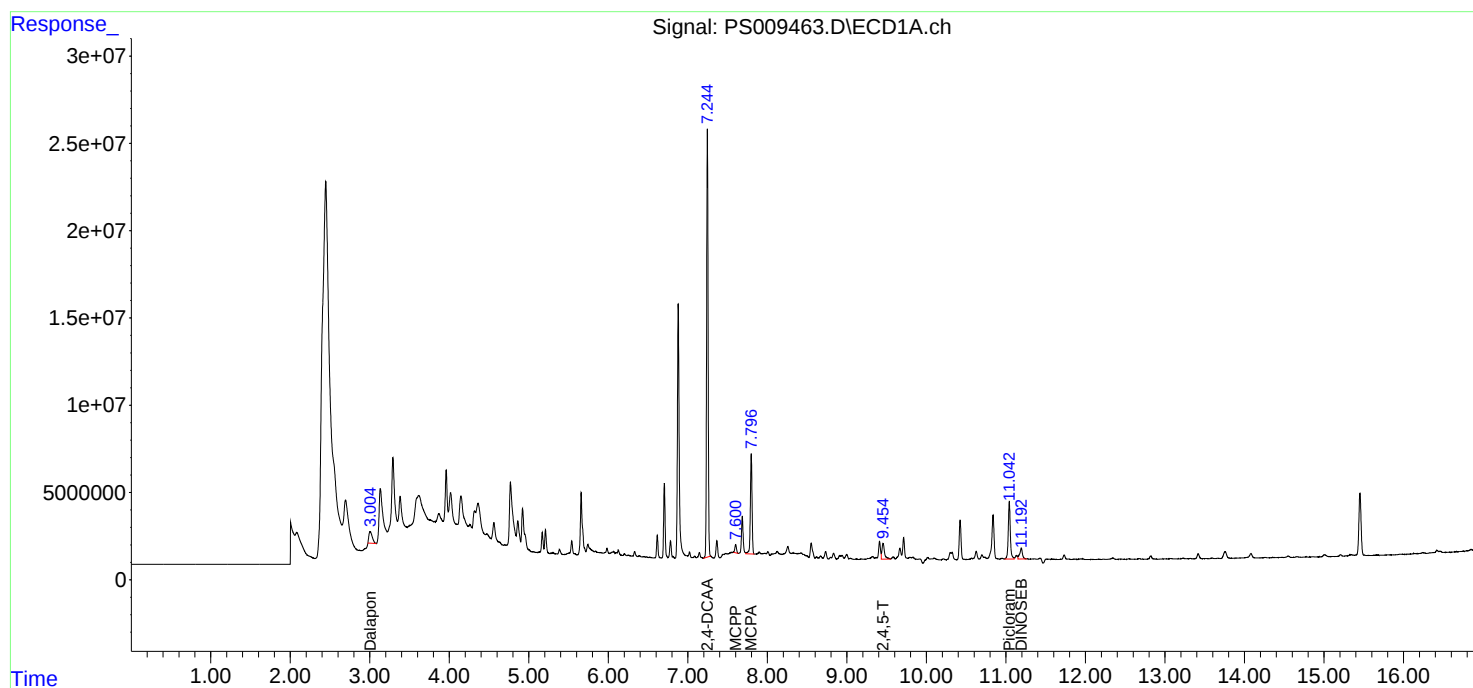


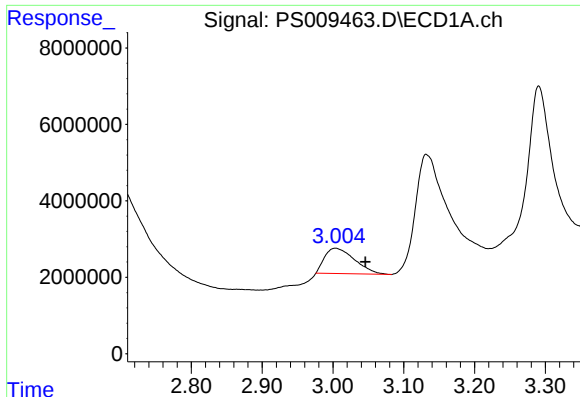

#1 Dalapon


R.T.: 3.004 min
Delta R.T.: -0.042 min
Response: 19499270
Conc: 25.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB127835BL

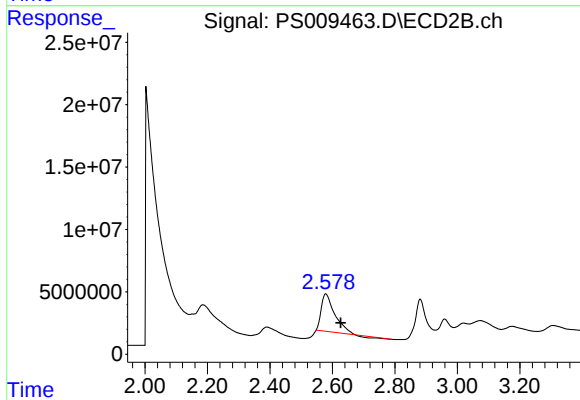


#1 Dalapon

R.T.: 2.579 min
Delta R.T.: -0.048 min
Response: 87539340
Conc: 111.18 ng/ml

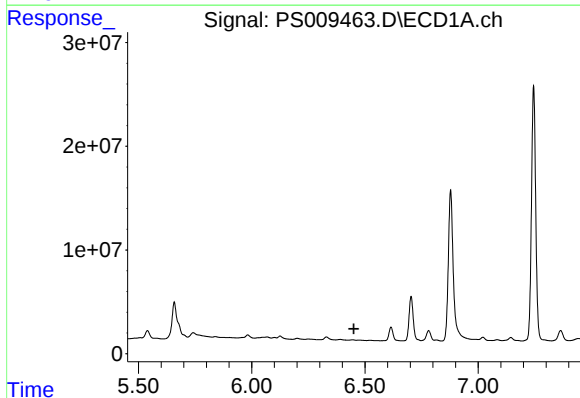


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

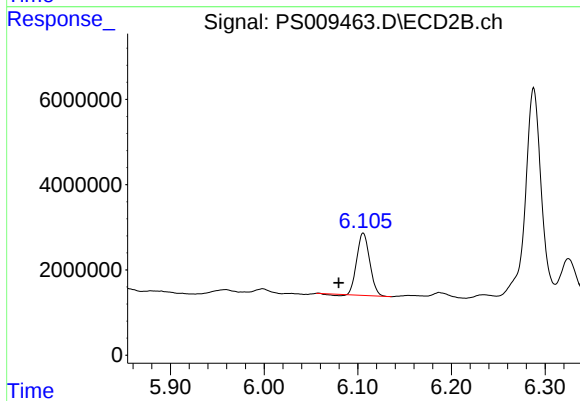

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.106 min
Delta R.T.: 0.026 min
Response: 13793562
Conc: 16.96 ng/ml

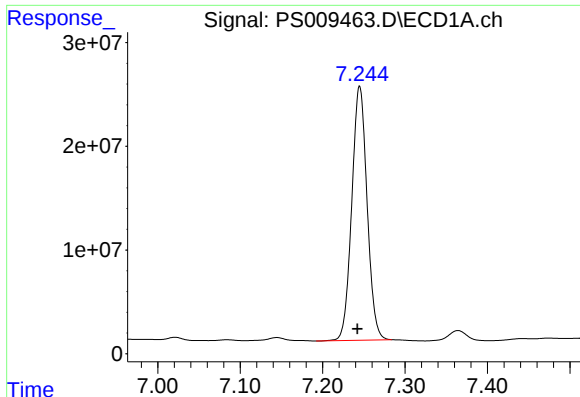

#4 2,4-DCAA


R.T.: 7.245 min
Delta R.T.: 0.003 min
Response: 316380479
Conc: 571.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB127835BL

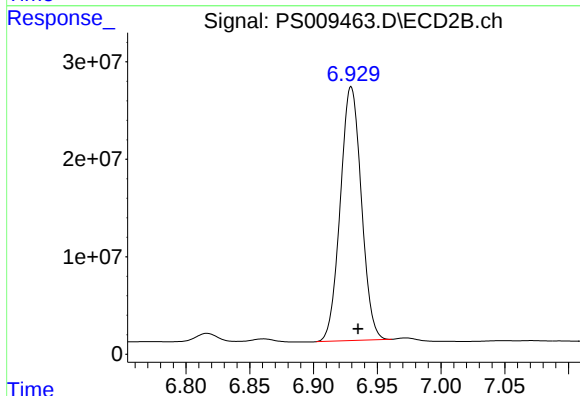


#4 2,4-DCAA

R.T.: 6.930 min
Delta R.T.: -0.005 min
Response: 299069179
Conc: 544.56 ng/ml

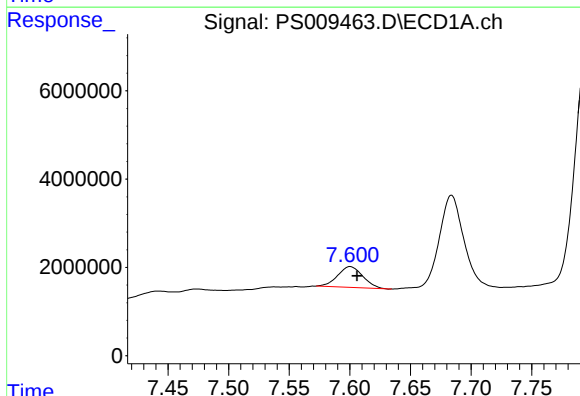


#6 MCP

R.T.: 7.600 min
Delta R.T.: -0.006 min
Response: 6790655
Conc: 2.76 ug/ml

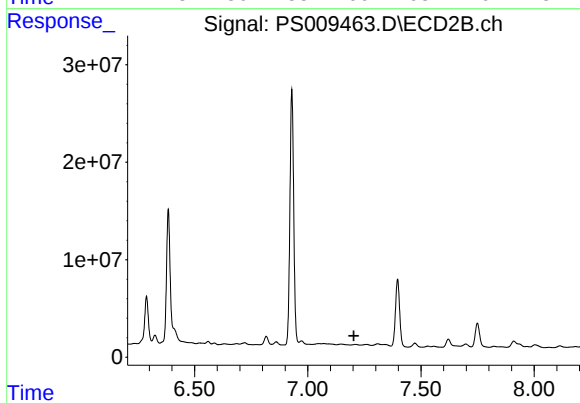

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.204 min
Response: 0
Conc: N.D.

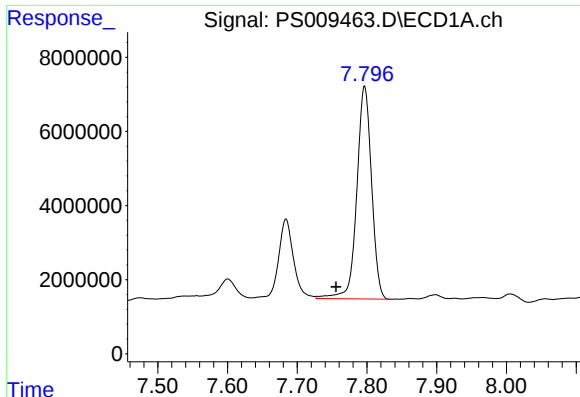

#7 MCPA


R.T.: 7.797 min
Delta R.T.: 0.041 min
Response: 84490429
Conc: 27.74 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB127835BL

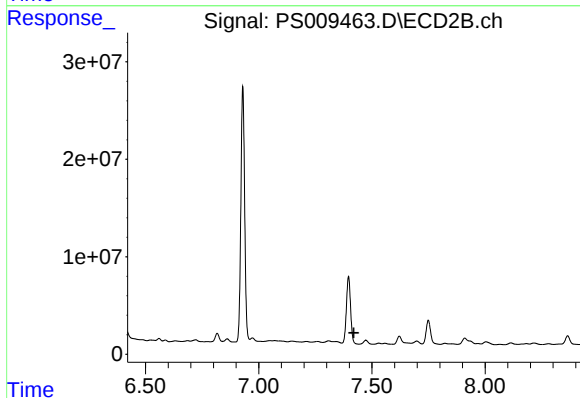


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.420 min
Response: 0
Conc: N.D.

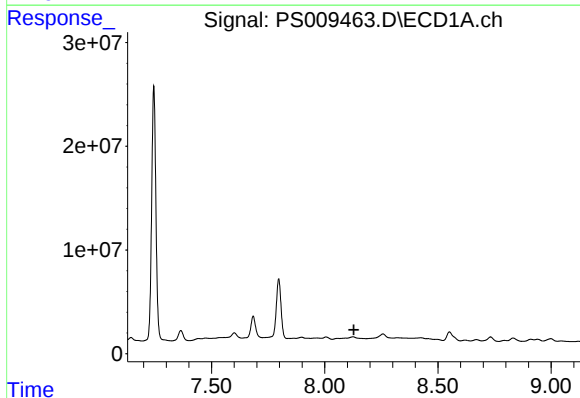


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.129 min
Response: 0
Conc: N.D.

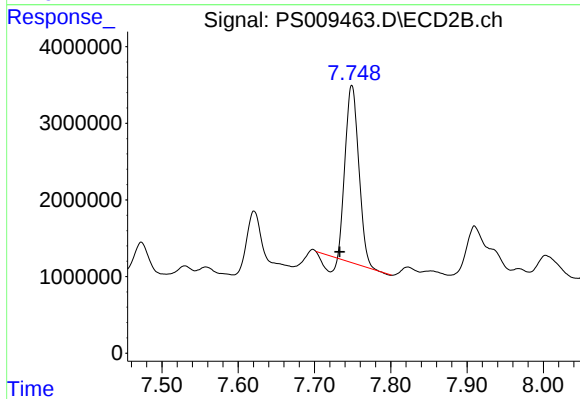

#8 DICHLORPROP


R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 26705785
Conc: 48.13 ng/ml

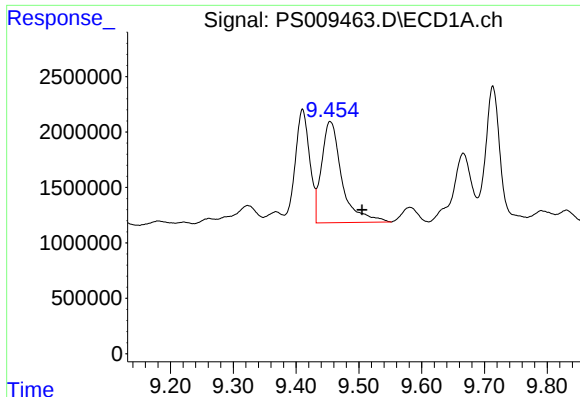

#12 2,4,5-T


R.T.: 9.455 min
Delta R.T.: -0.050 min
Response: 20502906
Conc: 8.06 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB127835BL

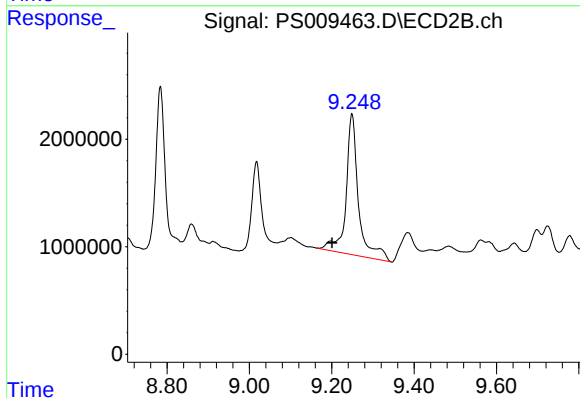


#12 2,4,5-T

R.T.: 9.249 min
Delta R.T.: 0.048 min
Response: 27533763
Conc: 9.33 ng/ml

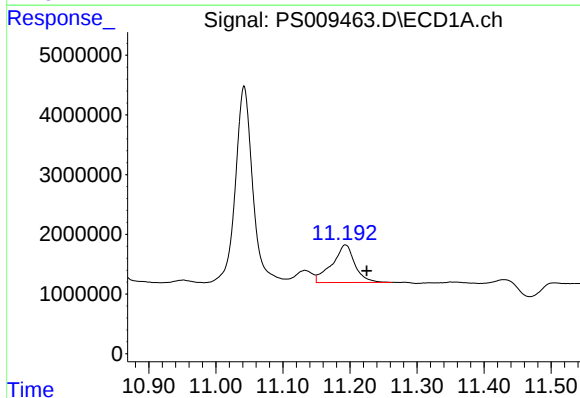


#14 DINOSEB

R.T.: 11.193 min
Delta R.T.: -0.032 min
Response: 14861615
Conc: 7.27 ng/ml

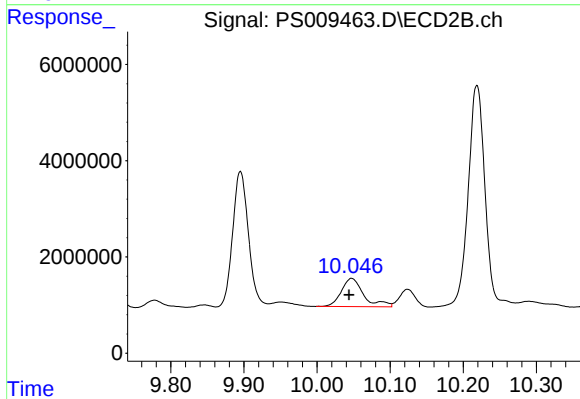

#14 DINOSEB


R.T.: 10.047 min
Delta R.T.: 0.004 min
Response: 12460733
Conc: 5.67 ng/ml

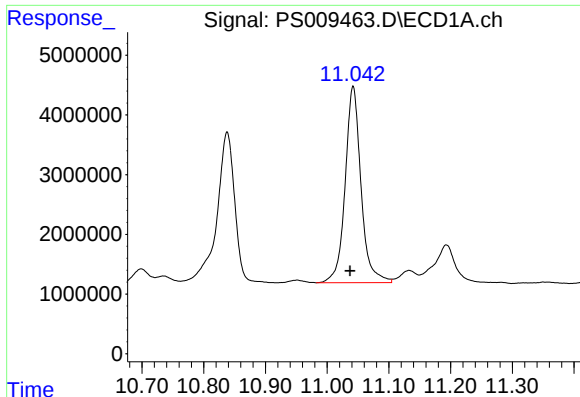

#15 Picloram


R.T.: 11.042 min
Delta R.T.: 0.005 min
Response: 58760125
Conc: 19.36 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB127835BL

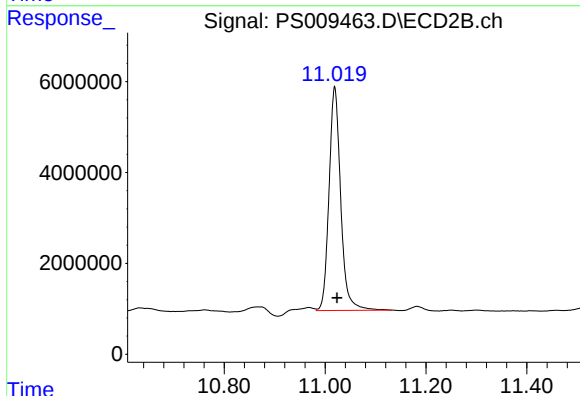


#15 Picloram

R.T.: 11.019 min
Delta R.T.: -0.004 min
Response: 78977329
Conc: 19.39 ng/ml

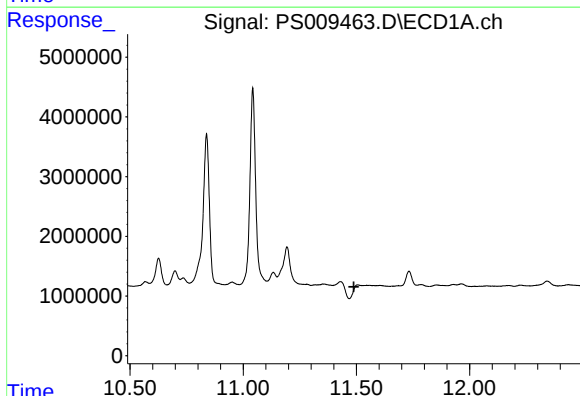

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

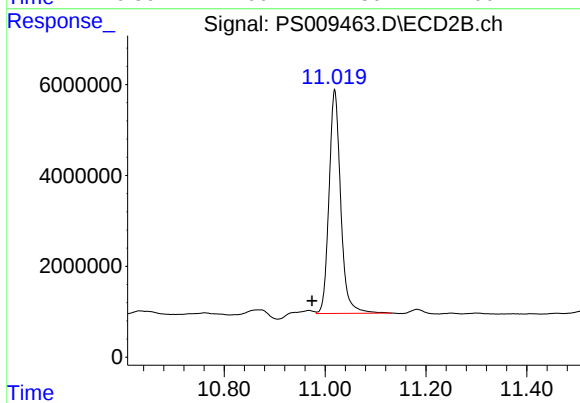

#16 DCPA

R.T.: 11.019 min
Delta R.T.: 0.045 min
Response: 78977329
Conc: 20.39 ng/ml