

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032720\
 Data File : PS009472.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 18:23
 Operator : DD\AJ
 Sample : L2033-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SLUDGE-PIT

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 05:45:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.931	193.1E6	183.5E6	349.096	334.125
Target Compounds							
1) T	Dalapon	3.005	2.587	22018698	79565716	28.235	101.053 #
2) T	3,5-DICHL...	0.000	6.108	0	76608293	N.D.	94.194
5) T	DICAMBA	0.000	7.047	0	12144790	N.D.	5.290
7) T	MCPA	0.000	7.474	0	17754153	N.D.	6.579
8) T	DICHLORPROP	0.000	7.750	0	43570293	N.D.	78.530
9) T	2,4-D	8.425	0.000	4135682	0	7.844	N.D. #
10) T	Pentachlo...	0.000	8.453	0	6010875	N.D.	<MDL
12) T	2,4,5-T	9.443	9.262	55011436	6322167	21.625	2.142 #
13) T	2,4-DB	0.000	9.698	0	4894533	N.D.	12.893
14) T	DINOSEB	0.000	10.054	0	5326256	N.D.	2.425
15) T	Picloram	0.000	11.049	0	5948056	N.D.	1.461



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032720\
Data File : PS009472.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 18:23
Operator : DD\AJ
Sample : L2033-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 05:45:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

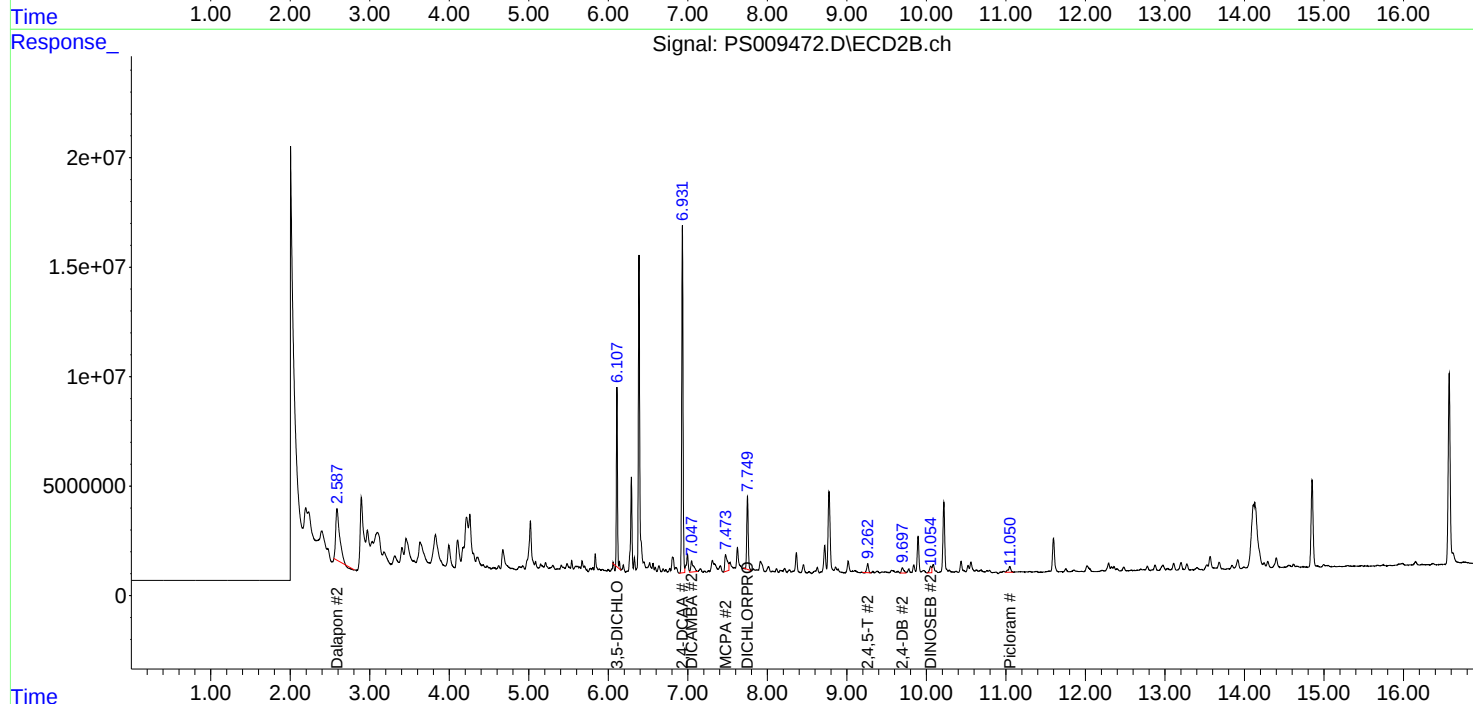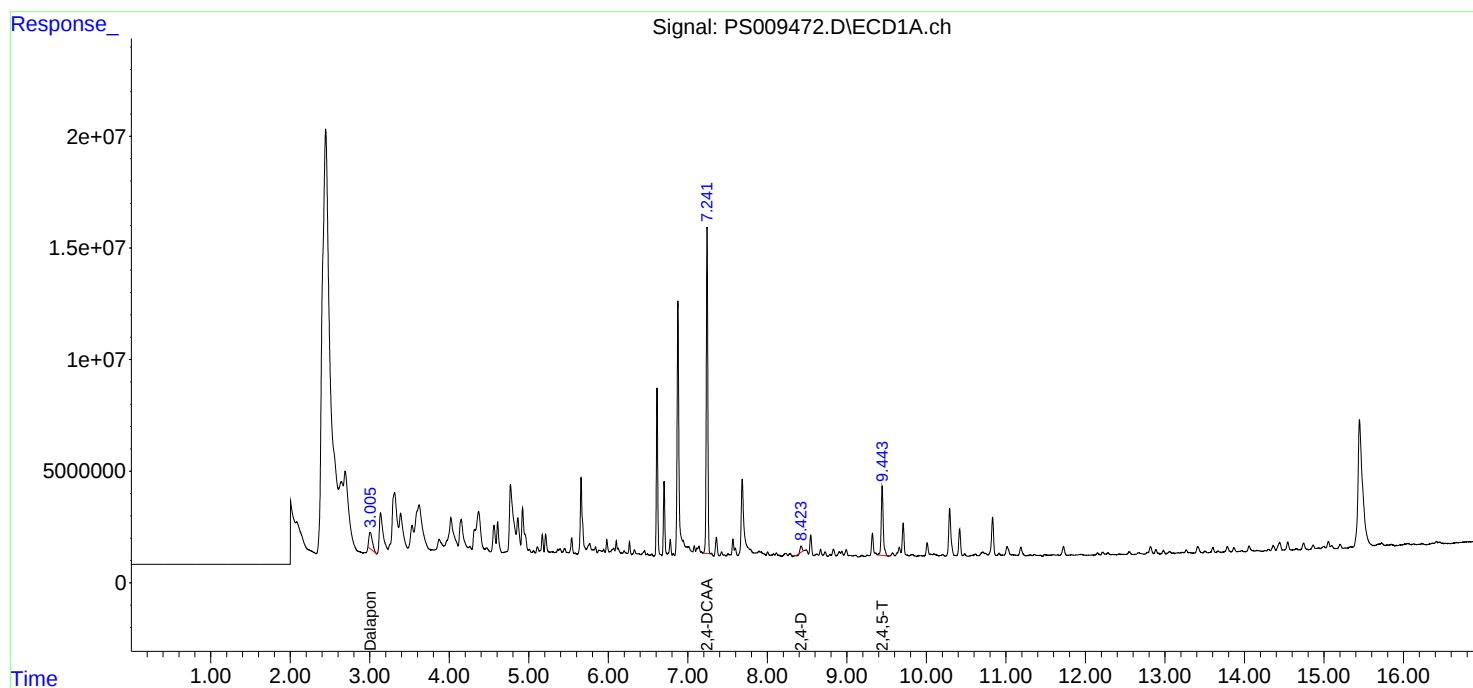


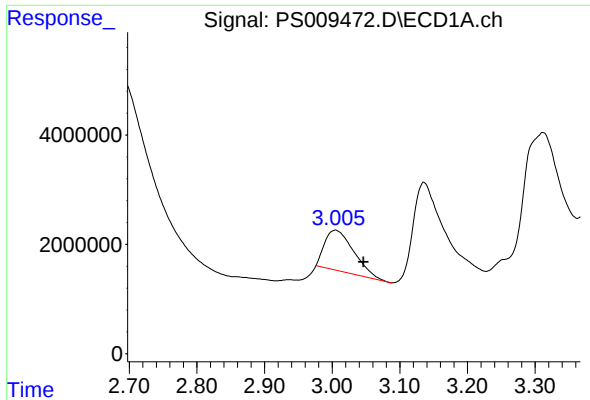

#1 Dalapon


R.T.: 3.005 min
Delta R.T.: -0.041 min
Response: 22018698
Conc: 28.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

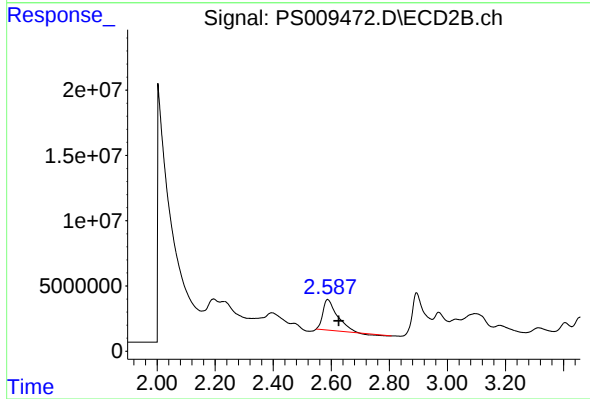


#1 Dalapon

R.T.: 2.587 min
Delta R.T.: -0.039 min
Response: 79565716
Conc: 101.05 ng/ml

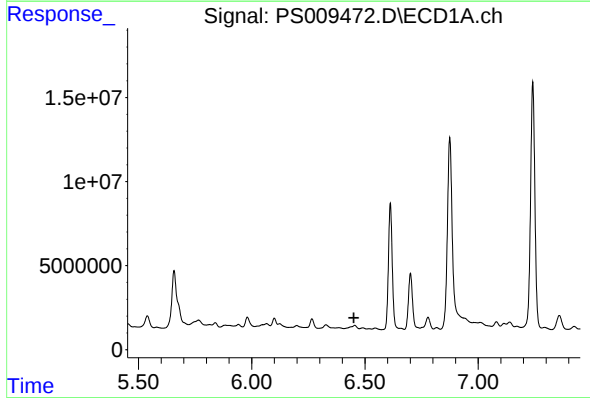


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

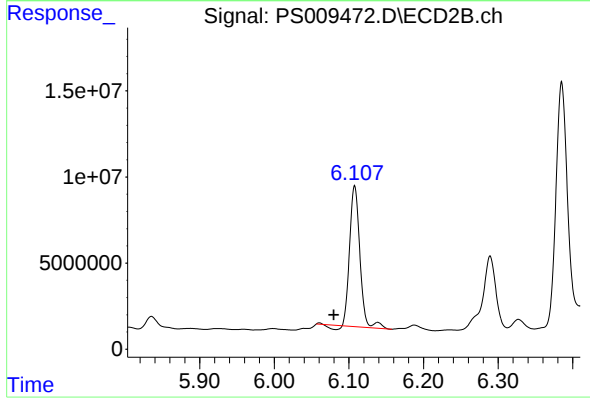

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.108 min
Delta R.T.: 0.028 min
Response: 76608293
Conc: 94.19 ng/ml

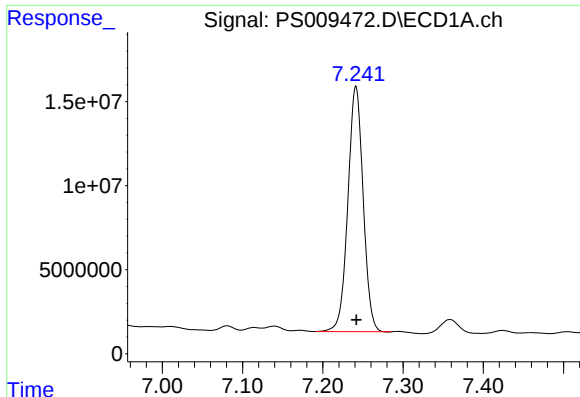

#4 2,4-DCAA


R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 193109238
Conc: 349.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

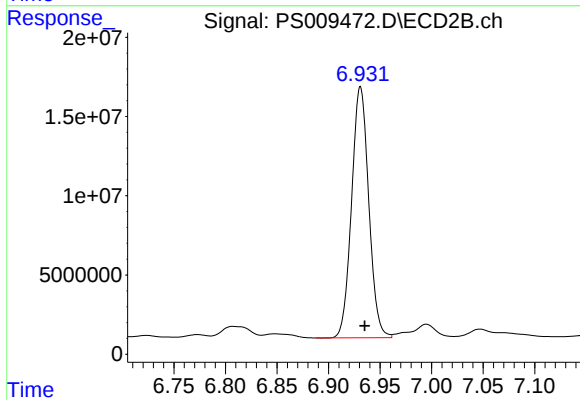


#4 2,4-DCAA

R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 183500691
Conc: 334.13 ng/ml

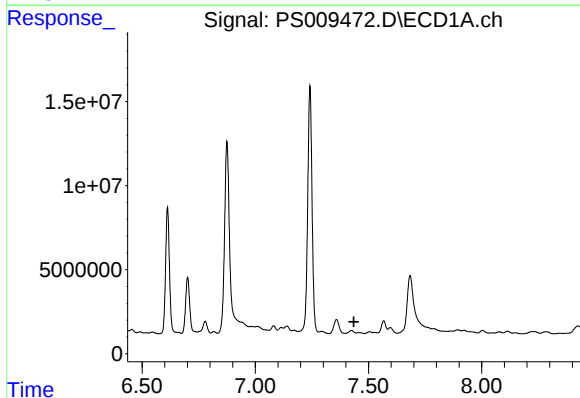


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.435 min
Response: 0
Conc: N.D.

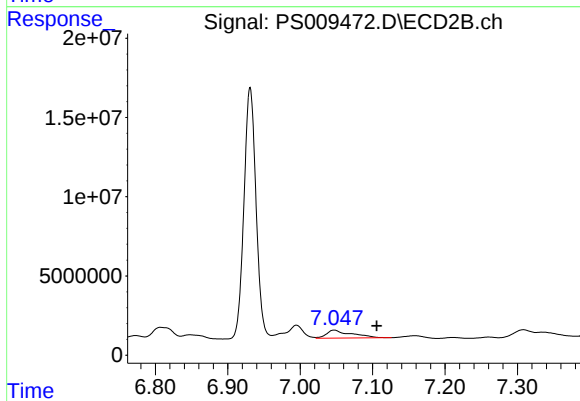

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.059 min
Response: 12144790
Conc: 5.29 ng/ml

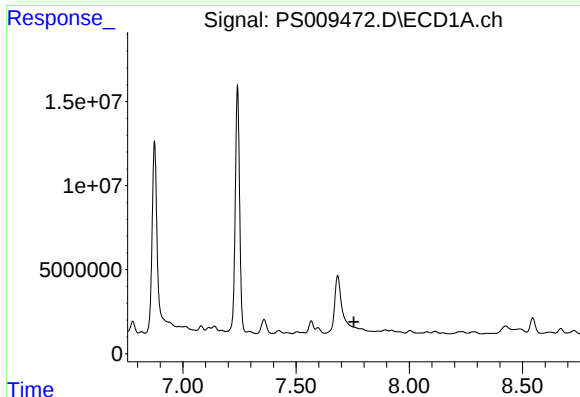

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

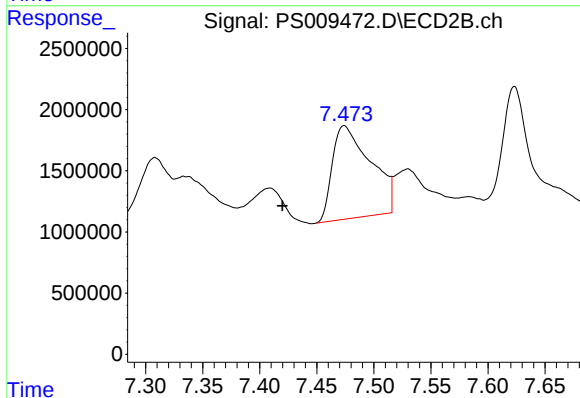


#7 MCPA

R.T.: 7.474 min
Delta R.T.: 0.054 min
Response: 17754153
Conc: 6.58 ug/ml

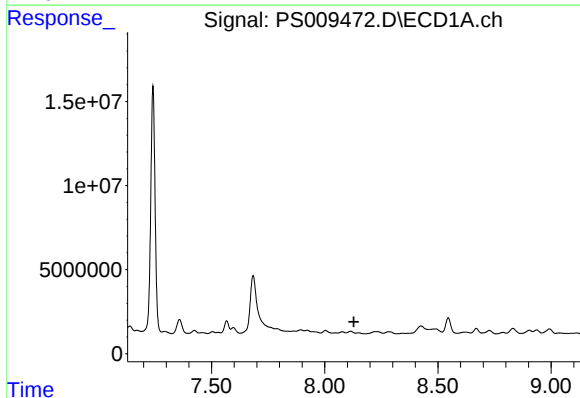


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

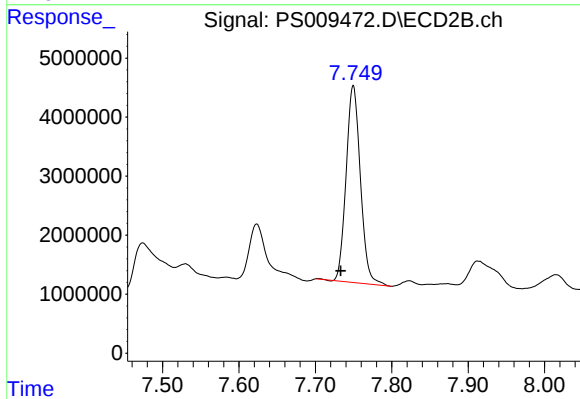

#8 DICHLORPROP


R.T.: 7.750 min
Delta R.T.: 0.017 min
Response: 43570293
Conc: 78.53 ng/ml

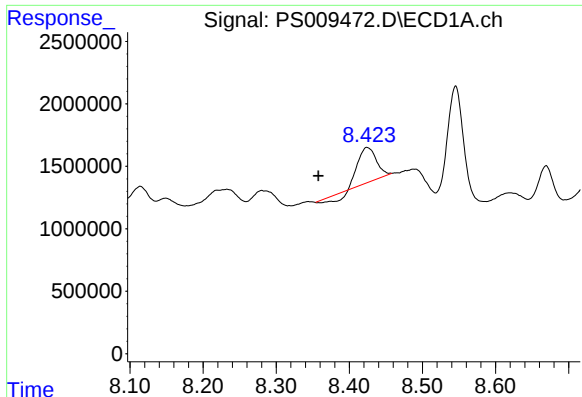

#9 2,4-D


R.T.: 8.425 min
Delta R.T.: 0.067 min
Response: 4135682
Conc: 7.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

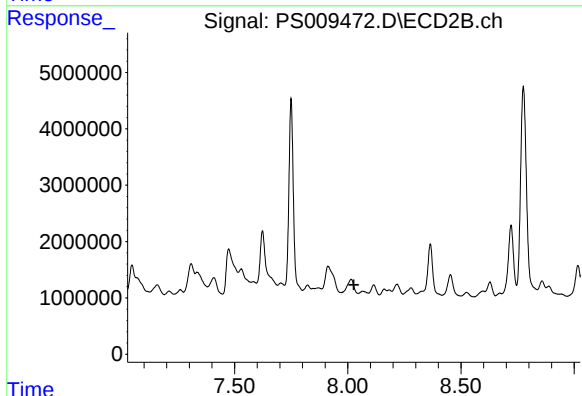


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.027 min
Response: 0
Conc: N.D.

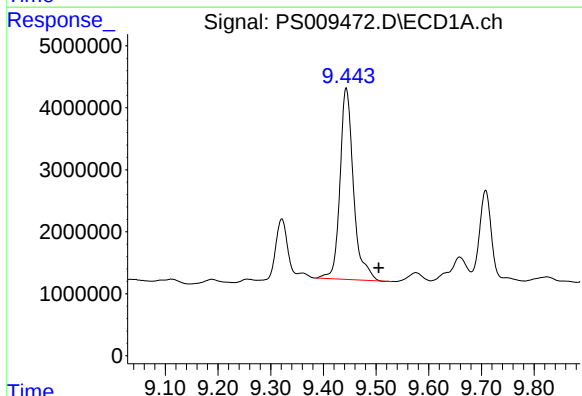


#12 2,4,5-T

R.T.: 9.443 min
Delta R.T.: -0.062 min
Response: 55011436
Conc: 21.63 ng/ml

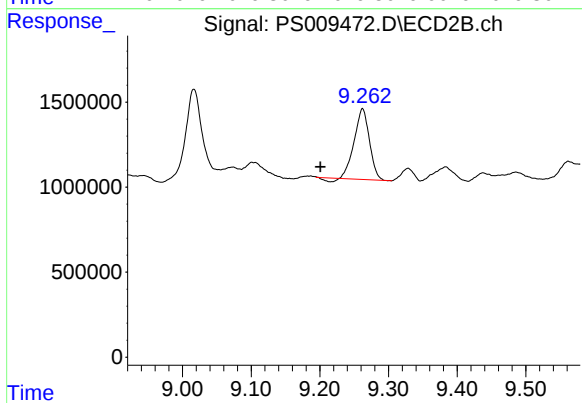

#12 2,4,5-T


R.T.: 9.262 min
Delta R.T.: 0.061 min
Response: 6322167
Conc: 2.14 ng/ml

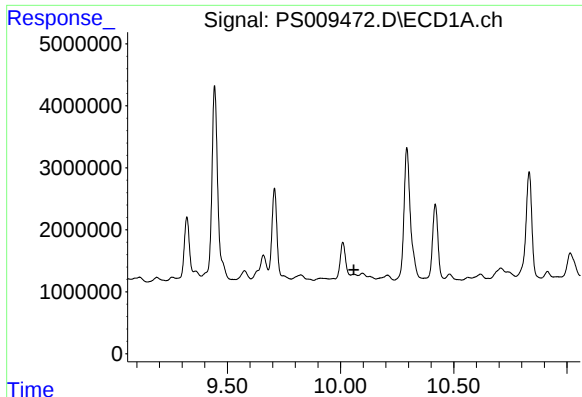

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

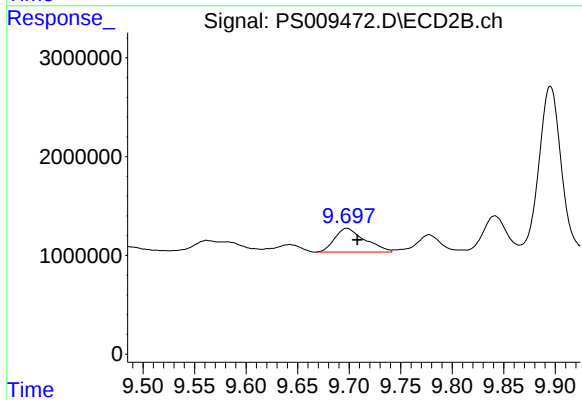


#13 2,4-DB

R.T.: 9.698 min
Delta R.T.: -0.010 min
Response: 4894533
Conc: 12.89 ng/ml

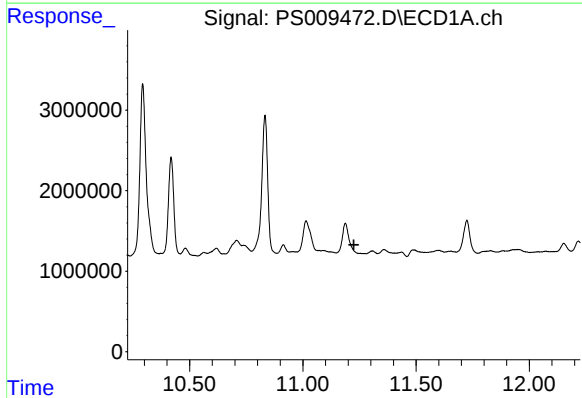


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.225 min
Response: 0
Conc: N.D.

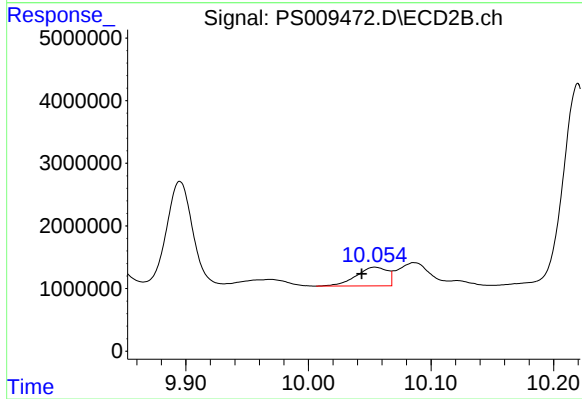

#14 DINOSEB


R.T.: 10.054 min
Delta R.T.: 0.011 min
Response: 5326256
Conc: 2.42 ng/ml

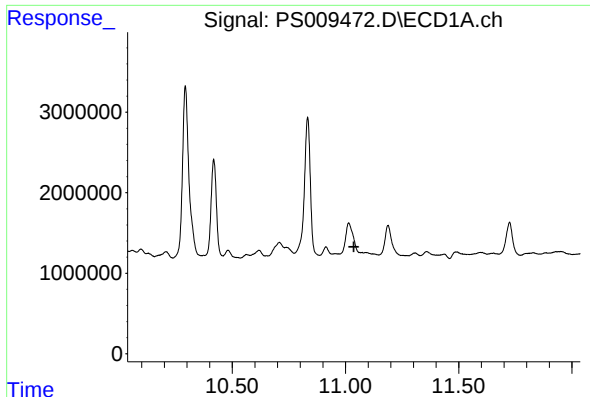

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SLUDGE-PIT

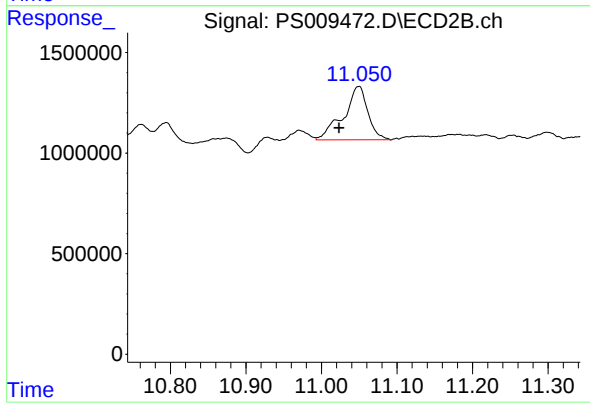

#15 Picloram

R.T.: 11.049 min
Delta R.T.: 0.026 min
Response: 5948056
Conc: 1.46 ng/ml