

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032720\
 Data File : PS009476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 19:55
 Operator : DD\AJ
 Sample : L2033-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 BUS-WASH

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 05:47:11 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.241	6.931	205.7E6	196.8E6	371.836	358.352
Target Compounds							
1) T	Dalapon	3.004	2.586	21607821	75105254	27.708	95.388 #
2) T	3,5-DICHL...	0.000	6.108	0	71145202	N.D.	87.476
5) T	DICAMBA	0.000	7.048	0	4777338	N.D.	2.081
7) T	MCPA	0.000	7.476	0	13467312	N.D.	4.990
8) T	DICHLORPROP	0.000	7.750	0	53125916	N.D.	95.753
9) T	2,4-D	8.427	0.000	11866047	0	22.507	N.D. #
10) T	Pentachlo...	0.000	8.452	0	4372271	N.D.	<MDL
12) T	2,4,5-T	9.444	9.262	47762935	7894561	18.776	2.674 #
13) T	2,4-DB	0.000	9.698	0	4782182	N.D.	12.597
14) T	DINOSEB	0.000	10.054	0	4971939	N.D.	2.264
15) T	Picloram	0.000	11.019	0	5387947	N.D.	1.323
16) T	DCPA	0.000	11.019	0	5387947	N.D.	1.391



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032720\
Data File : PS009476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 19:55
Operator : DD\AJ
Sample : L2033-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
BUS-WASH

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 05:47:11 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

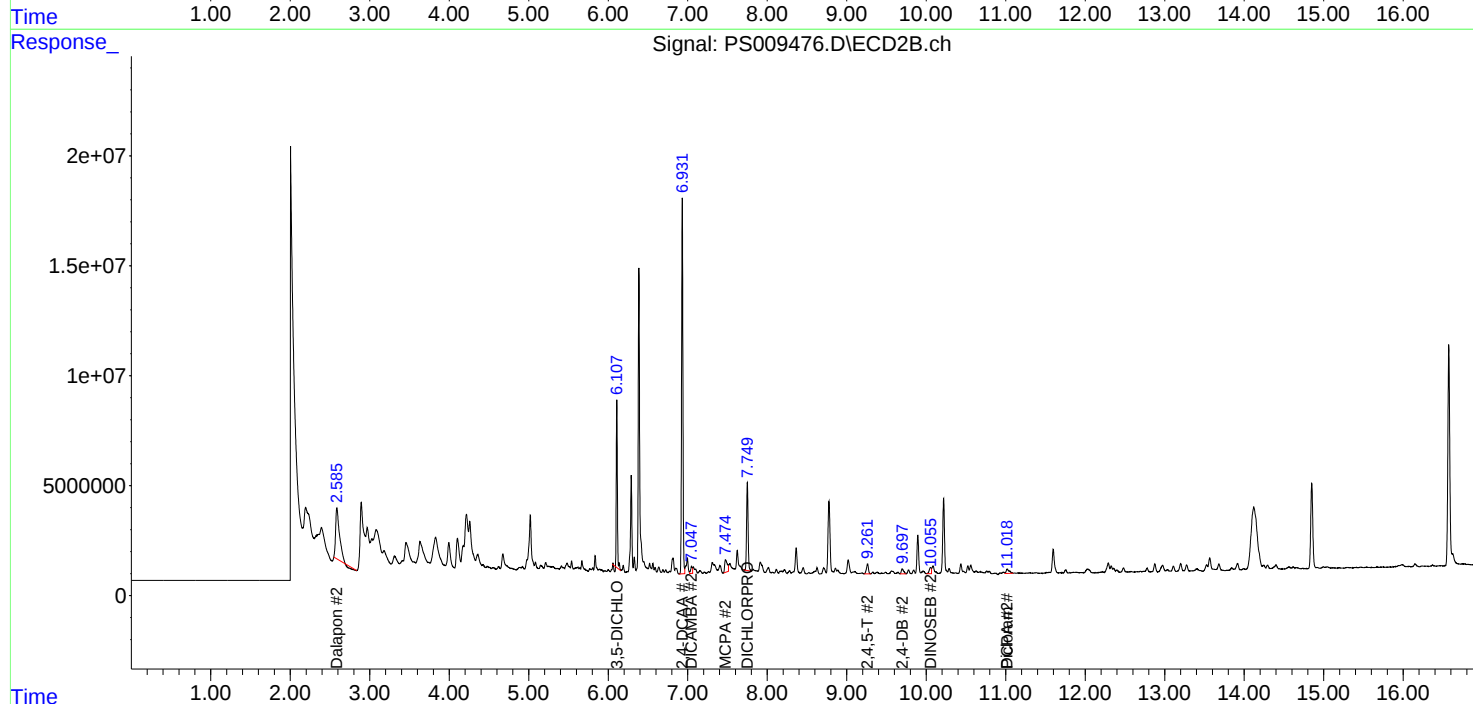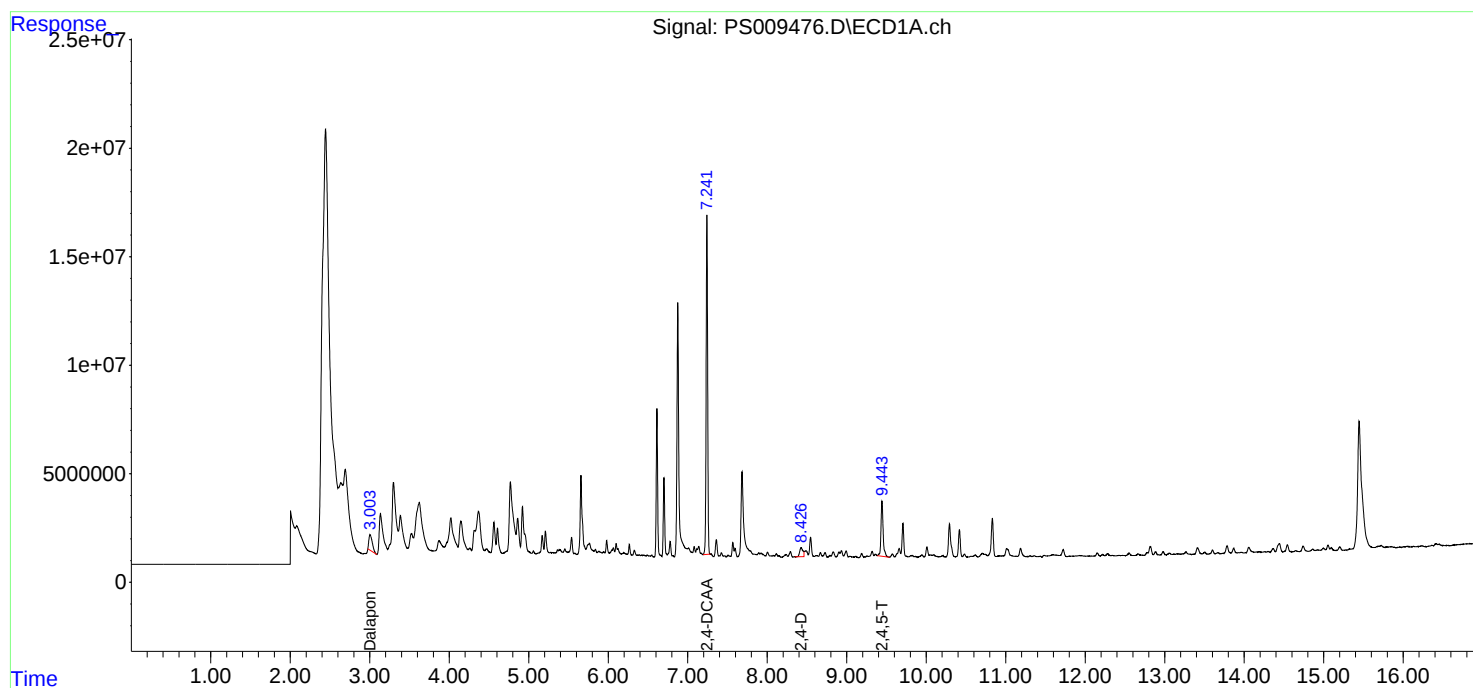


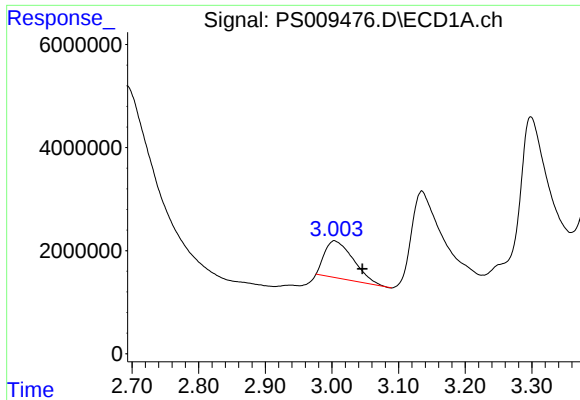

#1 Dalapon


R.T.: 3.004 min
Delta R.T.: -0.042 min
Response: 21607821
Conc: 27.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

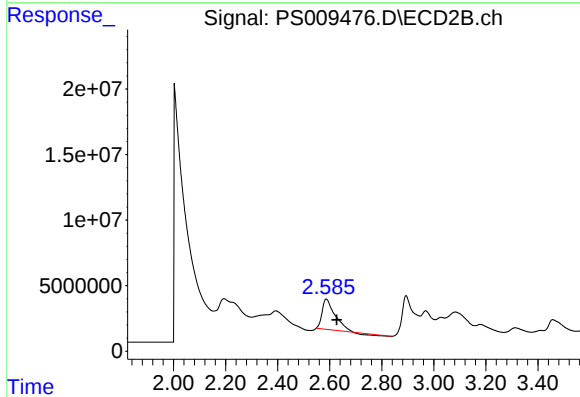


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.040 min
Response: 75105254
Conc: 95.39 ng/ml

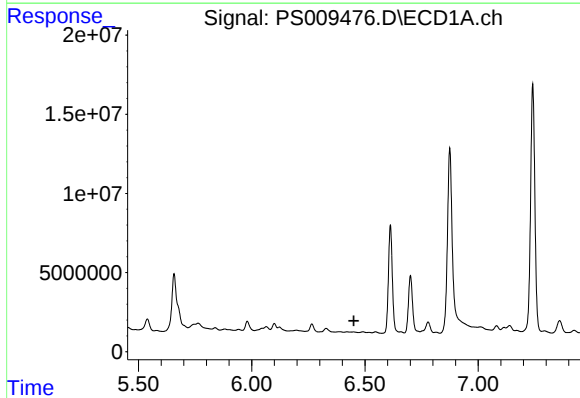


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

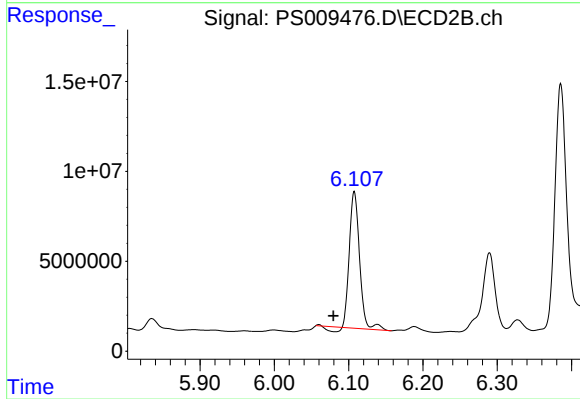

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.108 min
Delta R.T.: 0.028 min
Response: 71145202
Conc: 87.48 ng/ml

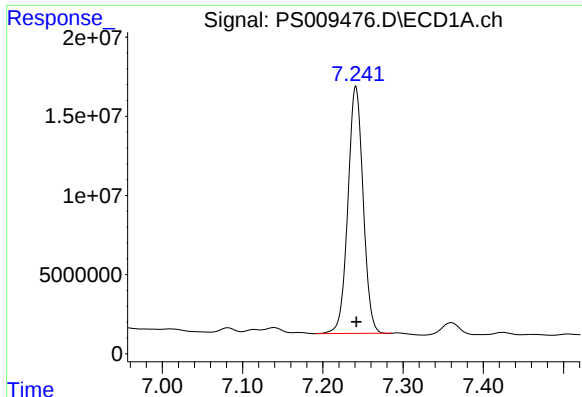

#4 2,4-DCAA


R.T.: 7.241 min
Delta R.T.: 0.000 min
Response: 205688710
Conc: 371.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

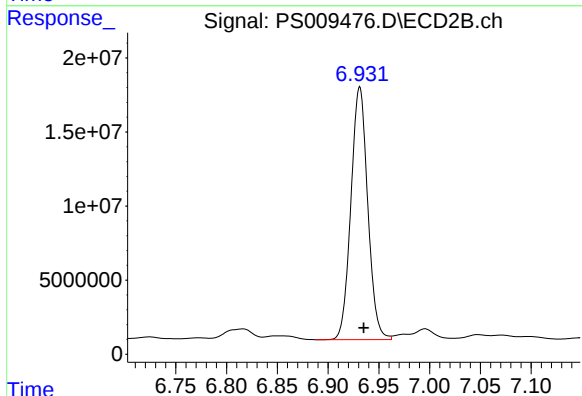


#4 2,4-DCAA

R.T.: 6.931 min
Delta R.T.: -0.004 min
Response: 196806277
Conc: 358.35 ng/ml

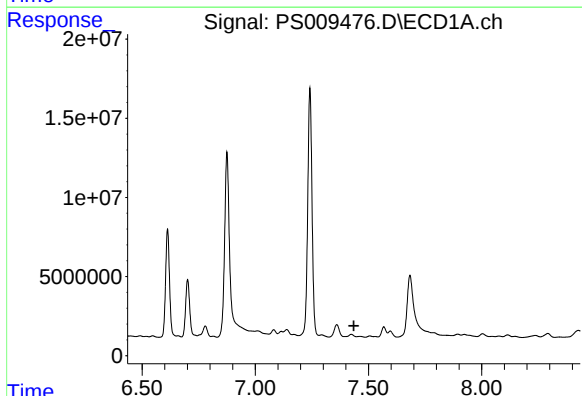


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.435 min
Response: 0
Conc: N.D.

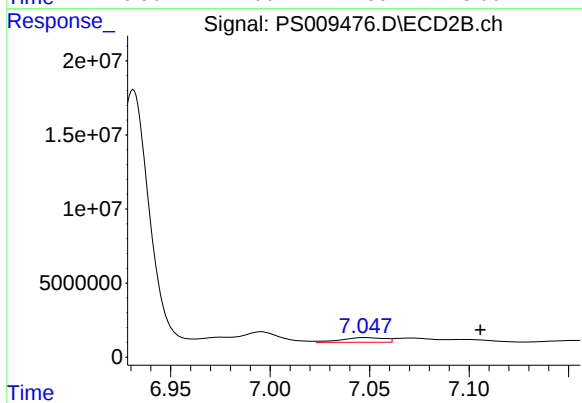

#5 DICAMBA


R.T.: 7.048 min
Delta R.T.: -0.058 min
Response: 4777338
Conc: 2.08 ng/ml

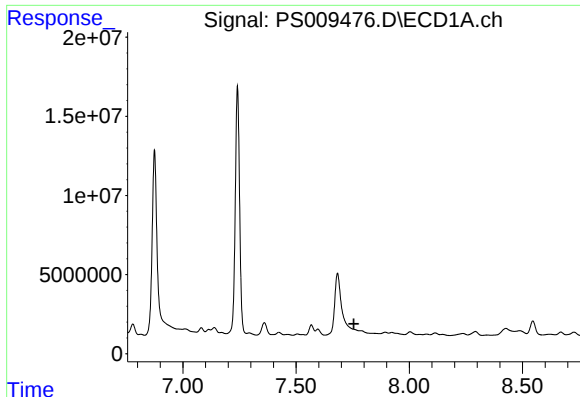

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.756 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

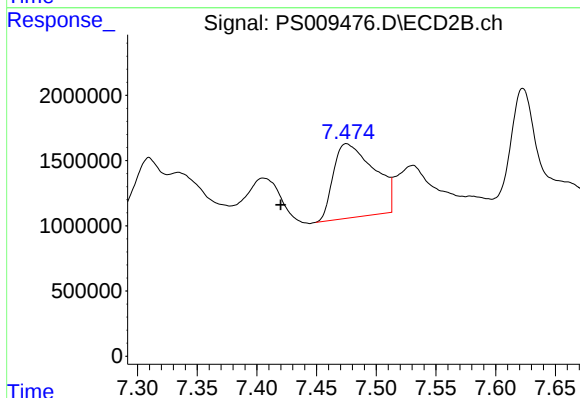


#7 MCPA

R.T.: 7.476 min
Delta R.T.: 0.056 min
Response: 13467312
Conc: 4.99 ug/ml

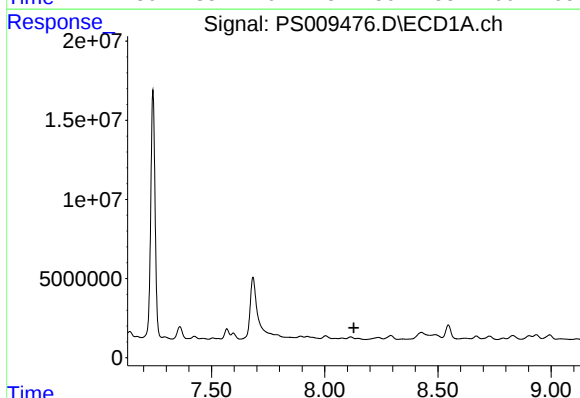


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

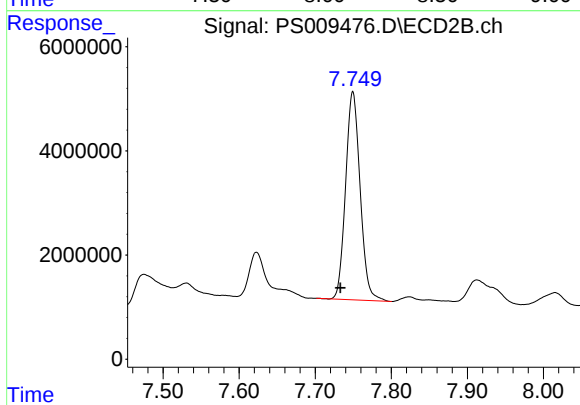

#8 DICHLORPROP


R.T.: 7.750 min
Delta R.T.: 0.016 min
Response: 53125916
Conc: 95.75 ng/ml

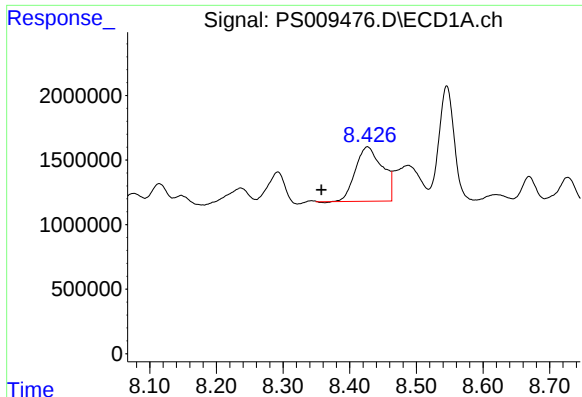

#9 2,4-D


R.T.: 8.427 min
Delta R.T.: 0.069 min
Response: 11866047
Conc: 22.51 ng/ml

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

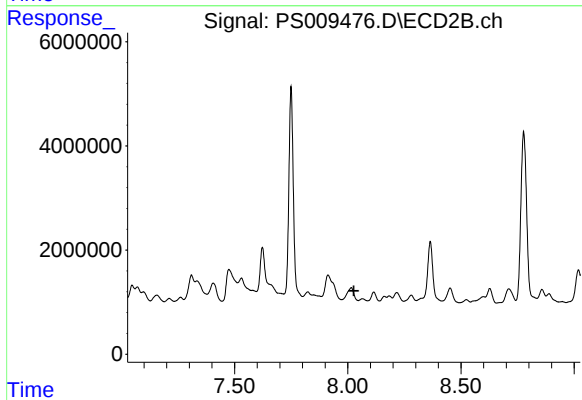


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 8.027 min
Response: 0
Conc: N.D.

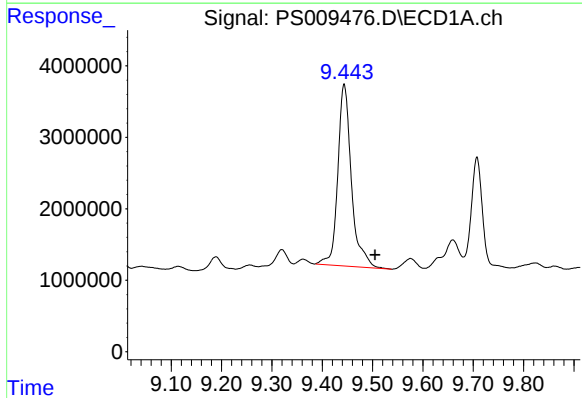


#12 2,4,5-T

R.T.: 9.444 min
Delta R.T.: -0.061 min
Response: 47762935
Conc: 18.78 ng/ml

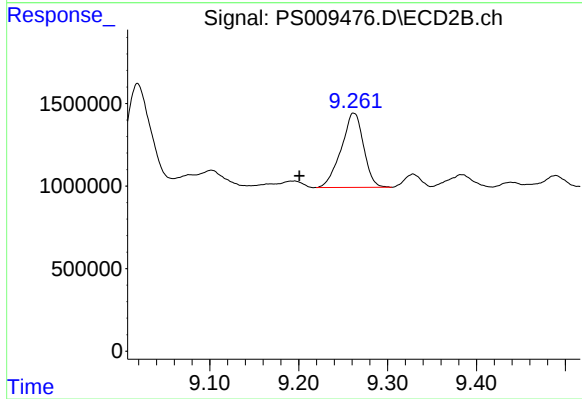

#12 2,4,5-T


R.T.: 9.262 min
Delta R.T.: 0.061 min
Response: 7894561
Conc: 2.67 ng/ml

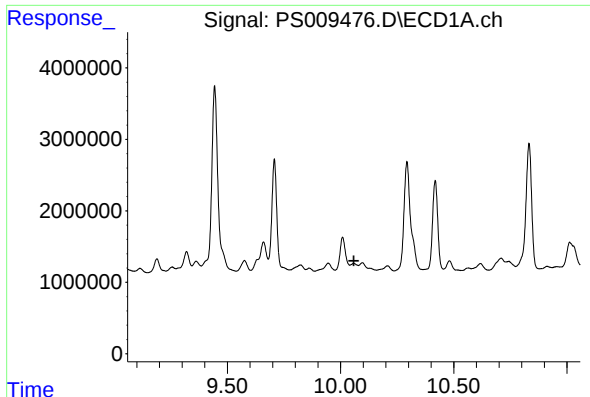

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 10.059 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

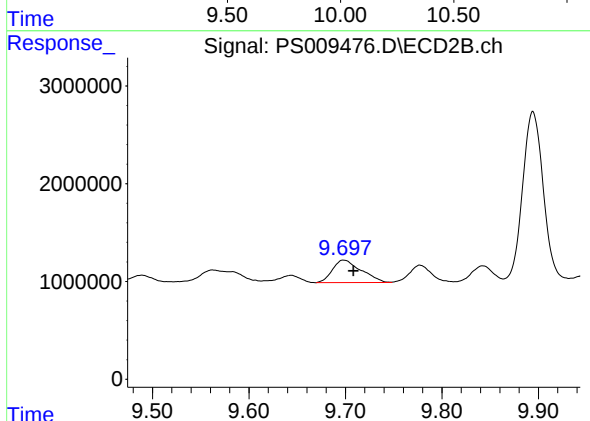


#13 2,4-DB

R.T.: 9.698 min
Delta R.T.: -0.010 min
Response: 4782182
Conc: 12.60 ng/ml

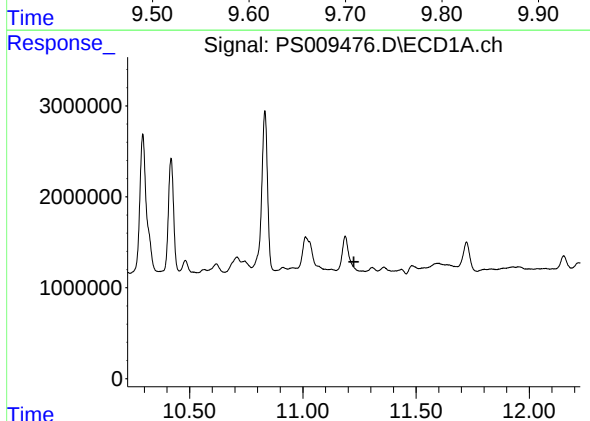


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 11.225 min
Response: 0
Conc: N.D.

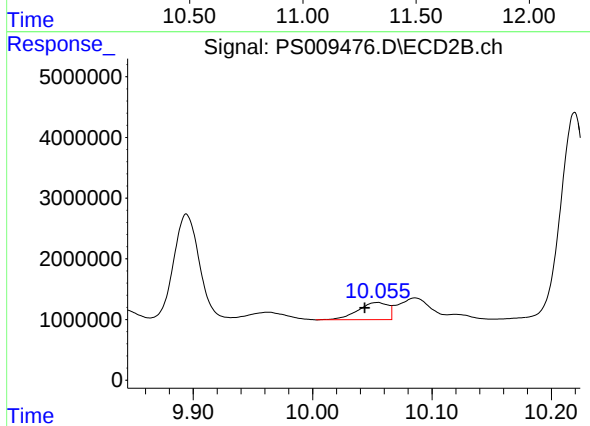

#14 DINOSEB


R.T.: 10.054 min
Delta R.T.: 0.010 min
Response: 4971939
Conc: 2.26 ng/ml

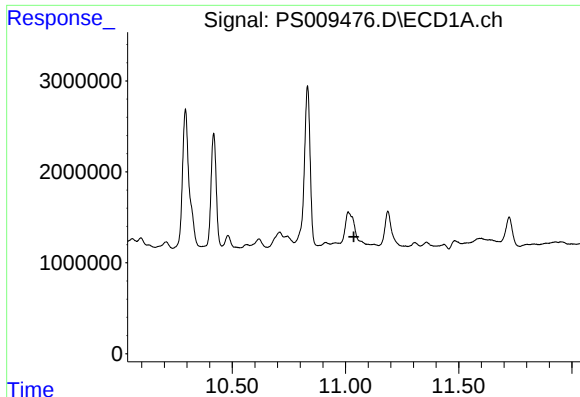

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 11.037 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
BUS-WASH

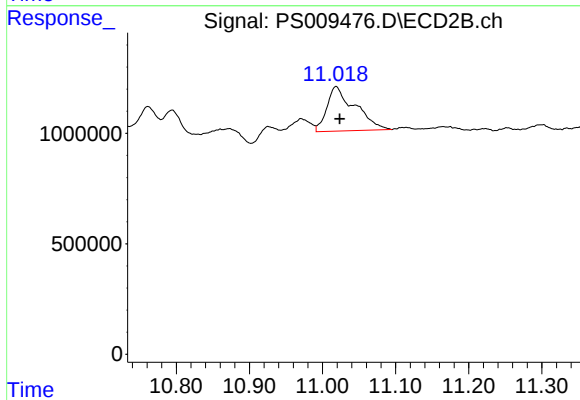


#15 Picloram

R.T.: 11.019 min
Delta R.T.: -0.005 min
Response: 5387947
Conc: 1.32 ng/ml

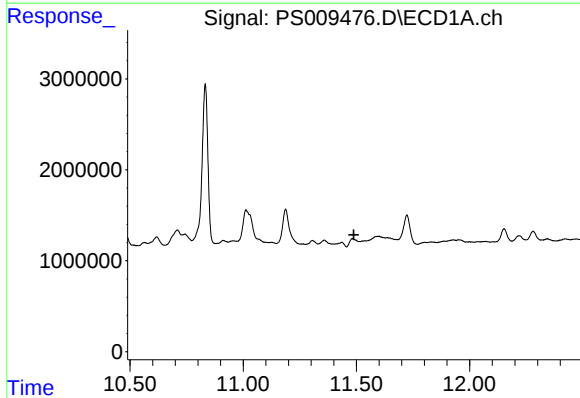

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 11.489 min
Response: 0
Conc: N.D.

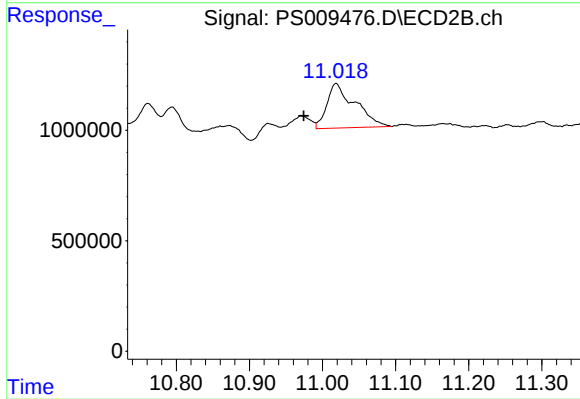

#16 DCPA

R.T.: 11.019 min
Delta R.T.: 0.045 min
Response: 5387947
Conc: 1.39 ng/ml