

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032720\
 Data File : PS009478.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Mar 2020 20:41
 Operator : DD\AJ
 Sample : L2040-06
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 RO-06

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 28 05:47:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
 Quant Title : 8080.M
 QLast Update : Thu Mar 12 07:13:24 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.240	6.930	243.3E6	197.0E6	439.842	358.751
Target Compounds							
1) T	Dalapon	3.005	2.586	22241125	84691201	28.520	107.563 #
2) T	3,5-DICHL...	0.000	6.107	0	60687424	N.D.	74.618
5) T	DICAMBA	0.000	7.152	0	5213446	N.D.	2.271
6) T	MCP	0.000	7.218	0	113.9E6	N.D.	62.600
8) T	DICHLORPROP	0.000	7.749	0	34757534	N.D.	62.646
10) T	Pentachlo...	8.670	8.454	2142.3E6	2073.2E6	304.683	273.147
11) T	2,4,5-TP ...	0.000	8.797	0	204.0E6	N.D.	68.432
12) T	2,4,5-T	9.443	9.262	63330442	4437683	24.895	1.503 #
13) T	2,4-DB	0.000	9.699	0	7121492	N.D.	18.760
14) T	DINOSEB	11.188	10.083	8288493	11635030	4.055	5.297 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032720\
Data File : PS009478.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Mar 2020 20:41
Operator : DD\AJ
Sample : L2040-06
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
RO-06

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 28 05:47:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS031120.M
Quant Title : 8080.M
QLast Update : Thu Mar 12 07:13:24 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

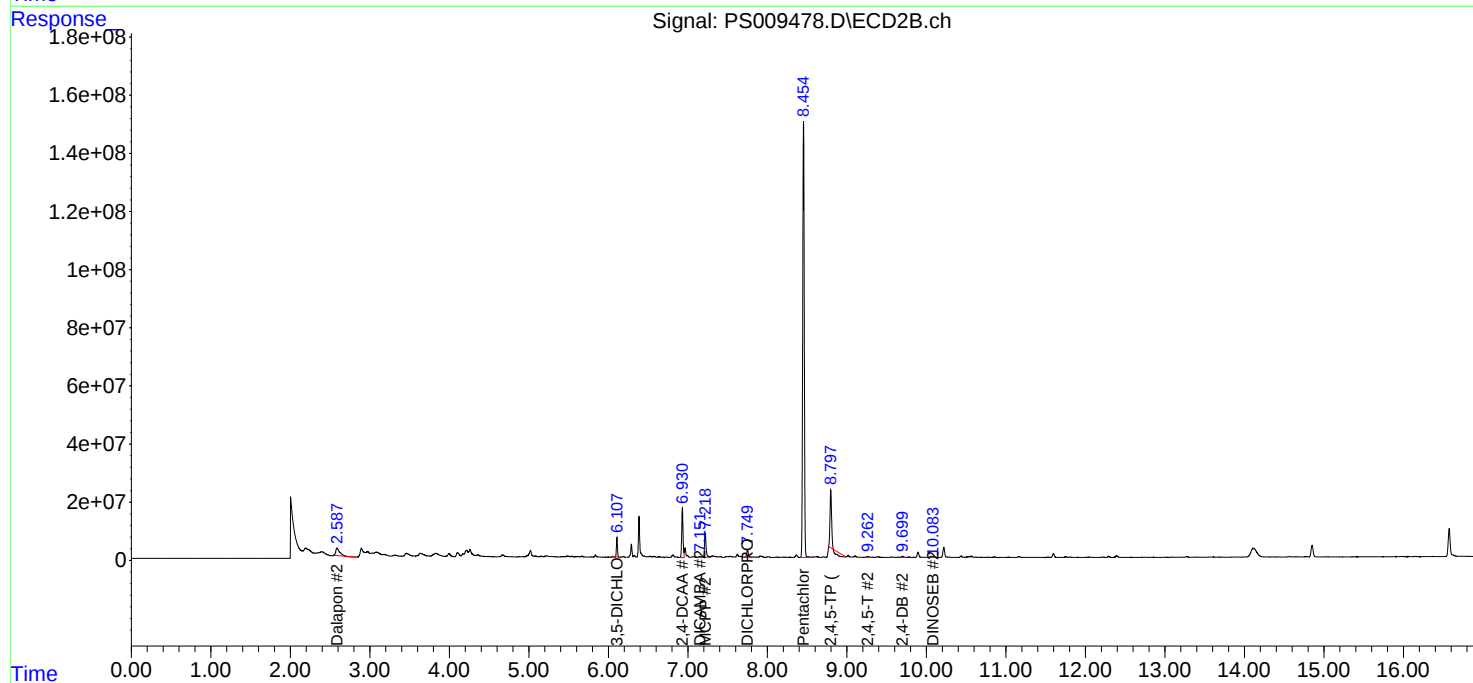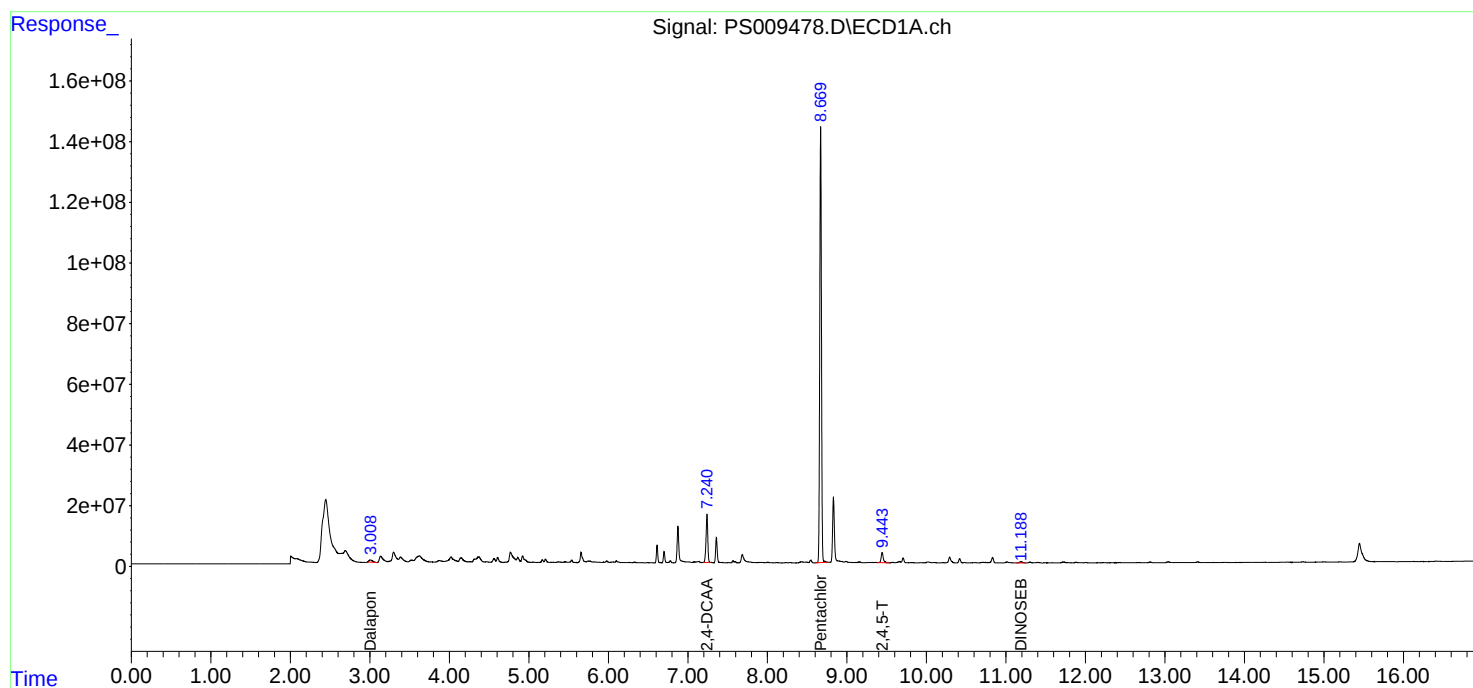


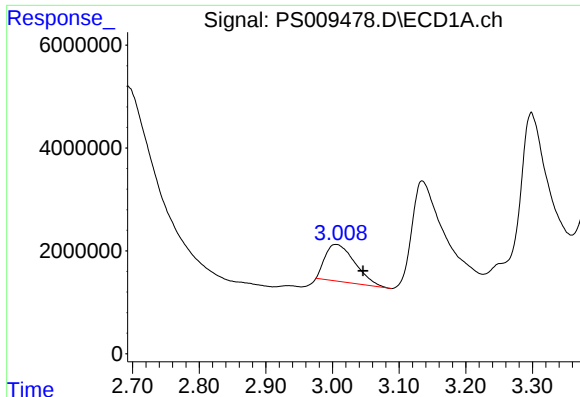

#1 Dalapon


R.T.: 3.005 min
Delta R.T.: -0.041 min
Response: 22241125
Conc: 28.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-06

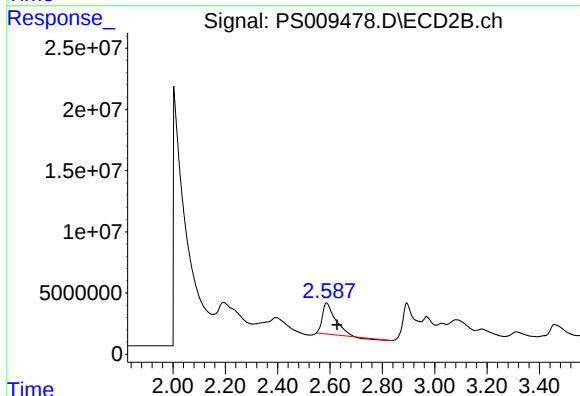


#1 Dalapon

R.T.: 2.586 min
Delta R.T.: -0.040 min
Response: 84691201
Conc: 107.56 ng/ml

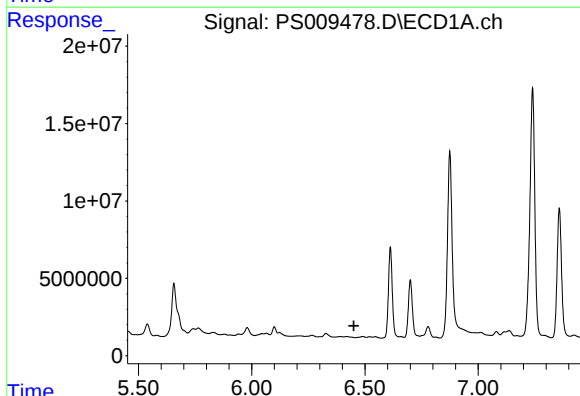


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.451 min
Response: 0
Conc: N.D.

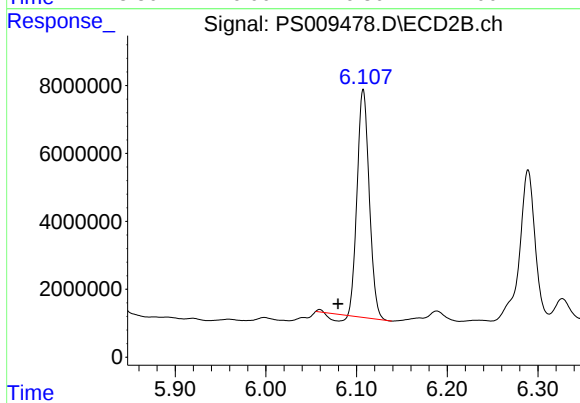

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.107 min
Delta R.T.: 0.028 min
Response: 60687424
Conc: 74.62 ng/ml

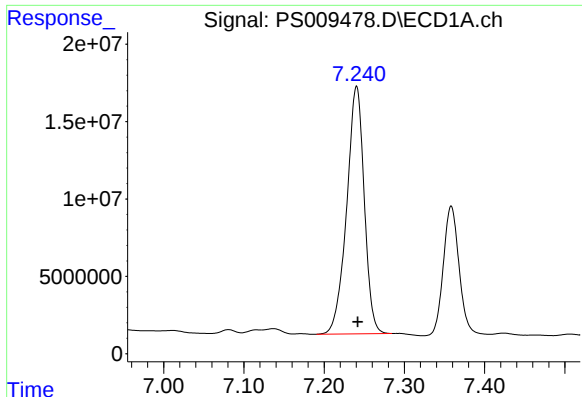

#4 2,4-DCAA


R.T.: 7.240 min
Delta R.T.: -0.002 min
Response: 243307280
Conc: 439.84 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-06

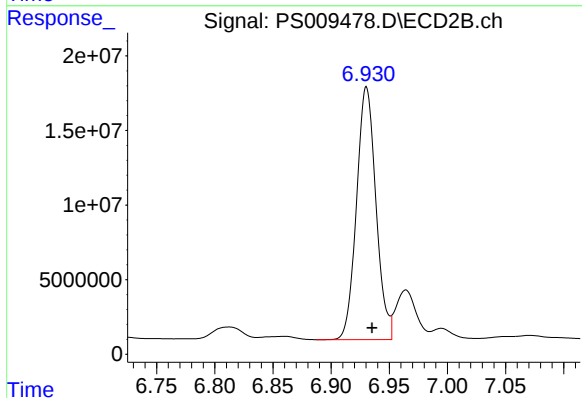


#4 2,4-DCAA

R.T.: 6.930 min
Delta R.T.: -0.005 min
Response: 197025473
Conc: 358.75 ng/ml

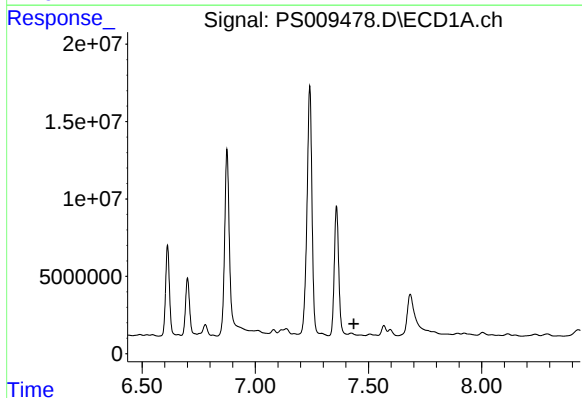


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 7.435 min
Response: 0
Conc: N.D.

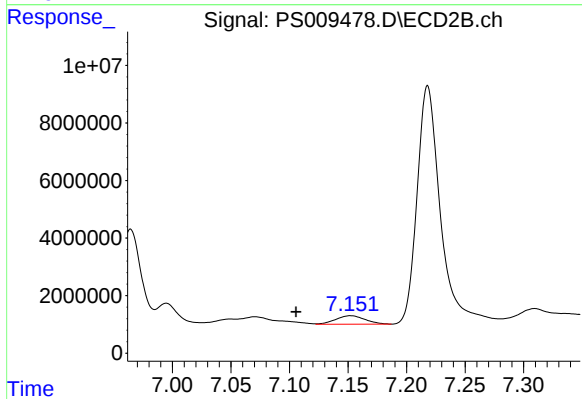

#5 DICAMBA


R.T.: 7.152 min
Delta R.T.: 0.047 min
Response: 5213446
Conc: 2.27 ng/ml

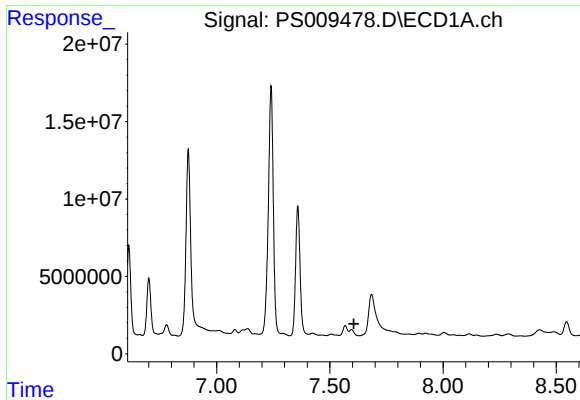

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.606 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
RO-06

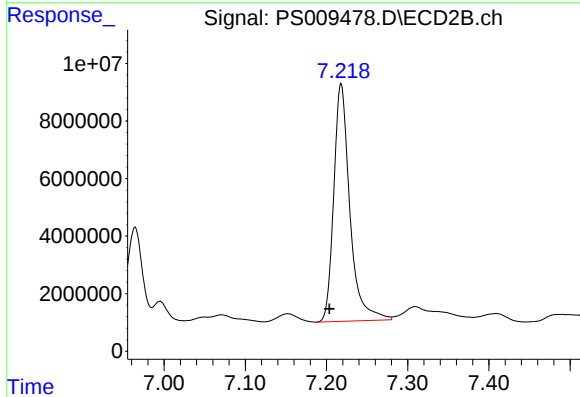


#6 MCP

R.T.: 7.218 min
Delta R.T.: 0.015 min
Response: 113857238
Conc: 62.60 ug/ml

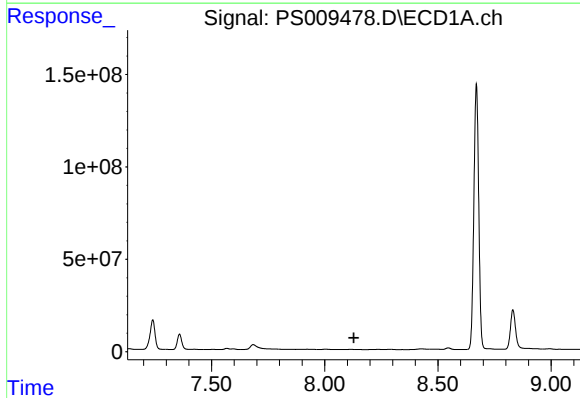


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.129 min
Response: 0
Conc: N.D.

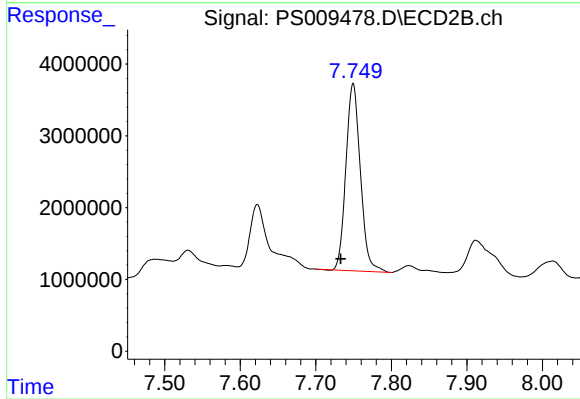

#8 DICHLORPROP


R.T.: 7.749 min
Delta R.T.: 0.016 min
Response: 34757534
Conc: 62.65 ng/ml

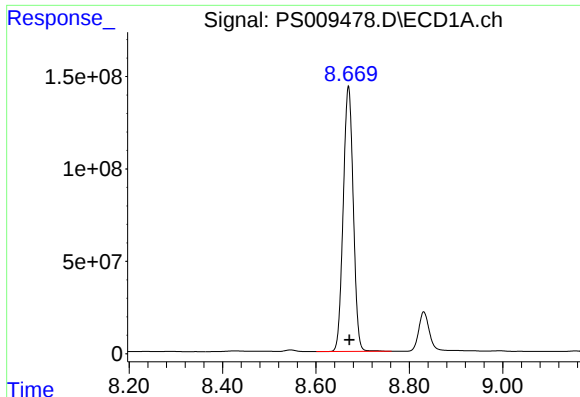

#10 Pentachlorophenol


R.T.: 8.670 min
Delta R.T.: -0.002 min
Response: 2142300361
Conc: 304.68 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-06

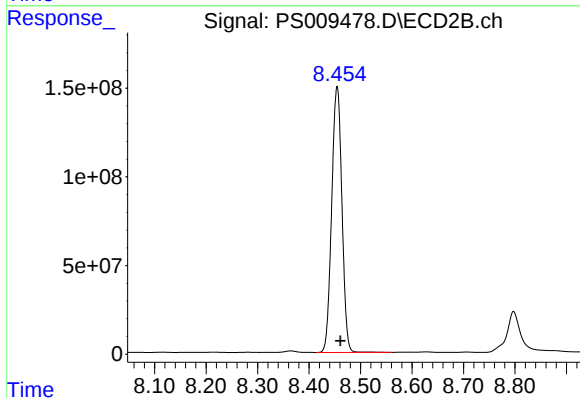


#10 Pentachlorophenol

R.T.: 8.454 min
Delta R.T.: -0.006 min
Response: 2073179090
Conc: 273.15 ng/ml

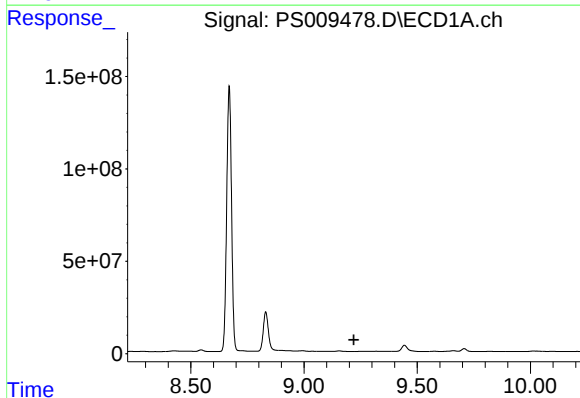


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.221 min
Response: 0
Conc: N.D.

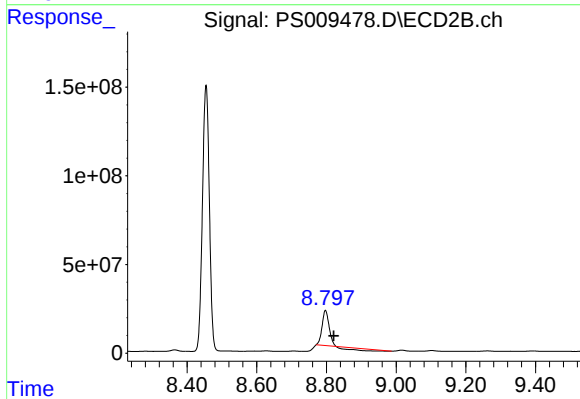

#11 2,4,5-TP (SILVEX)


R.T.: 8.797 min
Delta R.T.: -0.024 min
Response: 204002575
Conc: 68.43 ng/ml

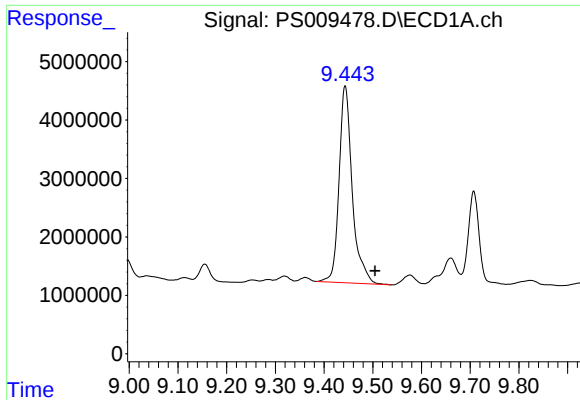

#12 2,4,5-T


R.T.: 9.443 min
Delta R.T.: -0.062 min
Response: 63330442
Conc: 24.90 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-06

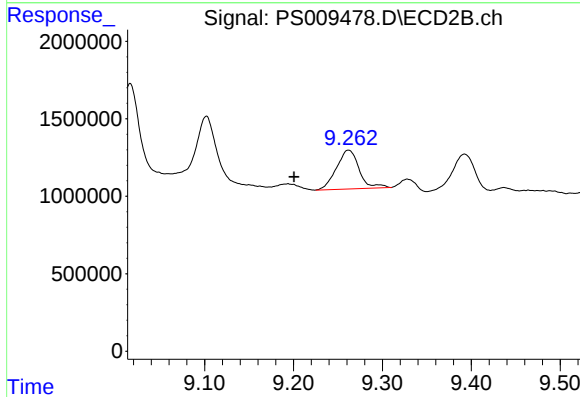


#12 2,4,5-T

R.T.: 9.262 min
Delta R.T.: 0.061 min
Response: 4437683
Conc: 1.50 ng/ml

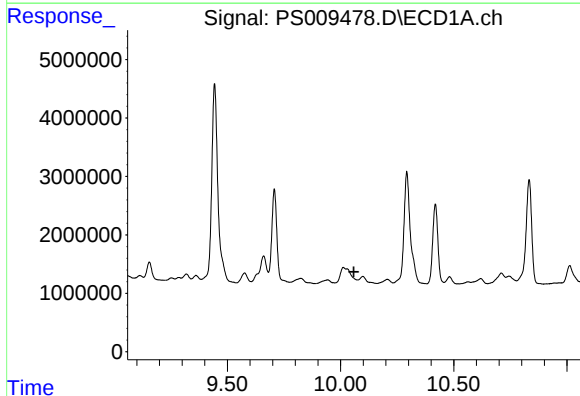


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 10.059 min
Response: 0
Conc: N.D.

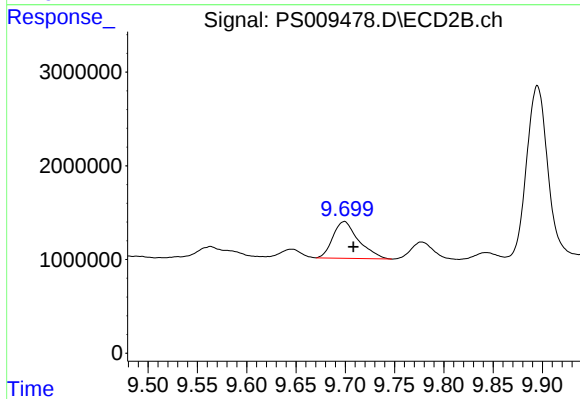

#13 2,4-DB


R.T.: 9.699 min
Delta R.T.: -0.009 min
Response: 7121492
Conc: 18.76 ng/ml

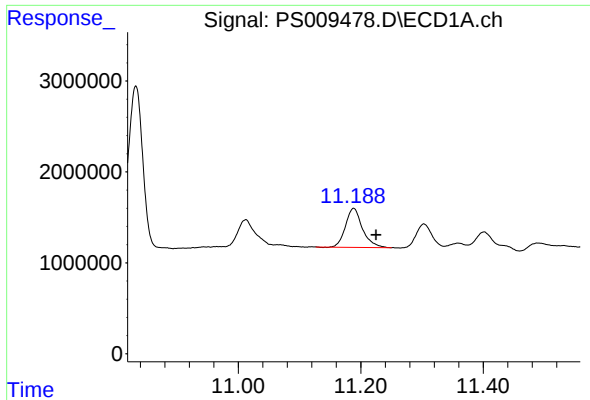

#14 DINOSEB

R.T.: 11.188 min
Delta R.T.: -0.037 min
Response: 8288493
Conc: 4.05 ng/ml

Instrument :
ECD_S
ClientSampleId :
RO-06

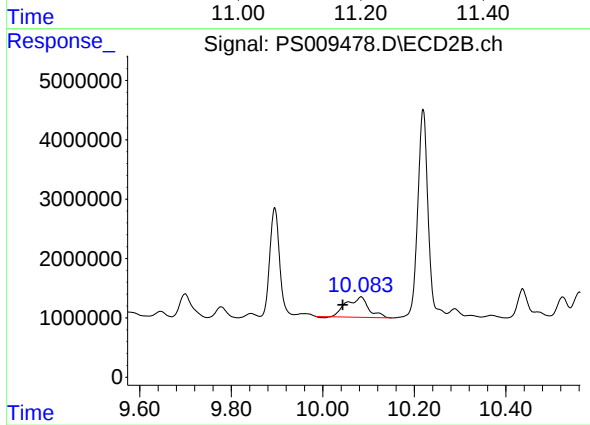

#14 DINOSEB

R.T.: 10.083 min
Delta R.T.: 0.040 min
Response: 11635030
Conc: 5.30 ng/ml