

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032725\
 Data File : PS029543.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2025 12:12
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 16:27:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032625.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 26 16:20:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.133	7.544	1108.2E6	454.4E6	267.080	482.874 #
Target Compounds							
1) T	Dalapon	2.640f	2.566f	15526352	70335560	2.331	29.851 #
3) T	4-Nitroph...	6.948	0.000	5036006	0	7.361	N.D. #
6) T	MCP	0.000	7.818	0	5790400	N.D.	2.420
7) T	MCPA	7.613	0.000	145797	0	<MDL	N.D. #
8) T	DICHLORPROP	7.998	0.000	225603	0	<MDL	N.D. #
9) T	2,4-D	8.216	0.000	721683	0	<MDL	N.D. #
10) T	Pentachlo...	8.542	9.271	2216271	7108062	<MDL	<MDL #
11) T	2,4,5-TP ...	9.080	0.000	2369288	0	<MDL	N.D. #
12) T	2,4,5-T	9.336f	0.000	1055710	0	<MDL	N.D. #
13) T	2,4-DB	9.975	0.000	277493	0	<MDL	N.D. #
14) T	DINOSEB	11.150	0.000	881155	0	<MDL	N.D. #
15) T	Picloram	10.966	0.000	1466849	0	<MDL	N.D. #
16) T	DCPA	11.416	0.000	359648	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032725\
Data File : PS029543.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2025 12:12
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 16:27:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032625.M
Quant Title : 8080.M
QLast Update : Wed Mar 26 16:20:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

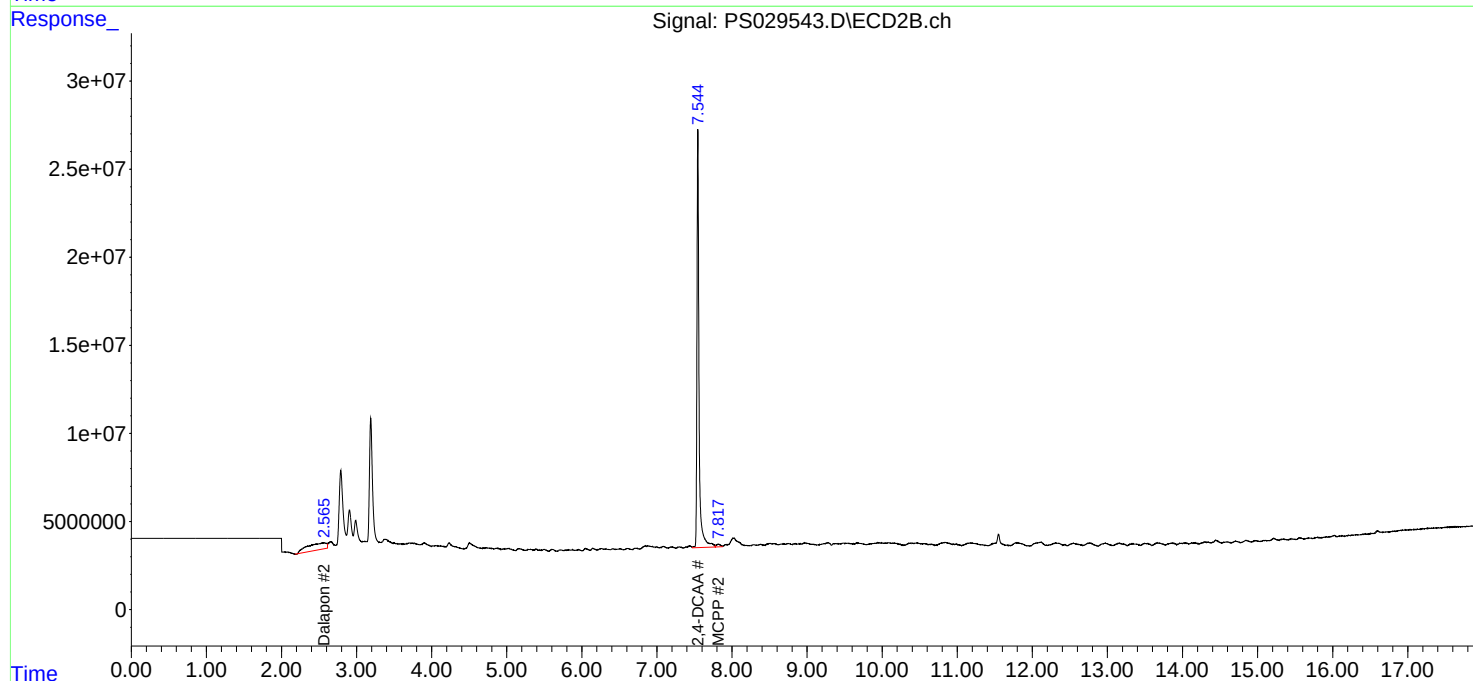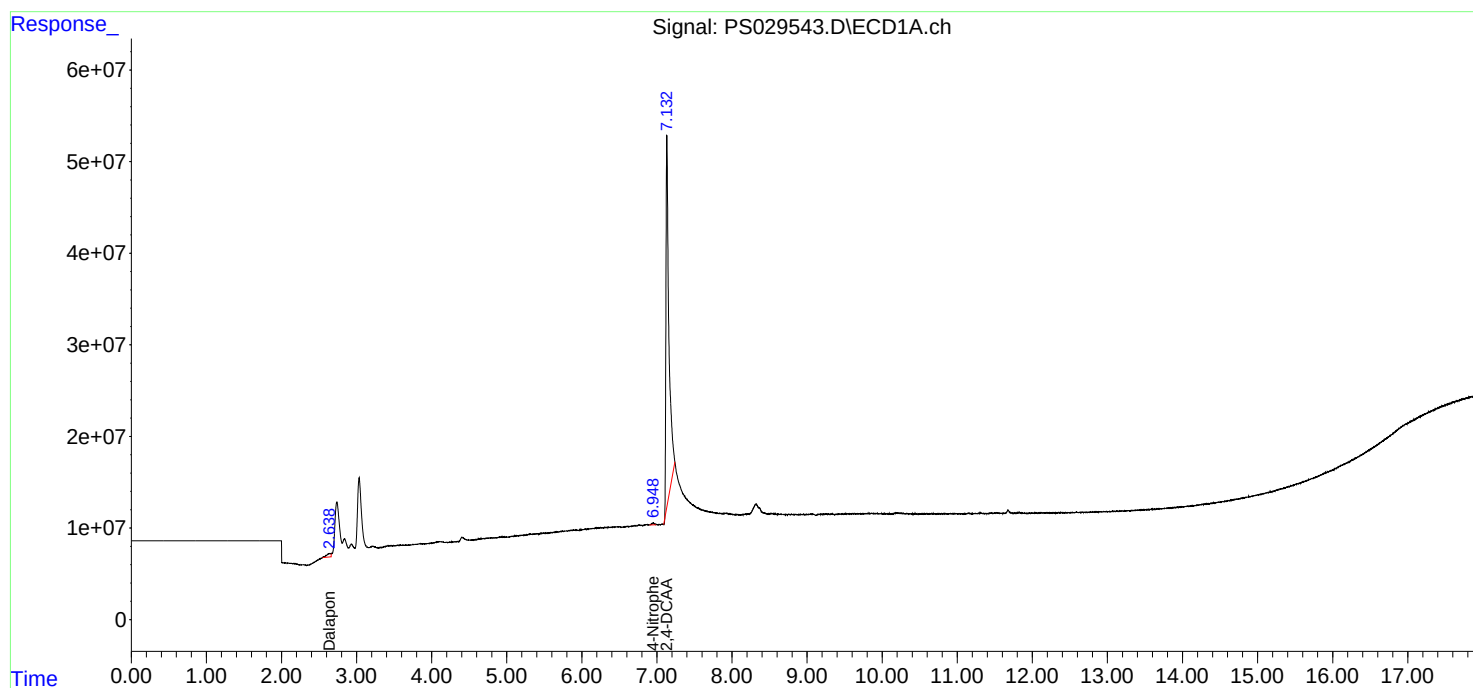


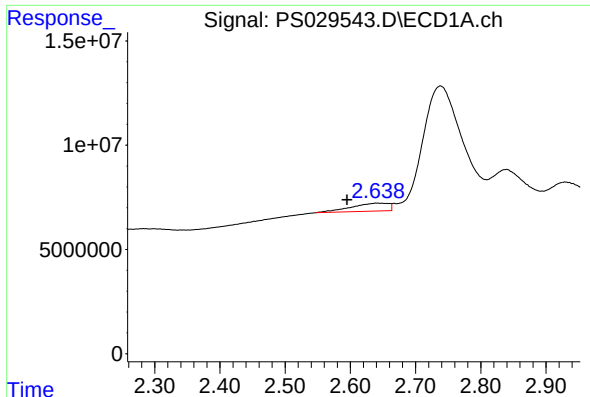

#1 Dalapon


R.T.: 2.640 min
Delta R.T.: 0.045 min
Response: 15526352
Conc: 2.33 ng/ml

Instrument :
ECD_S
ClientSampleId :

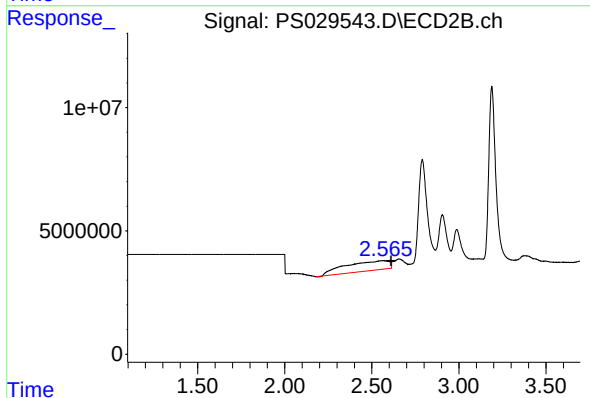


#1 Dalapon

R.T.: 2.566 min
Delta R.T.: -0.044 min
Response: 70335560
Conc: 29.85 ng/ml

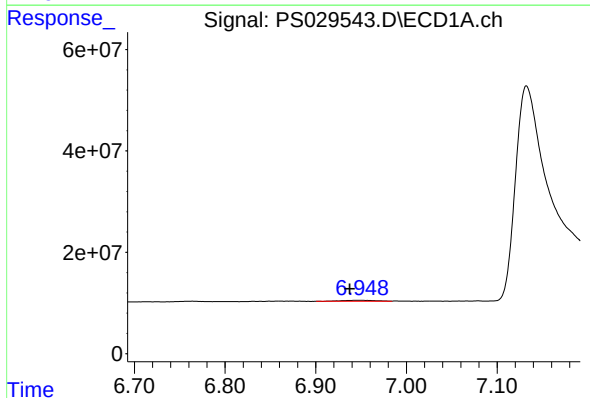


#3 4-Nitrophenol

R.T.: 6.948 min
Delta R.T.: 0.010 min
Response: 5036006
Conc: 7.36 ng/ml

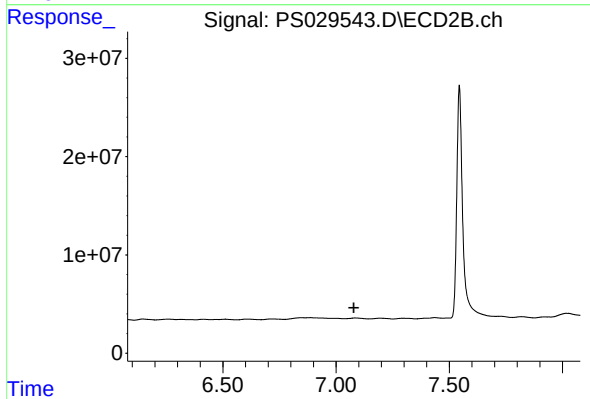

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.079 min
Response: 0
Conc: N.D.

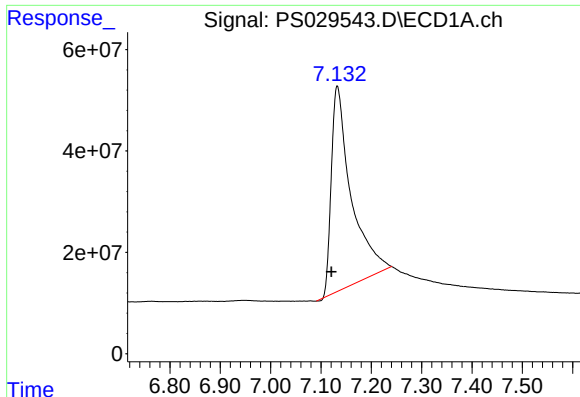

#4 2,4-DCAA


R.T.: 7.133 min
Delta R.T.: 0.011 min
Response: 1108231360
Conc: 267.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

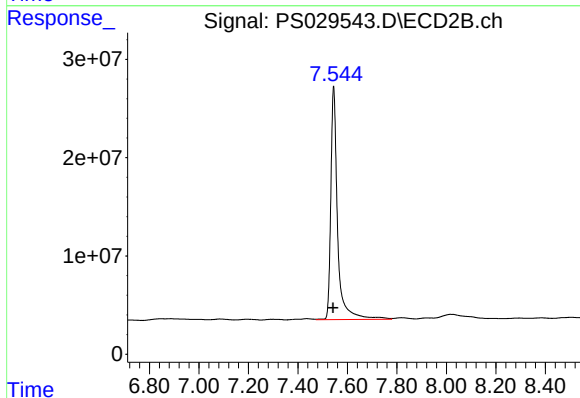


#4 2,4-DCAA

R.T.: 7.544 min
Delta R.T.: 0.003 min
Response: 454362049
Conc: 482.87 ng/ml

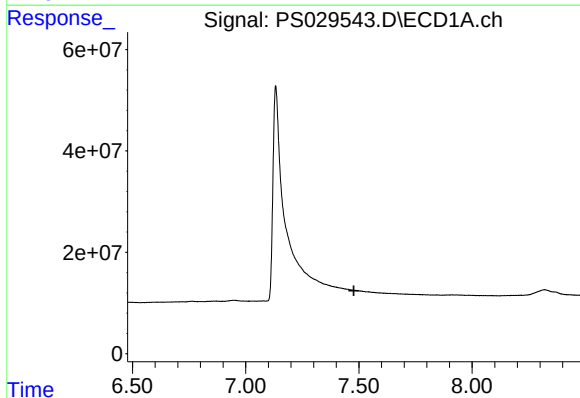

#6 MCP

R.T.: 0.000 min
Exp R.T. : 7.478 min
Response: 0
Conc: N.D.

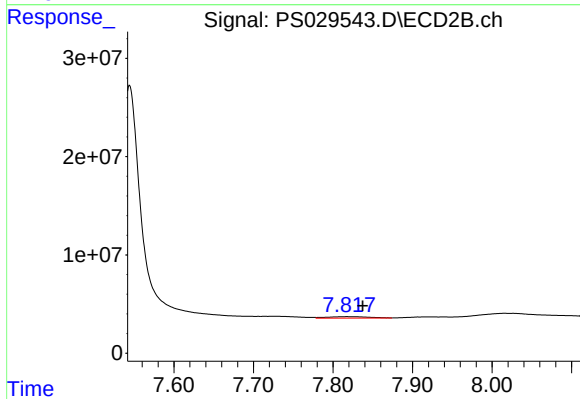

#6 MCP

R.T.: 7.818 min
Delta R.T.: -0.019 min
Response: 5790400
Conc: 2.42 ug/ml