

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032725\
 Data File : PS029551.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Mar 2025 16:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 26 17:09:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032625.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 26 16:20:53 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.125	7.541	1548.0E6	442.0E6	373.052	469.727 #
Target Compounds							
1) T	Dalapon	0.000	2.565f	0	63989050	N.D.	27.157
2) T	3,5-DICHL...	6.313	0.000	972649	0	<MDL	N.D. #
3) T	4-Nitroph...	6.917	7.065	13190681	6194556	19.279	6.806 #
5) T	DICAMBA	0.000	7.731	0	4625287	N.D.	<MDL
6) T	MCP	7.459	0.000	1909599	0	<MDL	N.D. #
7) T	MCPA	7.647	0.000	5388584	0	<MDL	N.D. #
8) T	DICHLORPROP	7.985	8.483f	395697	5370227	<MDL	4.306 #
9) T	2,4-D	8.215	8.708f	1558418	5288245	<MDL	3.822 #
10) T	Pentachlo...	8.523	9.262	11497526	9804730	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	9.650	0	4779554	N.D.	<MDL
12) T	2,4,5-T	9.415f	10.069	27543962	7477886	1.398	<MDL #
14) T	DINOSEB	11.134	0.000	42296531	0	2.350	N.D. #
15) T	Picloram	0.000	12.066	0	53122912	N.D.	3.869
16) T	DCPA	11.428	0.000	6764682	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032725\
Data File : PS029551.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Mar 2025 16:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 26 17:09:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032625.M
Quant Title : 8080.M
QLast Update : Wed Mar 26 16:20:53 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

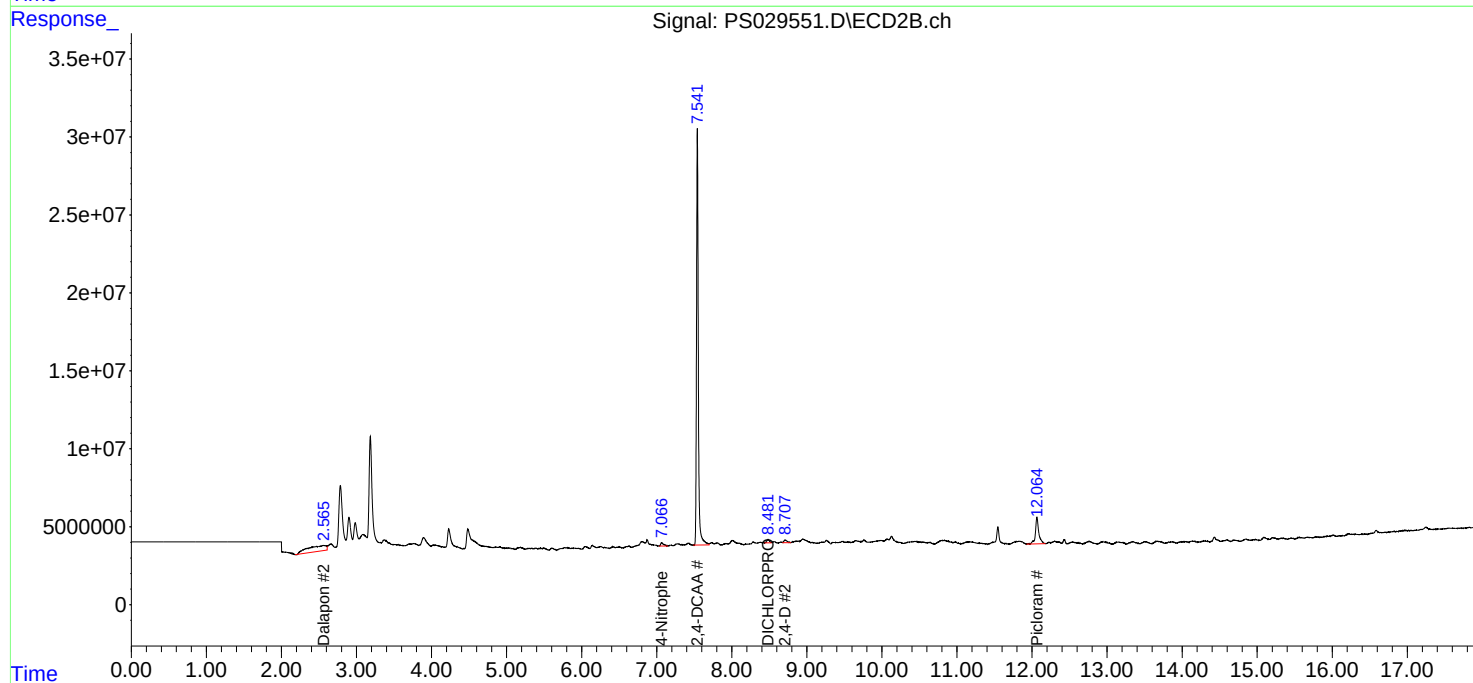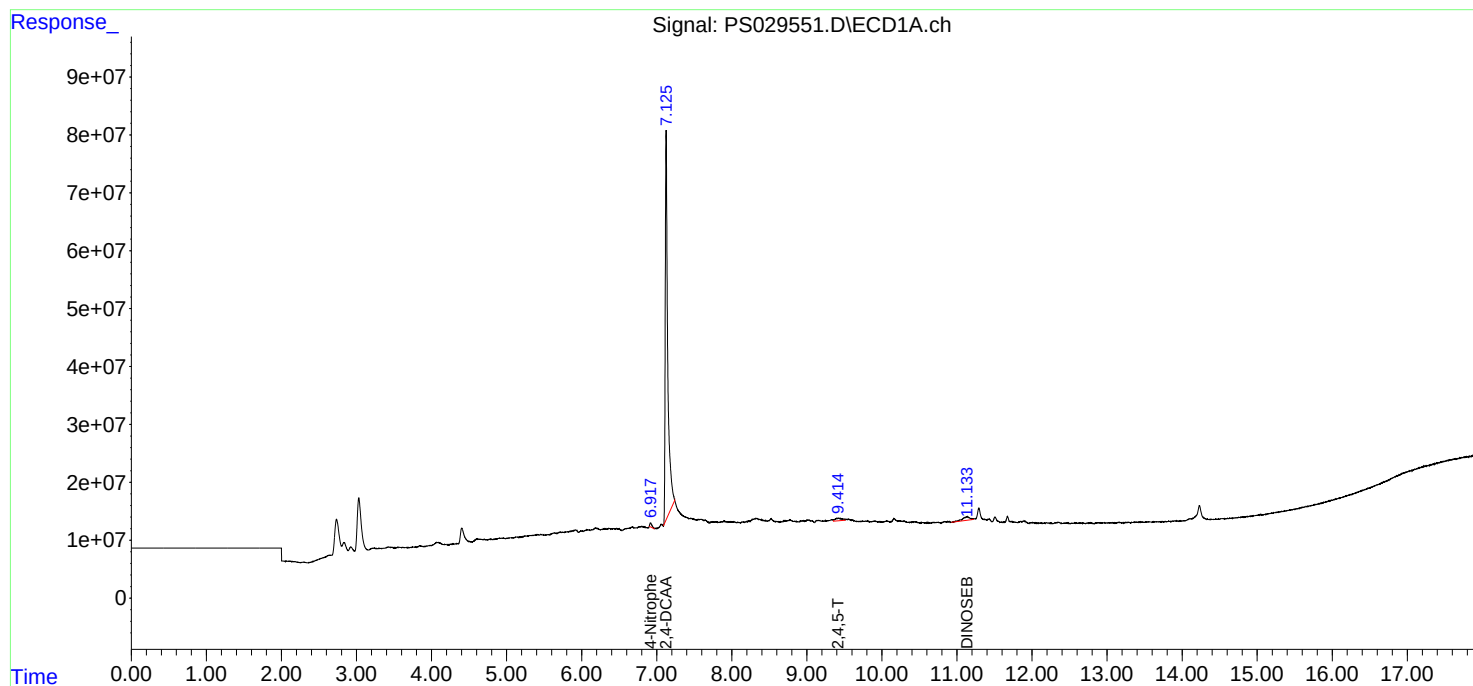


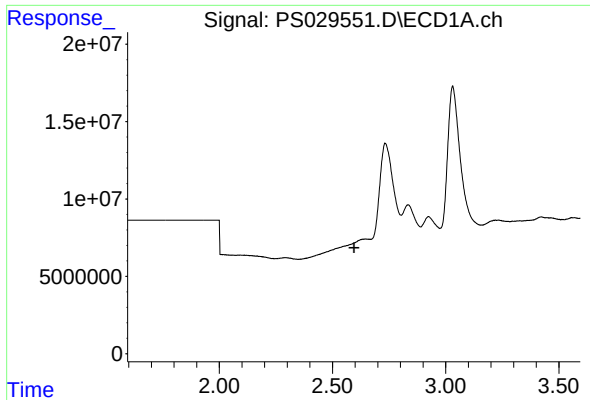

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.595 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

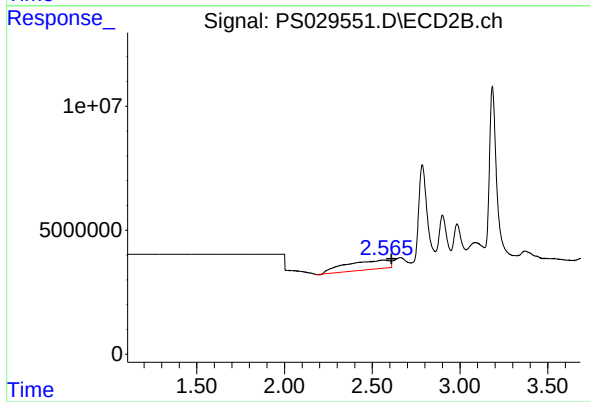


#1 Dalapon

R.T.: 2.565 min
Delta R.T.: -0.045 min
Response: 63989050
Conc: 27.16 ng/ml

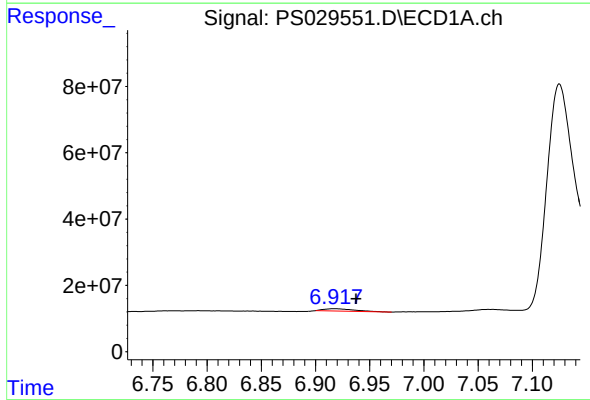


#3 4-Nitrophenol

R.T.: 6.917 min
Delta R.T.: -0.021 min
Response: 13190681
Conc: 19.28 ng/ml

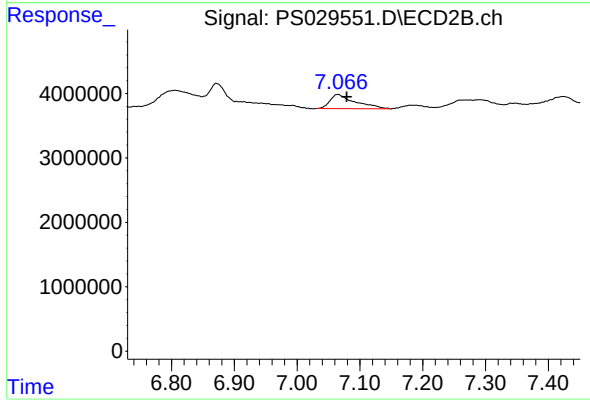

#3 4-Nitrophenol


R.T.: 7.065 min
Delta R.T.: -0.014 min
Response: 6194556
Conc: 6.81 ng/ml

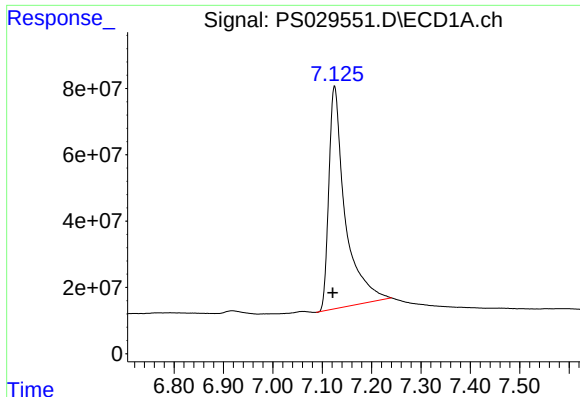

#4 2,4-DCAA


R.T.: 7.125 min
Delta R.T.: 0.004 min
Response: 1547954235
Conc: 373.05 ng/ml

Instrument :
ECD_S
ClientSampleId :

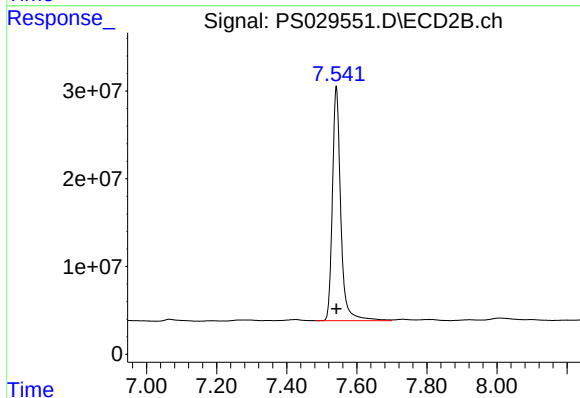


#4 2,4-DCAA

R.T.: 7.541 min
Delta R.T.: 0.000 min
Response: 441990814
Conc: 469.73 ng/ml

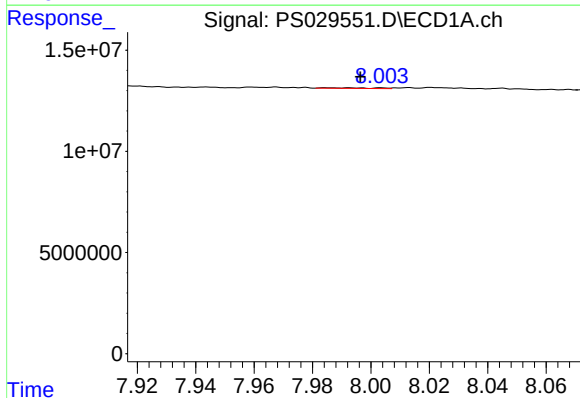


#8 DICHLORPROP

R.T.: 7.985 min
Delta R.T.: -0.011 min
Response: 395697
Conc: N.D.

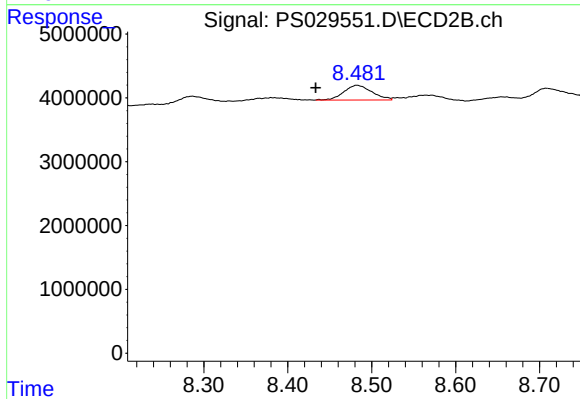

#8 DICHLORPROP


R.T.: 8.483 min
Delta R.T.: 0.049 min
Response: 5370227
Conc: 4.31 ng/ml

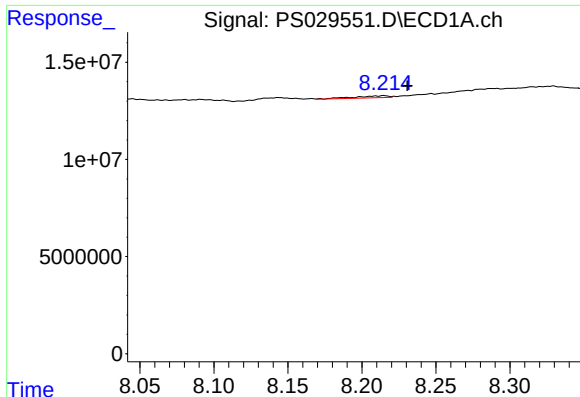

#9 2,4-D


R.T.: 8.215 min
Delta R.T.: -0.016 min
Response: 1558418
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

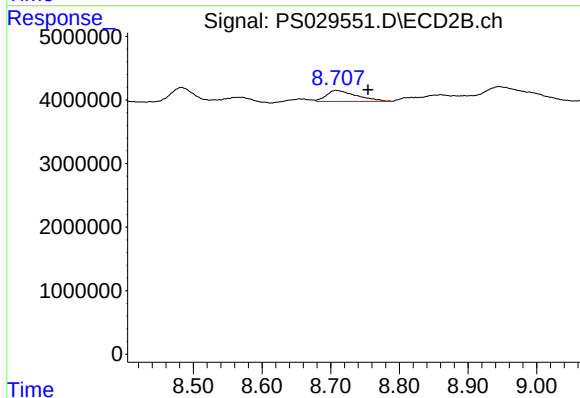


#9 2,4-D

R.T.: 8.708 min
Delta R.T.: -0.046 min
Response: 5288245
Conc: 3.82 ng/ml

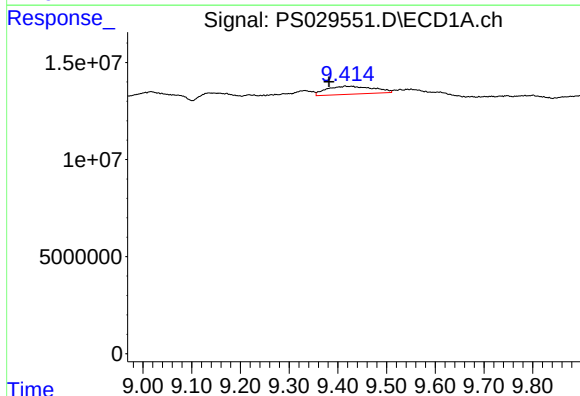


#12 2,4,5-T

R.T.: 9.415 min
Delta R.T.: 0.033 min
Response: 27543962
Conc: 1.40 ng/ml

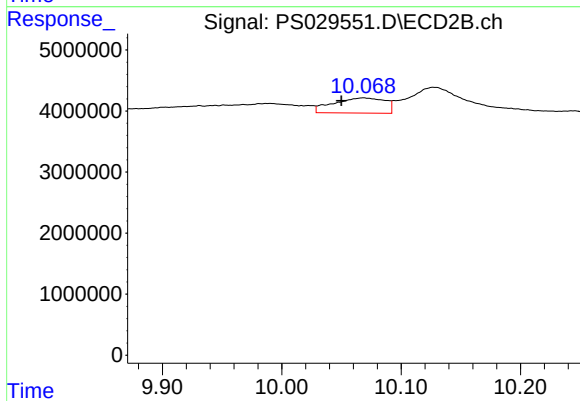

#12 2,4,5-T


R.T.: 10.069 min
Delta R.T.: 0.019 min
Response: 7477886
Conc: N.D.

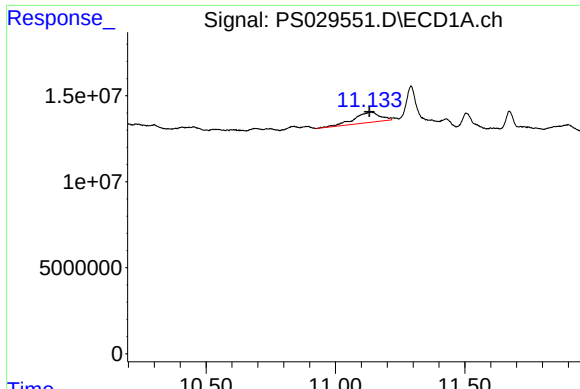

#14 DINOSEB


R.T.: 11.134 min
Delta R.T.: 0.002 min
Response: 42296531
Conc: 2.35 ng/ml

Instrument :
ECD_S
ClientSampleId :

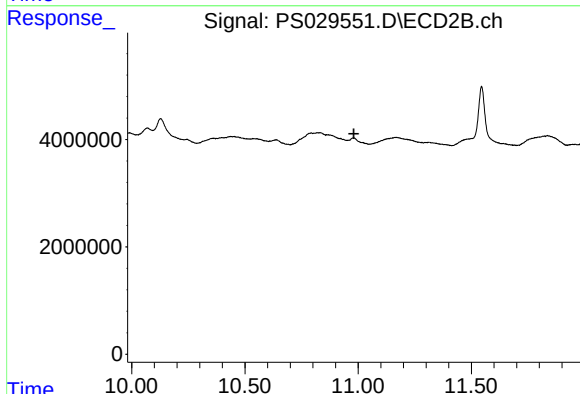


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 10.981 min
Response: 0
Conc: N.D.

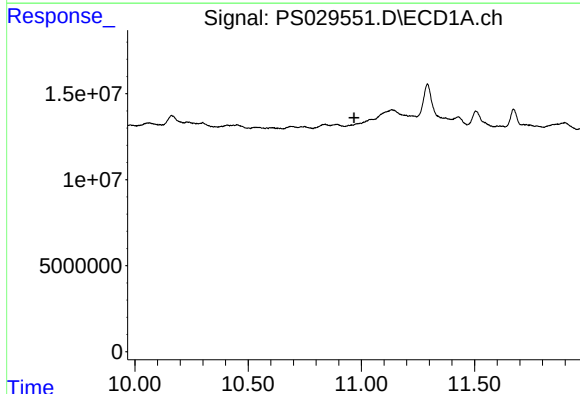

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 10.967 min
Response: 0
Conc: N.D.

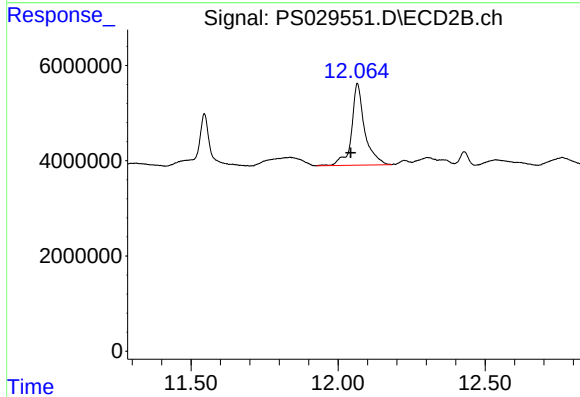

#15 Picloram

R.T.: 12.066 min
Delta R.T.: 0.022 min
Response: 53122912
Conc: 3.87 ng/ml