

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
 Data File : PS003805.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 09:08
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 04:55:54 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.296	10.794	178.5E6	174.7E6	409.117	356.016
Target Compounds							
2) T	3,5-DICHL...	0.000	8.956	0	253734	N.D.	0.398 #
3) T	4-Nitroph...	0.000	9.931	0	194312	N.D.	0.856 #
7) T	MCPA	0.000	11.682	0	371593	N.D.	0.208 #
8) T	DICHLORPROP	0.000	12.191	0	21429	N.D.	0.046 #
9) T	2,4-D	0.000	12.657	0	106846	N.D.	0.201 #
10) T	Pentachlo...	0.000	13.156	0	317715	N.D.	0.046 #
11) T	2,4,5-TP ...	0.000	13.795	0	219779	N.D.	0.083 #
12) T	2,4,5-T	0.000	14.354	0	154604	N.D.	0.071 #
13) T	2,4-DB	0.000	14.972	0	499084	N.D.	1.681 #
14) T	DINOSEB	0.000	15.471	0	478483	N.D.	0.249 #
15) T	Picloram	0.000	16.642	0	478535	N.D.	0.151 #
16) T	DCPA	0.000	16.642	0	478535	N.D.	0.142 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
Data File : PS003805.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 09:08
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 04:55:54 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

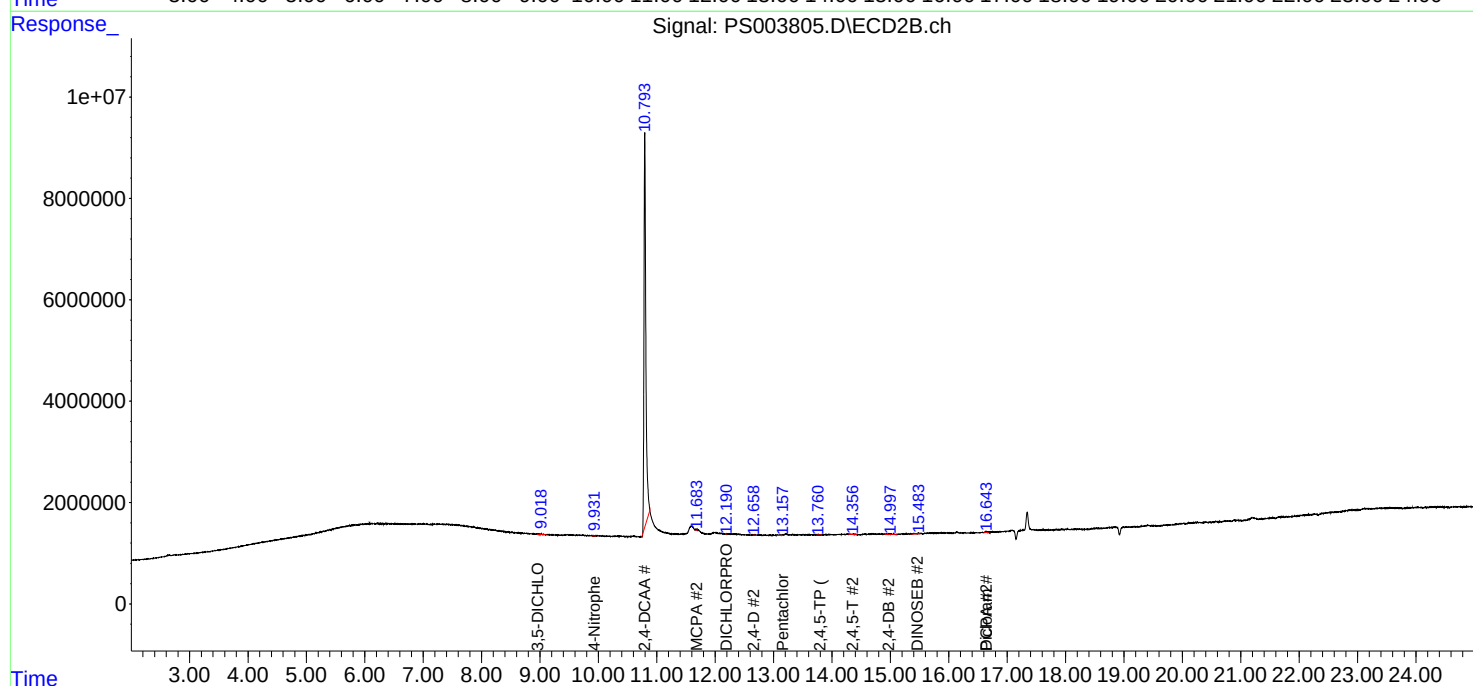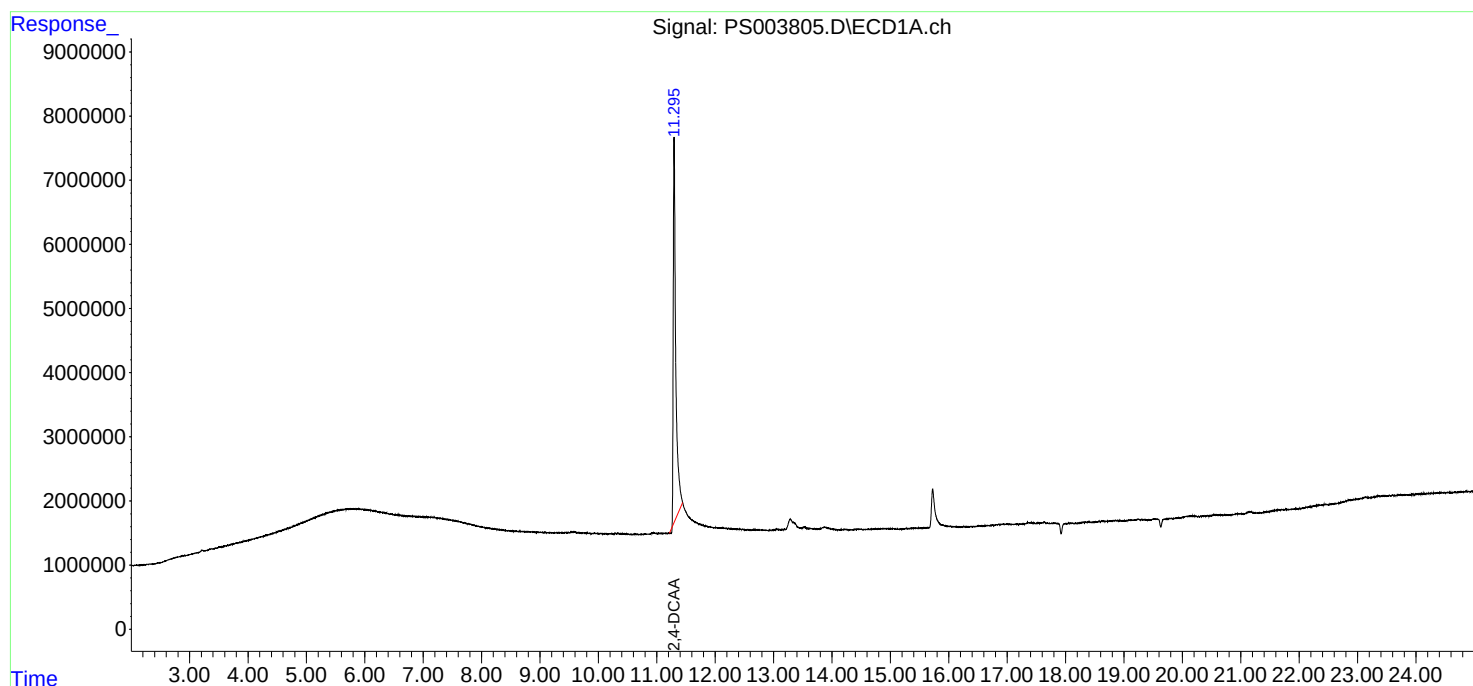


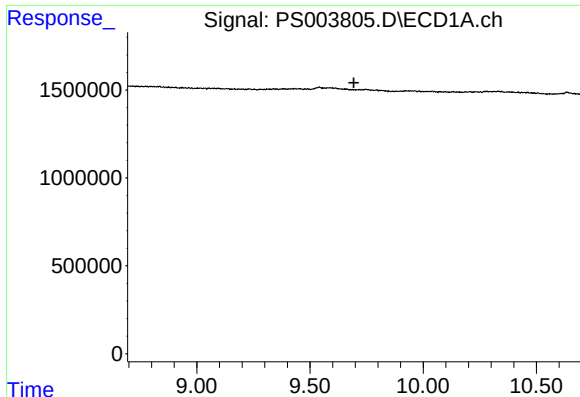

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

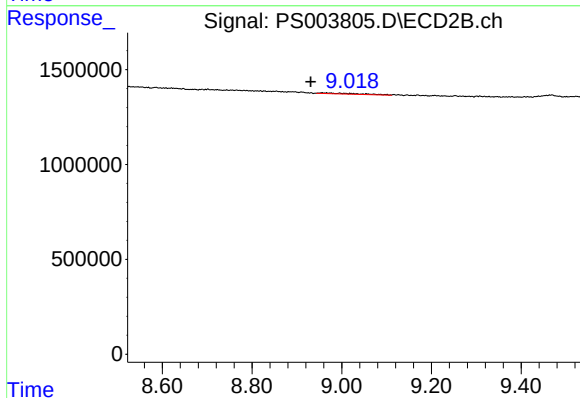


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.956 min
Delta R.T.: 0.025 min
Response: 253734
Conc: 0.40 ng/ml

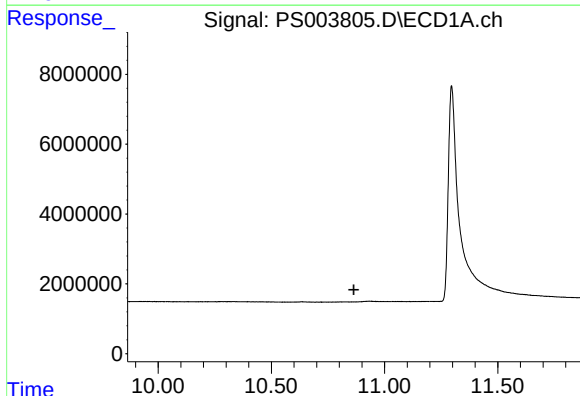


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

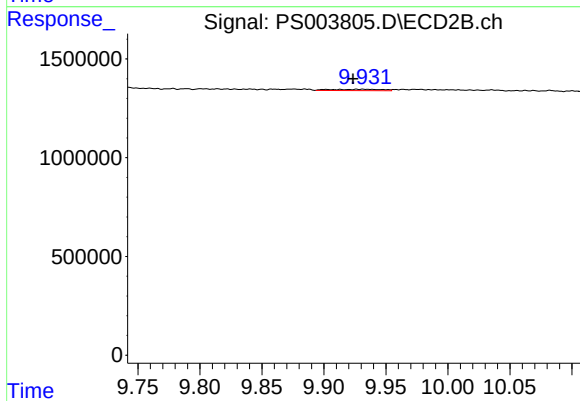

#3 4-Nitrophenol


R.T.: 9.931 min
Delta R.T.: 0.008 min
Response: 194312
Conc: 0.86 ng/ml

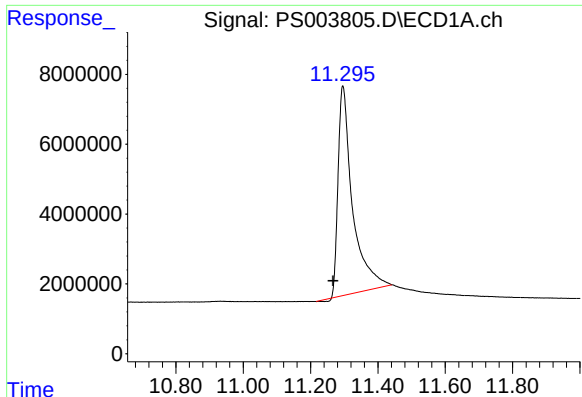

#4 2,4-DCAA


R.T.: 11.296 min
Delta R.T.: 0.029 min
Response: 178461851
Conc: 409.12 ng/ml

Instrument :
ECD_S
ClientSampleId :

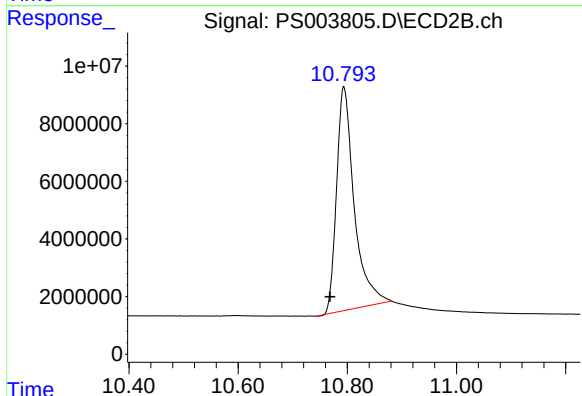


#4 2,4-DCAA

R.T.: 10.794 min
Delta R.T.: 0.025 min
Response: 174682394
Conc: 356.02 ng/ml

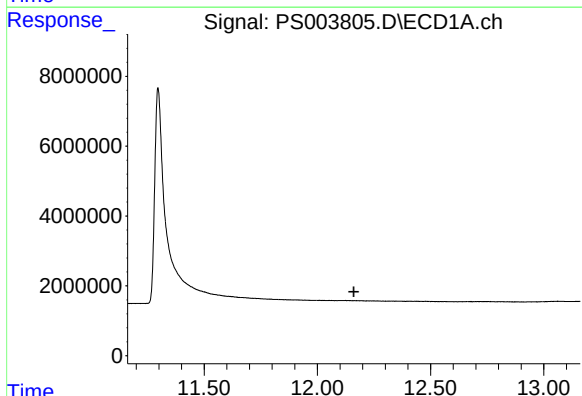


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.162 min
Response: 0
Conc: N.D.

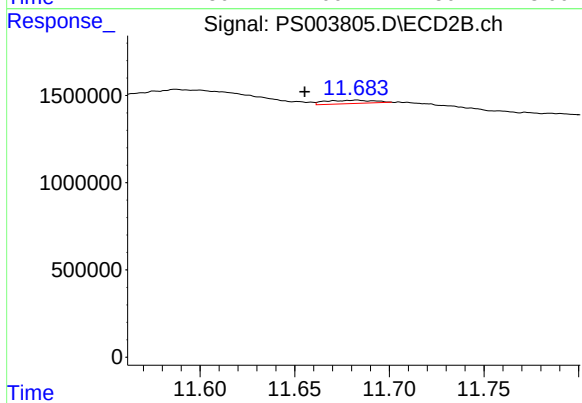

#7 MCPA


R.T.: 11.682 min
Delta R.T.: 0.027 min
Response: 371593
Conc: 0.21 ug/ml

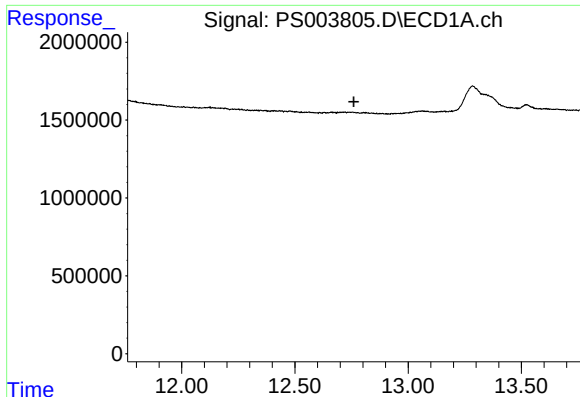

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

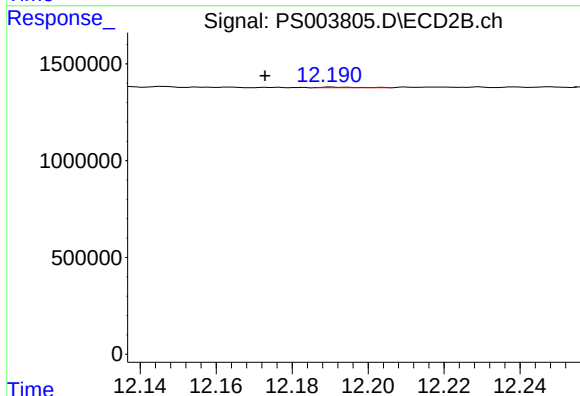


#8 DICHLORPROP

R.T.: 12.191 min
Delta R.T.: 0.019 min
Response: 21429
Conc: 0.05 ng/ml

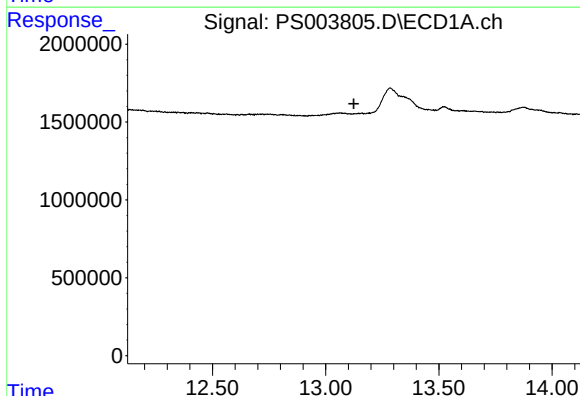


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

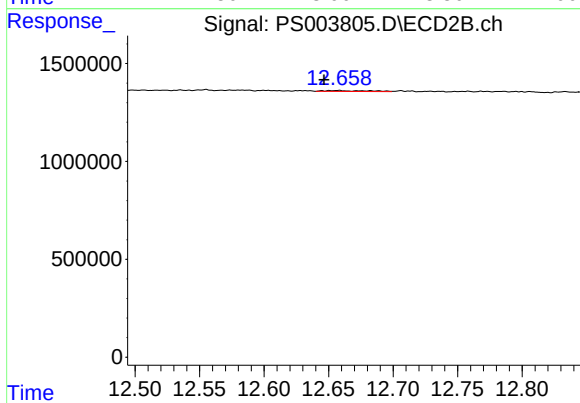

#9 2,4-D


R.T.: 12.657 min
Delta R.T.: 0.011 min
Response: 106846
Conc: 0.20 ng/ml

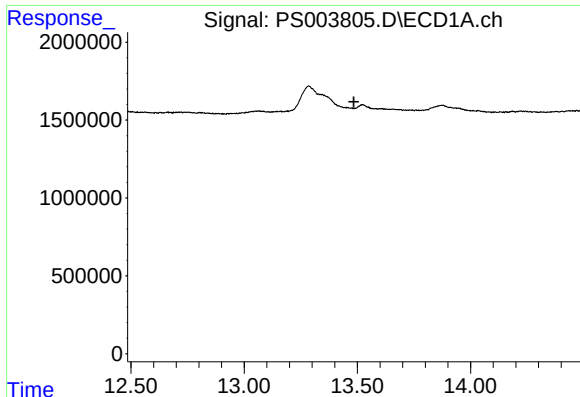

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

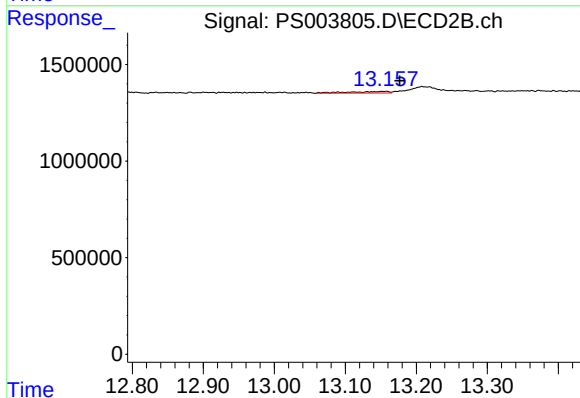


#10 Pentachlorophenol

R.T.: 13.156 min
Delta R.T.: -0.021 min
Response: 317715
Conc: 0.05 ng/ml

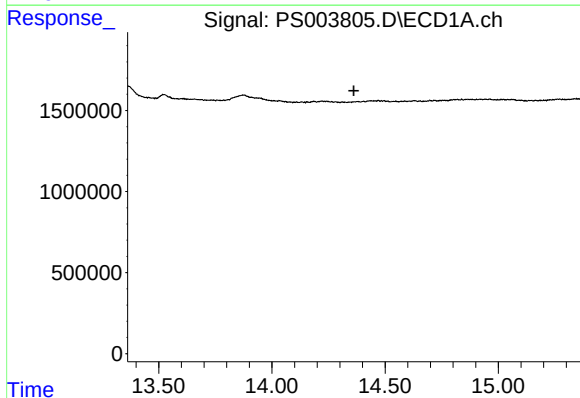


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

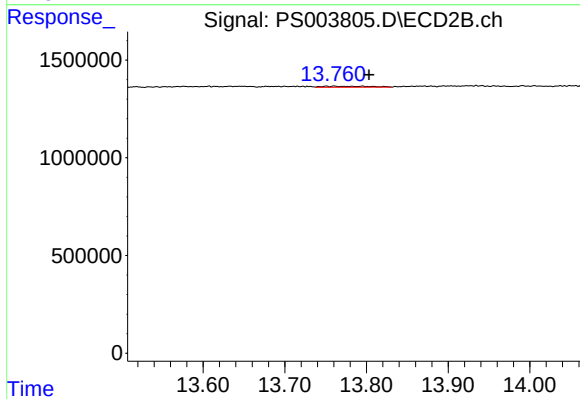

#11 2,4,5-TP (SILVEX)


R.T.: 13.795 min
Delta R.T.: -0.009 min
Response: 219779
Conc: 0.08 ng/ml

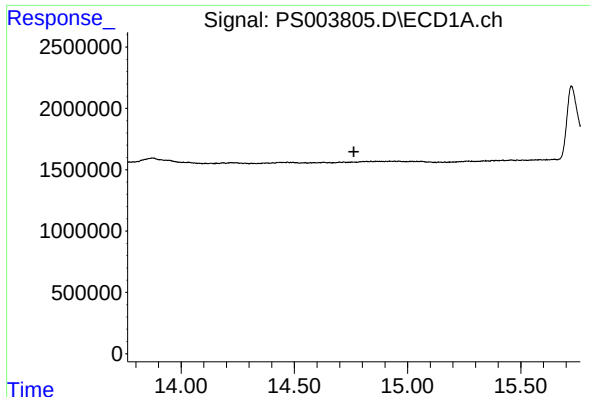

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

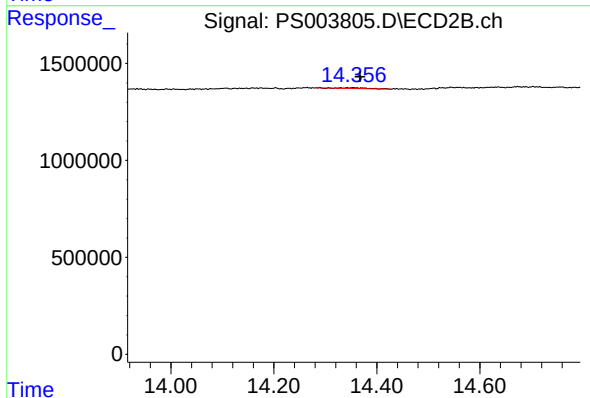


#12 2,4,5-T

R.T.: 14.354 min
Delta R.T.: -0.013 min
Response: 154604
Conc: 0.07 ng/ml

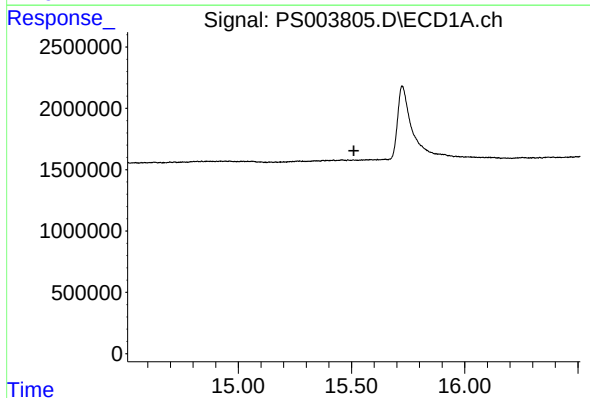


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

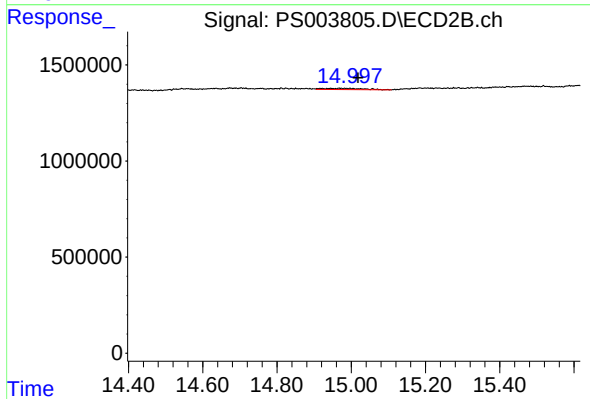

#13 2,4-DB


R.T.: 14.972 min
Delta R.T.: -0.047 min
Response: 499084
Conc: 1.68 ng/ml

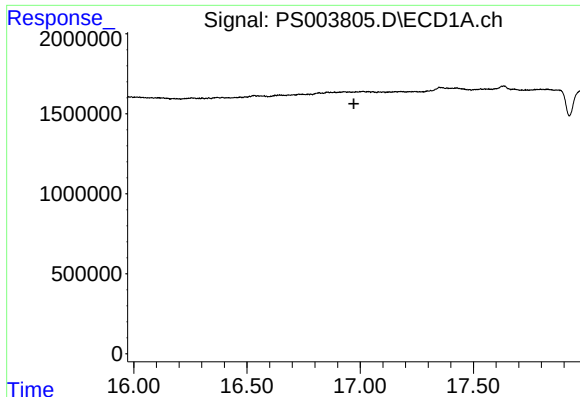

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

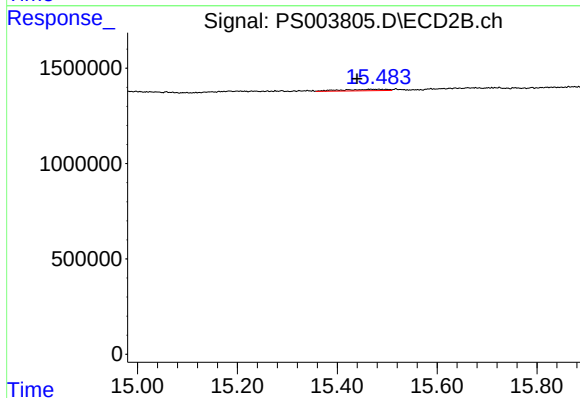


#14 DINOSEB

R.T.: 15.471 min
Delta R.T.: 0.031 min
Response: 478483
Conc: 0.25 ng/ml

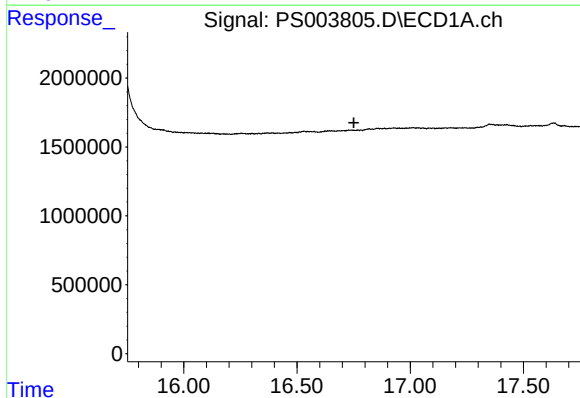


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

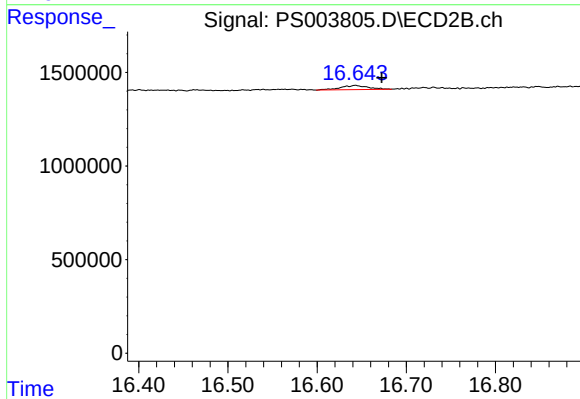

#15 Picloram


R.T.: 16.642 min
Delta R.T.: -0.030 min
Response: 478535
Conc: 0.15 ng/ml

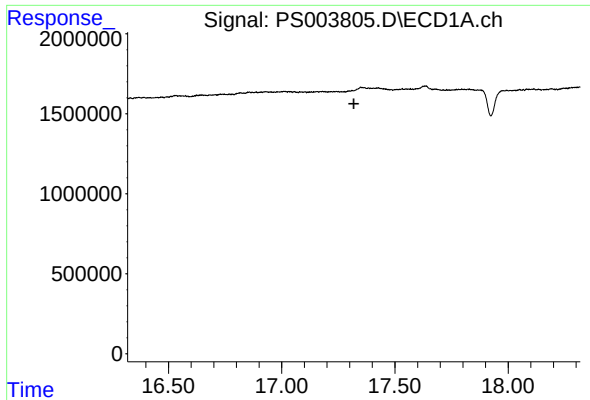

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

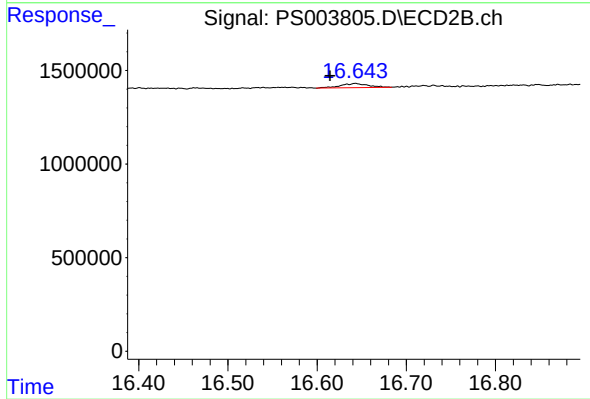

#16 DCPA

R.T.: 16.642 min
Delta R.T.: 0.028 min
Response: 478535
Conc: 0.14 ng/ml