

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
 Data File : PS003814.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 15:27
 Operator : EI\SJ
 Sample : K2086-09
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 05:00:43 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.267	10.770	211.7E6	199.6E6	485.356	406.740
Target Compounds							
1) T	Dalapon	2.787	2.285	45529729	103.3E6	61.070	141.642 #
2) T	3,5-DICHL...	0.000	8.935	0	5468431	N.D.	8.573 #
3) T	4-Nitroph...	0.000	9.942	0	17281719	N.D.	76.119 #
6) T	MCP	11.979	11.252	6072915	-508468	4.366	N.D. #
7) T	MCPA	12.160	0.000	127.9E6	0	60.613	N.D. #
9) T	2,4-D	0.000	12.629	0	1933227	N.D.	3.635 #
10) T	Pentachlo...	0.000	13.177	0	1176383	N.D.	0.170 #
12) T	2,4,5-T	0.000	14.403	0	10592408	N.D.	4.873 #
13) T	2,4-DB	0.000	14.999	0	1746283	N.D.	5.881 #
14) T	DINOSEB	0.000	15.442	0	919622	N.D.	0.479 #
15) T	Picloram	0.000	16.709	0	16782910	N.D.	5.292 #
16) T	DCPA	0.000	16.622	0	3644366	N.D.	1.078 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
Data File : PS003814.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 15:27
Operator : EI\SJ
Sample : K2086-09
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 05:00:43 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

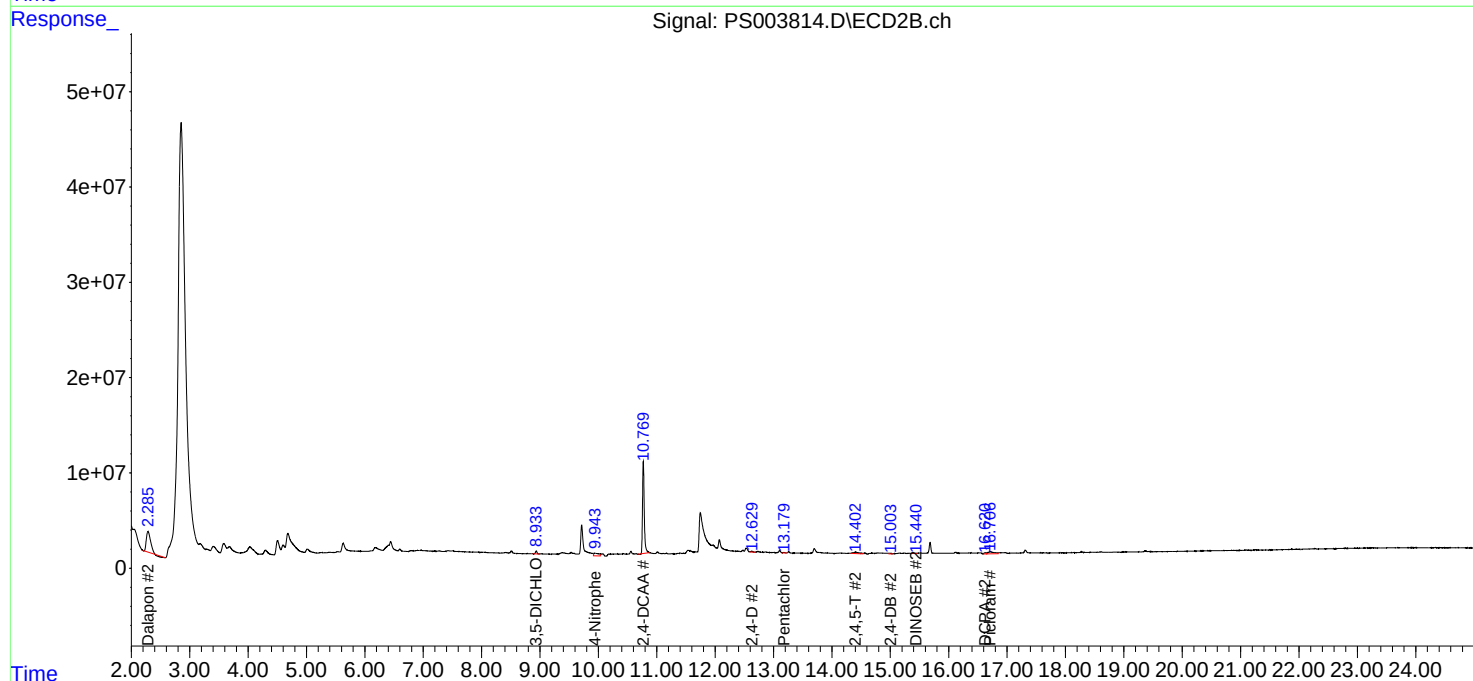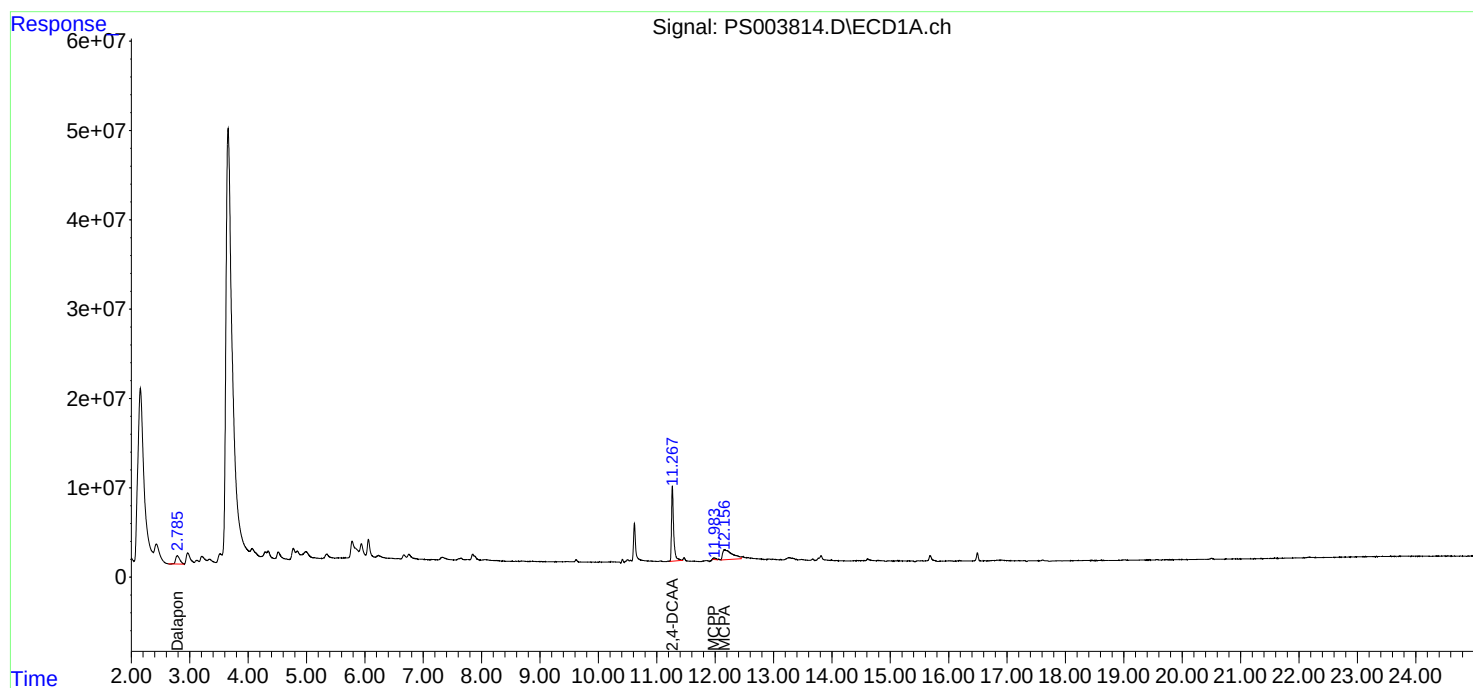


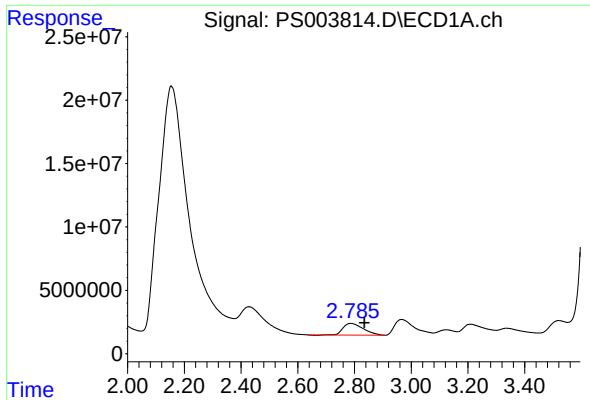

#1 Dalapon


R.T.: 2.787 min
Delta R.T.: -0.048 min
Response: 45529729
Conc: 61.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

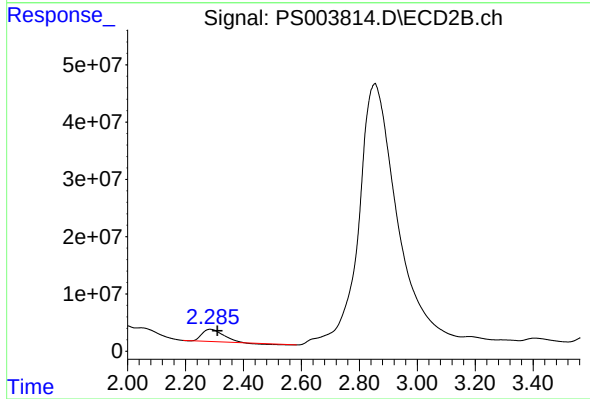


#1 Dalapon

R.T.: 2.285 min
Delta R.T.: -0.026 min
Response: 103346034
Conc: 141.64 ng/ml

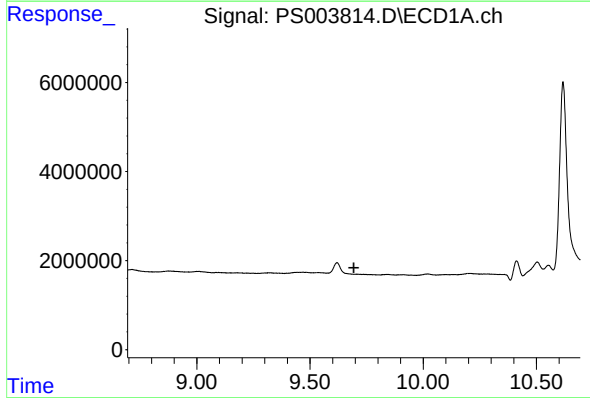


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 9.693 min
Response: 0
Conc: N.D.

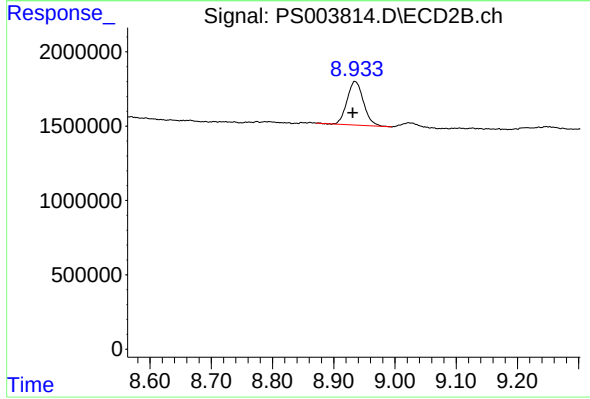

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 8.935 min
Delta R.T.: 0.004 min
Response: 5468431
Conc: 8.57 ng/ml

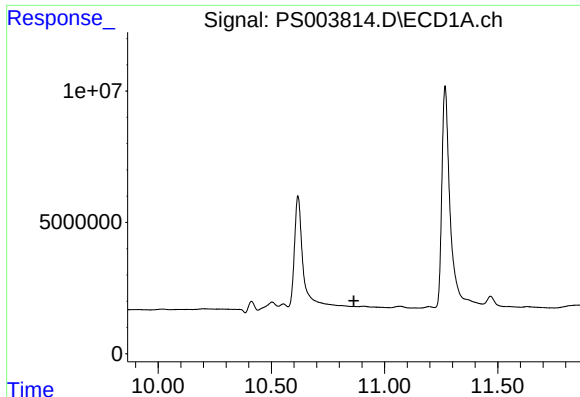

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

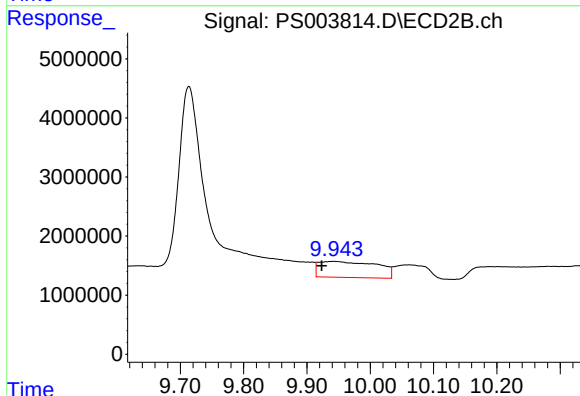


#3 4-Nitrophenol

R.T.: 9.942 min
Delta R.T.: 0.018 min
Response: 17281719
Conc: 76.12 ng/ml

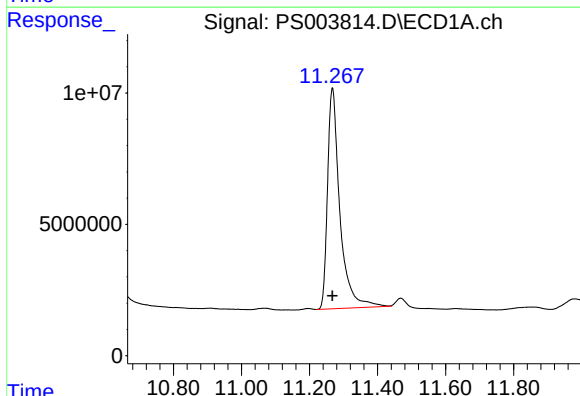


#4 2,4-DCAA

R.T.: 11.267 min
Delta R.T.: 0.000 min
Response: 211718229
Conc: 485.36 ng/ml

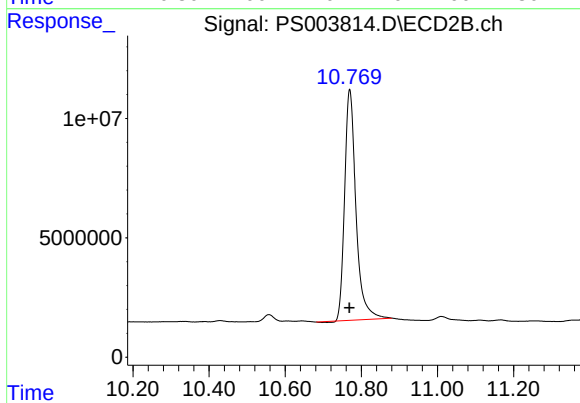

#4 2,4-DCAA


R.T.: 10.770 min
Delta R.T.: 0.000 min
Response: 199570239
Conc: 406.74 ng/ml

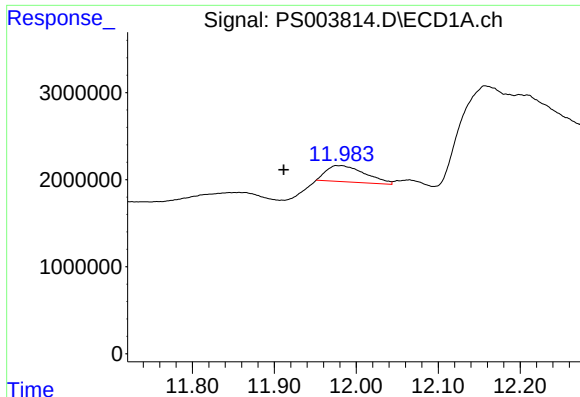

#6 MCPP


R.T.: 11.979 min
Delta R.T.: 0.068 min
Response: 6072915
Conc: 4.37 ug/ml

Instrument :
ECD_S
ClientSampleId :

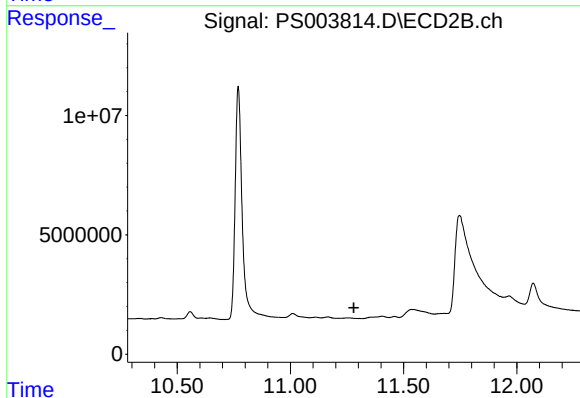


#6 MCPP

R.T.: 11.252 min
Delta R.T.: -0.028 min
Response: -508468
Conc: N.D.

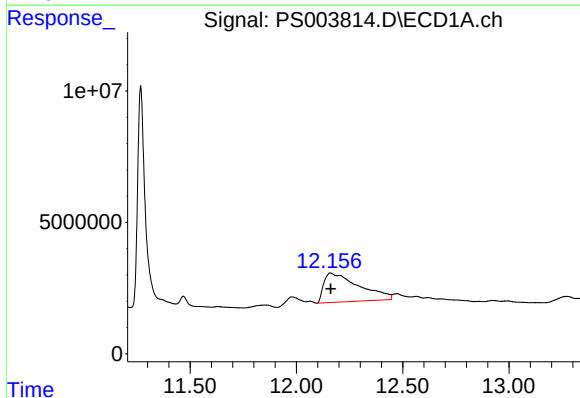


#7 MCPA

R.T.: 12.160 min
Delta R.T.: -0.001 min
Response: 127879458
Conc: 60.61 ug/ml

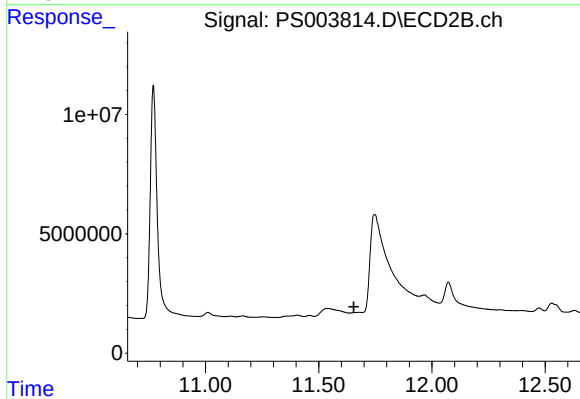

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 11.655 min
Response: 0
Conc: N.D.

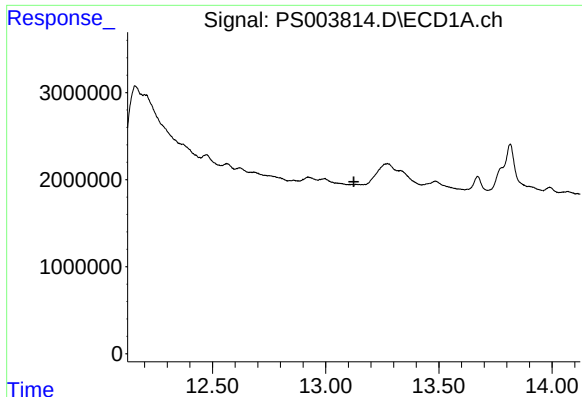

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

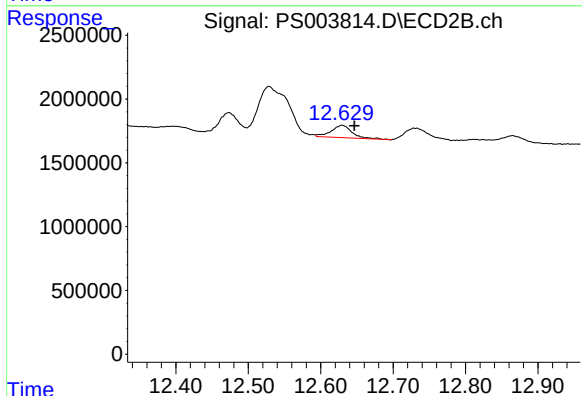


#9 2,4-D

R.T.: 12.629 min
Delta R.T.: -0.017 min
Response: 1933227
Conc: 3.63 ng/ml

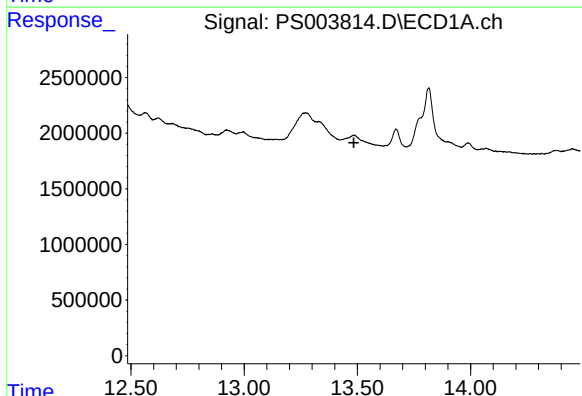


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

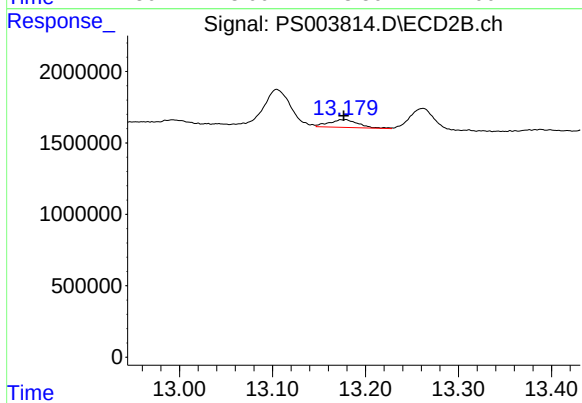

#10 Pentachlorophenol


R.T.: 13.177 min
Delta R.T.: 0.000 min
Response: 1176383
Conc: 0.17 ng/ml

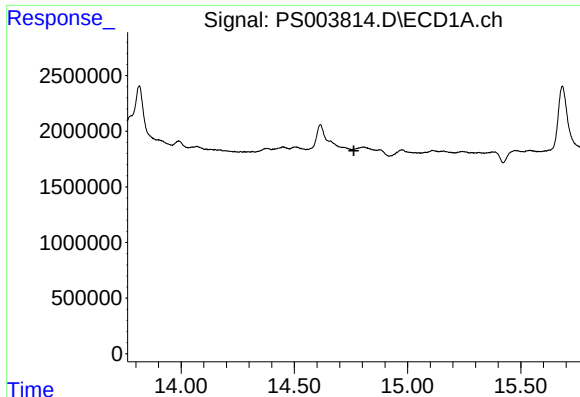

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.763 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

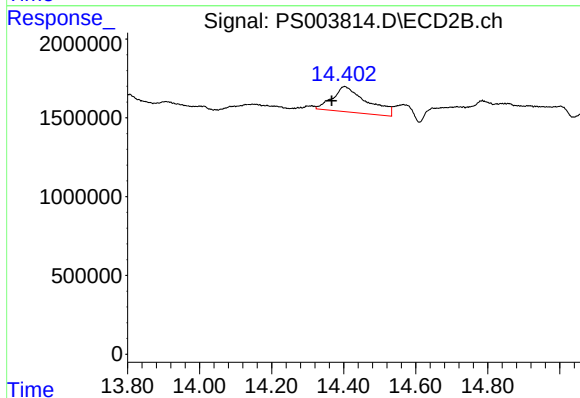


#12 2,4,5-T

R.T.: 14.403 min
Delta R.T.: 0.036 min
Response: 10592408
Conc: 4.87 ng/ml

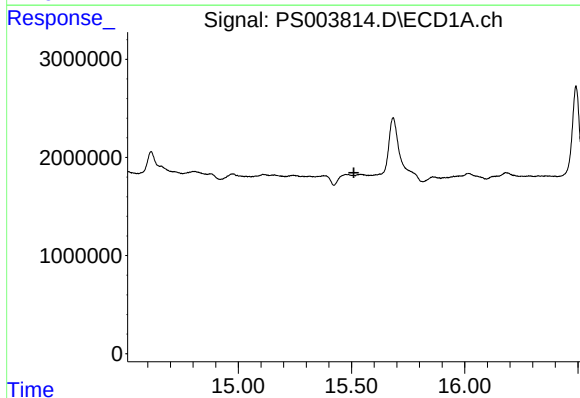


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

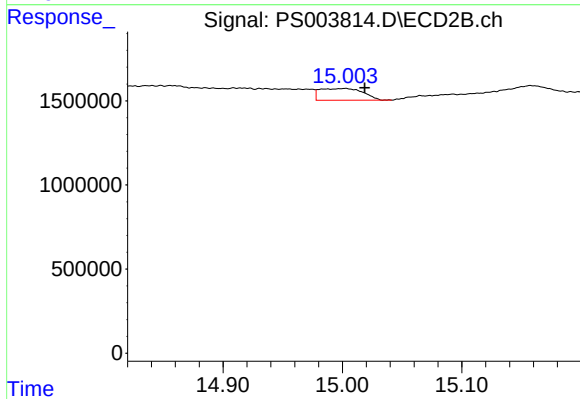

#13 2,4-DB


R.T.: 14.999 min
Delta R.T.: -0.020 min
Response: 1746283
Conc: 5.88 ng/ml

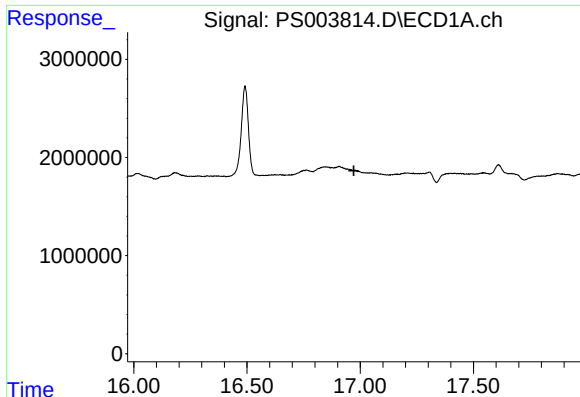

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

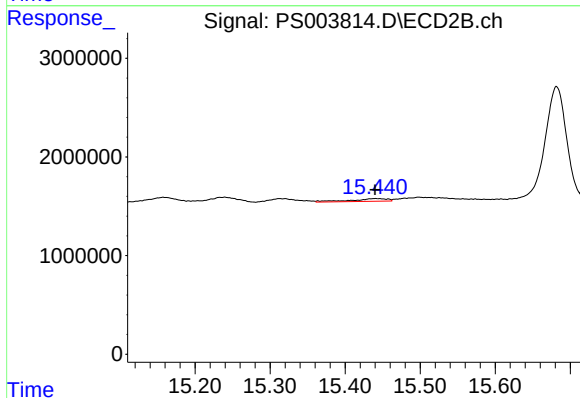


#14 DINOSEB

R.T.: 15.442 min
Delta R.T.: 0.002 min
Response: 919622
Conc: 0.48 ng/ml

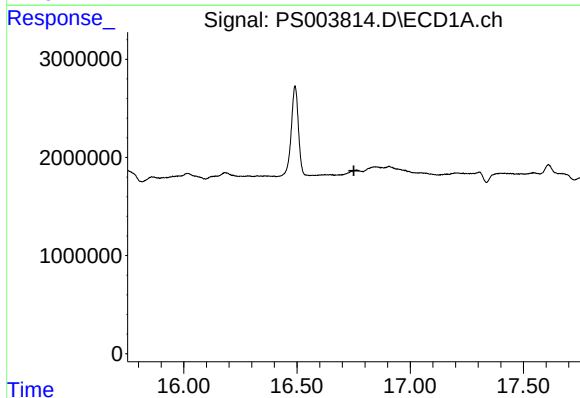


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.752 min
Response: 0
Conc: N.D.

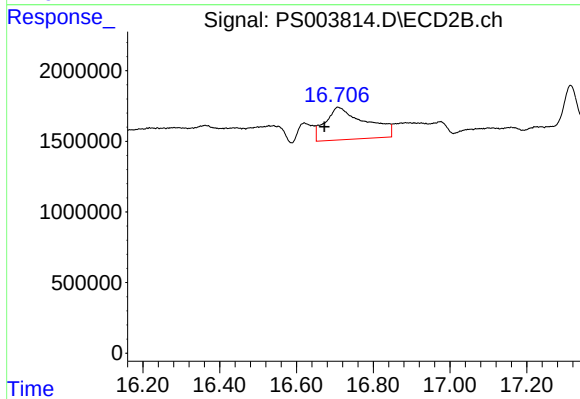

#15 Picloram


R.T.: 16.709 min
Delta R.T.: 0.037 min
Response: 16782910
Conc: 5.29 ng/ml

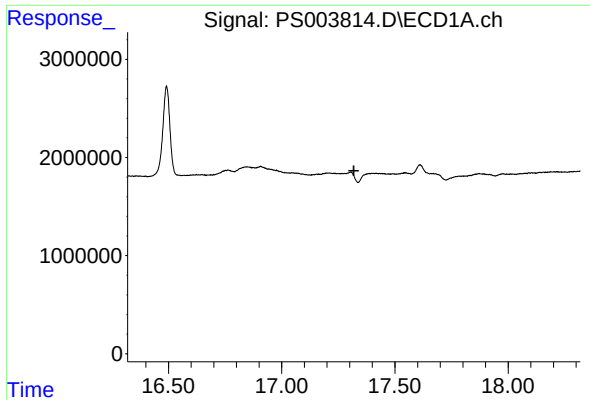

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

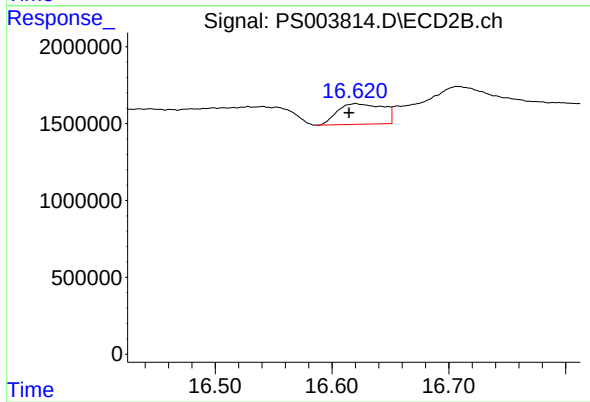

#16 DCPA

R.T.: 16.622 min
Delta R.T.: 0.007 min
Response: 3644366
Conc: 1.08 ng/ml