

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
 Data File : PS003816.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 28 Mar 2019 16:30
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 29 05:01:31 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
 Quant Title : 8080.M
 QLast Update : Wed Mar 27 05:52:44 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.272	10.772	210.5E6	200.9E6	482.592	409.473
Target Compounds							
2) T	3,5-DICHL...	0.000	8.923	0	22482	N.D.	0.035 #
3) T	4-Nitroph...	0.000	9.965	0	431566	N.D.	1.901 #
6) T	MCP	0.000	11.306	0	31339	N.D.	0.027 #
7) T	MCPA	0.000	11.655	0	1246625	N.D.	0.699 #
8) T	DICHLORPROP	0.000	12.173	0	1156206	N.D.	2.484 #
9) T	2,4-D	0.000	12.608	0	577938	N.D.	1.087 #
10) T	Pentachlo...	0.000	13.186	0	1777119	N.D.	0.257 #
11) T	2,4,5-TP ...	0.000	13.813	0	410270	N.D.	0.155 #
13) T	2,4-DB	0.000	15.063	0	21378	N.D.	0.072 #
14) T	DINOSEB	0.000	15.448	0	2783177	N.D.	1.451 #
15) T	Picloram	0.000	16.619	0	621549	N.D.	0.196 #
16) T	DCPA	0.000	16.619	0	621549	N.D.	0.184 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS032819\
Data File : PS003816.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 28 Mar 2019 16:30
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 29 05:01:31 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS032619.M
Quant Title : 8080.M
QLast Update : Wed Mar 27 05:52:44 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

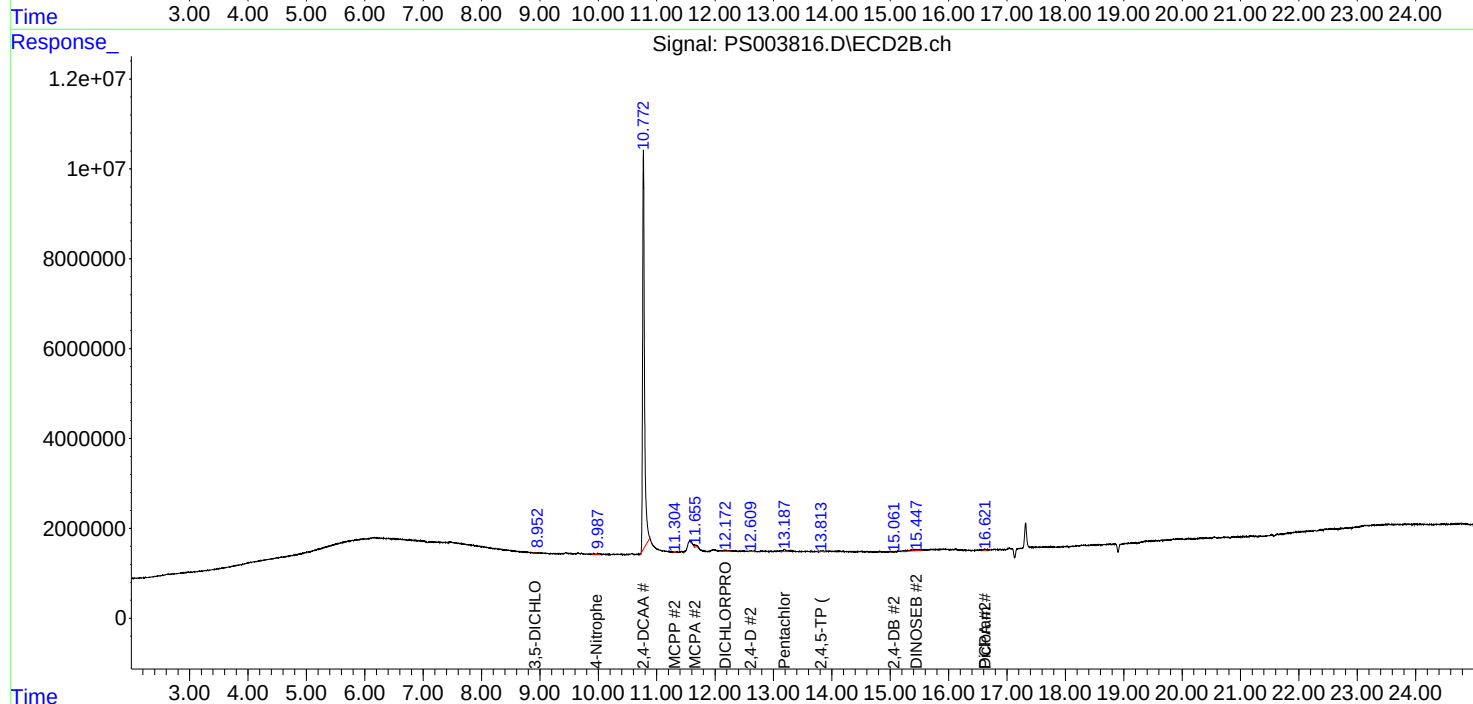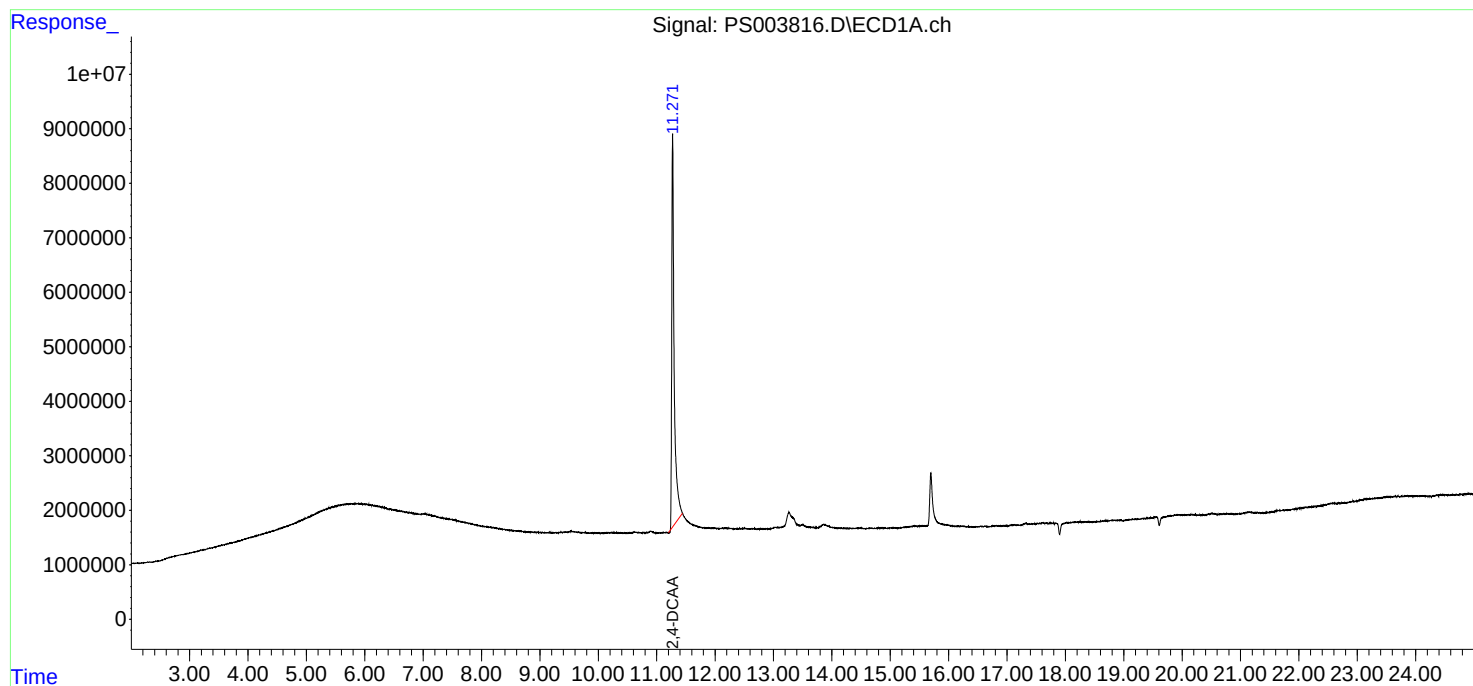


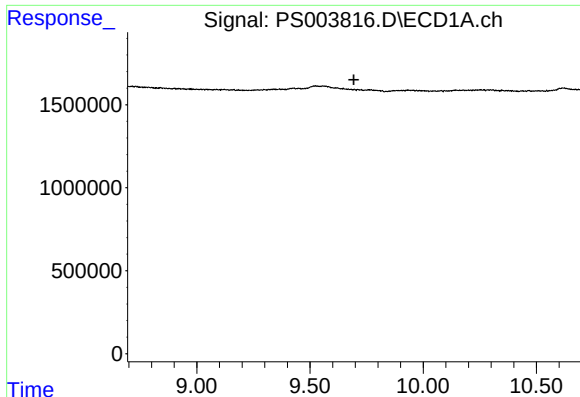

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 9.693 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

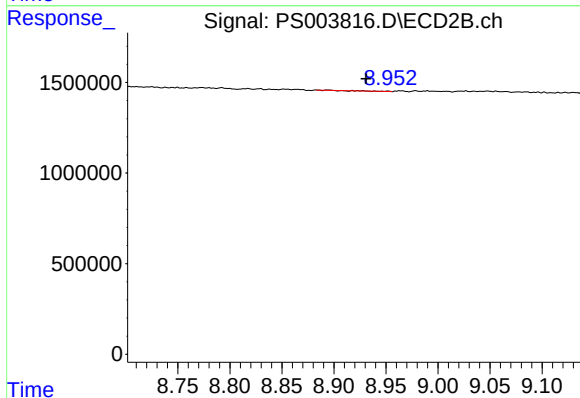


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 8.923 min
Delta R.T.: -0.008 min
Response: 22482
Conc: 0.04 ng/ml

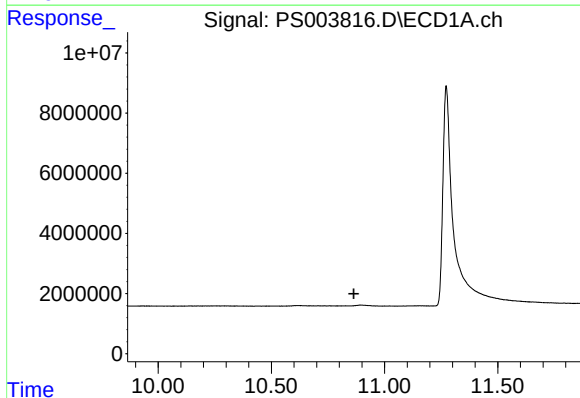


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T.: 10.865 min
Response: 0
Conc: N.D.

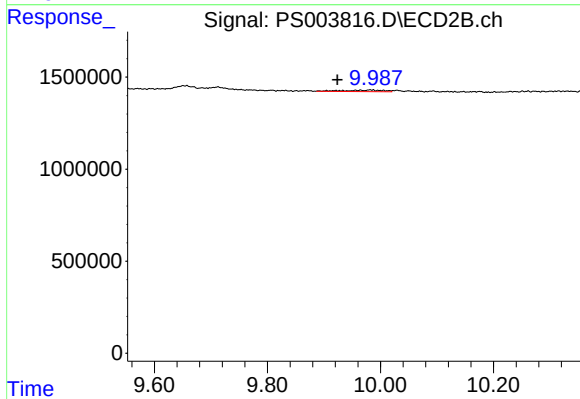

#3 4-Nitrophenol


R.T.: 9.965 min
Delta R.T.: 0.041 min
Response: 431566
Conc: 1.90 ng/ml

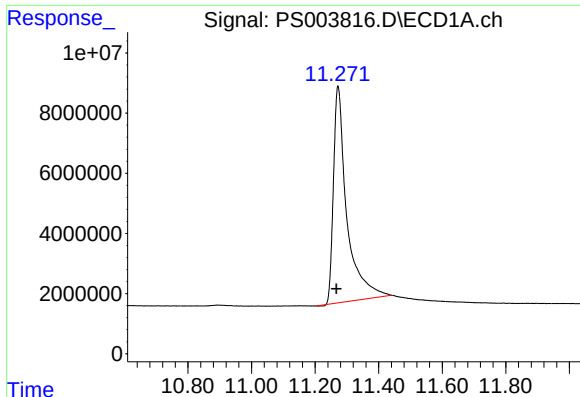

#4 2,4-DCAA


R.T.: 11.272 min
Delta R.T.: 0.006 min
Response: 210512734
Conc: 482.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

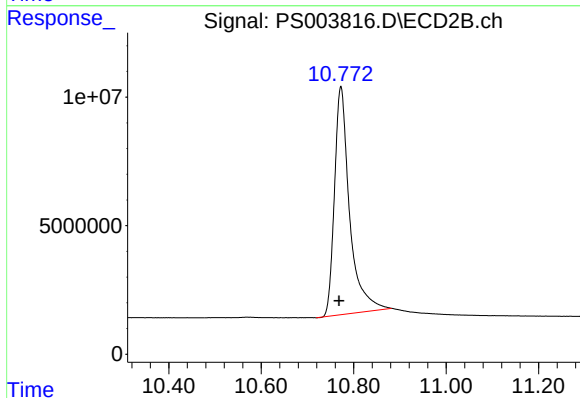


#4 2,4-DCAA

R.T.: 10.772 min
Delta R.T.: 0.004 min
Response: 200911396
Conc: 409.47 ng/ml

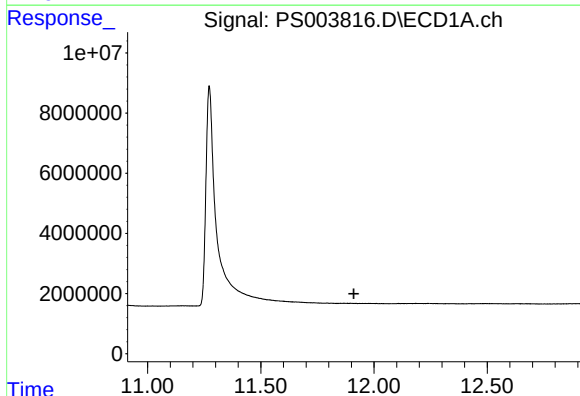


#6 MCP

R.T.: 0.000 min
Exp R.T. : 11.911 min
Response: 0
Conc: N.D.

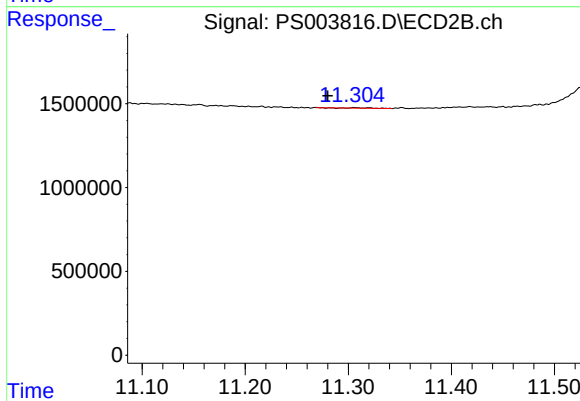

#6 MCP


R.T.: 11.306 min
Delta R.T.: 0.026 min
Response: 31339
Conc: 0.03 ug/ml

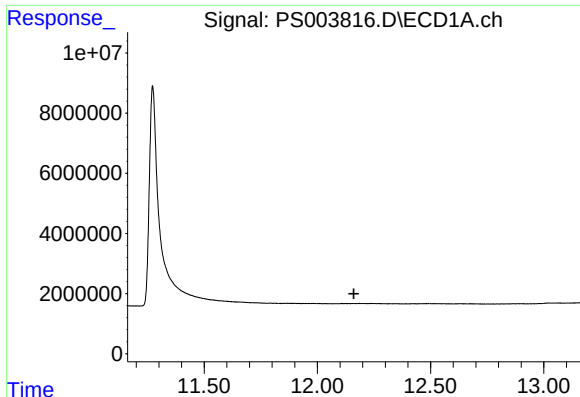

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.162 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

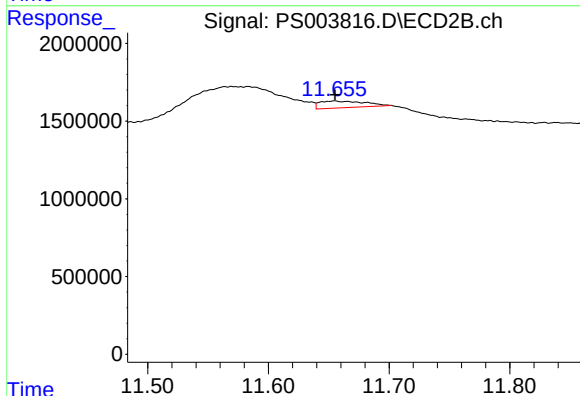


#7 MCPA

R.T.: 11.655 min
Delta R.T.: 0.000 min
Response: 1246625
Conc: 0.70 ug/ml

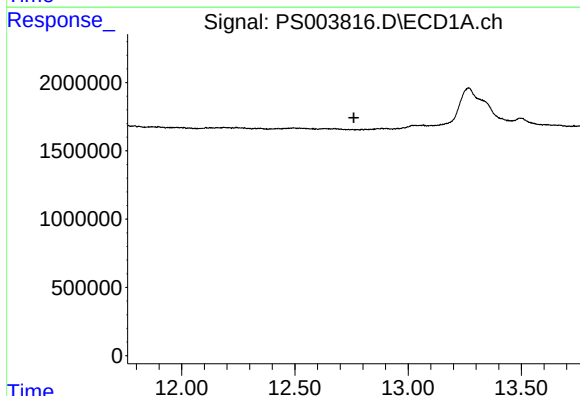


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 12.760 min
Response: 0
Conc: N.D.

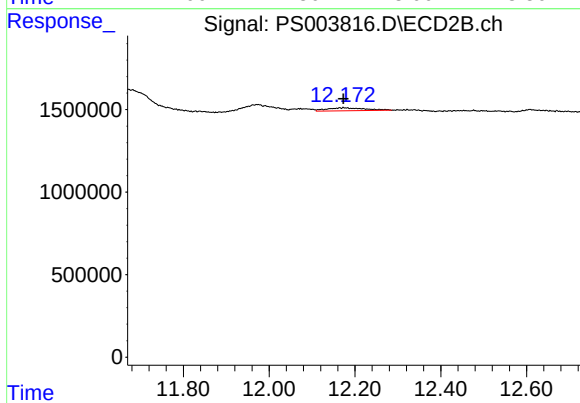

#8 DICHLORPROP


R.T.: 12.173 min
Delta R.T.: 0.000 min
Response: 1156206
Conc: 2.48 ng/ml

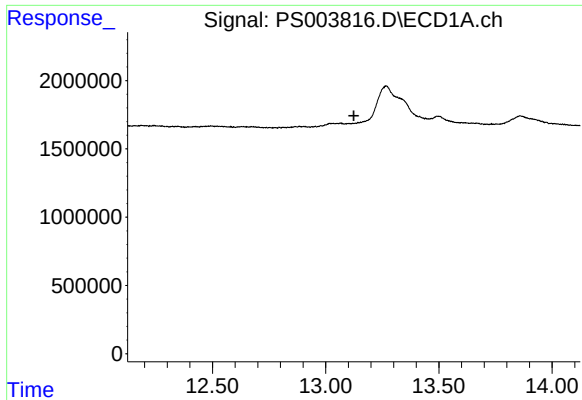

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.125 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

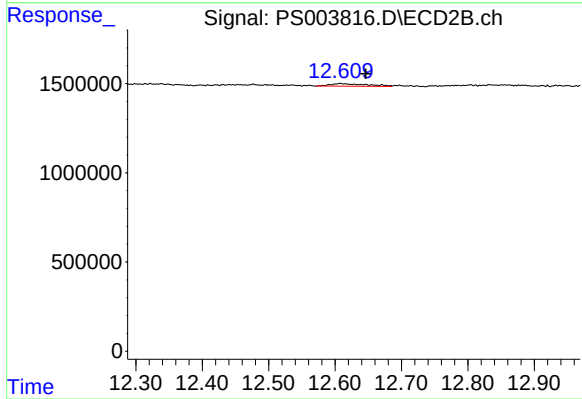


#9 2,4-D

R.T.: 12.608 min
Delta R.T.: -0.039 min
Response: 577938
Conc: 1.09 ng/ml

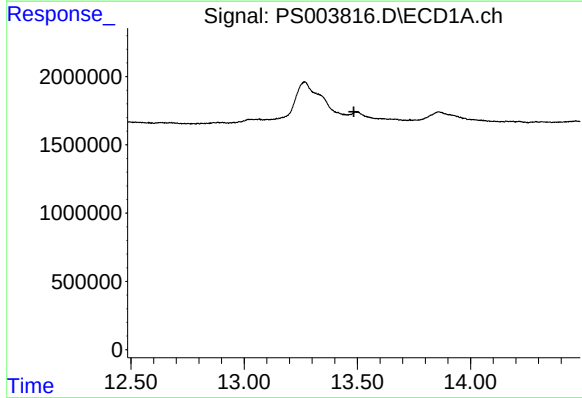


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 13.485 min
Response: 0
Conc: N.D.

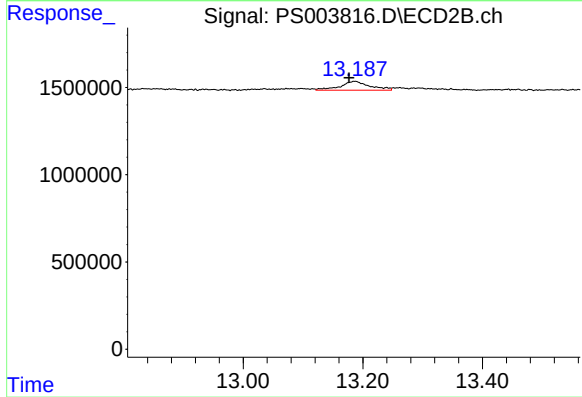

#10 Pentachlorophenol


R.T.: 13.186 min
Delta R.T.: 0.010 min
Response: 1777119
Conc: 0.26 ng/ml

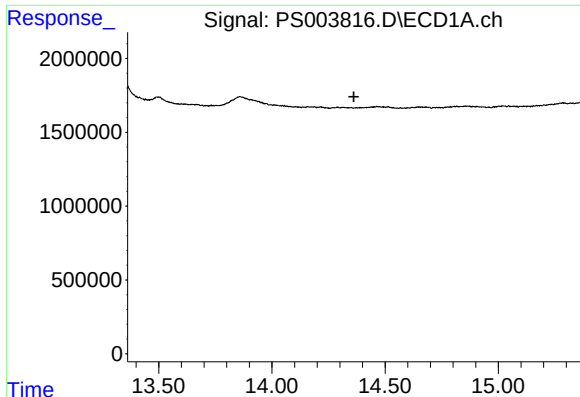

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

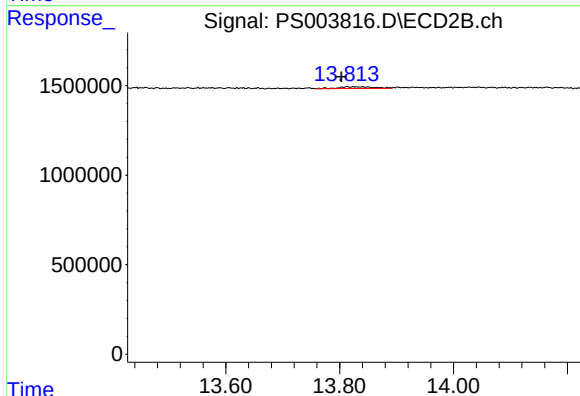


#11 2,4,5-TP (SILVEX)

R.T.: 13.813 min
Delta R.T.: 0.009 min
Response: 410270
Conc: 0.15 ng/ml

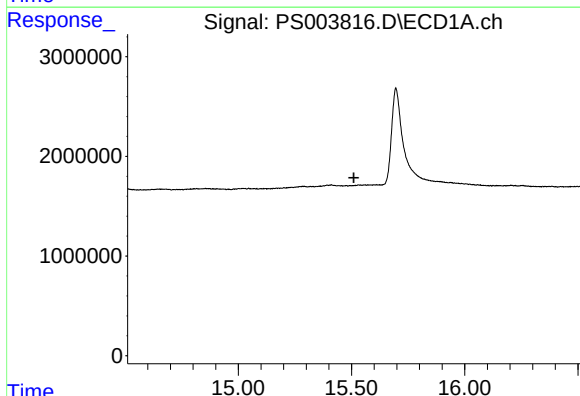


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 15.510 min
Response: 0
Conc: N.D.

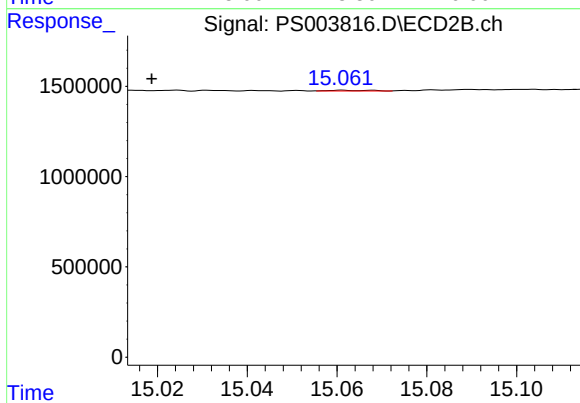

#13 2,4-DB


R.T.: 15.063 min
Delta R.T.: 0.045 min
Response: 21378
Conc: 0.07 ng/ml

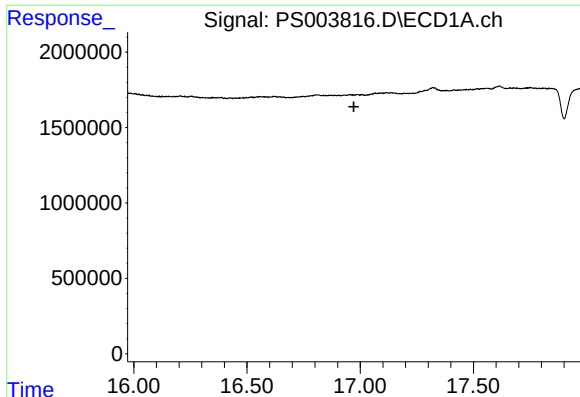

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 16.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

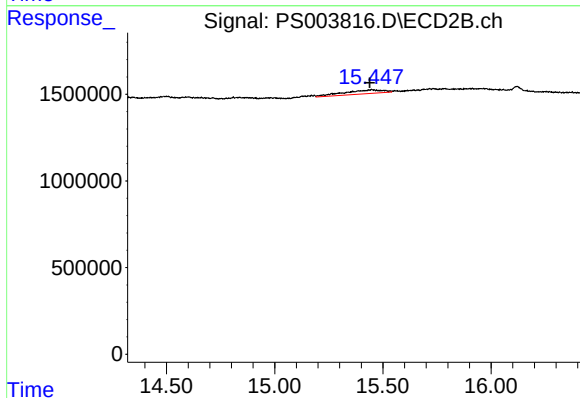


#14 DINOSEB

R.T.: 15.448 min
Delta R.T.: 0.008 min
Response: 2783177
Conc: 1.45 ng/ml

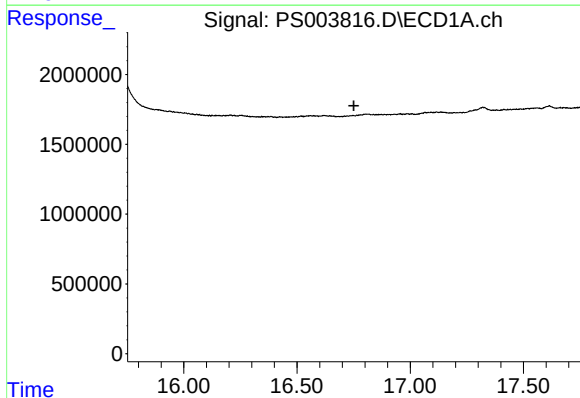


#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.752 min
Response: 0
Conc: N.D.

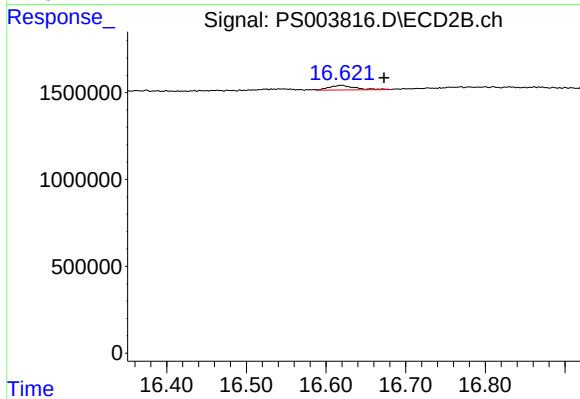

#15 Picloram


R.T.: 16.619 min
Delta R.T.: -0.054 min
Response: 621549
Conc: 0.20 ng/ml

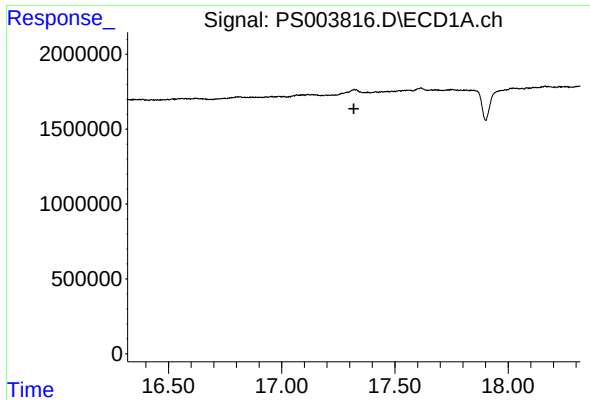

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

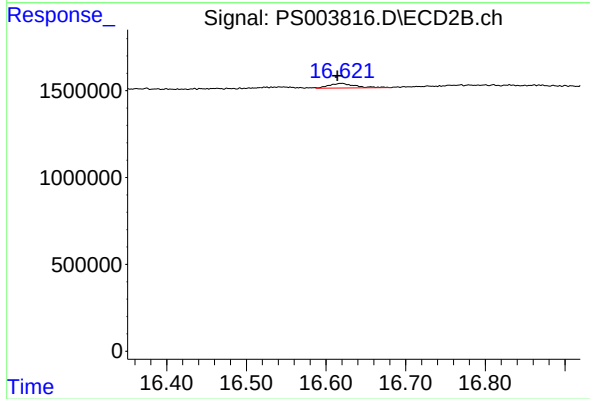

#16 DCPA

R.T.: 16.619 min
Delta R.T.: 0.005 min
Response: 621549
Conc: 0.18 ng/ml